

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021319\
 Data File : PS003162.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Feb 2019 19:53
 Operator : EI\SJ
 Sample : K1461-08
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 00:49:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.282	10.783	123.8E6	191.7E6	325.977	448.347 #
Target Compounds							
1) T	Dalapon	0.000	2.286	0	46803769	N.D.	87.333 #
2) T	3,5-DICHL...	0.000	9.035	0	1539579	N.D.	2.732 #
6) T	MCP	11.953	11.344	10748895	7262842	8.971	6.585 #
10) T	Pentachlo...	13.508	0.000	3100990	0	0.484	N.D. #
15) T	Picloram	0.000	16.713	0	7260587	N.D.	2.415 #
16) T	DCPA	17.412	16.654	-2639482	7379583	N.D.	2.382



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021319\
Data File : PS003162.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Feb 2019 19:53
Operator : EI\SJ
Sample : K1461-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 00:49:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

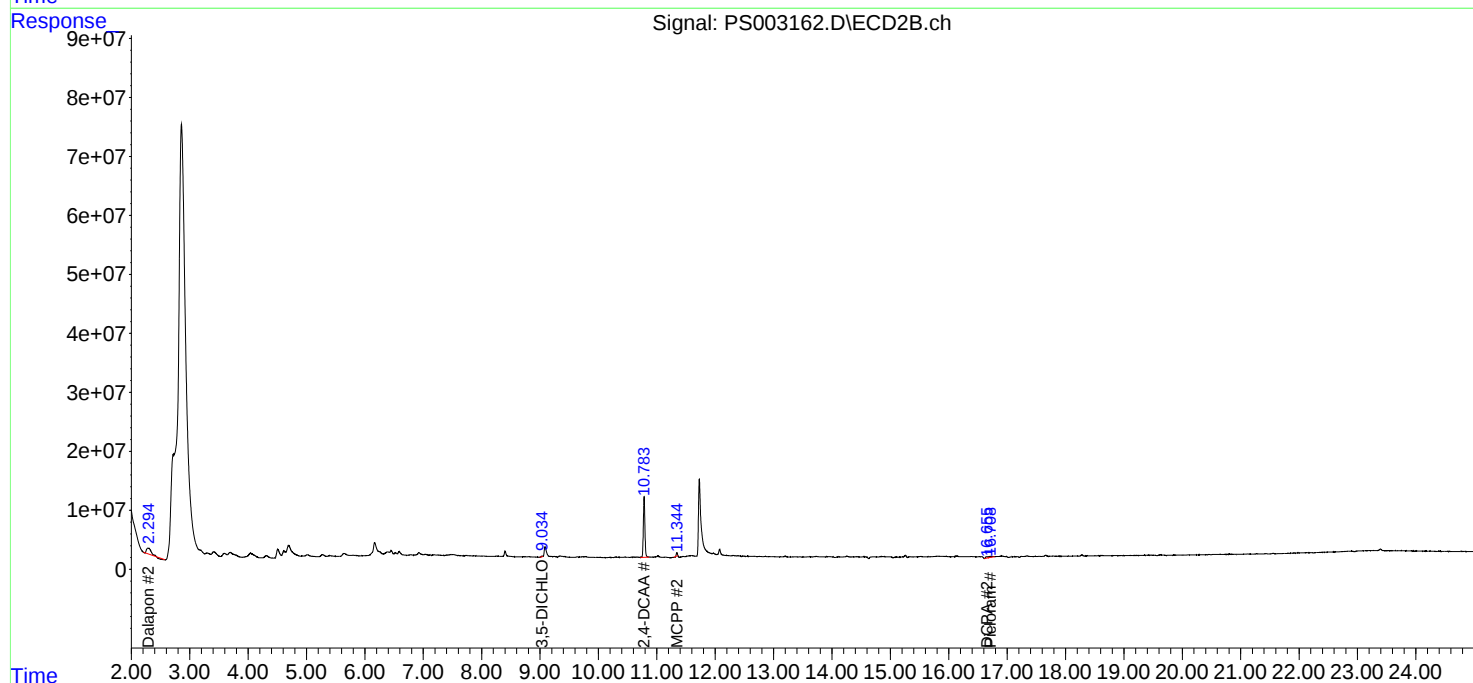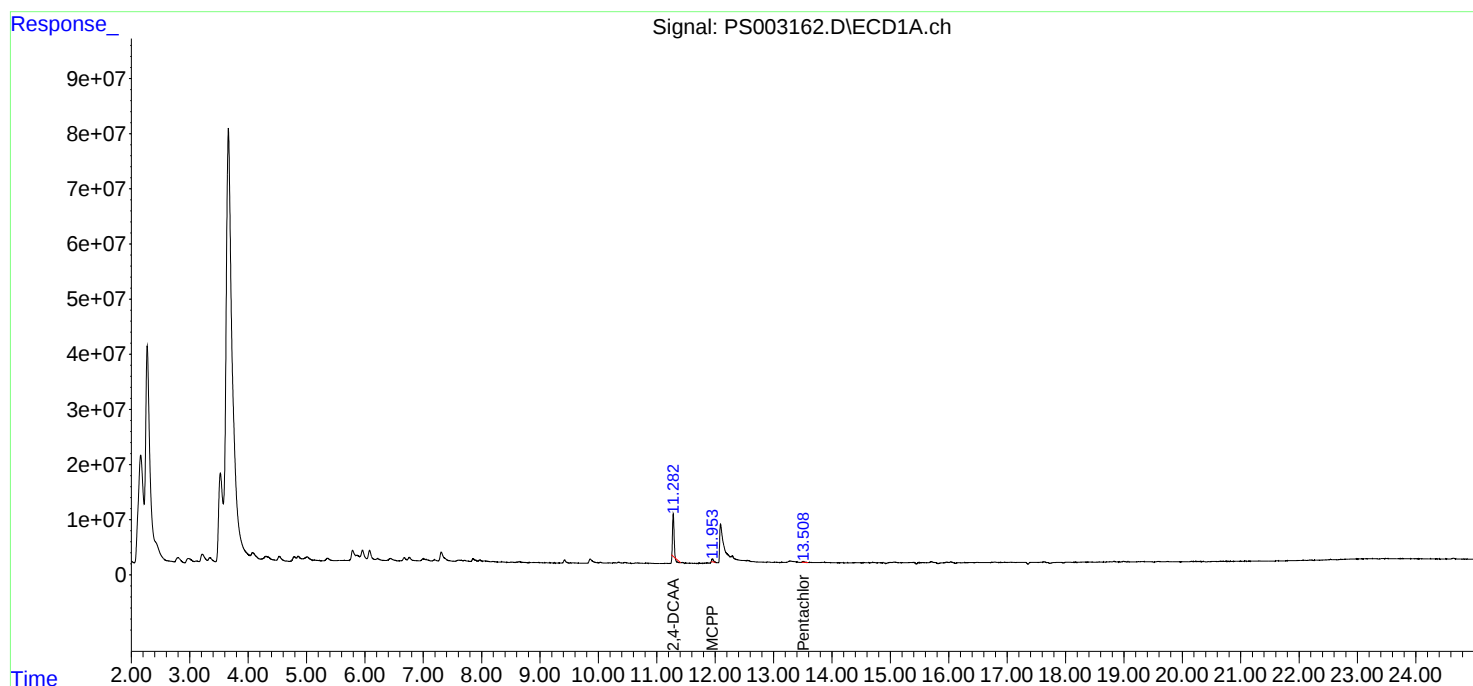


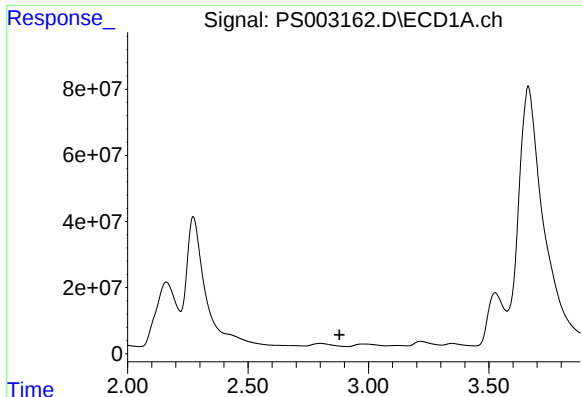

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

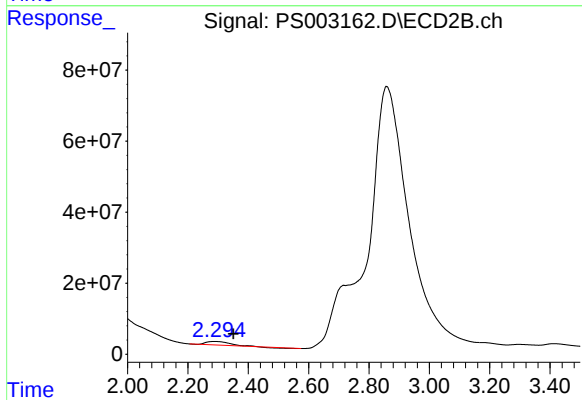


#1 Dalapon

R.T.: 2.286 min
Delta R.T.: -0.064 min
Response: 46803769
Conc: 87.33 ng/ml

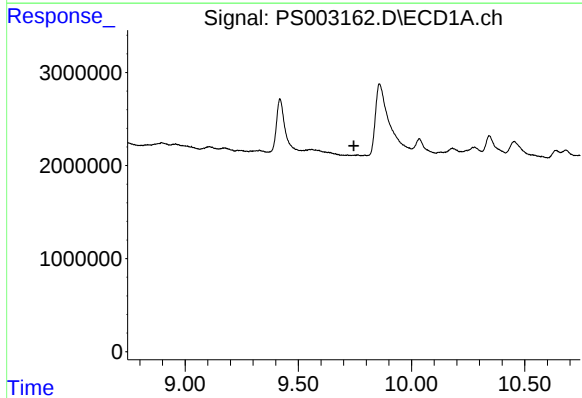


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 9.745 min
Response: 0
Conc: N.D.

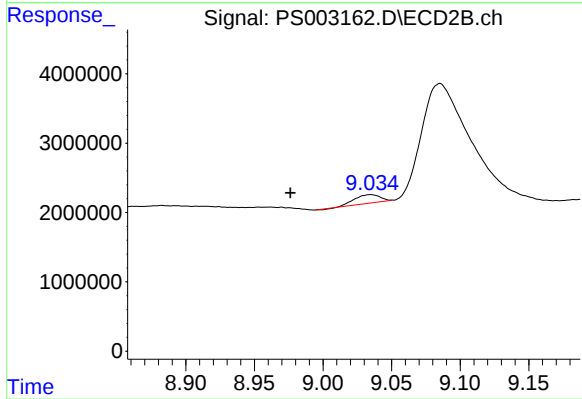

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.035 min
Delta R.T.: 0.058 min
Response: 1539579
Conc: 2.73 ng/ml

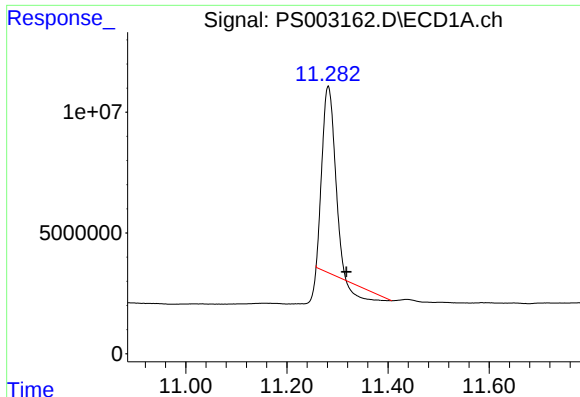

#4 2,4-DCAA


R.T.: 11.282 min
Delta R.T.: -0.036 min
Response: 123754197
Conc: 325.98 ng/ml

Instrument :
ECD_S
ClientSampleId :

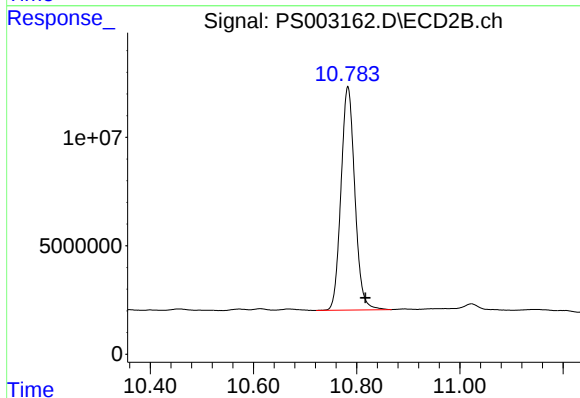


#4 2,4-DCAA

R.T.: 10.783 min
Delta R.T.: -0.034 min
Response: 191688821
Conc: 448.35 ng/ml

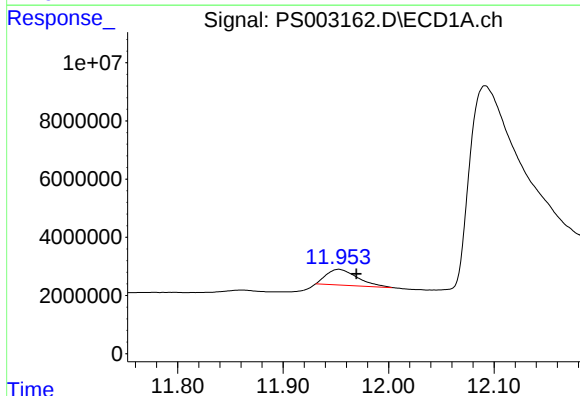


#6 MCP

R.T.: 11.953 min
Delta R.T.: -0.017 min
Response: 10748895
Conc: 8.97 ug/ml

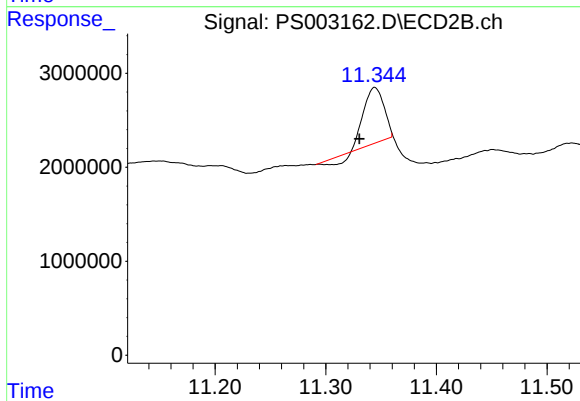

#6 MCP


R.T.: 11.344 min
Delta R.T.: 0.014 min
Response: 7262842
Conc: 6.58 ug/ml

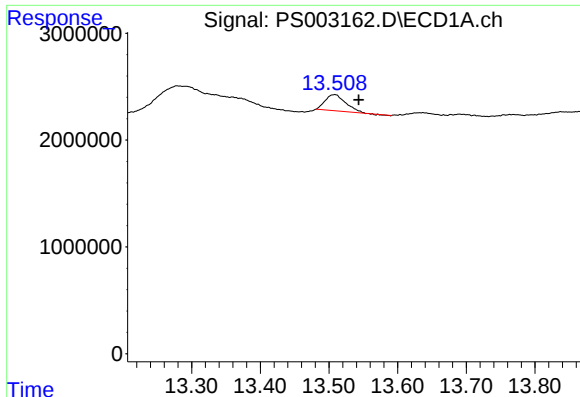

#10 Pentachlorophenol


R.T.: 13.508 min
Delta R.T.: -0.036 min
Response: 3100990
Conc: 0.48 ng/ml

Instrument :
ECD_S
ClientSampleId :

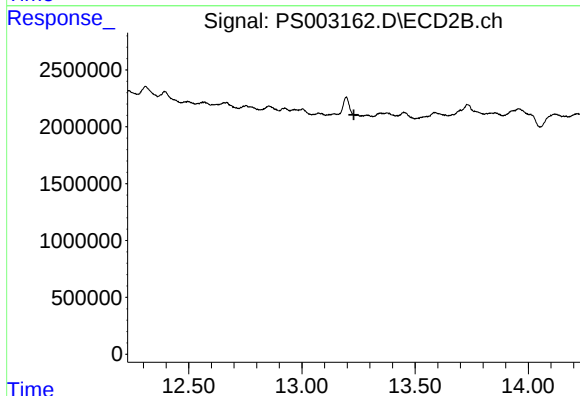


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.229 min
Response: 0
Conc: N.D.

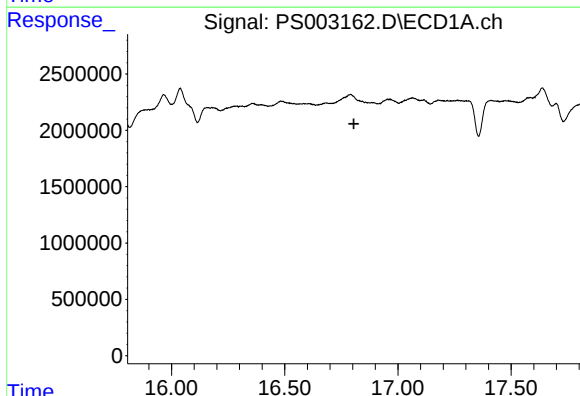


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.806 min
Response: 0
Conc: N.D.

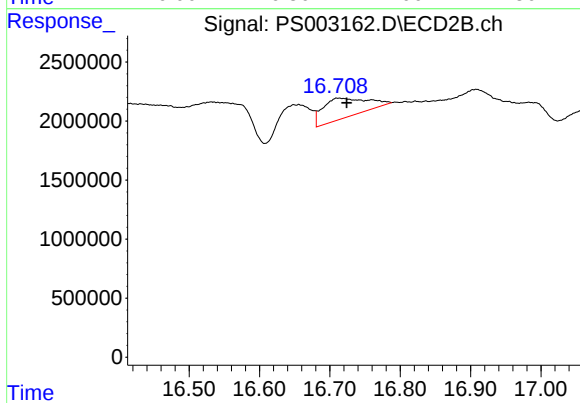

#15 Picloram


R.T.: 16.713 min
Delta R.T.: -0.012 min
Response: 7260587
Conc: 2.42 ng/ml

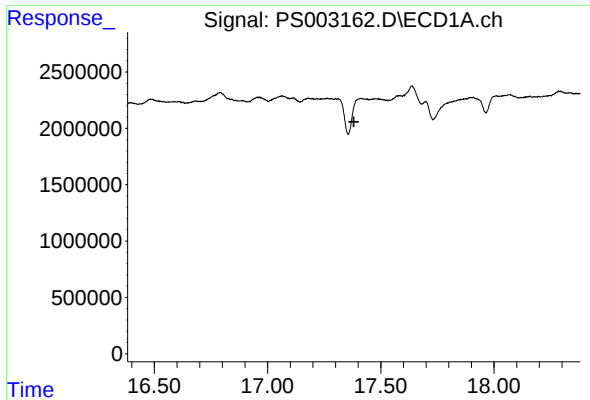

#16 DCPA

R.T.: 17.412 min
Delta R.T.: 0.031 min
Response: -2639482
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

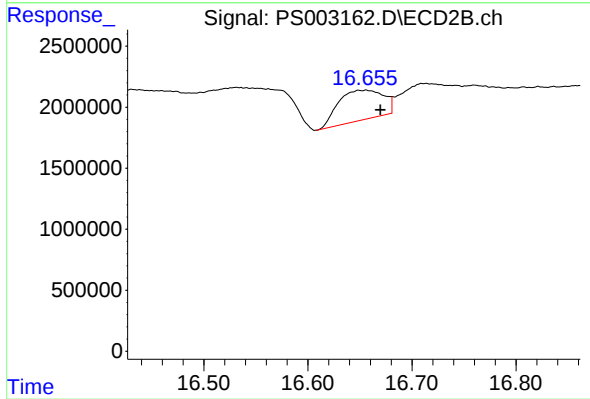

#16 DCPA

R.T.: 16.654 min
Delta R.T.: -0.016 min
Response: 7379583
Conc: 2.38 ng/ml