

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021319\
 Data File : PS003163.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Feb 2019 20:25
 Operator : EI\SJ
 Sample : K1462-04
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 00:49:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.295	10.780	199.3E6	197.4E6	524.881	461.660
Target Compounds							
6) T	MCP	11.969	11.342	18735497	7237902	15.637	6.562 #
15) T	Picloram	0.000	16.718	0	12490830	N.D.	4.155 #
16) T	DCPA	0.000	16.718	0	12490830	N.D.	4.032 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021319\
Data File : PS003163.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Feb 2019 20:25
Operator : EI\SJ
Sample : K1462-04
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 00:49:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

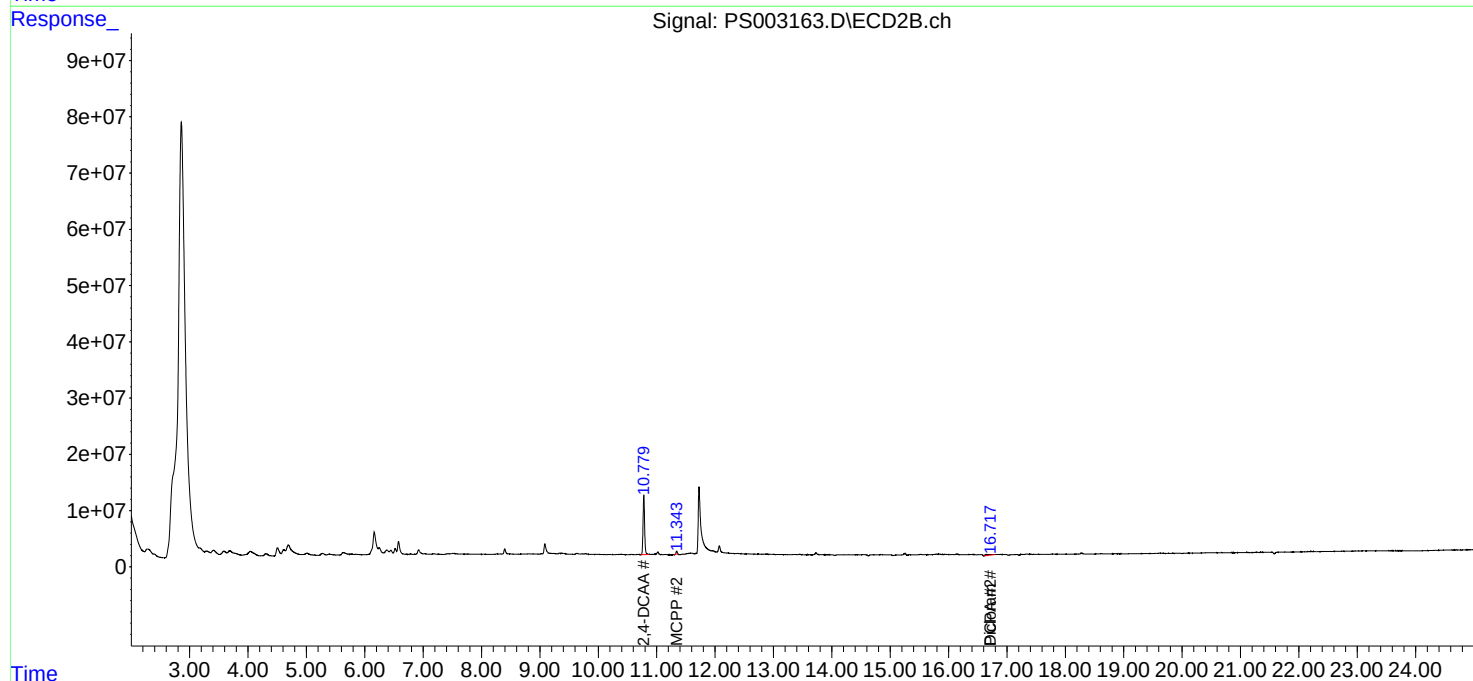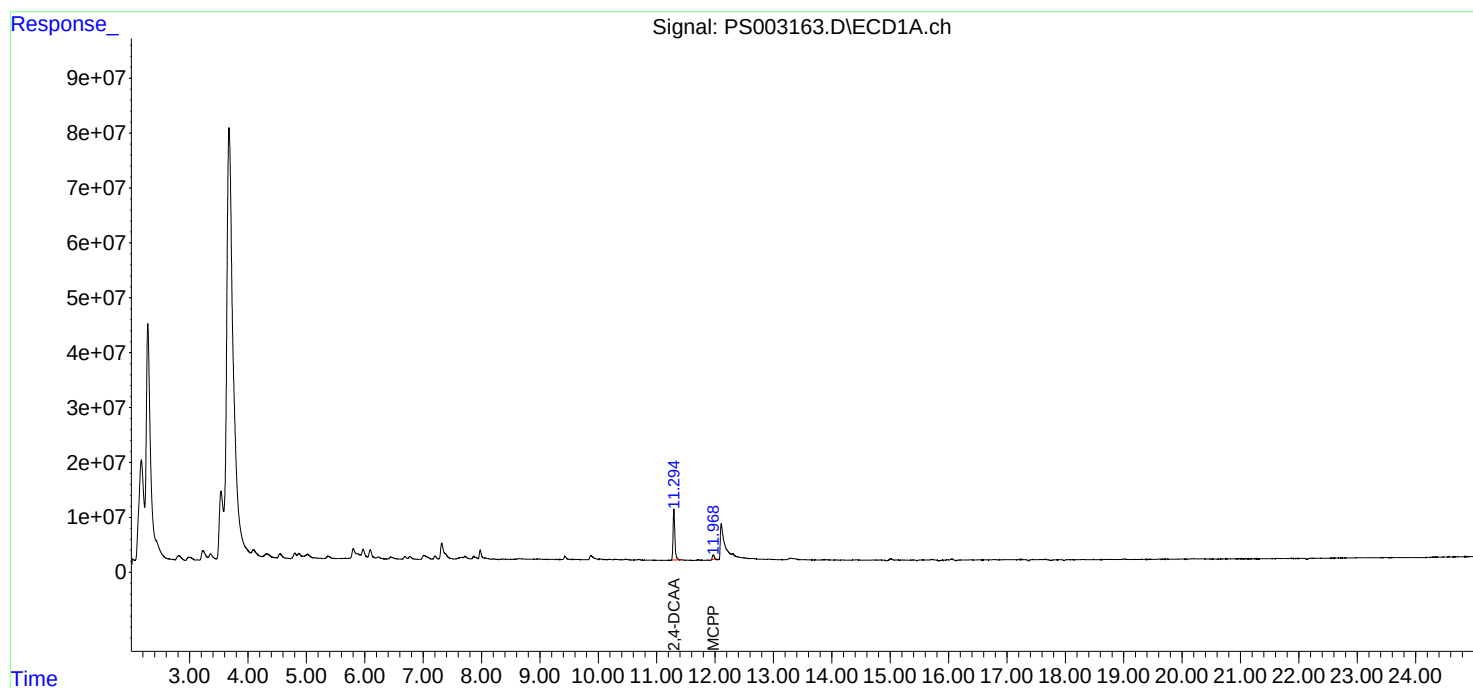


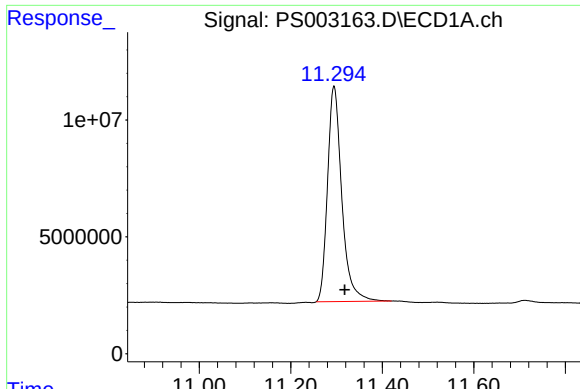

#4 2,4-DCAA


R.T.: 11.295 min
Delta R.T.: -0.023 min
Response: 199266380
Conc: 524.88 ng/ml

Instrument :
ECD_S
ClientSampleId :

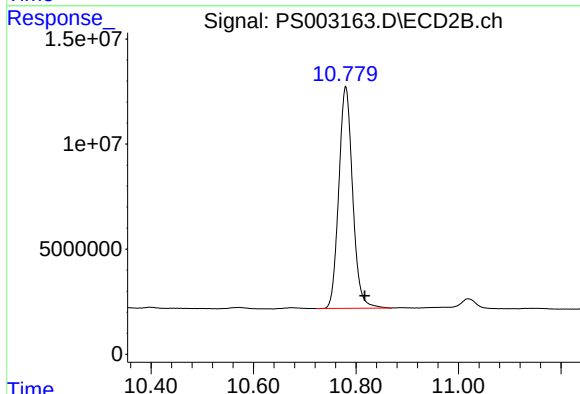


#4 2,4-DCAA

R.T.: 10.780 min
Delta R.T.: -0.037 min
Response: 197380801
Conc: 461.66 ng/ml

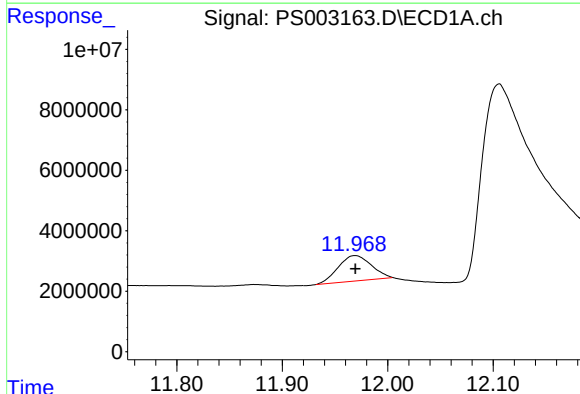


#6 MCP

R.T.: 11.969 min
Delta R.T.: 0.000 min
Response: 18735497
Conc: 15.64 ug/ml

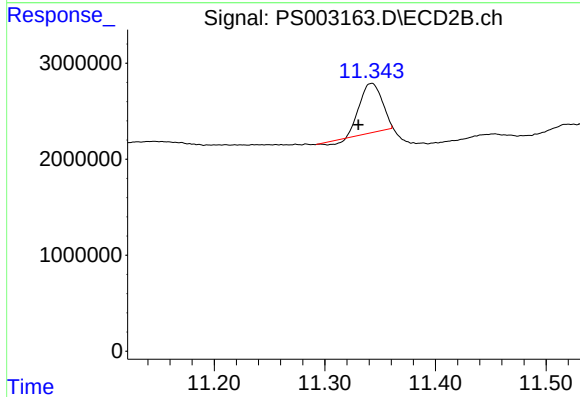

#6 MCP


R.T.: 11.342 min
Delta R.T.: 0.012 min
Response: 7237902
Conc: 6.56 ug/ml

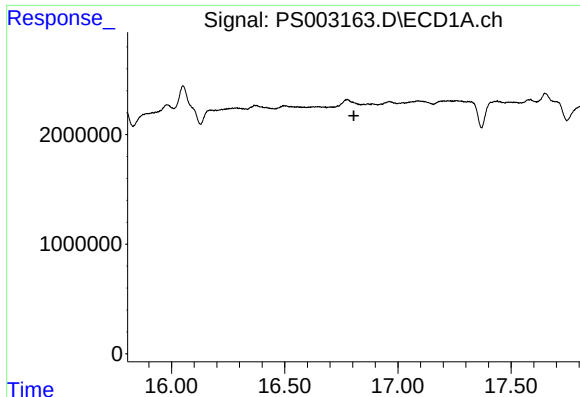

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.806 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

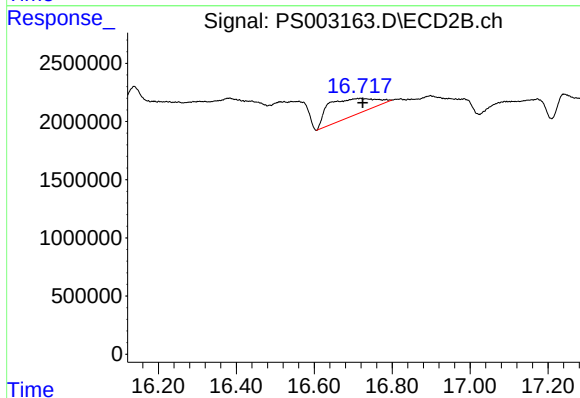


#15 Picloram

R.T.: 16.718 min
Delta R.T.: -0.007 min
Response: 12490830
Conc: 4.15 ng/ml

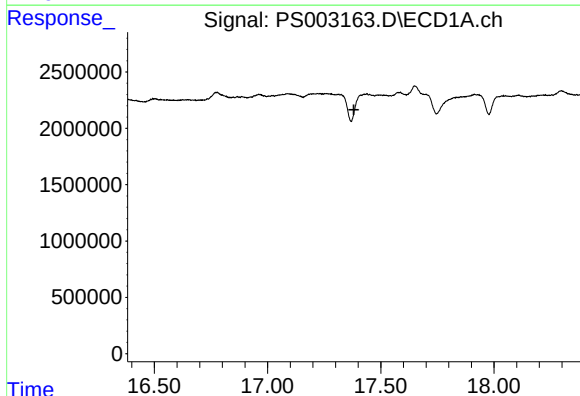

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

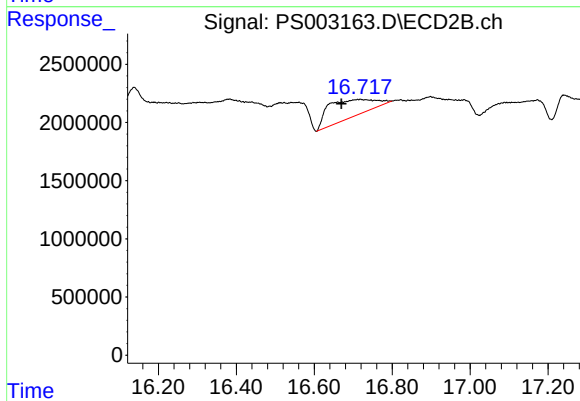

#16 DCPA

R.T.: 16.718 min
Delta R.T.: 0.048 min
Response: 12490830
Conc: 4.03 ng/ml