

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021319\
 Data File : PS003170.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Feb 2019 00:02
 Operator : EI\SJ
 Sample : K1462-24MSD
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 00:51:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.761	0	199.3E6	N.D.	466.064 #
Target Compounds							
1) T	Dalapon	2.822	2.295	-20919271	314.5E6	N.D.	586.843
6) T	MCPD	11.909	11.317	67239909	-3604365	56.121	N.D. #
7) T	MCPA	12.157	11.710	83006241	77112530	46.897	49.021
8) T	DICHLORPROP	0.000	12.165	0	276.9E6	N.D.	724.189 #
11) T	2,4,5-TP ...	14.359	13.797	1753.1E6	1611.2E6	696.143	649.567
12) T	2,4,5-T	14.756	14.429	1680.5E6	-105443229	688.896	N.D. #
14) T	DINOSEB	16.973	0.000	945.3E6	0	502.441	N.D. #
15) T	Picloram	16.745	16.765	1936.1E6	60689656	611.976	20.187 #
16) T	DCPA	17.449	16.668	7650128	1802.4E6	2.544	581.860 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021319\
Data File : PS003170.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Feb 2019 00:02
Operator : EI\SJ
Sample : K1462-24MSD
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 00:51:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

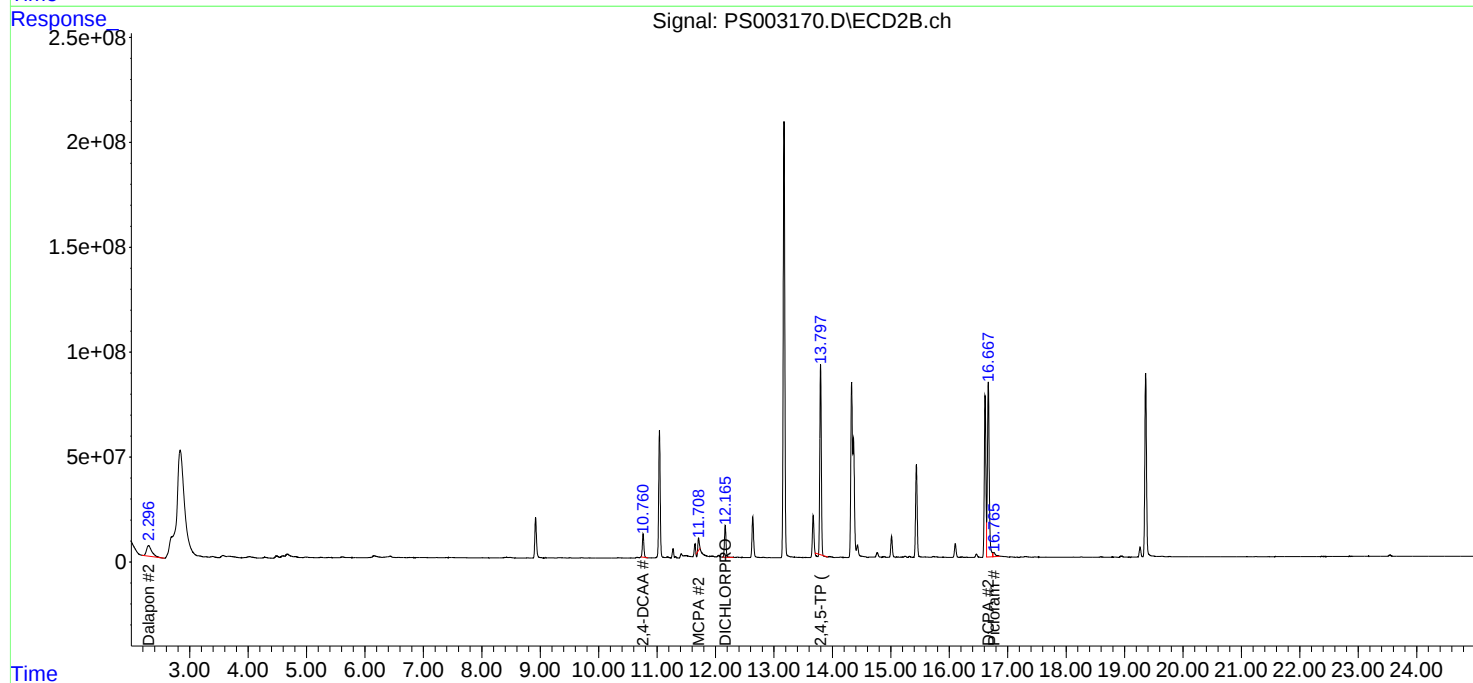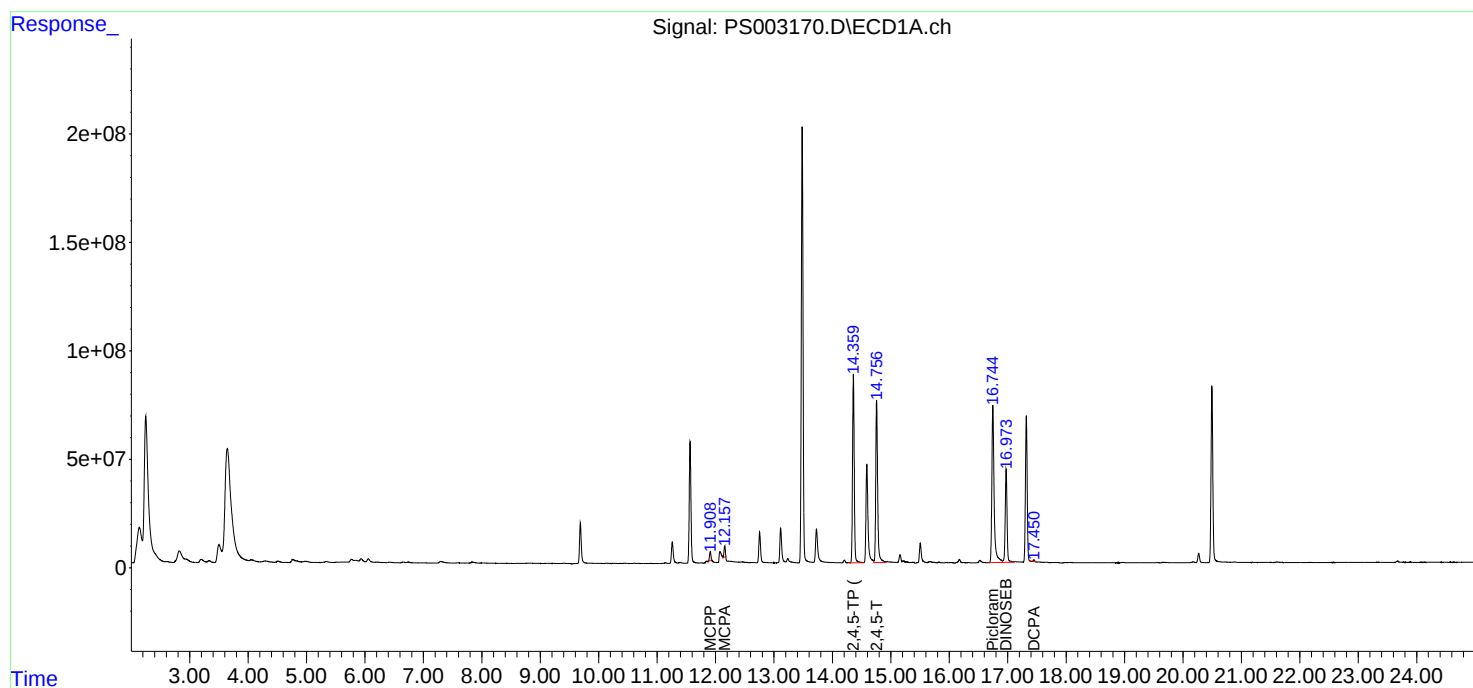


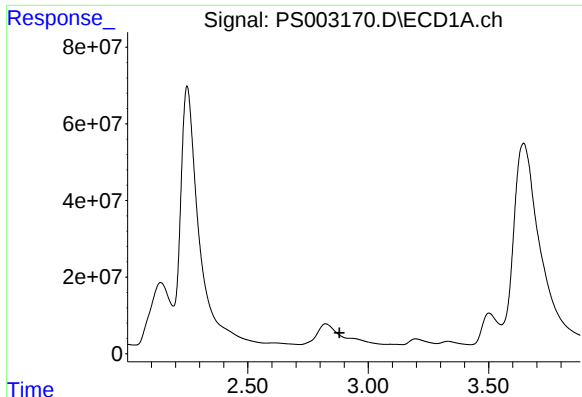

#1 Dalapon


R.T.: 2.822 min
Delta R.T.: -0.058 min
Response: -20919271
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

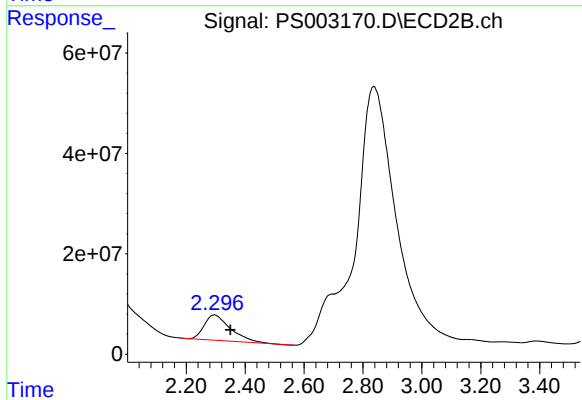


#1 Dalapon

R.T.: 2.295 min
Delta R.T.: -0.056 min
Response: 314501849
Conc: 586.84 ng/ml

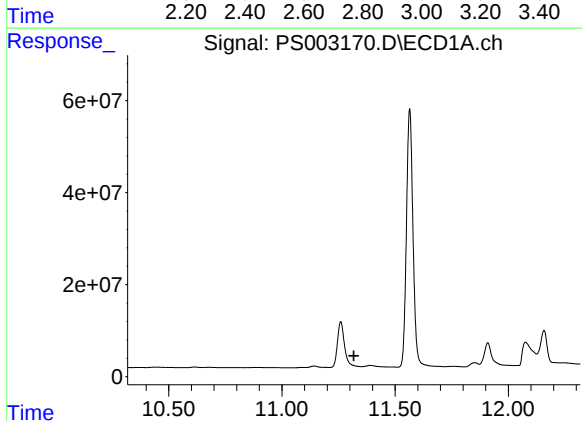


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 11.318 min
Response: 0
Conc: N.D.

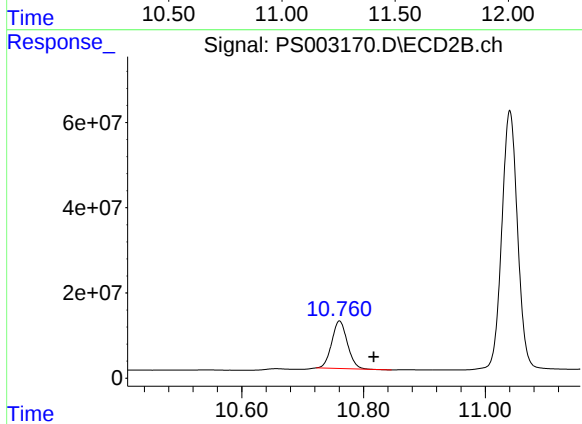

#4 2,4-DCAA


R.T.: 10.761 min
Delta R.T.: -0.056 min
Response: 199263481
Conc: 466.06 ng/ml

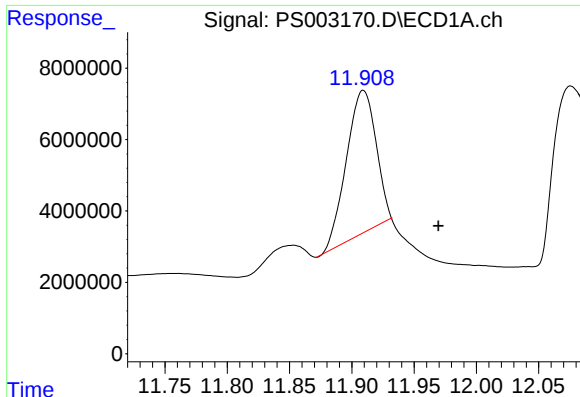

#6 MCPP


R.T.: 11.909 min
Delta R.T.: -0.060 min
Response: 67239909
Conc: 56.12 ug/ml

Instrument :
ECD_S
ClientSampleId :

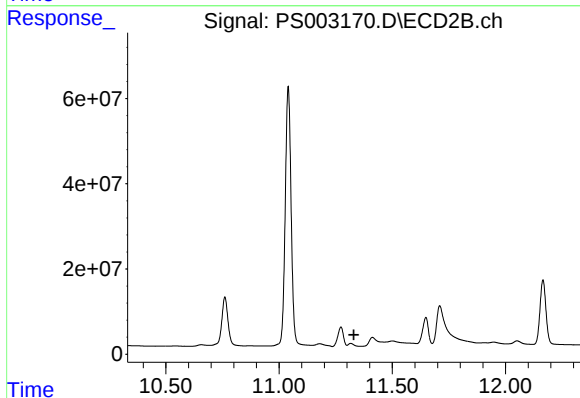


#6 MCPP

R.T.: 11.317 min
Delta R.T.: -0.014 min
Response: -3604365
Conc: N.D.

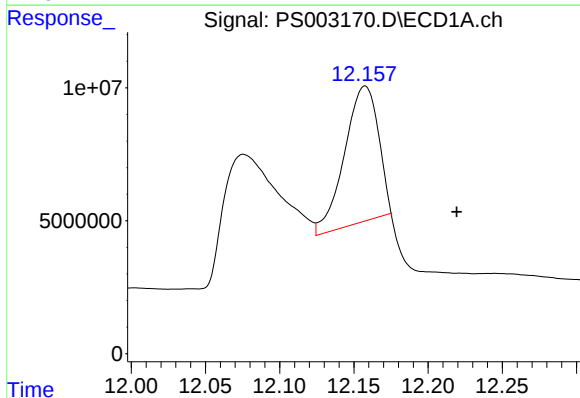


#7 MCPA

R.T.: 12.157 min
Delta R.T.: -0.062 min
Response: 83006241
Conc: 46.90 ug/ml

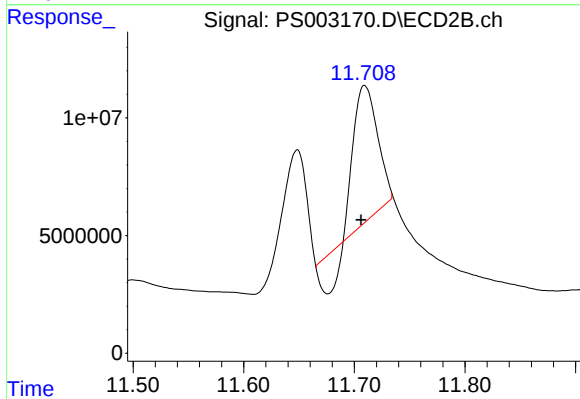

#7 MCPA


R.T.: 11.710 min
Delta R.T.: 0.003 min
Response: 77112530
Conc: 49.02 ug/ml

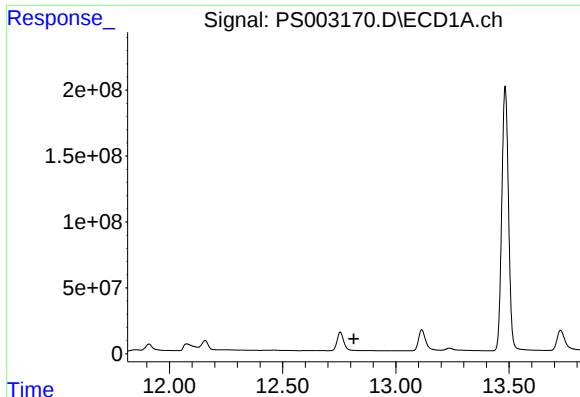

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.815 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

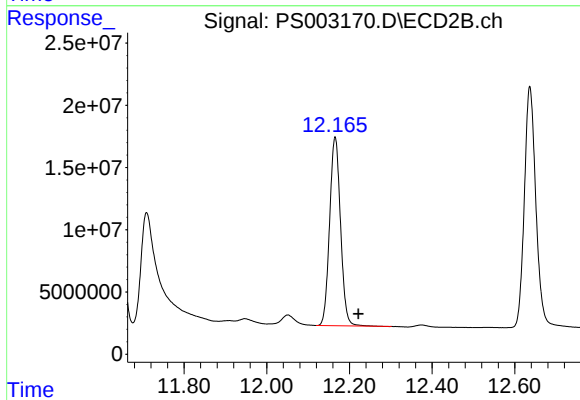


#8 DICHLORPROP

R.T.: 12.165 min
Delta R.T.: -0.057 min
Response: 276887333
Conc: 724.19 ng/ml

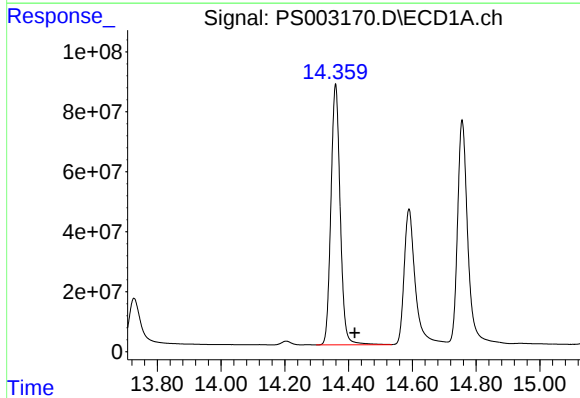


#11 2,4,5-TP (SILVEX)

R.T.: 14.359 min
Delta R.T.: -0.060 min
Response: 1753147733
Conc: 696.14 ng/ml

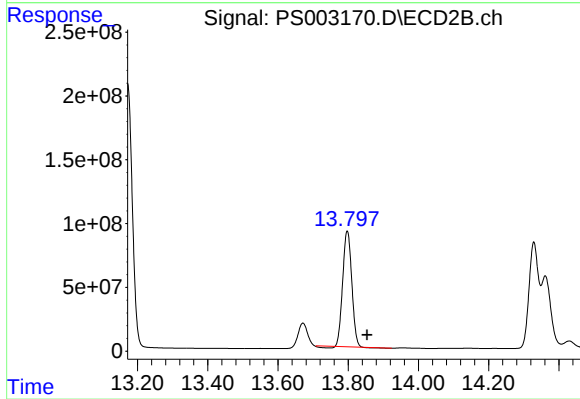

#11 2,4,5-TP (SILVEX)


R.T.: 13.797 min
Delta R.T.: -0.057 min
Response: 1611157199
Conc: 649.57 ng/ml

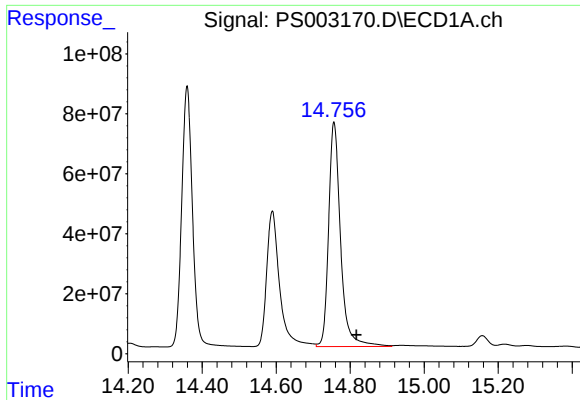

#12 2,4,5-T


R.T.: 14.756 min
Delta R.T.: -0.060 min
Response: 1680497000
Conc: 688.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

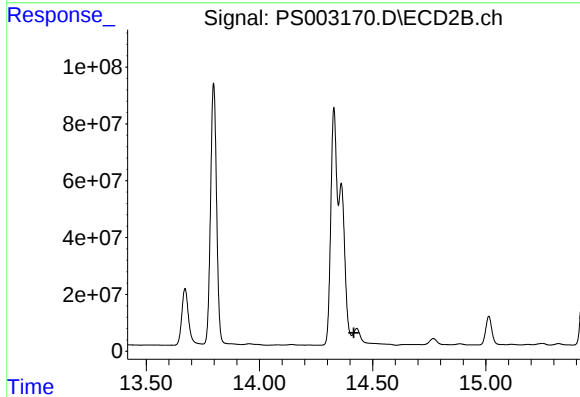


#12 2,4,5-T

R.T.: 14.429 min
Delta R.T.: 0.012 min
Response: -105443229
Conc: N.D.

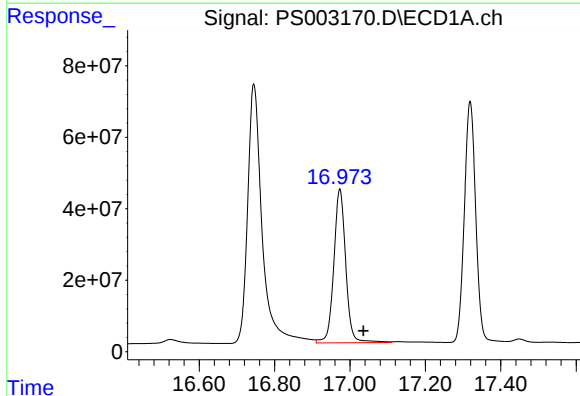


#14 DINOSEB

R.T.: 16.973 min
Delta R.T.: -0.062 min
Response: 945255493
Conc: 502.44 ng/ml

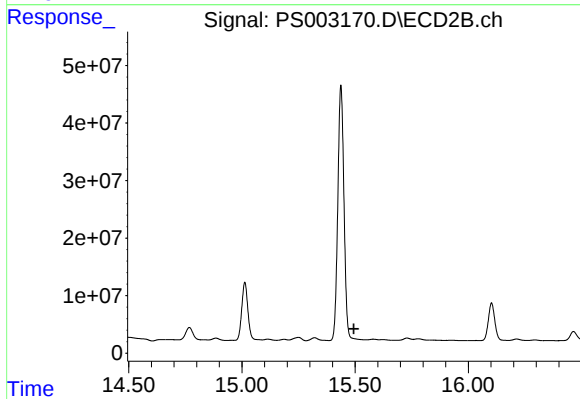

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 15.495 min
Response: 0
Conc: N.D.

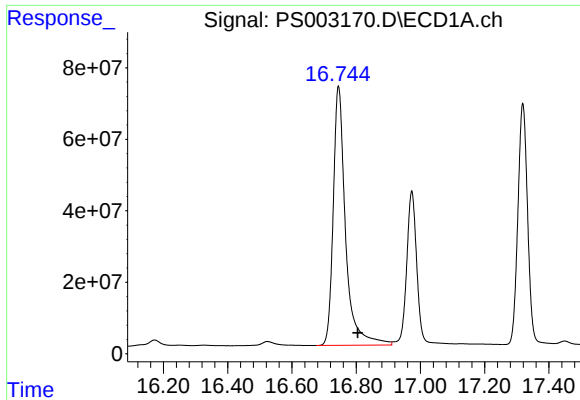

#15 Picloram


R.T.: 16.745 min
Delta R.T.: -0.061 min
Response: 1936066642
Conc: 611.98 ng/ml

Instrument :
ECD_S
ClientSampleId :

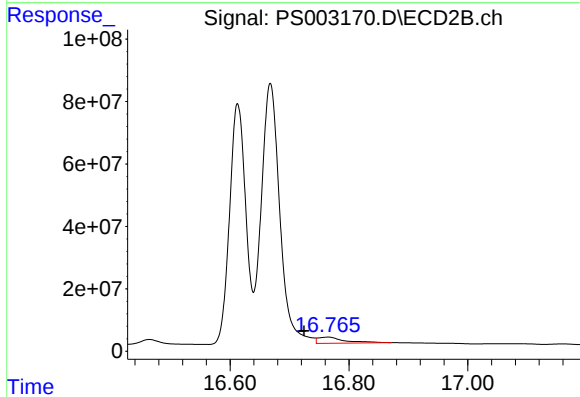


#15 Picloram

R.T.: 16.765 min
Delta R.T.: 0.040 min
Response: 60689656
Conc: 20.19 ng/ml

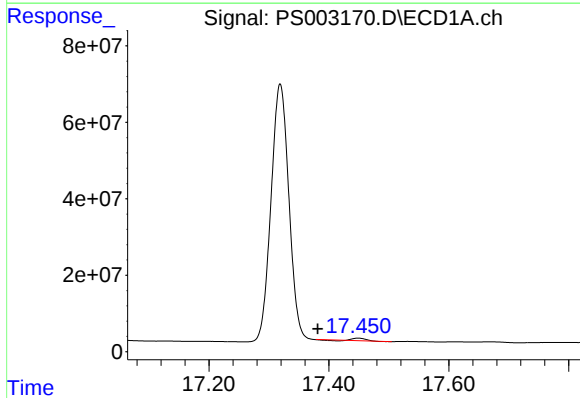

#16 DCPA

R.T.: 17.449 min
Delta R.T.: 0.067 min
Response: 7650128
Conc: 2.54 ng/ml

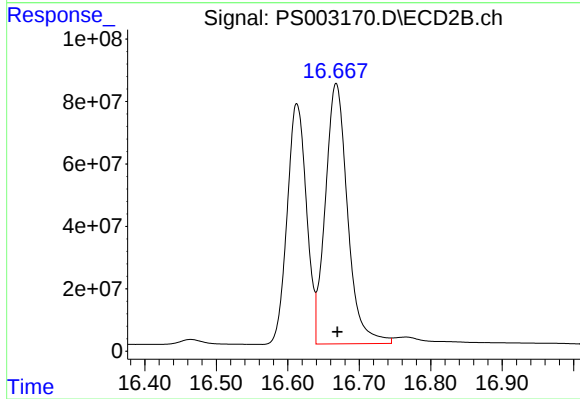

#16 DCPA

R.T.: 16.668 min
Delta R.T.: -0.002 min
Response: 1802364017
Conc: 581.86 ng/ml