

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021319\
 Data File : PS003180.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Feb 2019 05:13
 Operator : EI\SJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 06:50:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.775	0	322.9E6	N.D.	755.176 #
Target Compounds							
1) T	Dalapon	2.837	2.309	30638690	383.9E6	55.540	716.340 #
3) T	4-Nitroph...	0.000	9.925	0	156.3E6	N.D.	747.661 #
8) T	DICHLORPROP	0.000	12.181	0	285.6E6	N.D.	746.882 #
9) T	2,4-D	0.000	12.653	0	167.6E6	N.D.	334.310 #
11) T	2,4,5-TP ...	14.375	13.813	1943.4E6	1793.1E6	771.681	722.911
12) T	2,4,5-T	14.774	14.377	1888.9E6	-139461623	774.346	N.D. #
14) T	DINOSEB	16.988	0.000	1449.3E6	0	770.343	N.D. #
15) T	Picloram	16.764	16.684	2313.5E6	2183.5E6	731.290	726.288
16) T	DCPA	0.000	16.684	0	2183.5E6	N.D.	704.908 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021319\
Data File : PS003180.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Feb 2019 05:13
Operator : EI\SJ
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 06:50:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

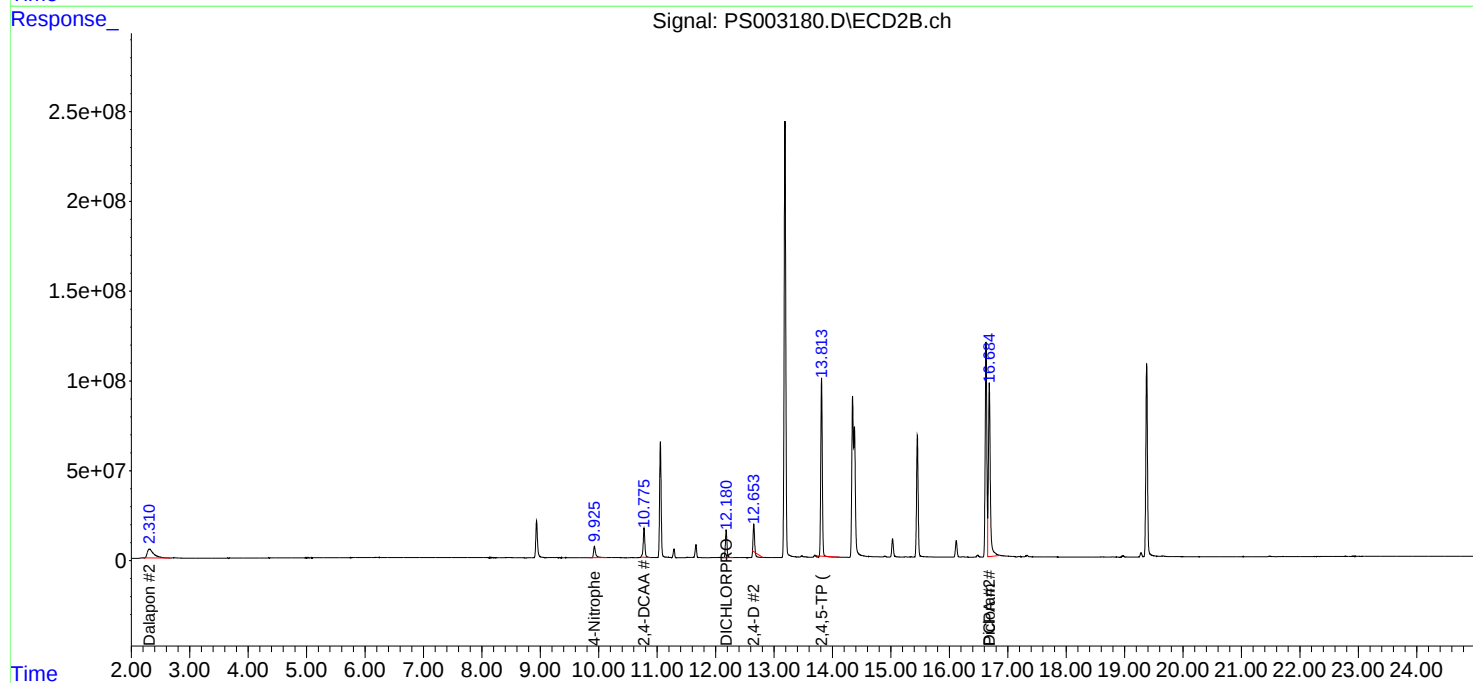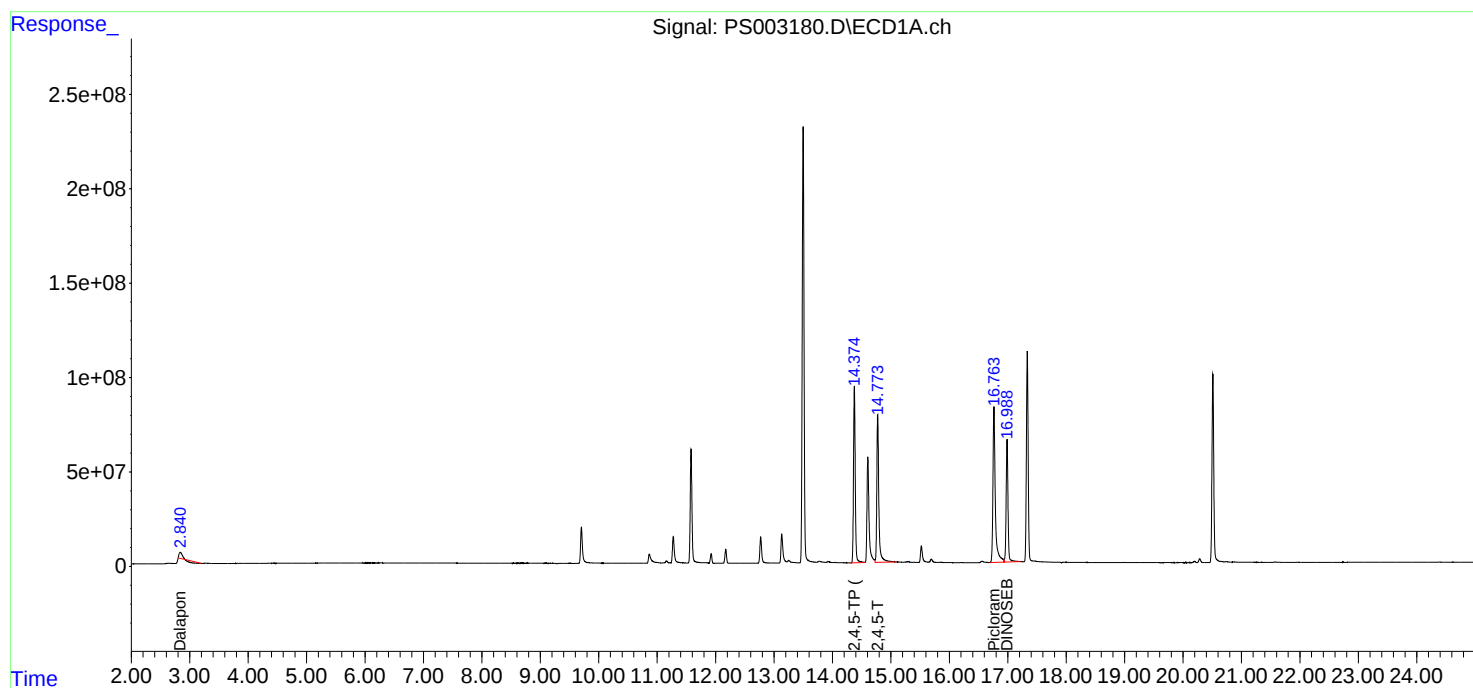


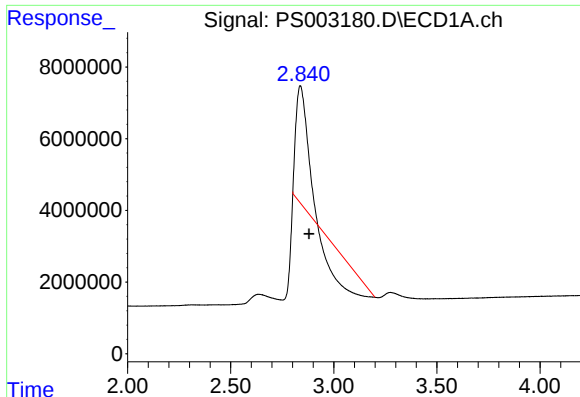

#1 Dalapon


R.T.: 2.837 min
Delta R.T.: -0.043 min
Response: 30638690
Conc: 55.54 ng/ml

Instrument :
ECD_S
ClientSampleId :

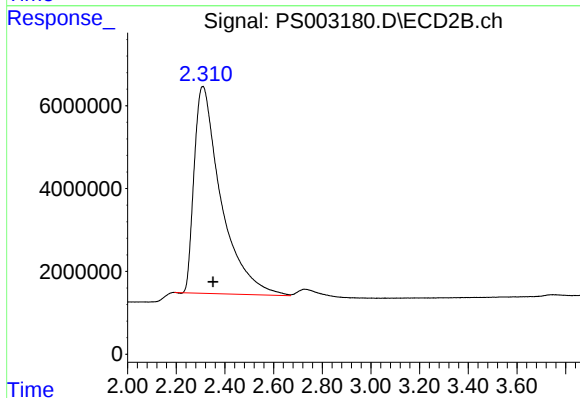


#1 Dalapon

R.T.: 2.309 min
Delta R.T.: -0.042 min
Response: 383901684
Conc: 716.34 ng/ml

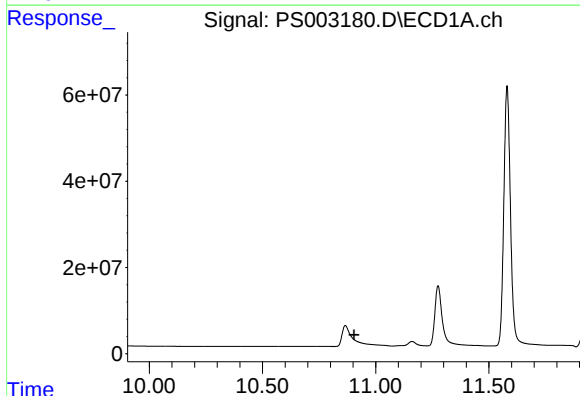


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 10.904 min
Response: 0
Conc: N.D.

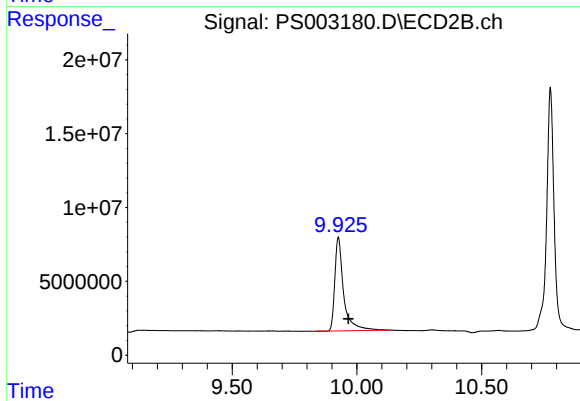

#3 4-Nitrophenol


R.T.: 9.925 min
Delta R.T.: -0.040 min
Response: 156277843
Conc: 747.66 ng/ml

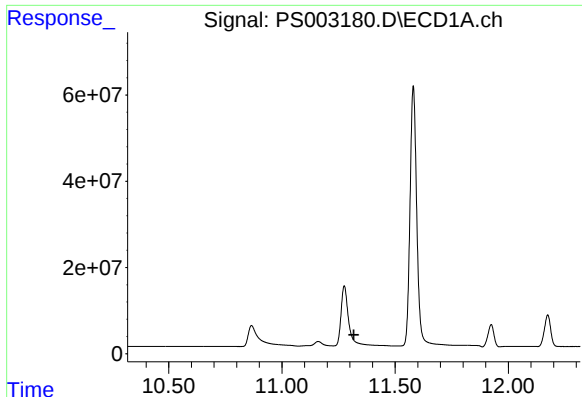

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 11.318 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

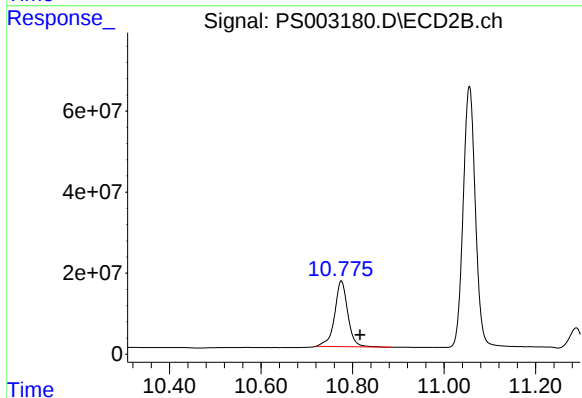


#4 2,4-DCAA

R.T.: 10.775 min
Delta R.T.: -0.041 min
Response: 322872374
Conc: 755.18 ng/ml

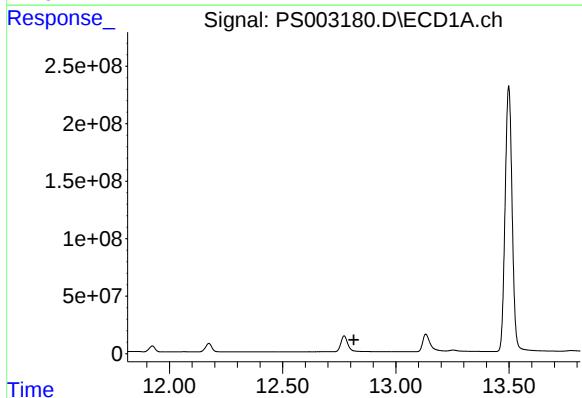


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.815 min
Response: 0
Conc: N.D.

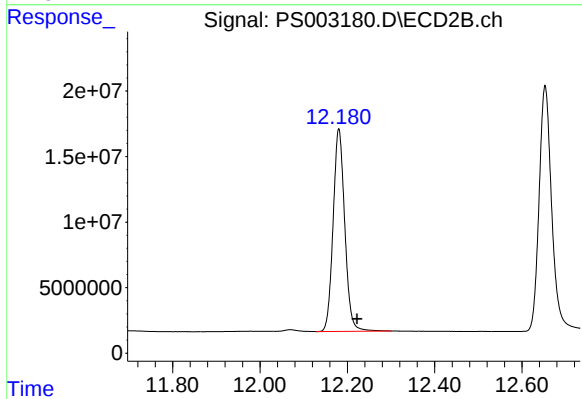

#8 DICHLORPROP


R.T.: 12.181 min
Delta R.T.: -0.042 min
Response: 285563688
Conc: 746.88 ng/ml

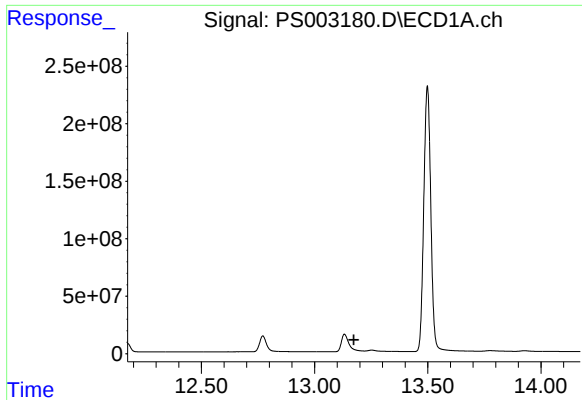

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.173 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

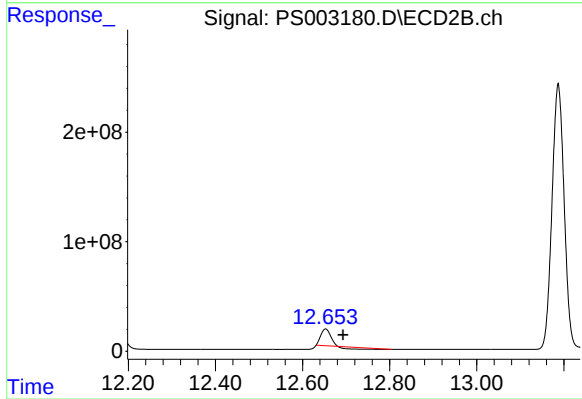


#9 2,4-D

R.T.: 12.653 min
Delta R.T.: -0.040 min
Response: 167618218
Conc: 334.31 ng/ml

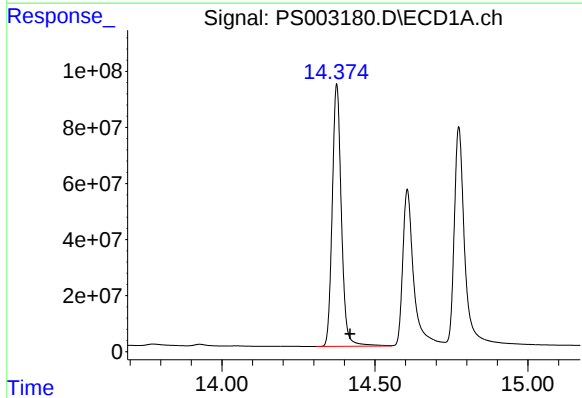


#11 2,4,5-TP (SILVEX)

R.T.: 14.375 min
Delta R.T.: -0.044 min
Response: 1943381272
Conc: 771.68 ng/ml

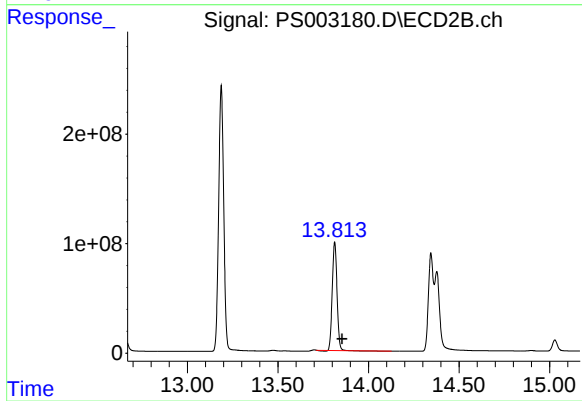

#11 2,4,5-TP (SILVEX)


R.T.: 13.813 min
Delta R.T.: -0.041 min
Response: 1793076836
Conc: 722.91 ng/ml

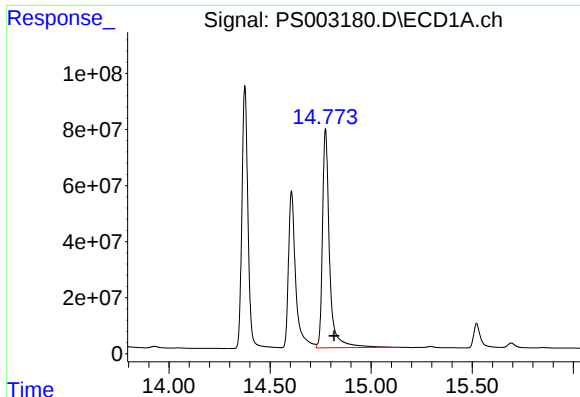

#12 2,4,5-T


R.T.: 14.774 min
Delta R.T.: -0.042 min
Response: 1888942283
Conc: 774.35 ng/ml

Instrument :
ECD_S
ClientSampleId :

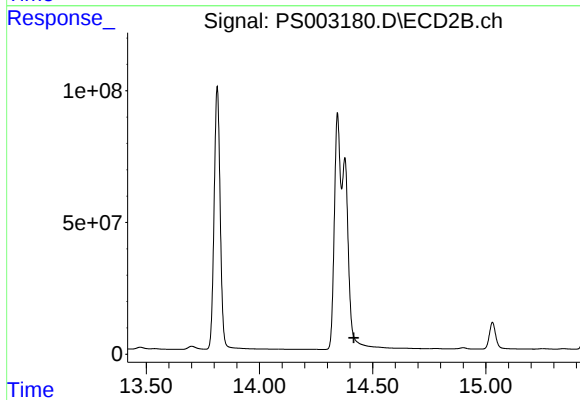


#12 2,4,5-T

R.T.: 14.377 min
Delta R.T.: -0.040 min
Response: -139461623
Conc: N.D.

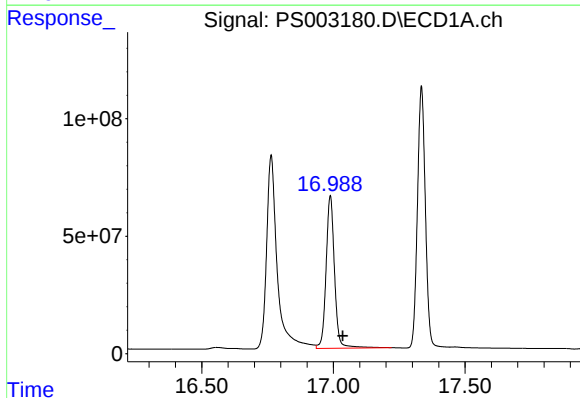


#14 DINOSEB

R.T.: 16.988 min
Delta R.T.: -0.047 min
Response: 1449267854
Conc: 770.34 ng/ml

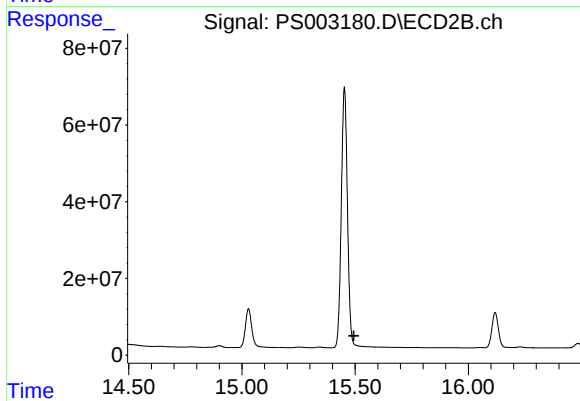

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 15.495 min
Response: 0
Conc: N.D.

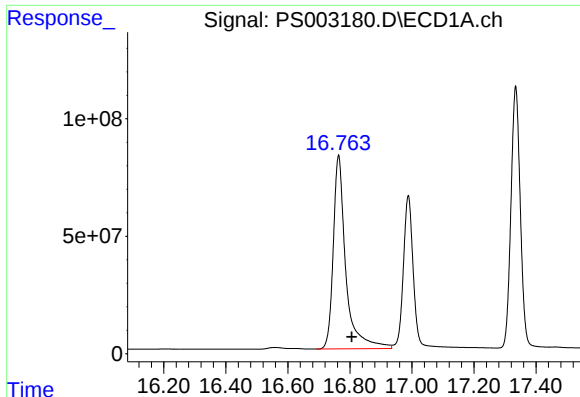

#15 Picloram


R.T.: 16.764 min
Delta R.T.: -0.042 min
Response: 2313534113
Conc: 731.29 ng/ml

Instrument :
ECD_S
ClientSampleId :

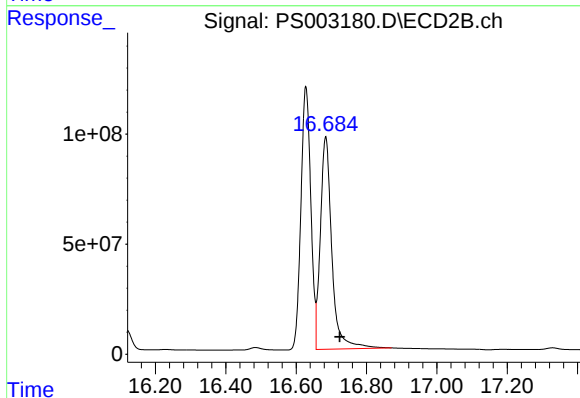


#15 Picloram

R.T.: 16.684 min
Delta R.T.: -0.040 min
Response: 2183515761
Conc: 726.29 ng/ml

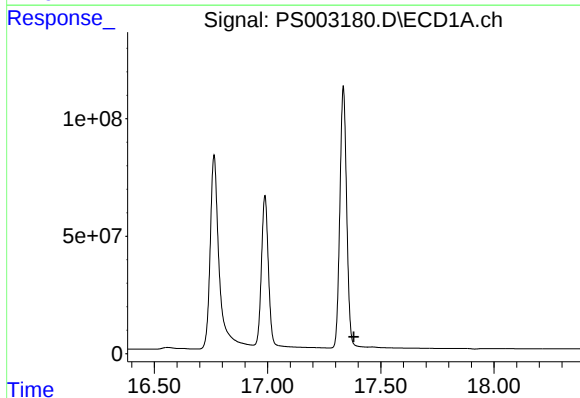

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

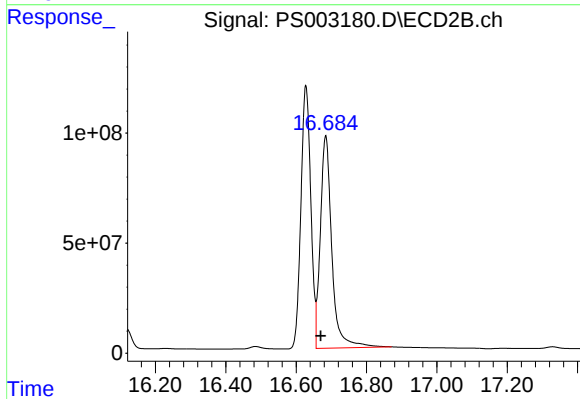

#16 DCPA

R.T.: 16.684 min
Delta R.T.: 0.014 min
Response: 2183515761
Conc: 704.91 ng/ml