

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021320\
 Data File : PS008834.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Feb 2020 16:47
 Operator : DD\AJ
 Sample : PB126796BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 02:07:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 05 02:36:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.248	6.942	1126.9E6	537.5E6	525.019	579.916
Target Compounds							
1) T	Dalapon	0.000	2.594	0	245.3E6	N.D.	204.499
2) T	3,5-DICHL...	0.000	6.117	0	75248468	N.D.	54.691
7) T	MCPA	7.800	7.410	75843799	83215080	8.829	19.939 #
12) T	2,4,5-T	0.000	9.263	0	48097808	N.D.	9.308
15) T	Picloram	11.046	11.034	506.6E6	276.4E6	33.450	36.613
16) T	DCPA	0.000	11.034	0	276.4E6	N.D.	42.489



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021320\
Data File : PS008834.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Feb 2020 16:47
Operator : DD\AJ
Sample : PB126796BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 02:07:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
Quant Title : 8080.M
QLast Update : Wed Feb 05 02:36:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

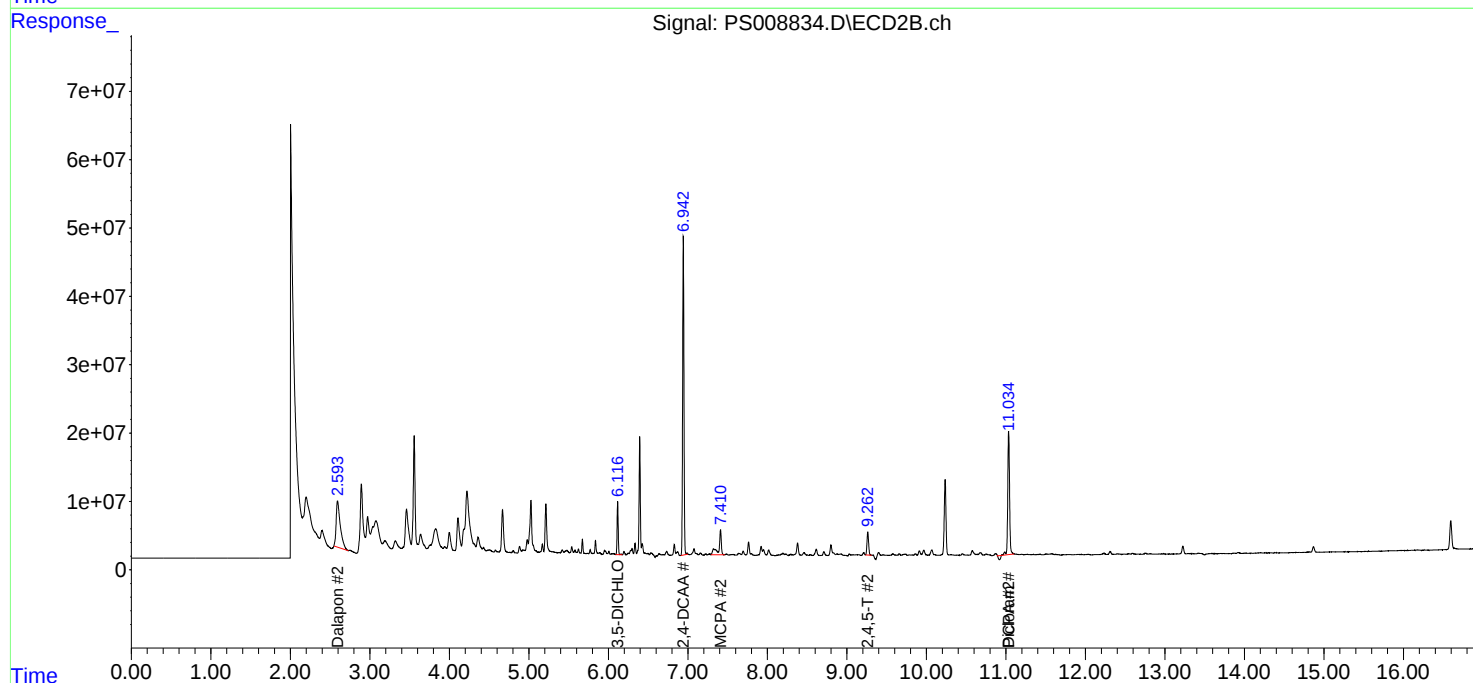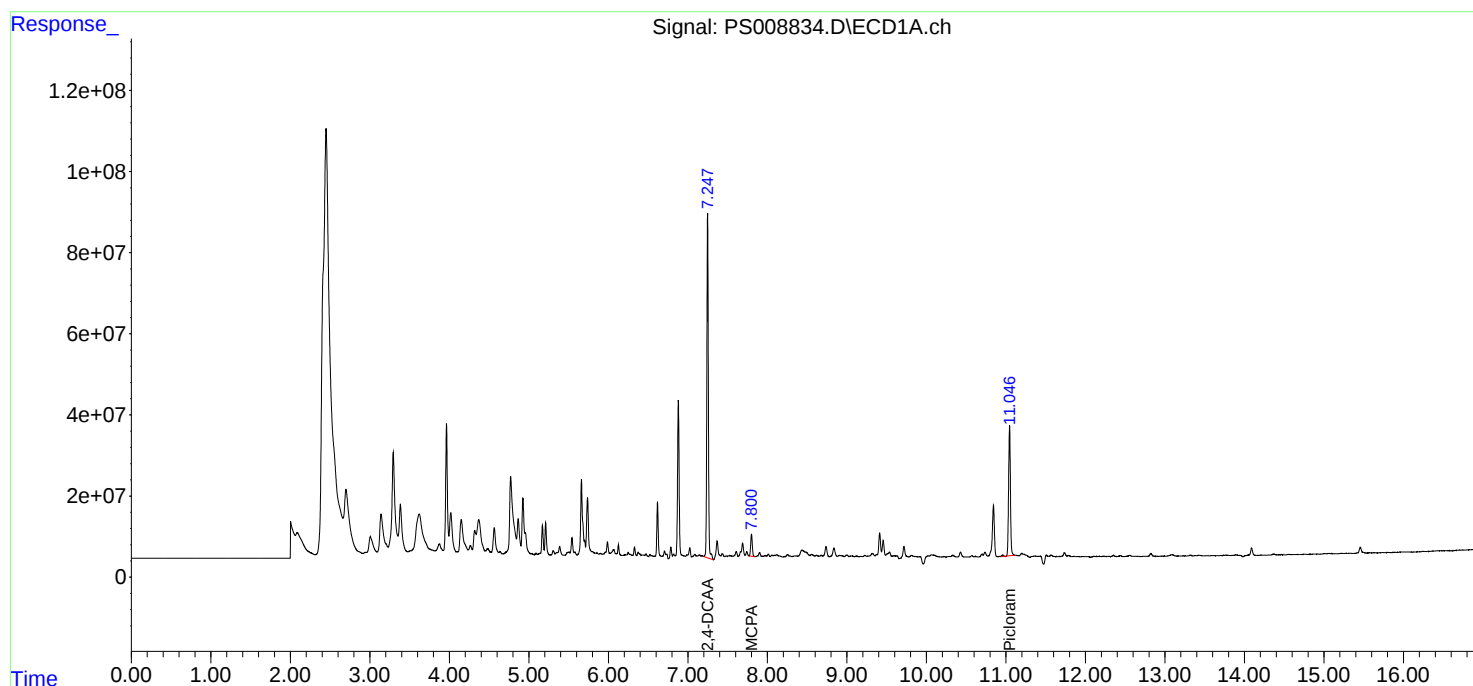


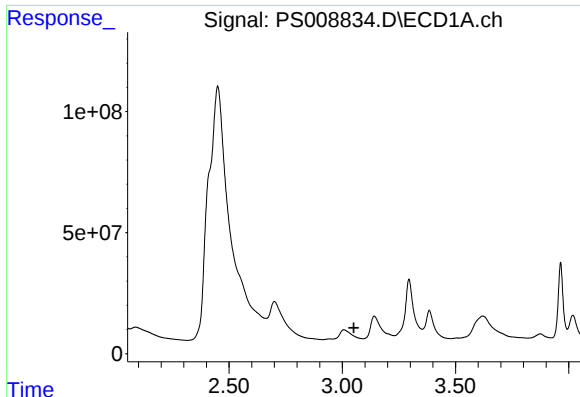

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.051 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

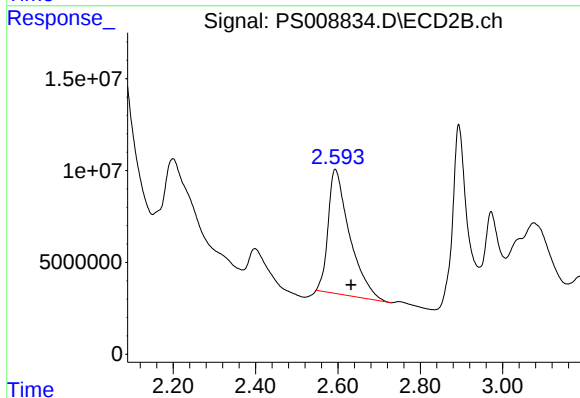


#1 Dalapon

R.T.: 2.594 min
Delta R.T.: -0.038 min
Response: 245258883
Conc: 204.50 ng/ml

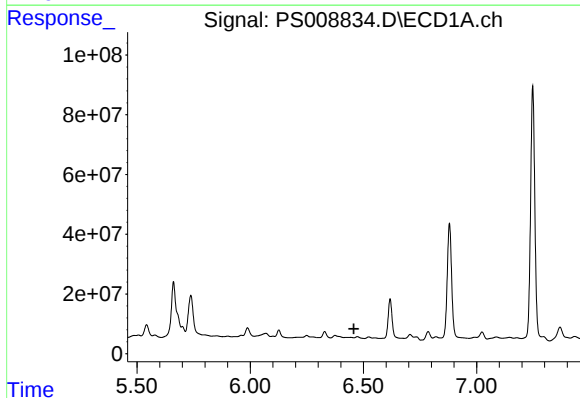


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.458 min
Response: 0
Conc: N.D.

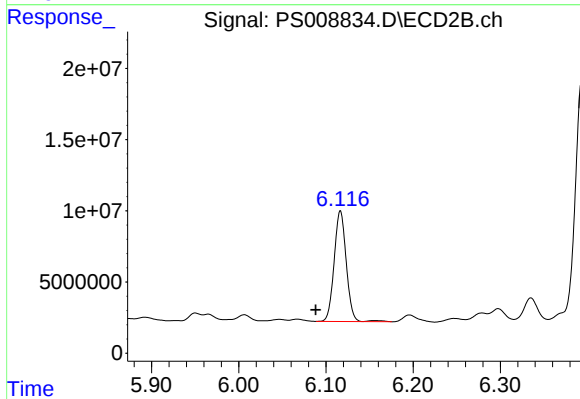

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.117 min
Delta R.T.: 0.028 min
Response: 75248468
Conc: 54.69 ng/ml

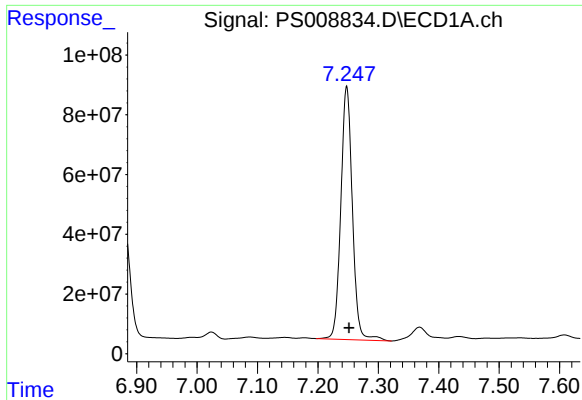

#4 2,4-DCAA


R.T.: 7.248 min
Delta R.T.: -0.004 min
Response: 1126853694
Conc: 525.02 ng/ml

Instrument :
ECD_S
ClientSampleId :

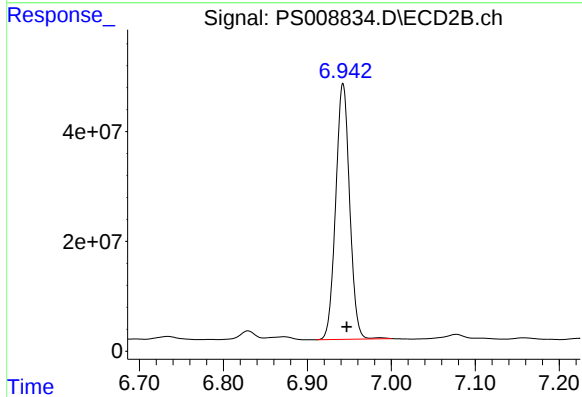


#4 2,4-DCAA

R.T.: 6.942 min
Delta R.T.: -0.004 min
Response: 537480460
Conc: 579.92 ng/ml

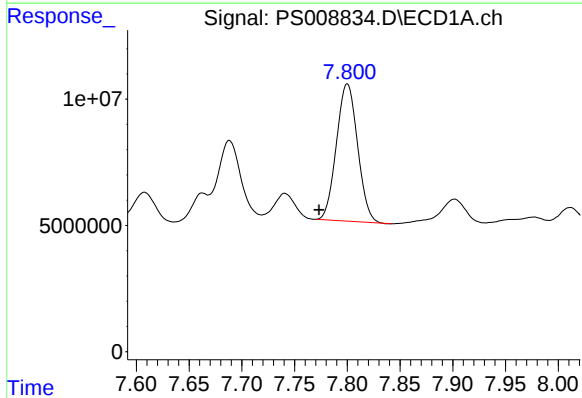


#7 MCPA

R.T.: 7.800 min
Delta R.T.: 0.027 min
Response: 75843799
Conc: 8.83 ug/ml

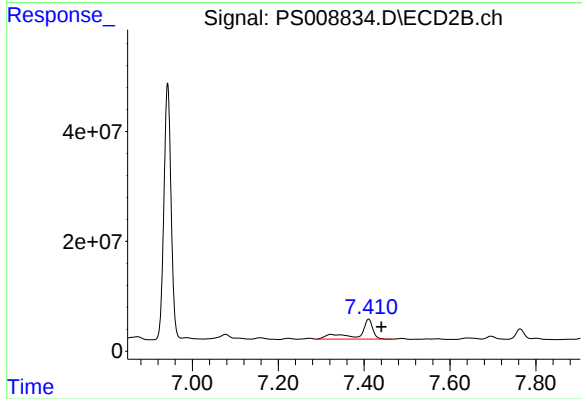

#7 MCPA


R.T.: 7.410 min
Delta R.T.: -0.030 min
Response: 83215080
Conc: 19.94 ug/ml

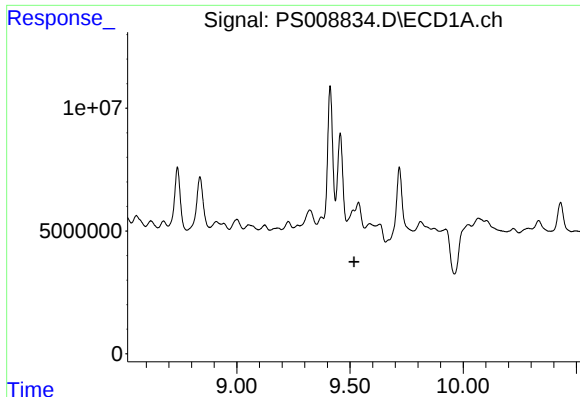

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.517 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

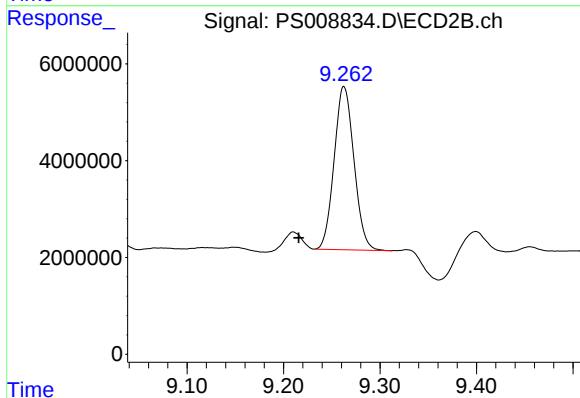


#12 2,4,5-T

R.T.: 9.263 min
Delta R.T.: 0.047 min
Response: 48097808
Conc: 9.31 ng/ml

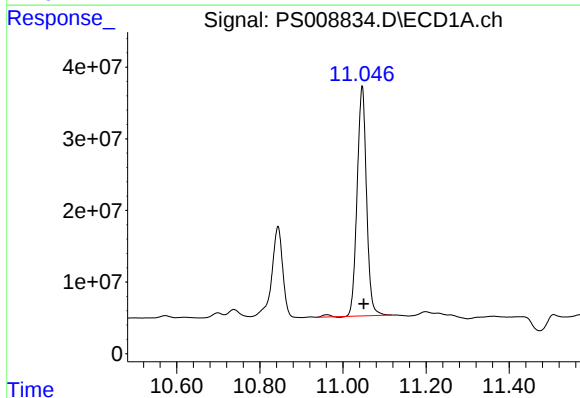


#15 Picloram

R.T.: 11.046 min
Delta R.T.: -0.004 min
Response: 506566439
Conc: 33.45 ng/ml

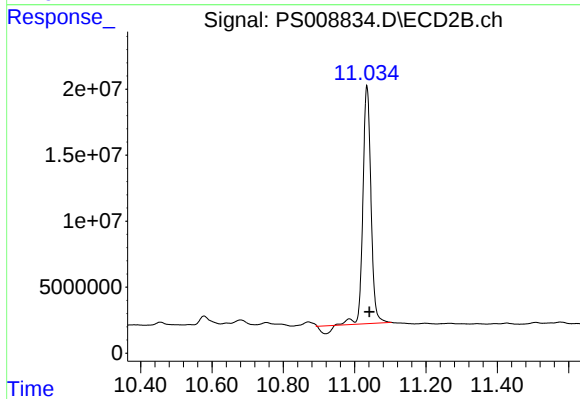

#15 Picloram


R.T.: 11.034 min
Delta R.T.: -0.007 min
Response: 276355319
Conc: 36.61 ng/ml

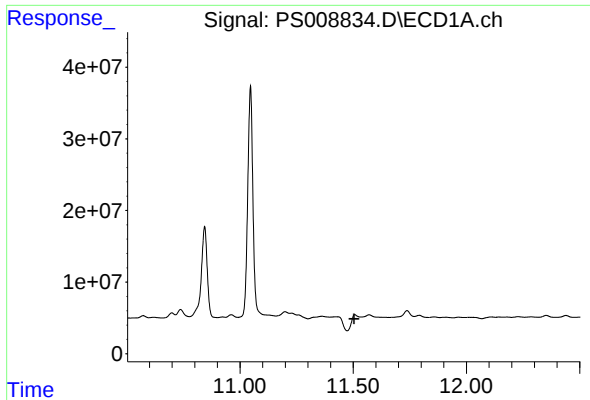

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.503 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

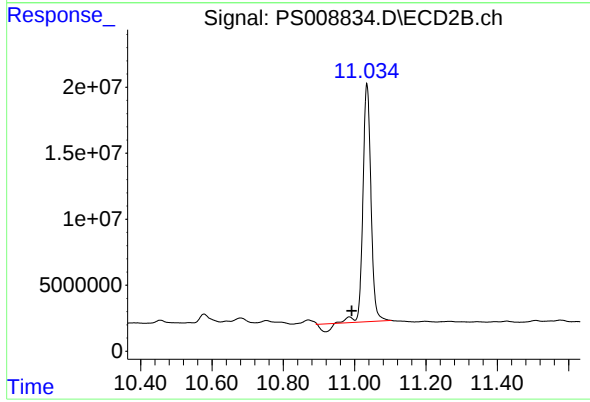

#16 DCPA

R.T.: 11.034 min
Delta R.T.: 0.042 min
Response: 276355319
Conc: 42.49 ng/ml