

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021320\
 Data File : PS008846.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Feb 2020 21:22
 Operator : DD\AJ
 Sample : L1385-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 02:09:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 05 02:36:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.247	6.943	945.2E6	454.5E6	440.381	490.421
Target Compounds							
2) T	3,5-DICHL...	0.000	6.117	0	155.0E6	N.D.	112.669
11) T	2,4,5-TP ...	0.000	8.799	0	67811602	N.D.	13.231
12) T	2,4,5-T	0.000	9.263	0	59595570	N.D.	11.533
15) T	Picloram	11.044	11.035	353.4E6	192.9E6	23.335	25.550
16) T	DCPA	0.000	11.035	0	192.9E6	N.D.	29.650



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021320\
Data File : PS008846.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Feb 2020 21:22
Operator : DD\AJ
Sample : L1385-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 02:09:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
Quant Title : 8080.M
QLast Update : Wed Feb 05 02:36:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

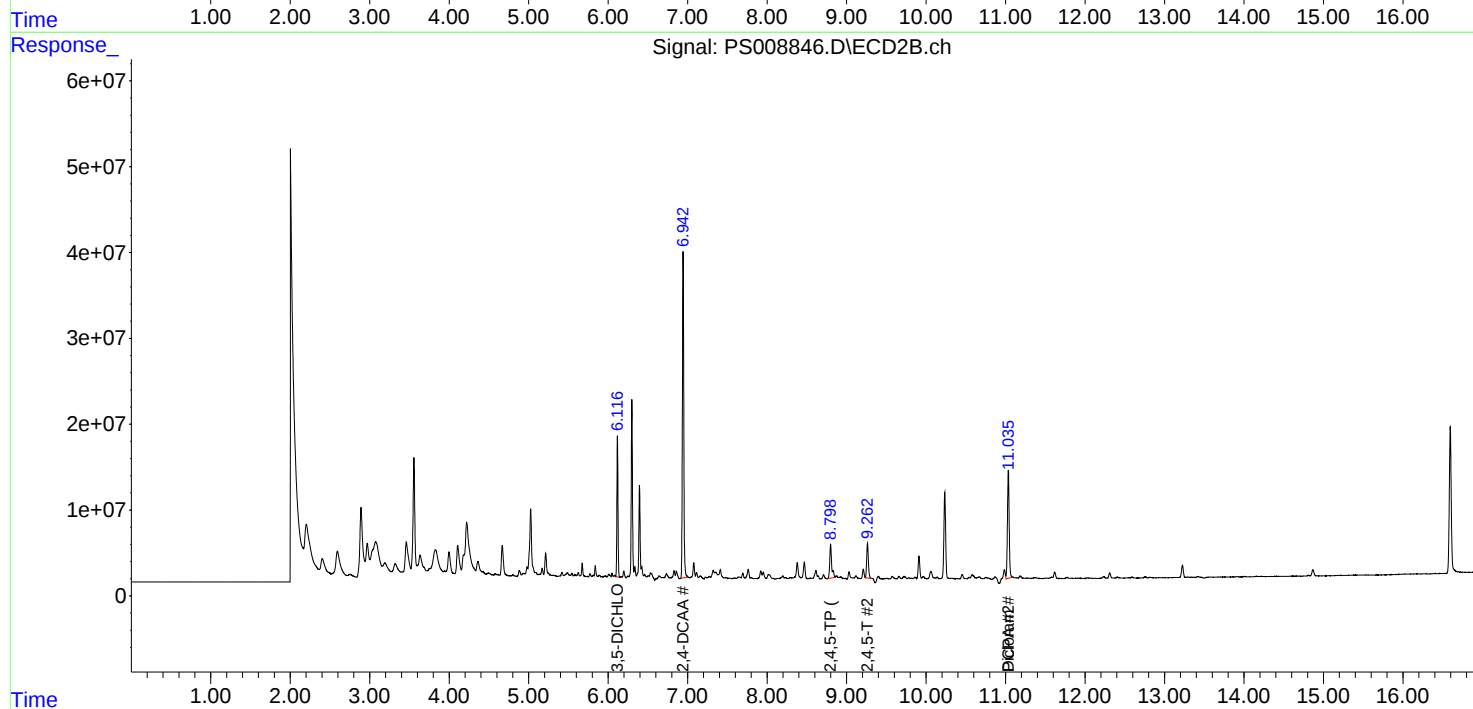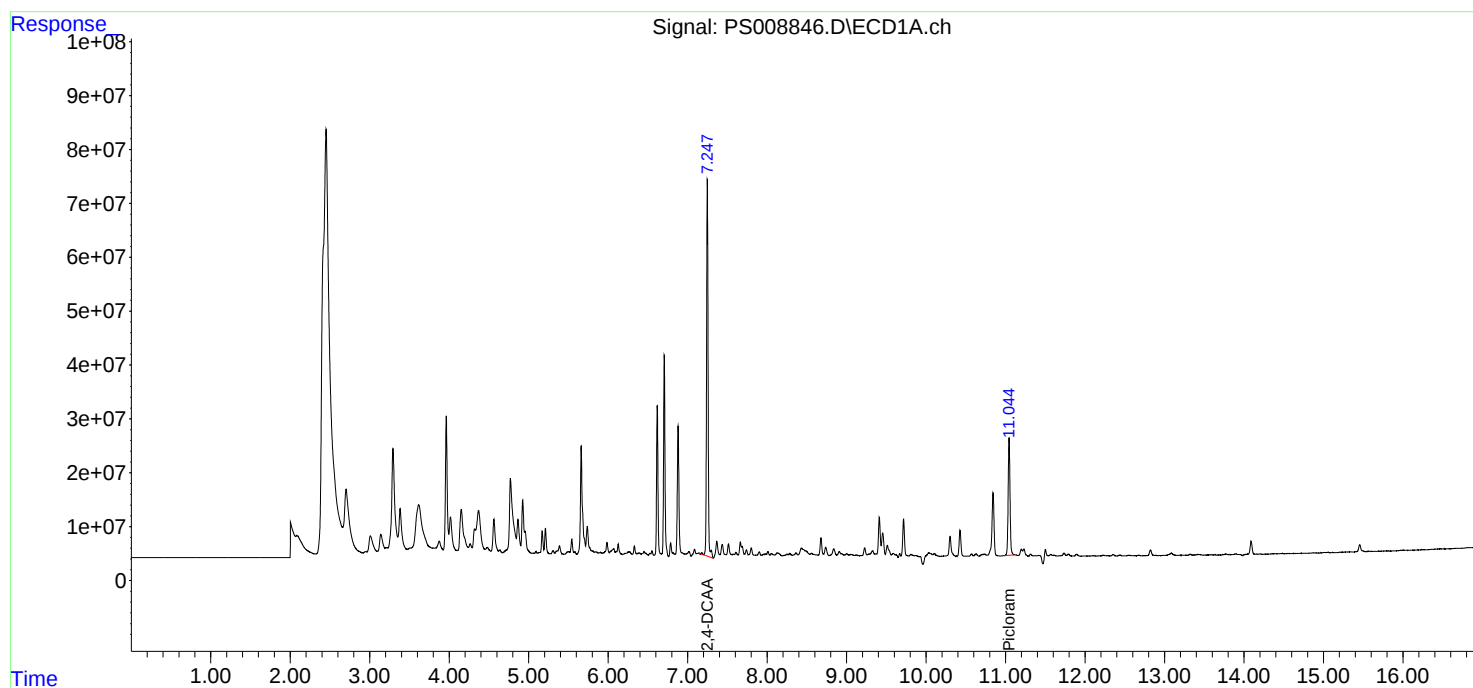


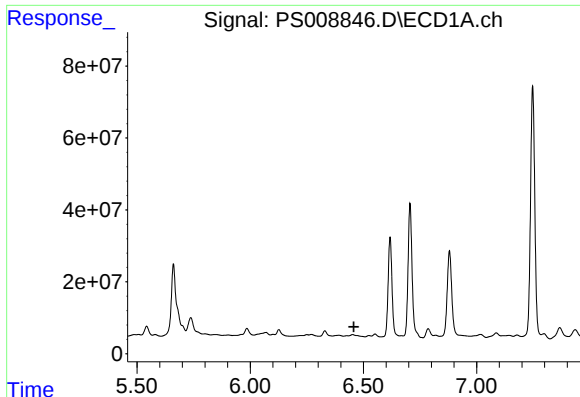

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.458 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

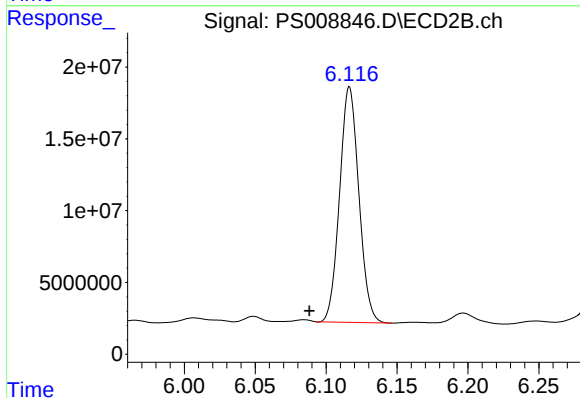


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.117 min
Delta R.T.: 0.028 min
Response: 155019527
Conc: 112.67 ng/ml

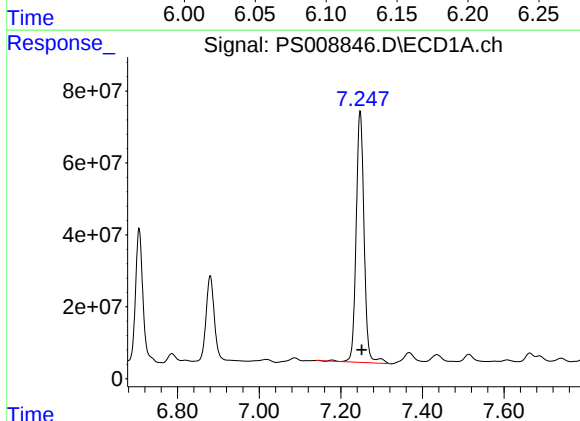


#4 2,4-DCAA

R.T.: 7.247 min
Delta R.T.: -0.004 min
Response: 945193275
Conc: 440.38 ng/ml

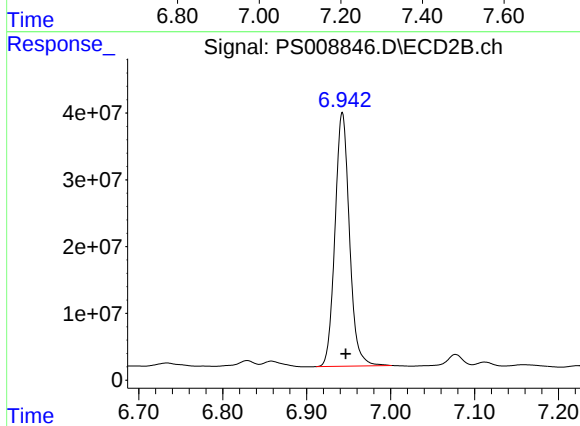

#4 2,4-DCAA


R.T.: 6.943 min
Delta R.T.: -0.004 min
Response: 454533776
Conc: 490.42 ng/ml

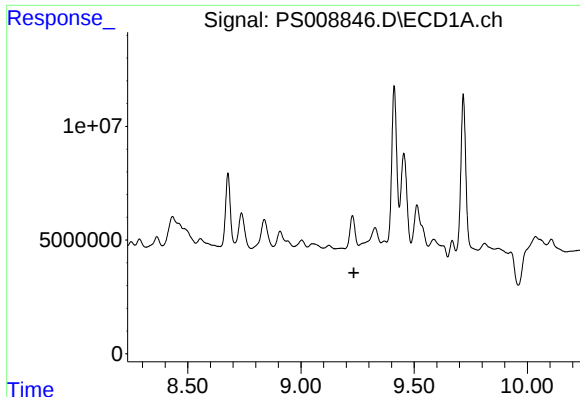

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.234 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

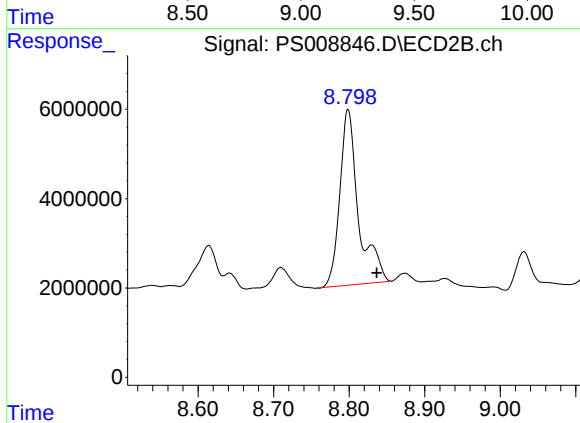


#11 2,4,5-TP (SILVEX)

R.T.: 8.799 min
Delta R.T.: -0.038 min
Response: 67811602
Conc: 13.23 ng/ml

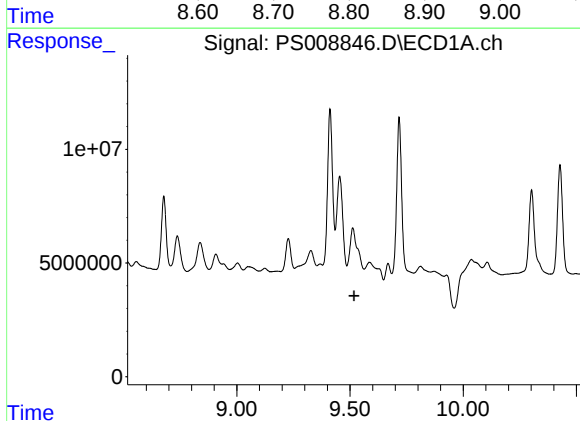


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 9.517 min
Response: 0
Conc: N.D.

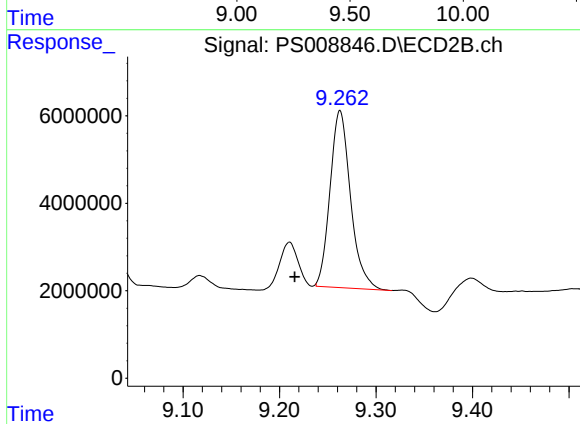

#12 2,4,5-T


R.T.: 9.263 min
Delta R.T.: 0.047 min
Response: 59595570
Conc: 11.53 ng/ml

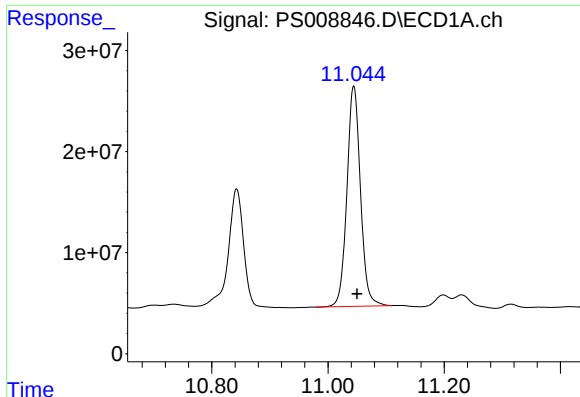

#15 Picloram


R.T.: 11.044 min
Delta R.T.: -0.005 min
Response: 353380950
Conc: 23.34 ng/ml

Instrument :
ECD_S
ClientSampleId :

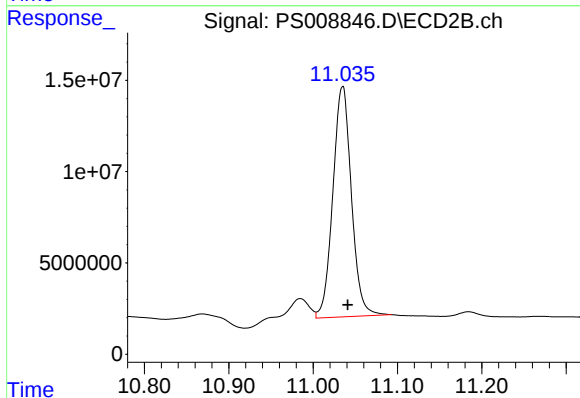


#15 Picloram

R.T.: 11.035 min
Delta R.T.: -0.006 min
Response: 192851512
Conc: 25.55 ng/ml

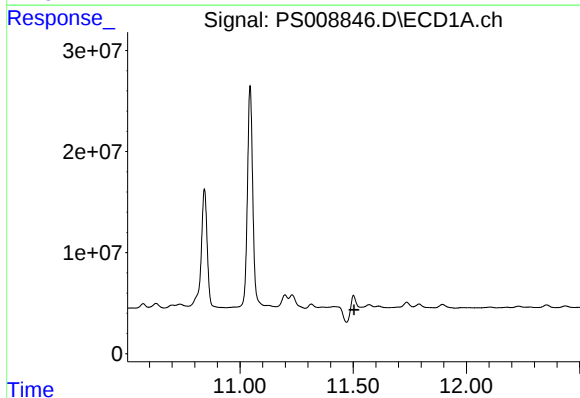

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.503 min
Response: 0
Conc: N.D.

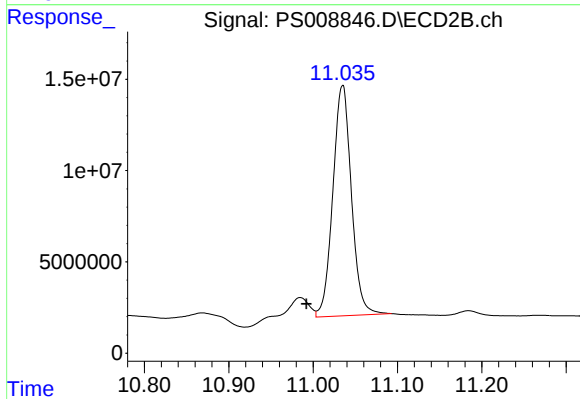

#16 DCPA

R.T.: 11.035 min
Delta R.T.: 0.043 min
Response: 192851512
Conc: 29.65 ng/ml