

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021320\
 Data File : PS008848.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Feb 2020 22:07
 Operator : DD\AJ
 Sample : L1509-12
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 02:10:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 05 02:36:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.247	6.942	811.3E6	406.1E6	377.998	438.135
Target Compounds							
2) T	3,5-DICHL...	0.000	6.116	0	139.4E6	N.D.	101.305
6) T	MCP	7.691	0.000	104.0E6	0	16.913	N.D. #
9) T	2,4-D	8.429	0.000	68547637	0	32.031	N.D. #
12) T	2,4,5-T	9.454	0.000	89306719	0	8.114	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021320\
Data File : PS008848.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Feb 2020 22:07
Operator : DD\AJ
Sample : L1509-12
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 02:10:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
Quant Title : 8080.M
QLast Update : Wed Feb 05 02:36:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

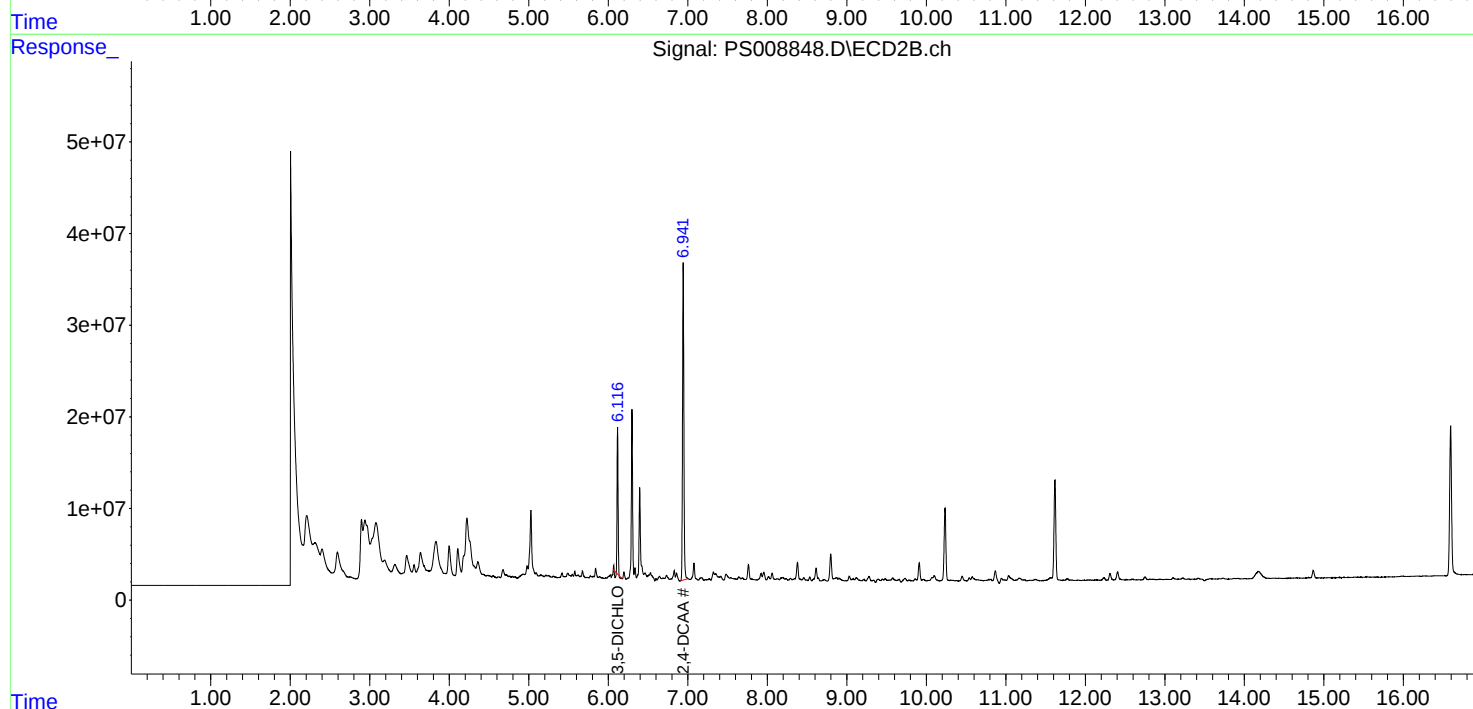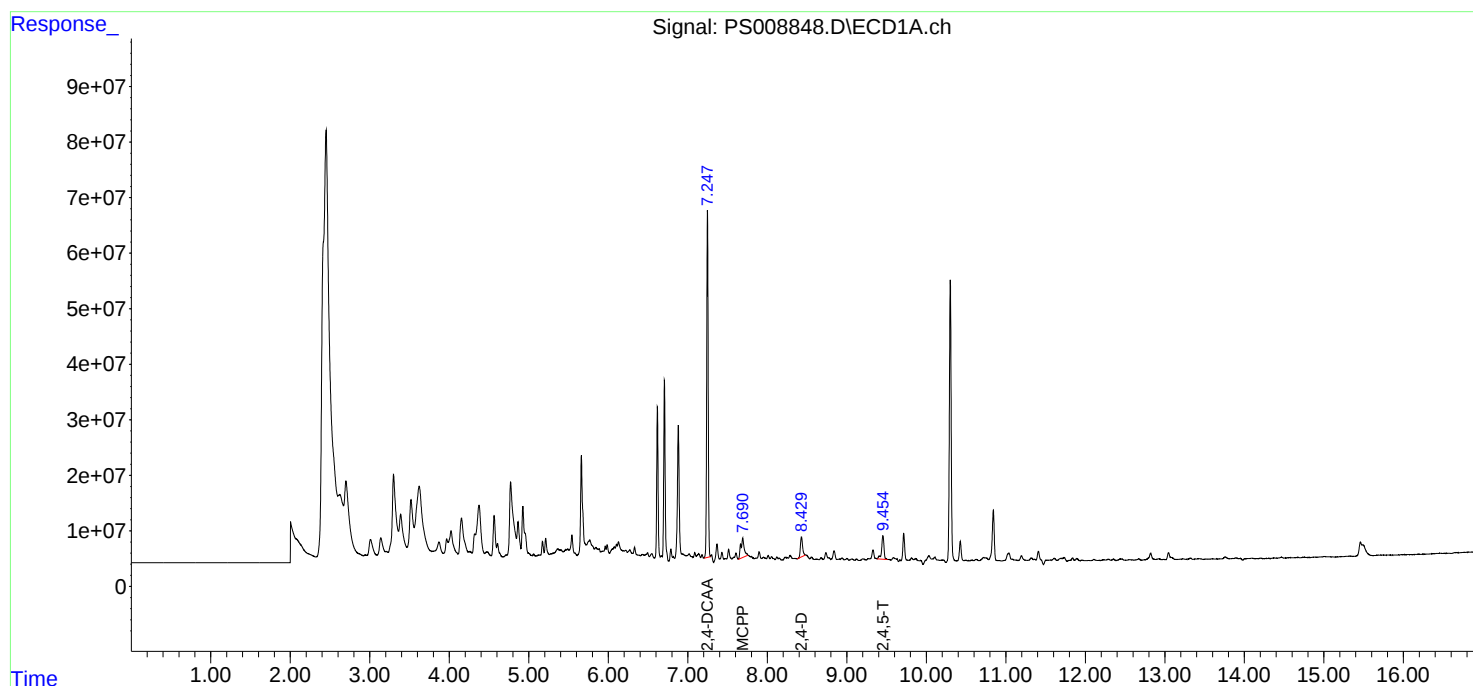


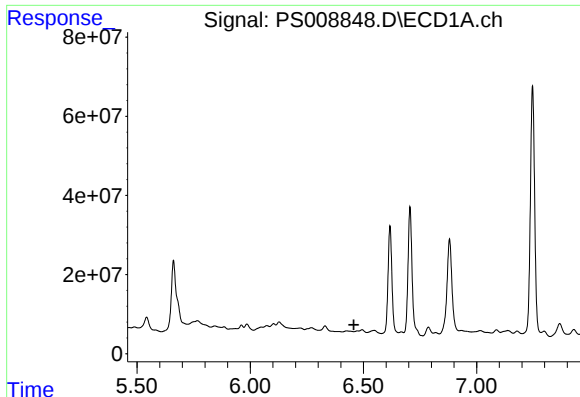

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.458 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

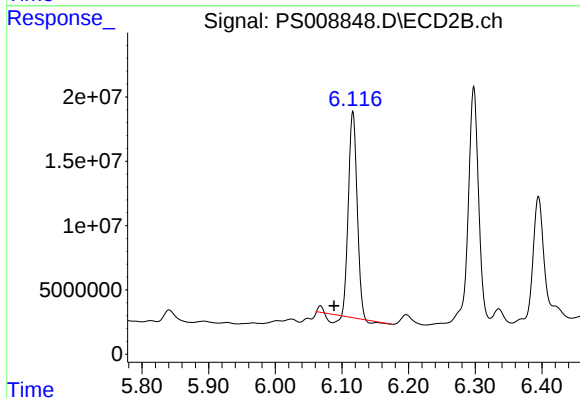


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.116 min
Delta R.T.: 0.028 min
Response: 139383977
Conc: 101.31 ng/ml

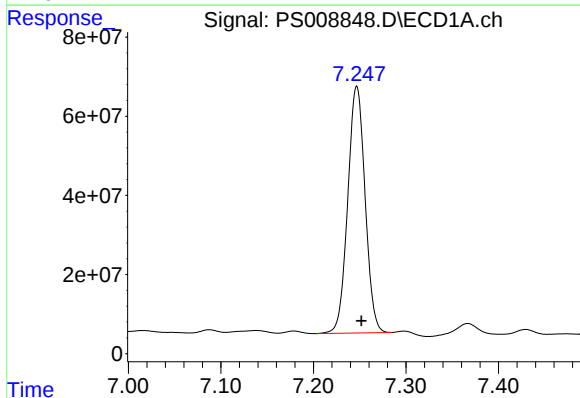


#4 2,4-DCAA

R.T.: 7.247 min
Delta R.T.: -0.005 min
Response: 811300714
Conc: 378.00 ng/ml

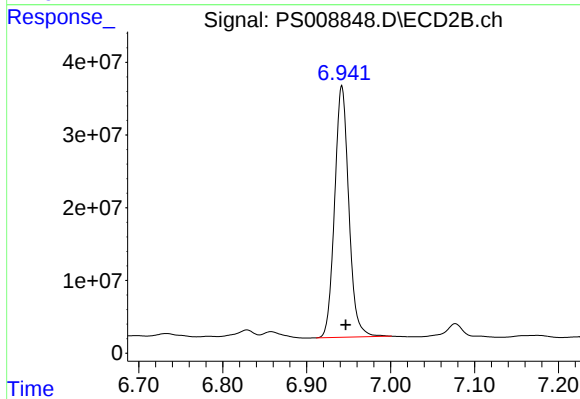

#4 2,4-DCAA


R.T.: 6.942 min
Delta R.T.: -0.005 min
Response: 406074298
Conc: 438.14 ng/ml

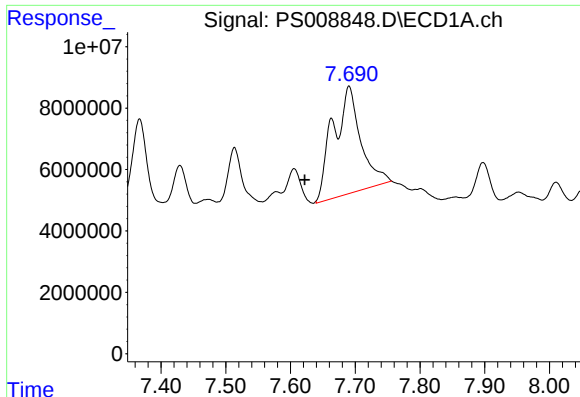

#6 MCP


R.T.: 7.691 min
Delta R.T.: 0.069 min
Response: 103958435
Conc: 16.91 ug/ml

Instrument :
ECD_S
ClientSampleId :

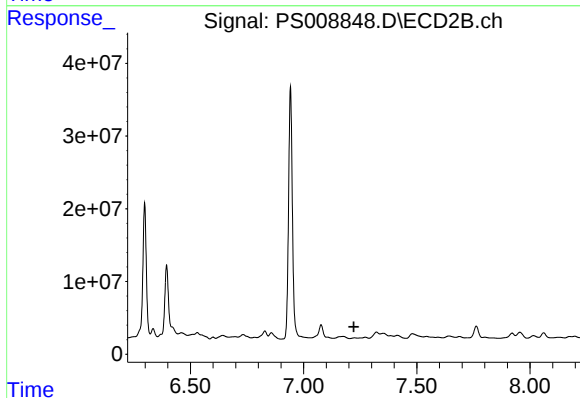


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.222 min
Response: 0
Conc: N.D.

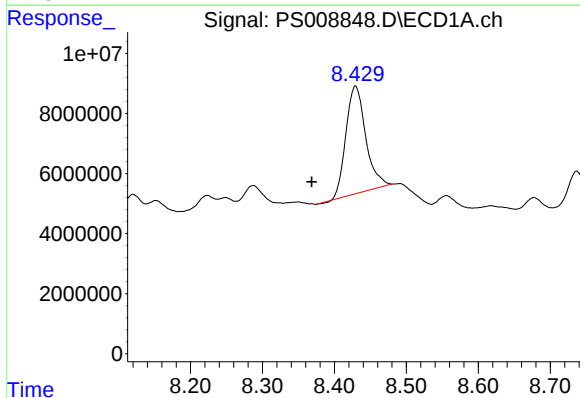


#9 2,4-D

R.T.: 8.429 min
Delta R.T.: 0.061 min
Response: 68547637
Conc: 32.03 ng/ml

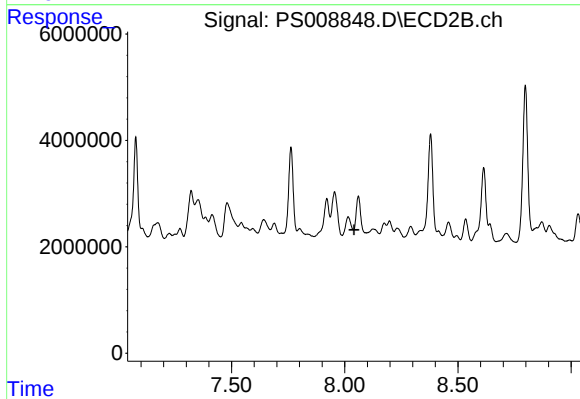

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 8.041 min
Response: 0
Conc: N.D.

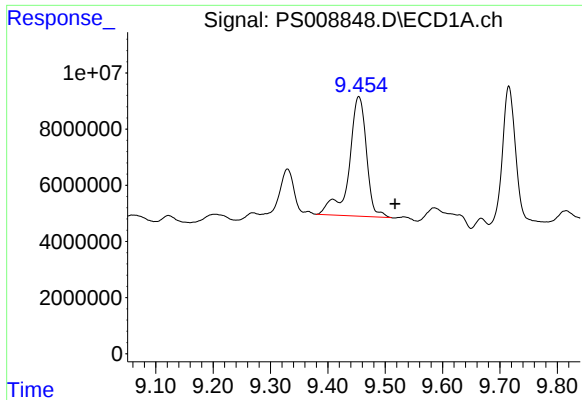

#12 2,4,5-T

R.T.: 9.454 min
Delta R.T.: -0.063 min
Response: 89306719
Conc: 8.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

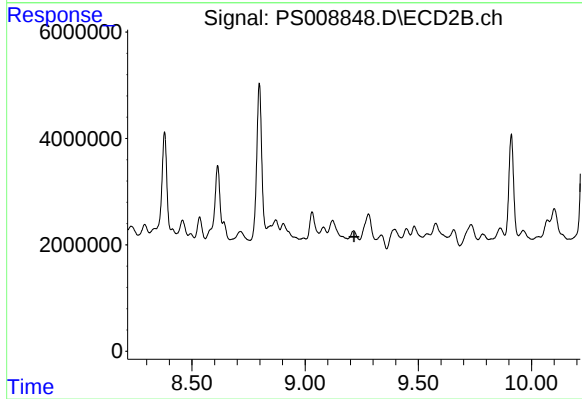

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.216 min
Response: 0
Conc: N.D.