

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021419\
 Data File : PS003187.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Feb 2019 18:41
 Operator : EI\SJ
 Sample : PB117116BS
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB117116BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 23:37:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.277	10.777	113.7E6	212.6E6	299.564	497.370 #
Target Compounds							
1) T	Dalapon	2.838	2.308	48661686	254.8E6	88.212	475.453 #
3) T	4-Nitroph...	10.873	9.928	63503400	103.4E6	328.117	494.625 #
8) T	DICHLORPROP	0.000	12.181	0	187.5E6	N.D.	490.508 #
9) T	2,4-D	13.136	12.655	71201056	135.1E6	154.430	269.483 #
11) T	2,4,5-TP ...	14.376	13.814	1248.9E6	1188.8E6	495.934	479.273
12) T	2,4,5-T	14.777	14.378	1208.0E6	145.6E6	495.214	76.081 #
14) T	DINOSEB	16.988	0.000	954.6E6	0	507.425	N.D. #
15) T	Picloram	16.767	16.685	1373.8E6	1308.1E6	434.244	435.115
16) T	DCPA	0.000	16.685	0	1308.1E6	N.D.	422.307 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021419\
Data File : PS003187.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Feb 2019 18:41
Operator : EI\SJ
Sample : PB117116BS
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
PB117116BS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 23:37:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

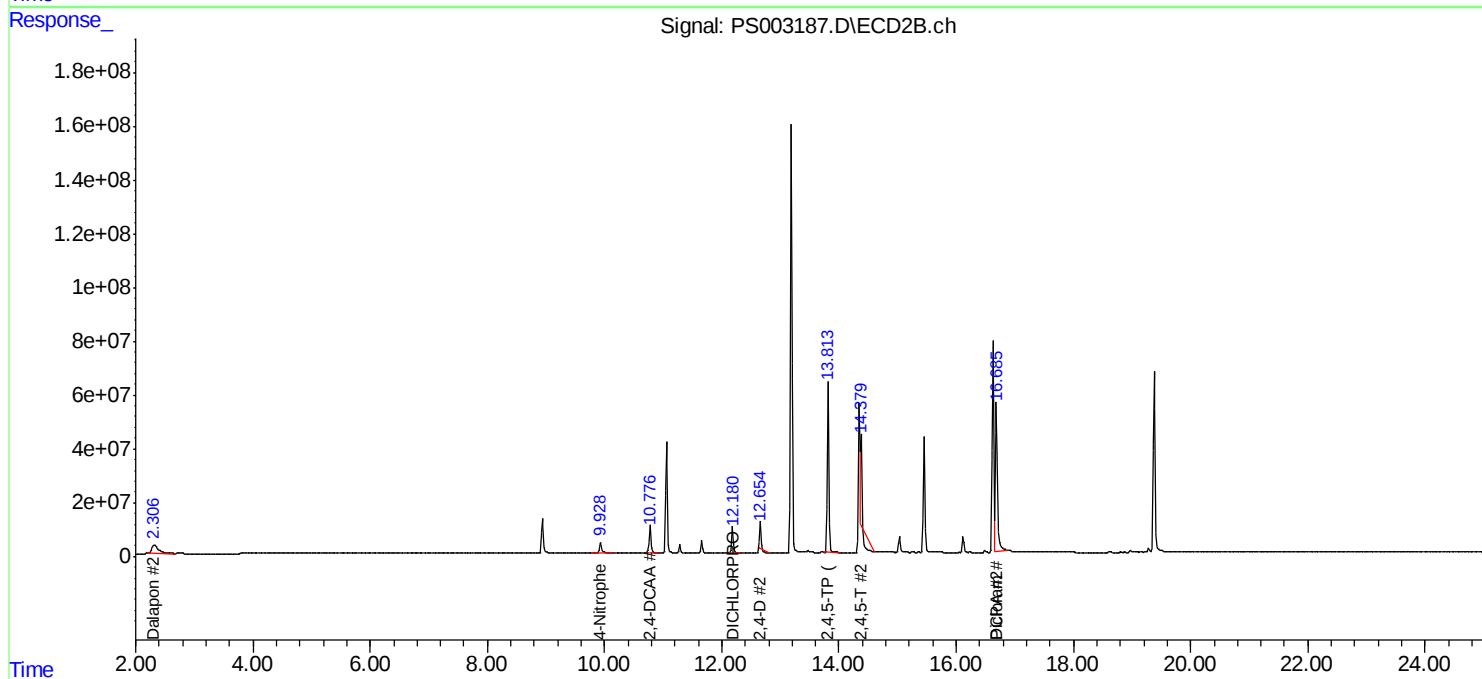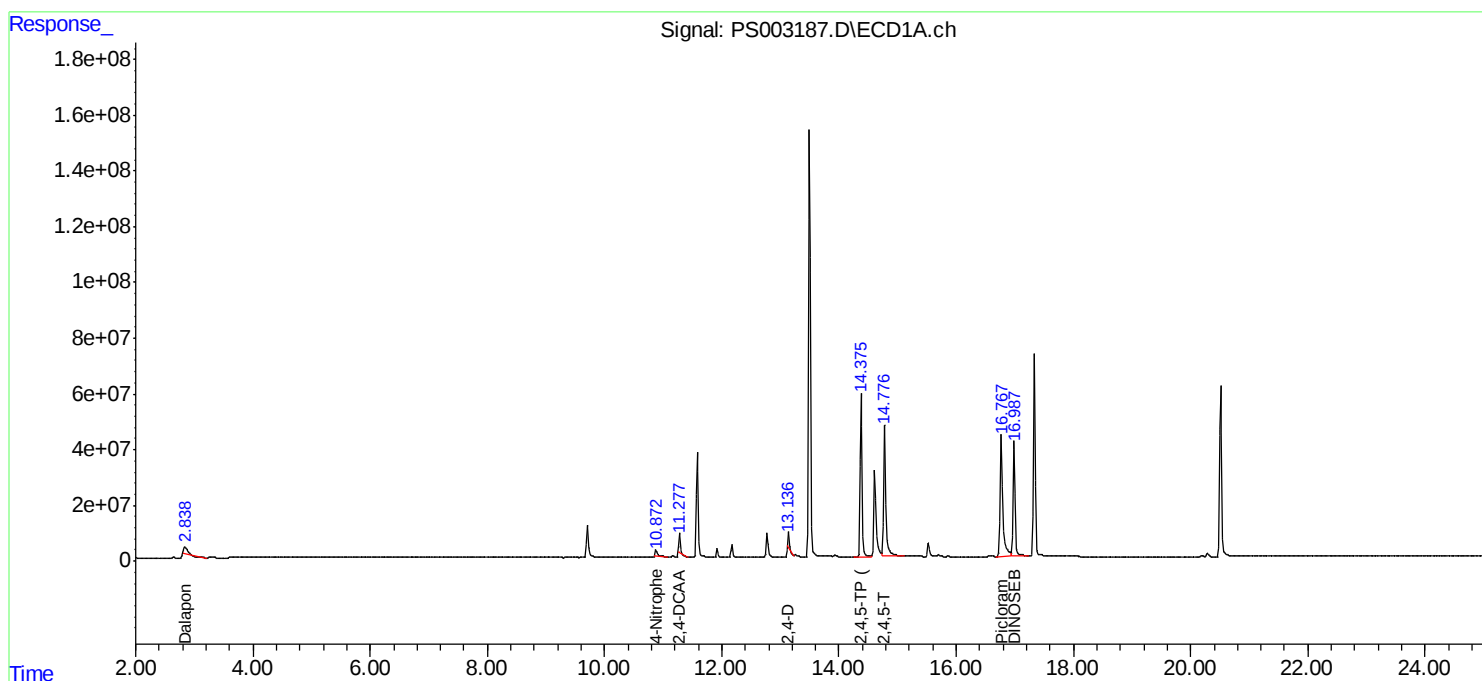


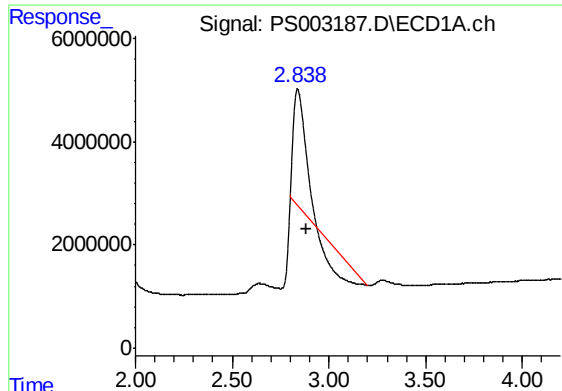

#1 Dalapon


R.T.: 2.838 min
Delta R.T.: -0.042 min
Response: 48661686
Conc: 88.21 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB117116BS

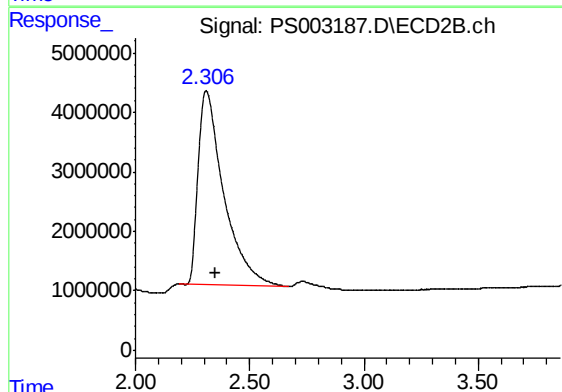


#1 Dalapon

R.T.: 2.308 min
Delta R.T.: -0.043 min
Response: 254805334
Conc: 475.45 ng/ml

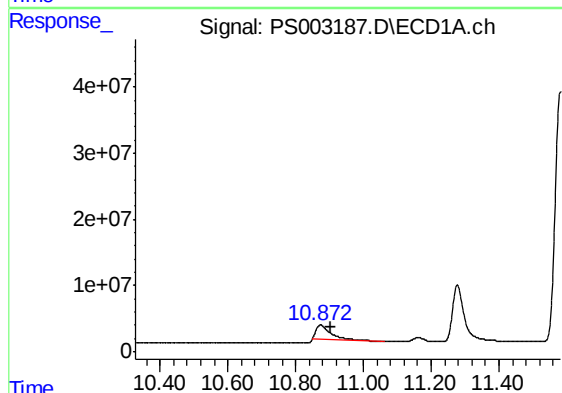


#3 4-Nitrophenol

R.T.: 10.873 min
Delta R.T.: -0.031 min
Response: 63503400
Conc: 328.12 ng/ml

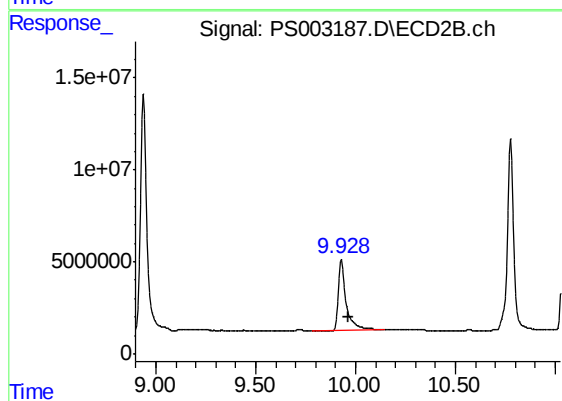

#3 4-Nitrophenol


R.T.: 9.928 min
Delta R.T.: -0.037 min
Response: 103387658
Conc: 494.62 ng/ml

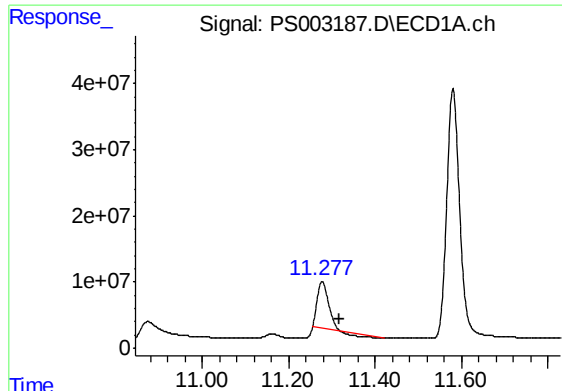

#4 2,4-DCAA


R.T.: 11.277 min
Delta R.T.: -0.040 min
Response: 113726814
Conc: 299.56 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB117116BS

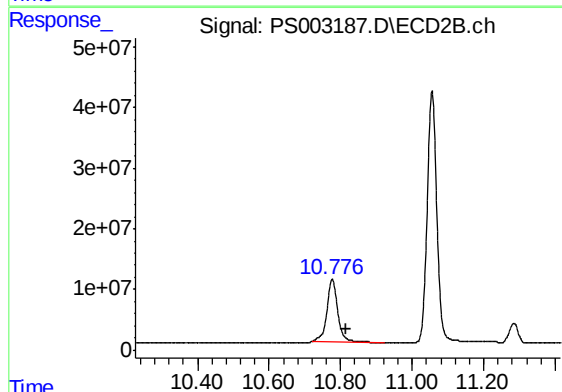


#4 2,4-DCAA

R.T.: 10.777 min
Delta R.T.: -0.040 min
Response: 212648230
Conc: 497.37 ng/ml

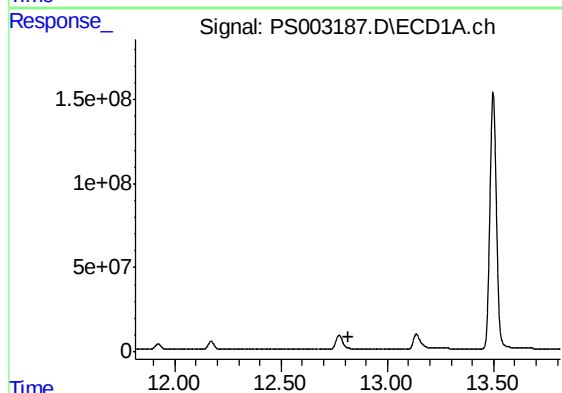


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.815 min
Response: 0
Conc: N.D.

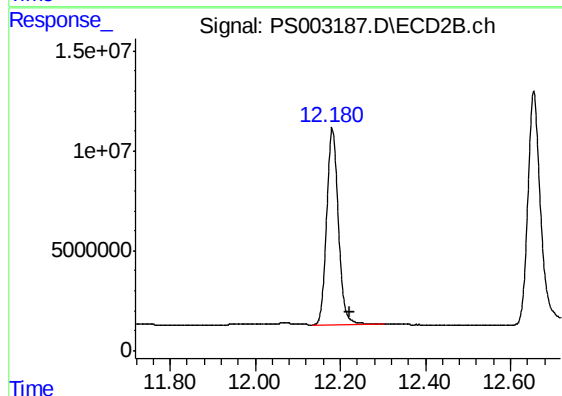

#8 DICHLORPROP


R.T.: 12.181 min
Delta R.T.: -0.041 min
Response: 187541453
Conc: 490.51 ng/ml

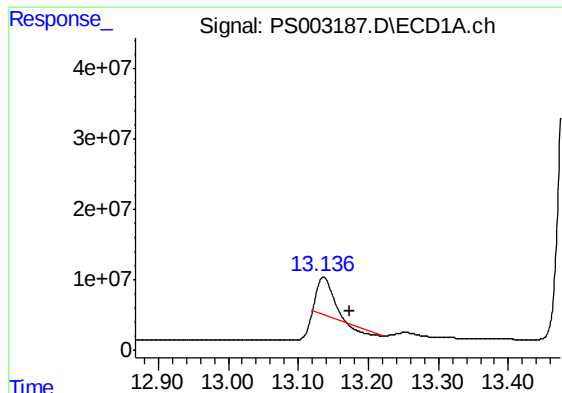

#9 2,4-D


R.T.: 13.136 min
Delta R.T.: -0.038 min
Response: 71201056
Conc: 154.43 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB117116BS

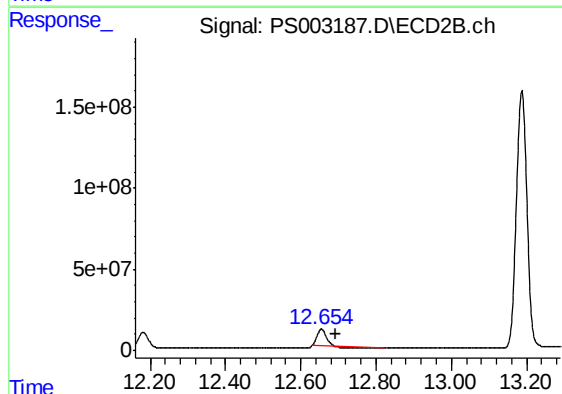


#9 2,4-D

R.T.: 12.655 min
Delta R.T.: -0.038 min
Response: 135115090
Conc: 269.48 ng/ml

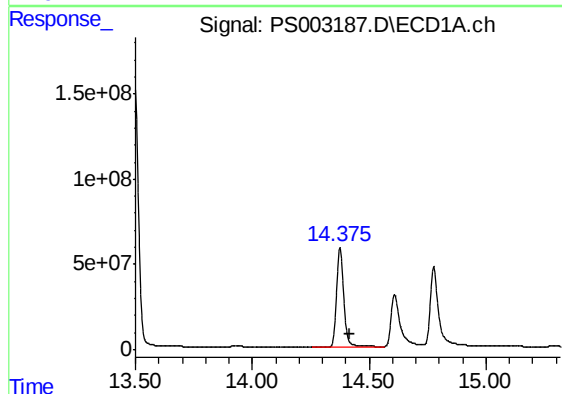


#11 2,4,5-TP (SILVEX)

R.T.: 14.376 min
Delta R.T.: -0.044 min
Response: 1248946374
Conc: 495.93 ng/ml

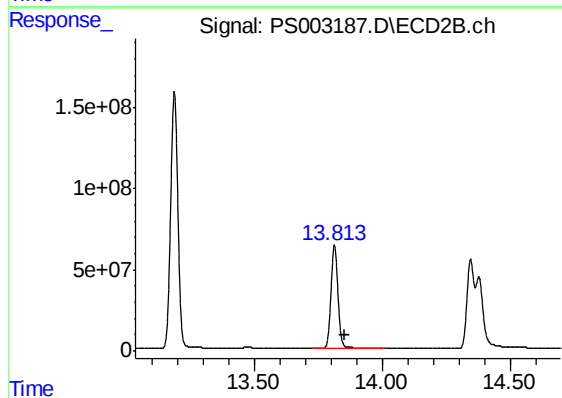

#11 2,4,5-TP (SILVEX)


R.T.: 13.814 min
Delta R.T.: -0.041 min
Response: 1188767440
Conc: 479.27 ng/ml

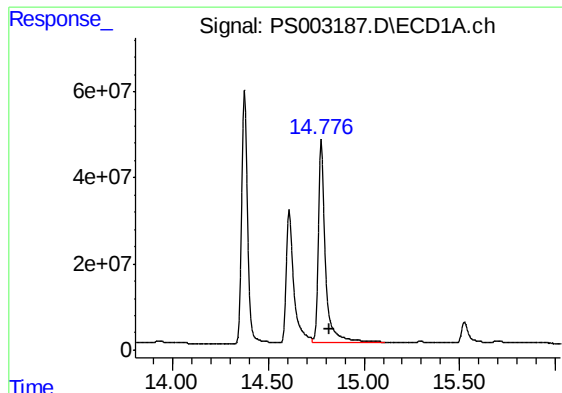

#12 2,4,5-T


R.T.: 14.777 min
Delta R.T.: -0.040 min
Response: 1208028281
Conc: 495.21 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB117116BS

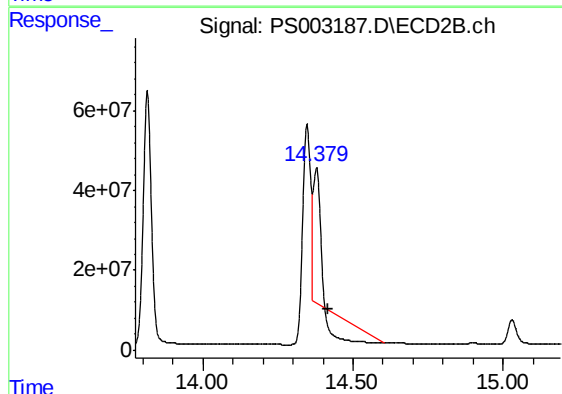


#12 2,4,5-T

R.T.: 14.378 min
Delta R.T.: -0.039 min
Response: 145580832
Conc: 76.08 ng/ml

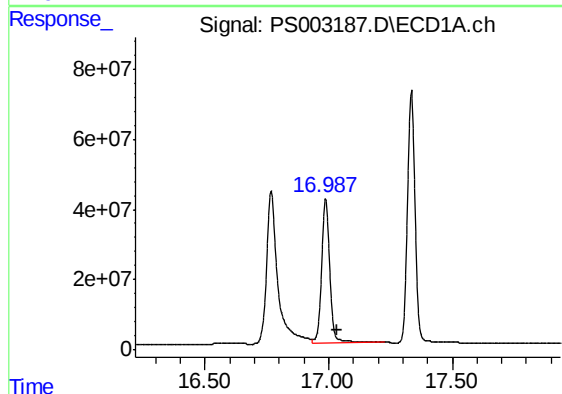


#14 DINOSEB

R.T.: 16.988 min
Delta R.T.: -0.047 min
Response: 954632001
Conc: 507.42 ng/ml

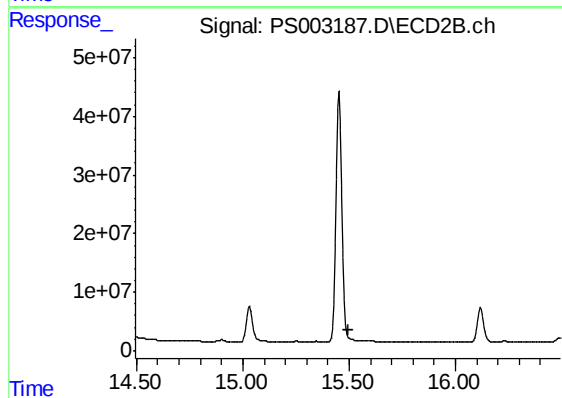

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 15.495 min
Response: 0
Conc: N.D.

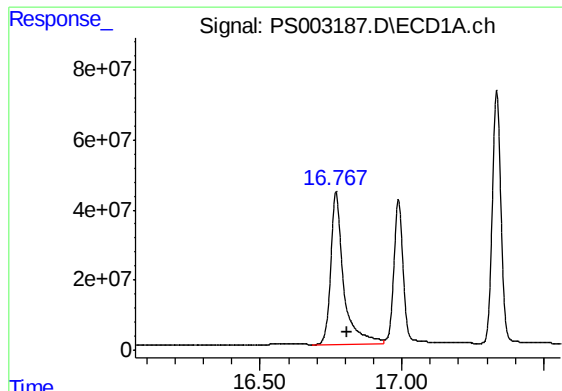

#15 Picloram


R.T.: 16.767 min
Delta R.T.: -0.038 min
Response: 1373787668
Conc: 434.24 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB117116BS

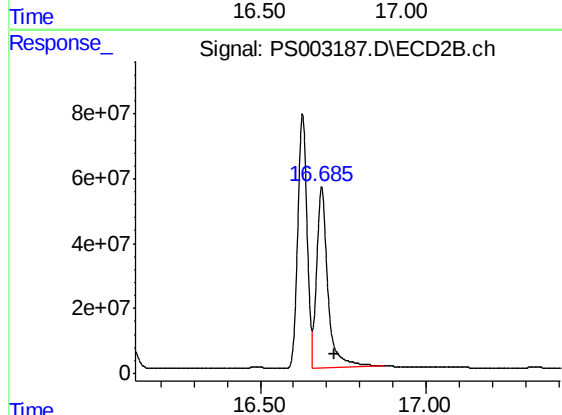


#15 Picloram

R.T.: 16.685 min
Delta R.T.: -0.039 min
Response: 1308132203
Conc: 435.12 ng/ml

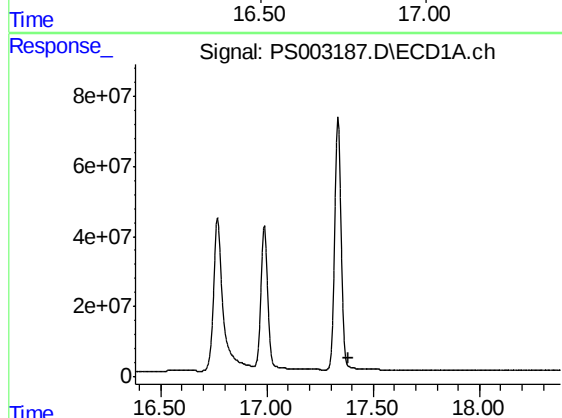

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

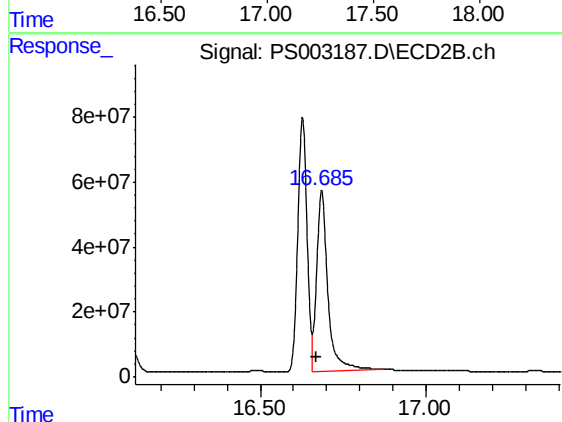

#16 DCPA

R.T.: 16.685 min
Delta R.T.: 0.016 min
Response: 1308132203
Conc: 422.31 ng/ml