

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021419\
 Data File : PS003188.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Feb 2019 19:12
 Operator : EI\SJ
 Sample : PB117116TB
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB117116TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 23:37:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.299	10.799	183.2E6	182.2E6	482.687	426.051
Target Compounds							
1) T	Dalapon	0.000	2.289	0	9623555	N.D.	17.957 #
6) T	MCPD	11.979	0.000	12624646	0	10.537	N.D. #
7) T	MCPA	12.221	11.757	7507248	67769347	4.241	43.081 #
12) T	2,4,5-T	0.000	14.419	0	4732553	N.D.	2.473 #
14) T	DINOSEB	0.000	15.527	0	2967279	N.D.	1.693 #
15) T	Picloram	16.834	16.726	5695280	30105330	1.800	10.014 #
16) T	DCPA	0.000	16.726	0	30105330	N.D.	9.719 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021419\
Data File : PS003188.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Feb 2019 19:12
Operator : EI\SJ
Sample : PB117116TB
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB117116TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 23:37:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

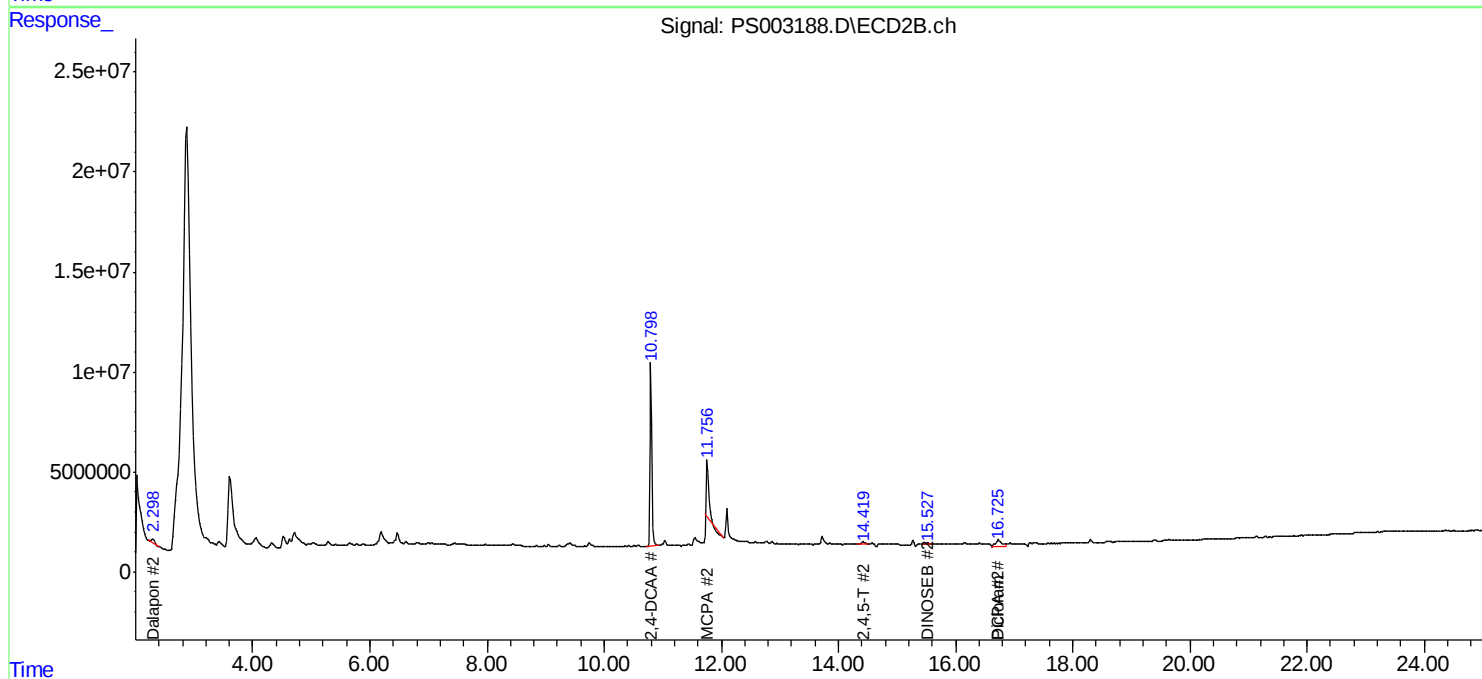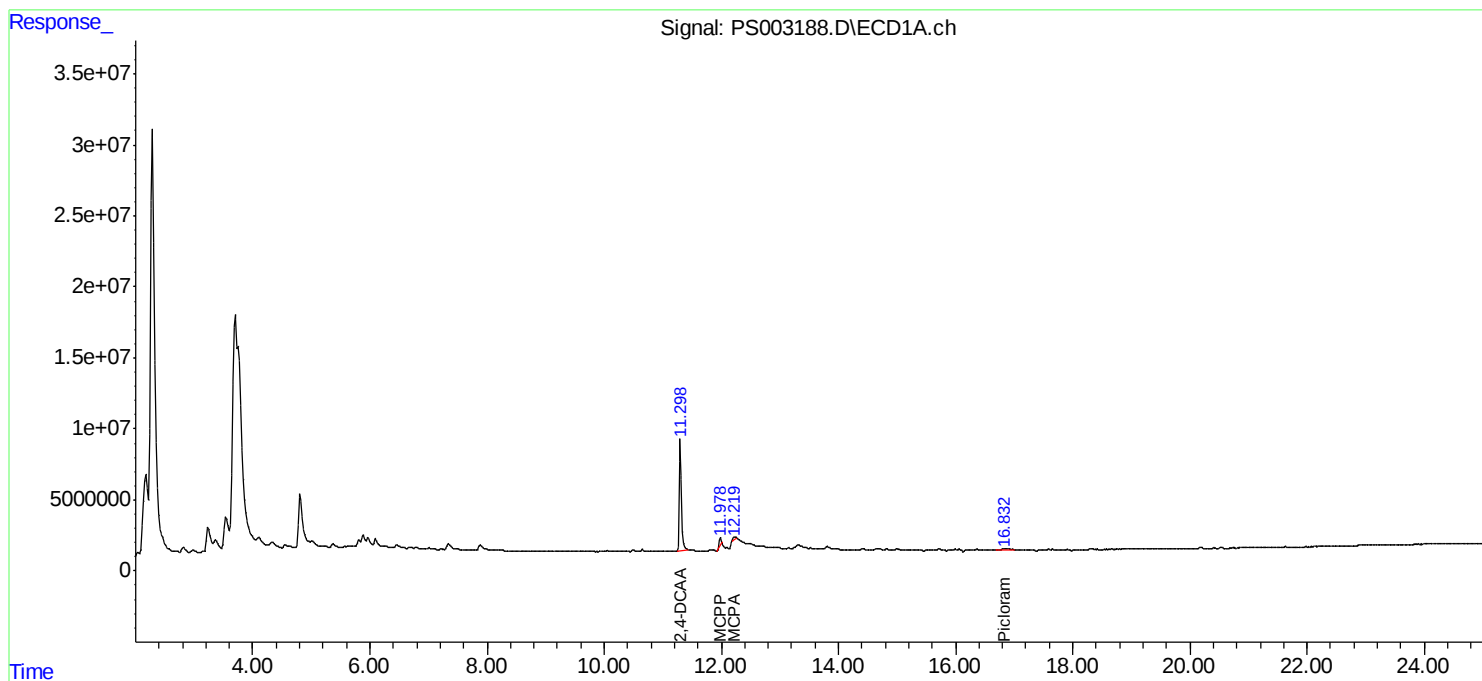


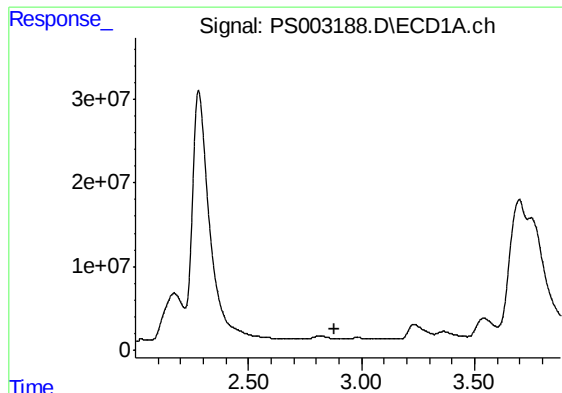

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB117116TB

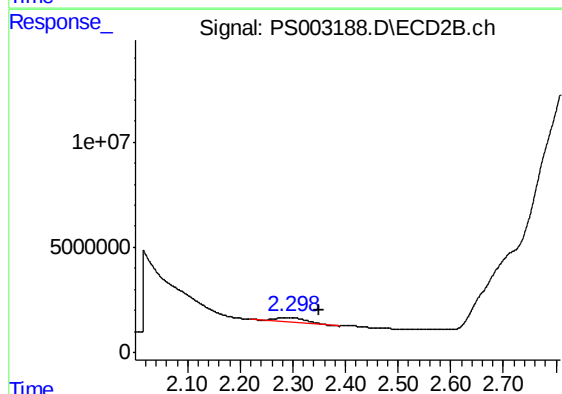


#1 Dalapon

R.T.: 2.289 min
Delta R.T.: -0.062 min
Response: 9623555
Conc: 17.96 ng/ml

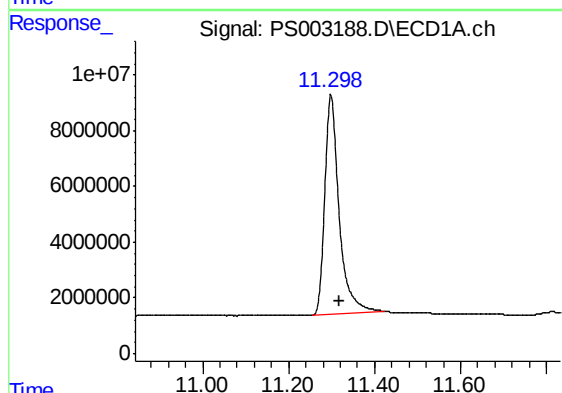


#4 2,4-DCAA

R.T.: 11.299 min
Delta R.T.: -0.019 min
Response: 183247696
Conc: 482.69 ng/ml

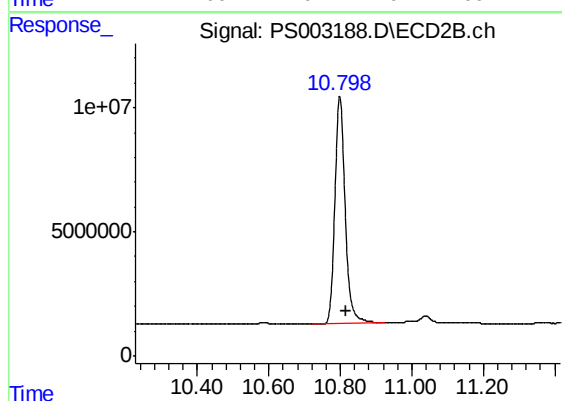

#4 2,4-DCAA


R.T.: 10.799 min
Delta R.T.: -0.018 min
Response: 182156314
Conc: 426.05 ng/ml

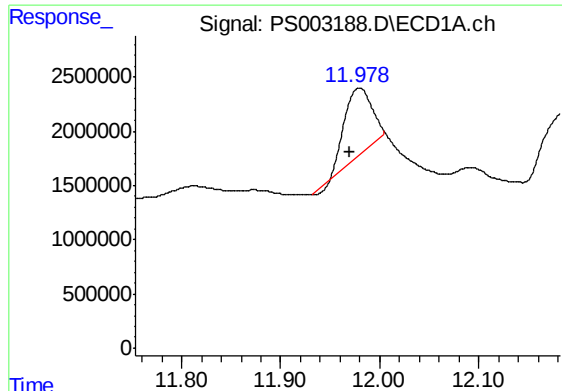

#6 MCPP


R.T.: 11.979 min
Delta R.T.: 0.010 min
Response: 12624646
Conc: 10.54 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB117116TB

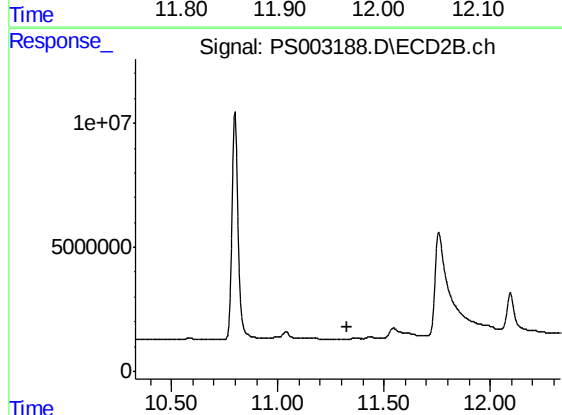


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.330 min
Response: 0
Conc: N.D.

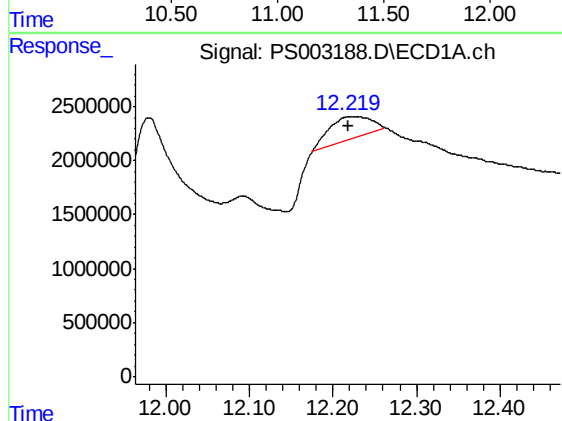


#7 MCPA

R.T.: 12.221 min
Delta R.T.: 0.002 min
Response: 7507248
Conc: 4.24 ug/ml

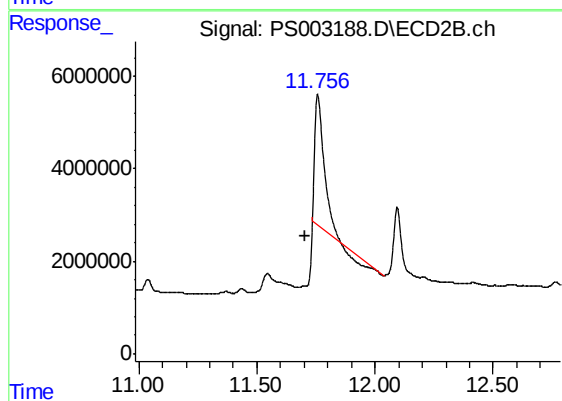

#7 MCPA


R.T.: 11.757 min
Delta R.T.: 0.051 min
Response: 67769347
Conc: 43.08 ug/ml

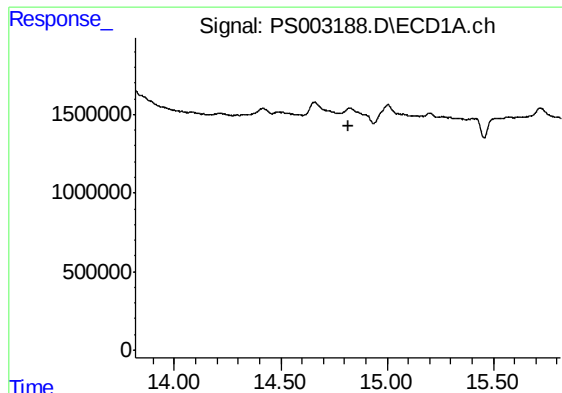

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 14.817 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB117116TB

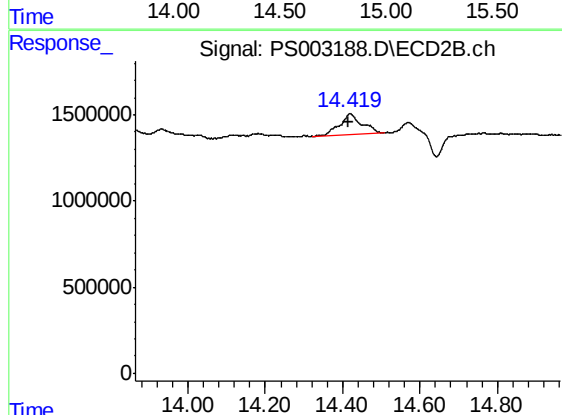


#12 2,4,5-T

R.T.: 14.419 min
Delta R.T.: 0.002 min
Response: 4732553
Conc: 2.47 ng/ml

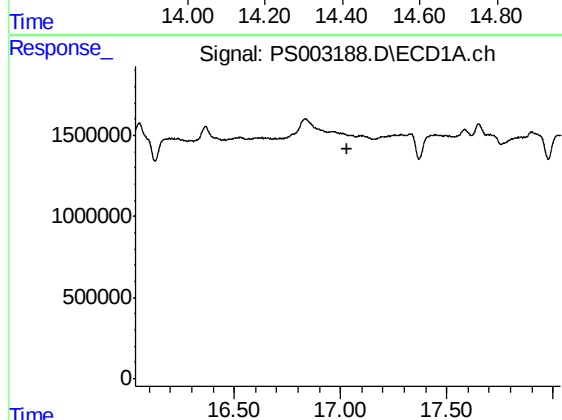


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.035 min
Response: 0
Conc: N.D.

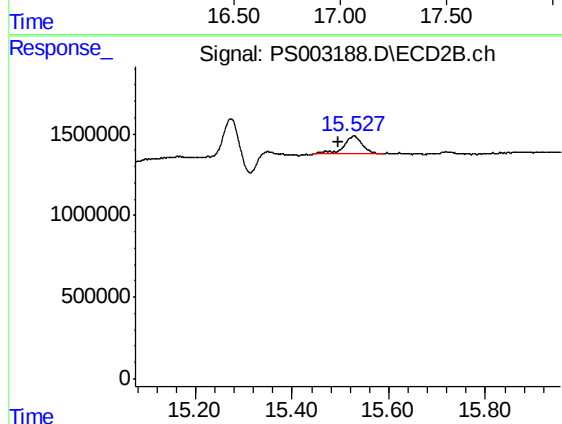

#14 DINOSEB


R.T.: 15.527 min
Delta R.T.: 0.032 min
Response: 2967279
Conc: 1.69 ng/ml

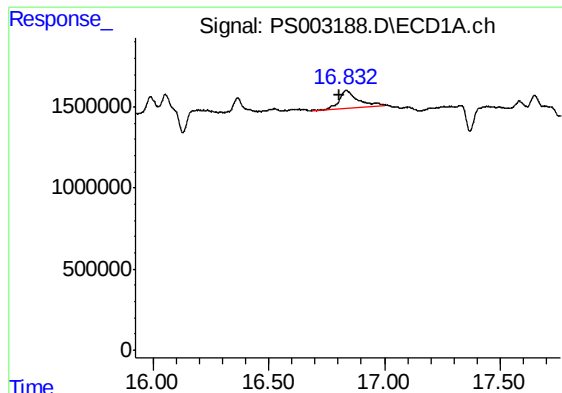

#15 Picloram


R.T.: 16.834 min
Delta R.T.: 0.028 min
Response: 5695280
Conc: 1.80 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB117116TB

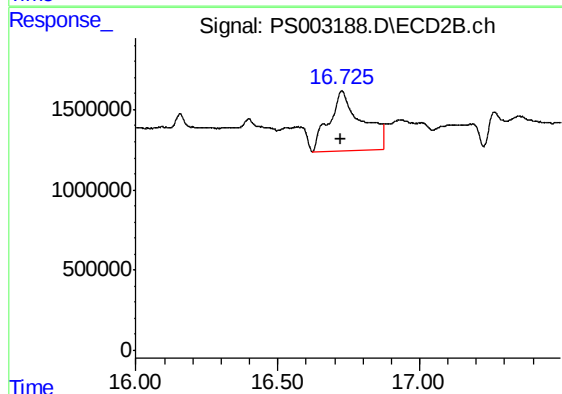


#15 Picloram

R.T.: 16.726 min
Delta R.T.: 0.001 min
Response: 30105330
Conc: 10.01 ng/ml

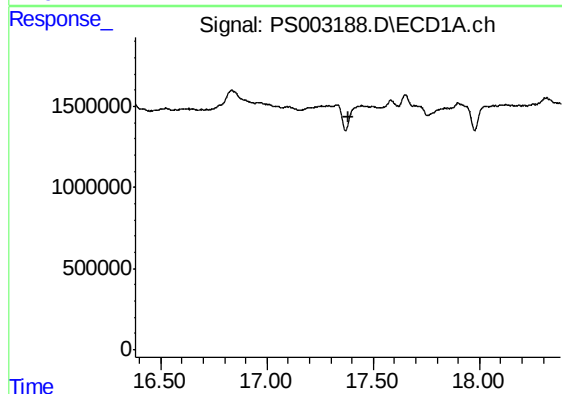

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

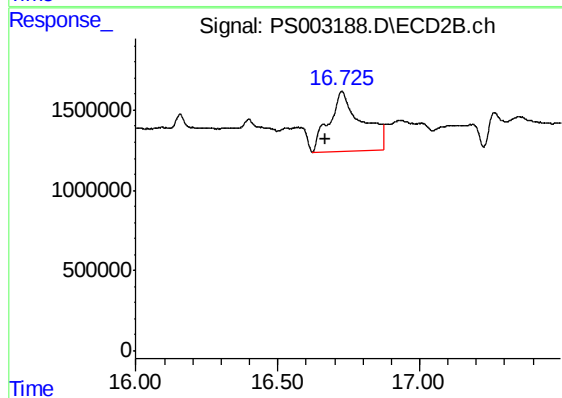

#16 DCPA

R.T.: 16.726 min
Delta R.T.: 0.056 min
Response: 30105330
Conc: 9.72 ng/ml