

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021419\
 Data File : PS003191.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Feb 2019 20:45
 Operator : EI\SJ
 Sample : K1349-06MSD
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 OR-01-021319-AMSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 23:38:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.384	10.777	-917420	86762650	N.D.	202.932
Target Compounds							
1) T	Dalapon	2.822	2.314	-8898259	188.4E6	N.D.	351.456
3) T	4-Nitroph...	0.000	9.981	0	113.1E6	N.D.	540.989 #
6) T	MCP	11.900	0.000	49802608	0	41.567	N.D. #
7) T	MCPA	0.000	11.719	0	40911634	N.D.	26.008 #
8) T	DICHLORPROP	12.749	12.181	19268098	214.1E6	50.239	559.843 #
11) T	2,4,5-TP ...	14.352	13.813	1341.4E6	1169.2E6	532.641	471.383
12) T	2,4,5-T	14.751	14.445	1352.2E6	199.0E6	554.312	104.022 #
14) T	DINOSEB	16.967	0.000	350.6E6	0	186.332	N.D. #
15) T	Picloram	16.742	16.684	1229.8E6	1106.8E6	388.721	368.134
16) T	DCPA	17.441	16.684	-162211345	1106.8E6	N.D.	357.297



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021419\
Data File : PS003191.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Feb 2019 20:45
Operator : EI\SJ
Sample : K1349-06MSD
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
OR-01-021319-AMSD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 23:38:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

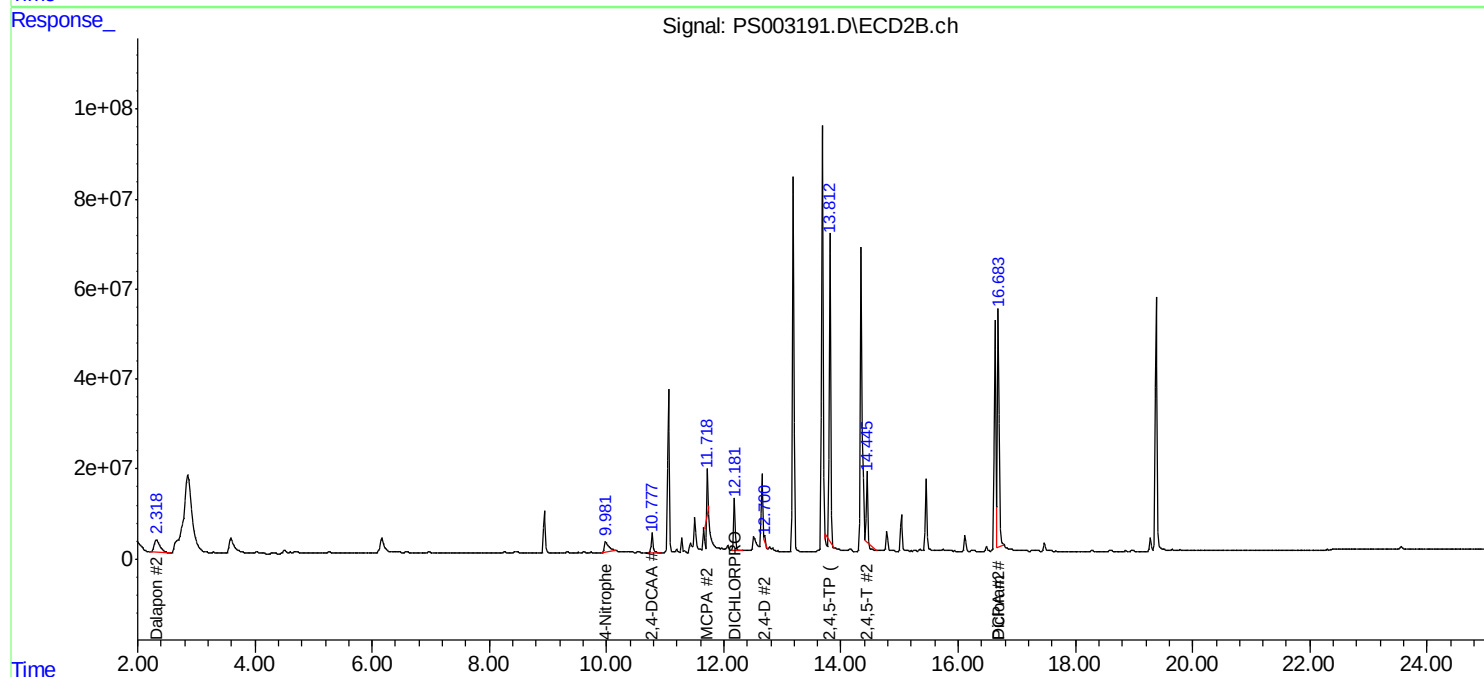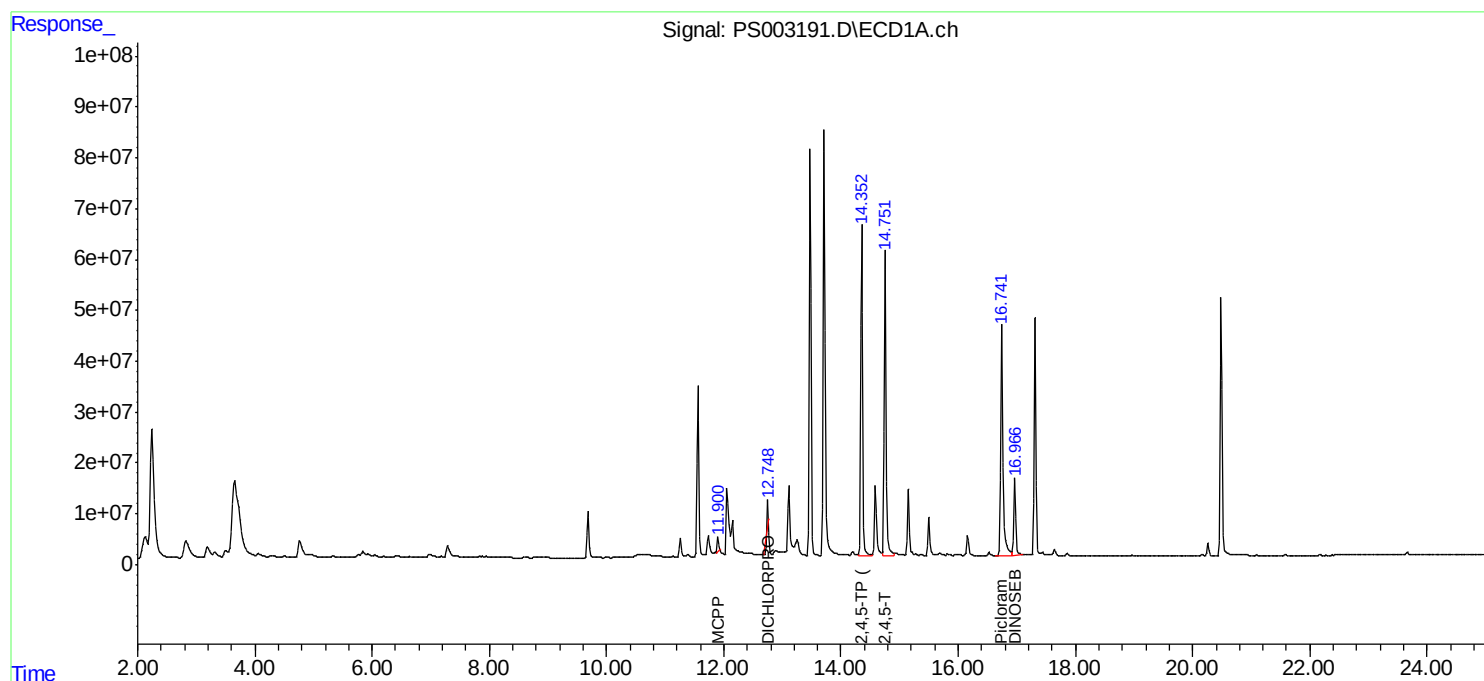


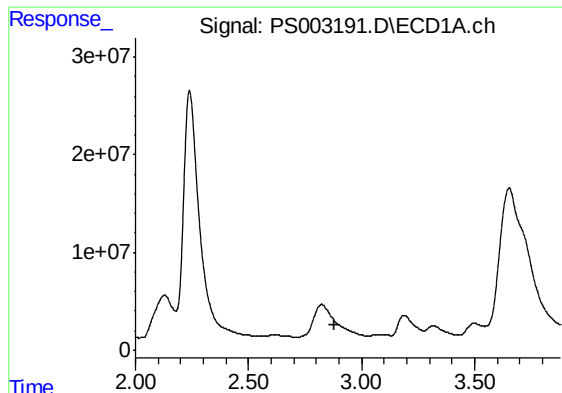

#1 Dalapon


R.T.: 2.822 min
Delta R.T.: -0.058 min
Response: -8898259
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
OR-01-021319-AMSD

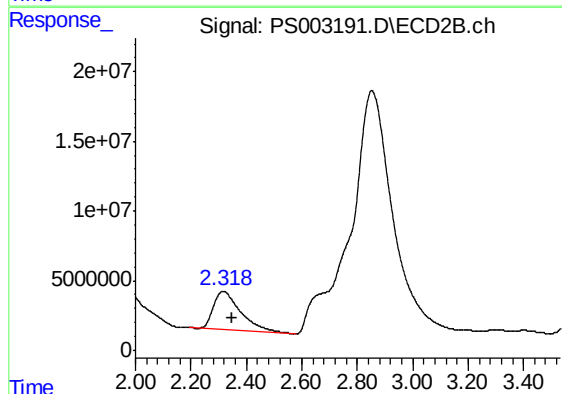


#1 Dalapon

R.T.: 2.314 min
Delta R.T.: -0.036 min
Response: 188352833
Conc: 351.46 ng/ml

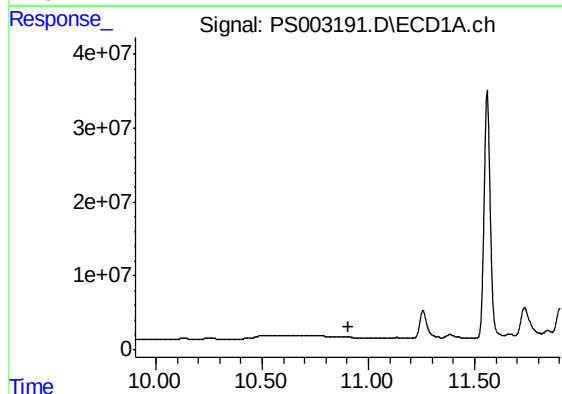


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 10.904 min
Response: 0
Conc: N.D.

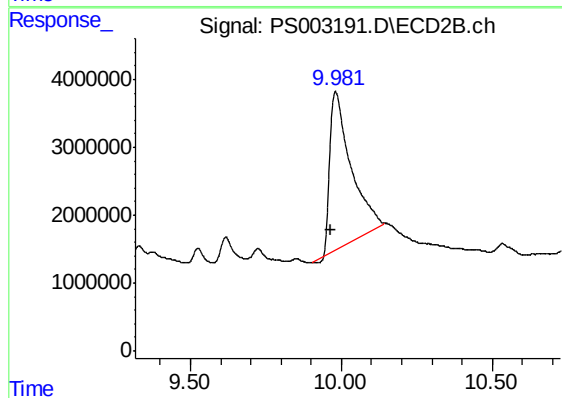

#3 4-Nitrophenol


R.T.: 9.981 min
Delta R.T.: 0.016 min
Response: 113078944
Conc: 540.99 ng/ml

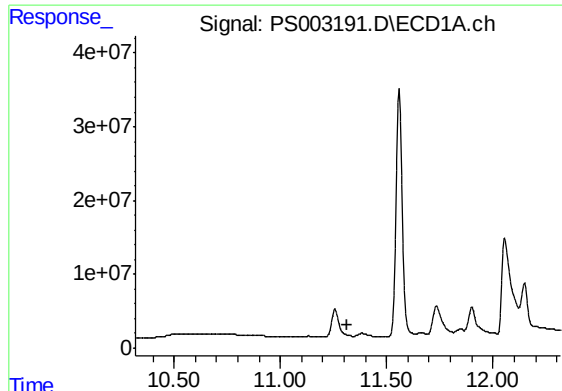

#4 2,4-DCAA


R.T.: 11.384 min
Delta R.T.: 0.066 min
Response: -917420
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
OR-01-021319-AMSD

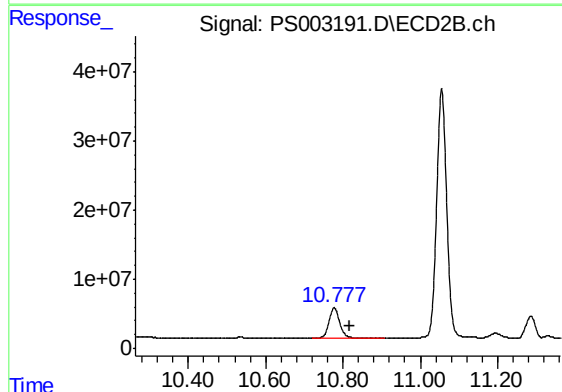


#4 2,4-DCAA

R.T.: 10.777 min
Delta R.T.: -0.039 min
Response: 86762650
Conc: 202.93 ng/ml

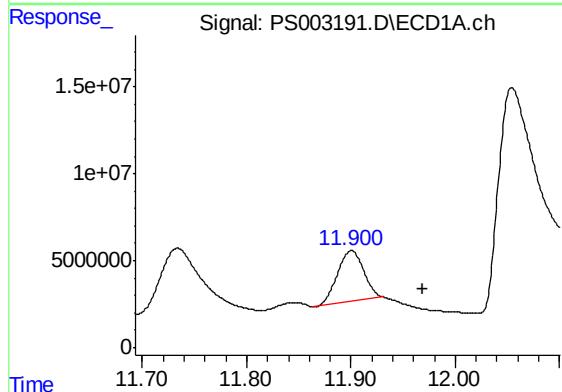


#6 MCPP

R.T.: 11.900 min
Delta R.T.: -0.069 min
Response: 49802608
Conc: 41.57 ug/ml

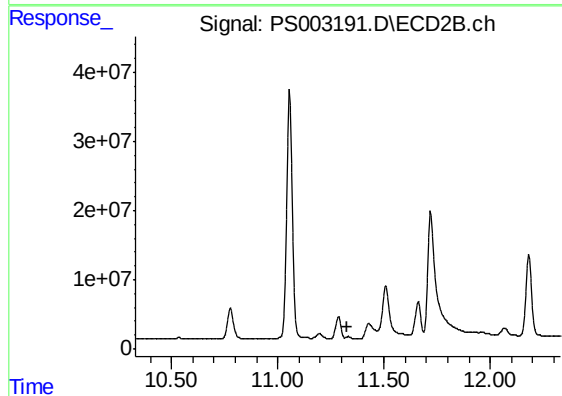

#6 MCPP


R.T.: 0.000 min
Exp R.T. : 11.330 min
Response: 0
Conc: N.D.

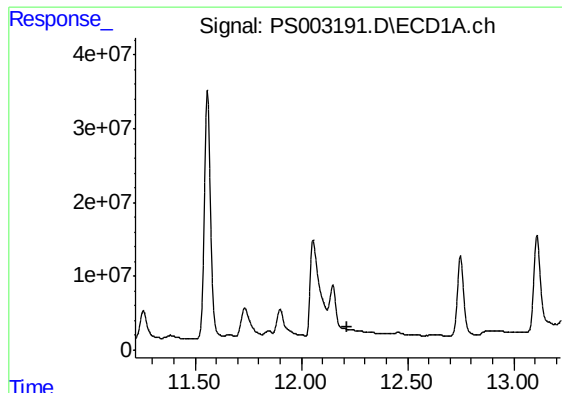

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.219 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
OR-01-021319-AMSD

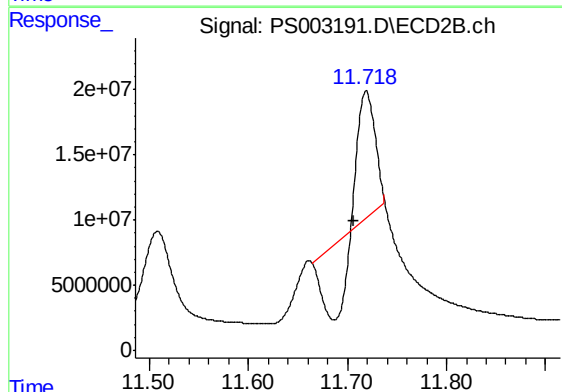


#7 MCPA

R.T.: 11.719 min
Delta R.T.: 0.013 min
Response: 40911634
Conc: 26.01 ug/ml

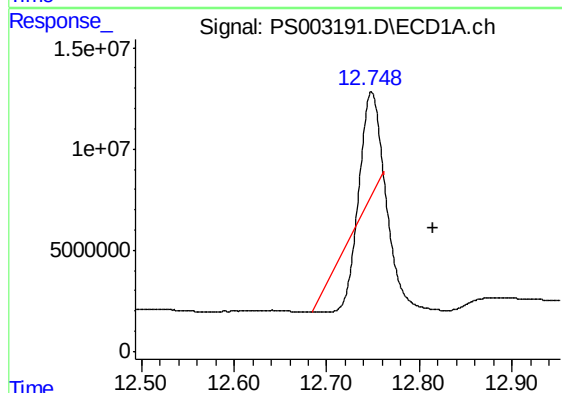


#8 DICHLORPROP

R.T.: 12.749 min
Delta R.T.: -0.066 min
Response: 19268098
Conc: 50.24 ng/ml

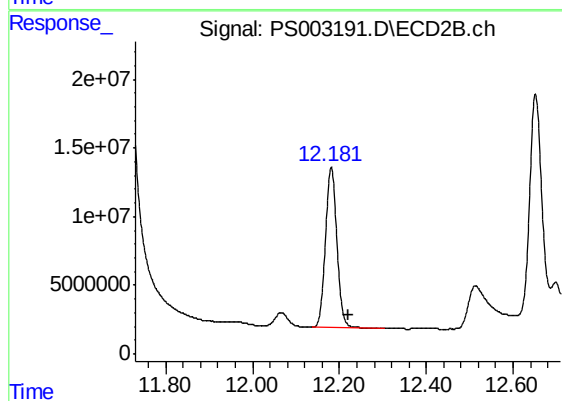

#8 DICHLORPROP


R.T.: 12.181 min
Delta R.T.: -0.041 min
Response: 214050820
Conc: 559.84 ng/ml

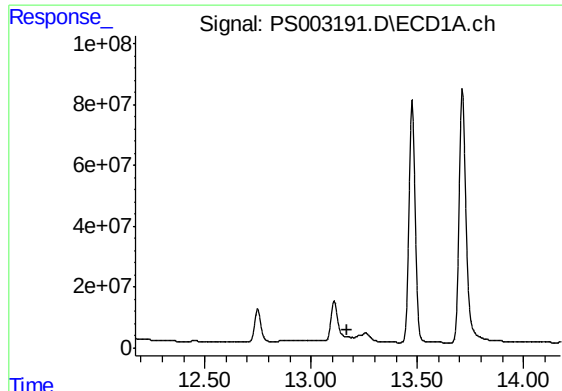

#9 2,4-D


R.T.: 13.109 min
Delta R.T.: -0.065 min
Response: -205773487
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
OR-01-021319-AMSD

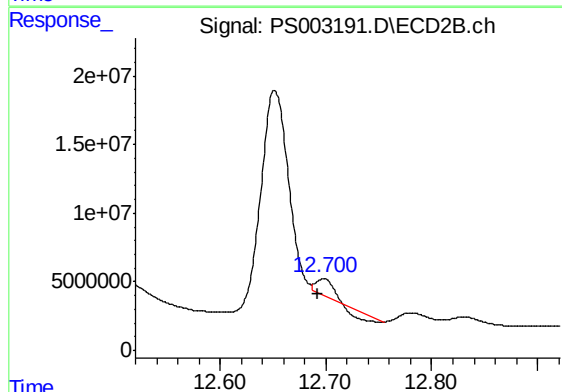


#9 2,4-D

R.T.: 12.698 min
Delta R.T.: 0.005 min
Response: 5396251
Conc: 10.76 ng/ml

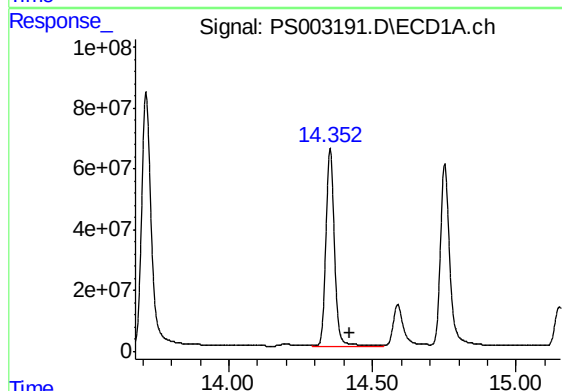


#11 2,4,5-TP (SILVEX)

R.T.: 14.352 min
Delta R.T.: -0.067 min
Response: 1341387811
Conc: 532.64 ng/ml

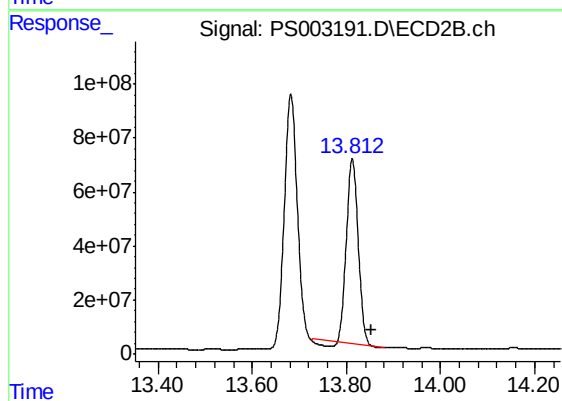

#11 2,4,5-TP (SILVEX)


R.T.: 13.813 min
Delta R.T.: -0.042 min
Response: 1169197317
Conc: 471.38 ng/ml

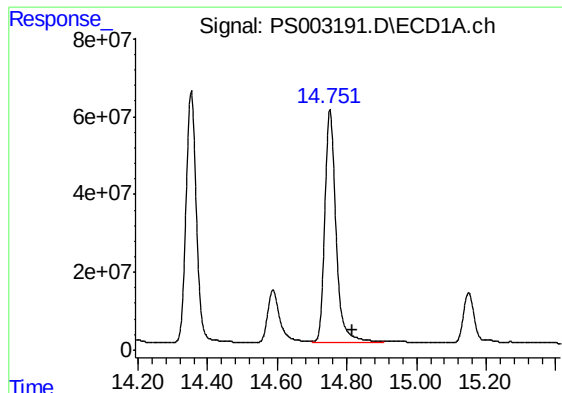

#12 2,4,5-T


R.T.: 14.751 min
Delta R.T.: -0.065 min
Response: 1352192059
Conc: 554.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
OR-01-021319-AMSD

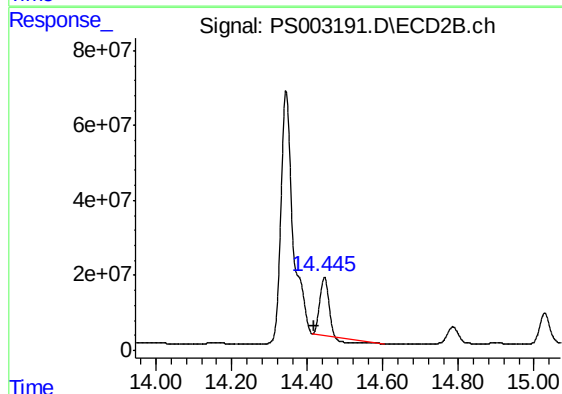


#12 2,4,5-T

R.T.: 14.445 min
Delta R.T.: 0.028 min
Response: 199045481
Conc: 104.02 ng/ml

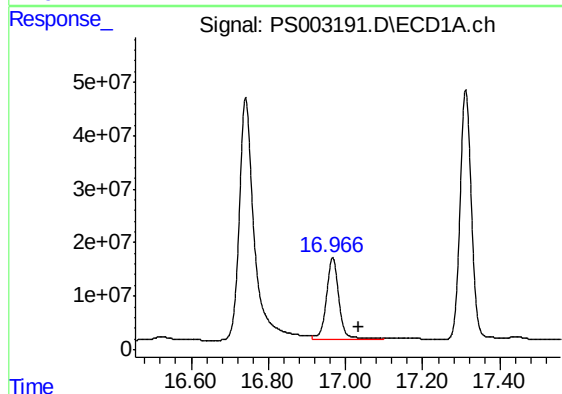


#14 DINOSEB

R.T.: 16.967 min
Delta R.T.: -0.069 min
Response: 350551120
Conc: 186.33 ng/ml

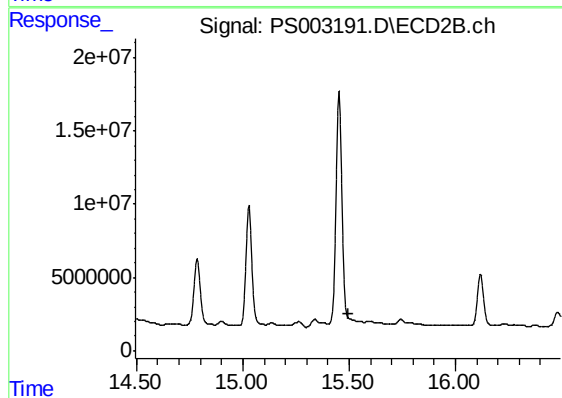

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 15.495 min
Response: 0
Conc: N.D.

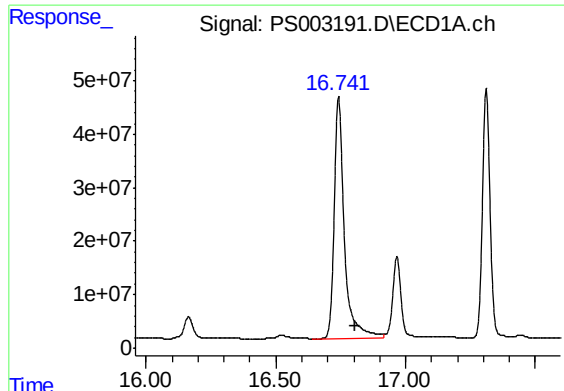

#15 Picloram


R.T.: 16.742 min
Delta R.T.: -0.064 min
Response: 1229771579
Conc: 388.72 ng/ml

Instrument :
ECD_S
ClientSampleId :
OR-01-021319-AMSD

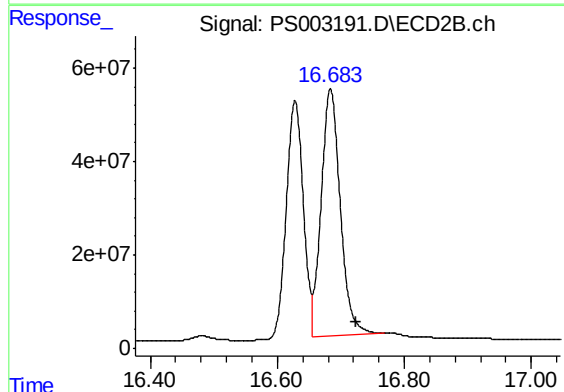


#15 Picloram

R.T.: 16.684 min
Delta R.T.: -0.040 min
Response: 1106759208
Conc: 368.13 ng/ml

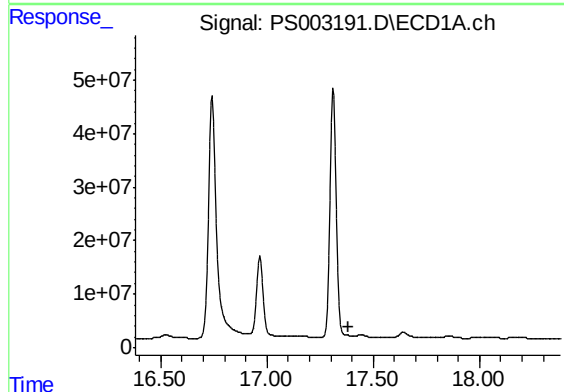

#16 DCPA

R.T.: 17.441 min
Delta R.T.: 0.060 min
Response: -162211345
Conc: N.D.

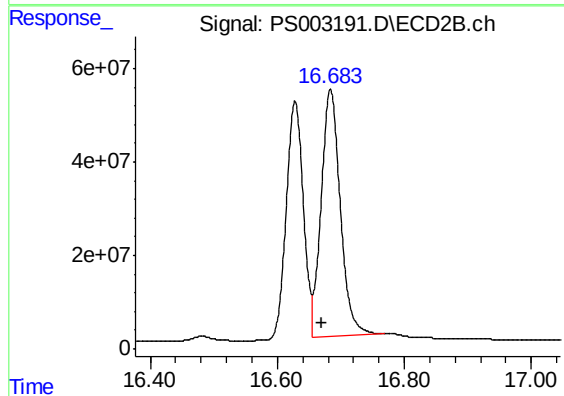

#16 DCPA

R.T.: 16.684 min
Delta R.T.: 0.014 min
Response: 1106759208
Conc: 357.30 ng/ml