

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021419\
 Data File : PS003193.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Feb 2019 21:47
 Operator : EI\SJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 23:38:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.761	0	247.7E6	N.D.	579.397 #
Target Compounds							
1) T	Dalapon	2.822	2.294	-247985093	376.7E6	N.D.	702.927
3) T	4-Nitroph...	0.000	9.911	0	158.2E6	N.D.	756.991 #
6) T	MCP	11.908	11.274	67811636	55988008	56.598	50.762
7) T	MCPA	12.158	11.649	76199072	82610159	43.051	52.515
8) T	DICHLORPROP	0.000	12.166	0	280.8E6	N.D.	734.419 #
11) T	2,4,5-TP ...	14.359	13.798	1896.2E6	1772.9E6	752.965	714.779
14) T	DINOSEB	16.973	0.000	1428.8E6	0	759.471	N.D. #
15) T	Picloram	16.748	16.669	2191.5E6	2074.4E6	692.707	689.982
16) T	DCPA	0.000	16.669	0	2074.4E6	N.D.	669.671 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021419\
Data File : PS003193.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Feb 2019 21:47
Operator : EI\SJ
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 23:38:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

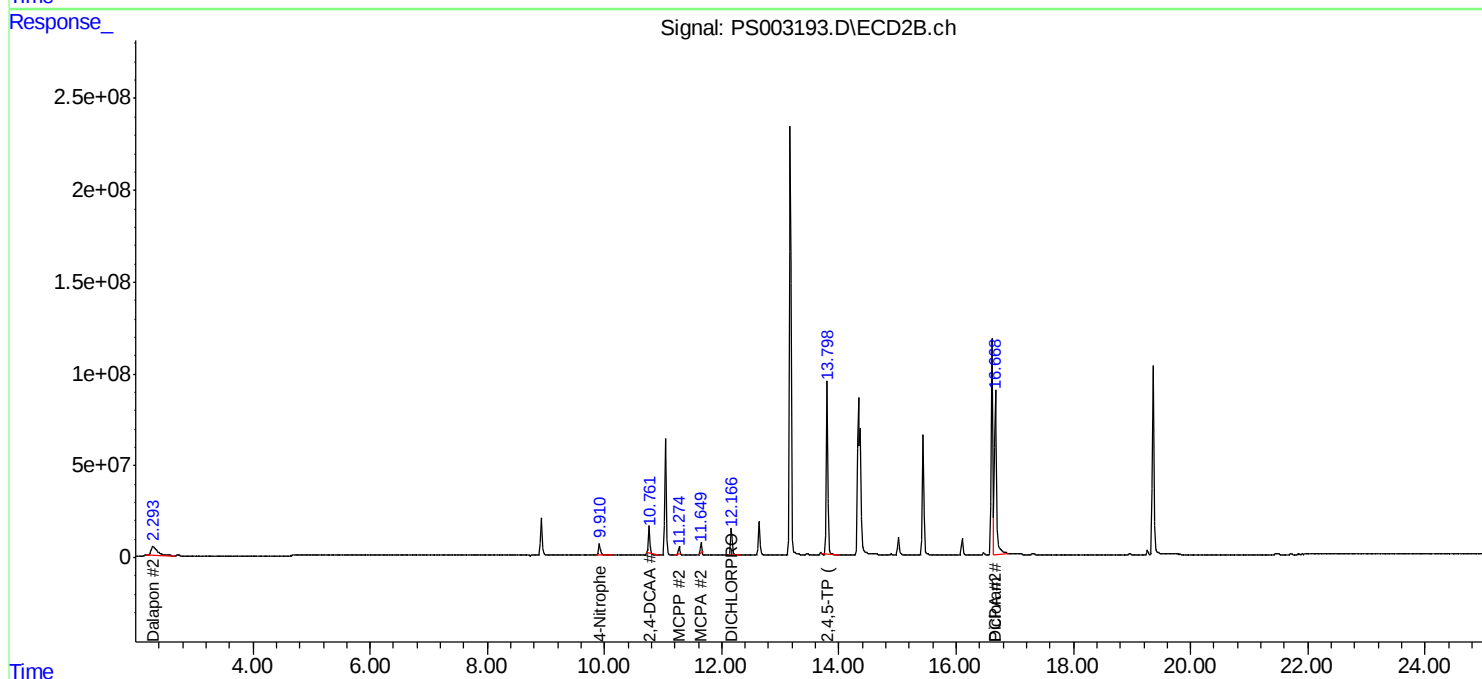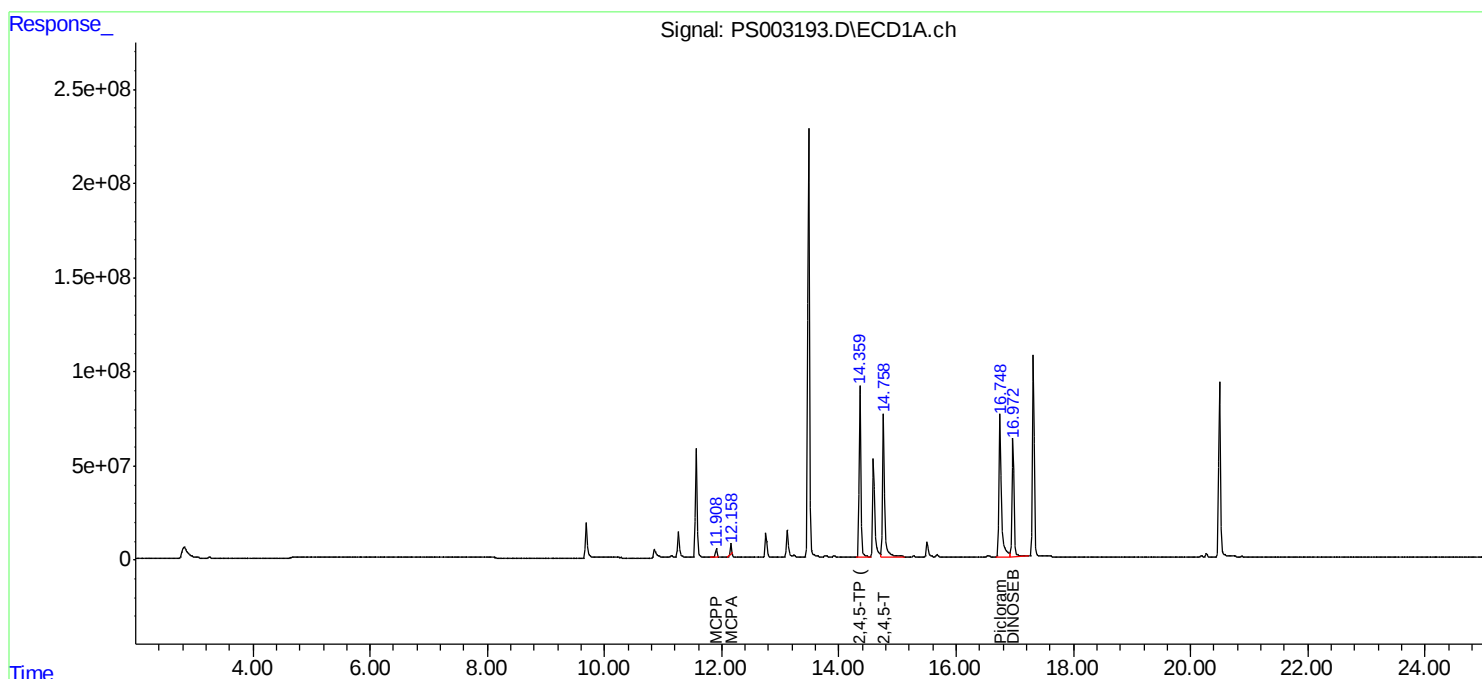


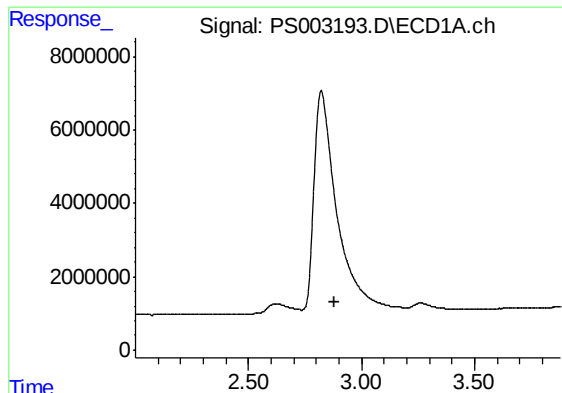

#1 Dalapon


R.T.: 2.822 min
Delta R.T.: -0.058 min
Response: -247985093
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

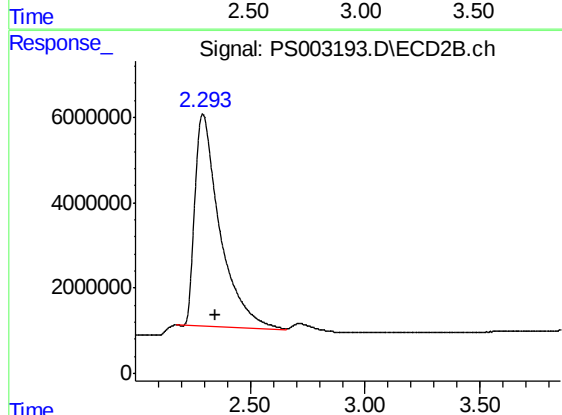


#1 Dalapon

R.T.: 2.294 min
Delta R.T.: -0.057 min
Response: 376713782
Conc: 702.93 ng/ml

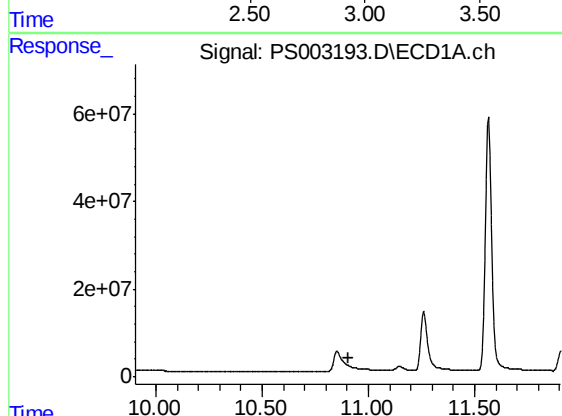


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 10.904 min
Response: 0
Conc: N.D.

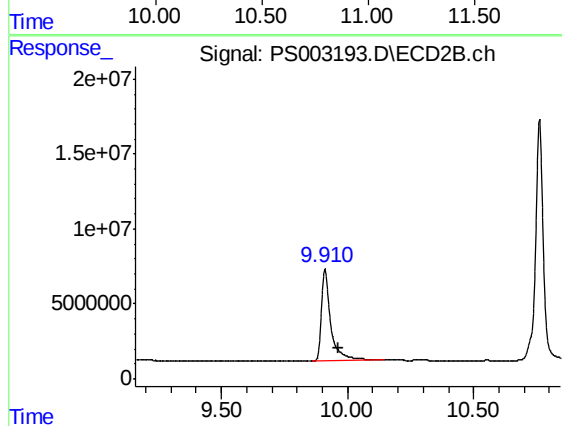

#3 4-Nitrophenol


R.T.: 9.911 min
Delta R.T.: -0.055 min
Response: 158228186
Conc: 756.99 ng/ml

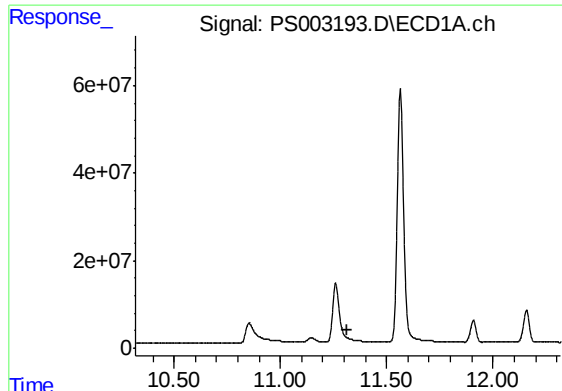

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 11.318 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

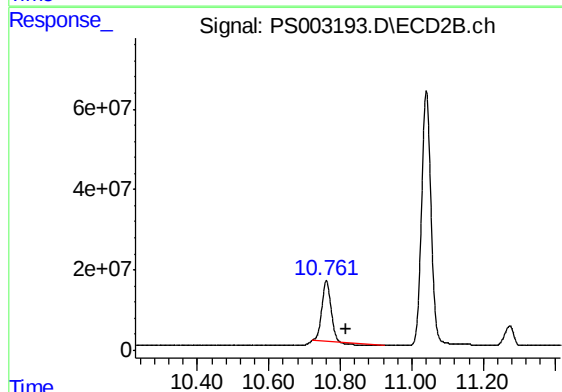


#4 2,4-DCAA

R.T.: 10.761 min
Delta R.T.: -0.056 min
Response: 247718768
Conc: 579.40 ng/ml

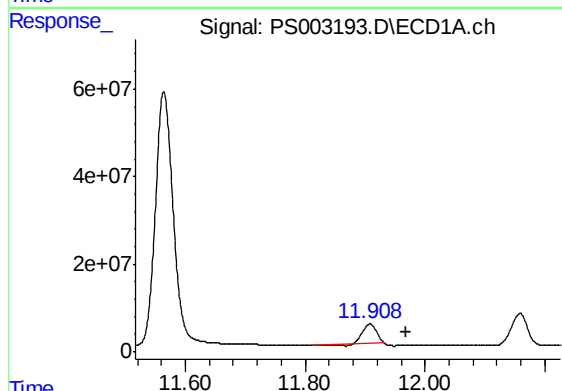


#6 MCPP

R.T.: 11.908 min
Delta R.T.: -0.061 min
Response: 67811636
Conc: 56.60 ug/ml

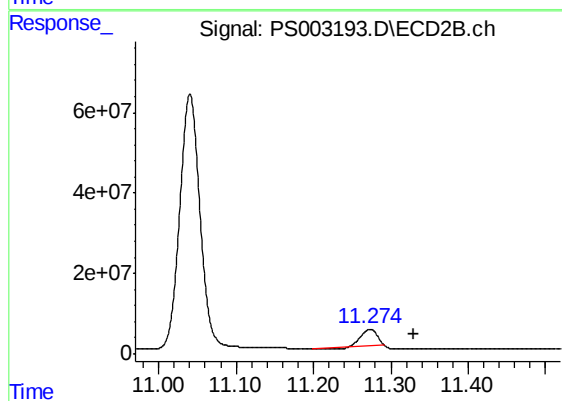

#6 MCPP


R.T.: 11.274 min
Delta R.T.: -0.057 min
Response: 55988008
Conc: 50.76 ug/ml

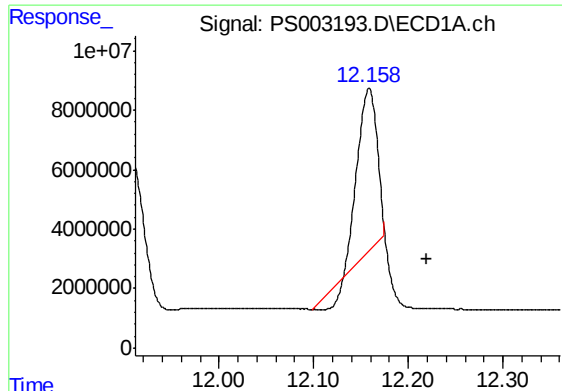

#7 MCPA


R.T.: 12.158 min
Delta R.T.: -0.061 min
Response: 76199072
Conc: 43.05 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

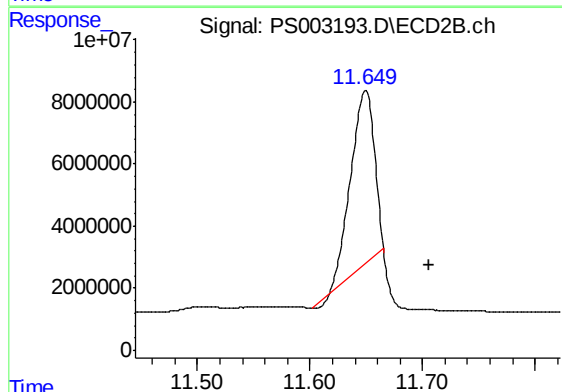


#7 MCPA

R.T.: 11.649 min
Delta R.T.: -0.057 min
Response: 82610159
Conc: 52.52 ug/ml

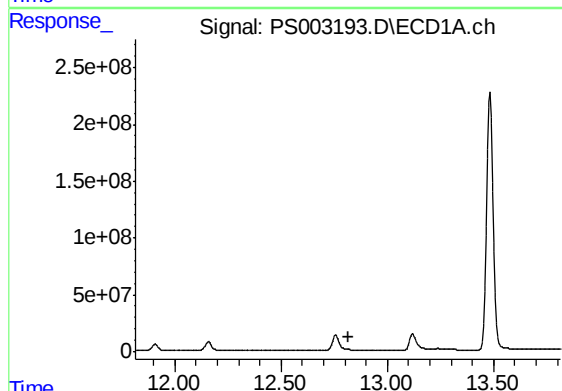


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.815 min
Response: 0
Conc: N.D.

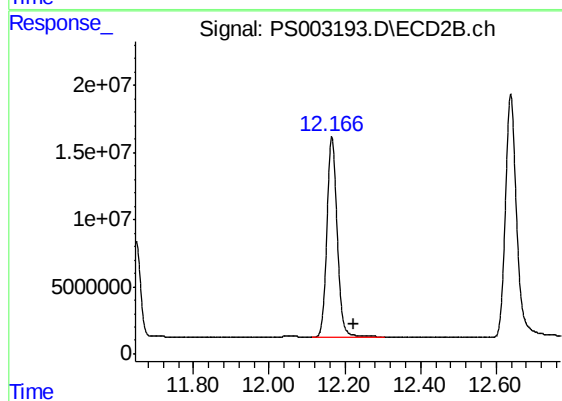

#8 DICHLORPROP


R.T.: 12.166 min
Delta R.T.: -0.056 min
Response: 280798742
Conc: 734.42 ng/ml

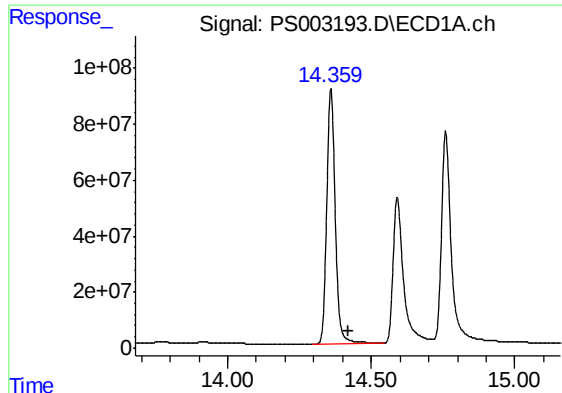

#11 2,4,5-TP (SILVEX)


R.T.: 14.359 min
Delta R.T.: -0.060 min
Response: 1896246525
Conc: 752.96 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

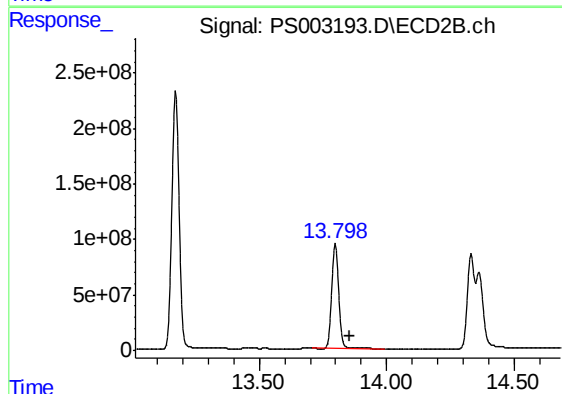


#11 2,4,5-TP (SILVEX)

R.T.: 13.798 min
Delta R.T.: -0.056 min
Response: 1772904946
Conc: 714.78 ng/ml

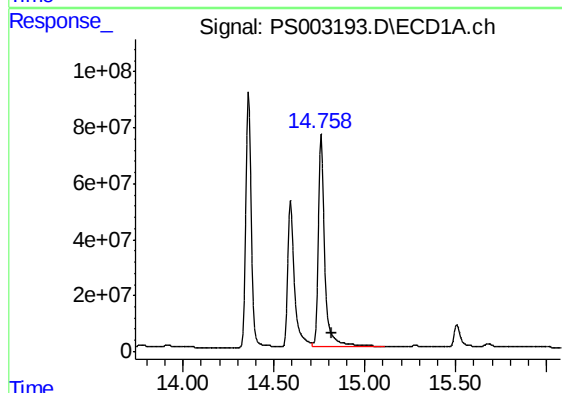


#12 2,4,5-T

R.T.: 14.759 min
Delta R.T.: -0.058 min
Response: 1841310589
Conc: 754.82 ng/ml

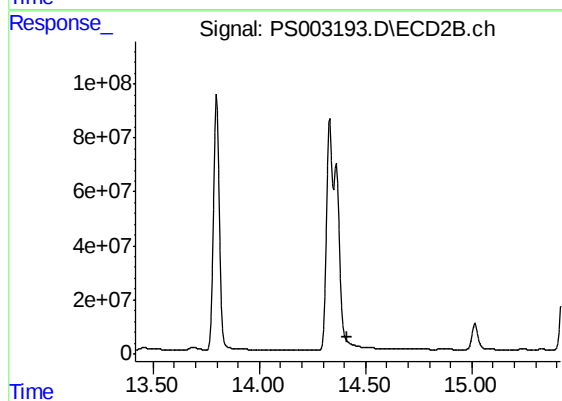

#12 2,4,5-T


R.T.: 14.361 min
Delta R.T.: -0.056 min
Response: -3487174225
Conc: N.D.

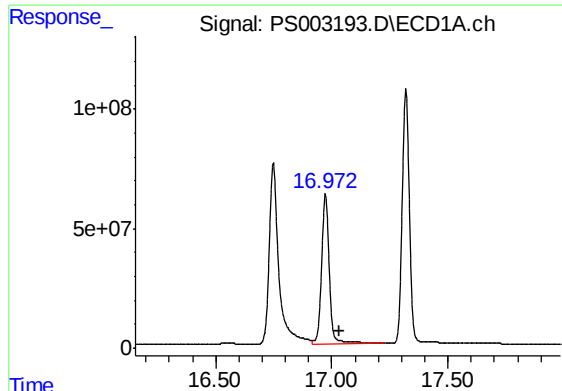

#14 DINOSEB


R.T.: 16.973 min
Delta R.T.: -0.063 min
Response: 1428812879
Conc: 759.47 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

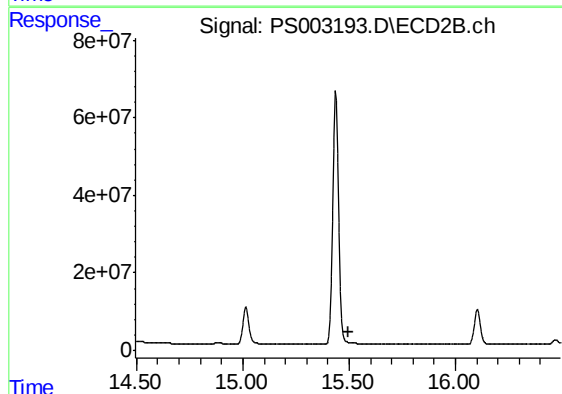


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 15.495 min
Response: 0
Conc: N.D.

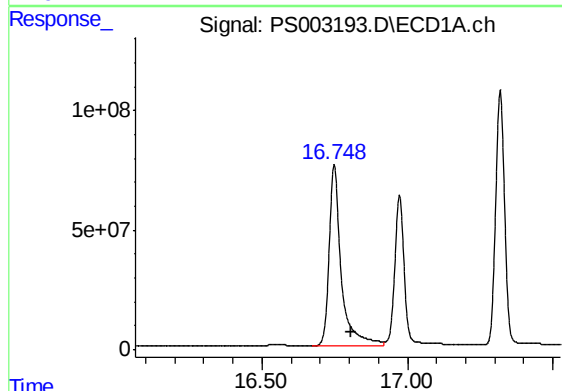


#15 Picloram

R.T.: 16.748 min
Delta R.T.: -0.058 min
Response: 2191470591
Conc: 692.71 ng/ml

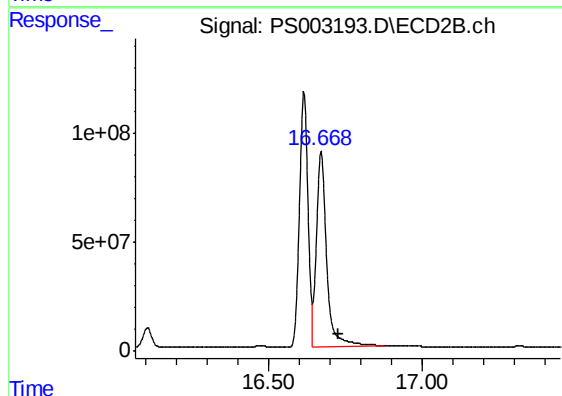

#15 Picloram


R.T.: 16.669 min
Delta R.T.: -0.055 min
Response: 2074365673
Conc: 689.98 ng/ml

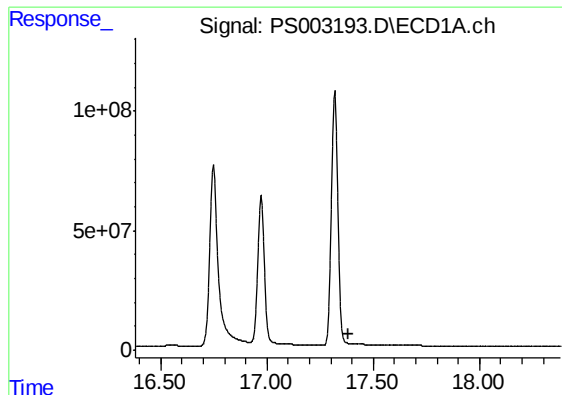

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

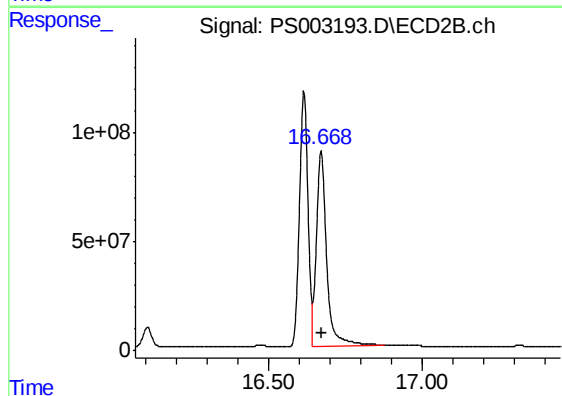

#16 DCPA

R.T.: 16.669 min
Delta R.T.: 0.000 min
Response: 2074365673
Conc: 669.67 ng/ml