

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021419\
 Data File : PS003194.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Feb 2019 22:18
 Operator : EI\SJ
 Sample : K1349-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 OR-01-021319-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 23:38:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.303	10.802	84631160	84424563	222.924	197.463
Target Compounds							
6) T	MCP	11.982	0.000	6340805	0	5.292	N.D. #
12) T	2,4,5-T	0.000	14.417	0	5239595	N.D.	2.738 #
15) T	Picloram	16.829	16.722	10736905	13669979	3.394	4.547 #
16) T	DCPA	0.000	16.656	0	2309022	N.D.	0.745 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021419\
Data File : PS003194.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Feb 2019 22:18
Operator : EI\SJ
Sample : K1349-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
OR-01-021319-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 23:38:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

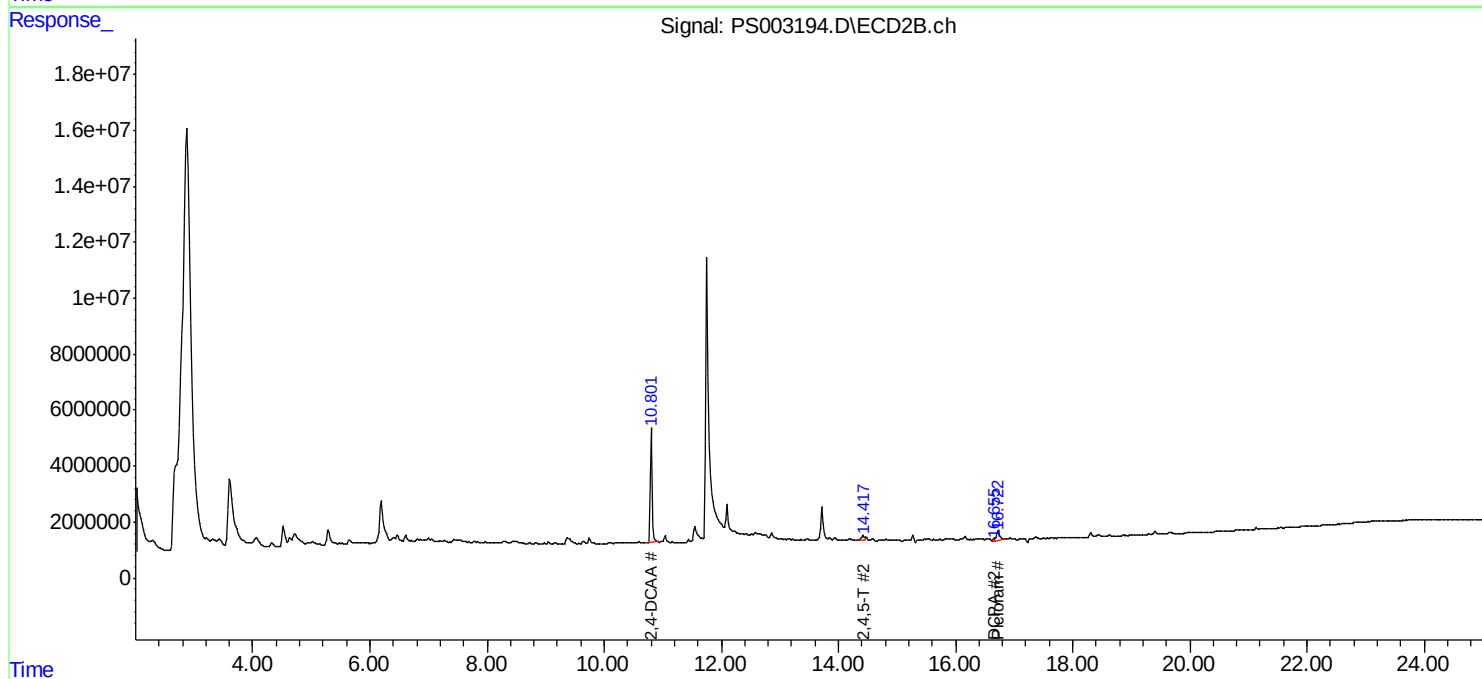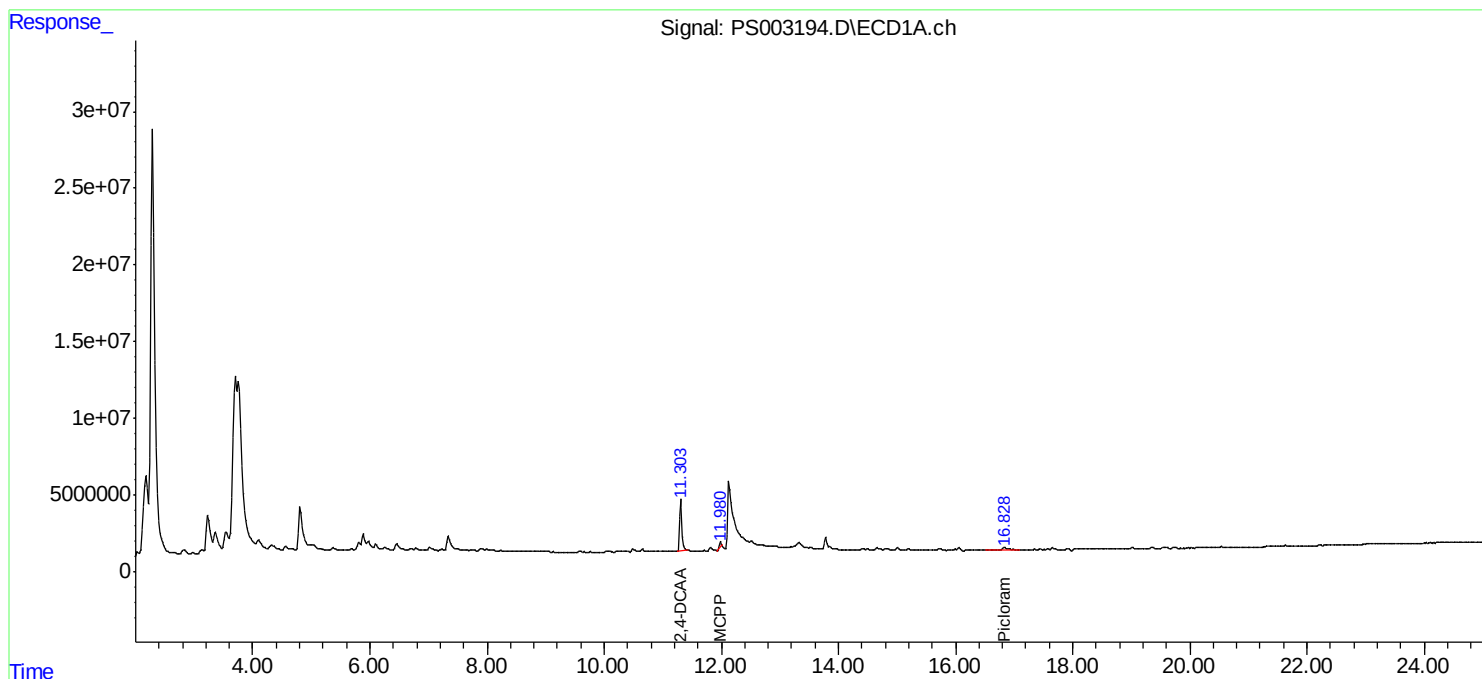


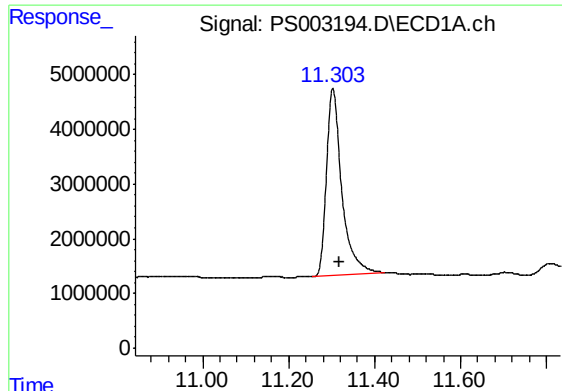

#4 2,4-DCAA


R.T.: 11.303 min
Delta R.T.: -0.015 min
Response: 84631160
Conc: 222.92 ng/ml

Instrument :
ECD_S
ClientSampleId :
OR-01-021319-B

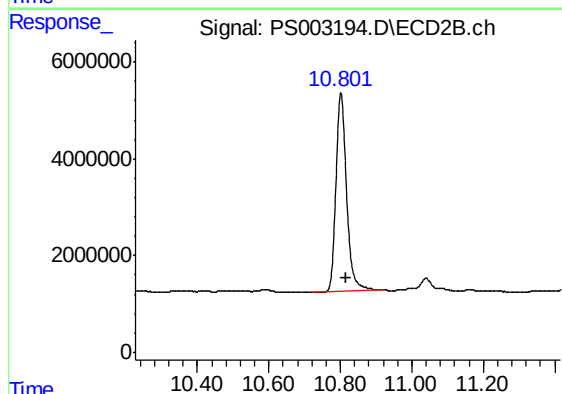


#4 2,4-DCAA

R.T.: 10.802 min
Delta R.T.: -0.015 min
Response: 84424563
Conc: 197.46 ng/ml

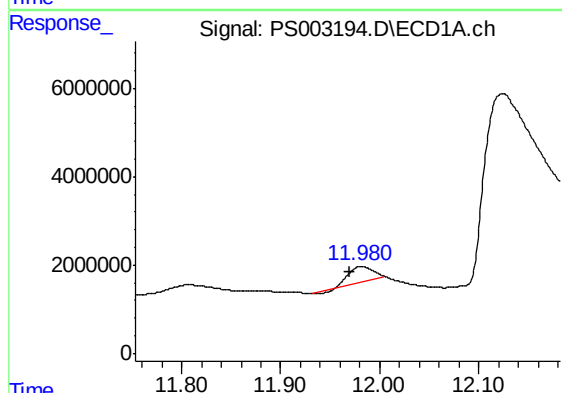


#6 MCP

R.T.: 11.982 min
Delta R.T.: 0.012 min
Response: 6340805
Conc: 5.29 ug/ml

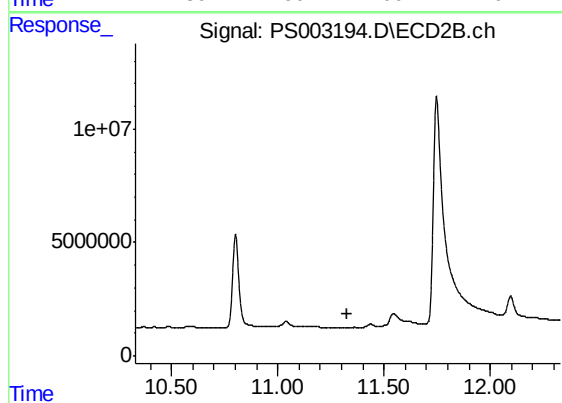

#6 MCP


R.T.: 0.000 min
Exp R.T. : 11.330 min
Response: 0
Conc: N.D.

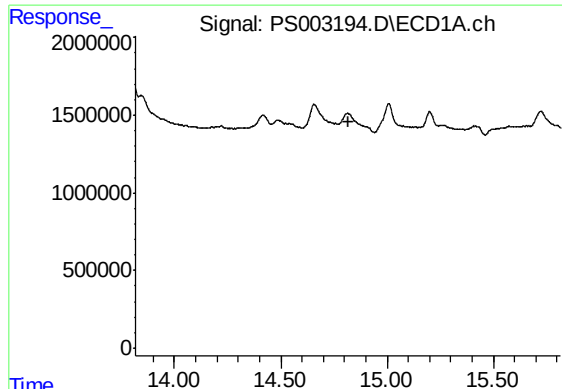

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.817 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
OR-01-021319-B

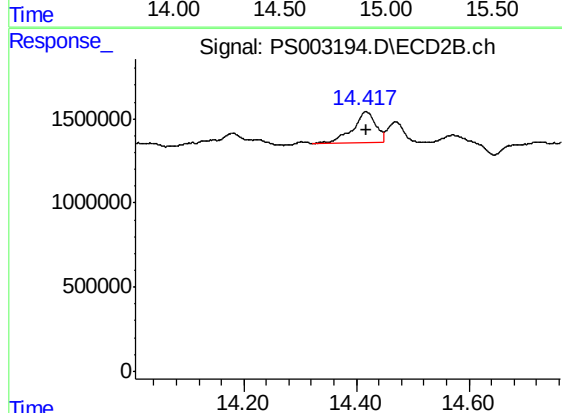


#12 2,4,5-T

R.T.: 14.417 min
Delta R.T.: 0.000 min
Response: 5239595
Conc: 2.74 ng/ml

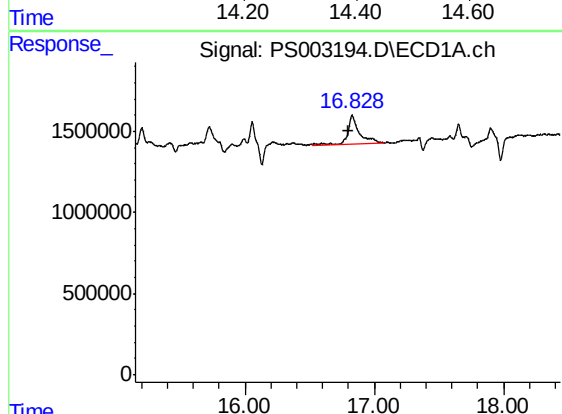


#15 Picloram

R.T.: 16.829 min
Delta R.T.: 0.023 min
Response: 10736905
Conc: 3.39 ng/ml

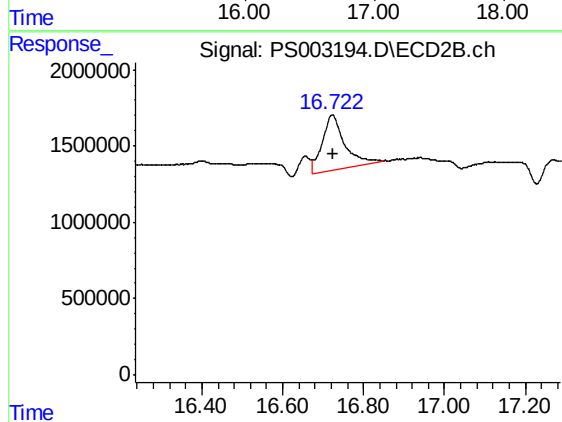

#15 Picloram


R.T.: 16.722 min
Delta R.T.: -0.002 min
Response: 13669979
Conc: 4.55 ng/ml

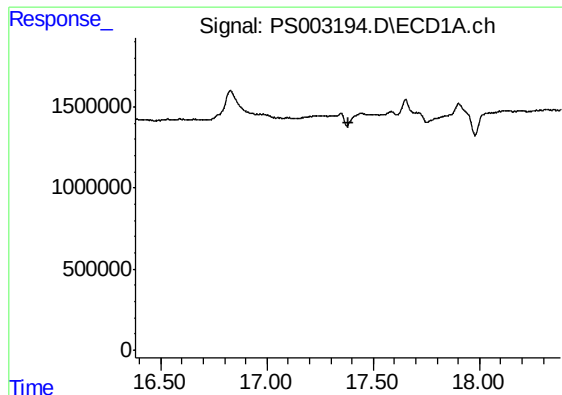

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
OR-01-021319-B

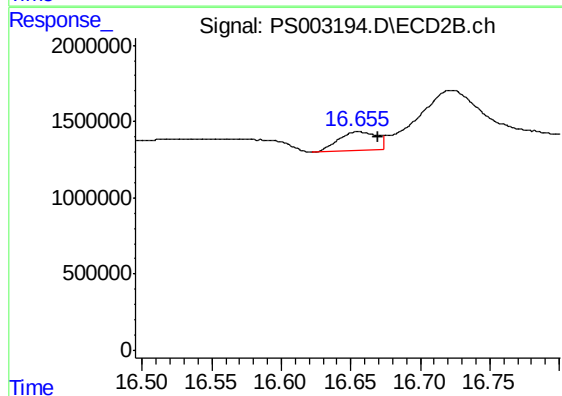

#16 DCPA

R.T.: 16.656 min
Delta R.T.: -0.014 min
Response: 2309022
Conc: 0.75 ng/ml