

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021419\
 Data File : PS003195.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Feb 2019 22:49
 Operator : EI\SJ
 Sample : K1350-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 EO-02-021319-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 23:38:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.299	10.799	124.2E6	122.8E6	327.138	287.173
Target Compounds							
1) T	Dalapon	0.000	2.286	0	8025628	N.D.	14.975 #
6) T	MCP	11.982	0.000	6229669	0	5.200	N.D. #
15) T	Picloram	0.000	16.724	0	7759598	N.D.	2.581 #
16) T	DCPA	0.000	16.724	0	7759598	N.D.	2.505 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021419\
Data File : PS003195.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Feb 2019 22:49
Operator : EI\SJ
Sample : K1350-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
EO-02-021319-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 23:38:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

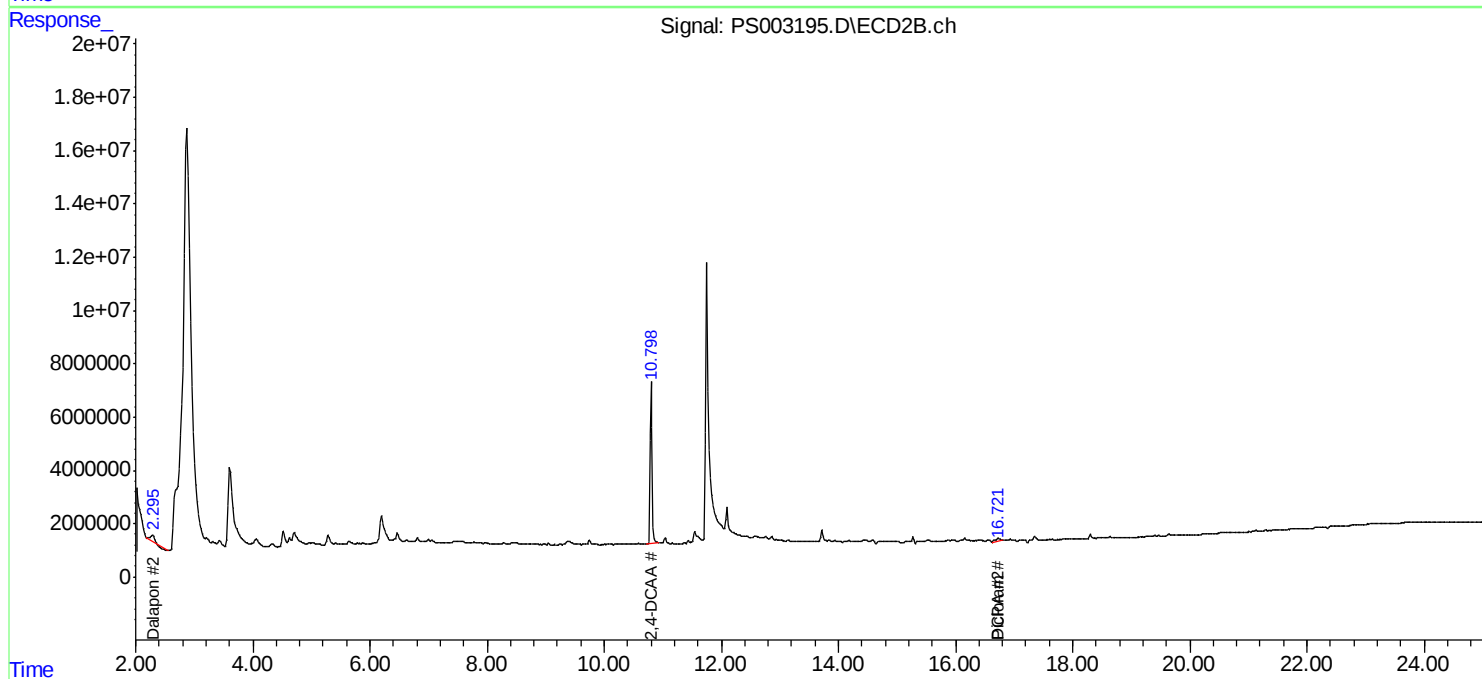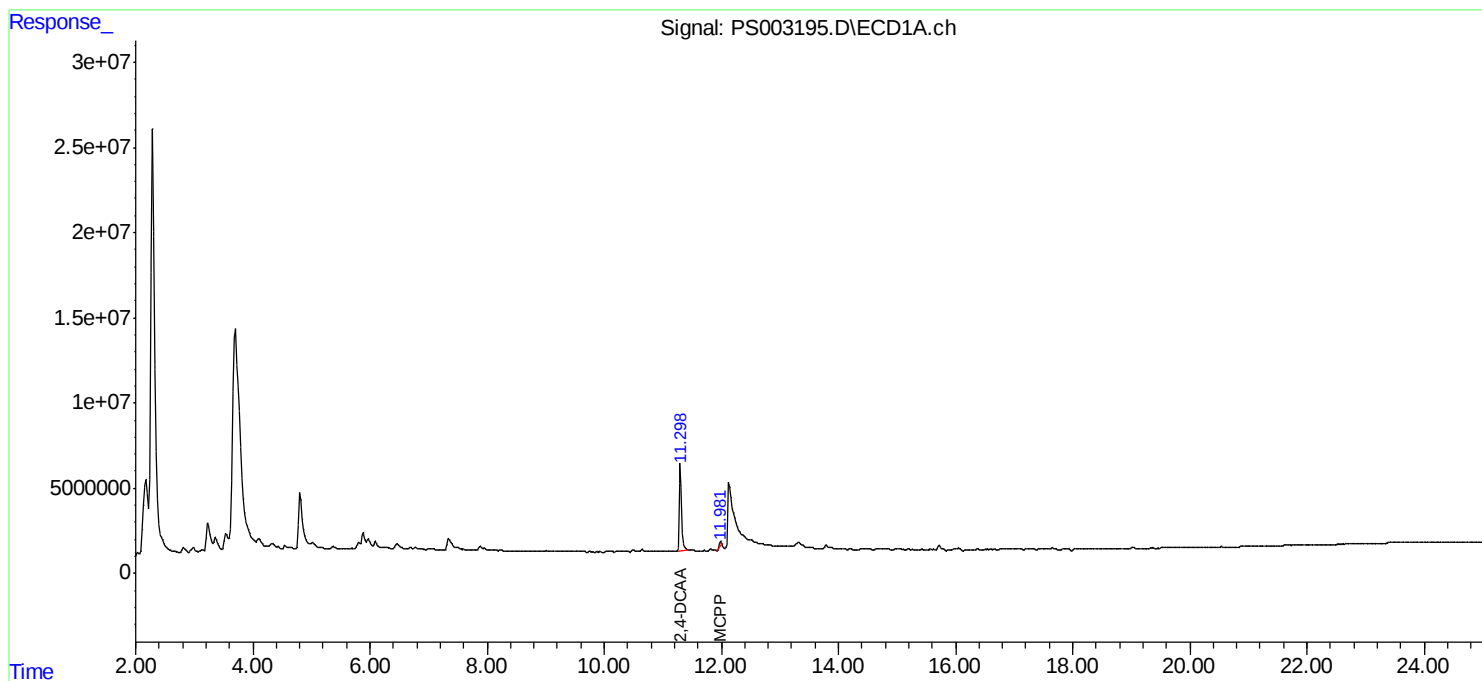


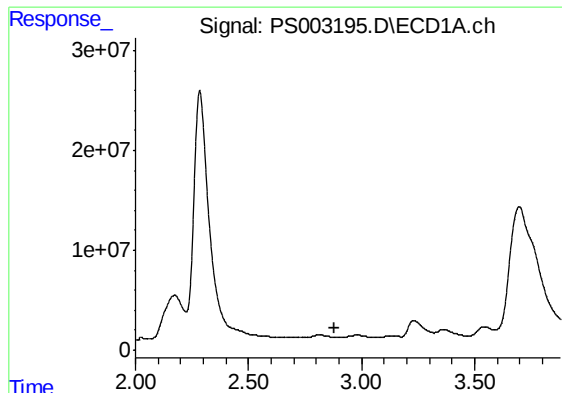

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
EO-02-021319-A

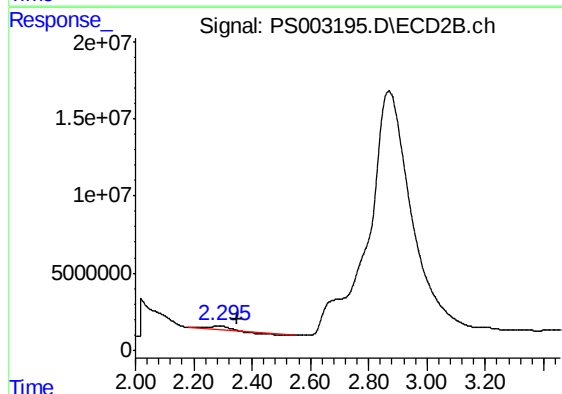


#1 Dalapon

R.T.: 2.286 min
Delta R.T.: -0.064 min
Response: 8025628
Conc: 14.98 ng/ml

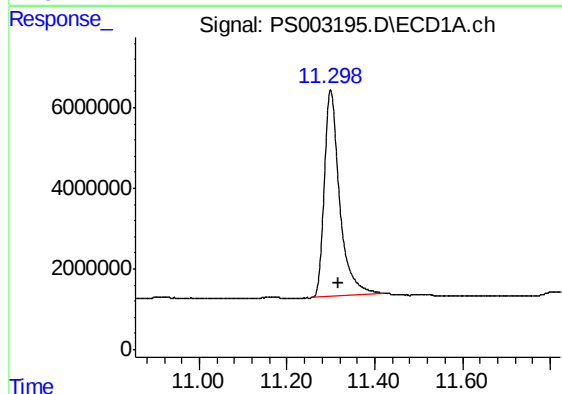


#4 2,4-DCAA

R.T.: 11.299 min
Delta R.T.: -0.019 min
Response: 124195057
Conc: 327.14 ng/ml

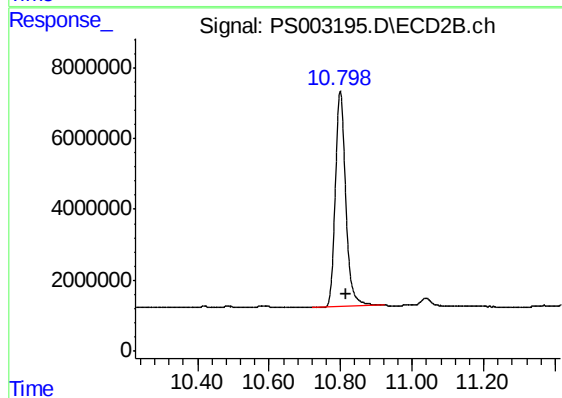

#4 2,4-DCAA


R.T.: 10.799 min
Delta R.T.: -0.018 min
Response: 122779380
Conc: 287.17 ng/ml

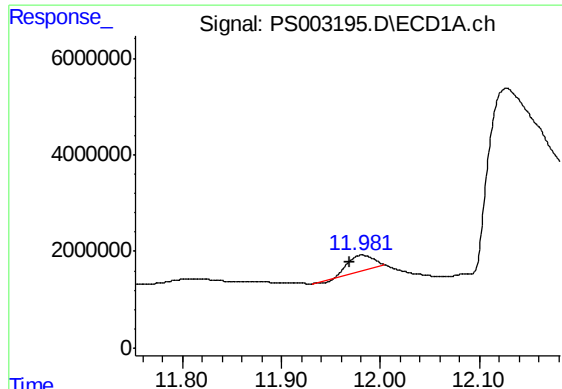

#6 MCP


R.T.: 11.982 min
Delta R.T.: 0.012 min
Response: 6229669
Conc: 5.20 ug/ml

Instrument :
ECD_S
ClientSampleId :
EO-02-021319-A

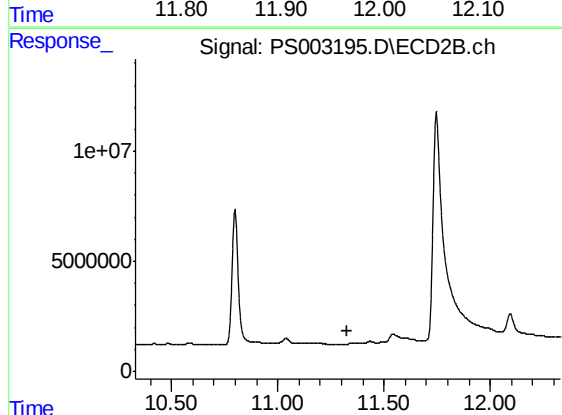


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.330 min
Response: 0
Conc: N.D.

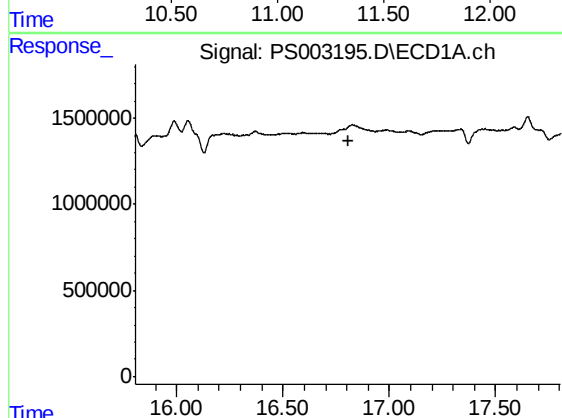


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.806 min
Response: 0
Conc: N.D.

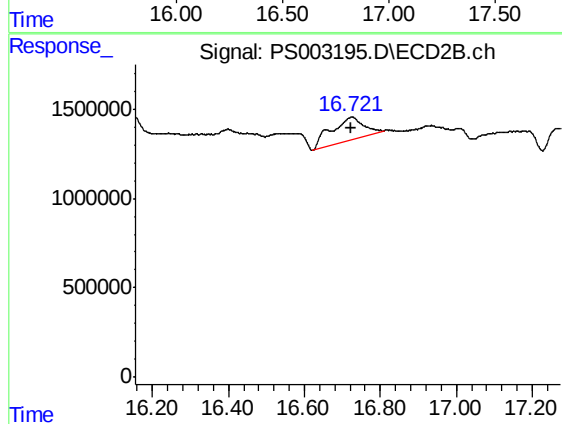

#15 Picloram


R.T.: 16.724 min
Delta R.T.: 0.000 min
Response: 7759598
Conc: 2.58 ng/ml

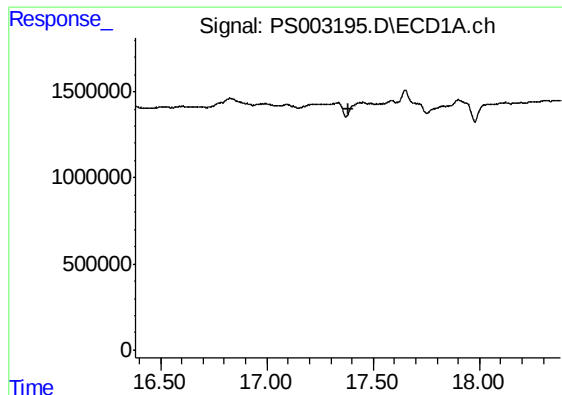

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
EO-02-021319-A

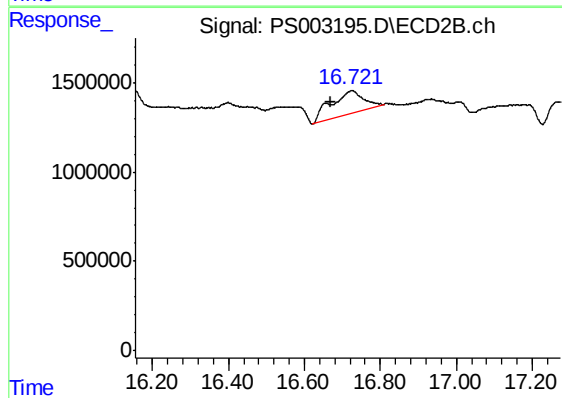

#16 DCPA

R.T.: 16.724 min
Delta R.T.: 0.055 min
Response: 7759598
Conc: 2.51 ng/ml