

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021419\
 Data File : PS003196.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Feb 2019 23:20
 Operator : EI\SJ
 Sample : K1350-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 15 01:19:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.280	10.780	76731847	158.7E6	202.117	371.226 #
Target Compounds							
2) T	3,5-DICHL...	0.000	9.030	0	2492453	N.D.	4.423 #
3) T	4-Nitroph...	0.000	9.950	0	1676583	N.D.	8.021 #
5) T	DICAMBA	11.693	11.148	17869793	549436	11.148	0.346 #
6) T	MCP	11.954	0.000	20948224	0	17.484	N.D. #
7) T	MCPA	0.000	11.721	0	198.3E6	N.D.	126.032 #
9) T	2,4-D	13.194	0.000	6943358	0	15.060	N.D. #
12) T	2,4,5-T	0.000	14.388	0	6188881	N.D.	3.234 #
15) T	Picloram	16.787	16.696	6009615	5820011	1.900	1.936
16) T	DCPA	17.404	16.696	-1078931	5820011	N.D.	1.879



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021419\
Data File : PS003196.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Feb 2019 23:20
Operator : EI\SJ
Sample : K1350-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 15 01:19:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

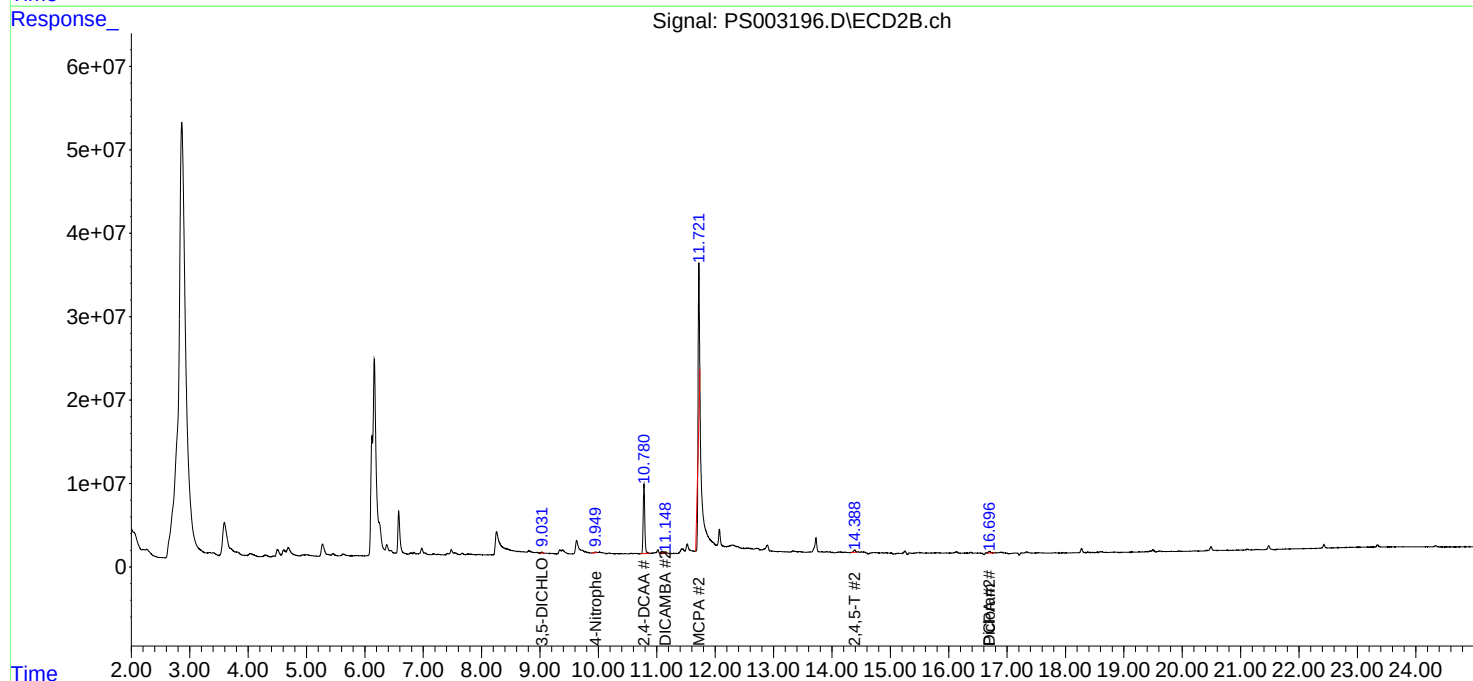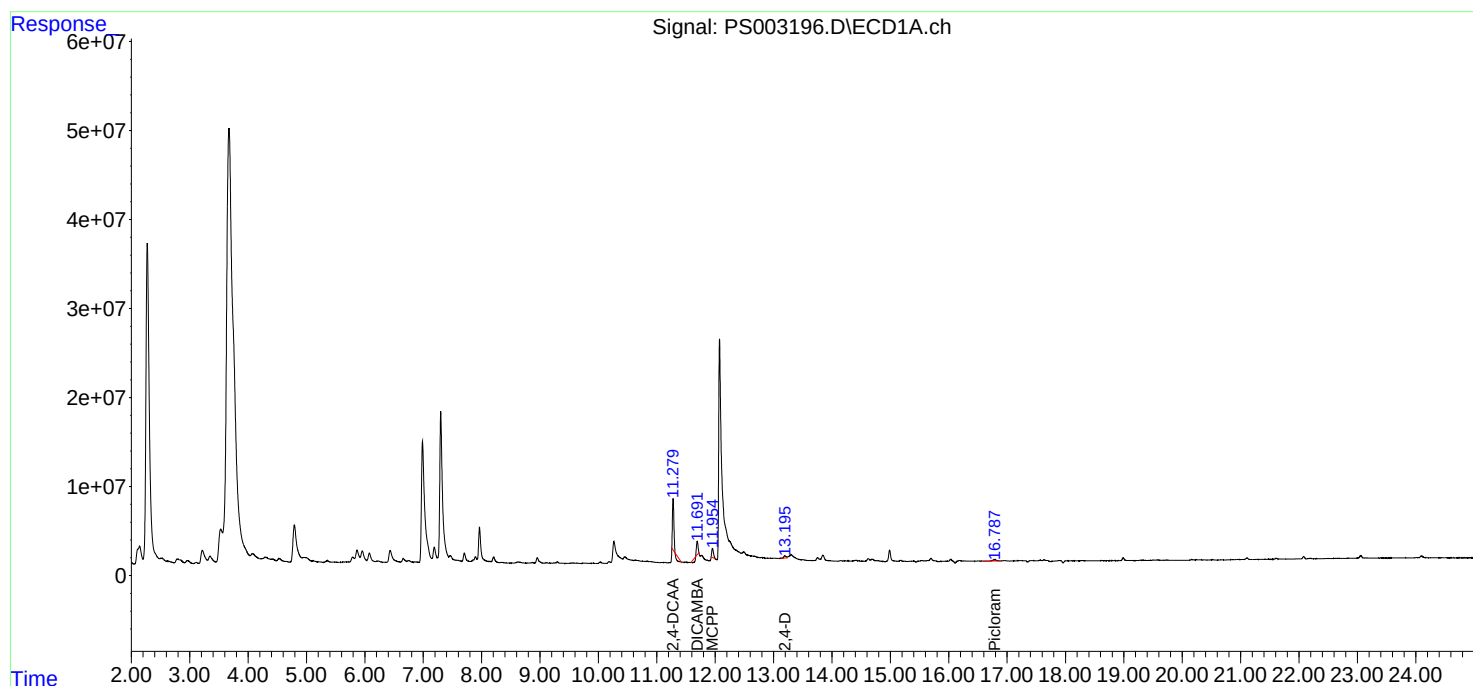


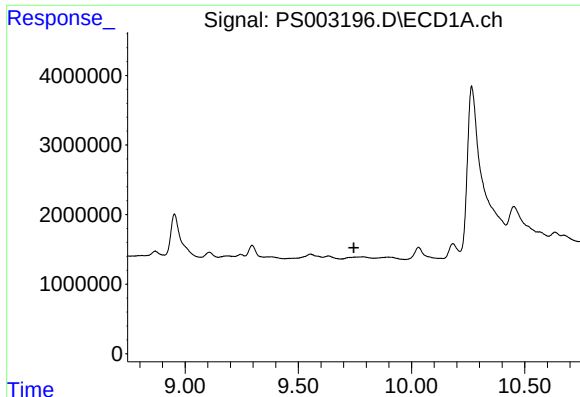

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.745 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

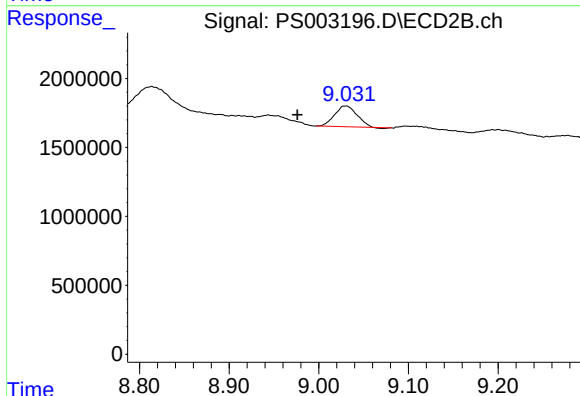


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.030 min
Delta R.T.: 0.054 min
Response: 2492453
Conc: 4.42 ng/ml

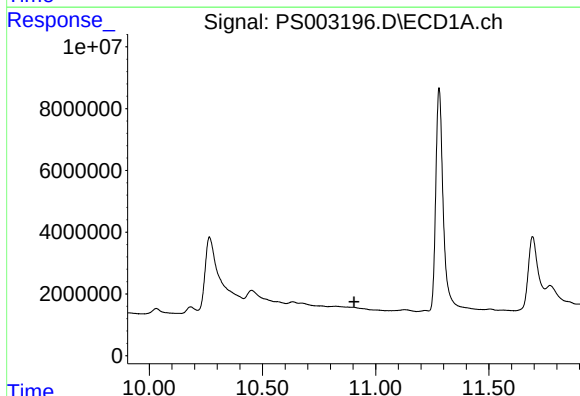


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 10.904 min
Response: 0
Conc: N.D.

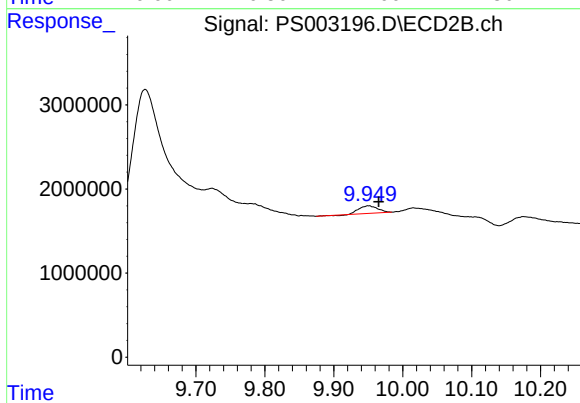

#3 4-Nitrophenol


R.T.: 9.950 min
Delta R.T.: -0.015 min
Response: 1676583
Conc: 8.02 ng/ml

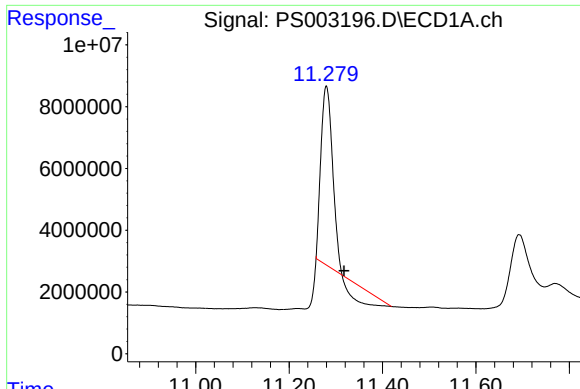

#4 2,4-DCAA


R.T.: 11.280 min
Delta R.T.: -0.038 min
Response: 76731847
Conc: 202.12 ng/ml

Instrument :
ECD_S
ClientSampleId :

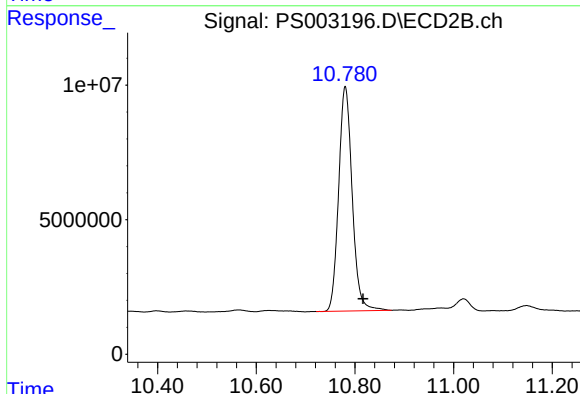


#4 2,4-DCAA

R.T.: 10.780 min
Delta R.T.: -0.036 min
Response: 158716302
Conc: 371.23 ng/ml

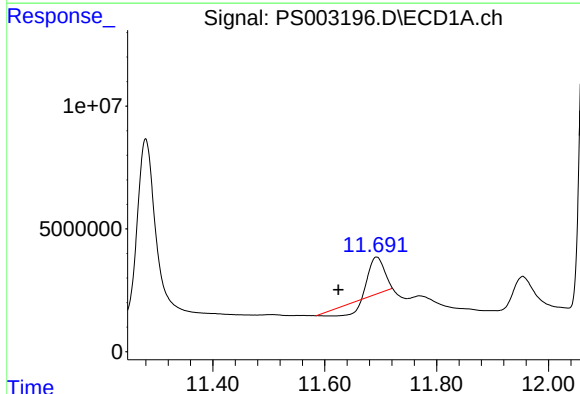


#5 DICAMBA

R.T.: 11.693 min
Delta R.T.: 0.069 min
Response: 17869793
Conc: 11.15 ng/ml

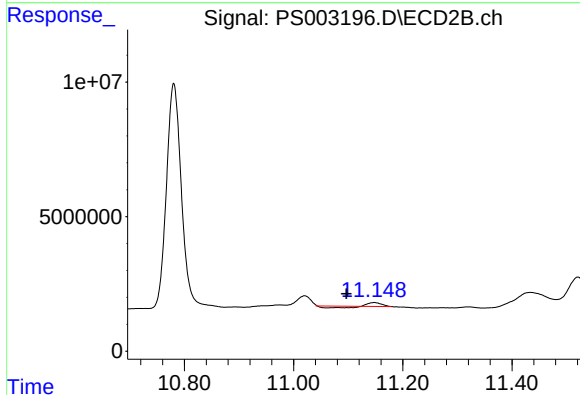

#5 DICAMBA


R.T.: 11.148 min
Delta R.T.: 0.051 min
Response: 549436
Conc: 0.35 ng/ml

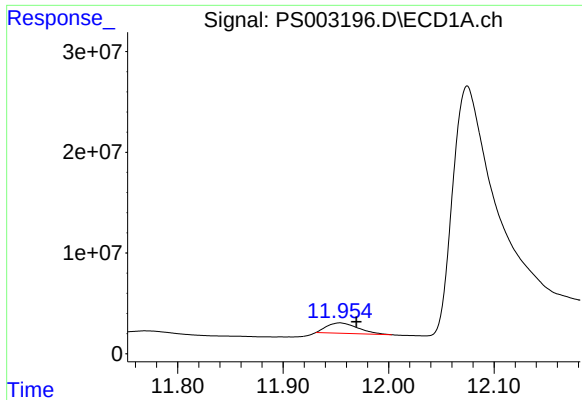

#6 MCPP


R.T.: 11.954 min
Delta R.T.: -0.015 min
Response: 20948224
Conc: 17.48 ug/ml

Instrument :
ECD_S
ClientSampleId :

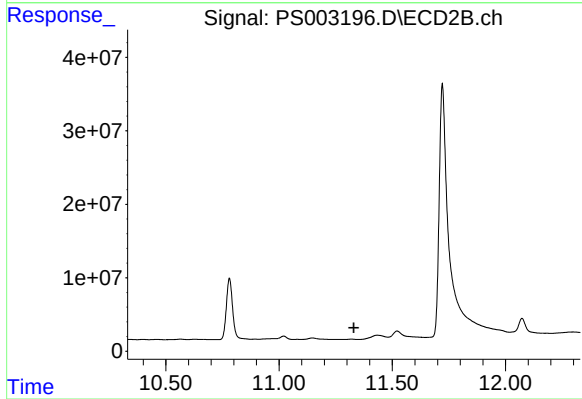


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.330 min
Response: 0
Conc: N.D.

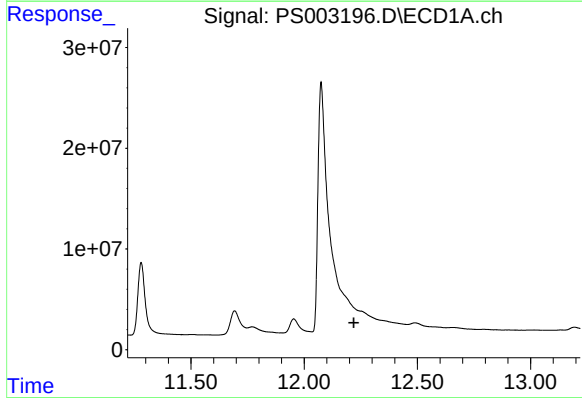


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.219 min
Response: 0
Conc: N.D.

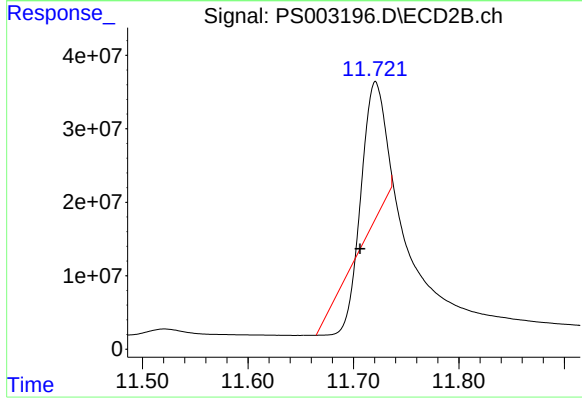

#7 MCPA


R.T.: 11.721 min
Delta R.T.: 0.015 min
Response: 198255751
Conc: 126.03 ug/ml

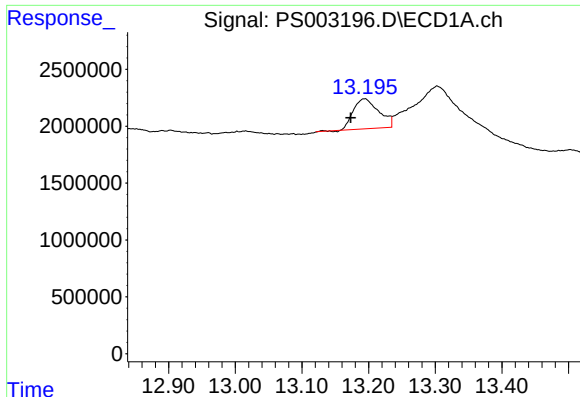

#9 2,4-D


R.T.: 13.194 min
Delta R.T.: 0.020 min
Response: 6943358
Conc: 15.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

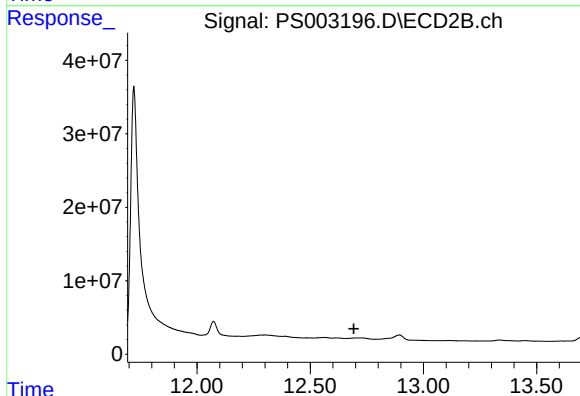


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 12.693 min
Response: 0
Conc: N.D.

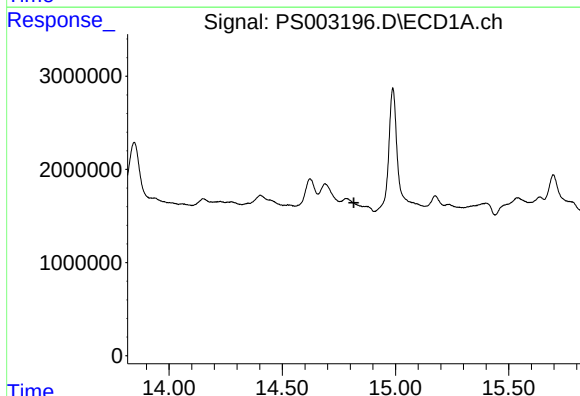


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.817 min
Response: 0
Conc: N.D.

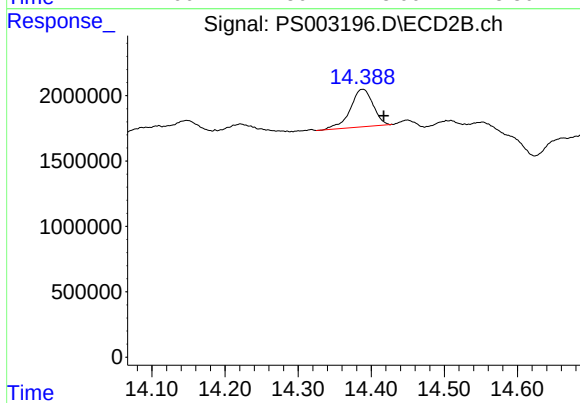

#12 2,4,5-T


R.T.: 14.388 min
Delta R.T.: -0.029 min
Response: 6188881
Conc: 3.23 ng/ml

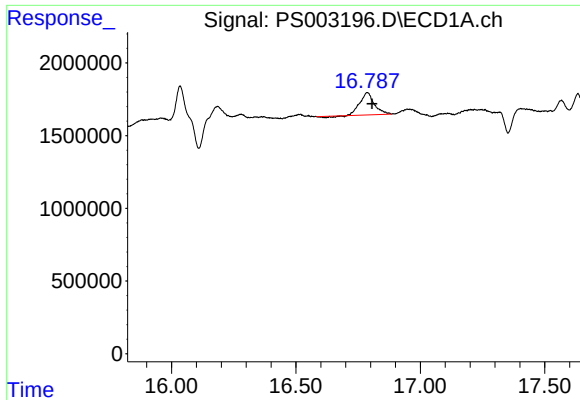

#15 Picloram


R.T.: 16.787 min
Delta R.T.: -0.019 min
Response: 6009615
Conc: 1.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

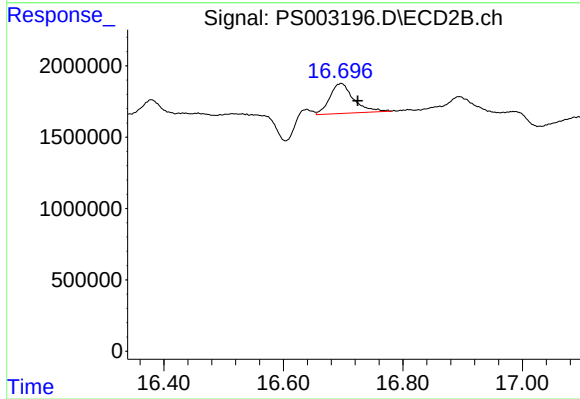


#15 Picloram

R.T.: 16.696 min
Delta R.T.: -0.028 min
Response: 5820011
Conc: 1.94 ng/ml

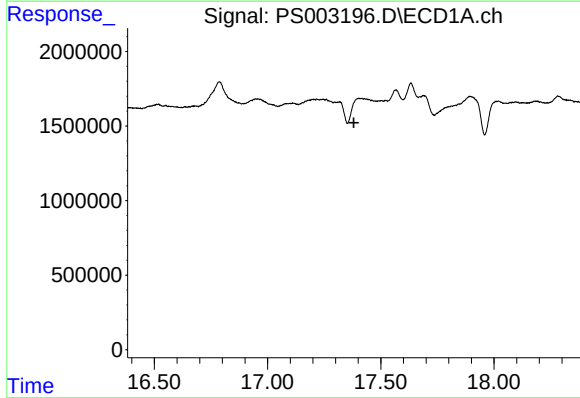

#16 DCPA

R.T.: 17.404 min
Delta R.T.: 0.023 min
Response: -1078931
Conc: N.D.

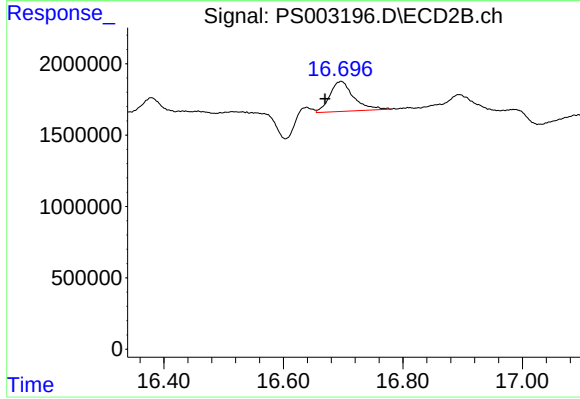

#16 DCPA

R.T.: 16.696 min
Delta R.T.: 0.026 min
Response: 5820011
Conc: 1.88 ng/ml