

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021419\
 Data File : PS003197.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Feb 2019 23:51
 Operator : EI\SJ
 Sample : K1350-10
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 15 01:19:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.759	0	137.9E6	N.D.	322.642 #
Target Compounds							
1) T	Dalapon	2.947	0.000	18765624	0	34.017	N.D. #
2) T	3,5-DICHL...	0.000	9.009	0	1339436	N.D.	2.377 #
3) T	4-Nitroph...	0.000	9.922	0	36538058	N.D.	174.804 #
5) T	DICAMBA	11.671	11.126	53813365	6341367	33.573	3.997 #
7) T	MCPA	0.000	11.698	0	637.4E6	N.D.	405.193 #
8) T	DICHLORPROP	0.000	12.276	0	1952974	N.D.	5.108 #
9) T	2,4-D	13.170	0.000	12722657	0	27.594	N.D. #
12) T	2,4,5-T	0.000	14.367	0	3251127	N.D.	1.699 #
15) T	Picloram	0.000	16.674	0	8696328	N.D.	2.893 #
16) T	DCPA	17.412	16.674	2366622	8696328	0.787	2.807 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021419\
Data File : PS003197.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Feb 2019 23:51
Operator : EI\SJ
Sample : K1350-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 15 01:19:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

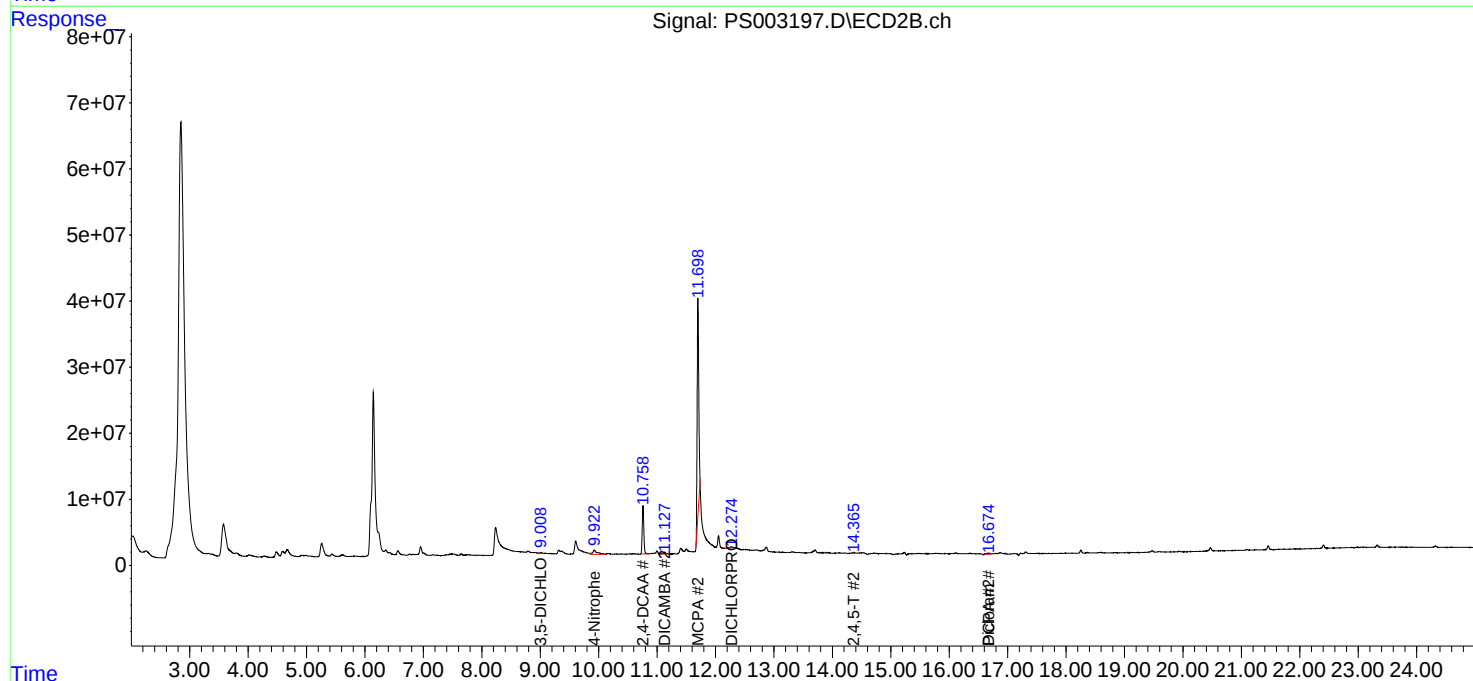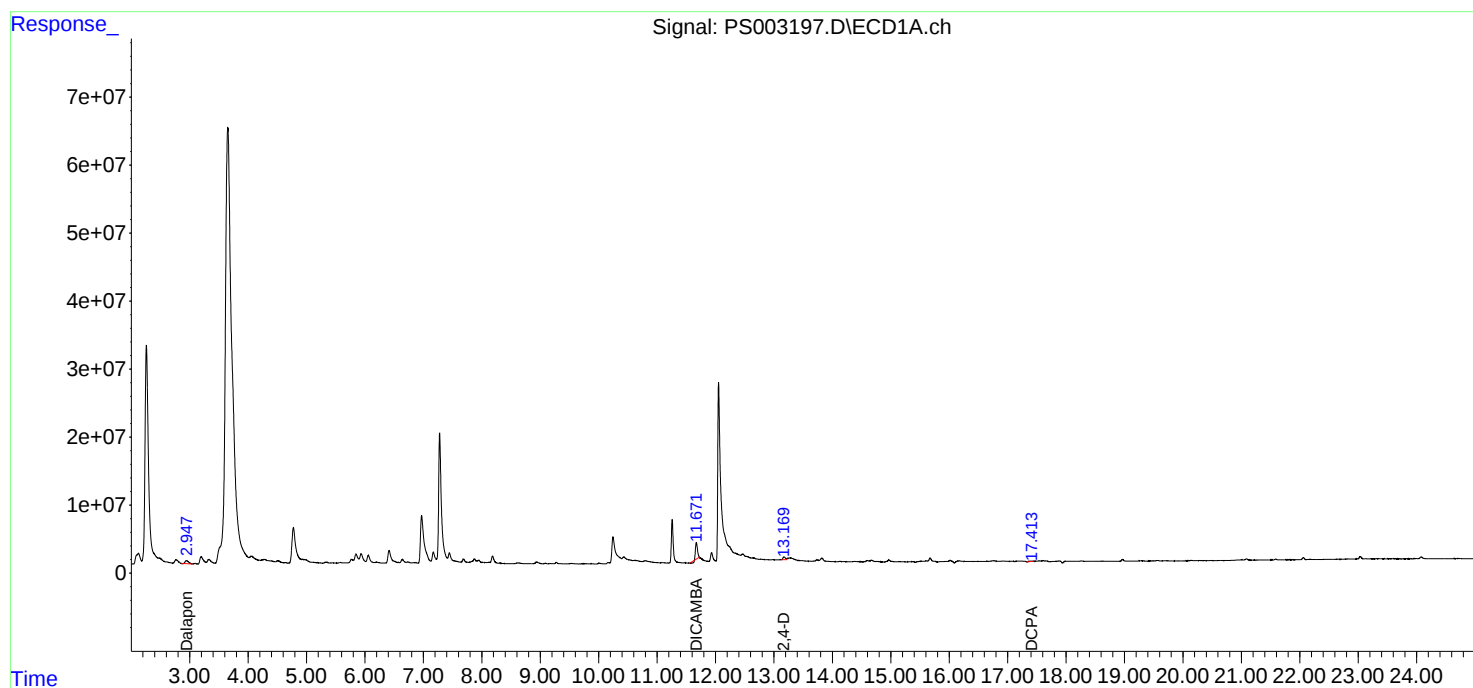


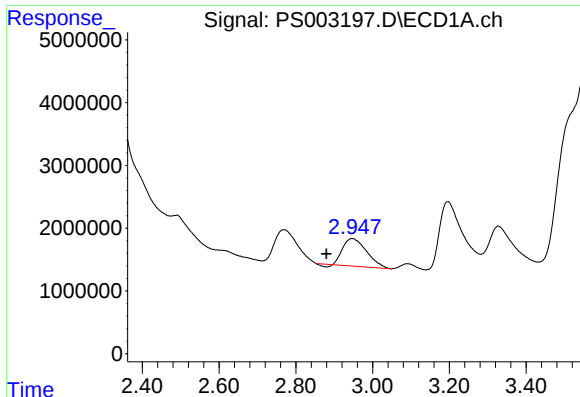

#1 Dalapon


R.T.: 2.947 min
Delta R.T.: 0.067 min
Response: 18765624
Conc: 34.02 ng/ml

Instrument :
ECD_S
ClientSampleId :

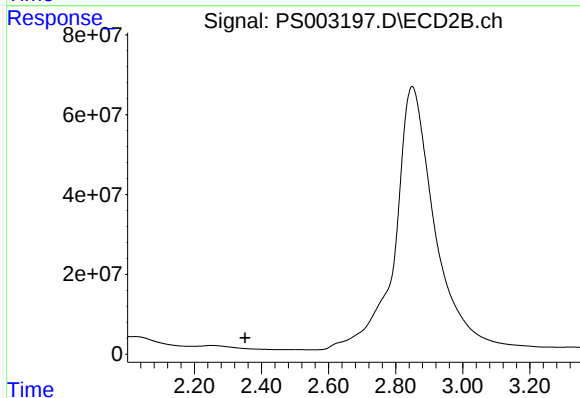


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.351 min
Response: 0
Conc: N.D.

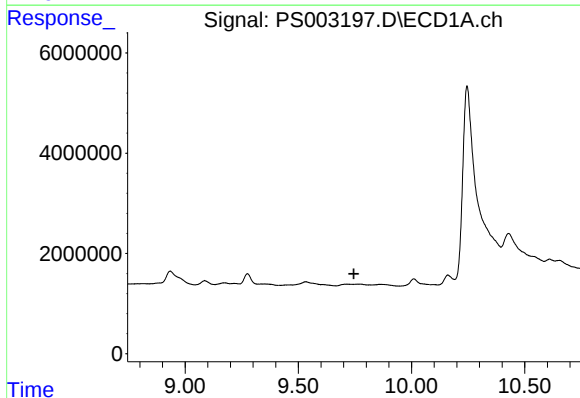


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.745 min
Response: 0
Conc: N.D.

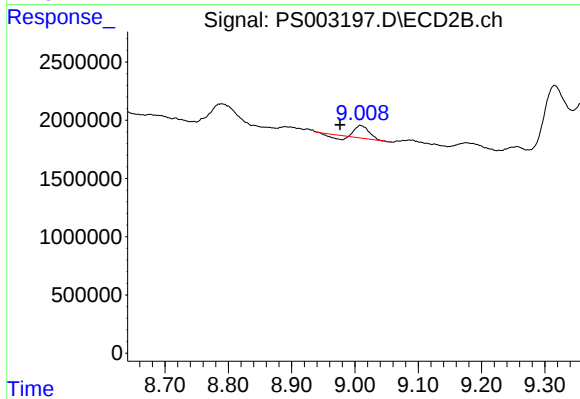

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.009 min
Delta R.T.: 0.033 min
Response: 1339436
Conc: 2.38 ng/ml

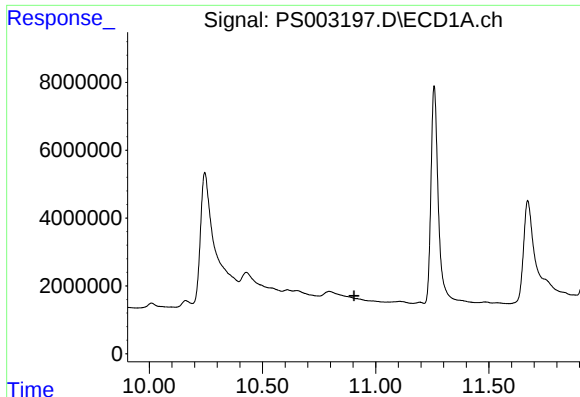

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.904 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

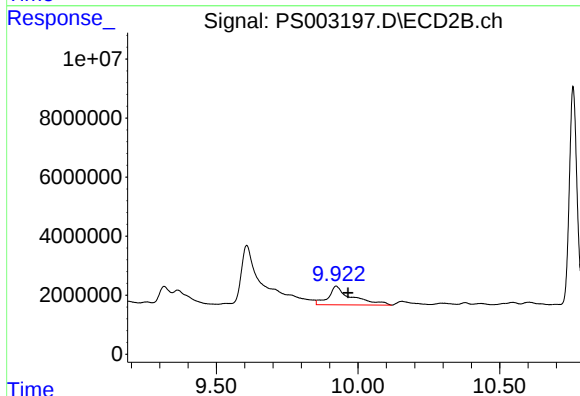


#3 4-Nitrophenol

R.T.: 9.922 min
Delta R.T.: -0.043 min
Response: 36538058
Conc: 174.80 ng/ml

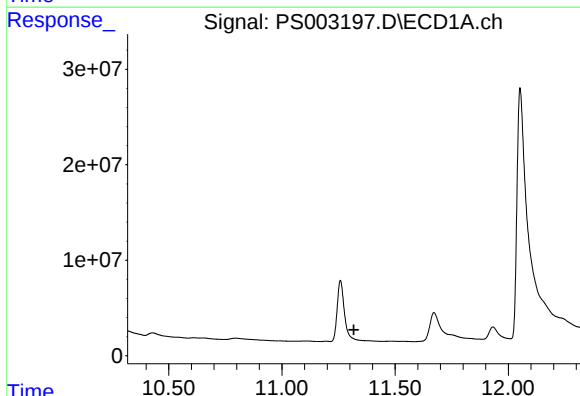


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 11.318 min
Response: 0
Conc: N.D.

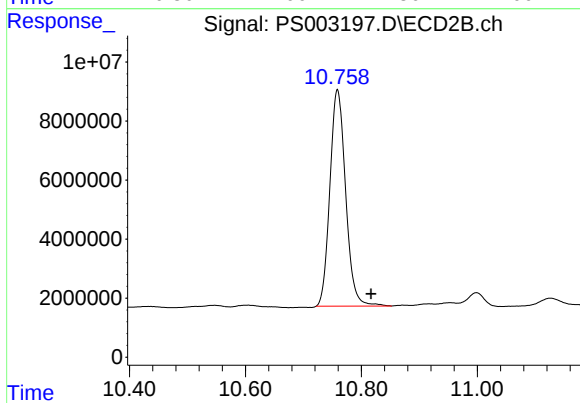

#4 2,4-DCAA


R.T.: 10.759 min
Delta R.T.: -0.058 min
Response: 137944122
Conc: 322.64 ng/ml

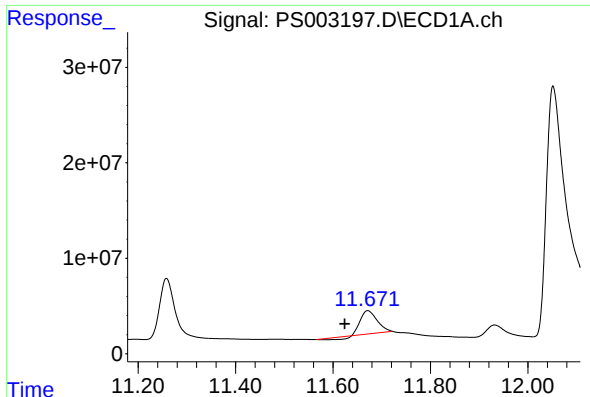

#5 DICAMBA


R.T.: 11.671 min
Delta R.T.: 0.047 min
Response: 53813365
Conc: 33.57 ng/ml

Instrument :
ECD_S
ClientSampleId :

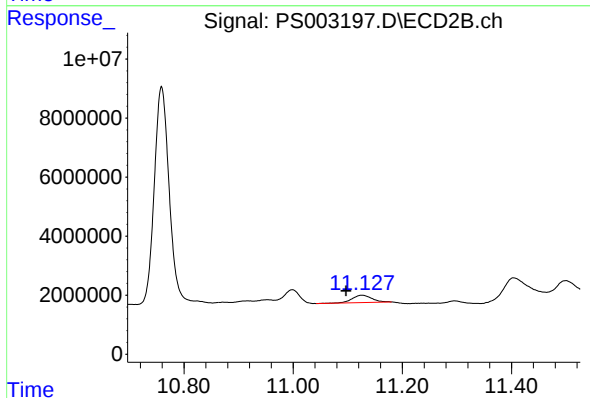


#5 DICAMBA

R.T.: 11.126 min
Delta R.T.: 0.029 min
Response: 6341367
Conc: 4.00 ng/ml

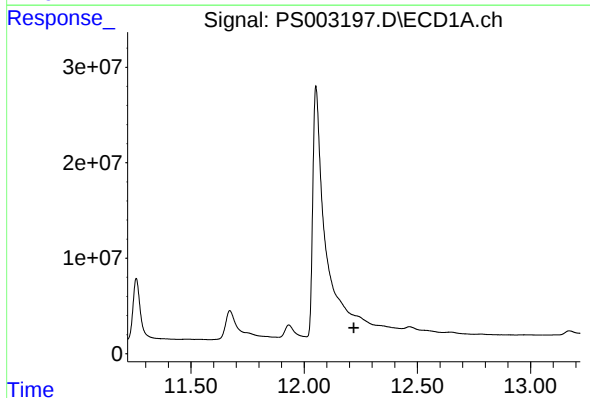


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.219 min
Response: 0
Conc: N.D.

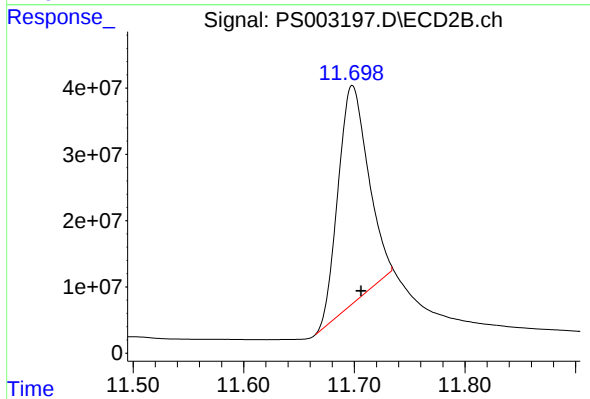

#7 MCPA


R.T.: 11.698 min
Delta R.T.: -0.008 min
Response: 637393896
Conc: 405.19 ug/ml

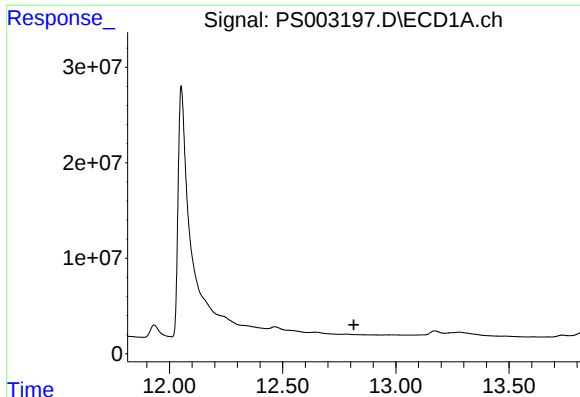

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.815 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

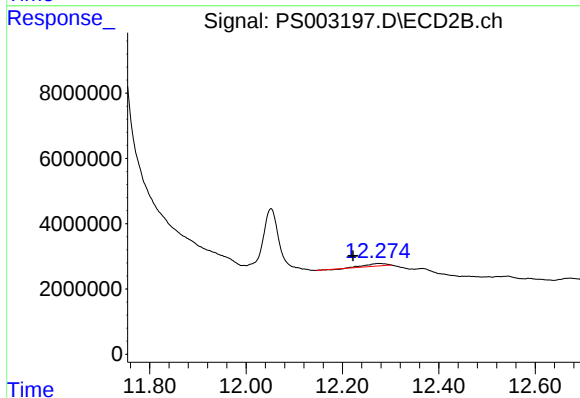


#8 DICHLORPROP

R.T.: 12.276 min
Delta R.T.: 0.054 min
Response: 1952974
Conc: 5.11 ng/ml

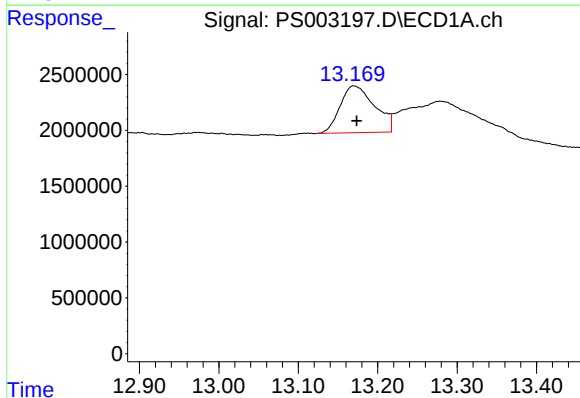


#9 2,4-D

R.T.: 13.170 min
Delta R.T.: -0.003 min
Response: 12722657
Conc: 27.59 ng/ml

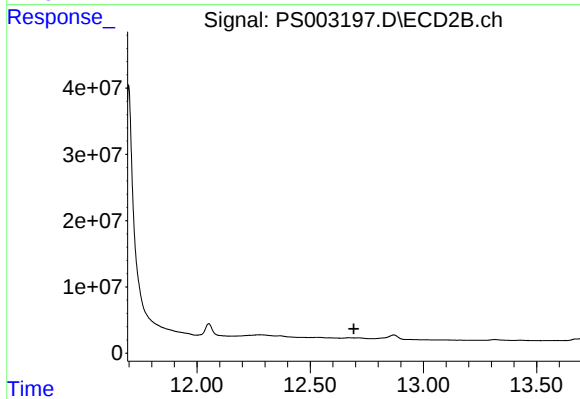

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 12.693 min
Response: 0
Conc: N.D.

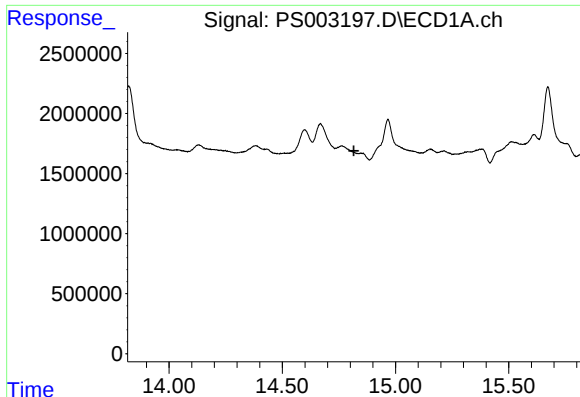

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 14.817 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

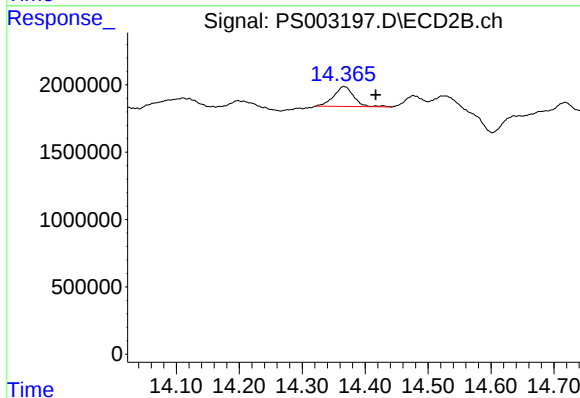


#12 2,4,5-T

R.T.: 14.367 min
Delta R.T.: -0.050 min
Response: 3251127
Conc: 1.70 ng/ml

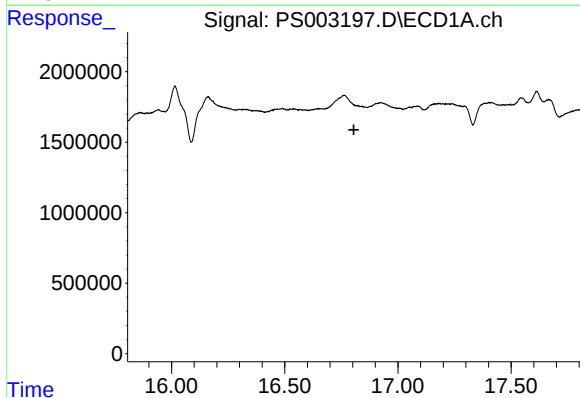


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.806 min
Response: 0
Conc: N.D.

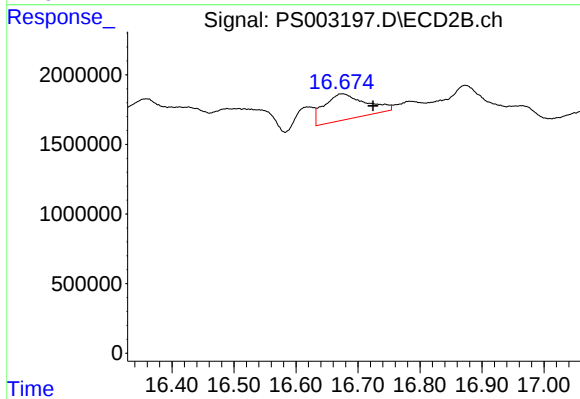

#15 Picloram


R.T.: 16.674 min
Delta R.T.: -0.050 min
Response: 8696328
Conc: 2.89 ng/ml

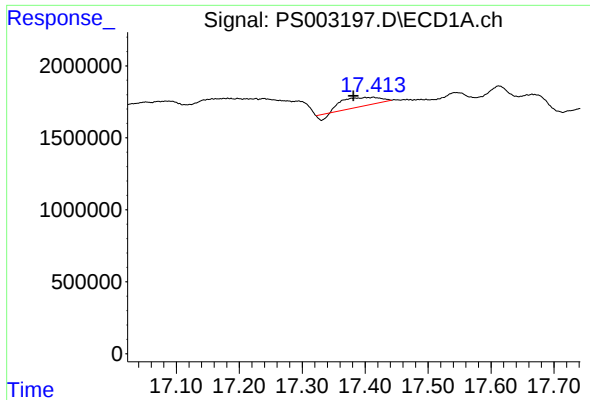

#16 DCPA

R.T.: 17.412 min
Delta R.T.: 0.031 min
Response: 2366622
Conc: 0.79 ng/ml

Instrument :
ECD_S
ClientSampleId :

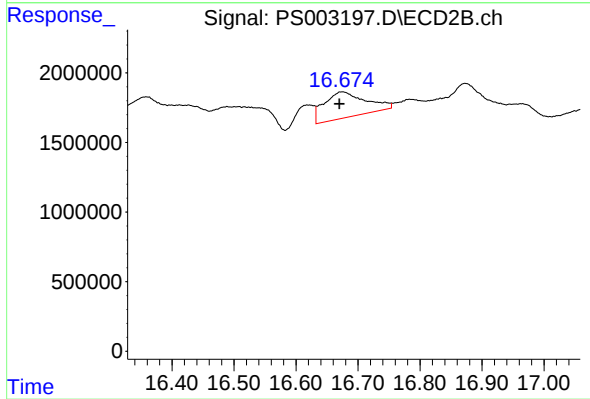

#16 DCPA

R.T.: 16.674 min
Delta R.T.: 0.005 min
Response: 8696328
Conc: 2.81 ng/ml