

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021419\
 Data File : PS003199.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Feb 2019 00:54
 Operator : EI\SJ
 Sample : K1480-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 15 01:20:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.278	10.780	120.9E6	172.0E6	318.500	402.316 #
Target Compounds							
3) T	4-Nitroph...	0.000	9.936	0	29492072	N.D.	141.095 #
5) T	DICAMBA	11.693	11.163	39351070	-728895	24.550	N.D. #
6) T	MCP	0.000	11.347	0	23386309	N.D.	21.203 #
7) T	MCPA	0.000	11.723	0	109.9E6	N.D.	69.850 #
8) T	DICHLORPROP	12.850	0.000	13907089	0	36.261	N.D. #
9) T	2,4-D	13.194	0.000	11081628	0	24.035	N.D. #
11) T	2,4,5-TP ...	14.485	13.858	12187932	18812449	4.840	7.585 #
13) T	2,4-DB	15.607	15.068	-804532	1210557	N.D.	4.766
15) T	Picloram	16.826	16.724	5965710	10701710	1.886	3.560 #
16) T	DCPA	0.000	16.635	0	5234742	N.D.	1.690 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021419\
Data File : PS003199.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Feb 2019 00:54
Operator : EI\SJ
Sample : K1480-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 15 01:20:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

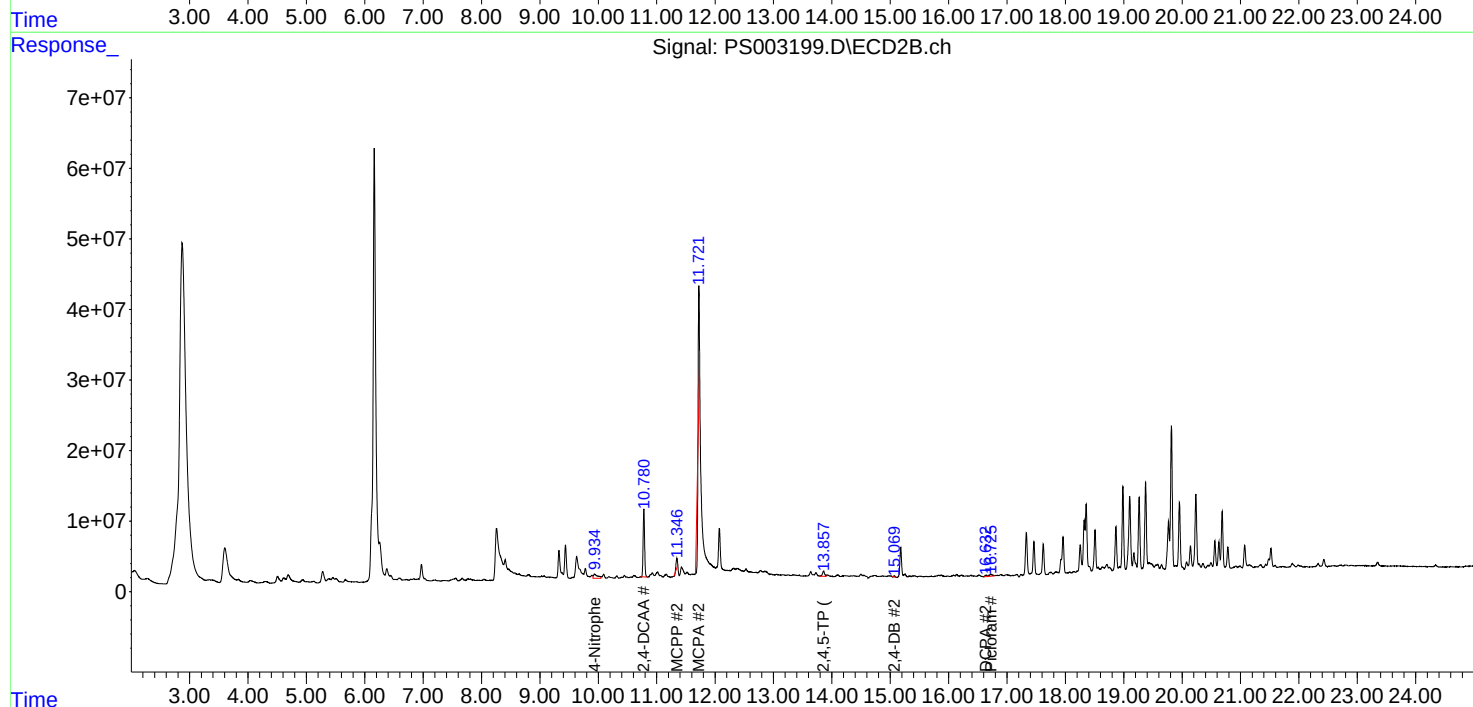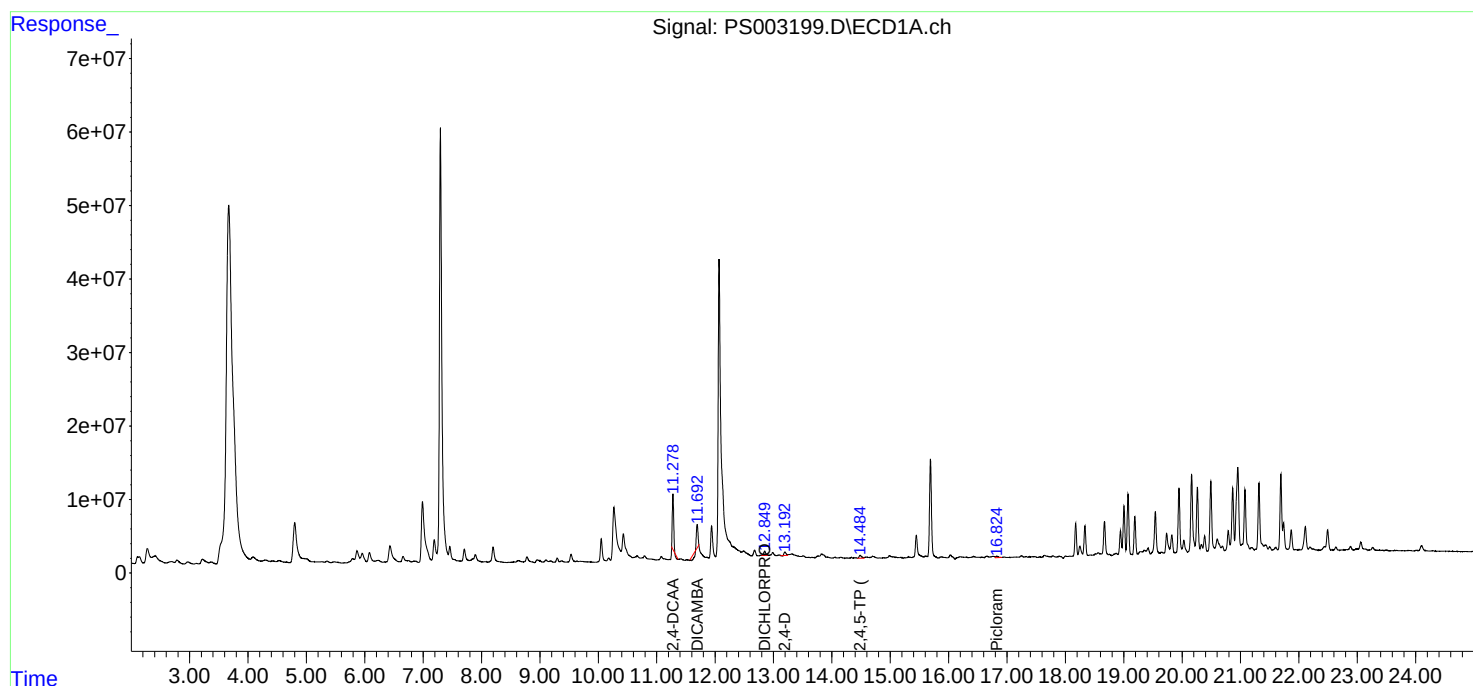


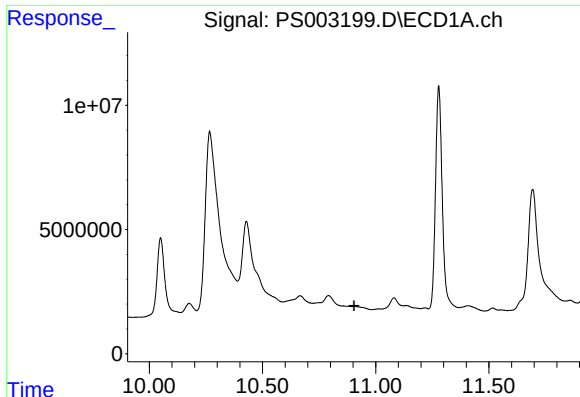

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.904 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

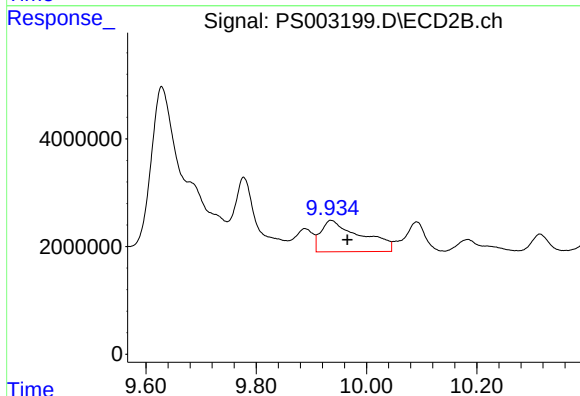


#3 4-Nitrophenol

R.T.: 9.936 min
Delta R.T.: -0.029 min
Response: 29492072
Conc: 141.10 ng/ml

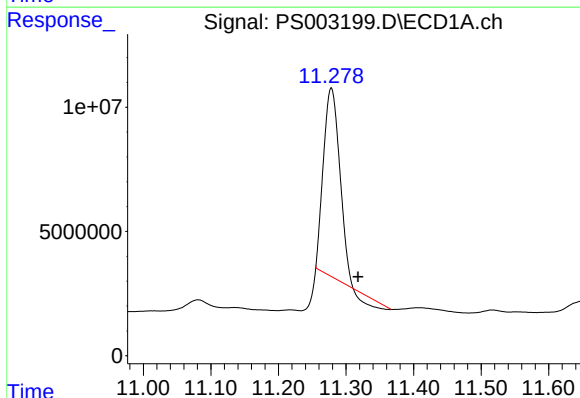


#4 2,4-DCAA

R.T.: 11.278 min
Delta R.T.: -0.039 min
Response: 120915419
Conc: 318.50 ng/ml

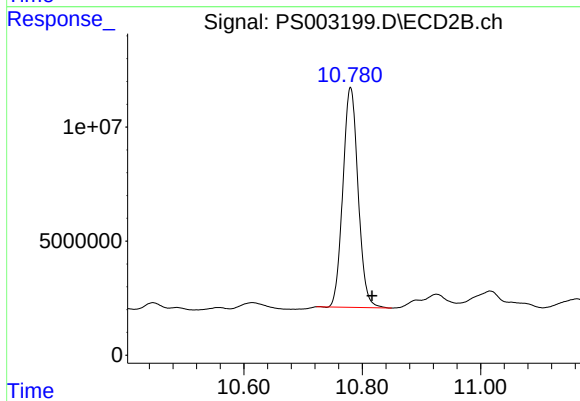

#4 2,4-DCAA


R.T.: 10.780 min
Delta R.T.: -0.036 min
Response: 172008446
Conc: 402.32 ng/ml

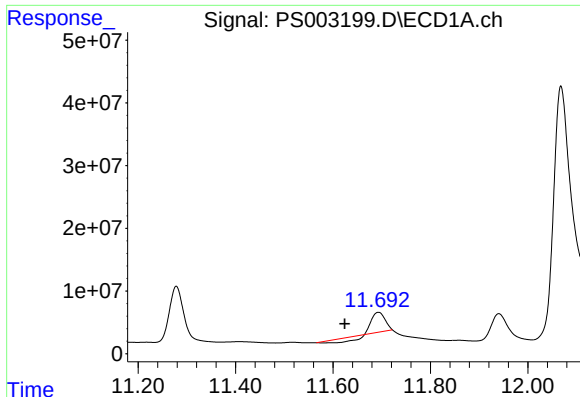

#5 DICAMBA


R.T.: 11.693 min
Delta R.T.: 0.069 min
Response: 39351070
Conc: 24.55 ng/ml

Instrument :
ECD_S
ClientSampleId :

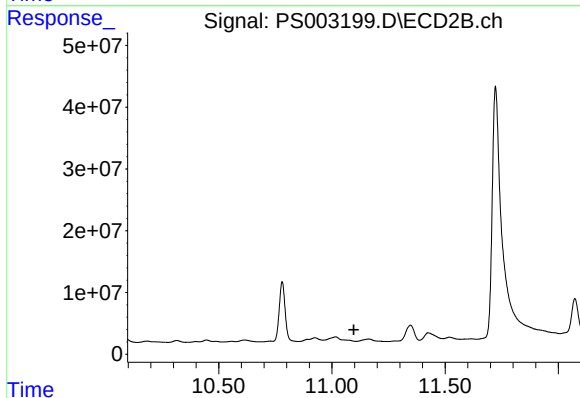


#5 DICAMBA

R.T.: 11.163 min
Delta R.T.: 0.066 min
Response: -728895
Conc: N.D.

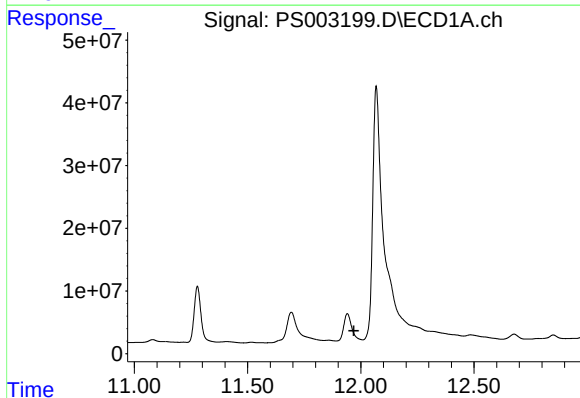


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.969 min
Response: 0
Conc: N.D.

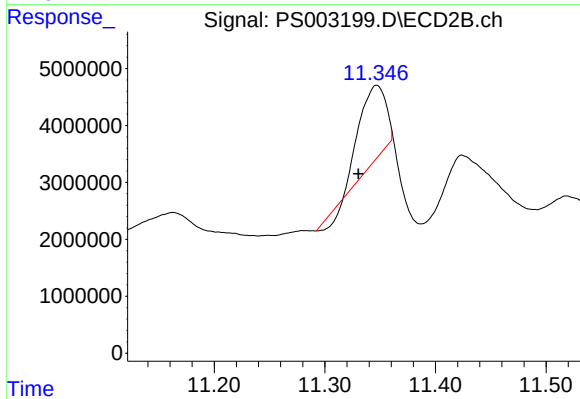

#6 MCP


R.T.: 11.347 min
Delta R.T.: 0.016 min
Response: 23386309
Conc: 21.20 ug/ml

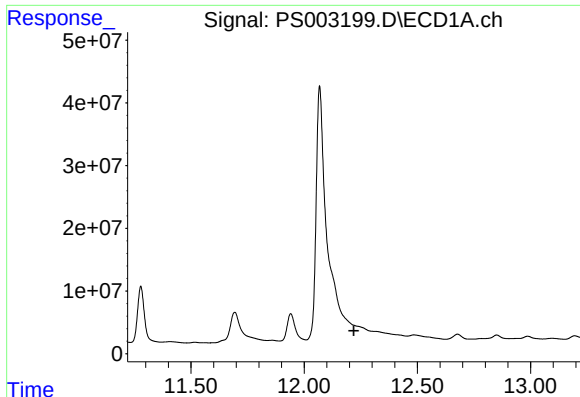

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.219 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

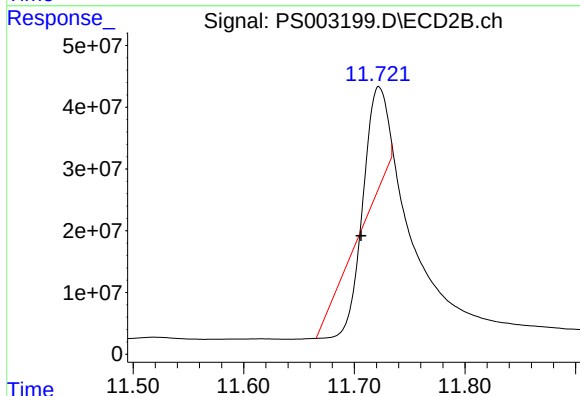


#7 MCPA

R.T.: 11.723 min
Delta R.T.: 0.016 min
Response: 109877963
Conc: 69.85 ug/ml

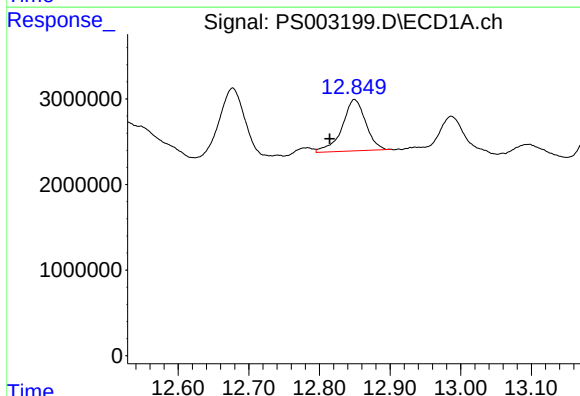


#8 DICHLORPROP

R.T.: 12.850 min
Delta R.T.: 0.035 min
Response: 13907089
Conc: 36.26 ng/ml

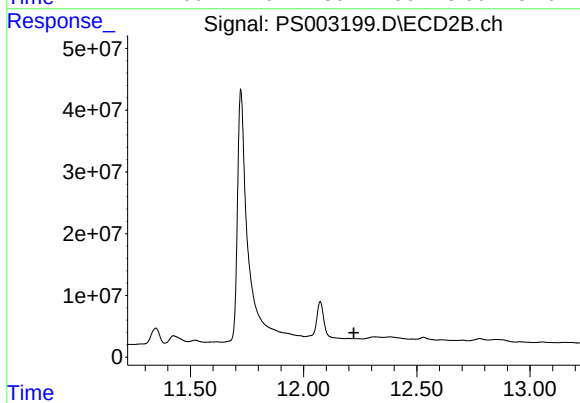

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.222 min
Response: 0
Conc: N.D.

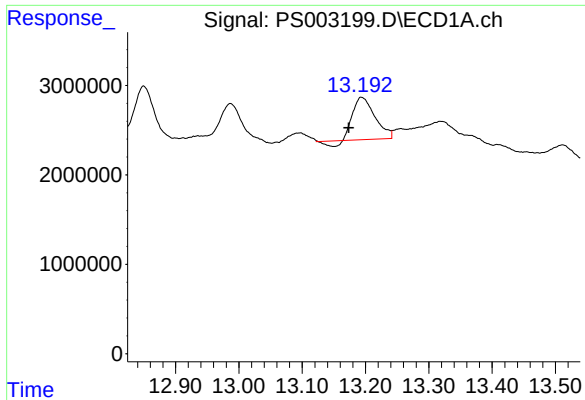

#9 2,4-D


R.T.: 13.194 min
Delta R.T.: 0.021 min
Response: 11081628
Conc: 24.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

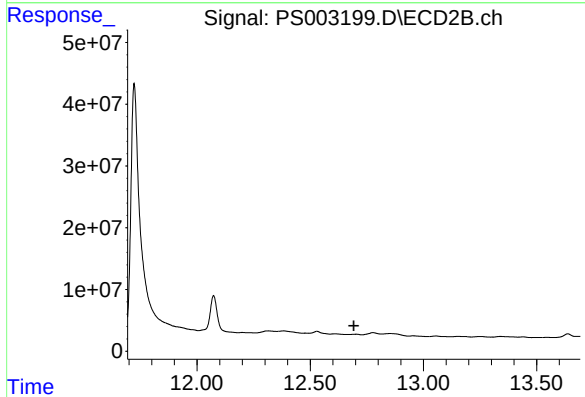


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 12.693 min
Response: 0
Conc: N.D.

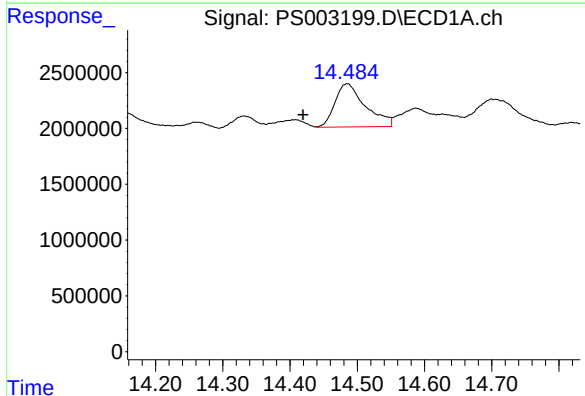


#11 2,4,5-TP (SILVEX)

R.T.: 14.485 min
Delta R.T.: 0.065 min
Response: 12187932
Conc: 4.84 ng/ml

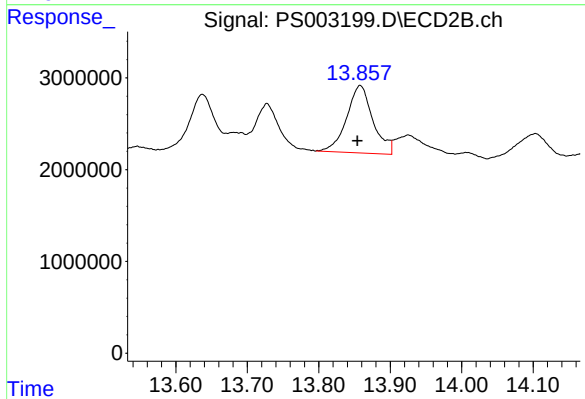

#11 2,4,5-TP (SILVEX)


R.T.: 13.858 min
Delta R.T.: 0.004 min
Response: 18812449
Conc: 7.58 ng/ml

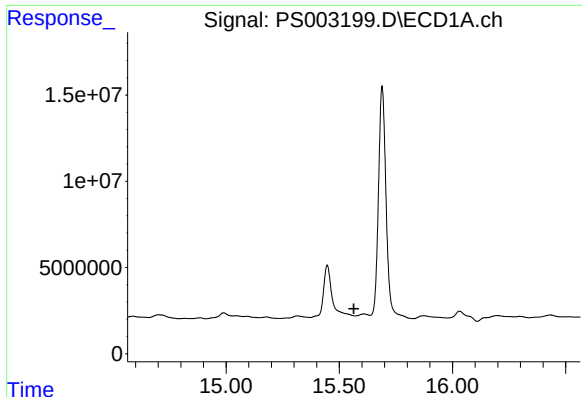

#13 2,4-DB


R.T.: 15.607 min
Delta R.T.: 0.042 min
Response: -804532
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

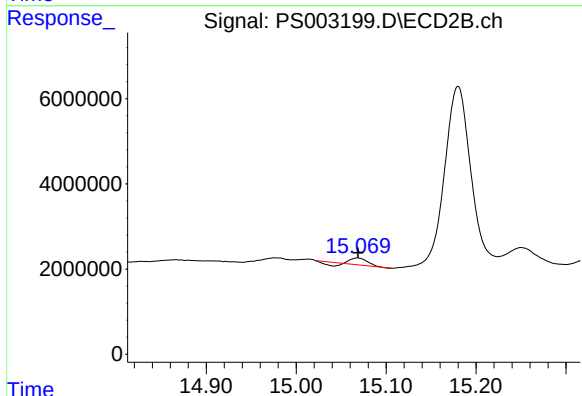


#13 2,4-DB

R.T.: 15.068 min
Delta R.T.: 0.000 min
Response: 1210557
Conc: 4.77 ng/ml

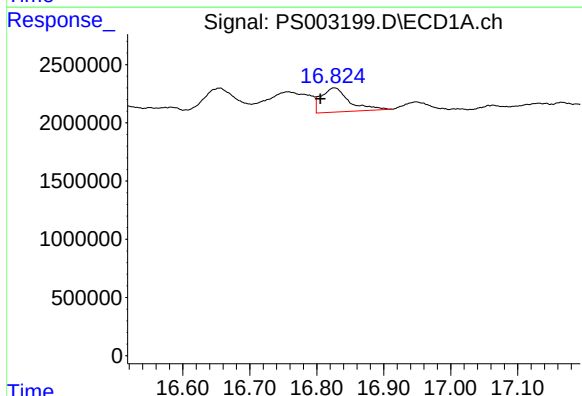


#15 Picloram

R.T.: 16.826 min
Delta R.T.: 0.021 min
Response: 5965710
Conc: 1.89 ng/ml

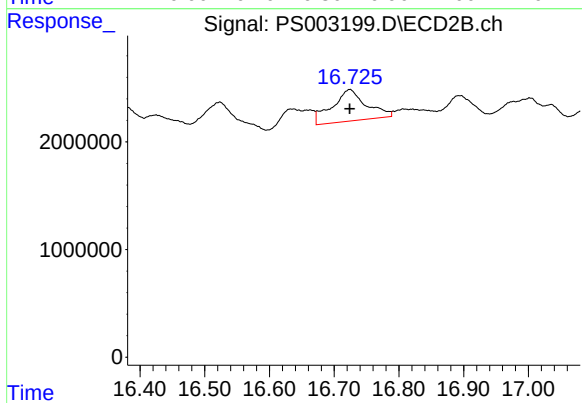

#15 Picloram


R.T.: 16.724 min
Delta R.T.: 0.000 min
Response: 10701710
Conc: 3.56 ng/ml

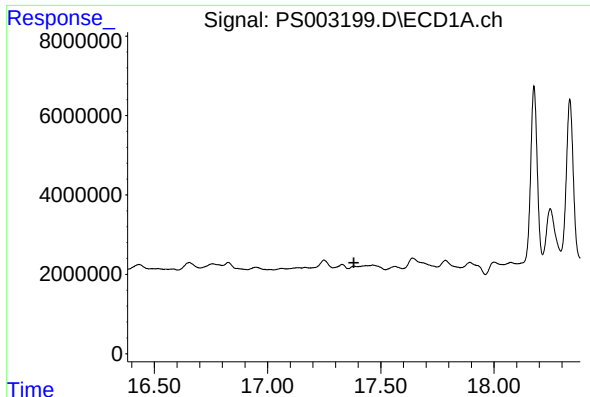

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

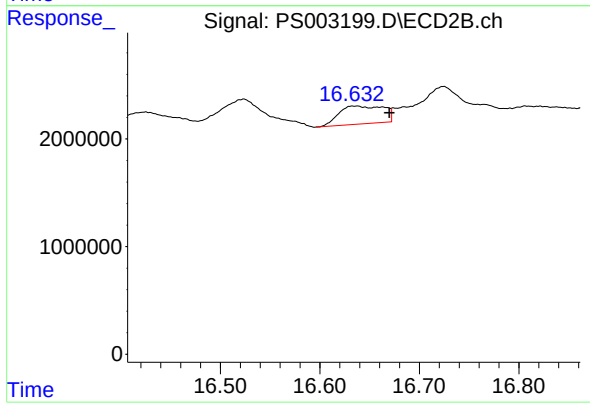

#16 DCPA

R.T.: 16.635 min
Delta R.T.: -0.035 min
Response: 5234742
Conc: 1.69 ng/ml