

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021424\
 Data File : PS025948.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Feb 2024 18:30
 Operator : AR\AJ
 Sample : P1453-01MSD
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-3MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 15 00:15:42 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS021424.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 14 15:17:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.277	7.811	2044.6E6	420.7E6	772.553	482.036 #
Target Compounds							
1) T	Dalapon	2.680	2.728	1803.1E6	667.8E6	403.063	409.531
2) T	3,5-DICHL...	6.443	6.758	1745.7E6	572.4E6	449.661	428.222
3) T	4-Nitroph...	7.073	7.338	58164310	12607121	36.685	26.148 #
5) T	DICAMBA	7.466	8.012	4492.9E6	1572.0E6	407.763	406.847
6) T	MCP	7.648	8.111	316.3E6	115.6E6	40.028	42.872
7) T	MCPA	7.798	8.356	465.4E6	166.6E6	40.916	43.240
8) T	DICHLORPROP	8.180	8.728	1231.6E6	401.2E6	436.544	416.509
9) T	2,4-D	8.412	9.060	1431.9E6	455.9E6	484.270	481.046
10) T	Pentachlo...	8.713	9.592	18005.9E6	6317.6E6	454.359	439.562
11) T	2,4,5-TP ...	9.299	9.967	7254.5E6	2474.7E6	465.429	454.825
12) T	2,4,5-T	9.592	10.389	6535.8E6	2113.5E6	429.761	423.297
13) T	2,4-DB	10.173	10.956	899.9E6	261.4E6	459.220	472.288
14) T	DINOSEB	11.393	11.335	4863.6E6	1549.6E6	438.781	431.838
15) T	Picloram	11.196	12.437	7081.5E6	2013.3E6	395.769	375.988
16) T	DCPA	11.684	12.382	7941.1E6	2734.3E6	403.904	424.585



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021424\
Data File : PS025948.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Feb 2024 18:30
Operator : AR\AJ
Sample : P1453-01MSD
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-3MSD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 15 00:15:42 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS021424.M
Quant Title : 8080.M
QLast Update : Wed Feb 14 15:17:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

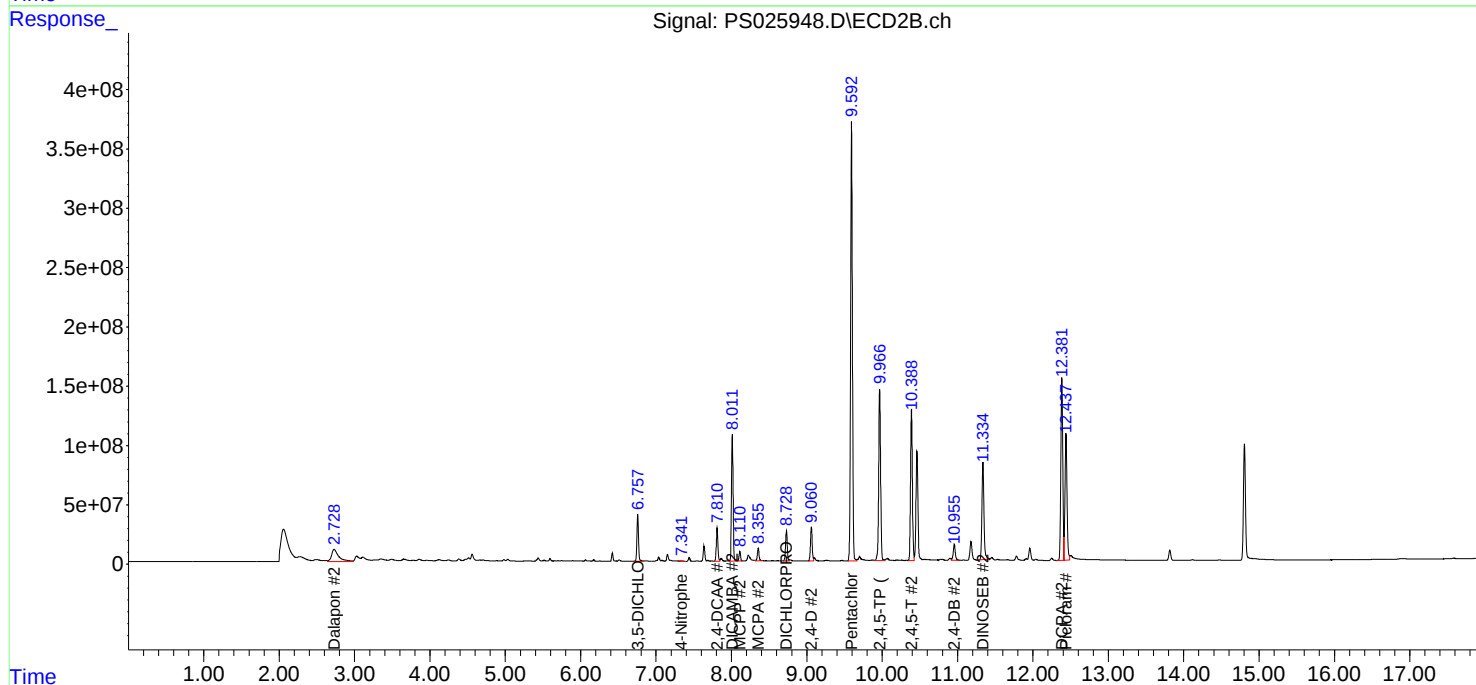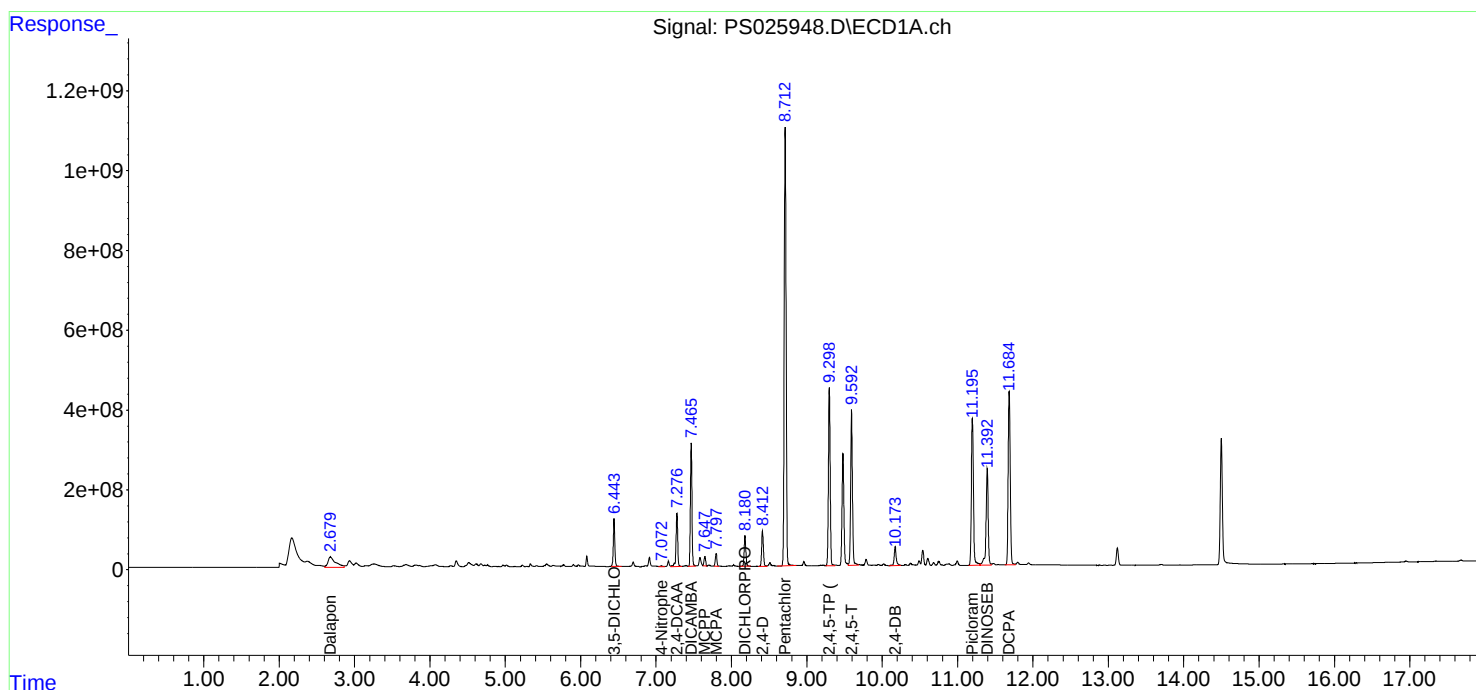


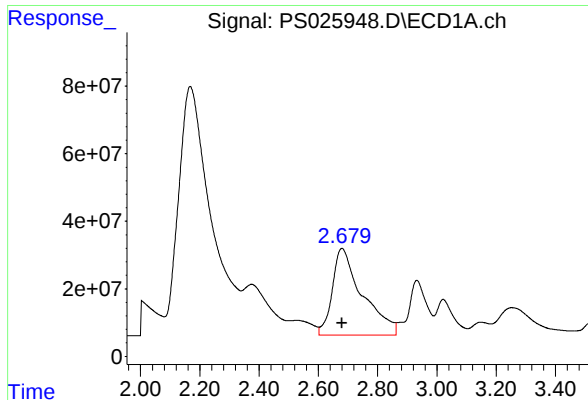

#1 Dalapon


R.T.: 2.680 min
Delta R.T.: 0.000 min
Response: 1803106714
Conc: 403.06 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3MSD

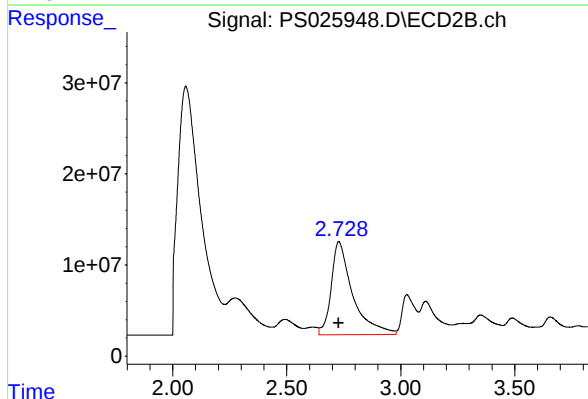


#1 Dalapon

R.T.: 2.728 min
Delta R.T.: 0.000 min
Response: 667784596
Conc: 409.53 ng/ml

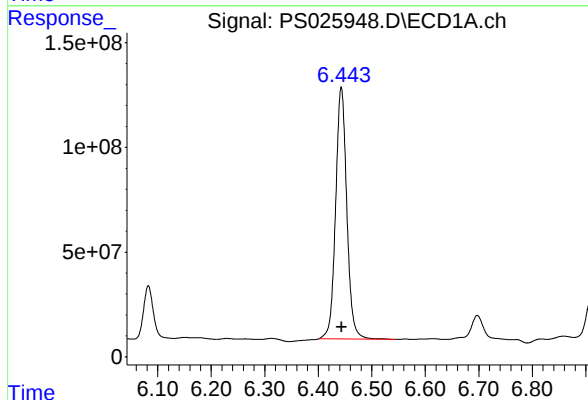


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.443 min
Delta R.T.: 0.000 min
Response: 1745660749
Conc: 449.66 ng/ml

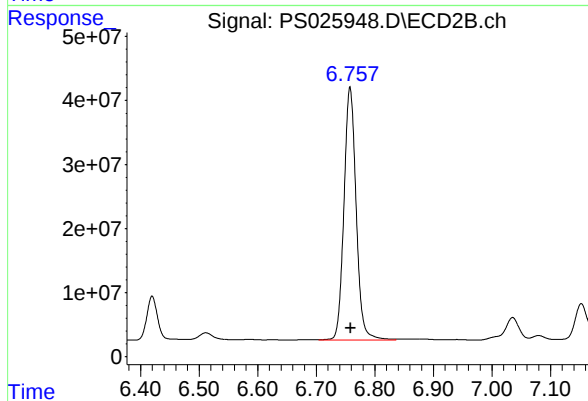

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.758 min
Delta R.T.: -0.001 min
Response: 572361991
Conc: 428.22 ng/ml

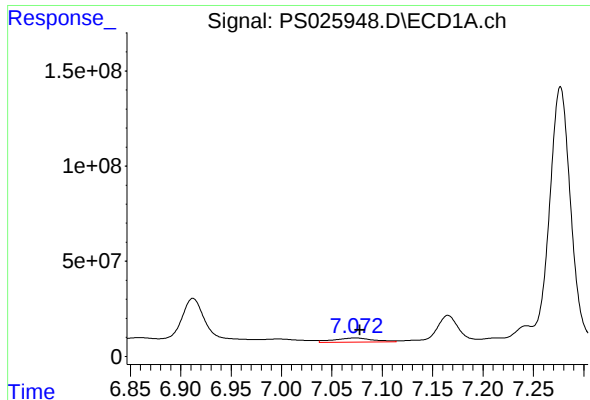

#3 4-Nitrophenol


R.T.: 7.073 min
Delta R.T.: -0.005 min
Response: 58164310
Conc: 36.68 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3MSD

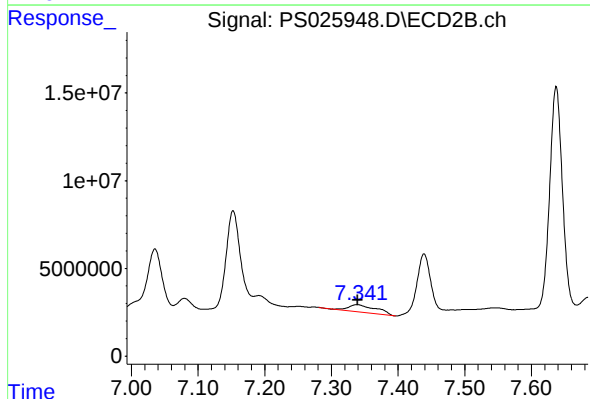


#3 4-Nitrophenol

R.T.: 7.338 min
Delta R.T.: -0.001 min
Response: 12607121
Conc: 26.15 ng/ml

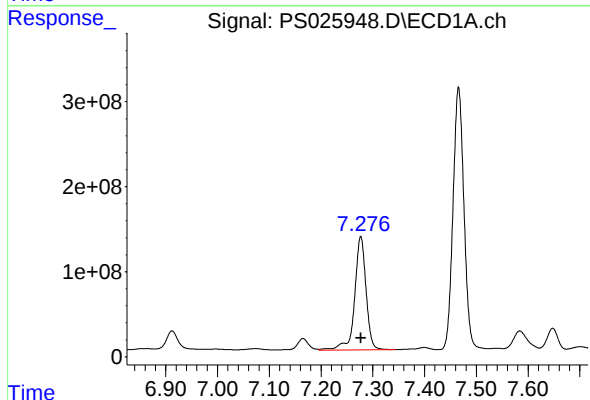


#4 2,4-DCAA

R.T.: 7.277 min
Delta R.T.: 0.000 min
Response: 2044618172
Conc: 772.55 ng/ml

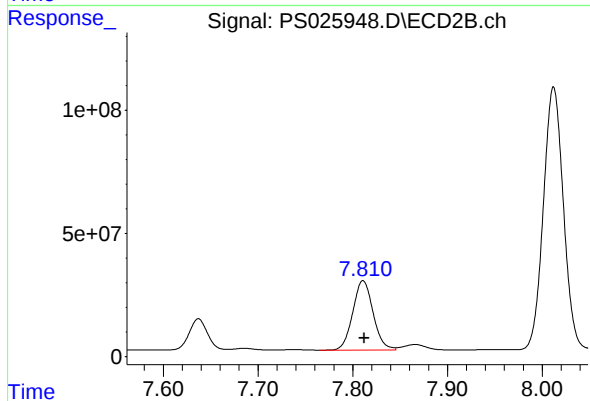

#4 2,4-DCAA


R.T.: 7.811 min
Delta R.T.: -0.001 min
Response: 420746058
Conc: 482.04 ng/ml

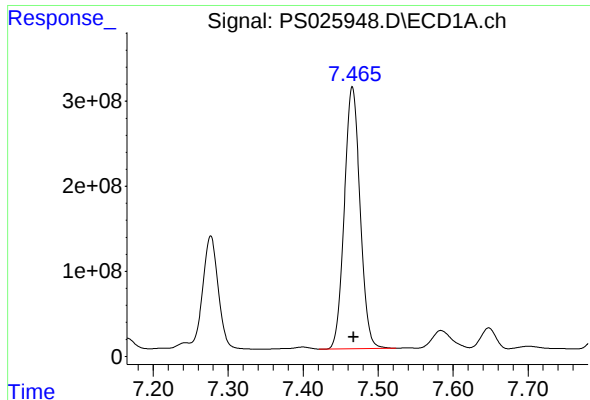

#5 DICAMBA


R.T.: 7.466 min
Delta R.T.: -0.002 min
Response: 4492907511
Conc: 407.76 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3MSD

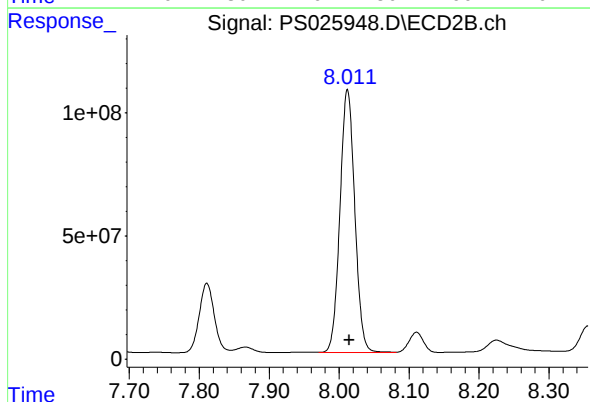


#5 DICAMBA

R.T.: 8.012 min
Delta R.T.: -0.002 min
Response: 1572026041
Conc: 406.85 ng/ml

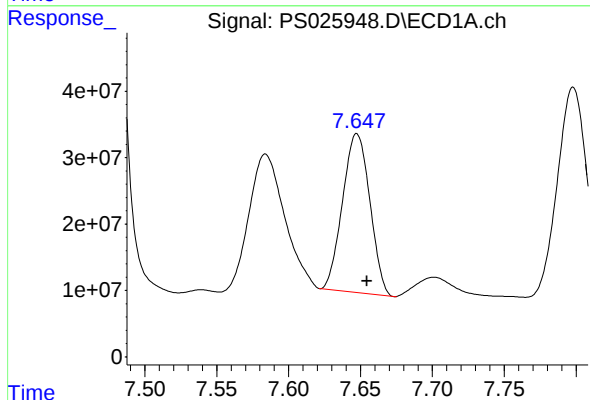


#6 MCPP

R.T.: 7.648 min
Delta R.T.: -0.007 min
Response: 316321015
Conc: 40.03 ug/ml

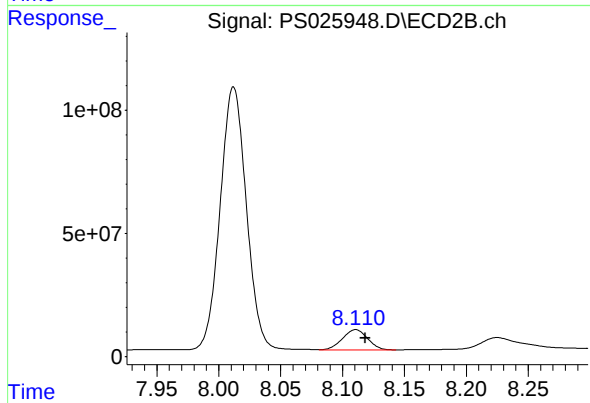

#6 MCPP


R.T.: 8.111 min
Delta R.T.: -0.007 min
Response: 115636080
Conc: 42.87 ug/ml

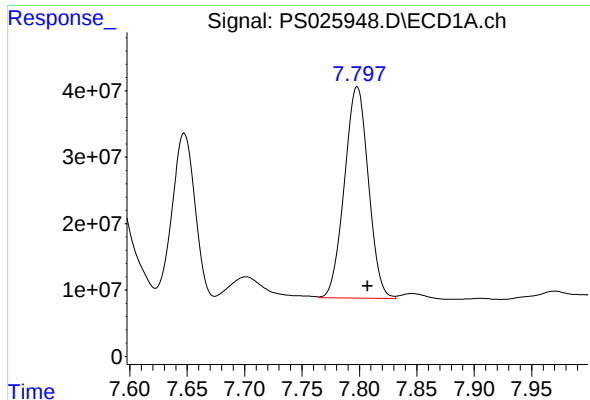

#7 MCPA


R.T.: 7.798 min
Delta R.T.: -0.009 min
Response: 465391400
Conc: 40.92 ug/ml

Instrument :
ECD_S
ClientSampleId :
TP-3MSD

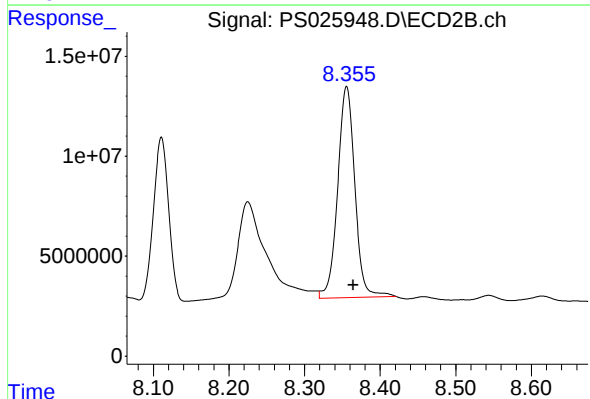


#7 MCPA

R.T.: 8.356 min
Delta R.T.: -0.009 min
Response: 166571914
Conc: 43.24 ug/ml

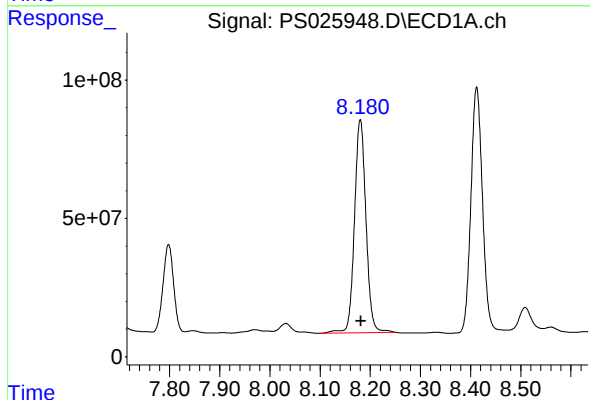


#8 DICHLORPROP

R.T.: 8.180 min
Delta R.T.: -0.002 min
Response: 1231563019
Conc: 436.54 ng/ml

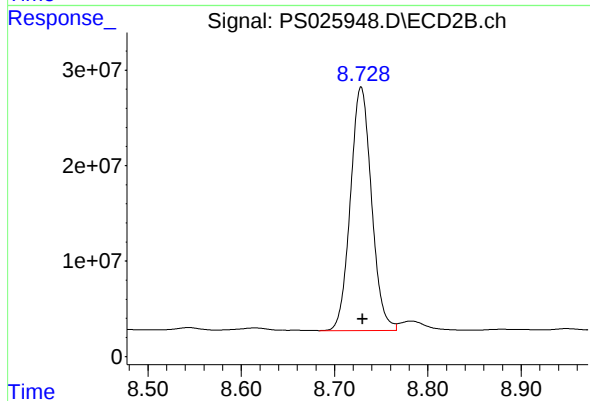

#8 DICHLORPROP


R.T.: 8.728 min
Delta R.T.: -0.002 min
Response: 401211161
Conc: 416.51 ng/ml

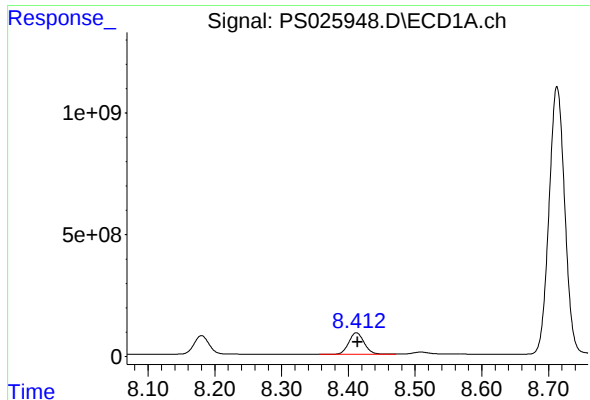

#9 2,4-D


R.T.: 8.412 min
Delta R.T.: -0.002 min
Response: 1431875499
Conc: 484.27 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3MSD

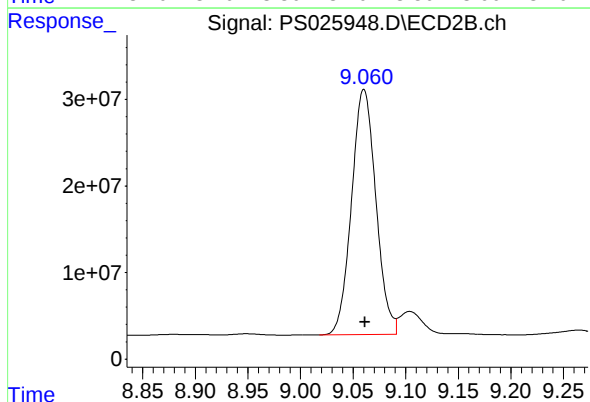


#9 2,4-D

R.T.: 9.060 min
Delta R.T.: -0.001 min
Response: 455936093
Conc: 481.05 ng/ml

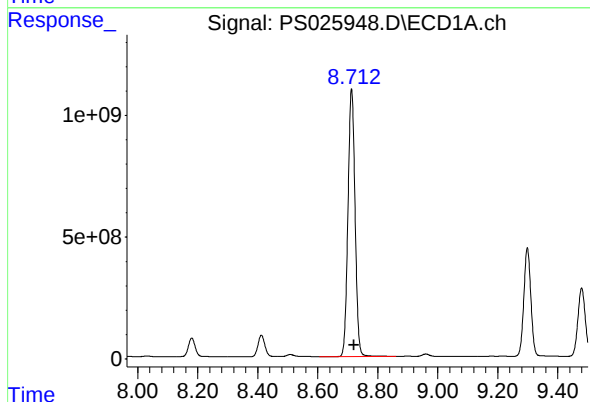


#10 Pentachlorophenol

R.T.: 8.713 min
Delta R.T.: -0.008 min
Response: 18005889590
Conc: 454.36 ng/ml

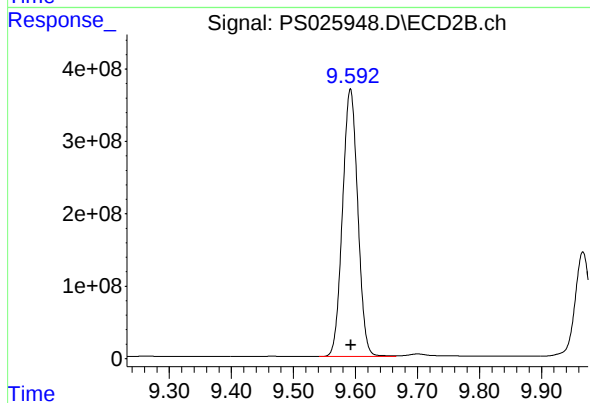

#10 Pentachlorophenol


R.T.: 9.592 min
Delta R.T.: 0.000 min
Response: 6317559433
Conc: 439.56 ng/ml

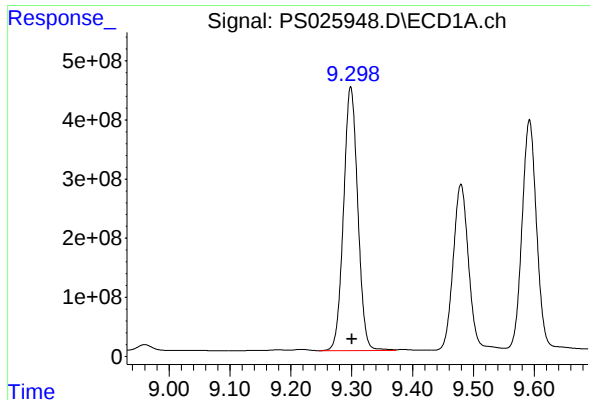

#11 2,4,5-TP (SILVEX)


R.T.: 9.299 min
Delta R.T.: -0.002 min
Response: 7254543382
Conc: 465.43 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3MSD

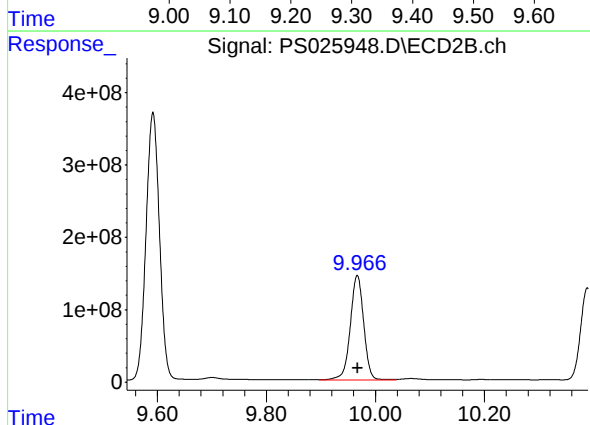


#11 2,4,5-TP (SILVEX)

R.T.: 9.967 min
Delta R.T.: 0.000 min
Response: 2474747053
Conc: 454.82 ng/ml

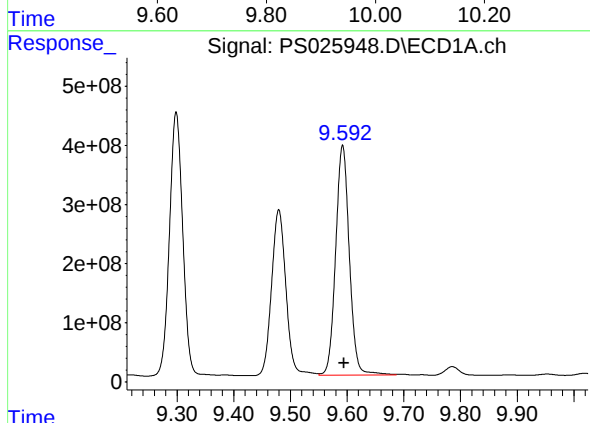


#12 2,4,5-T

R.T.: 9.592 min
Delta R.T.: -0.002 min
Response: 6535849403
Conc: 429.76 ng/ml

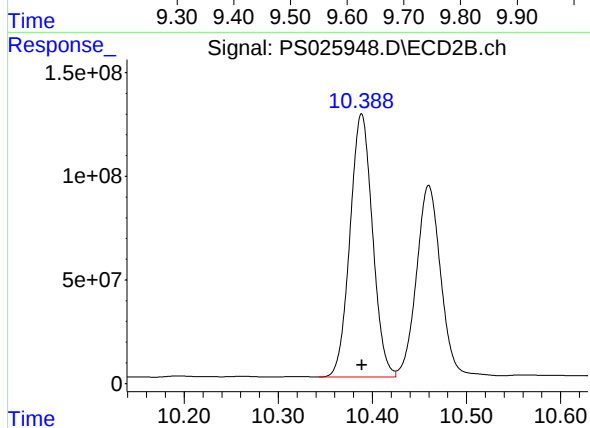

#12 2,4,5-T


R.T.: 10.389 min
Delta R.T.: 0.000 min
Response: 2113474207
Conc: 423.30 ng/ml

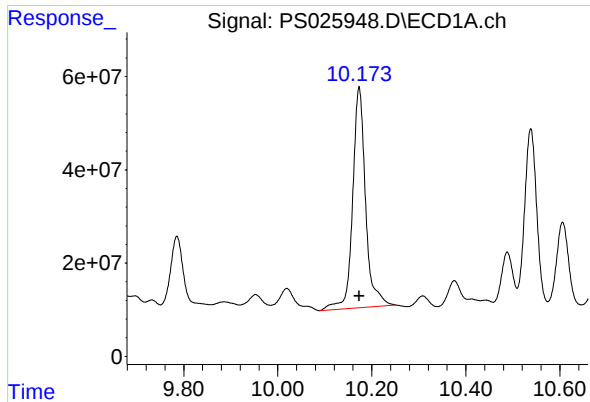

#13 2,4-DB


R.T.: 10.173 min
Delta R.T.: 0.000 min
Response: 899916600
Conc: 459.22 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3MSD

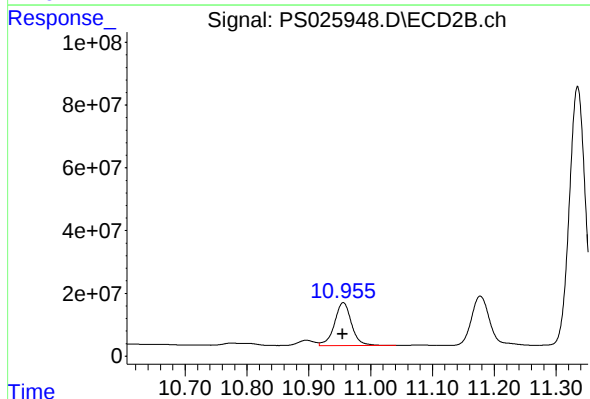


#13 2,4-DB

R.T.: 10.956 min
Delta R.T.: 0.000 min
Response: 261359847
Conc: 472.29 ng/ml

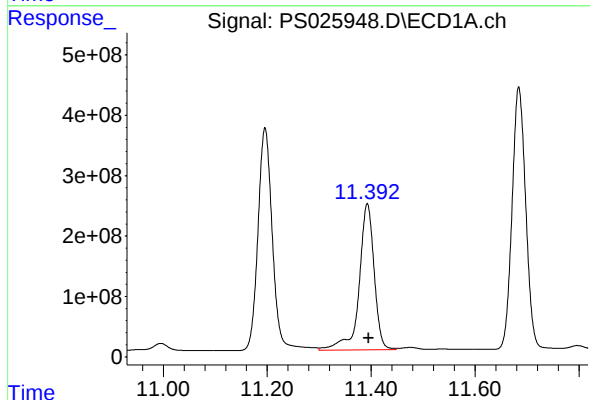


#14 DINOSEB

R.T.: 11.393 min
Delta R.T.: -0.002 min
Response: 4863555856
Conc: 438.78 ng/ml

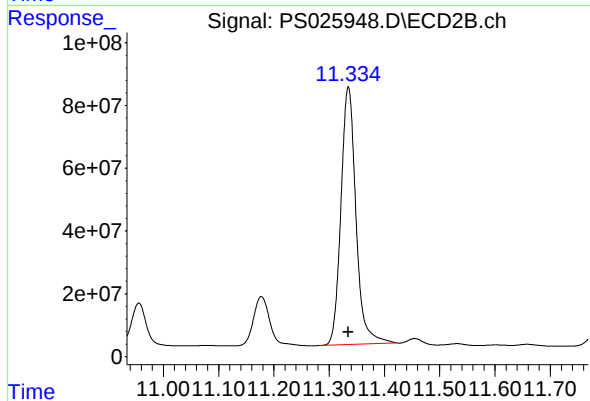

#14 DINOSEB


R.T.: 11.335 min
Delta R.T.: 0.000 min
Response: 1549561004
Conc: 431.84 ng/ml

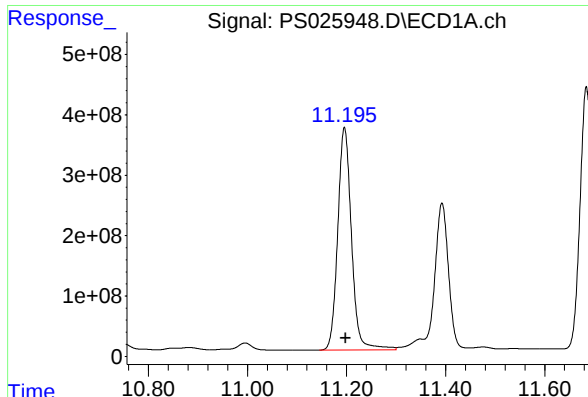

#15 Picloram


R.T.: 11.196 min
Delta R.T.: -0.002 min
Response: 7081467766
Conc: 395.77 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3MSD

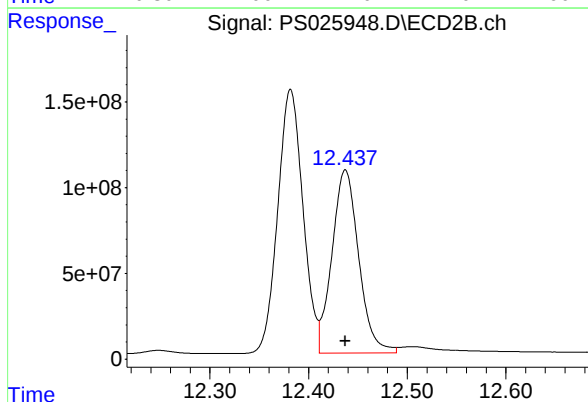


#15 Picloram

R.T.: 12.437 min
Delta R.T.: 0.000 min
Response: 2013286623
Conc: 375.99 ng/ml

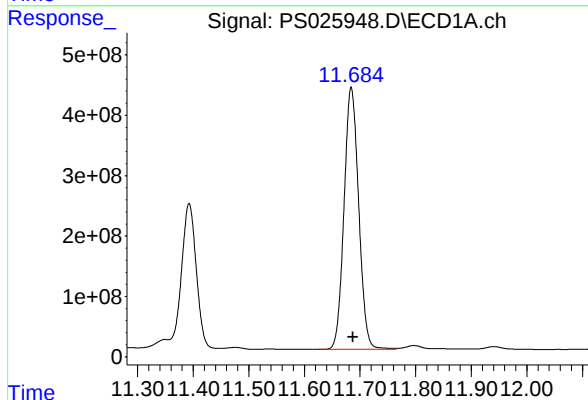

#16 DCPA

R.T.: 11.684 min
Delta R.T.: -0.003 min
Response: 7941137512
Conc: 403.90 ng/ml

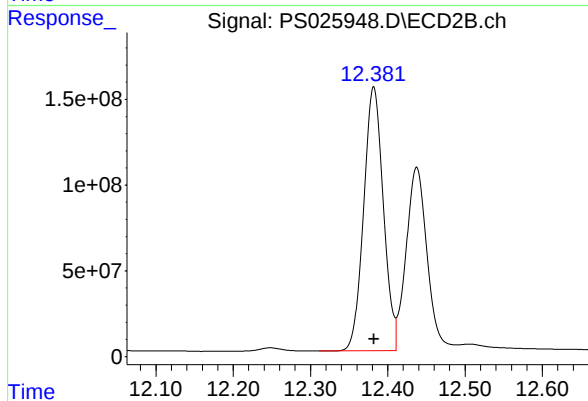

#16 DCPA

R.T.: 12.382 min
Delta R.T.: 0.000 min
Response: 2734325196
Conc: 424.59 ng/ml