

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021424\
 Data File : PS025961.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Feb 2024 00:08
 Operator : AR\AJ
 Sample : PB158779TB
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB158779TB

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/15/2024
 Supervised By :mohammad ahmed 02/15/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 15 00:48:57 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS021424.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 14 15:17:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.277	7.806	1462.0E6	393.1E6	552.408	450.334m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021424\
Data File : PS025961.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Feb 2024 00:08
Operator : AR\AJ
Sample : PB158779TB
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
PB158779TB


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/15/2024
Supervised By :mohammad ahmed 02/15/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 15 00:48:57 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS021424.M
Quant Title : 8080.M
QLast Update : Wed Feb 14 15:17:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

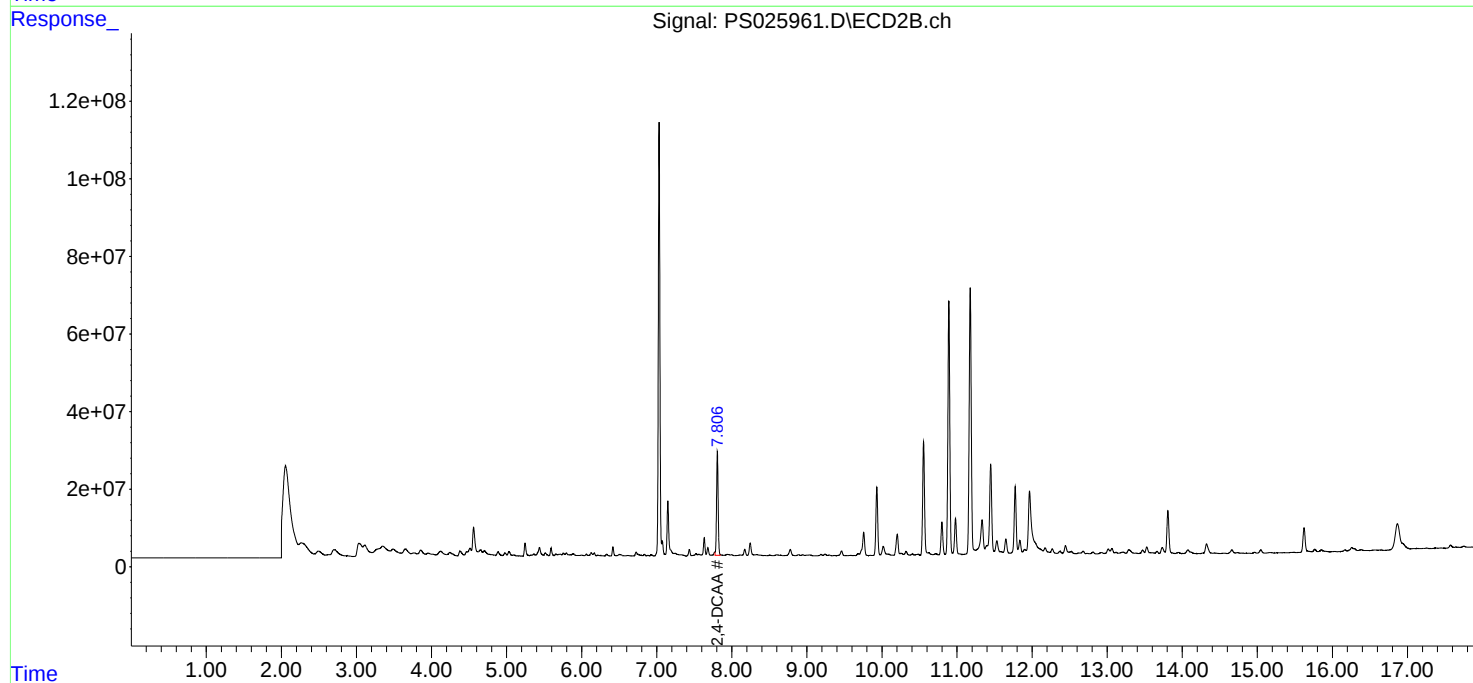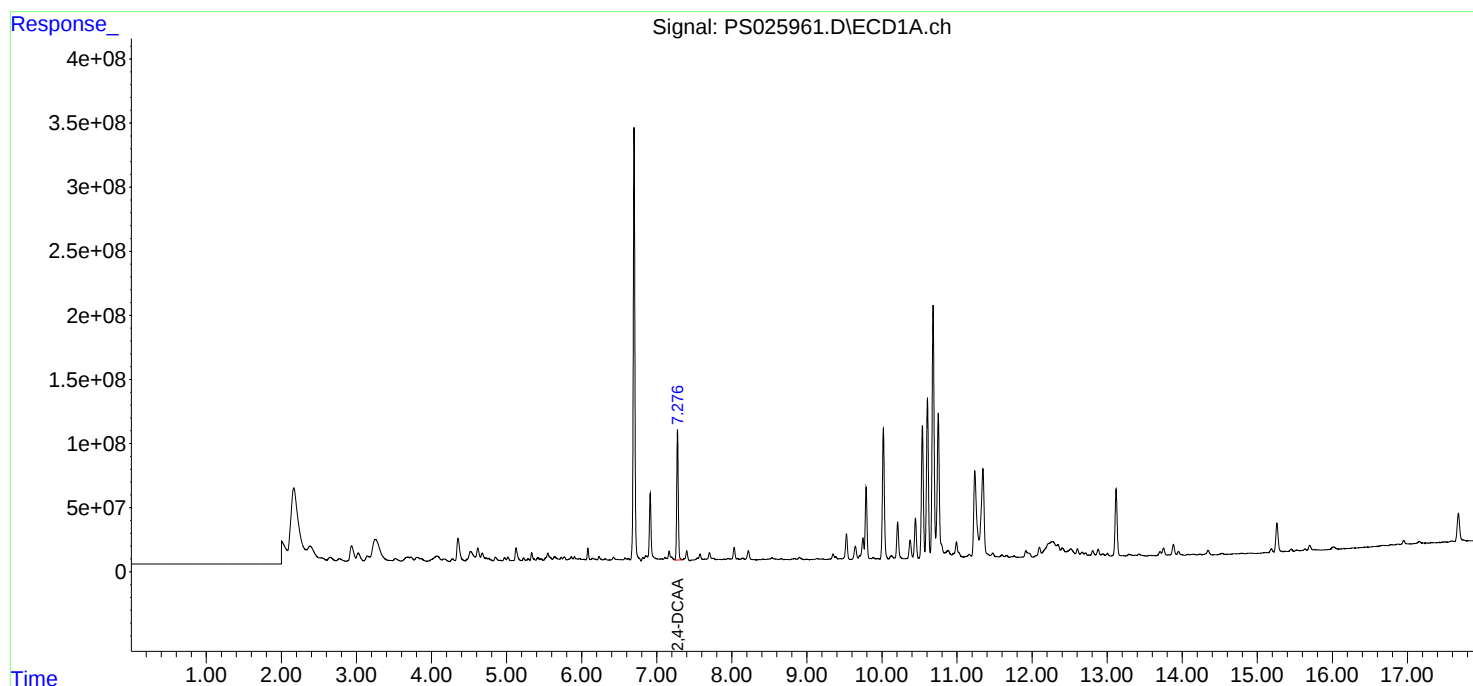

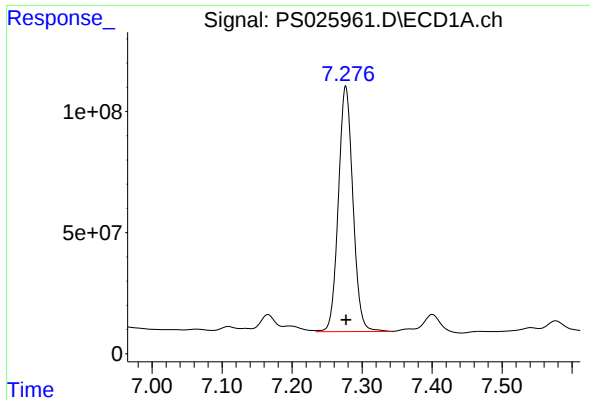


#4 2,4-DCAA

R.T.: 7.277 min
Delta R.T.: 0.000 min
Response: 1461987791
Conc: 552.41 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB158779TB

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/15/2024
Supervised By :mohammad ahmed 02/15/2024

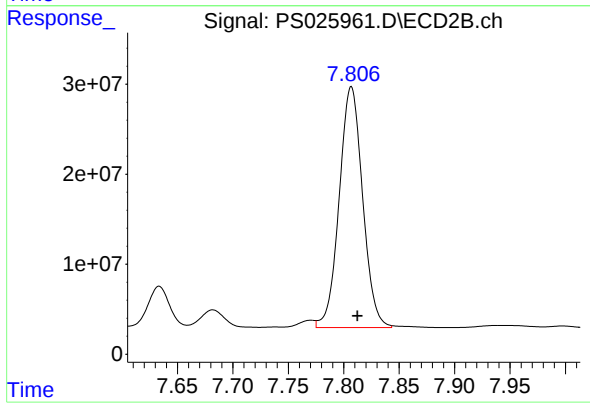

#4 2,4-DCAA

R.T.: 7.806 min
Delta R.T.: -0.006 min
Response: 393074632
Conc: 450.33 ng/ml m