

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021519\
 Data File : PS003204.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Feb 2019 13:39
 Operator : EI\SJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 15 22:02:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.776	0	322.4E6	N.D.	754.084 #
Target Compounds							
1) T	Dalapon	2.838	2.310	42298364	388.5E6	76.676	724.994 #
3) T	4-Nitroph...	0.000	9.926	0	159.4E6	N.D.	762.406 #
8) T	DICHLORPROP	0.000	12.181	0	284.4E6	N.D.	743.941 #
9) T	2,4-D	0.000	12.653	0	200.9E6	N.D.	400.782 #
11) T	2,4,5-TP ...	14.376	13.814	1930.8E6	1771.4E6	766.667	714.182
12) T	2,4,5-T	14.776	14.377	1877.1E6	544.0E6	769.505	284.306 #
14) T	DINOSEB	16.990	0.000	1450.3E6	0	770.914	N.D. #
15) T	Picloram	16.766	16.685	2224.7E6	2086.6E6	703.204	694.055
16) T	DCPA	0.000	16.685	0	2086.6E6	N.D.	673.624 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021519\
Data File : PS003204.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Feb 2019 13:39
Operator : EI\SJ
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 15 22:02:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

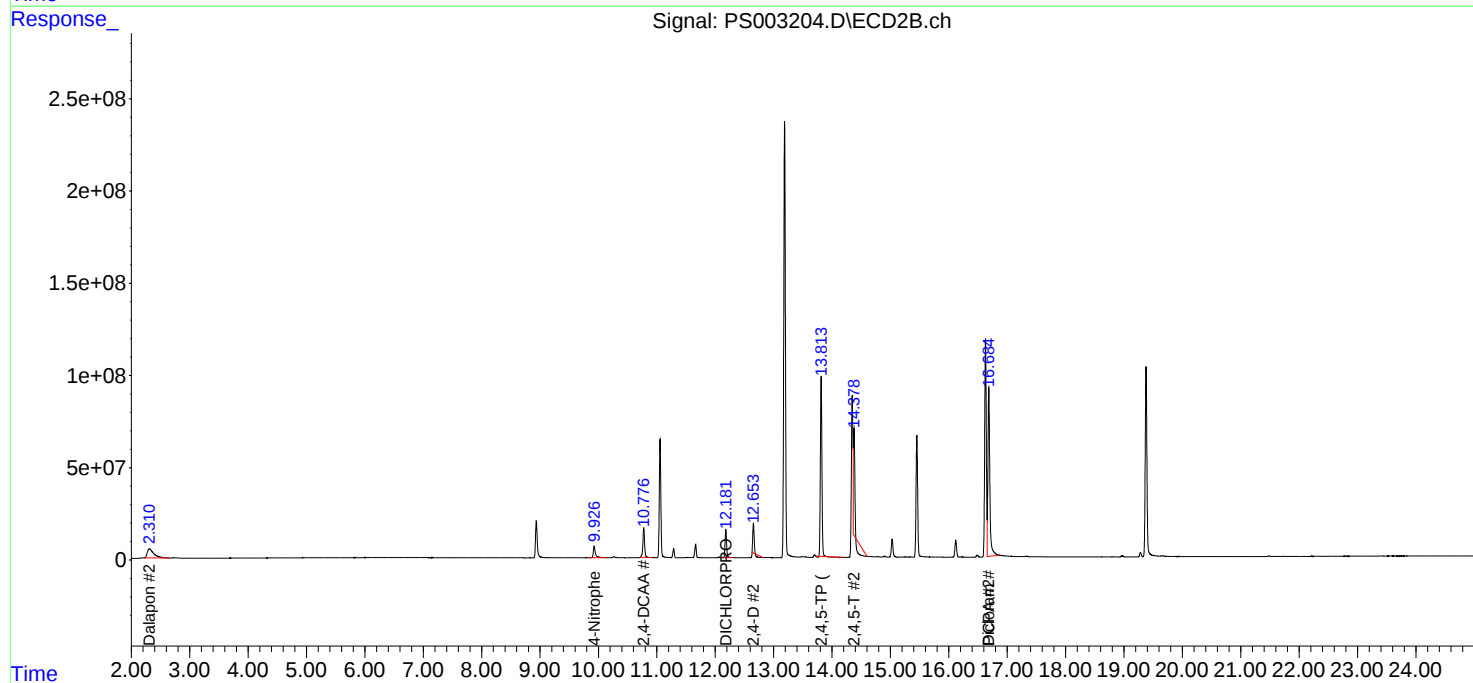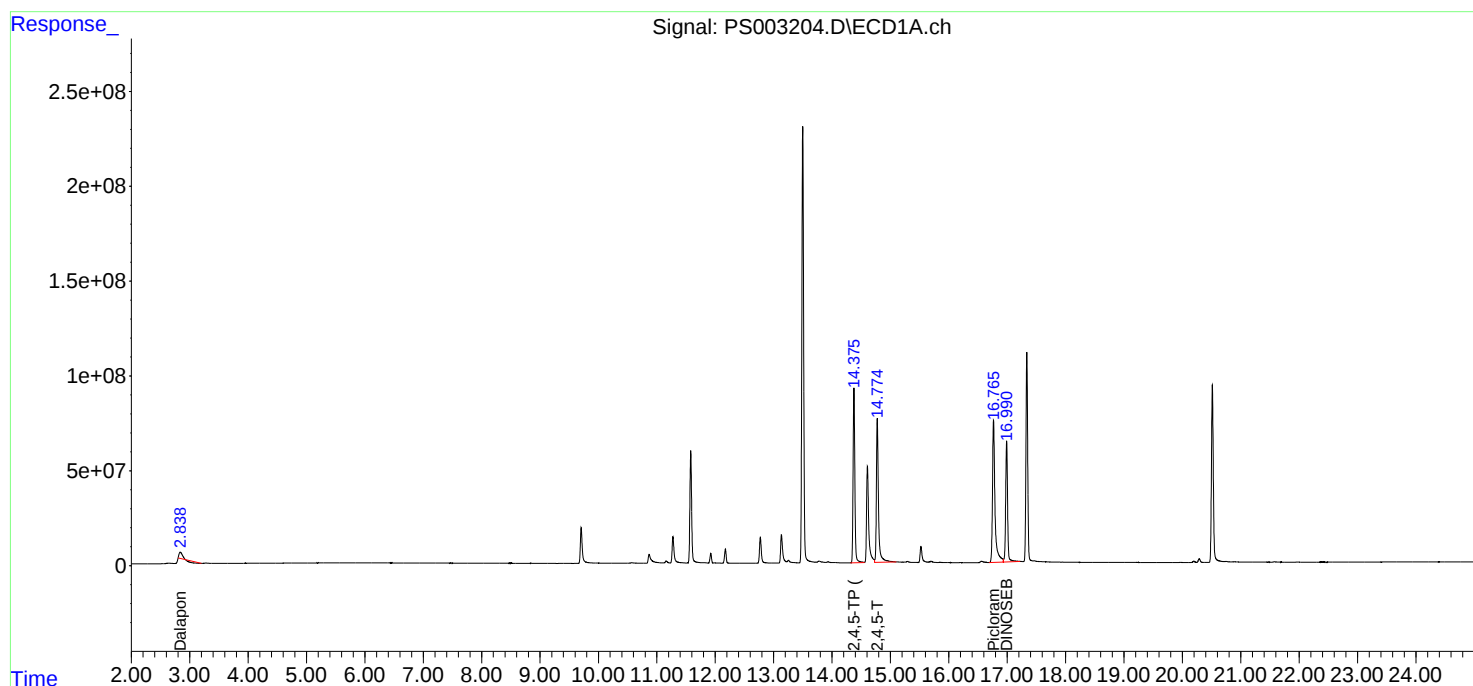


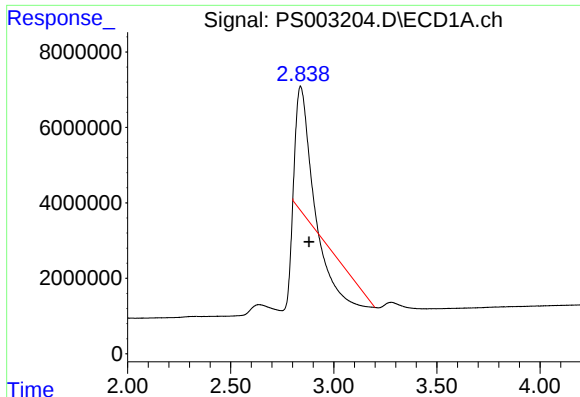

#1 Dalapon


R.T.: 2.838 min
Delta R.T.: -0.042 min
Response: 42298364
Conc: 76.68 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

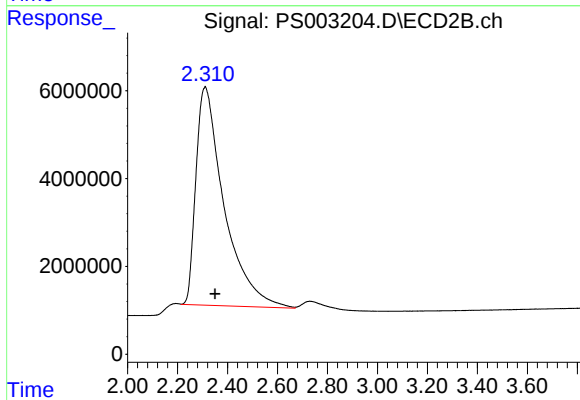


#1 Dalapon

R.T.: 2.310 min
Delta R.T.: -0.040 min
Response: 388539709
Conc: 724.99 ng/ml

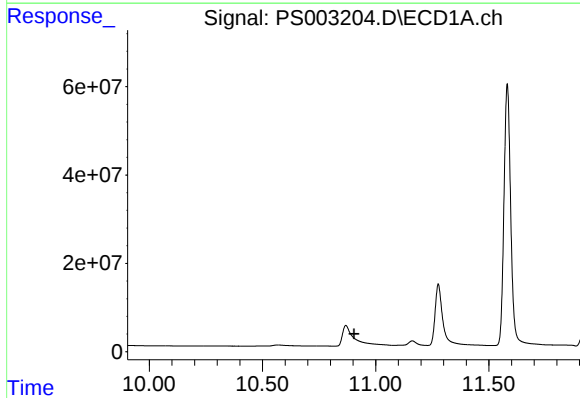


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 10.904 min
Response: 0
Conc: N.D.

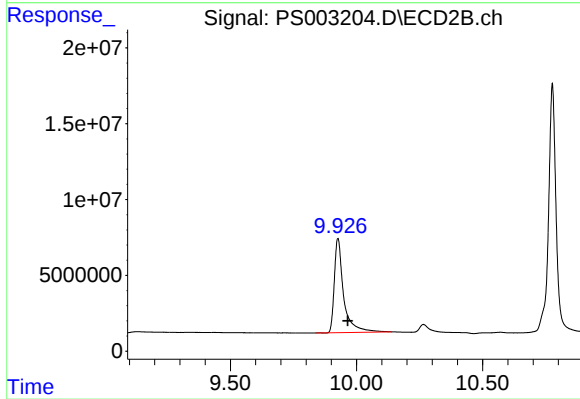

#3 4-Nitrophenol


R.T.: 9.926 min
Delta R.T.: -0.039 min
Response: 159359957
Conc: 762.41 ng/ml

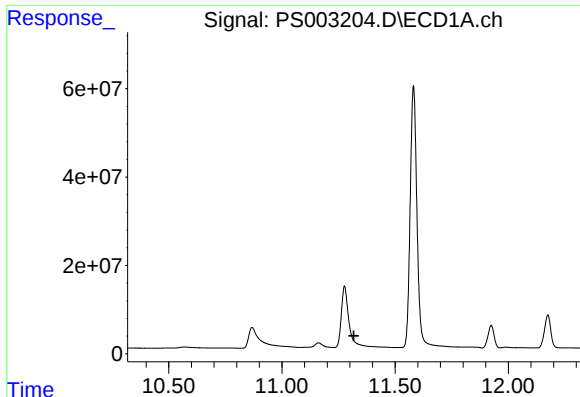

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 11.318 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

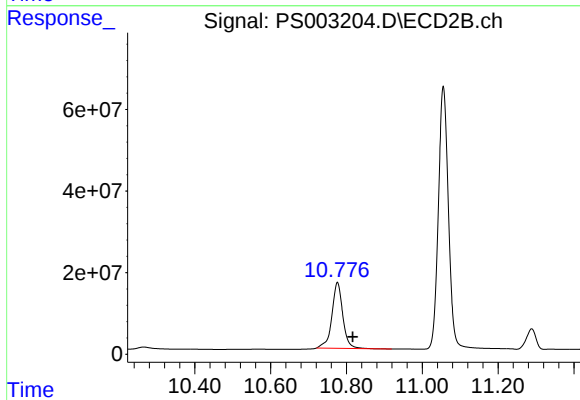


#4 2,4-DCAA

R.T.: 10.776 min
Delta R.T.: -0.040 min
Response: 322405320
Conc: 754.08 ng/ml

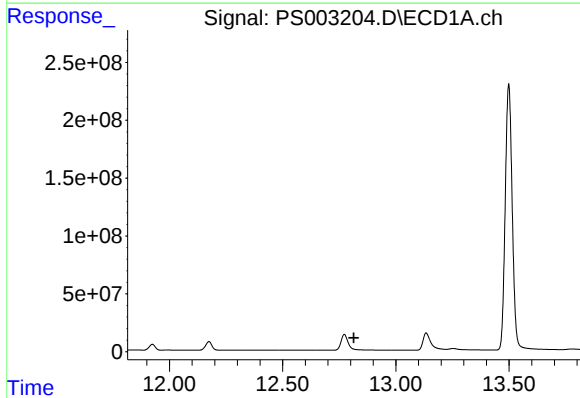


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 12.815 min
Response: 0
Conc: N.D.

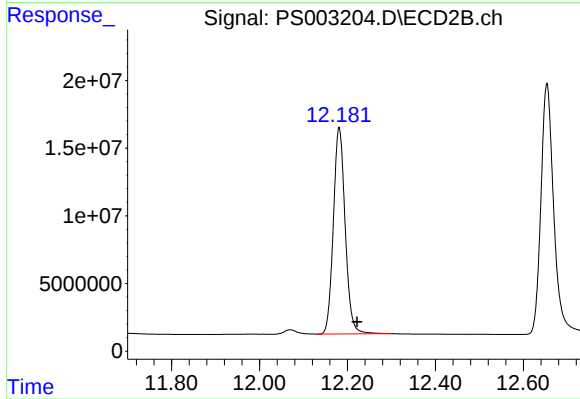

#8 DICHLORPROP


R.T.: 12.181 min
Delta R.T.: -0.041 min
Response: 284439236
Conc: 743.94 ng/ml

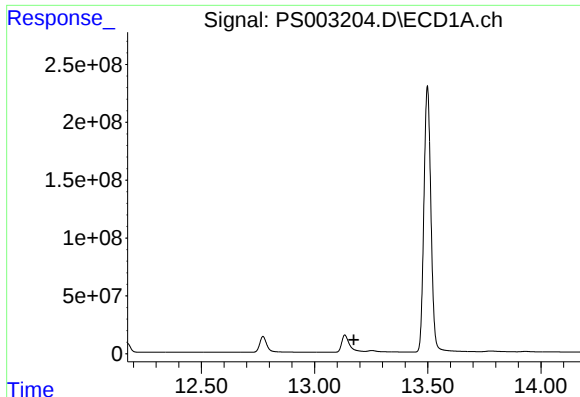

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.173 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

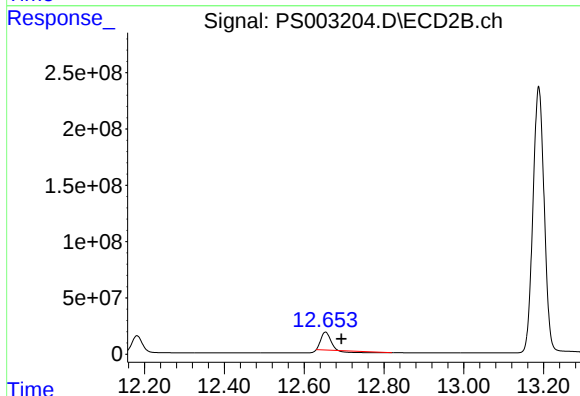


#9 2,4-D

R.T.: 12.653 min
Delta R.T.: -0.039 min
Response: 200946521
Conc: 400.78 ng/ml

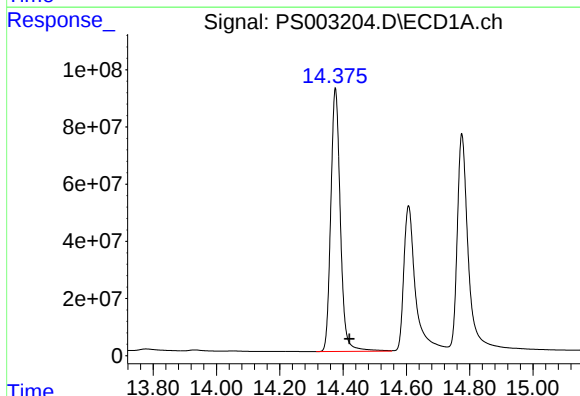


#11 2,4,5-TP (SILVEX)

R.T.: 14.376 min
Delta R.T.: -0.044 min
Response: 1930753520
Conc: 766.67 ng/ml

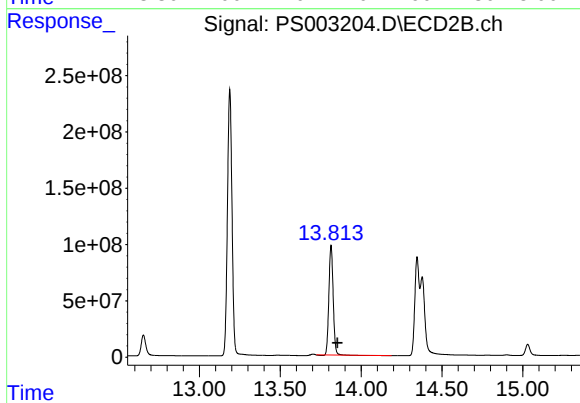

#11 2,4,5-TP (SILVEX)


R.T.: 13.814 min
Delta R.T.: -0.040 min
Response: 1771426360
Conc: 714.18 ng/ml

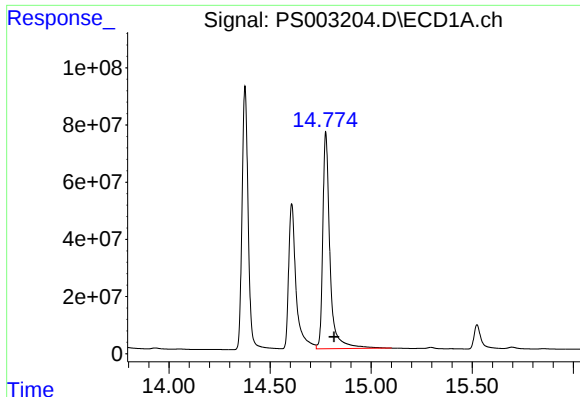

#12 2,4,5-T


R.T.: 14.776 min
Delta R.T.: -0.041 min
Response: 1877135432
Conc: 769.51 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

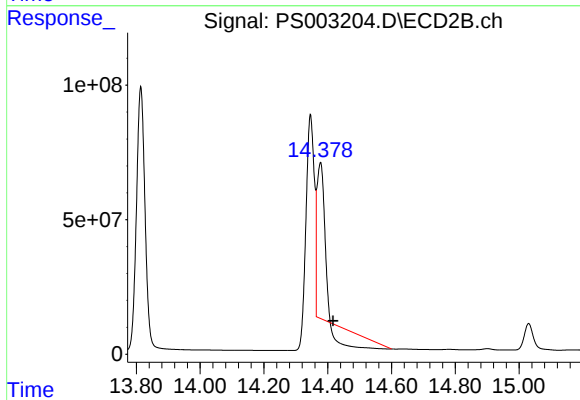


#12 2,4,5-T

R.T.: 14.377 min
Delta R.T.: -0.040 min
Response: 544015705
Conc: 284.31 ng/ml

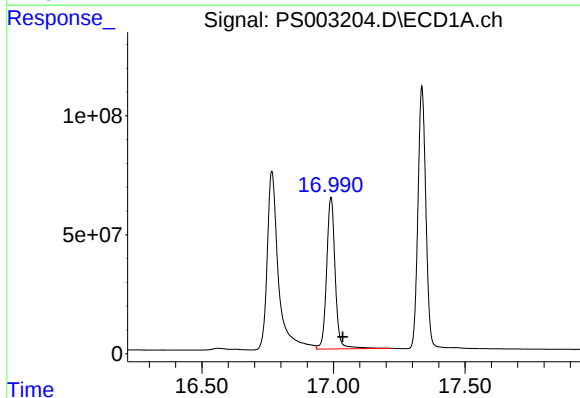


#14 DINOSEB

R.T.: 16.990 min
Delta R.T.: -0.045 min
Response: 1450341248
Conc: 770.91 ng/ml

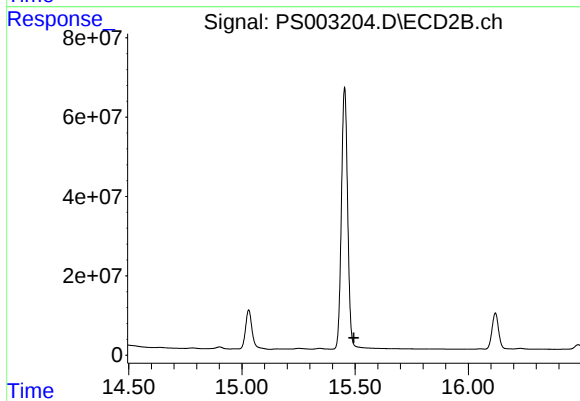

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 15.495 min
Response: 0
Conc: N.D.

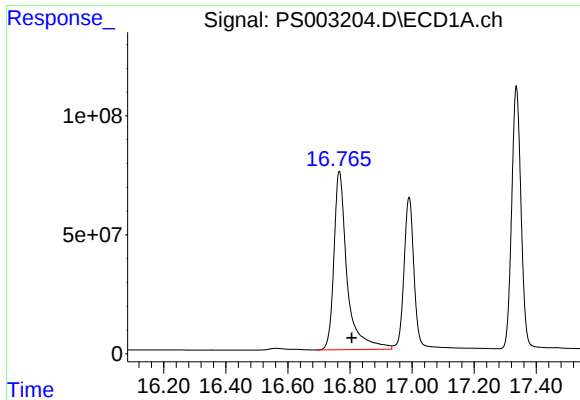

#15 Picloram


R.T.: 16.766 min
Delta R.T.: -0.040 min
Response: 2224680399
Conc: 703.20 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

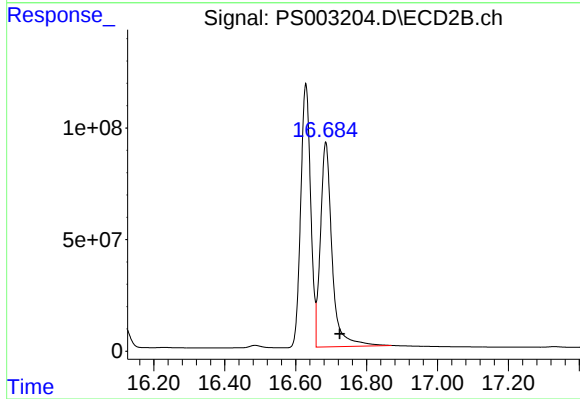


#15 Picloram

R.T.: 16.685 min
Delta R.T.: -0.039 min
Response: 2086609360
Conc: 694.05 ng/ml

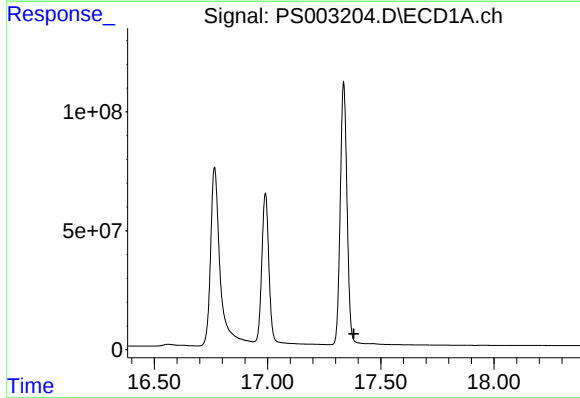

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

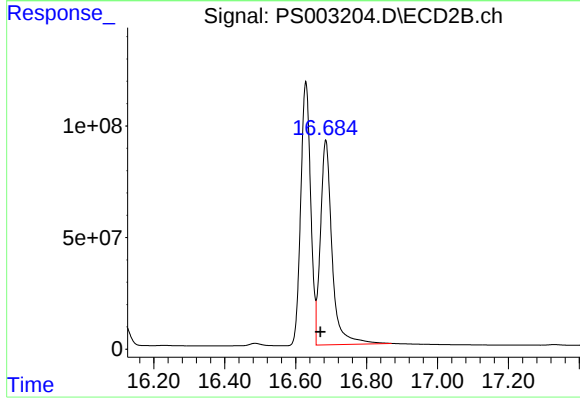

#16 DCPA

R.T.: 16.685 min
Delta R.T.: 0.015 min
Response: 2086609360
Conc: 673.62 ng/ml