

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021519\
 Data File : PS003205.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Feb 2019 18:14
 Operator : EI\SJ
 Sample : PB117147BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB117147BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 15 22:02:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.275	10.773	81057347	269.1E6	213.511	629.486 #
Target Compounds							
6) T	MCP	11.965	0.000	11704614	0	9.769	N.D. #
12) T	2,4,5-T	14.818	0.000	9462070	0	3.879	N.D. #
13) T	2,4-DB	15.562	15.053	41508840	4704395	158.777	18.521 #
14) T	DINOSEB	0.000	15.500	0	3938872	N.D.	2.247 #
15) T	Picloram	0.000	16.697	0	16305102	N.D.	5.423 #
16) T	DCPA	0.000	16.697	0	16305102	N.D.	5.264 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021519\
Data File : PS003205.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Feb 2019 18:14
Operator : EI\SJ
Sample : PB117147BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB117147BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 15 22:02:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

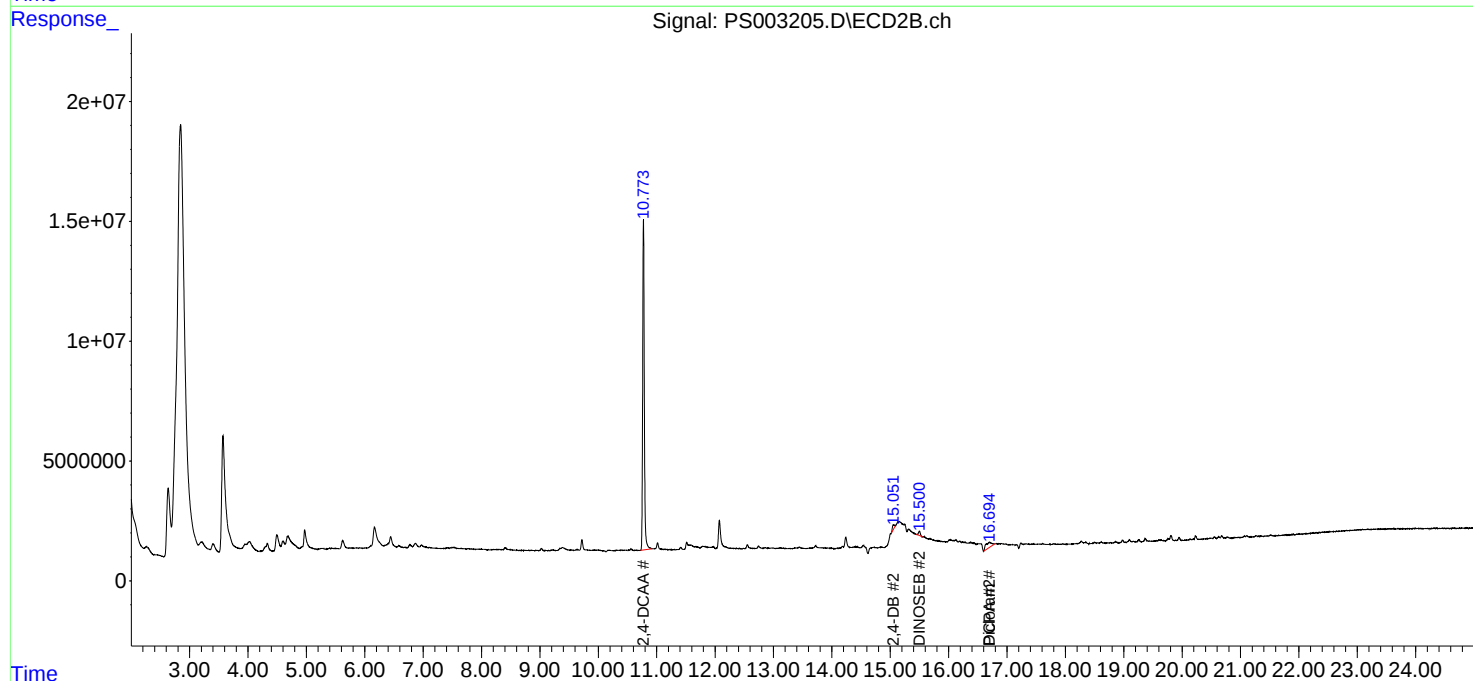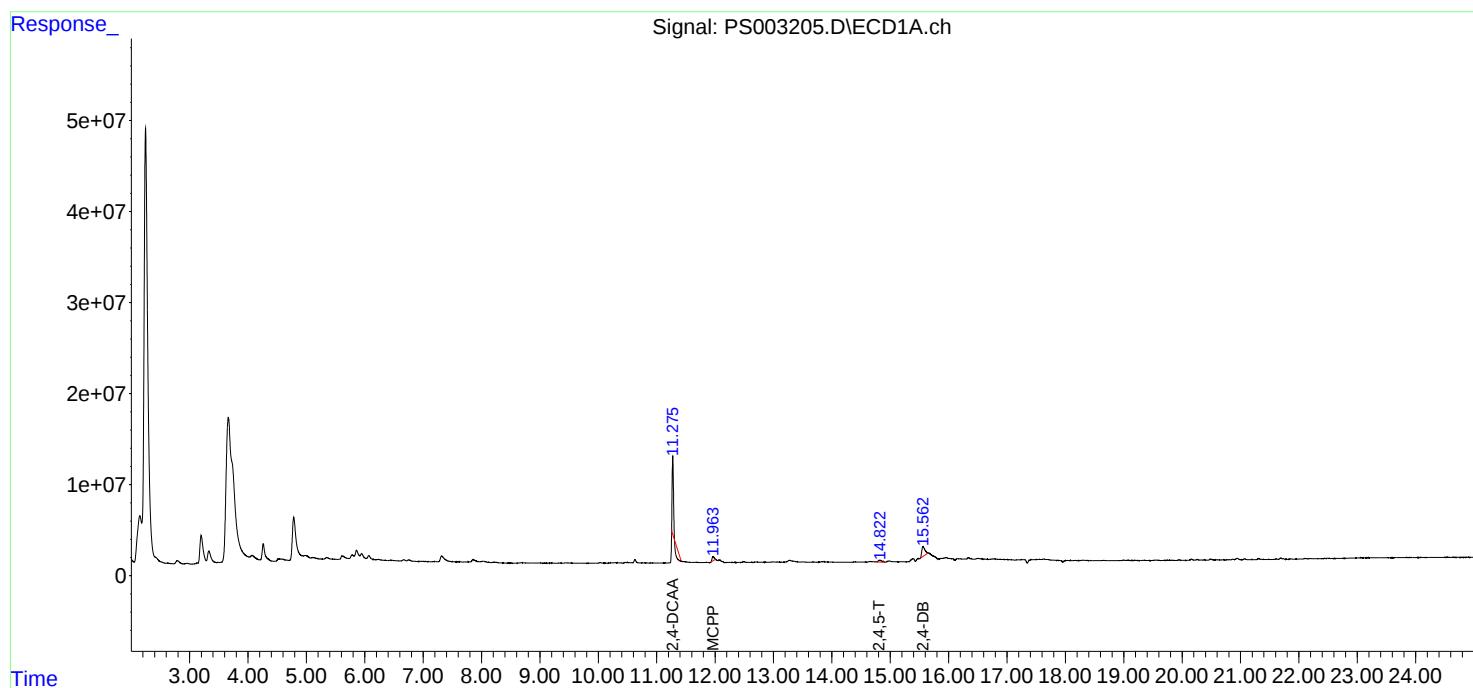


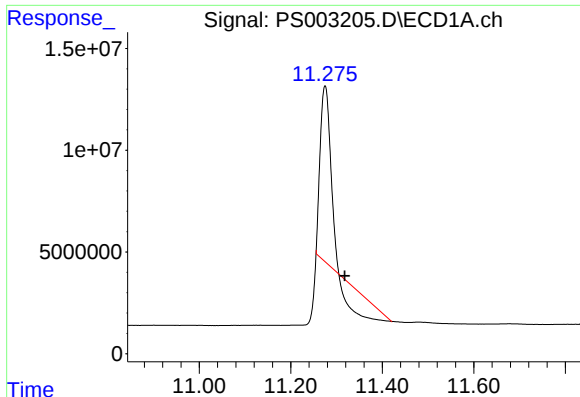

#4 2,4-DCAA


R.T.: 11.275 min
Delta R.T.: -0.043 min
Response: 81057347
Conc: 213.51 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB117147BL

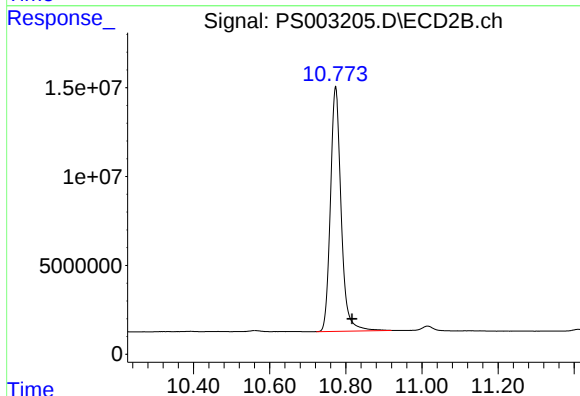


#4 2,4-DCAA

R.T.: 10.773 min
Delta R.T.: -0.044 min
Response: 269134211
Conc: 629.49 ng/ml

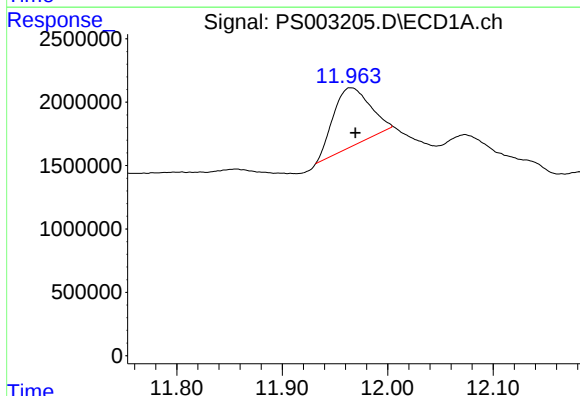


#6 MCPP

R.T.: 11.965 min
Delta R.T.: -0.004 min
Response: 11704614
Conc: 9.77 ug/ml

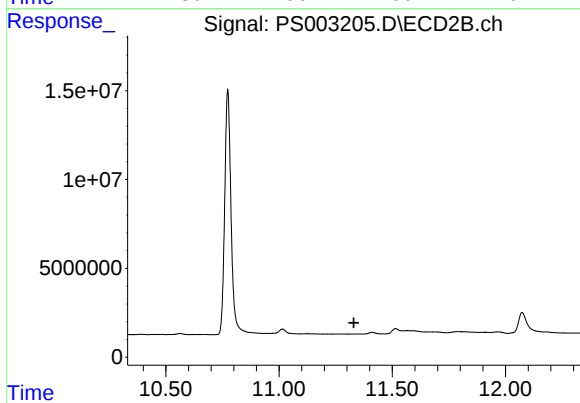

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 11.330 min
Response: 0
Conc: N.D.

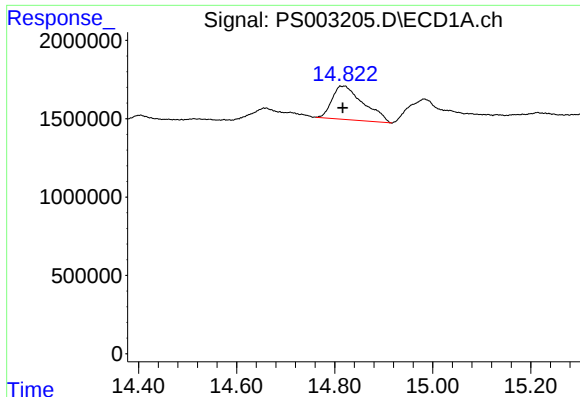

#12 2,4,5-T


R.T.: 14.818 min
Delta R.T.: 0.002 min
Response: 9462070
Conc: 3.88 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB117147BL

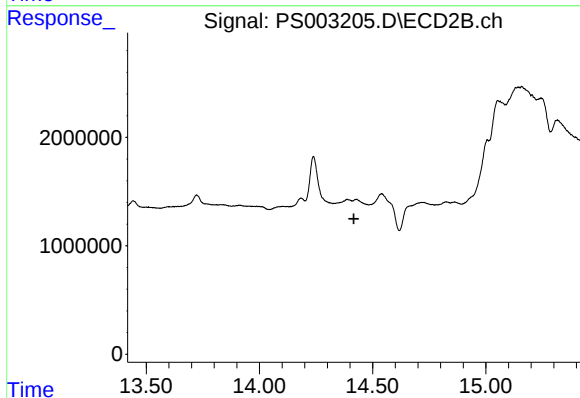


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.417 min
Response: 0
Conc: N.D.

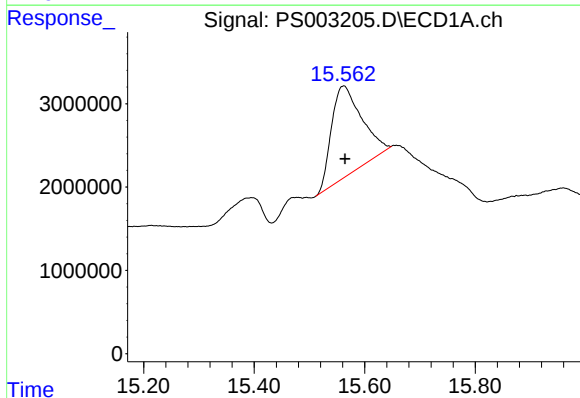


#13 2,4-DB

R.T.: 15.562 min
Delta R.T.: -0.003 min
Response: 41508840
Conc: 158.78 ng/ml

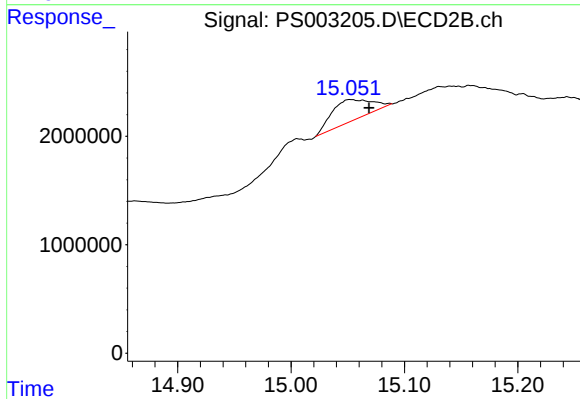

#13 2,4-DB


R.T.: 15.053 min
Delta R.T.: -0.016 min
Response: 4704395
Conc: 18.52 ng/ml

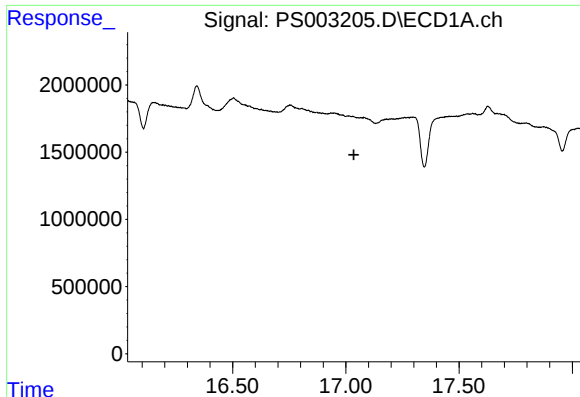

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB117147BL

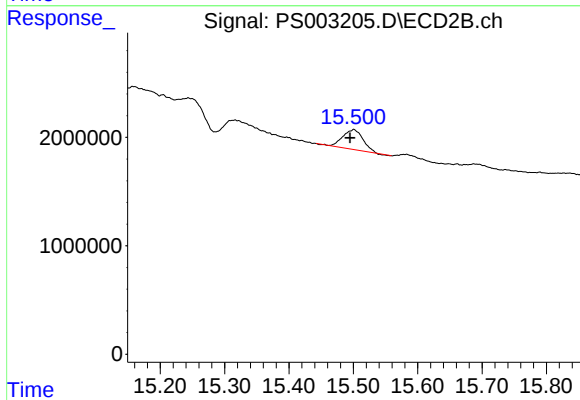


#14 DINOSEB

R.T.: 15.500 min
Delta R.T.: 0.005 min
Response: 3938872
Conc: 2.25 ng/ml

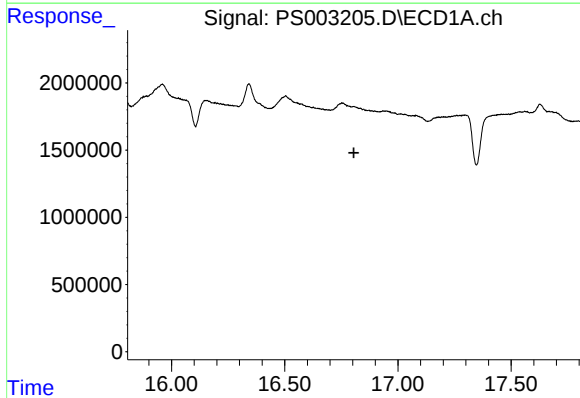


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.806 min
Response: 0
Conc: N.D.

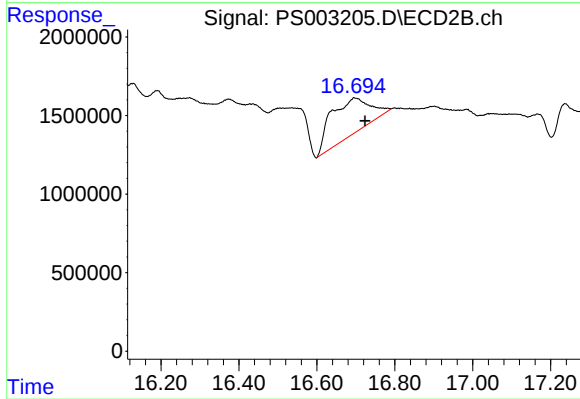

#15 Picloram


R.T.: 16.697 min
Delta R.T.: -0.027 min
Response: 16305102
Conc: 5.42 ng/ml

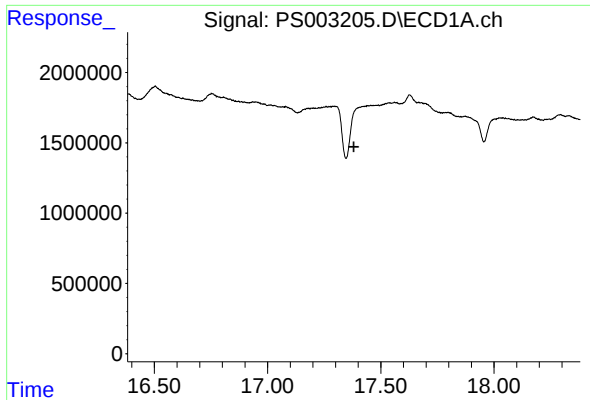

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB117147BL

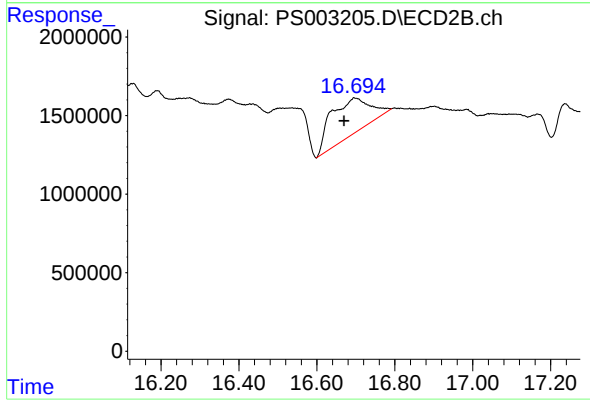

#16 DCPA

R.T.: 16.697 min
Delta R.T.: 0.027 min
Response: 16305102
Conc: 5.26 ng/ml