

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021519\
 Data File : PS003208.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Feb 2019 19:47
 Operator : EI\SJ
 Sample : K1346-08
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CL-01-021419-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 15 22:03:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.306	10.803	124.5E6	124.2E6	328.034	290.525
Target Compounds							
6) T	MCP	11.984	0.000	11789371	0	9.840	N.D. #
15) T	Picloram	0.000	16.730	0	5617717	N.D.	1.869 #
16) T	DCPA	0.000	16.730	0	5617717	N.D.	1.814 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021519\
Data File : PS003208.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Feb 2019 19:47
Operator : EI\SJ
Sample : K1346-08
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
CL-01-021419-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 15 22:03:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

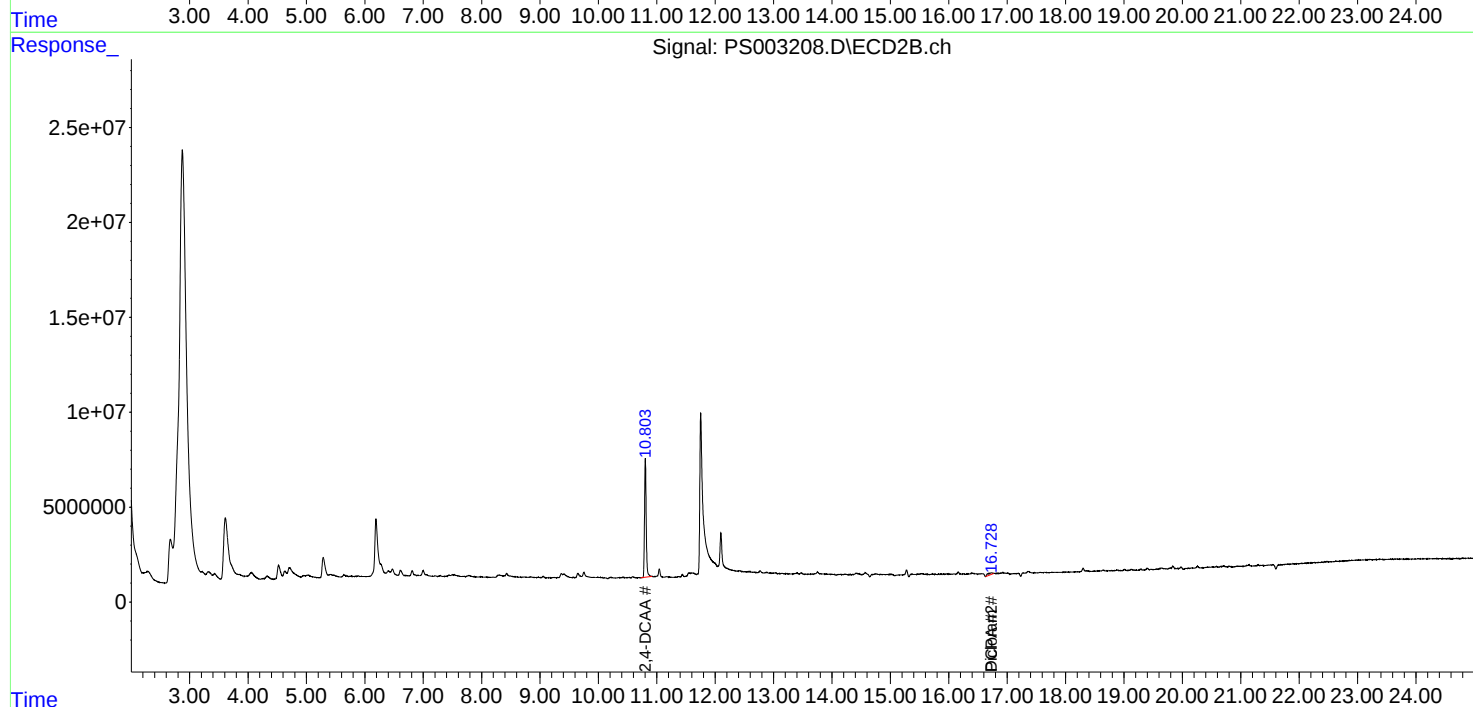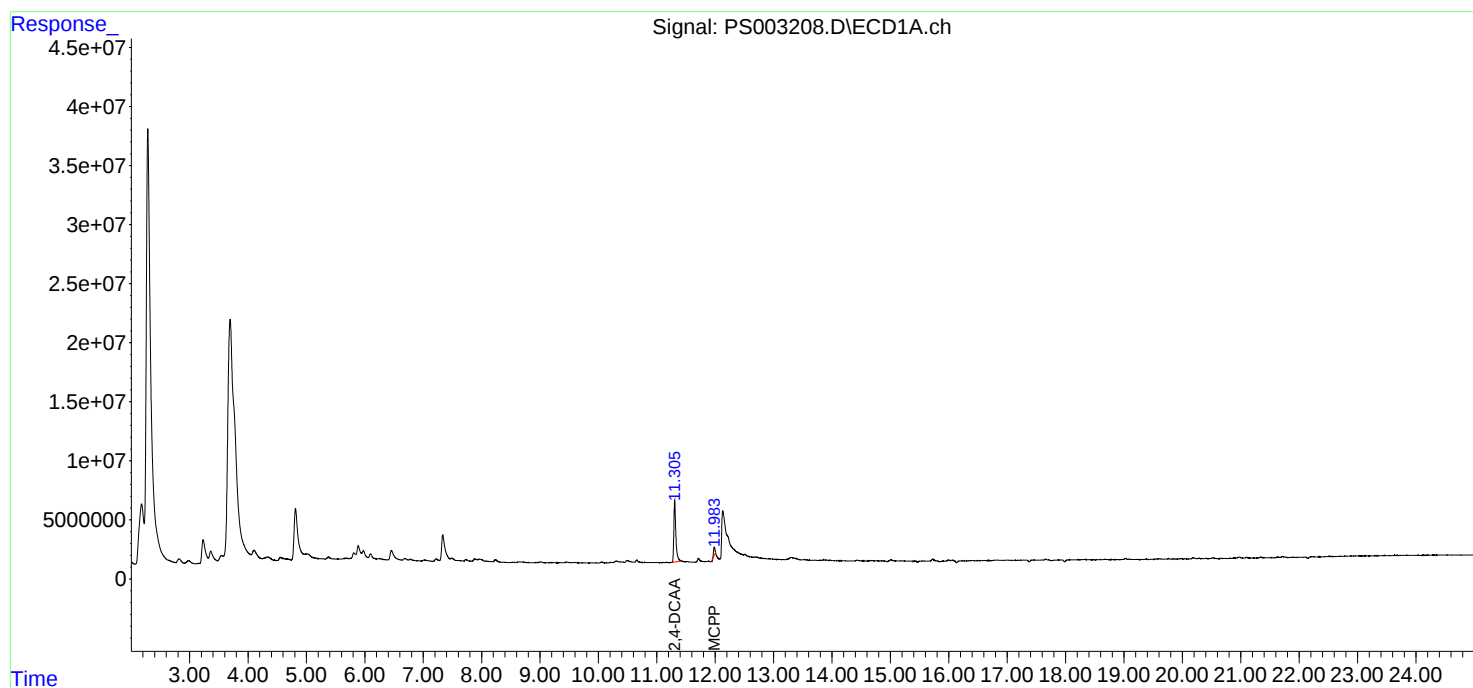


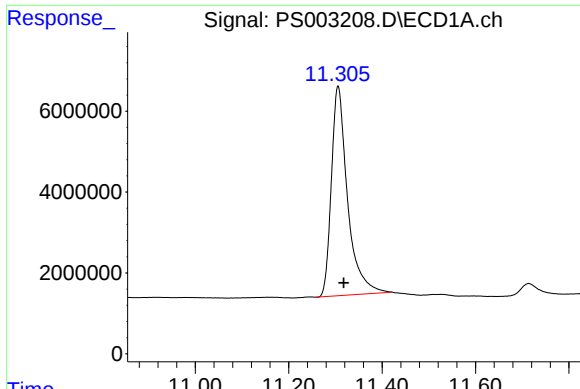

#4 2,4-DCAA


R.T.: 11.306 min
Delta R.T.: -0.012 min
Response: 124535033
Conc: 328.03 ng/ml

Instrument :
ECD_S
ClientSampleId :
CL-01-021419-A

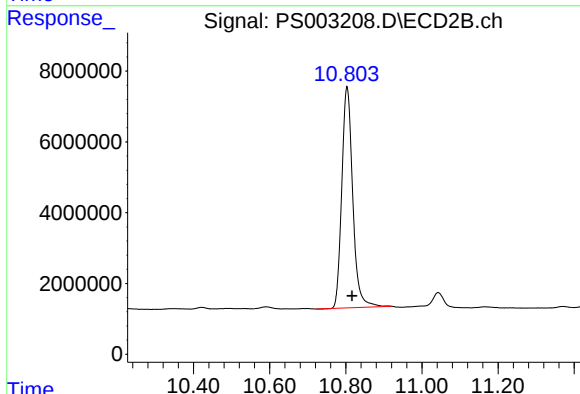


#4 2,4-DCAA

R.T.: 10.803 min
Delta R.T.: -0.013 min
Response: 124212873
Conc: 290.53 ng/ml

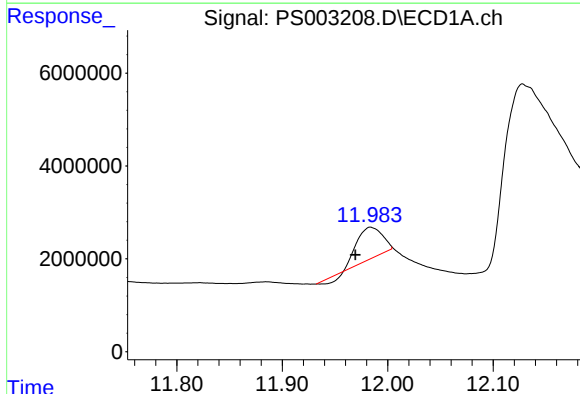


#6 MCPP

R.T.: 11.984 min
Delta R.T.: 0.015 min
Response: 11789371
Conc: 9.84 ug/ml

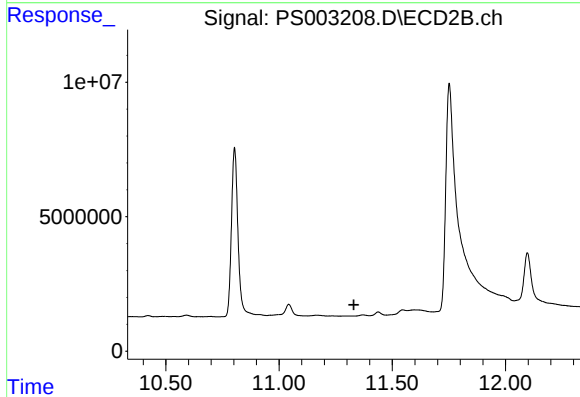

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 11.330 min
Response: 0
Conc: N.D.

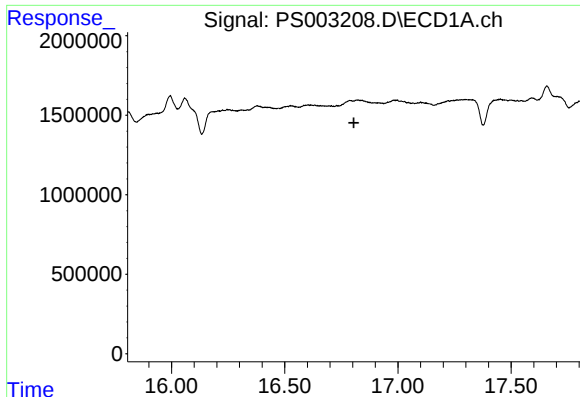

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.806 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-01-021419-A

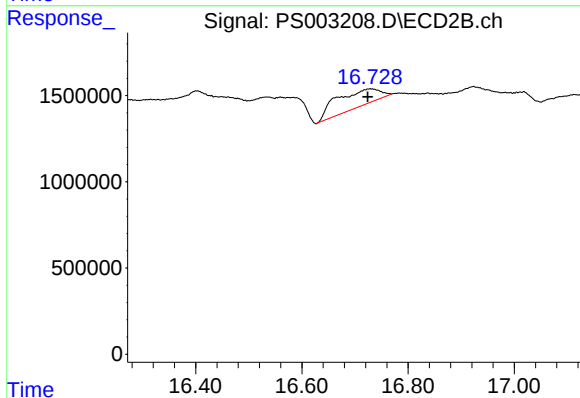


#15 Picloram

R.T.: 16.730 min
Delta R.T.: 0.005 min
Response: 5617717
Conc: 1.87 ng/ml

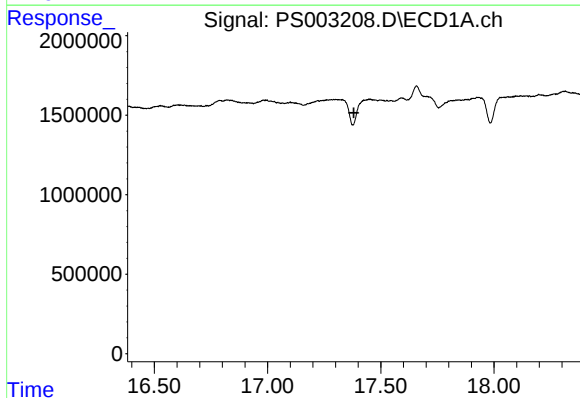

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

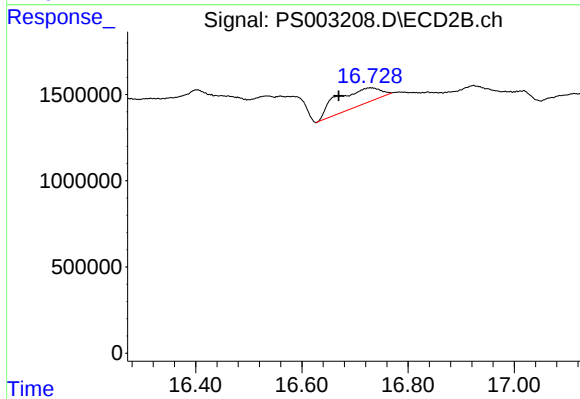

#16 DCPA

R.T.: 16.730 min
Delta R.T.: 0.060 min
Response: 5617717
Conc: 1.81 ng/ml