

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021519\
 Data File : PS003211.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Feb 2019 21:20
 Operator : EI\SJ
 Sample : K1346-10
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CL-01-021419-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 15 22:04:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.296	10.779	198.2E6	194.9E6	522.152	455.927
Target Compounds							
6) T	MCP	11.980	0.000	3321174	0	2.772	N.D. #
7) T	MCPA	12.223	0.000	5529639	0	3.124	N.D. #
14) T	DINOSEB	0.000	15.512	0	4470392	N.D.	2.550 #
15) T	Picloram	0.000	16.709	0	9466420	N.D.	3.149 #
16) T	DCPA	0.000	16.709	0	9466420	N.D.	3.056 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021519\
Data File : PS003211.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Feb 2019 21:20
Operator : EI\SJ
Sample : K1346-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
CL-01-021419-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 15 22:04:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

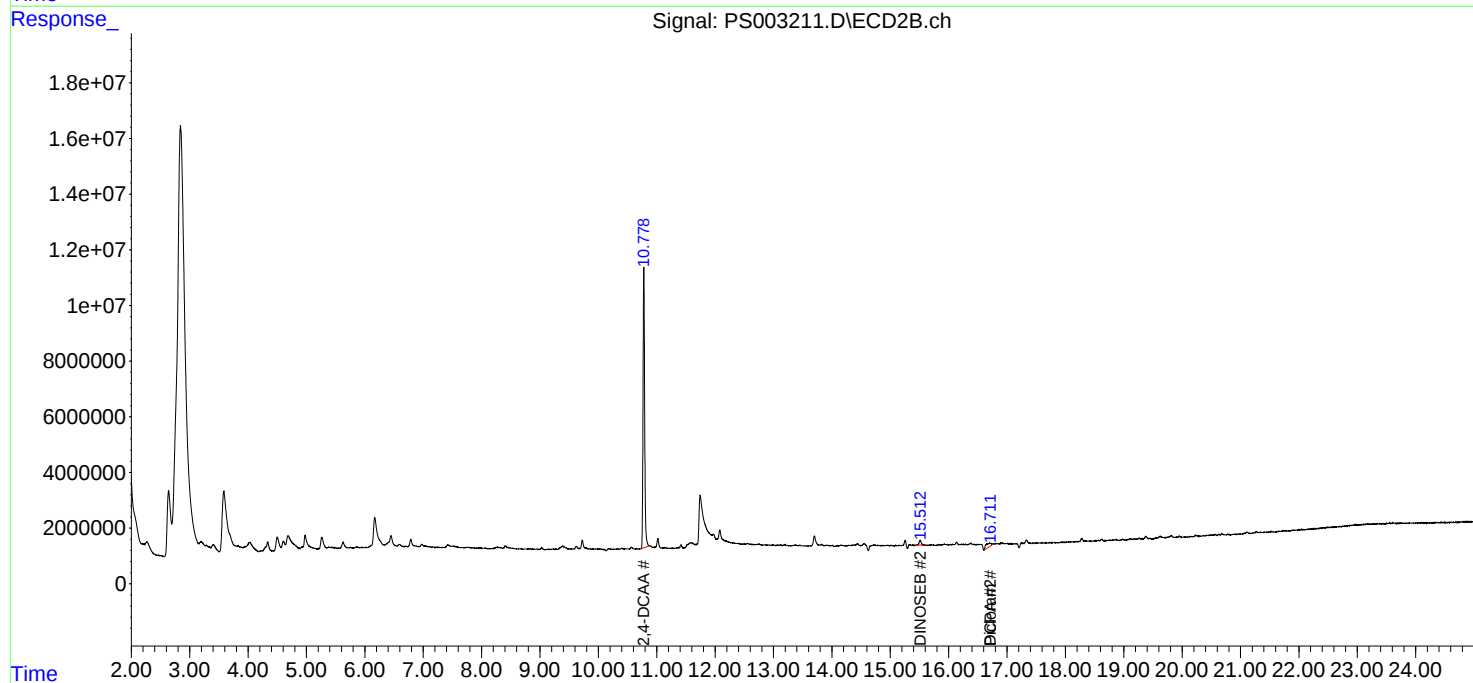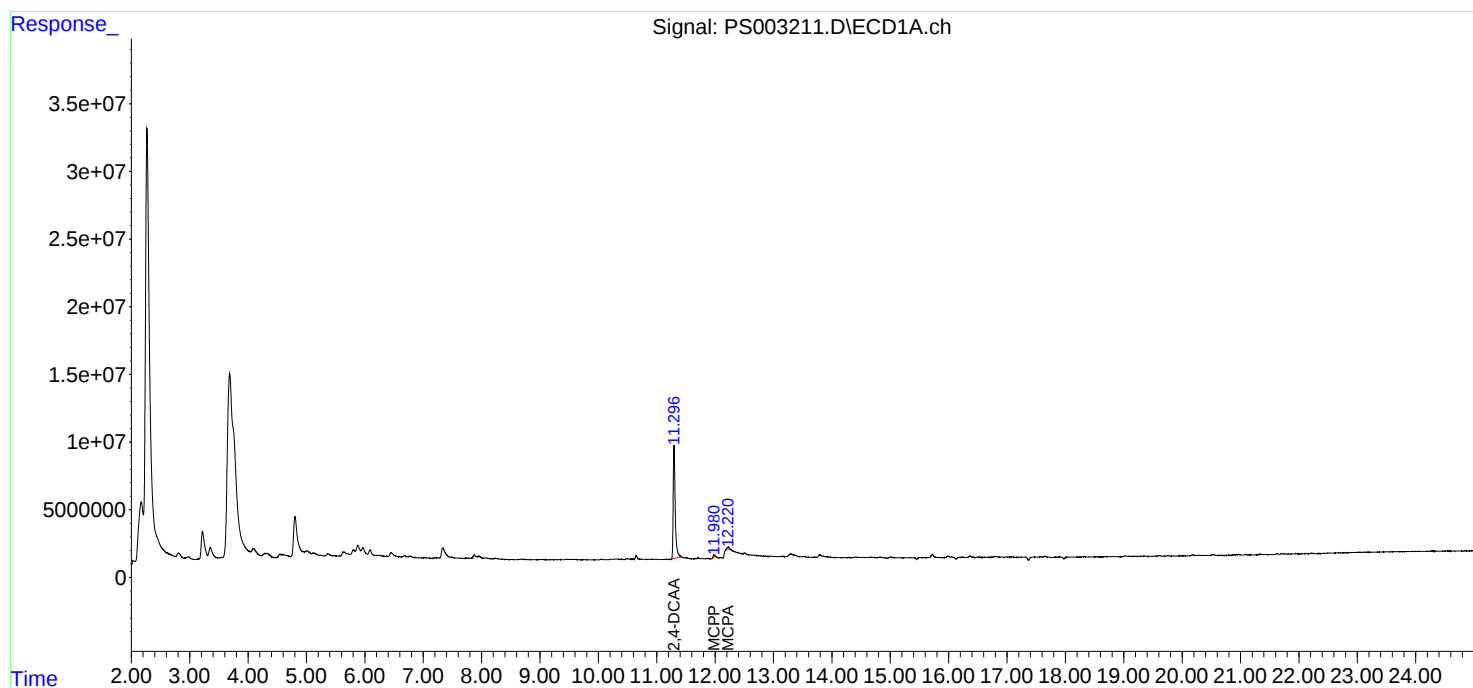


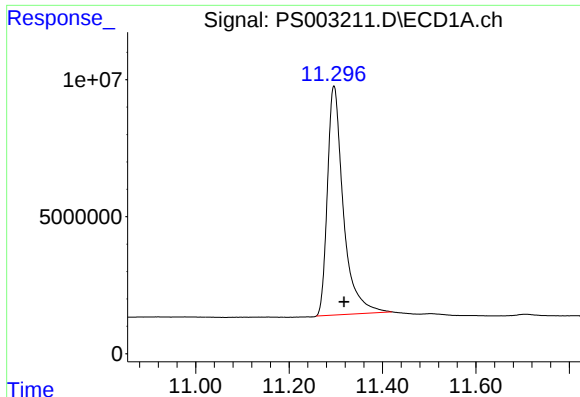

#4 2,4-DCAA


R.T.: 11.296 min
Delta R.T.: -0.022 min
Response: 198230364
Conc: 522.15 ng/ml

Instrument :
ECD_S
ClientSampleId :
CL-01-021419-B

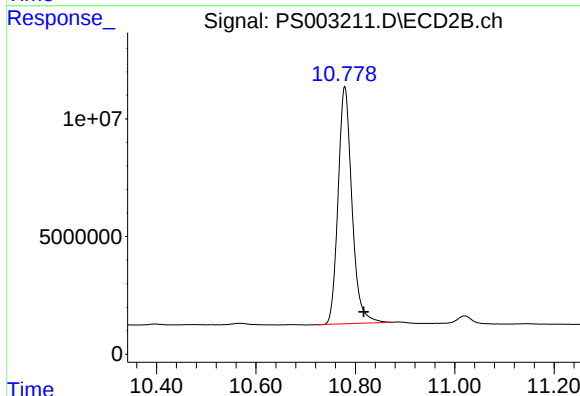


#4 2,4-DCAA

R.T.: 10.779 min
Delta R.T.: -0.038 min
Response: 194929644
Conc: 455.93 ng/ml

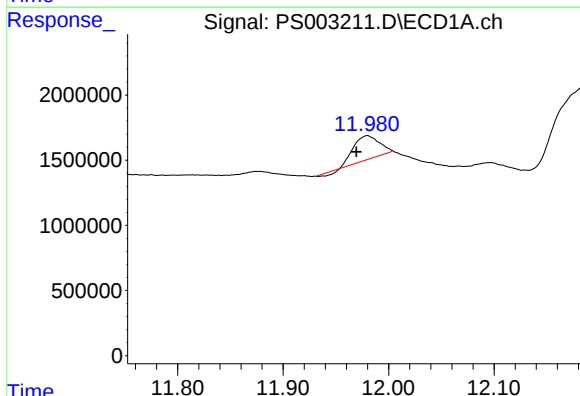


#6 MCP

R.T.: 11.980 min
Delta R.T.: 0.010 min
Response: 3321174
Conc: 2.77 ug/ml

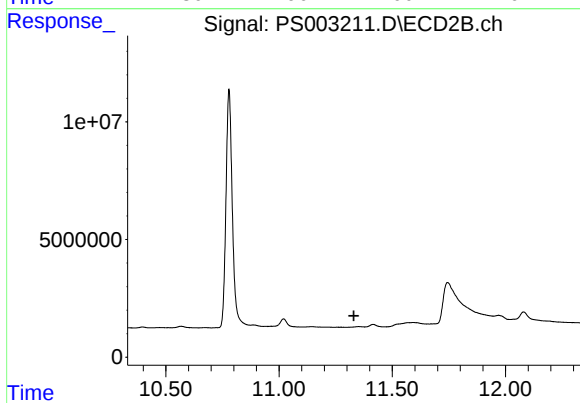

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.330 min
Response: 0
Conc: N.D.

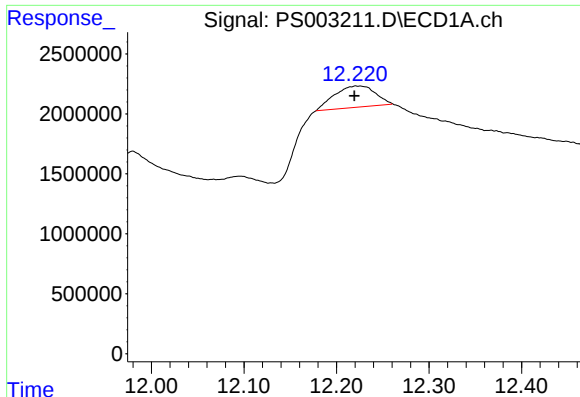

#7 MCPA


R.T.: 12.223 min
Delta R.T.: 0.004 min
Response: 5529639
Conc: 3.12 ug/ml

Instrument :
ECD_S
ClientSampleId :
CL-01-021419-B

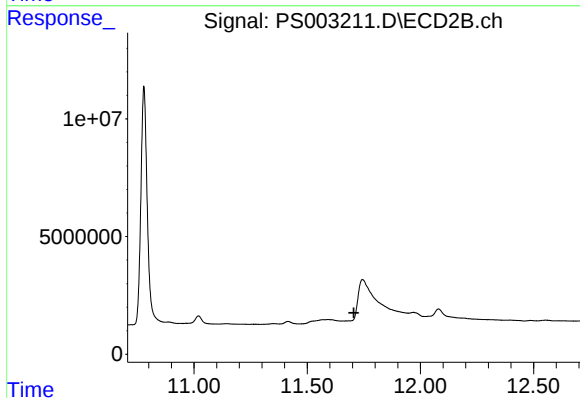


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 11.706 min
Response: 0
Conc: N.D.

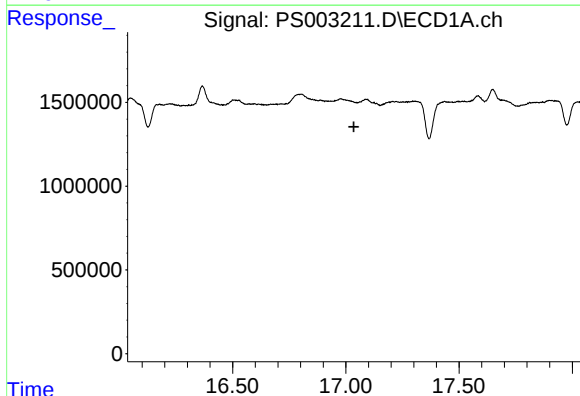


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.035 min
Response: 0
Conc: N.D.

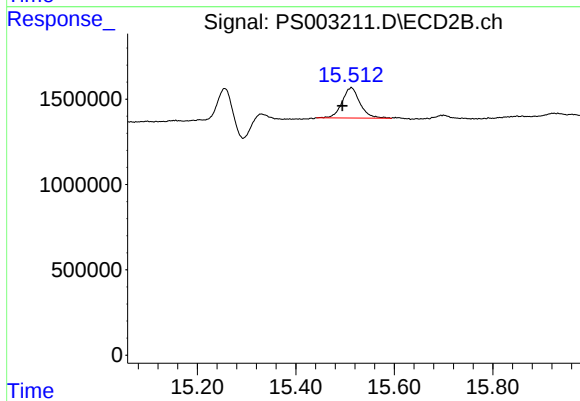

#14 DINOSEB


R.T.: 15.512 min
Delta R.T.: 0.017 min
Response: 4470392
Conc: 2.55 ng/ml

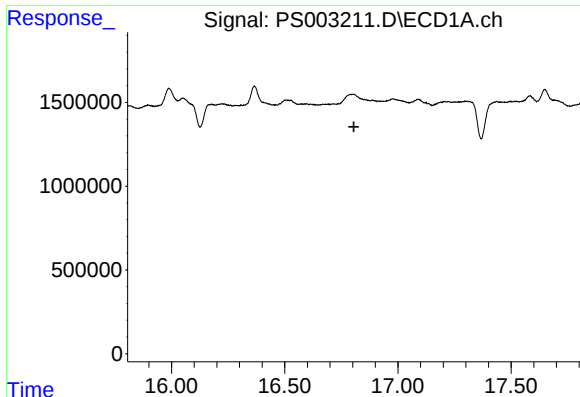

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.806 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-01-021419-B

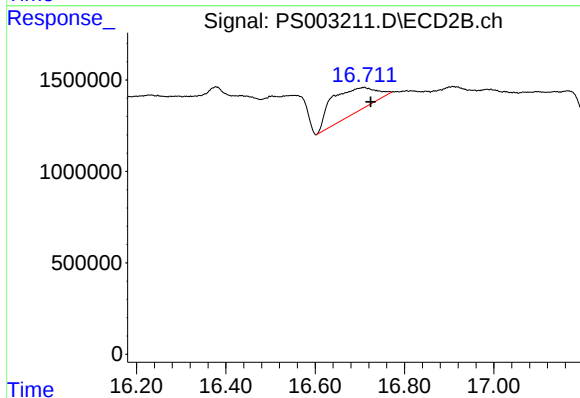


#15 Picloram

R.T.: 16.709 min
Delta R.T.: -0.015 min
Response: 9466420
Conc: 3.15 ng/ml

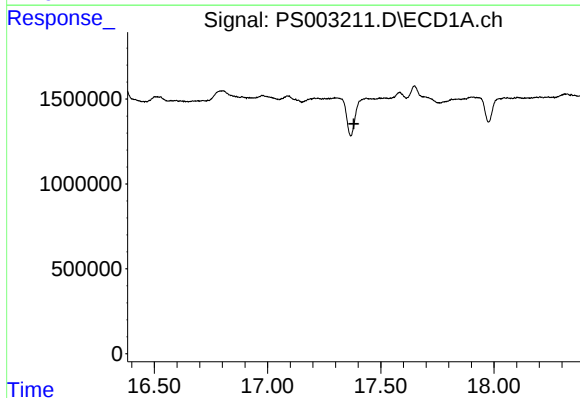

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

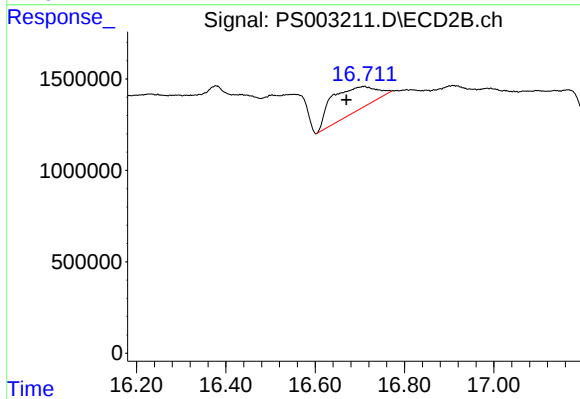

#16 DCPA

R.T.: 16.709 min
Delta R.T.: 0.040 min
Response: 9466420
Conc: 3.06 ng/ml