

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021519\
 Data File : PS003212.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Feb 2019 21:51
 Operator : EI\SJ
 Sample : K1346-12
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CL-01-021419-C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 16 00:44:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.290	10.786	94291094	98187005	248.369	229.653
Target Compounds							
2) T	3,5-DICHL...	0.000	9.034	0	2070770	N.D.	3.674 #
6) T	MCPP	11.971	0.000	7537286	0	6.291	N.D. #
11) T	2,4,5-TP ...	14.413	0.000	2784021	0	1.105	N.D. #
14) T	DINOSEB	0.000	15.520	0	2982479	N.D.	1.701 #
15) T	Picloram	0.000	16.715	0	7622750	N.D.	2.536 #
16) T	DCPA	0.000	16.715	0	7622750	N.D.	2.461 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021519\
Data File : PS003212.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Feb 2019 21:51
Operator : EI\SJ
Sample : K1346-12
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
CL-01-021419-C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 16 00:44:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

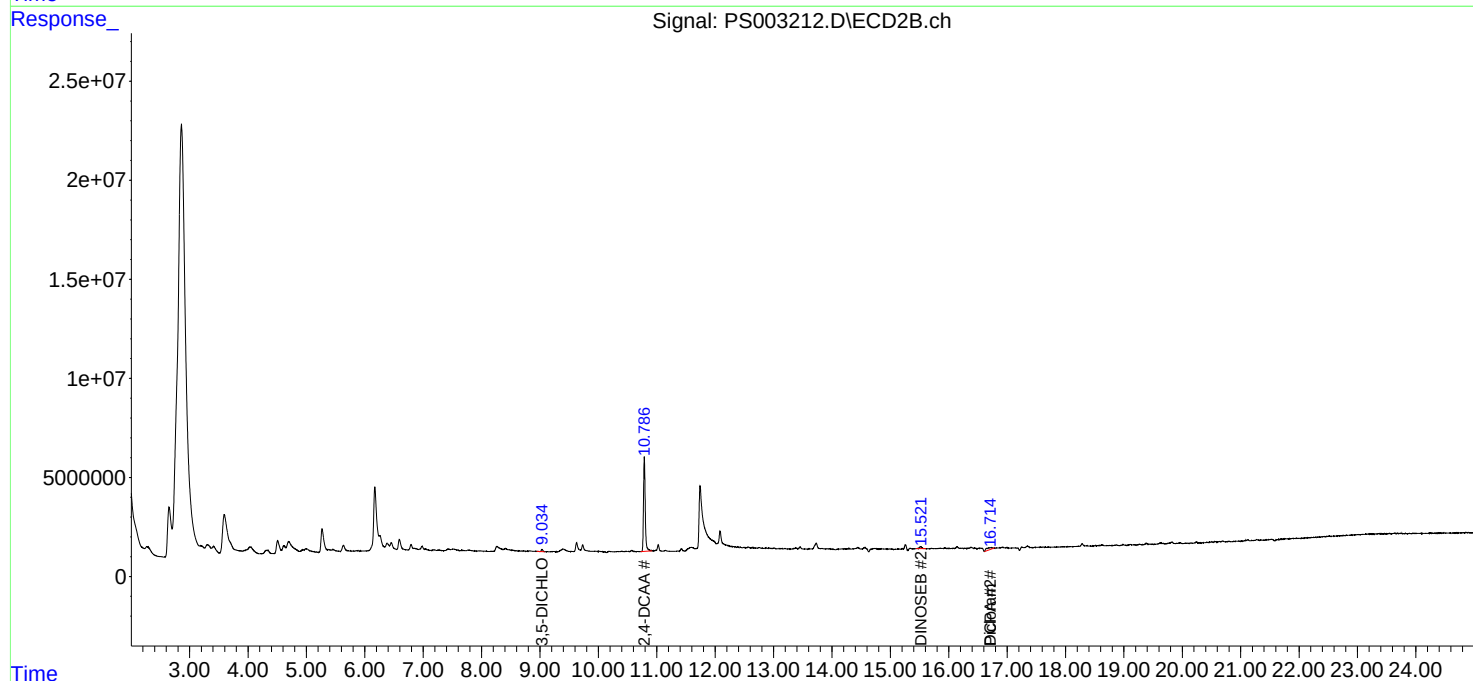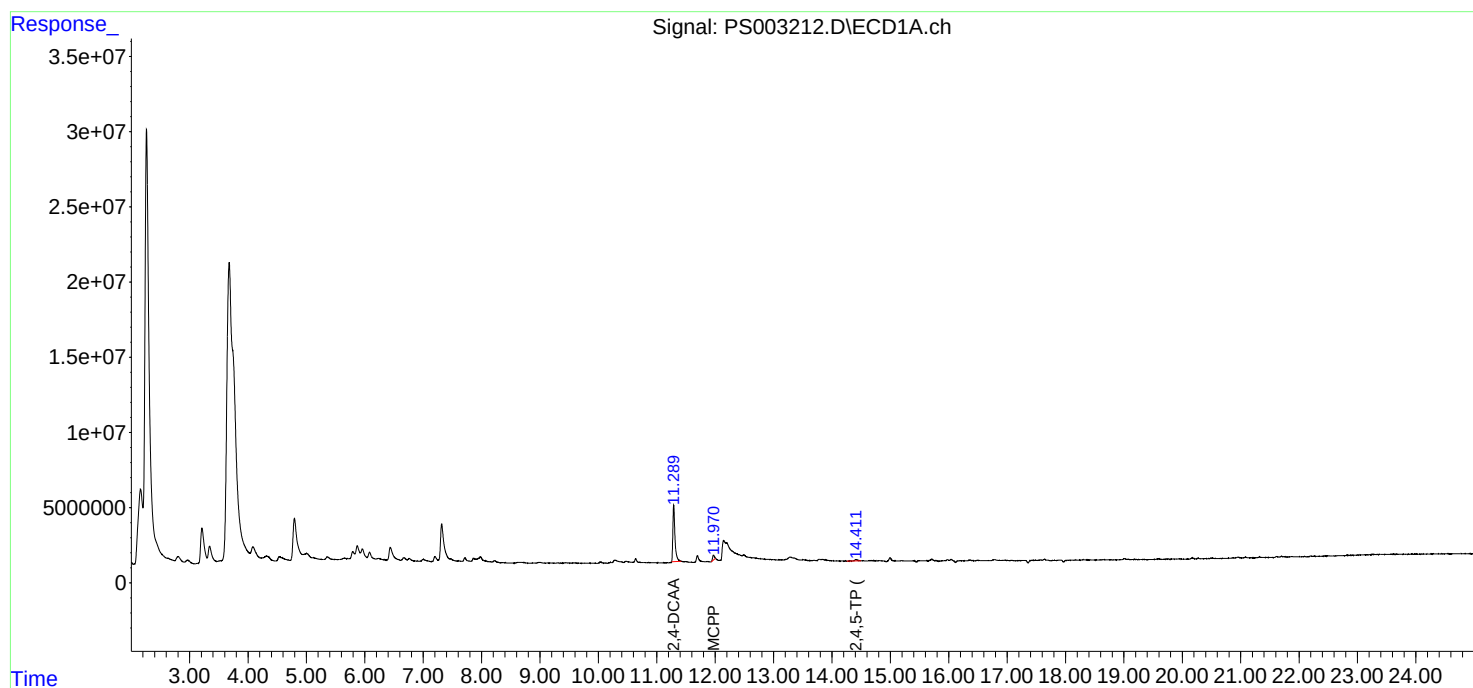


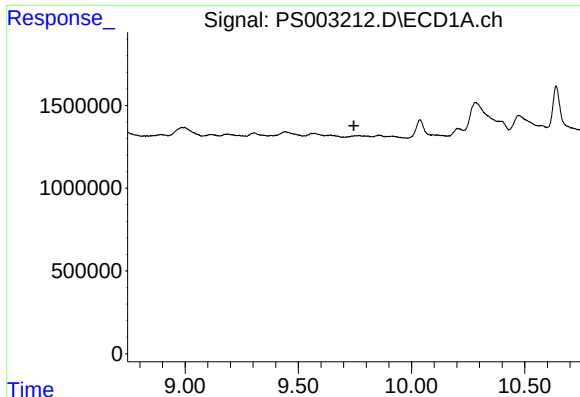

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.745 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-01-021419-C

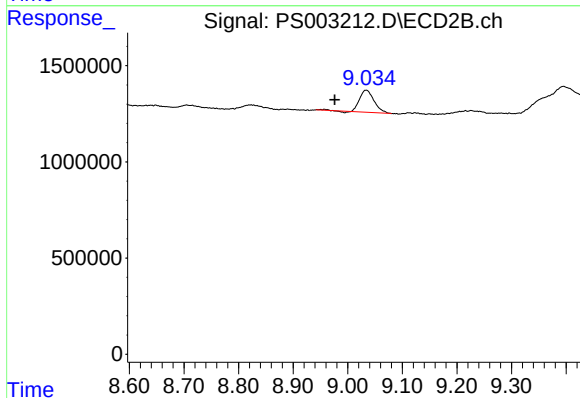


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.034 min
Delta R.T.: 0.057 min
Response: 2070770
Conc: 3.67 ng/ml

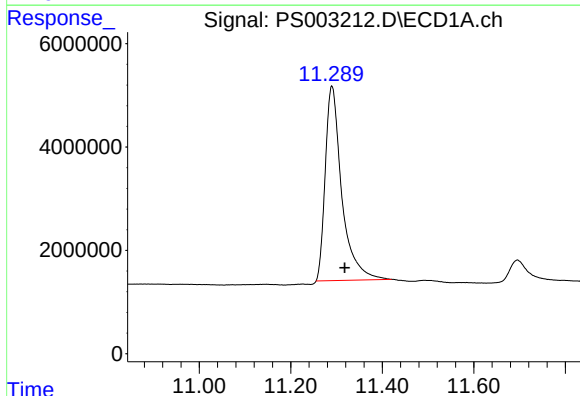


#4 2,4-DCAA

R.T.: 11.290 min
Delta R.T.: -0.028 min
Response: 94291094
Conc: 248.37 ng/ml

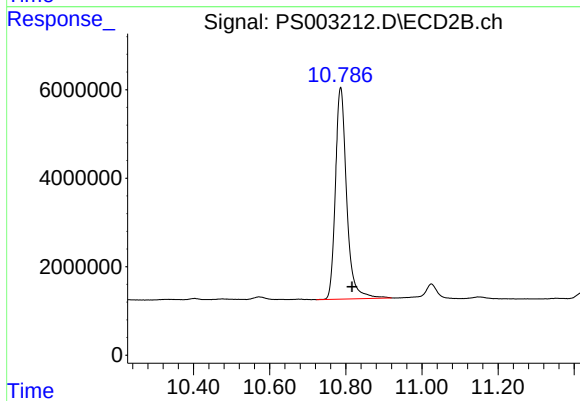

#4 2,4-DCAA


R.T.: 10.786 min
Delta R.T.: -0.030 min
Response: 98187005
Conc: 229.65 ng/ml

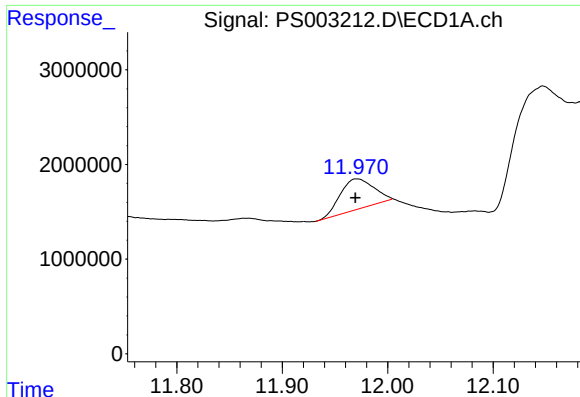

#6 MCPP


R.T.: 11.971 min
Delta R.T.: 0.002 min
Response: 7537286
Conc: 6.29 ug/ml

Instrument :
ECD_S
ClientSampleId :
CL-01-021419-C

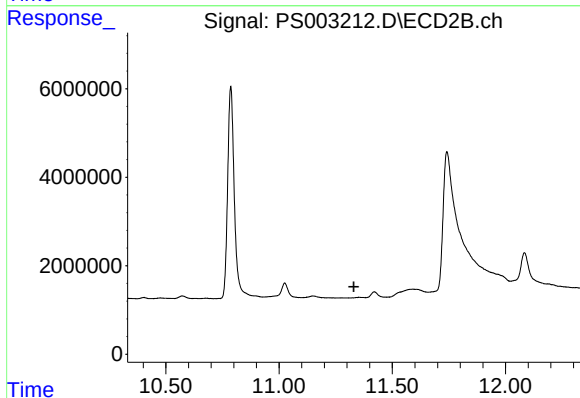


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.330 min
Response: 0
Conc: N.D.

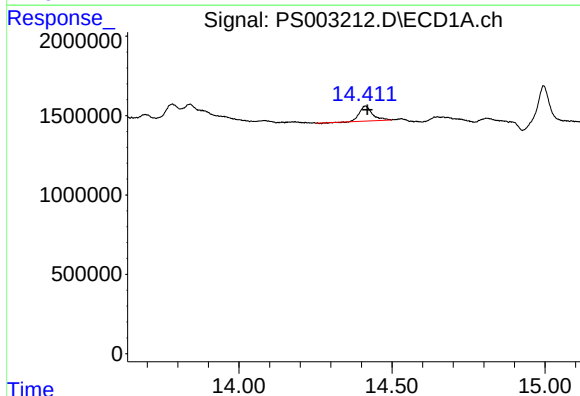


#11 2,4,5-TP (SILVEX)

R.T.: 14.413 min
Delta R.T.: -0.007 min
Response: 2784021
Conc: 1.11 ng/ml

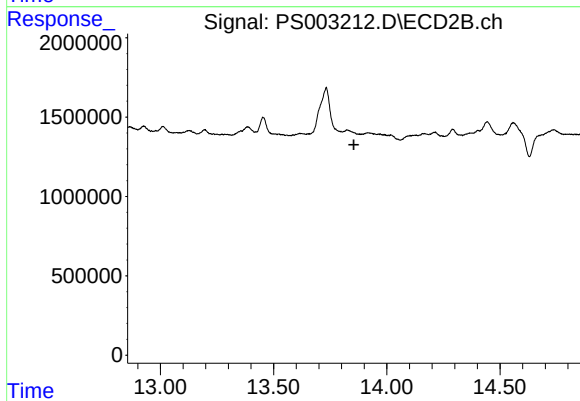

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 13.854 min
Response: 0
Conc: N.D.

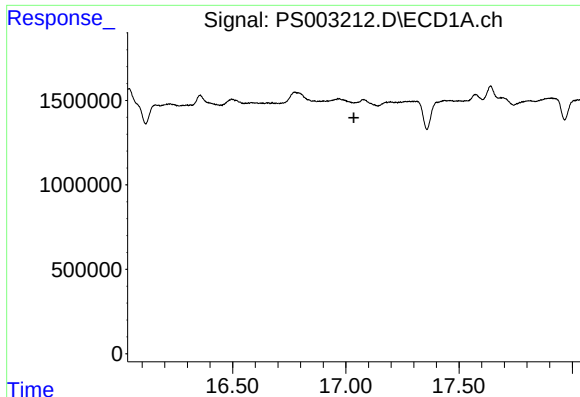

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-01-021419-C

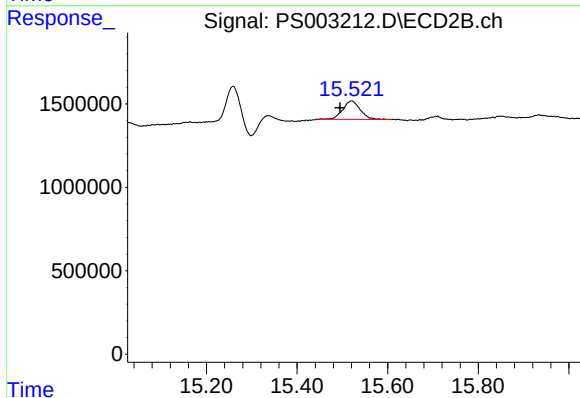


#14 DINOSEB

R.T.: 15.520 min
Delta R.T.: 0.025 min
Response: 2982479
Conc: 1.70 ng/ml

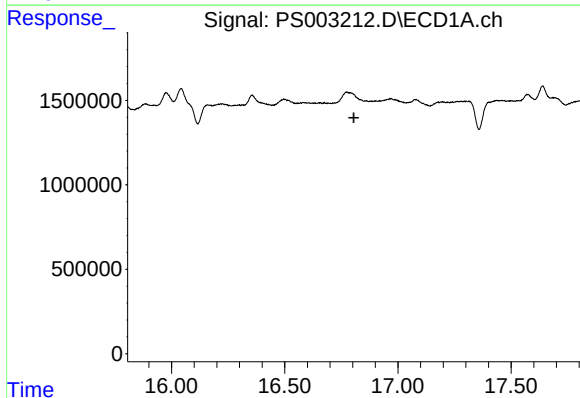


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.806 min
Response: 0
Conc: N.D.

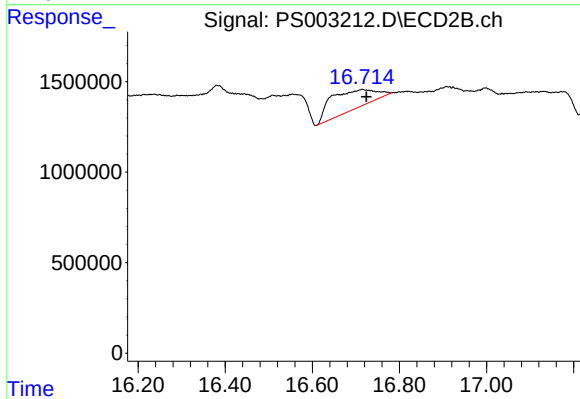

#15 Picloram


R.T.: 16.715 min
Delta R.T.: -0.009 min
Response: 7622750
Conc: 2.54 ng/ml

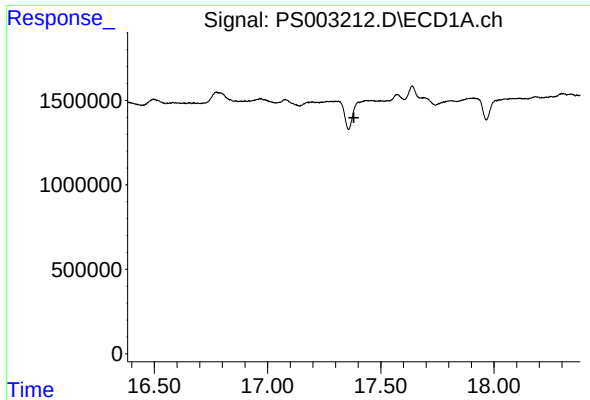

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-01-021419-C

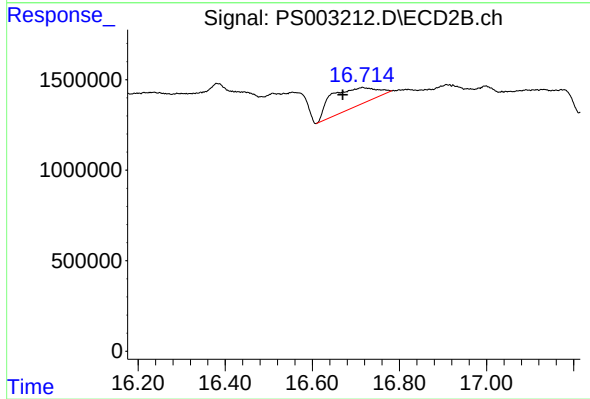

#16 DCPA

R.T.: 16.715 min
Delta R.T.: 0.045 min
Response: 7622750
Conc: 2.46 ng/ml