

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021519\
 Data File : PS003214.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Feb 2019 22:53
 Operator : EI\SJ
 Sample : K1346-16
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CL-01-021419-E

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 16 00:44:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.277	10.776	44961164	189.3E6	118.431	442.869 #
Target Compounds							
5) T	DICAMBA	11.687	0.000	3355873	0	2.094	N.D. #
6) T	MCCP	11.960	0.000	10767597	0	8.987	N.D. #
7) T	MCPA	0.000	11.724	0	27668063	N.D.	17.589 #
15) T	Picloram	0.000	16.707	0	6489467	N.D.	2.159 #
16) T	DCPA	0.000	16.707	0	6489467	N.D.	2.095 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021519\
Data File : PS003214.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Feb 2019 22:53
Operator : EI\SJ
Sample : K1346-16
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
CL-01-021419-E

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 16 00:44:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

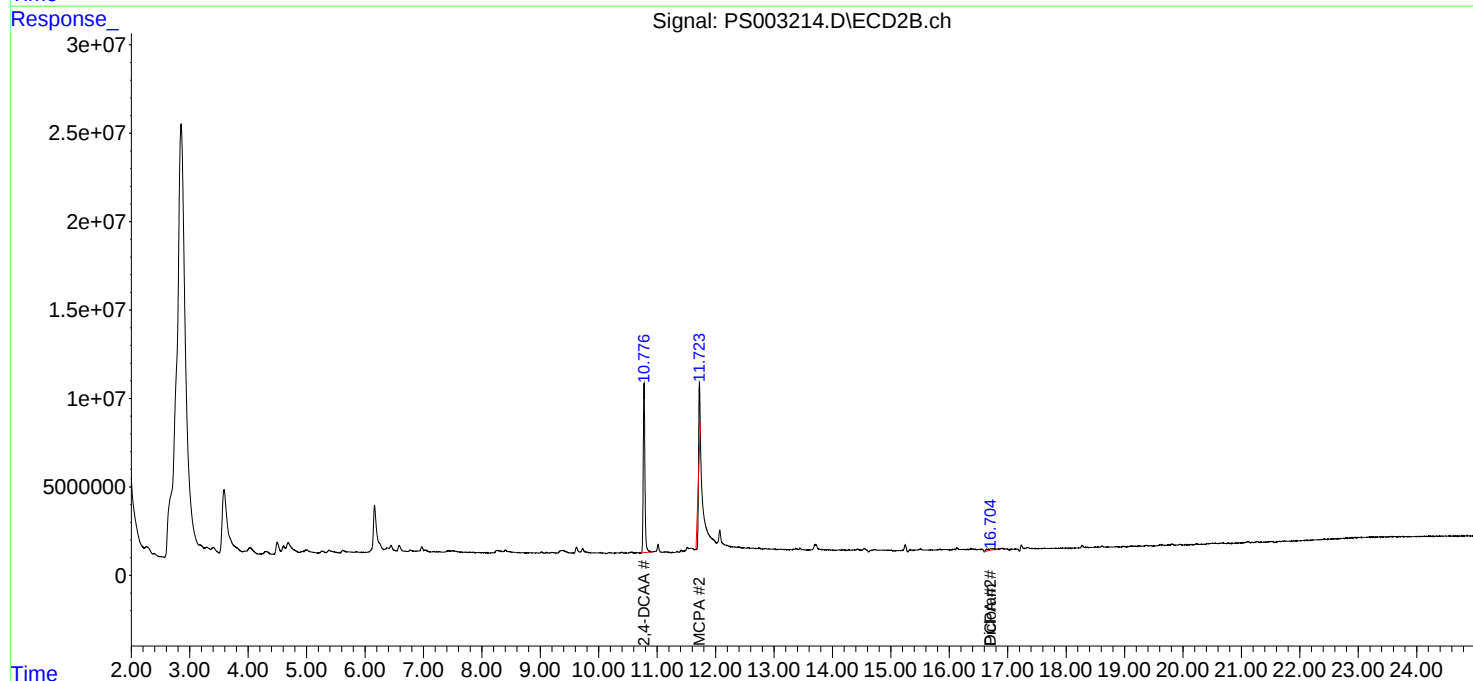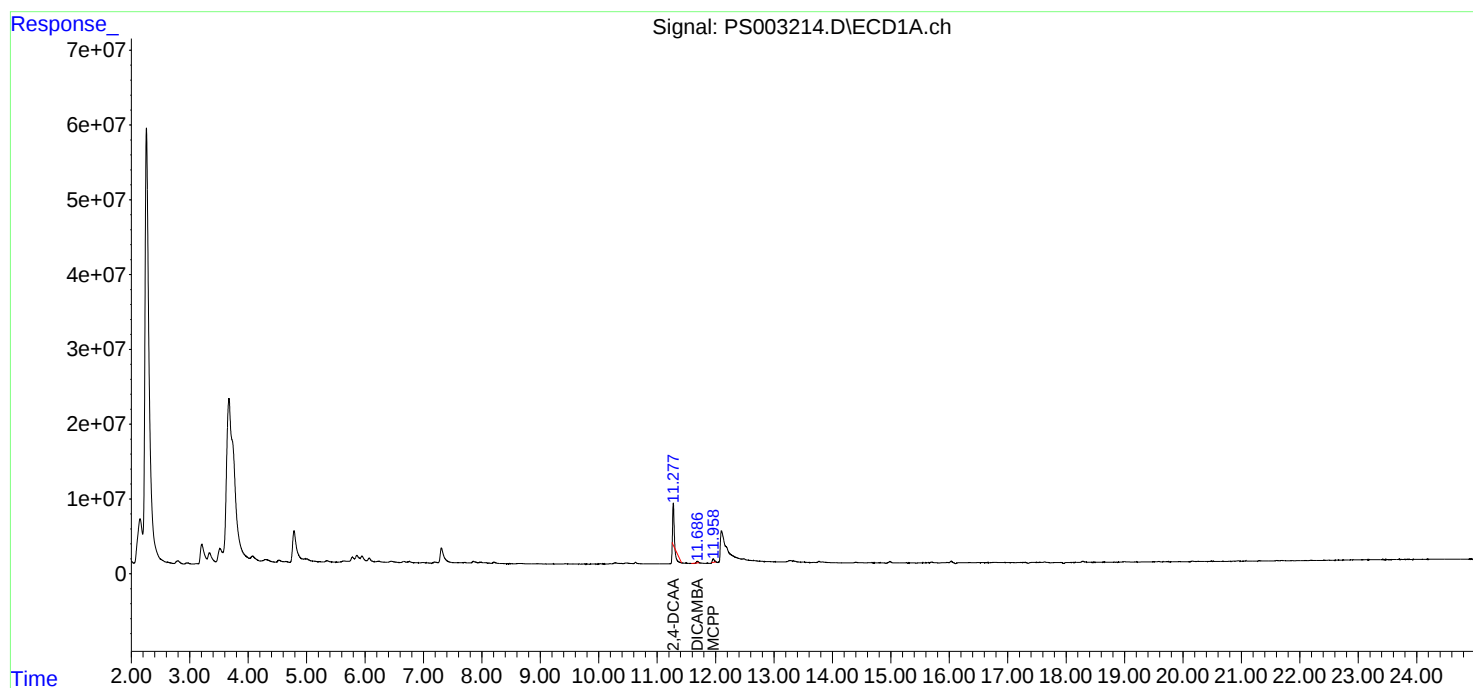


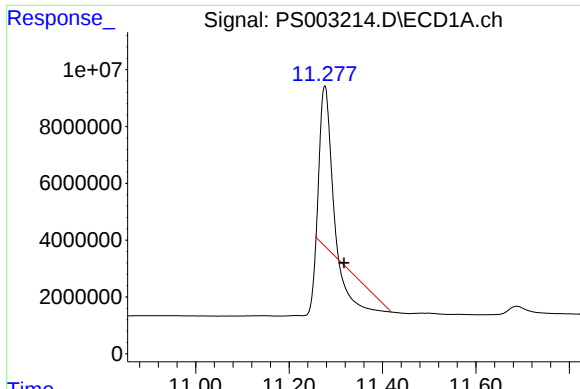

#4 2,4-DCAA


R.T.: 11.277 min
Delta R.T.: -0.041 min
Response: 44961164
Conc: 118.43 ng/ml

Instrument :
ECD_S
ClientSampleId :
CL-01-021419-E

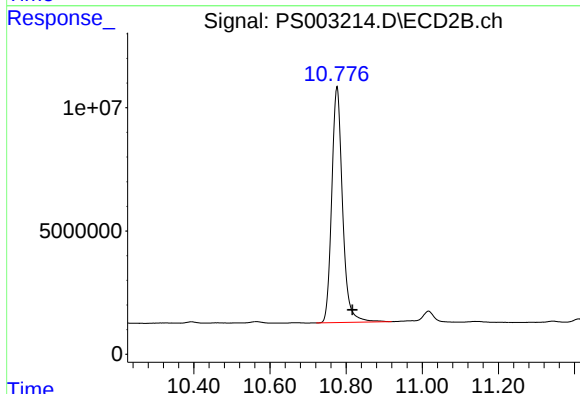


#4 2,4-DCAA

R.T.: 10.776 min
Delta R.T.: -0.041 min
Response: 189346947
Conc: 442.87 ng/ml

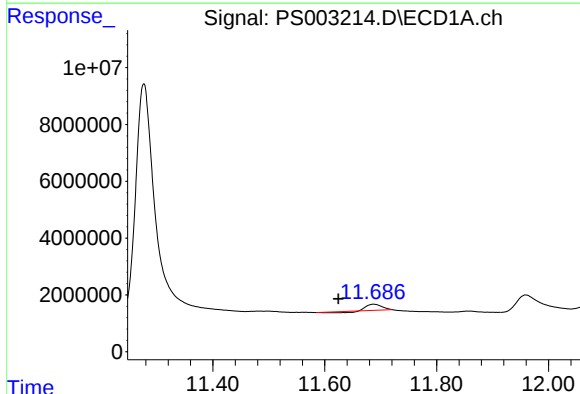


#5 DICAMBA

R.T.: 11.687 min
Delta R.T.: 0.063 min
Response: 3355873
Conc: 2.09 ng/ml

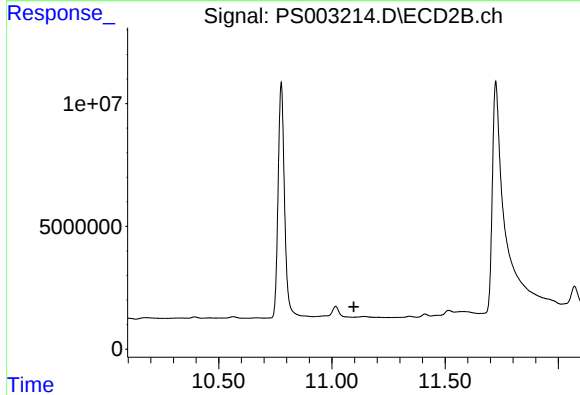

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.097 min
Response: 0
Conc: N.D.

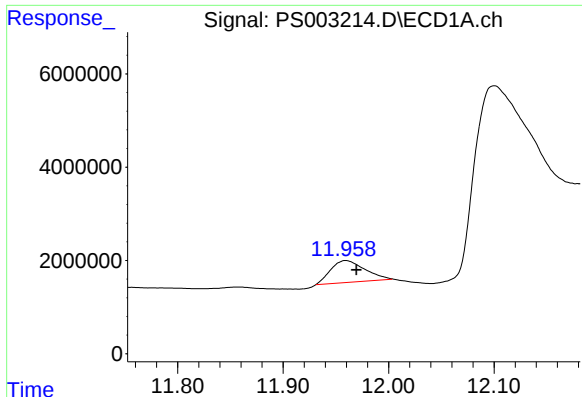

#6 MCPP


R.T.: 11.960 min
Delta R.T.: -0.010 min
Response: 10767597
Conc: 8.99 ug/ml

Instrument :
ECD_S
ClientSampleId :
CL-01-021419-E

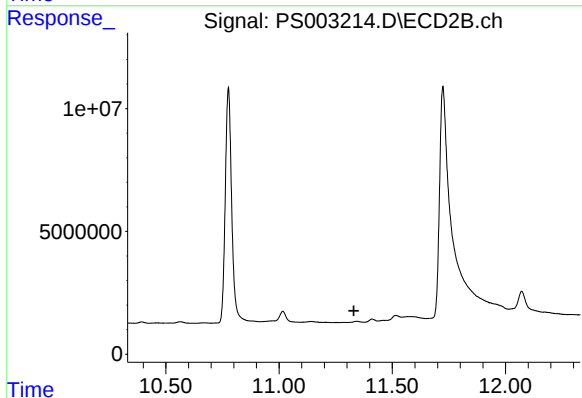


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.330 min
Response: 0
Conc: N.D.

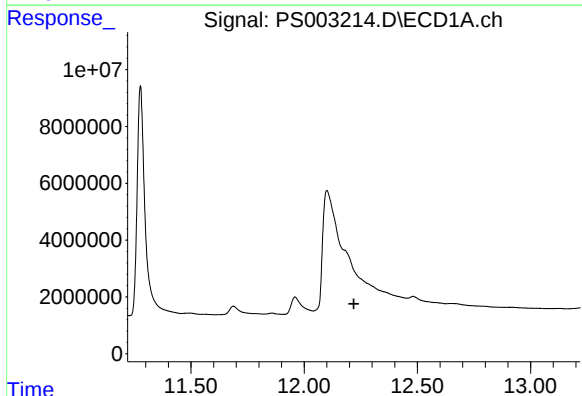


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.219 min
Response: 0
Conc: N.D.

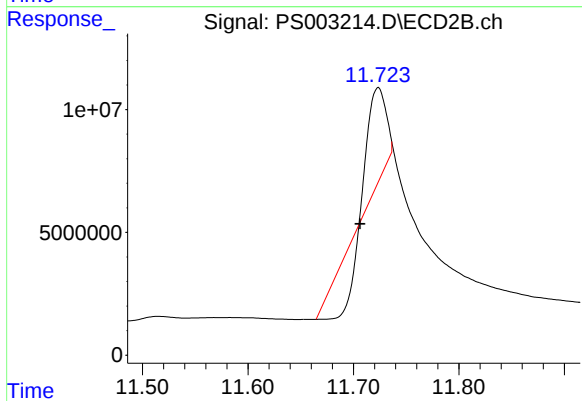

#7 MCPA


R.T.: 11.724 min
Delta R.T.: 0.017 min
Response: 27668063
Conc: 17.59 ug/ml

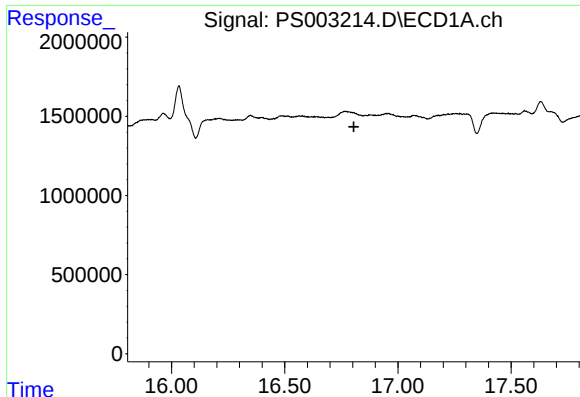

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.806 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-01-021419-E

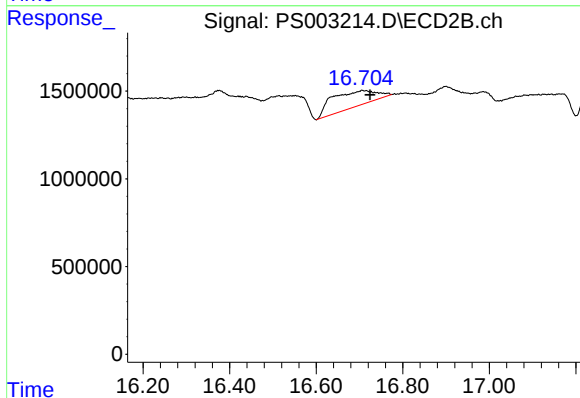


#15 Picloram

R.T.: 16.707 min
Delta R.T.: -0.017 min
Response: 6489467
Conc: 2.16 ng/ml

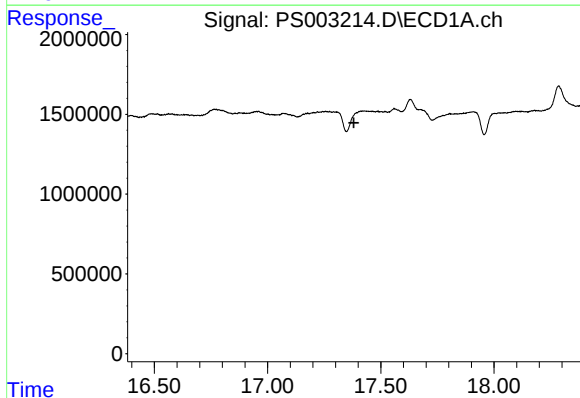

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

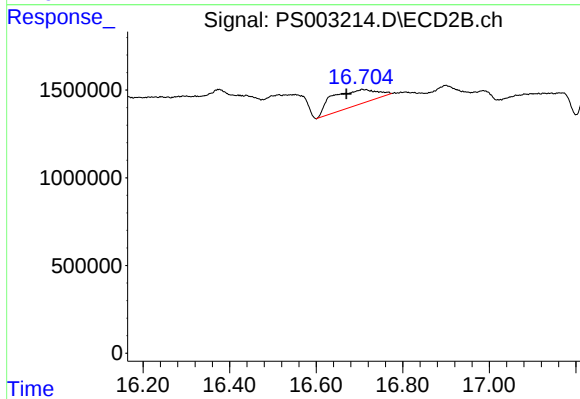

#16 DCPA

R.T.: 16.707 min
Delta R.T.: 0.037 min
Response: 6489467
Conc: 2.10 ng/ml