

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021519\
 Data File : PS003217.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Feb 2019 00:27
 Operator : EI\SJ
 Sample : K1358-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TR-04-021419

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 16 01:38:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.283	10.783	175.1E6	203.8E6	461.281	476.694
Target Compounds							
6) T	MCP	11.966	0.000	15281828	0	12.755	N.D. #
12) T	2,4,5-T	0.000	14.400	0	732885	N.D.	0.383 #
14) T	DINOSEB	0.000	15.512	0	5023087	N.D.	2.865 #
15) T	Picloram	16.813	16.705	5585045	10868002	1.765	3.615 #
16) T	DCPA	0.000	16.642	0	2692991	N.D.	0.869 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021519\
Data File : PS003217.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Feb 2019 00:27
Operator : EI\SJ
Sample : K1358-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TR-04-021419

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 16 01:38:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

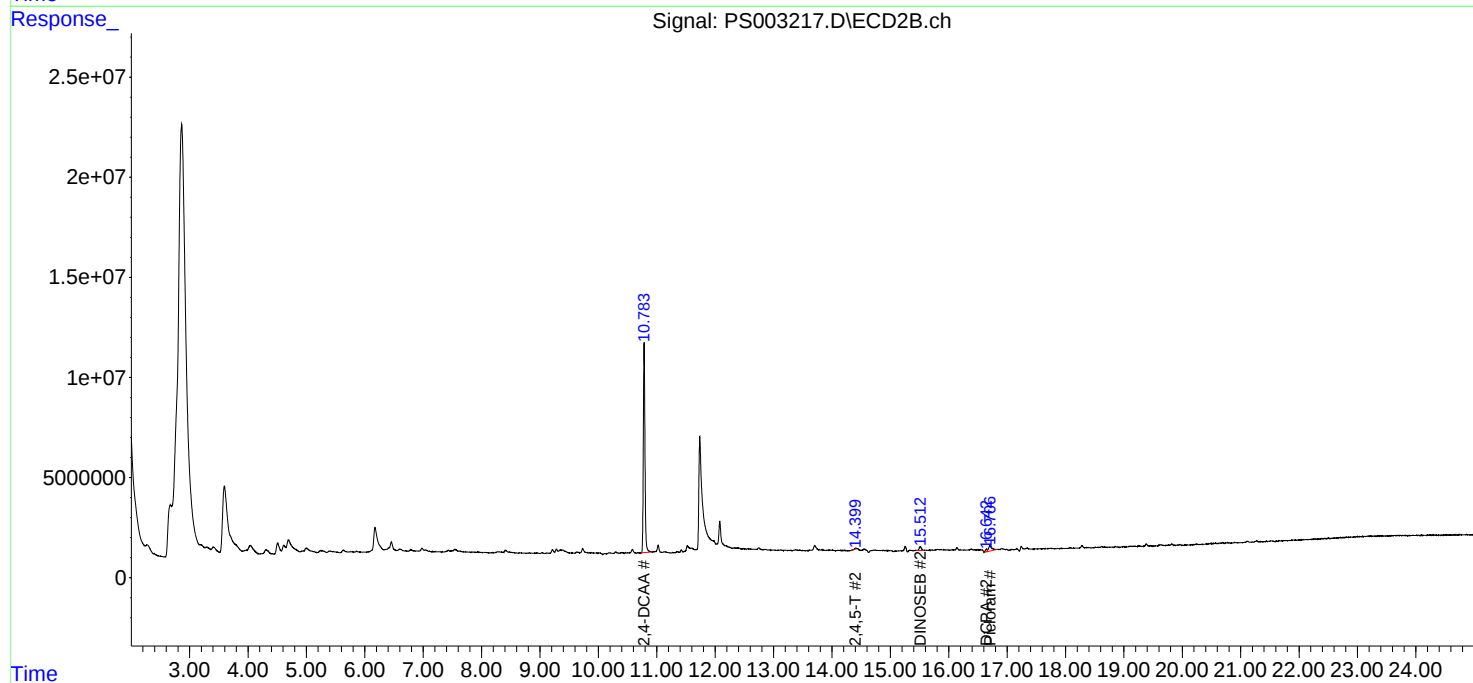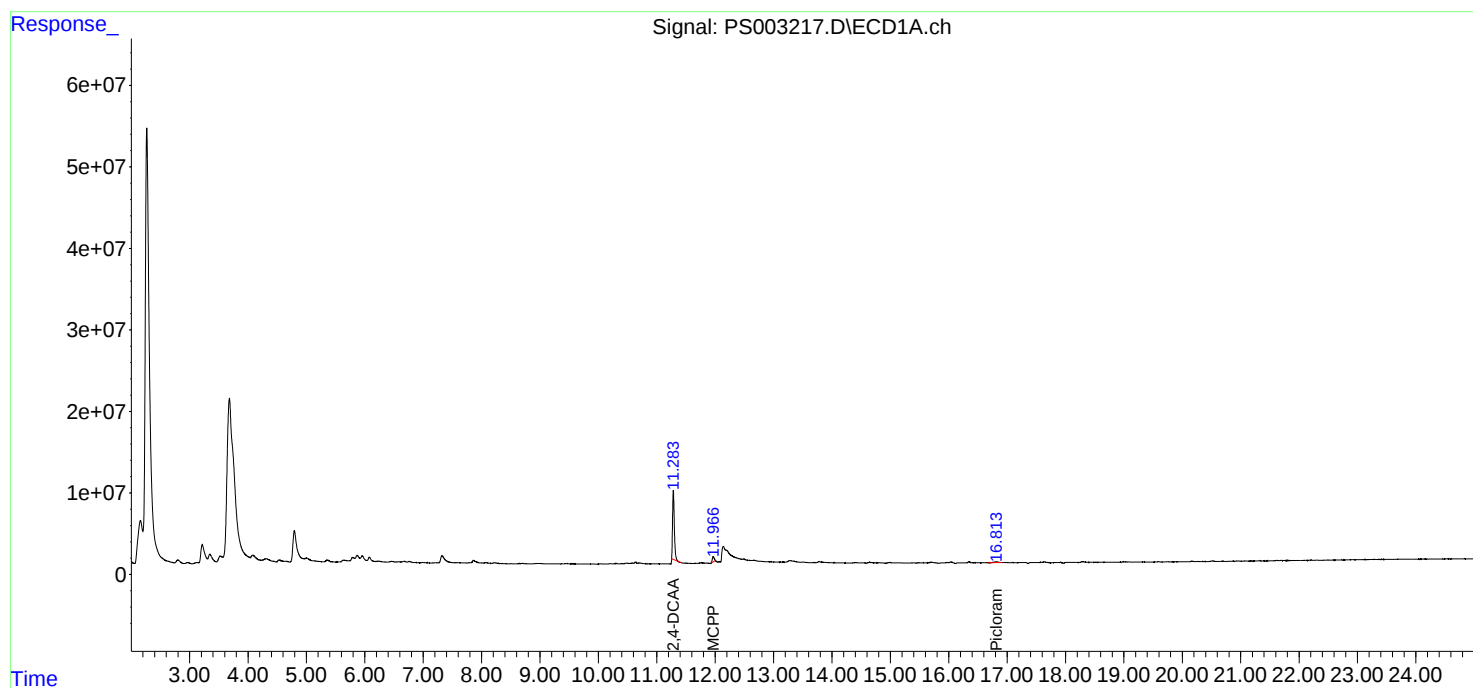


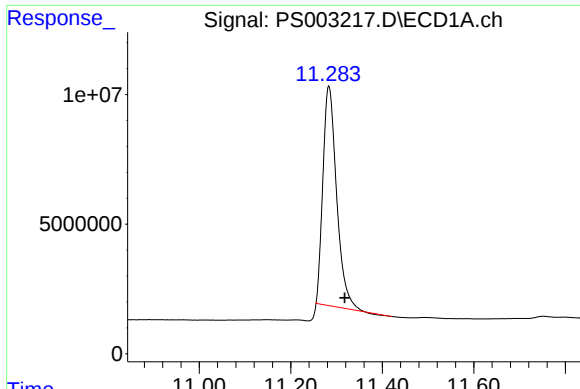

#4 2,4-DCAA


R.T.: 11.283 min
Delta R.T.: -0.034 min
Response: 175121033
Conc: 461.28 ng/ml

Instrument :
ECD_S
ClientSampleId :
TR-04-021419

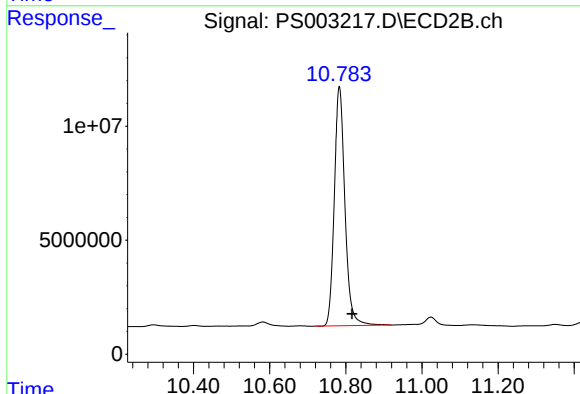


#4 2,4-DCAA

R.T.: 10.783 min
Delta R.T.: -0.033 min
Response: 203808601
Conc: 476.69 ng/ml

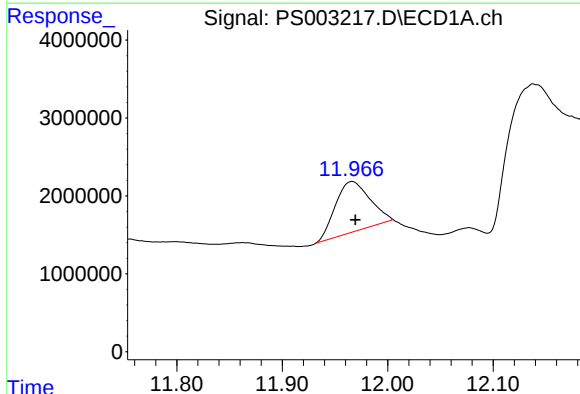


#6 MCP

R.T.: 11.966 min
Delta R.T.: -0.003 min
Response: 15281828
Conc: 12.75 ug/ml

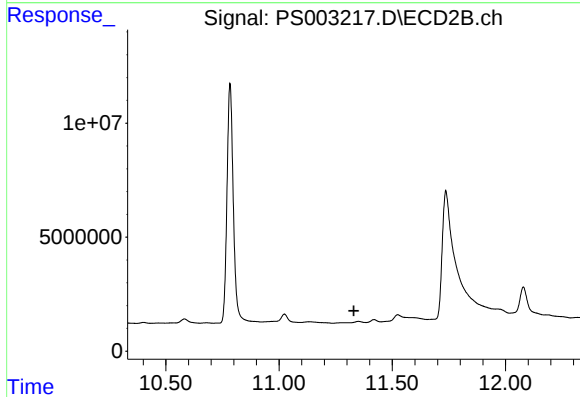

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.330 min
Response: 0
Conc: N.D.

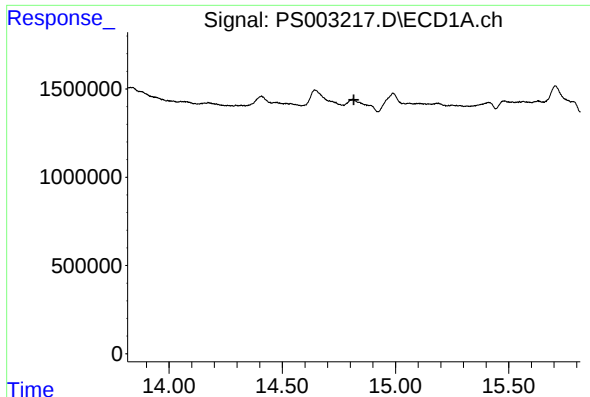

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.817 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TR-04-021419

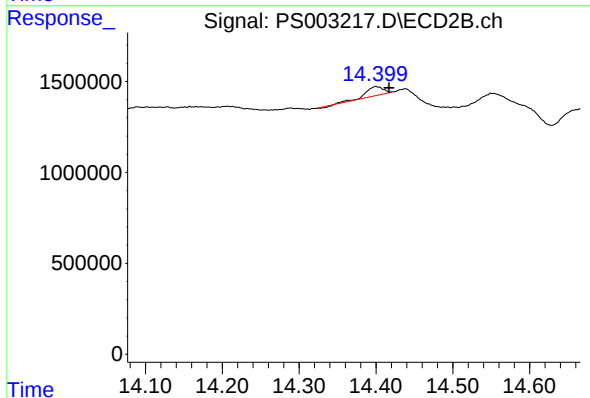


#12 2,4,5-T

R.T.: 14.400 min
Delta R.T.: -0.017 min
Response: 732885
Conc: 0.38 ng/ml

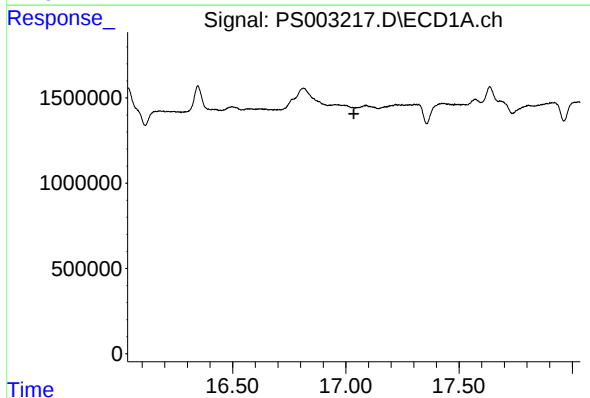


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 17.035 min
Response: 0
Conc: N.D.

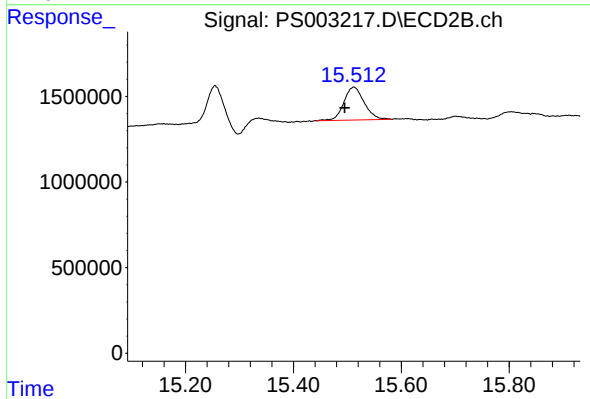

#14 DINOSEB


R.T.: 15.512 min
Delta R.T.: 0.017 min
Response: 5023087
Conc: 2.87 ng/ml

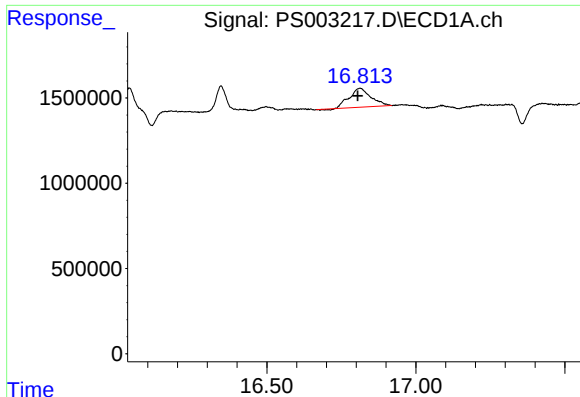

#15 Picloram


R.T.: 16.813 min
Delta R.T.: 0.007 min
Response: 5585045
Conc: 1.77 ng/ml

Instrument :
ECD_S
ClientSampleId :
TR-04-021419

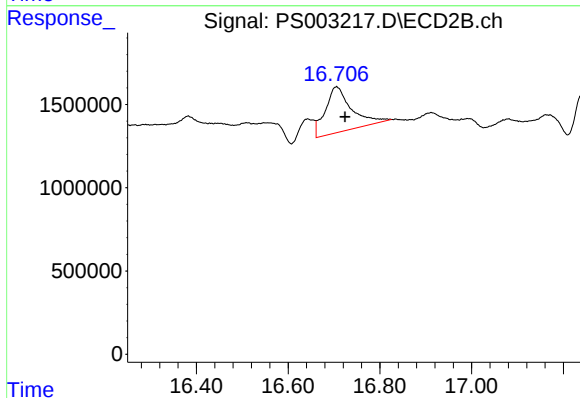


#15 Picloram

R.T.: 16.705 min
Delta R.T.: -0.019 min
Response: 10868002
Conc: 3.61 ng/ml

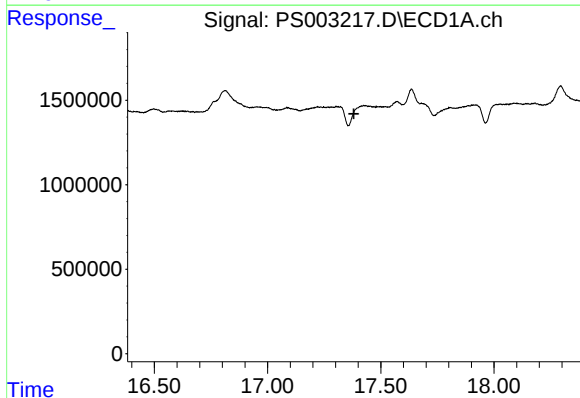

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

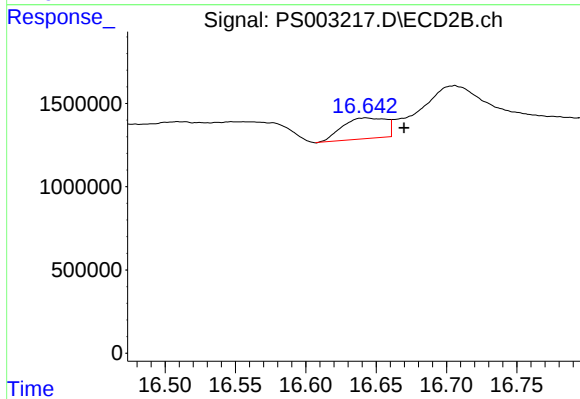

#16 DCPA

R.T.: 16.642 min
Delta R.T.: -0.027 min
Response: 2692991
Conc: 0.87 ng/ml