

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS021519\  
 Data File : PS003219.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 16 Feb 2019 01:29  
 Operator : EI\SJ  
 Sample : K1484-08  
 Misc :  
 ALS Vial : 16 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 M-2-D

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Feb 16 02:38:14 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS012819.M  
 Quant Title : 8080.M  
 QLast Update : Tue Jan 29 06:11:45 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound     | RT#1   | RT#2   | Resp#1   | Resp#2  | ng/ml   | ng/ml   |
|-----------------------------|--------------|--------|--------|----------|---------|---------|---------|
| -----                       |              |        |        |          |         |         |         |
| System Monitoring Compounds |              |        |        |          |         |         |         |
| 4) S                        | 2,4-DCAA     | 11.285 | 10.784 | 113.5E6  | 144.7E6 | 298.916 | 338.414 |
| Target Compounds            |              |        |        |          |         |         |         |
| 2) T                        | 3,5-DICHL... | 0.000  | 9.033  | 0        | 1570162 | N.D.    | 2.786 # |
| 5) T                        | DICAMBA      | 11.693 | 0.000  | 4303738  | 0       | 2.685   | N.D. #  |
| 6) T                        | MCP          | 11.968 | 0.000  | 11337894 | 0       | 9.463   | N.D. #  |
| 11) T                       | 2,4,5-TP ... | 14.410 | 0.000  | 4357566  | 0       | 1.730   | N.D. #  |
| 15) T                       | Picloram     | 0.000  | 16.717 | 0        | 5991591 | N.D.    | 1.993 # |
| 16) T                       | DCPA         | 0.000  | 16.717 | 0        | 5991591 | N.D.    | 1.934 # |
| -----                       |              |        |        |          |         |         |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS021519\  
Data File : PS003219.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 16 Feb 2019 01:29  
Operator : EI\SJ  
Sample : K1484-08  
Misc :  
ALS Vial : 16 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :  
M-2-D

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Feb 16 02:38:14 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS012819.M  
Quant Title : 8080.M  
QLast Update : Tue Jan 29 06:11:45 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

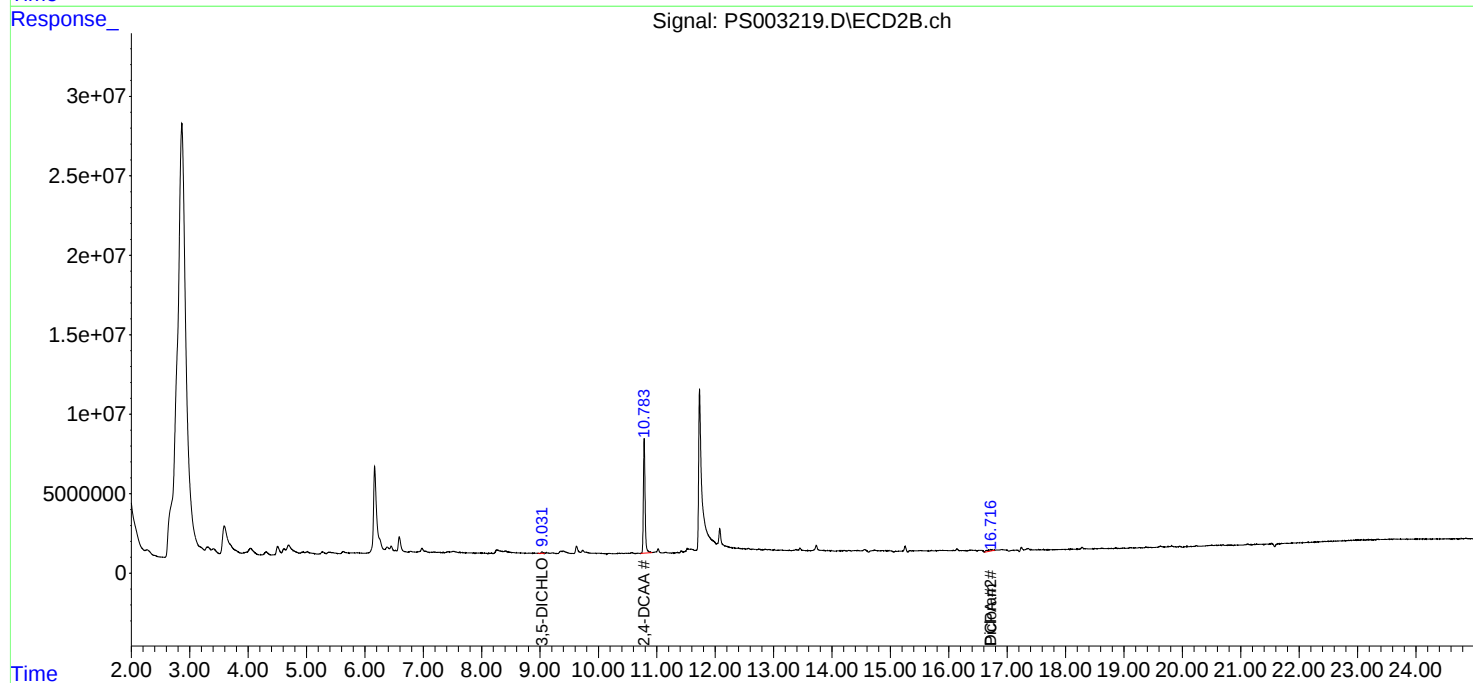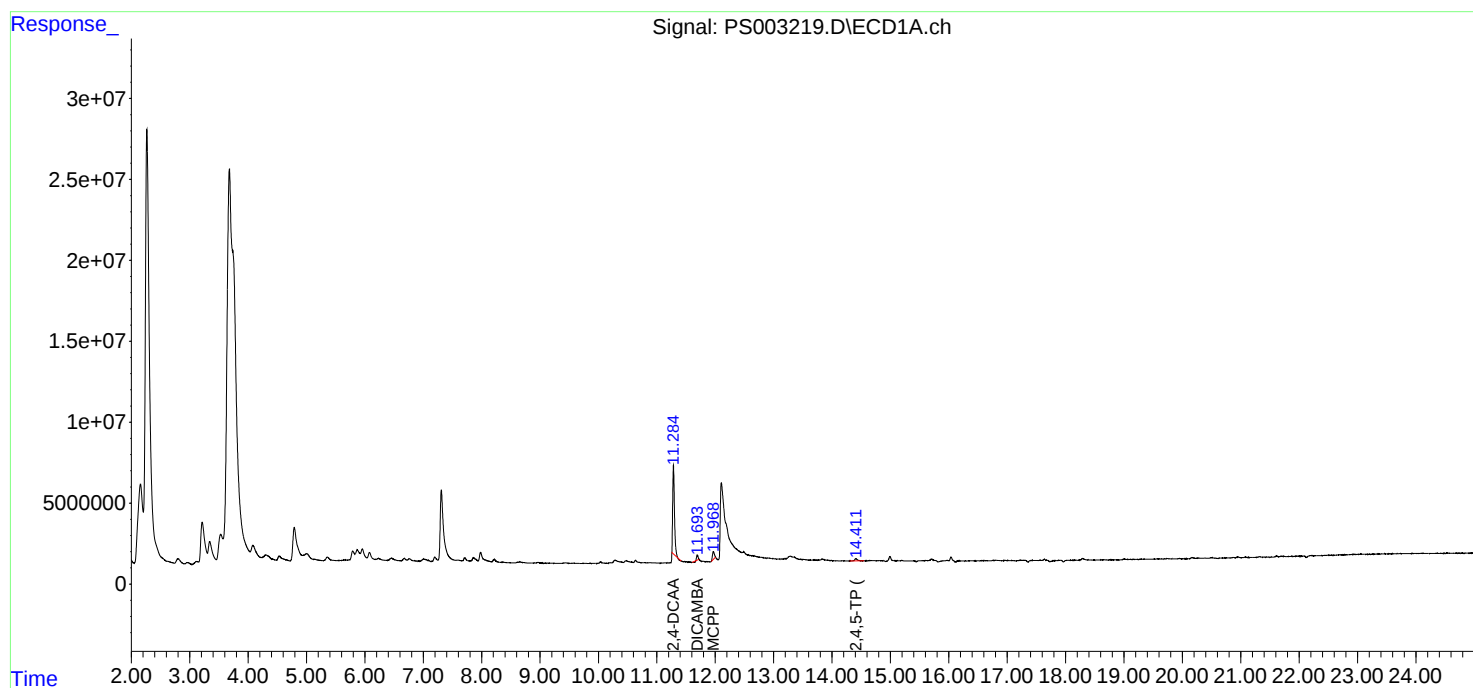


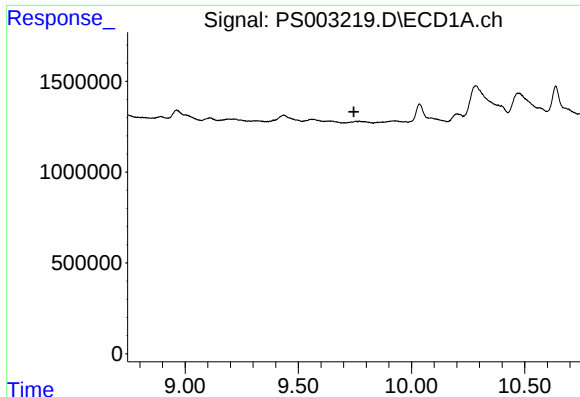

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min  
Exp R.T.: 9.745 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :  
M-2-D

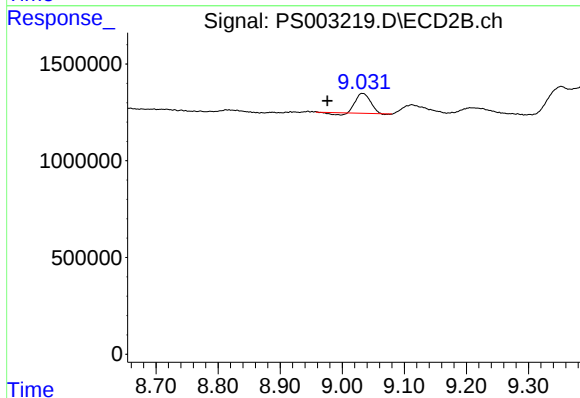


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.033 min  
Delta R.T.: 0.056 min  
Response: 1570162  
Conc: 2.79 ng/ml

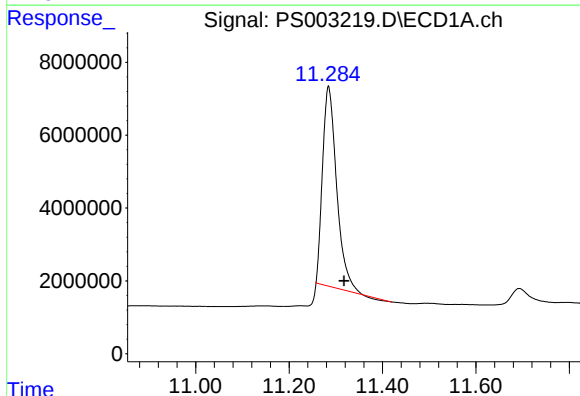


#4 2,4-DCAA

R.T.: 11.285 min  
Delta R.T.: -0.033 min  
Response: 113480786  
Conc: 298.92 ng/ml

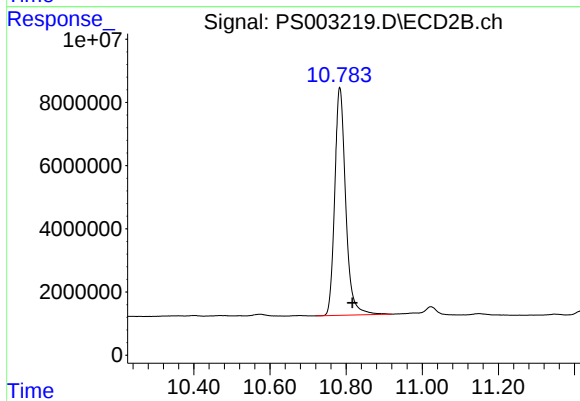

#4 2,4-DCAA


R.T.: 10.784 min  
Delta R.T.: -0.033 min  
Response: 144687650  
Conc: 338.41 ng/ml

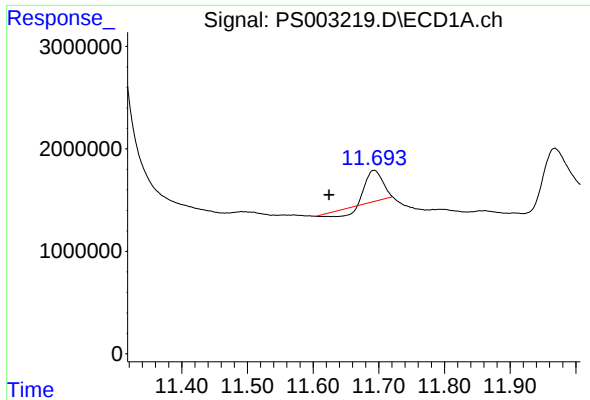

#5 DICAMBA


R.T.: 11.693 min  
Delta R.T.: 0.069 min  
Response: 4303738  
Conc: 2.68 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :  
M-2-D

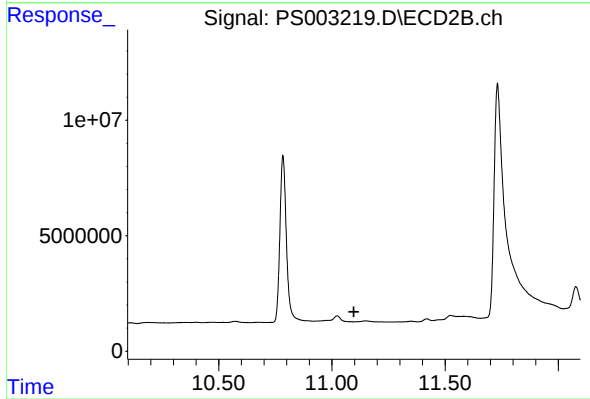


#5 DICAMBA

R.T.: 0.000 min  
Exp R.T. : 11.097 min  
Response: 0  
Conc: N.D.

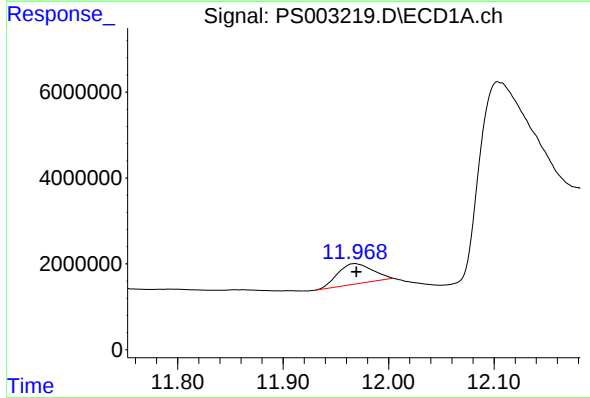


#6 MCPP

R.T.: 11.968 min  
Delta R.T.: -0.001 min  
Response: 11337894  
Conc: 9.46 ug/ml

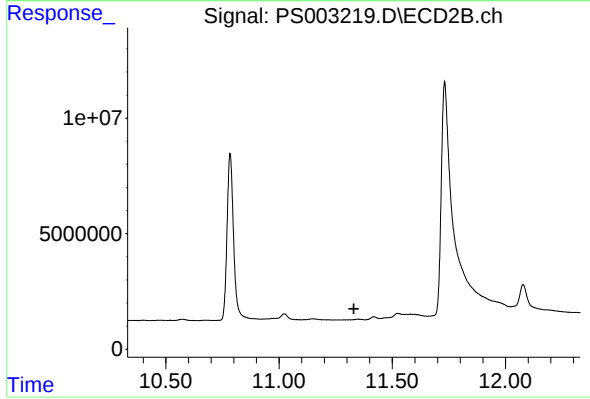

#6 MCPP


R.T.: 0.000 min  
Exp R.T. : 11.330 min  
Response: 0  
Conc: N.D.

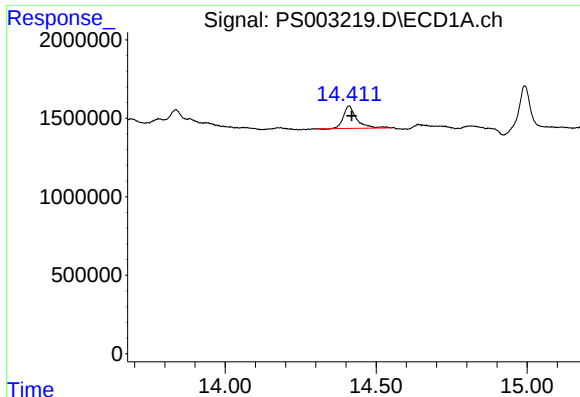

#11 2,4,5-TP (SILVEX)


R.T.: 14.410 min  
Delta R.T.: -0.009 min  
Response: 4357566  
Conc: 1.73 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :  
M-2-D

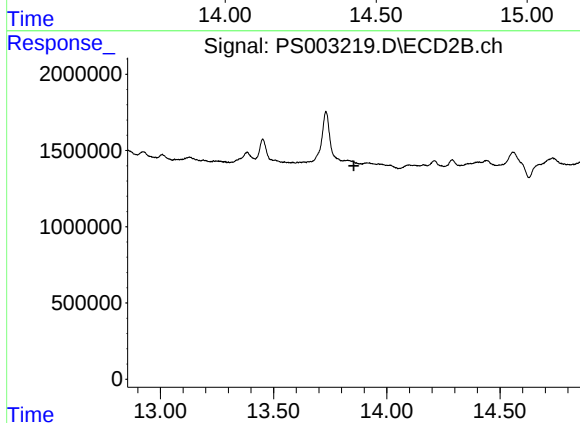


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min  
Exp R.T. : 13.854 min  
Response: 0  
Conc: N.D.

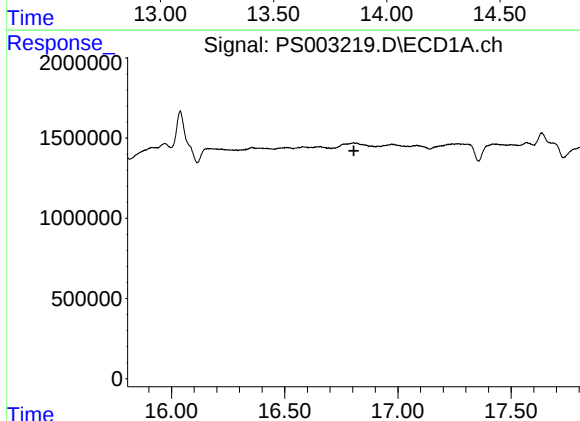


#15 Picloram

R.T.: 0.000 min  
Exp R.T. : 16.806 min  
Response: 0  
Conc: N.D.

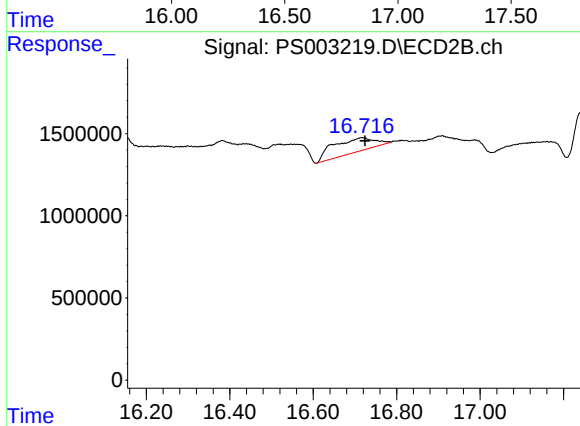

#15 Picloram


R.T.: 16.717 min  
Delta R.T.: -0.007 min  
Response: 5991591  
Conc: 1.99 ng/ml

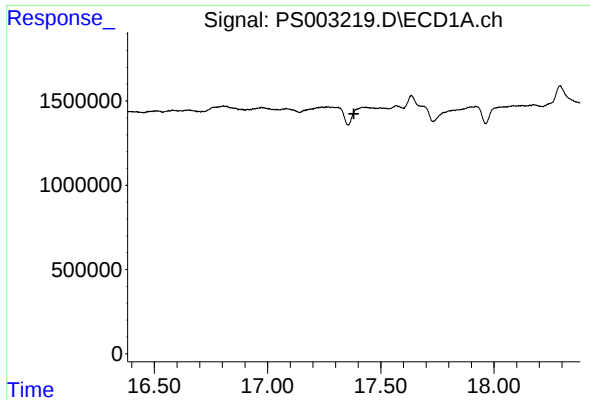

#16 DCPA

R.T.: 0.000 min  
Exp R.T.: 17.382 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :  
M-2-D

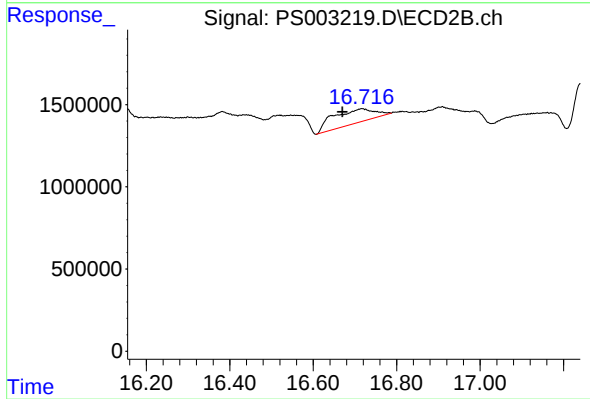

#16 DCPA

R.T.: 16.717 min  
Delta R.T.: 0.047 min  
Response: 5991591  
Conc: 1.93 ng/ml