

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021519\
 Data File : PS003221.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Feb 2019 02:31
 Operator : EI\SJ
 Sample : K1484-16
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 M-3-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 16 04:03:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.281	10.780	138.4E6	231.8E6	364.675	542.071 #
Target Compounds							
6) T	MCP	11.969	0.000	6231944	0	5.201	N.D. #
14) T	DINOSEB	0.000	15.503	0	8136221	N.D.	4.641 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021519\
Data File : PS003221.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Feb 2019 02:31
Operator : EI\SJ
Sample : K1484-16
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
M-3-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 16 04:03:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

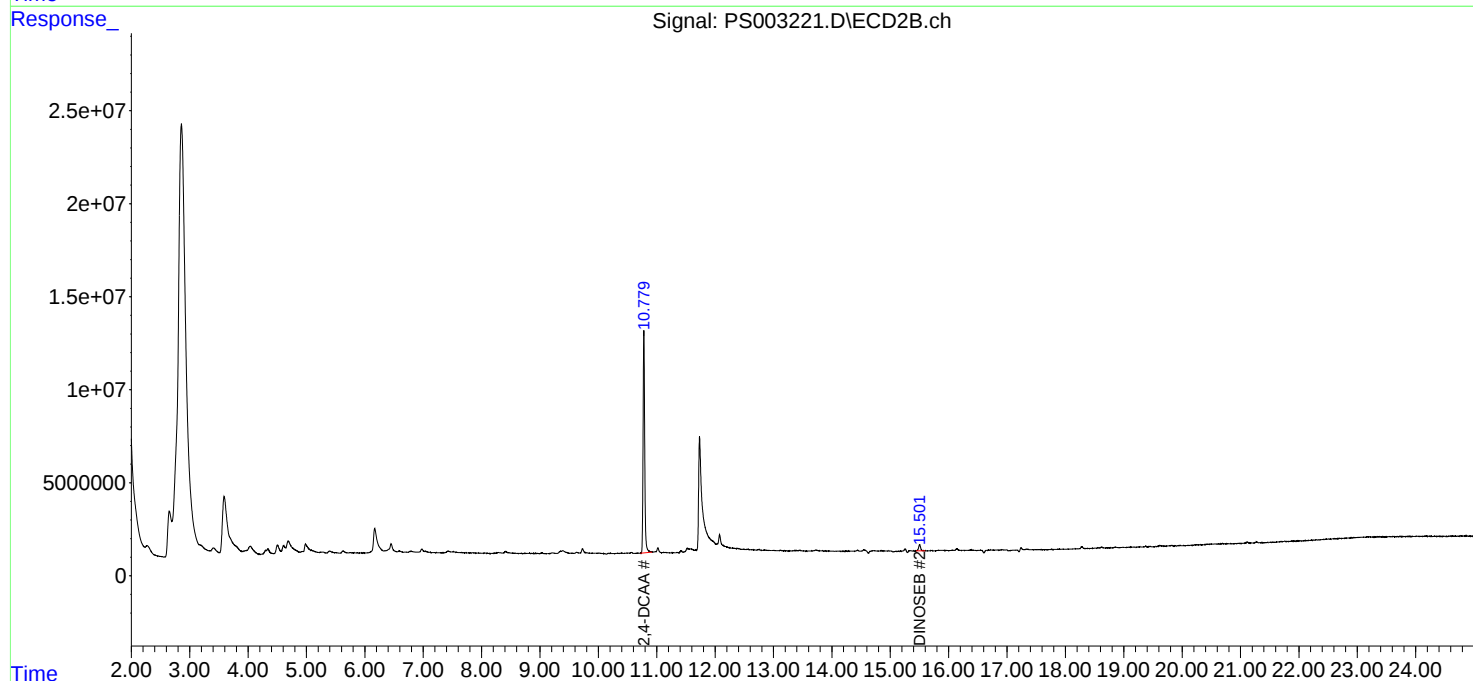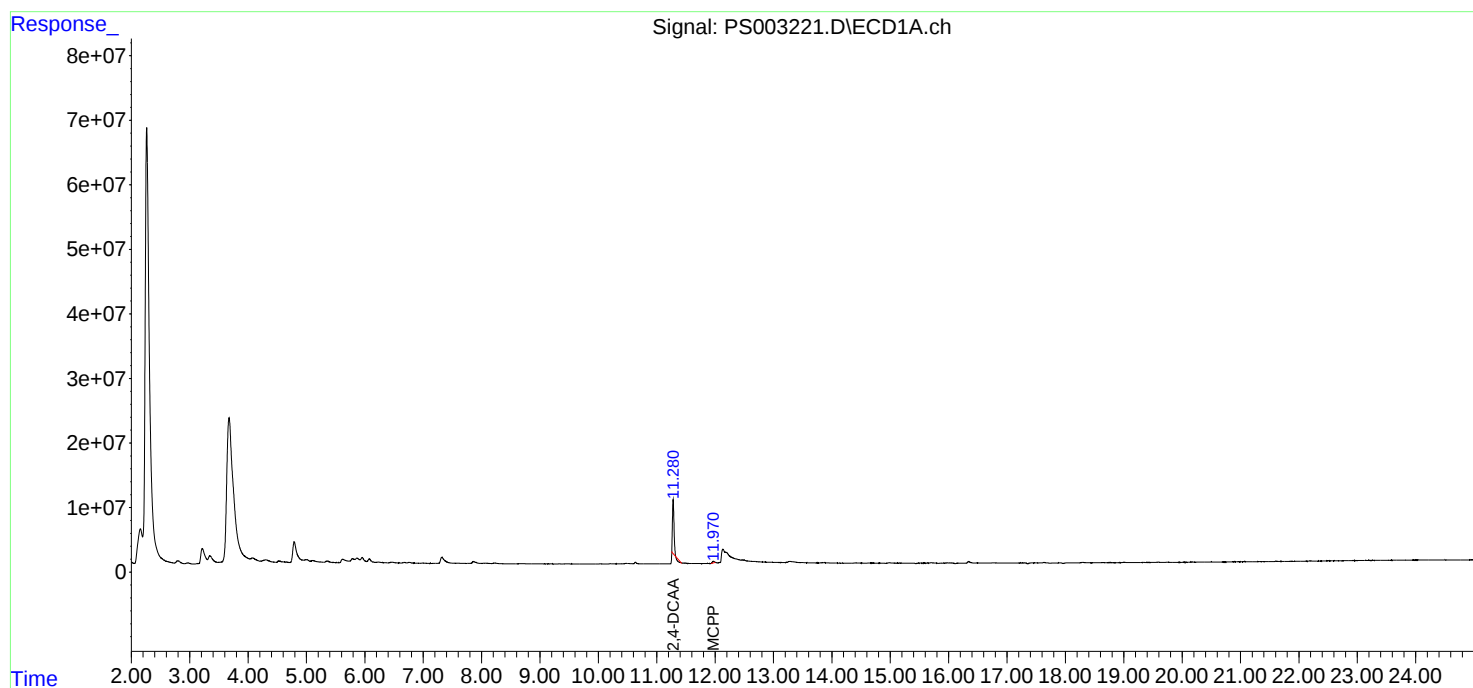


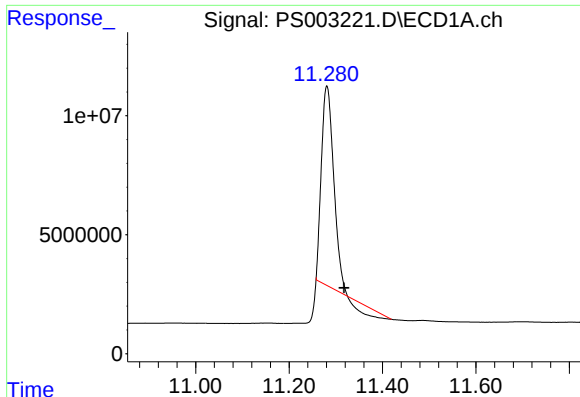

#4 2,4-DCAA


R.T.: 11.281 min
Delta R.T.: -0.037 min
Response: 138445558
Conc: 364.68 ng/ml

Instrument :
ECD_S
ClientSampleId :
M-3-D

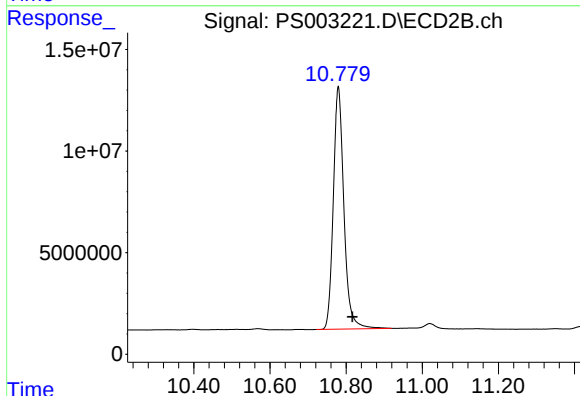


#4 2,4-DCAA

R.T.: 10.780 min
Delta R.T.: -0.037 min
Response: 231760284
Conc: 542.07 ng/ml

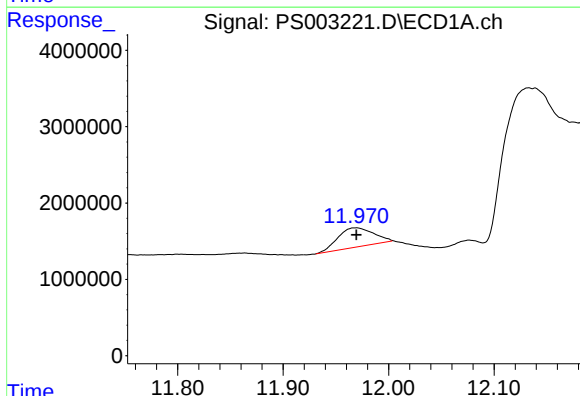


#6 MCP

R.T.: 11.969 min
Delta R.T.: 0.000 min
Response: 6231944
Conc: 5.20 ug/ml

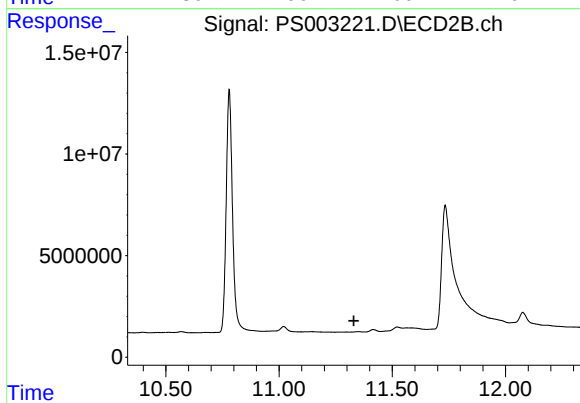

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.330 min
Response: 0
Conc: N.D.

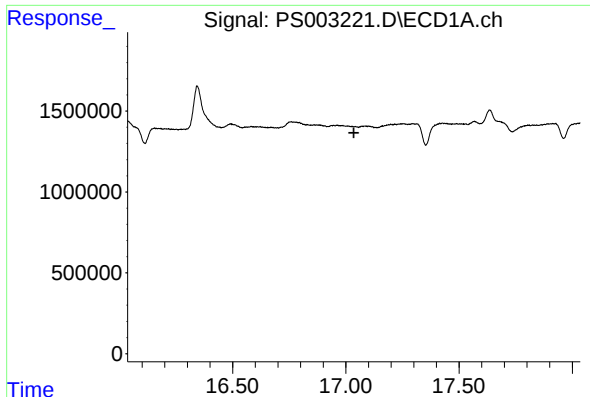

#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 17.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
M-3-D

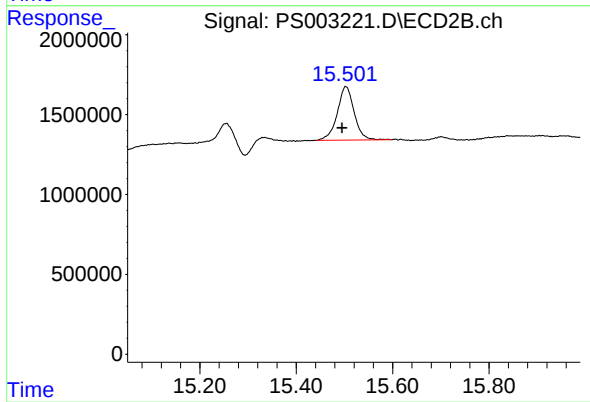

#14 DINOSEB

R.T.: 15.503 min
Delta R.T.: 0.008 min
Response: 8136221
Conc: 4.64 ng/ml