

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021522\
 Data File : PS018333.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Feb 2022 09:42
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 15 23:49:35 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020822.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 09 15:57:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
5) T	DICAMBA	7.218	0.000	10983310	0	1.739	N.D. #
8) T	DICHLORPROP	7.909	0.000	4066151	0	2.577	N.D. #
9) T	2,4-D	8.160	0.000	13836395	0	7.514	N.D. #
10) T	Pentachlo...	8.425	8.100	23930889	9652583	1.132	1.118
11) T	2,4,5-TP ...	8.979	8.466	17457772	7594805	2.043	2.050
12) T	2,4,5-T	9.275	8.856	44783801	11608196	5.061	3.278 #
13) T	2,4-DB	9.840	0.000	12025026	0	6.832	N.D. #
14) T	DINOSEB	10.946	0.000	21839064	0	3.271	N.D. #
15) T	Picloram	10.808	10.663	179.9E6	83976574	15.743	16.755
16) T	DCPA	11.214	10.585	23175770	9156720	2.103	2.012



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021522\
Data File : PS018333.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Feb 2022 09:42
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 15 23:49:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020822.M
Quant Title : 8080.M
QLast Update : Wed Feb 09 15:57:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

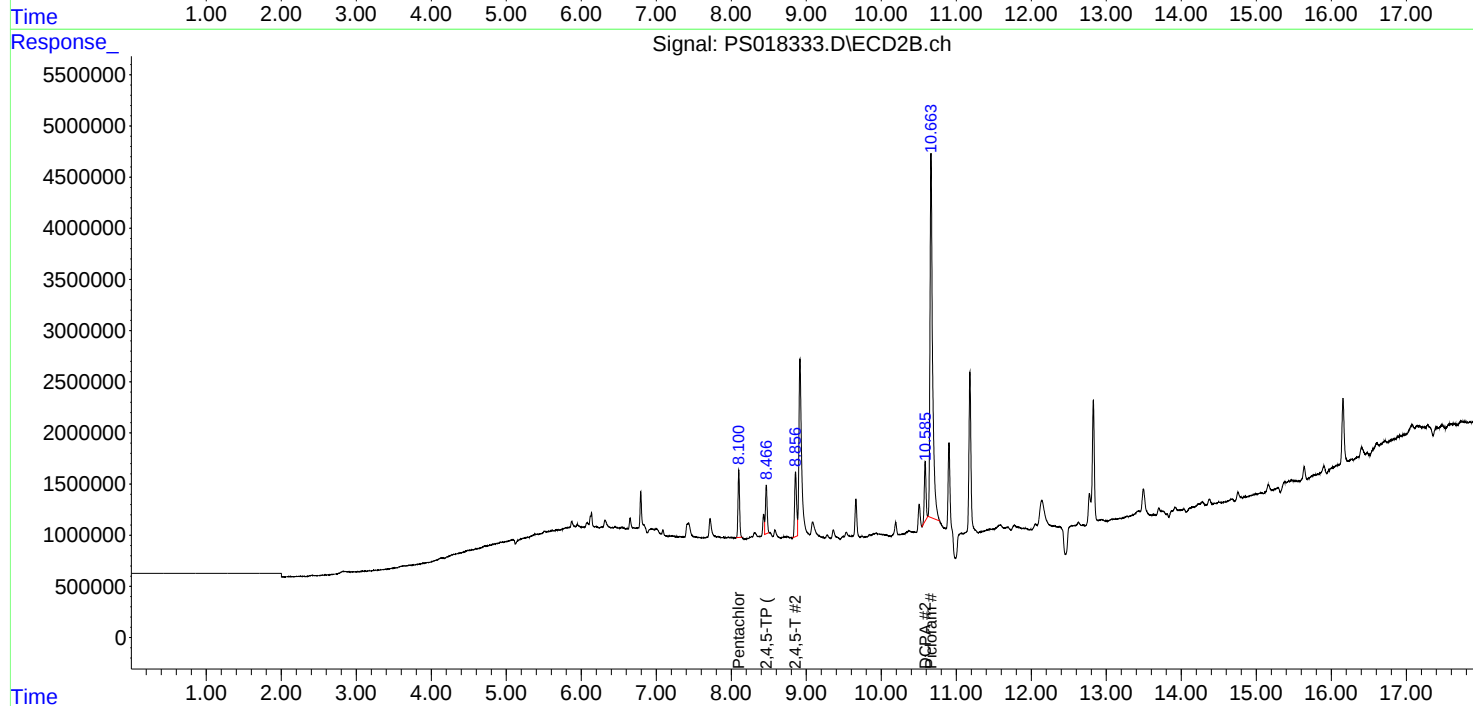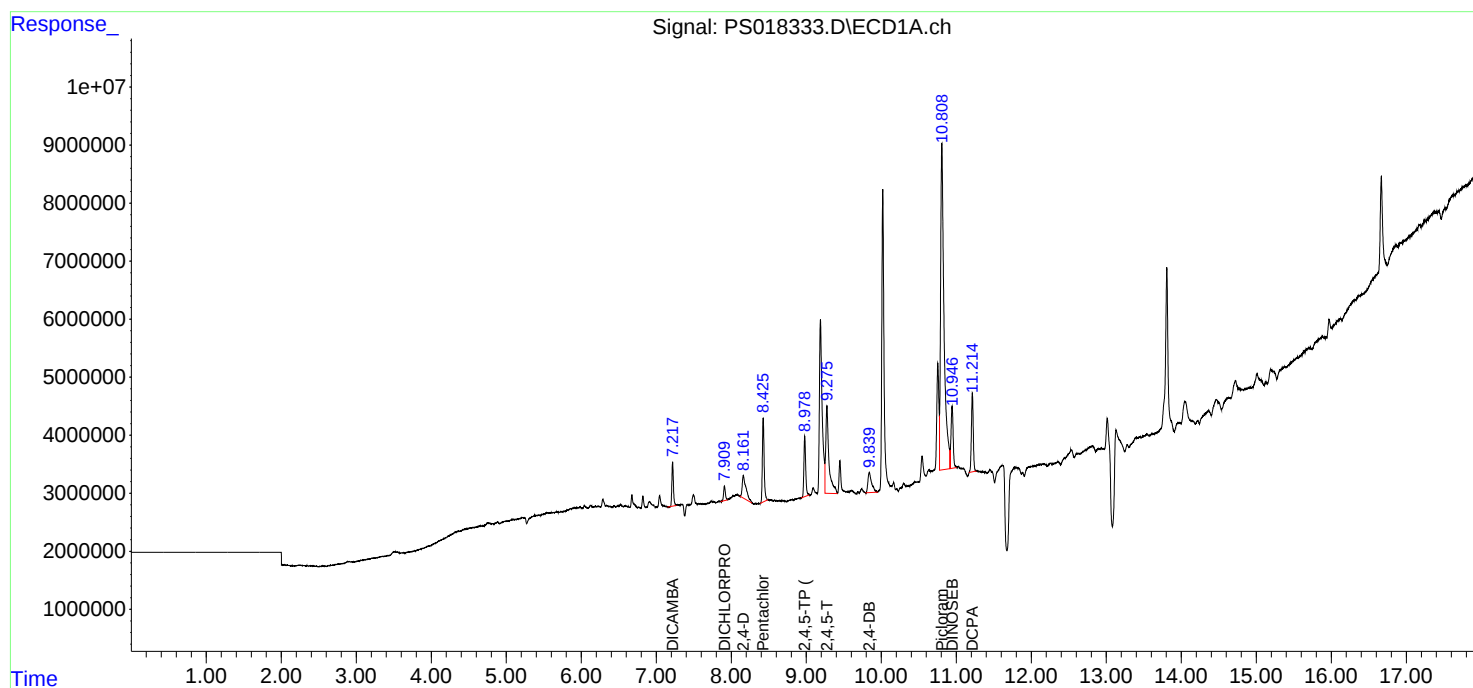


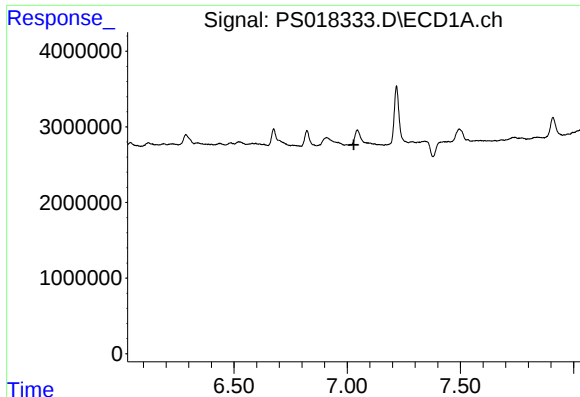

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.029 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

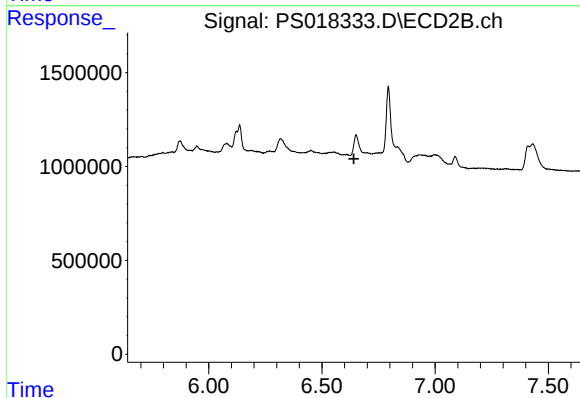


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.641 min
Response: 0
Conc: N.D.

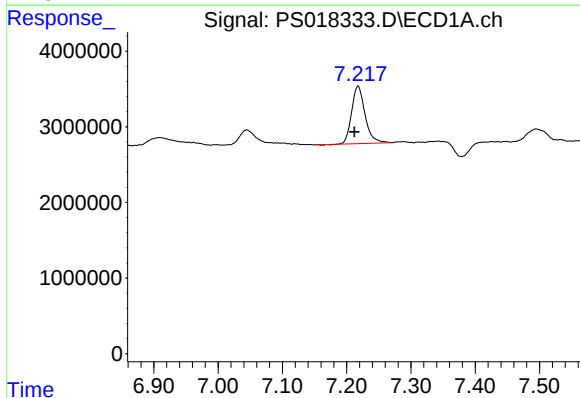


#5 DICAMBA

R.T.: 7.218 min
Delta R.T.: 0.006 min
Response: 10983310
Conc: 1.74 ng/ml

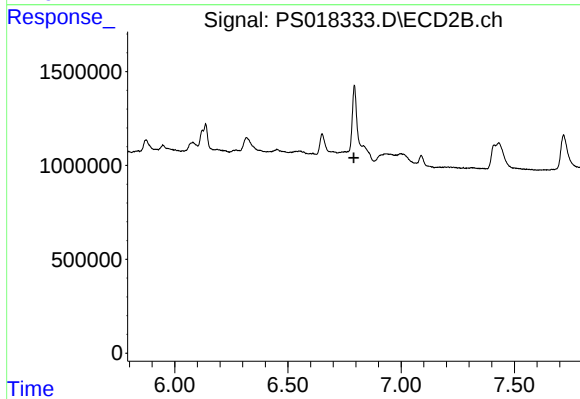

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.791 min
Response: 0
Conc: N.D.

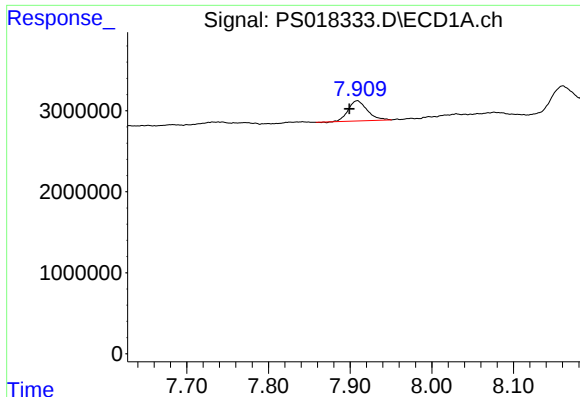

#8 DICHLORPROP


R.T.: 7.909 min
Delta R.T.: 0.010 min
Response: 4066151
Conc: 2.58 ng/ml

Instrument :
ECD_S
ClientSampleId :

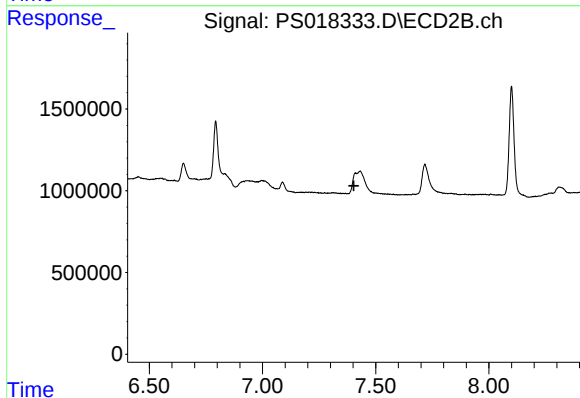


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.404 min
Response: 0
Conc: N.D.

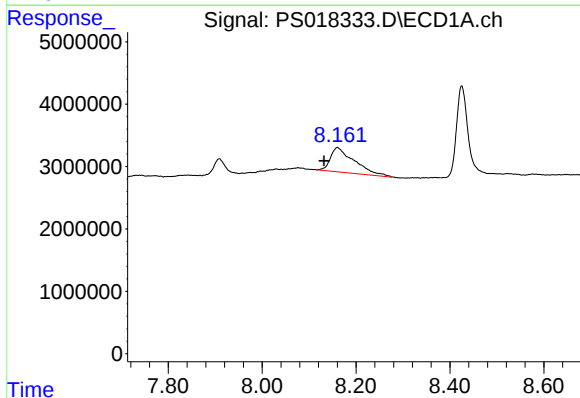


#9 2,4-D

R.T.: 8.160 min
Delta R.T.: 0.028 min
Response: 13836395
Conc: 7.51 ng/ml

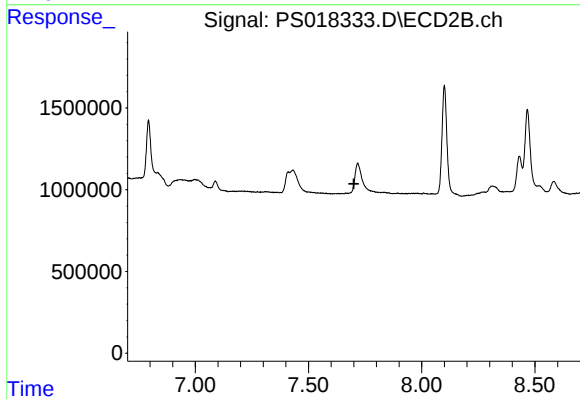

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.701 min
Response: 0
Conc: N.D.

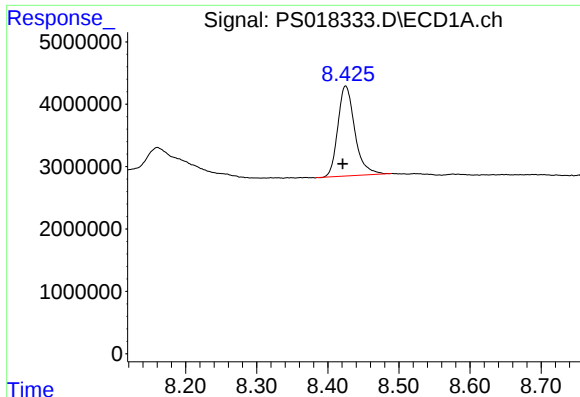

#10 Pentachlorophenol


R.T.: 8.425 min
Delta R.T.: 0.004 min
Response: 23930889
Conc: 1.13 ng/ml

Instrument :
ECD_S
ClientSampleId :

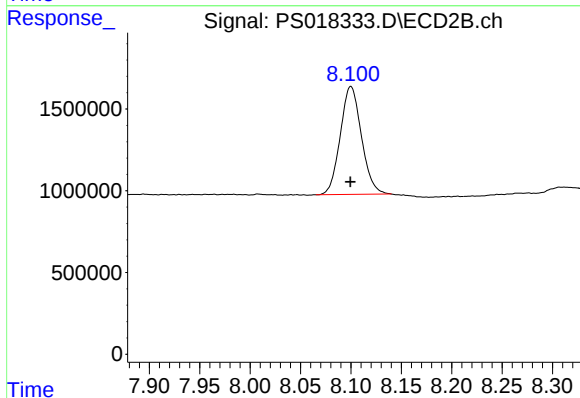


#10 Pentachlorophenol

R.T.: 8.100 min
Delta R.T.: 0.000 min
Response: 9652583
Conc: 1.12 ng/ml

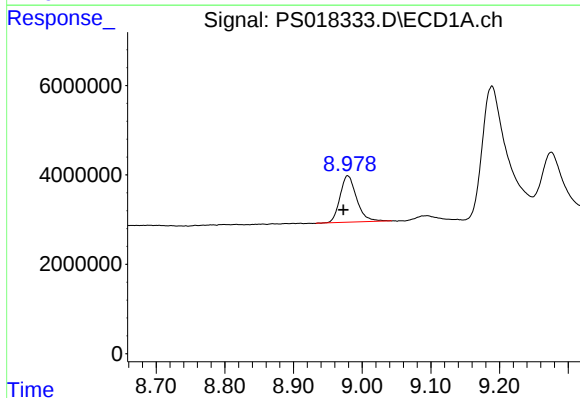


#11 2,4,5-TP (SILVEX)

R.T.: 8.979 min
Delta R.T.: 0.006 min
Response: 17457772
Conc: 2.04 ng/ml

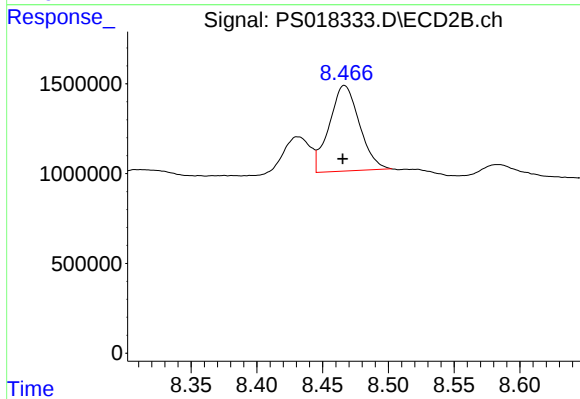

#11 2,4,5-TP (SILVEX)


R.T.: 8.466 min
Delta R.T.: 0.001 min
Response: 7594805
Conc: 2.05 ng/ml

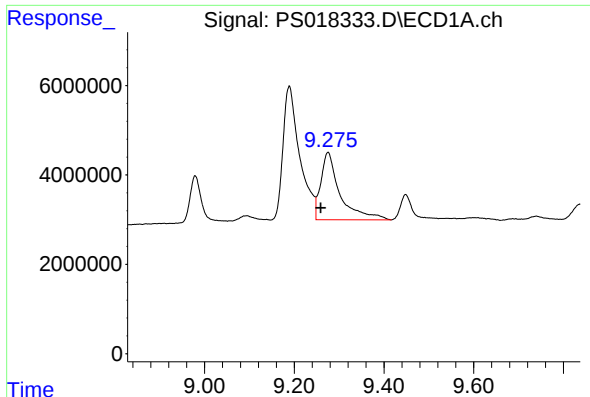

#12 2,4,5-T


R.T.: 9.275 min
Delta R.T.: 0.016 min
Response: 44783801
Conc: 5.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

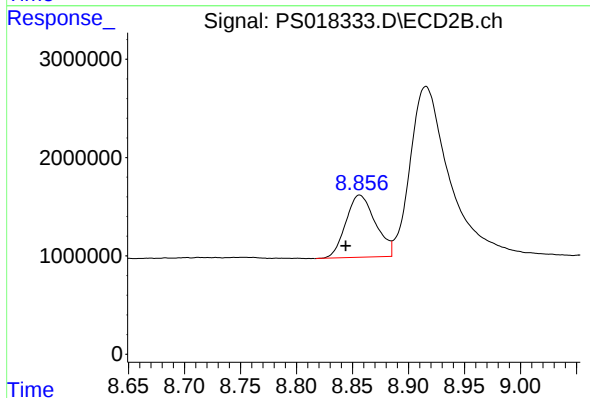


#12 2,4,5-T

R.T.: 8.856 min
Delta R.T.: 0.012 min
Response: 11608196
Conc: 3.28 ng/ml

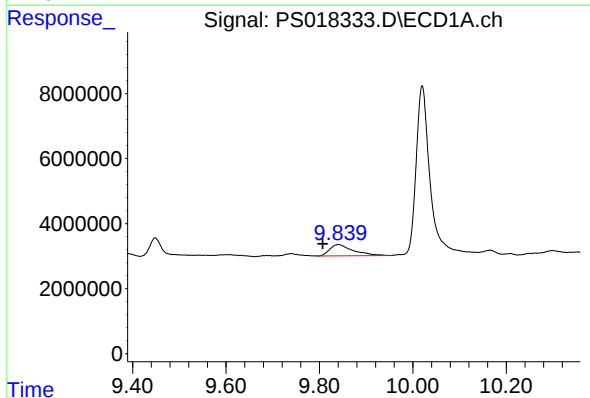


#13 2,4-DB

R.T.: 9.840 min
Delta R.T.: 0.033 min
Response: 12025026
Conc: 6.83 ng/ml

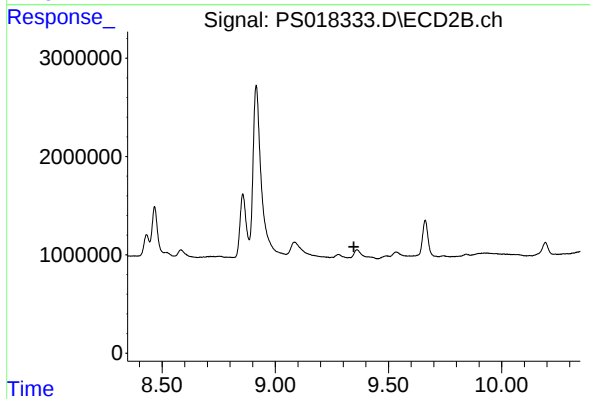

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.347 min
Response: 0
Conc: N.D.

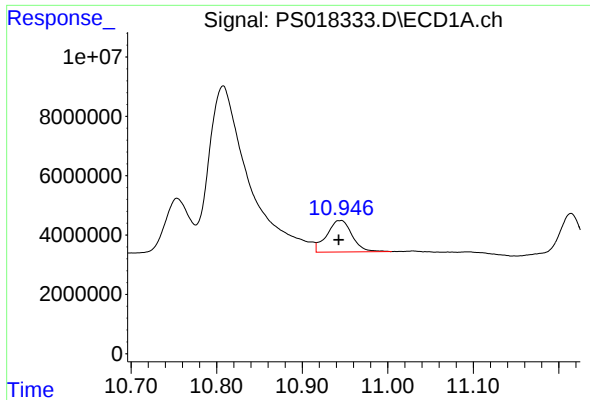

#14 DINOSEB


R.T.: 10.946 min
Delta R.T.: 0.003 min
Response: 21839064
Conc: 3.27 ng/ml

Instrument :
ECD_S
ClientSampleId :

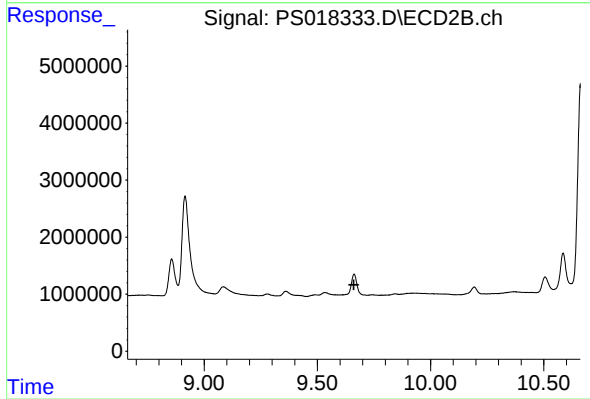


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.661 min
Response: 0
Conc: N.D.

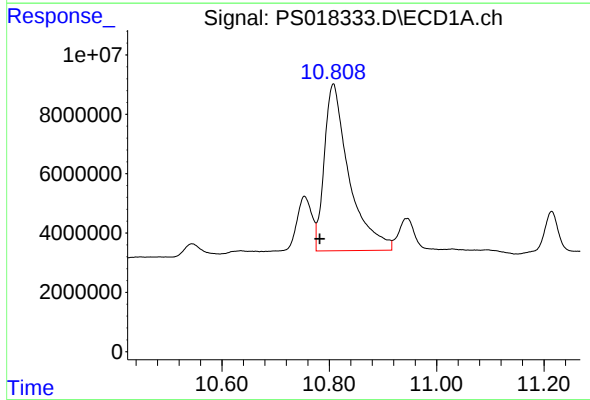


#15 Picloram

R.T.: 10.808 min
Delta R.T.: 0.025 min
Response: 179856912
Conc: 15.74 ng/ml

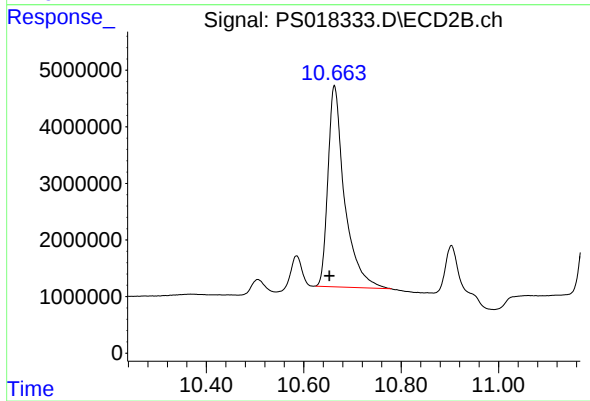

#15 Picloram


R.T.: 10.663 min
Delta R.T.: 0.010 min
Response: 83976574
Conc: 16.76 ng/ml

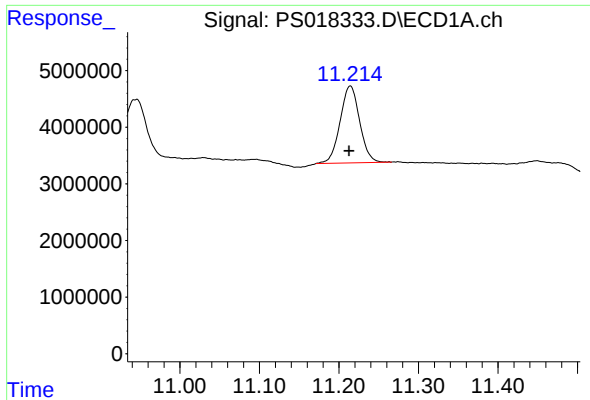

#16 DCPA

R.T.: 11.214 min
Delta R.T.: 0.002 min
Response: 23175770
Conc: 2.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

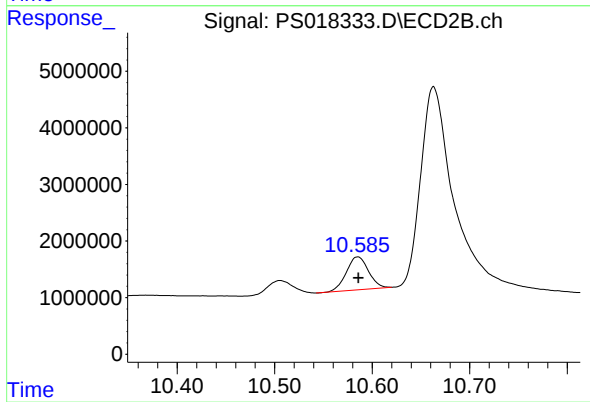

#16 DCPA

R.T.: 10.585 min
Delta R.T.: 0.000 min
Response: 9156720
Conc: 2.01 ng/ml