

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021522\
 Data File : PS018337.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Feb 2022 11:30
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 15 23:50:59 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020822.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 09 15:57:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.032	6.643	576.7E6	309.0E6	366.593	492.623 #
Target Compounds							
5) T	DICAMBA	7.218	0.000	8879065	0	1.406	N.D. #
10) T	Pentachlo...	8.428	8.112	16802205	7703664	<MDL	<MDL #
11) T	2,4,5-TP ...	8.989	8.484	14383376	15264053	1.683	4.121 #
12) T	2,4,5-T	9.222	8.889f	84957865	11284116	9.600	3.187 #
14) T	DINOSEB	10.941	0.000	70124988	0	10.502	N.D. #
15) T	Picloram	10.772	10.687	9663436	145.8E6	<MDL	29.089 #
16) T	DCPA	11.211	10.590	21200250	11688066	1.923	2.568 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021522\
Data File : PS018337.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Feb 2022 11:30
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 15 23:50:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020822.M
Quant Title : 8080.M
QLast Update : Wed Feb 09 15:57:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

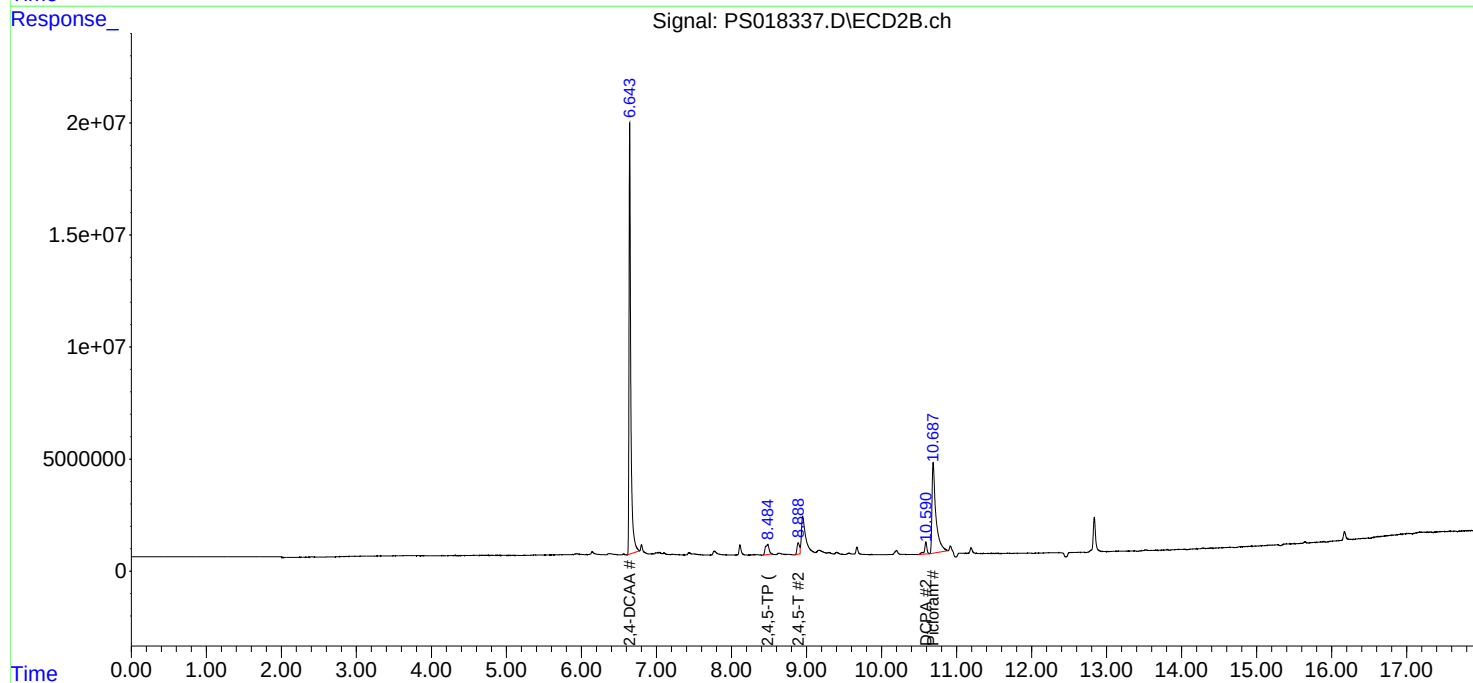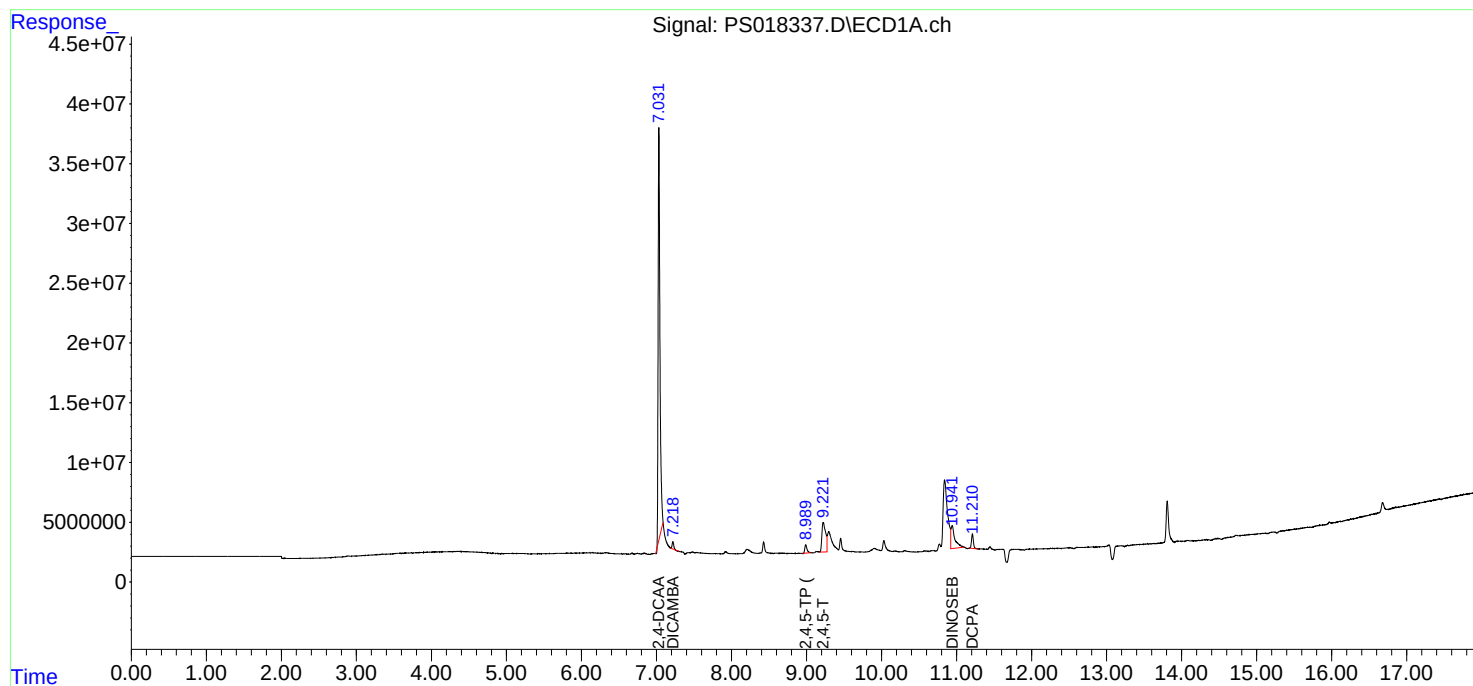


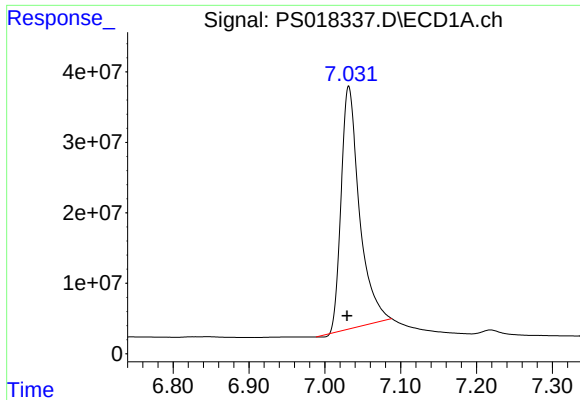

#4 2,4-DCAA


R.T.: 7.032 min
Delta R.T.: 0.002 min
Response: 576677724
Conc: 366.59 ng/ml

Instrument :
ECD_S
ClientSampleId :

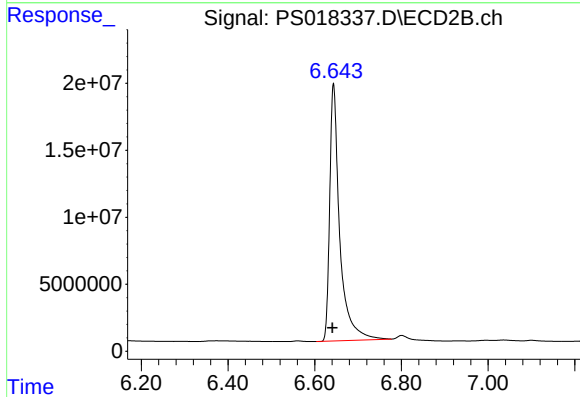


#4 2,4-DCAA

R.T.: 6.643 min
Delta R.T.: 0.002 min
Response: 308988454
Conc: 492.62 ng/ml

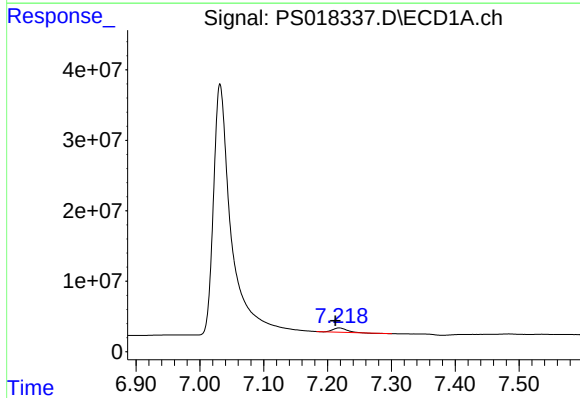


#5 DICAMBA

R.T.: 7.218 min
Delta R.T.: 0.006 min
Response: 8879065
Conc: 1.41 ng/ml

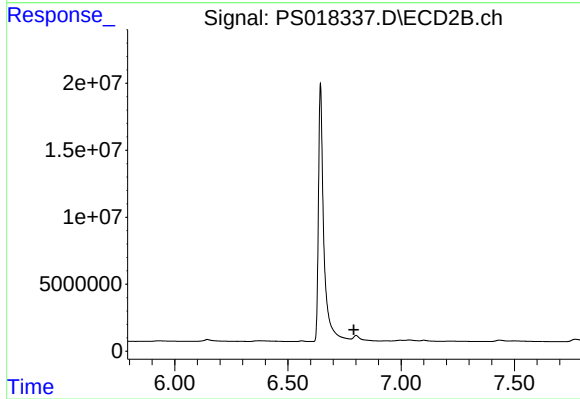

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 6.791 min
Response: 0
Conc: N.D.

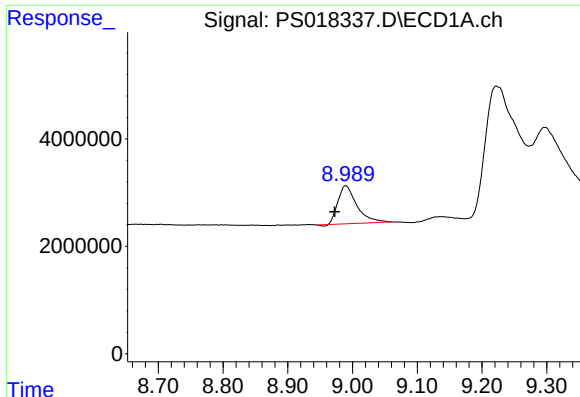

#11 2,4,5-TP (SILVEX)


R.T.: 8.989 min
Delta R.T.: 0.017 min
Response: 14383376
Conc: 1.68 ng/ml

Instrument :
ECD_S
ClientSampleId :

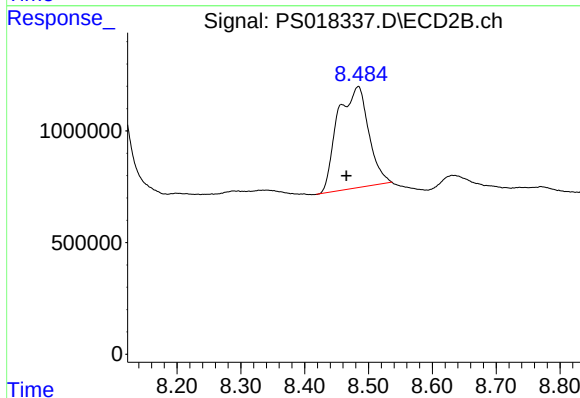


#11 2,4,5-TP (SILVEX)

R.T.: 8.484 min
Delta R.T.: 0.019 min
Response: 15264053
Conc: 4.12 ng/ml

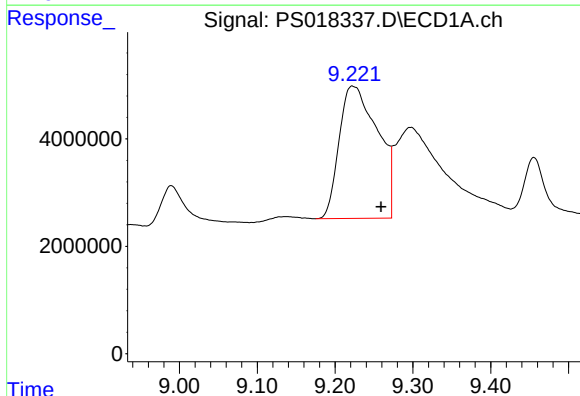


#12 2,4,5-T

R.T.: 9.222 min
Delta R.T.: -0.037 min
Response: 84957865
Conc: 9.60 ng/ml

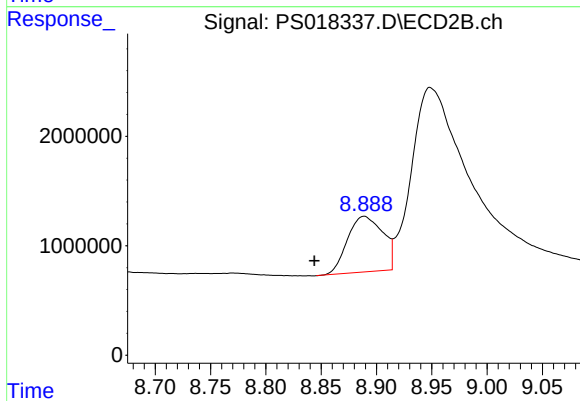

#12 2,4,5-T


R.T.: 8.889 min
Delta R.T.: 0.045 min
Response: 11284116
Conc: 3.19 ng/ml

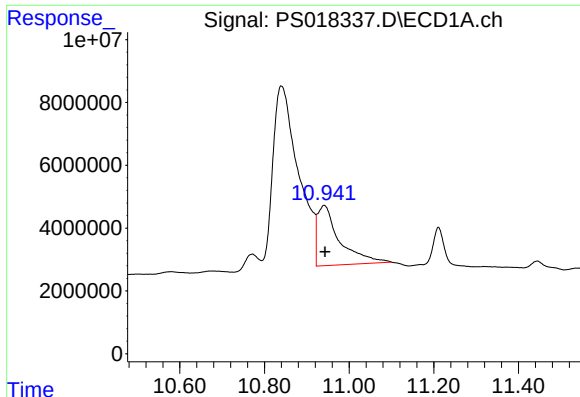

#14 DINOSEB


R.T.: 10.941 min
Delta R.T.: -0.002 min
Response: 70124988
Conc: 10.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

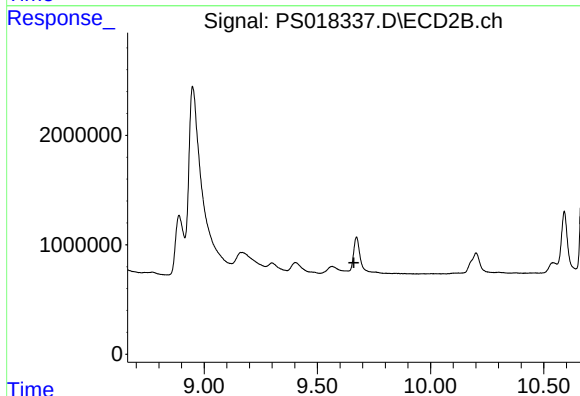


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.661 min
Response: 0
Conc: N.D.

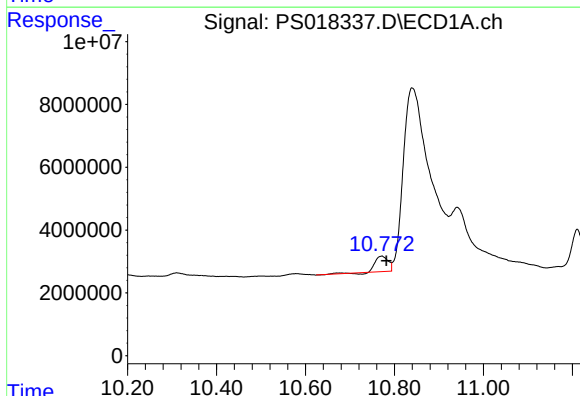


#15 Picloram

R.T.: 10.772 min
Delta R.T.: -0.011 min
Response: 9663436
Conc: N.D.

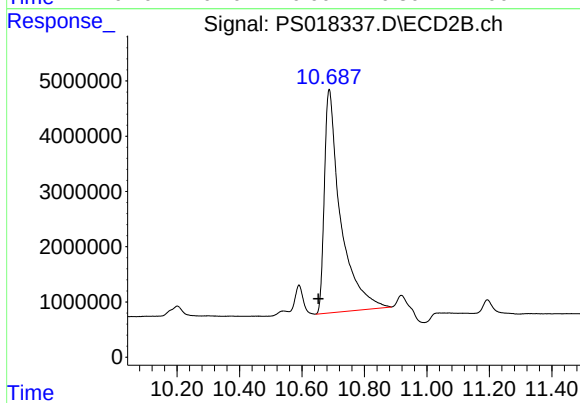

#15 Picloram


R.T.: 10.687 min
Delta R.T.: 0.035 min
Response: 145792910
Conc: 29.09 ng/ml

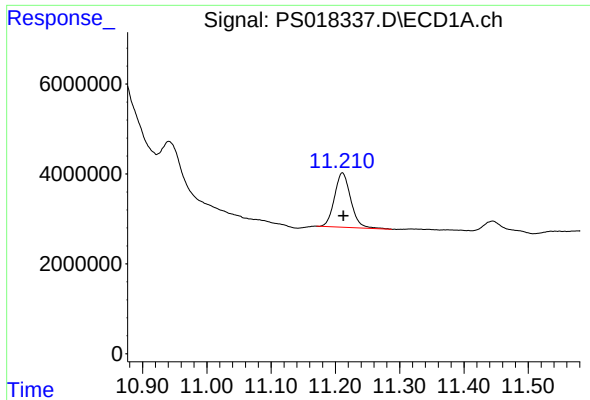

#16 DCPA

R.T.: 11.211 min
Delta R.T.: -0.002 min
Response: 21200250
Conc: 1.92 ng/ml

Instrument :
ECD_S
ClientSampleId :

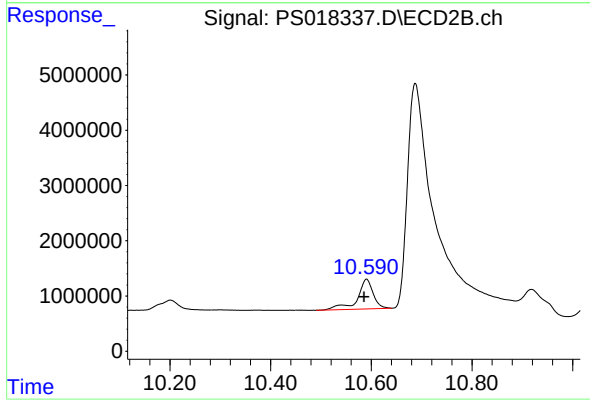

#16 DCPA

R.T.: 10.590 min
Delta R.T.: 0.005 min
Response: 11688066
Conc: 2.57 ng/ml