

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021522\
 Data File : PS018354.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Feb 2022 23:05
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 16 00:44:27 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020822.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 09 15:57:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.030	6.641	605.4E6	313.1E6	384.848	499.186 #
Target Compounds							
5) T	DICAMBA	7.215	0.000	9455614	0	1.497	N.D. #
9) T	2,4-D	8.196f	0.000	16230953	0	8.815	N.D. #
10) T	Pentachlo...	8.425	0.000	13123323	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.983	8.446	12649512	2250395	1.481	<MDL #
12) T	2,4,5-T	9.285	8.879	58949135	9896299	6.661	2.795 #
14) T	DINOSEB	10.940	0.000	56431802	0	8.451	N.D. #
15) T	Picloram	10.762	10.679	21602625	115.7E6	1.891	23.091 #
16) T	DCPA	11.209	10.588	22885227	8546304	2.076	1.878



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021522\
Data File : PS018354.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Feb 2022 23:05
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 16 00:44:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020822.M
Quant Title : 8080.M
QLast Update : Wed Feb 09 15:57:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

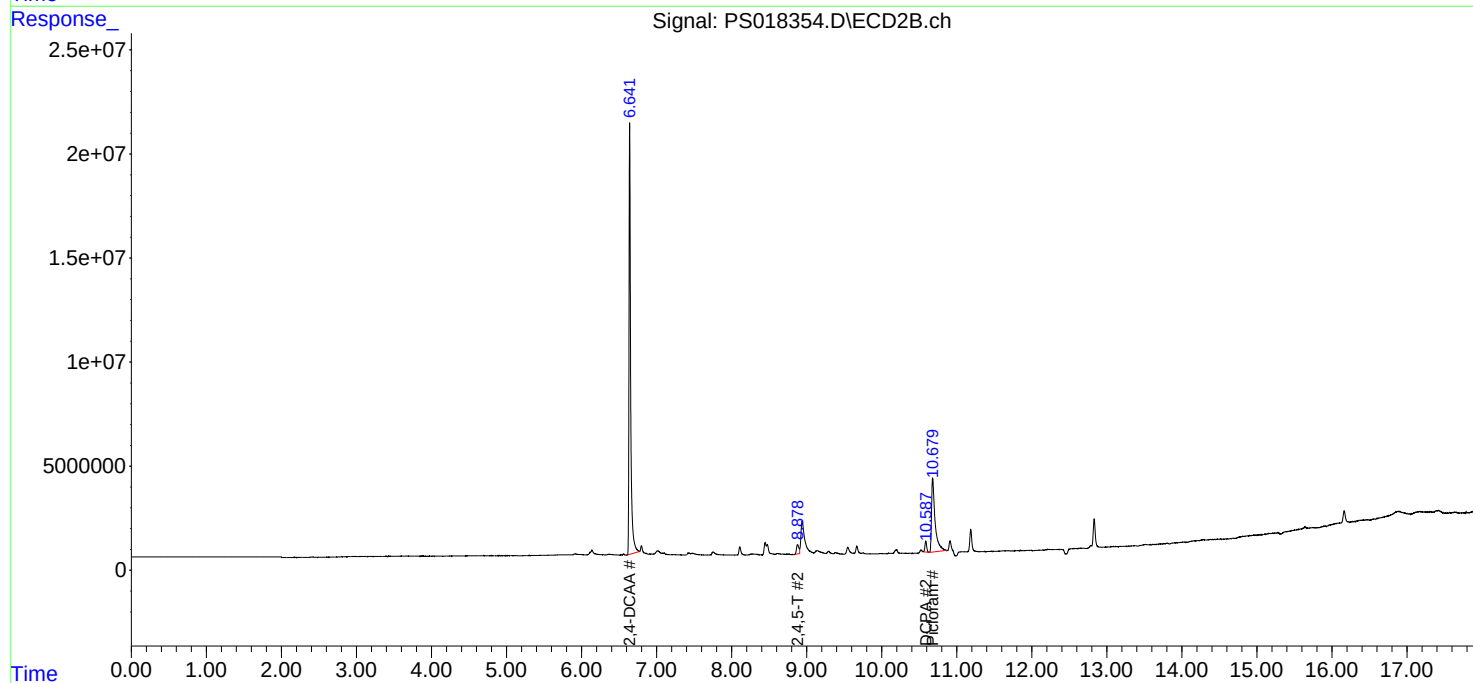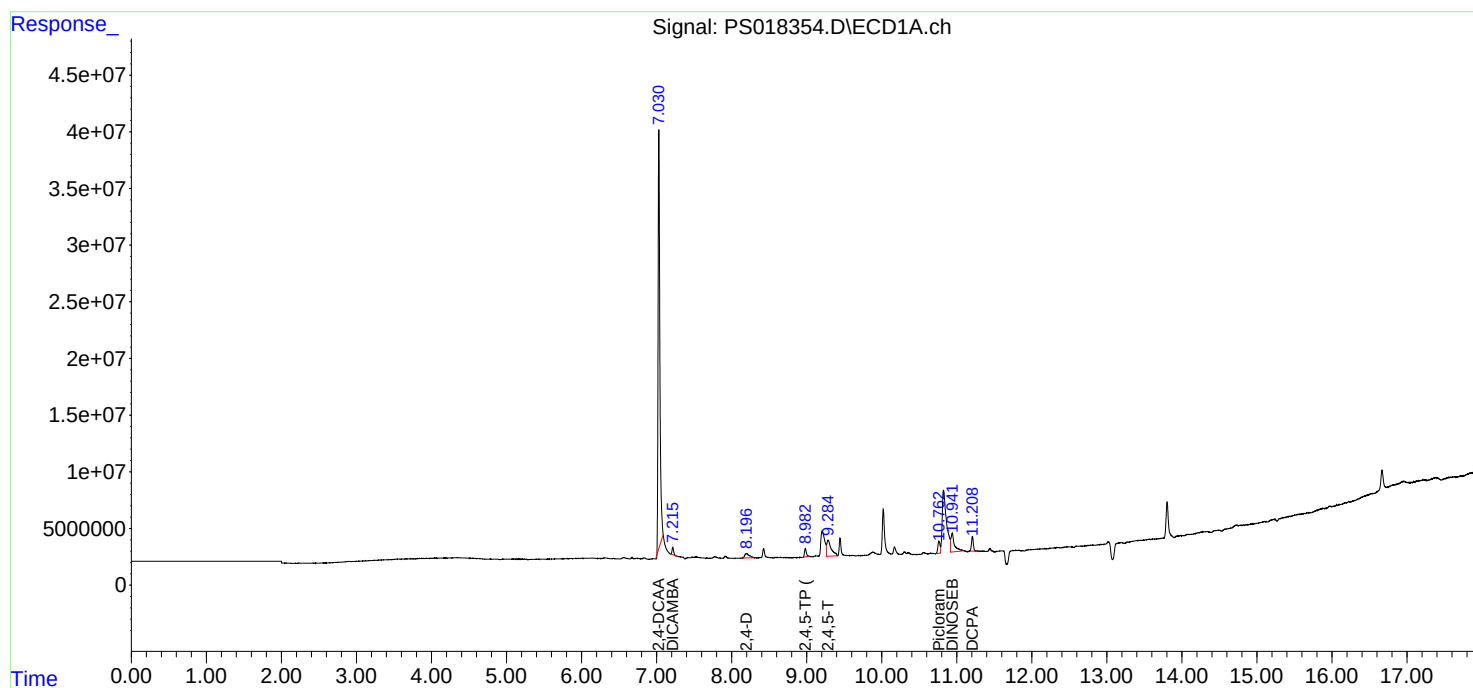


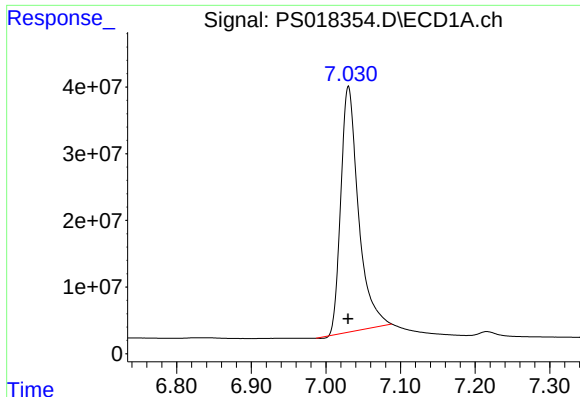

#4 2,4-DCAA


R.T.: 7.030 min
Delta R.T.: 0.000 min
Response: 605394022
Conc: 384.85 ng/ml

Instrument :
ECD_S
ClientSampleId :

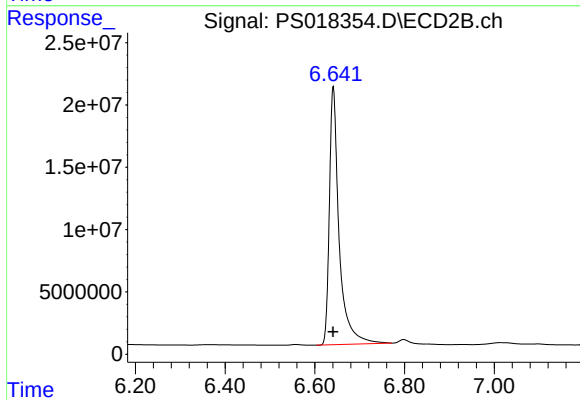


#4 2,4-DCAA

R.T.: 6.641 min
Delta R.T.: 0.000 min
Response: 313104873
Conc: 499.19 ng/ml

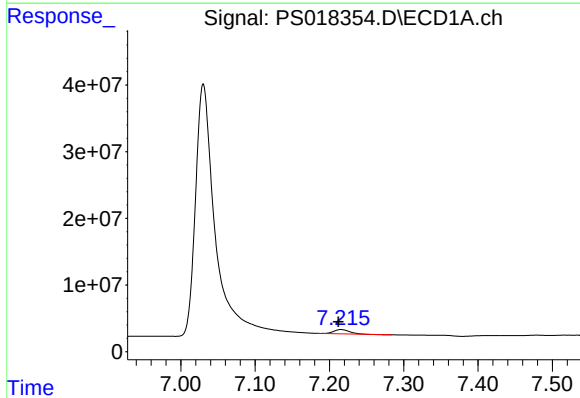


#5 DICAMBA

R.T.: 7.215 min
Delta R.T.: 0.003 min
Response: 9455614
Conc: 1.50 ng/ml

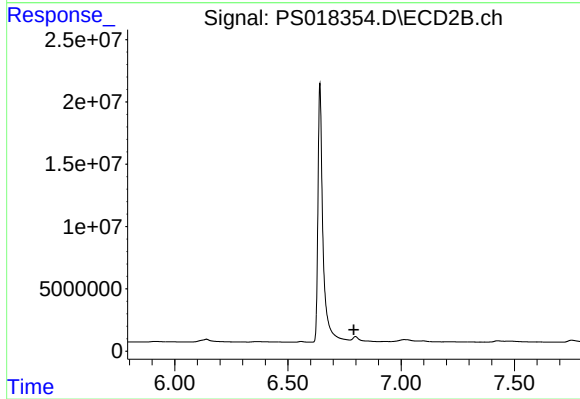

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 6.791 min
Response: 0
Conc: N.D.

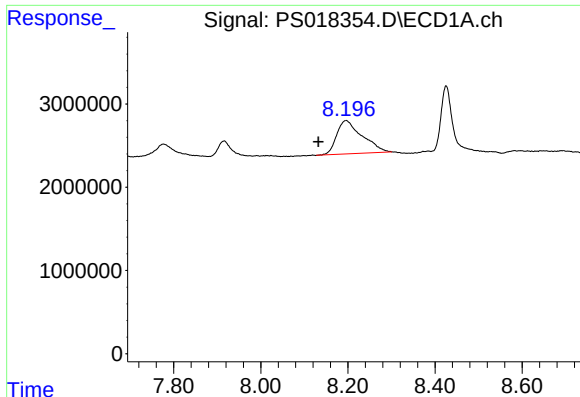

#9 2,4-D


R.T.: 8.196 min
Delta R.T.: 0.064 min
Response: 16230953
Conc: 8.81 ng/ml

Instrument :
ECD_S
ClientSampleId :

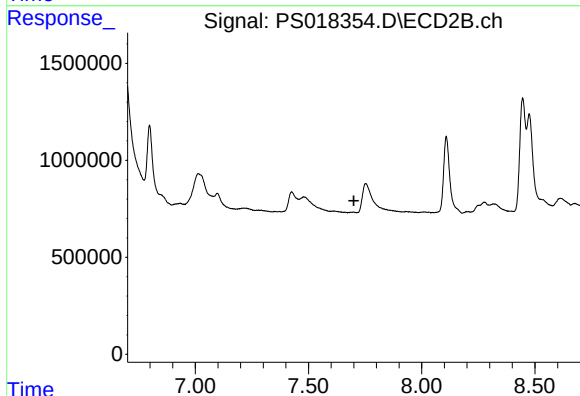


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.701 min
Response: 0
Conc: N.D.

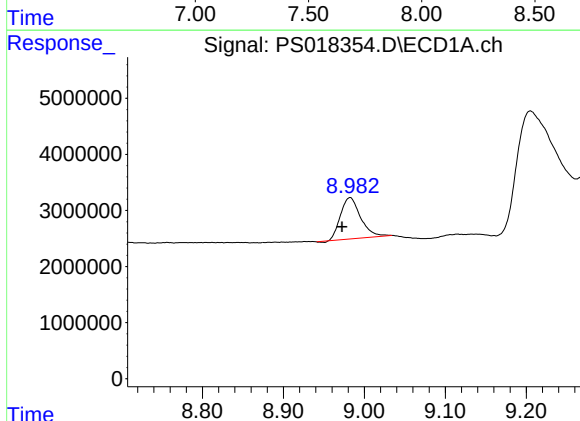


#11 2,4,5-TP (SILVEX)

R.T.: 8.983 min
Delta R.T.: 0.010 min
Response: 12649512
Conc: 1.48 ng/ml

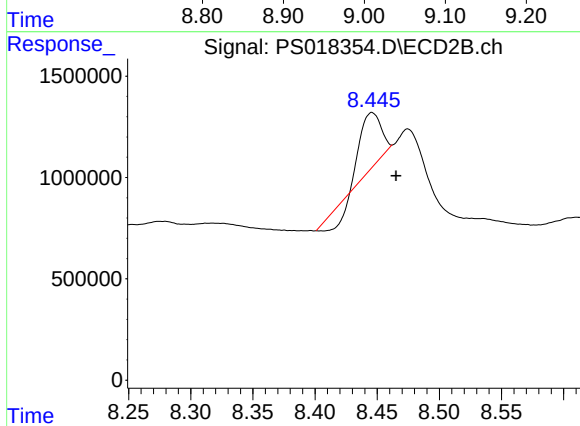

#11 2,4,5-TP (SILVEX)


R.T.: 8.446 min
Delta R.T.: -0.020 min
Response: 2250395
Conc: N.D.

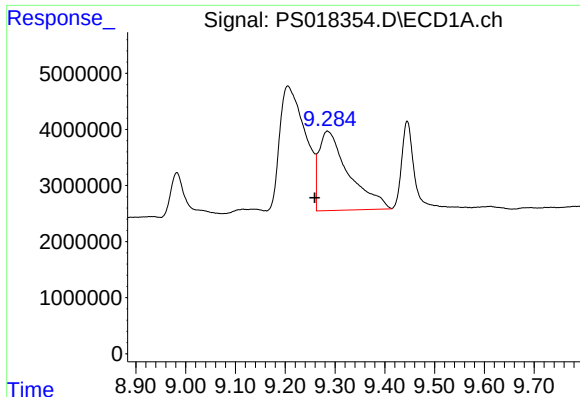

#12 2,4,5-T


R.T.: 9.285 min
Delta R.T.: 0.026 min
Response: 58949135
Conc: 6.66 ng/ml

Instrument :
ECD_S
ClientSampleId :

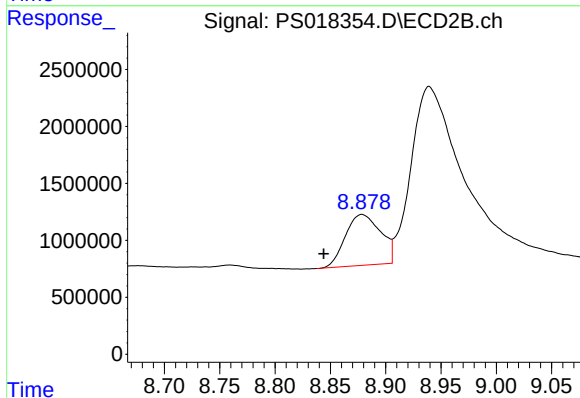


#12 2,4,5-T

R.T.: 8.879 min
Delta R.T.: 0.034 min
Response: 9896299
Conc: 2.80 ng/ml

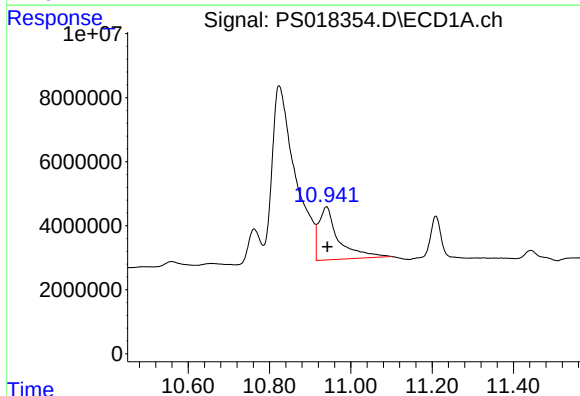


#14 DINOSEB

R.T.: 10.940 min
Delta R.T.: -0.002 min
Response: 56431802
Conc: 8.45 ng/ml

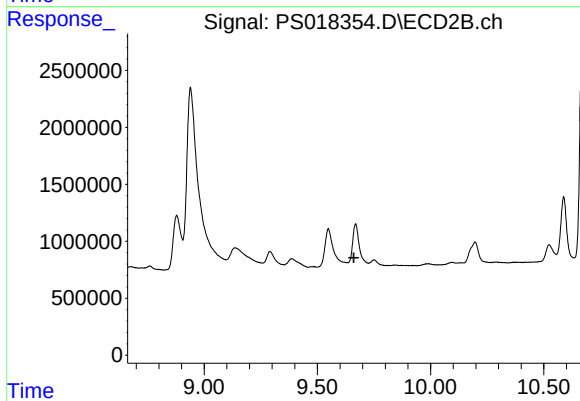

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.661 min
Response: 0
Conc: N.D.

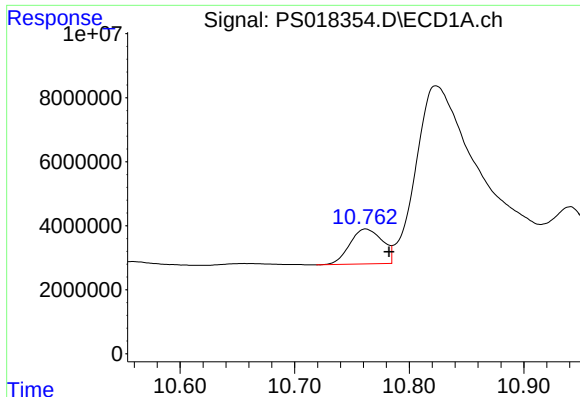

#15 Picloram


R.T.: 10.762 min
Delta R.T.: -0.020 min
Response: 21602625
Conc: 1.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

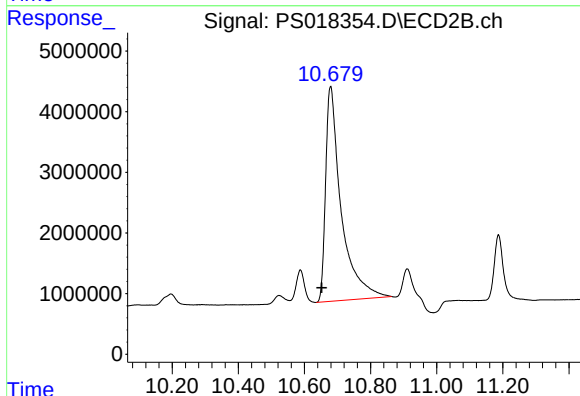


#15 Picloram

R.T.: 10.679 min
Delta R.T.: 0.027 min
Response: 115728104
Conc: 23.09 ng/ml

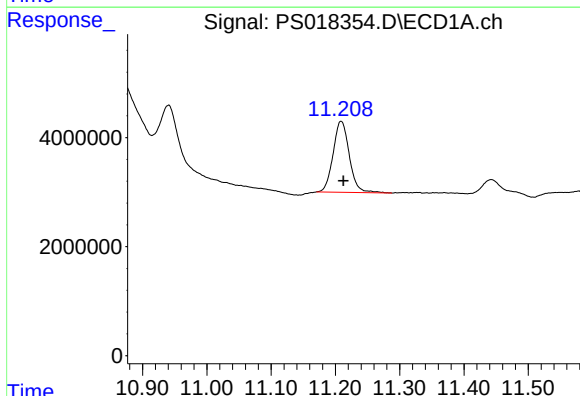

#16 DCPA

R.T.: 11.209 min
Delta R.T.: -0.004 min
Response: 22885227
Conc: 2.08 ng/ml

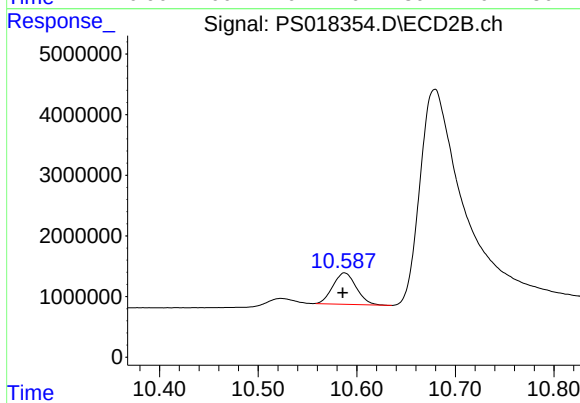

#16 DCPA

R.T.: 10.588 min
Delta R.T.: 0.002 min
Response: 8546304
Conc: 1.88 ng/ml