

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021523\
 Data File : PS022145.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Feb 2023 21:18
 Operator : AR\AJ
 Sample : 01538-08
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TEST-PIT-5-(TP5)-COMP-5

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 23:45:32 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020223.M
 Quant Title : 8080.M
 QLast Update : Fri Feb 03 10:03:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
3) T	4-Nitroph...	6.189f	0.000	9138713	0	6.790	N.D. #
6) T	MCPP	6.619	0.000	345898	0	<MDL	N.D. #
8) T	DICHLORPROP	6.968f	0.000	119885	0	<MDL	N.D. #
10) T	Pentachlo...	7.480	0.000	814485	0	<MDL	N.D. #
11) T	2,4,5-TP ...	7.940	0.000	224014	0	<MDL	N.D. #
12) T	2,4,5-T	8.245	0.000	395307	0	<MDL	N.D. #
15) T	Picloram	9.644	0.000	121560	0	<MDL	N.D. #
16) T	DCPA	10.053	0.000	416766	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021523\
Data File : PS022145.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Feb 2023 21:18
Operator : AR\AJ
Sample : 01538-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TEST-PIT-5-(TP5)-COMP-5

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 23:45:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020223.M
Quant Title : 8080.M
QLast Update : Fri Feb 03 10:03:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

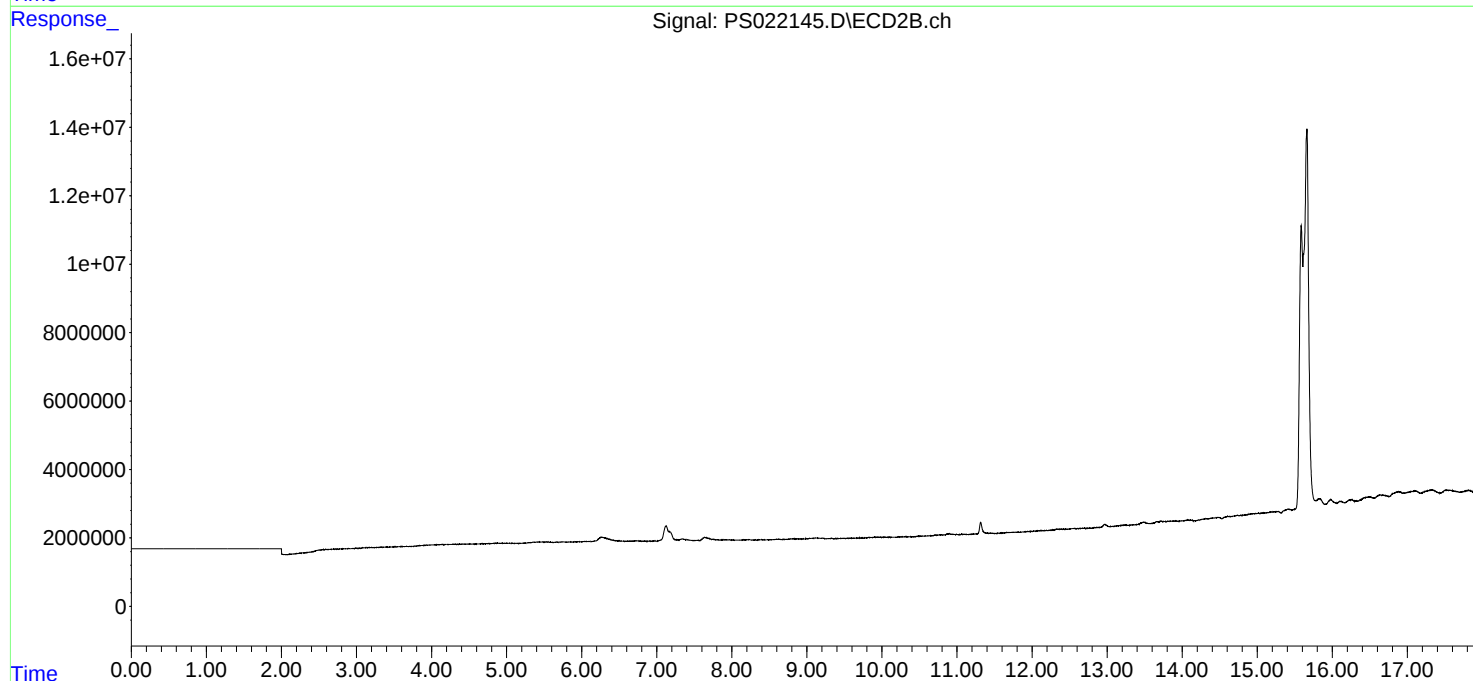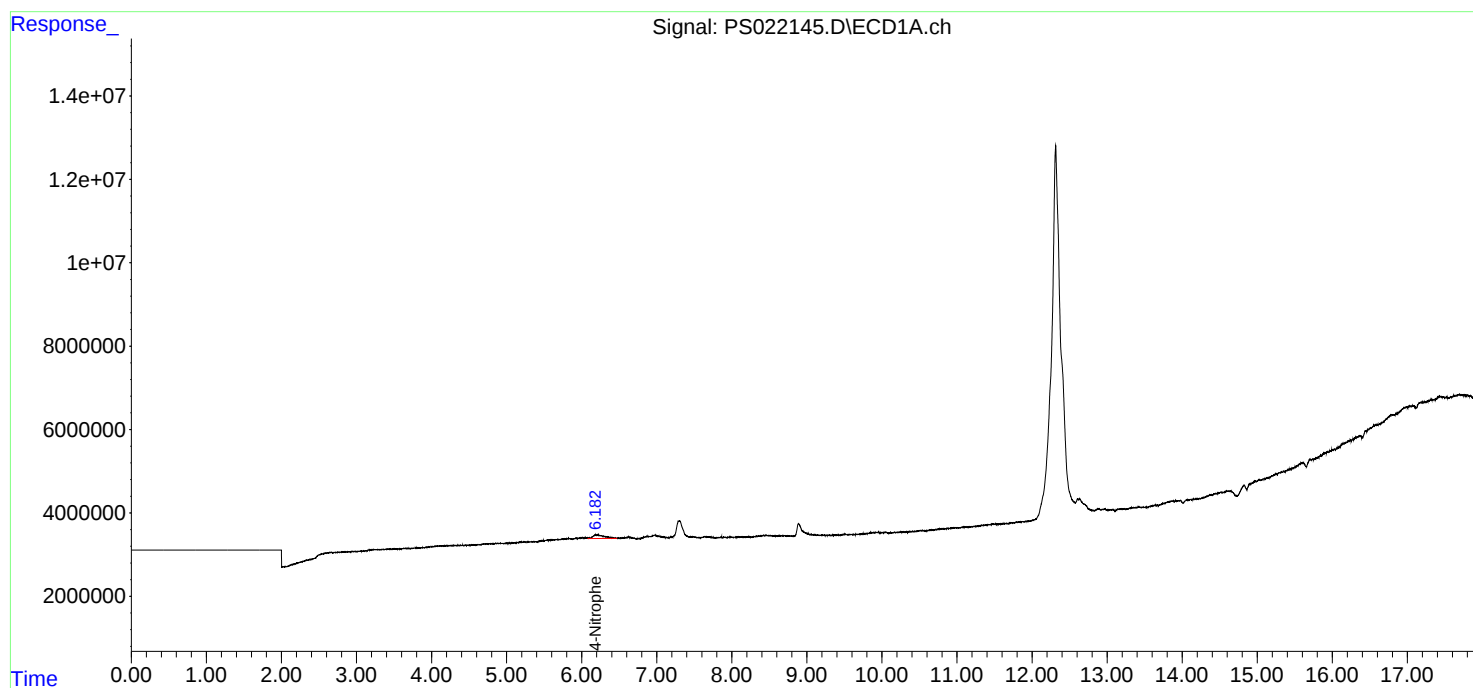


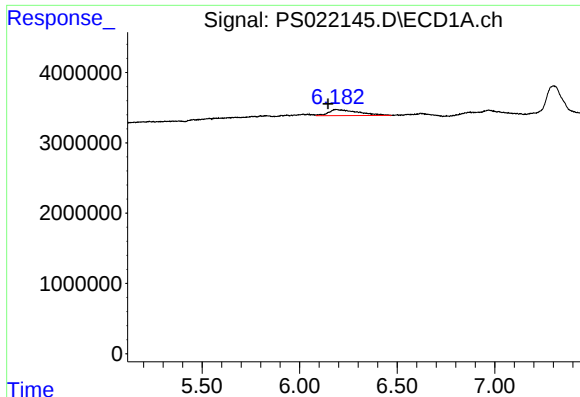

#3 4-Nitrophenol


R.T.: 6.189 min
Delta R.T.: 0.043 min
Response: 9138713
Conc: 6.79 ng/ml

Instrument :
ECD_S
ClientSampleId :
TEST-PIT-5-(TP5)-COMP-5

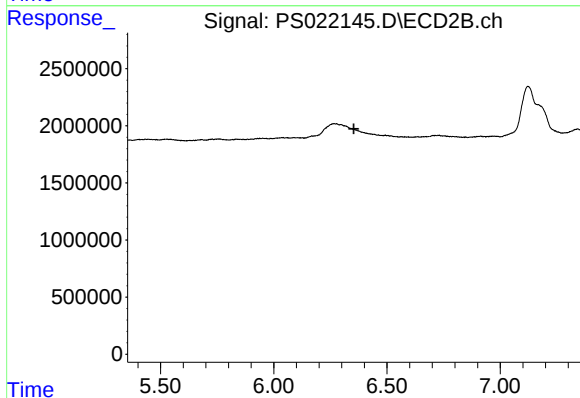


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.354 min
Response: 0
Conc: N.D.

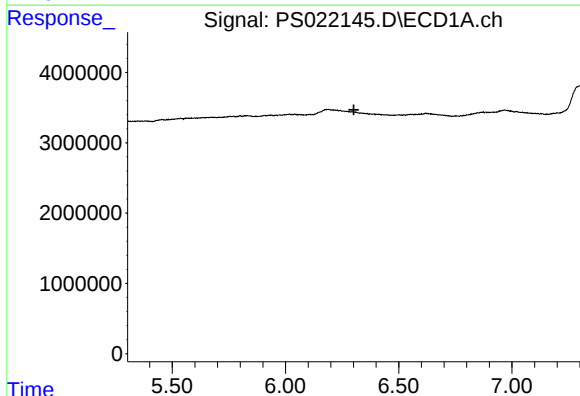

#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.302 min
Response: 0
Conc: N.D.

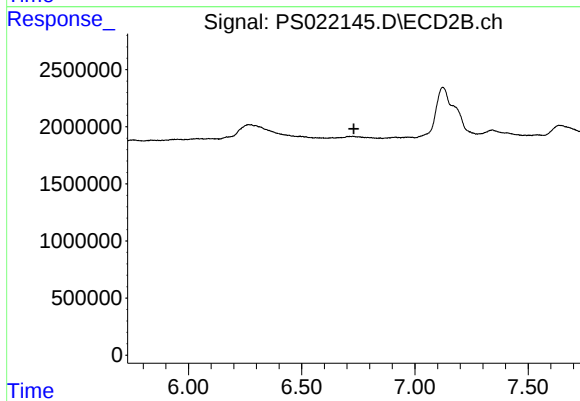

#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.730 min
Response: 0
Conc: N.D.