

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021524\
 Data File : PL088105.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Feb 2024 21:00
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 16 05:45:40 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 16 05:43:44 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.636	2.873f	212.0E6	130.9E6	73.661	74.699
28)	SA Decachlor...	9.306	8.106f	159.1E6	99611871	73.372	72.557
Target Compounds							
23)	Chlordane-1	4.821	3.897f	88041187	36160644	722.587	715.666
24)	Chlordane-2	5.358	4.448f	93984606	3646780	717.337	58.974 #
25)	Chlordane-3	6.078	5.126f	375.1E6	138.4E6	744.131	744.064
26)	Chlordane-4	6.162	5.191f	448.5E6	128.5E6	739.746	747.893
27)	Chlordane-5	7.021	5.867f	73834071	37333297	732.776	731.590



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021524\
Data File : PL088105.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Feb 2024 21:00
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 16 05:45:40 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
Quant Title : GC Extractables
QLast Update : Fri Feb 16 05:43:44 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

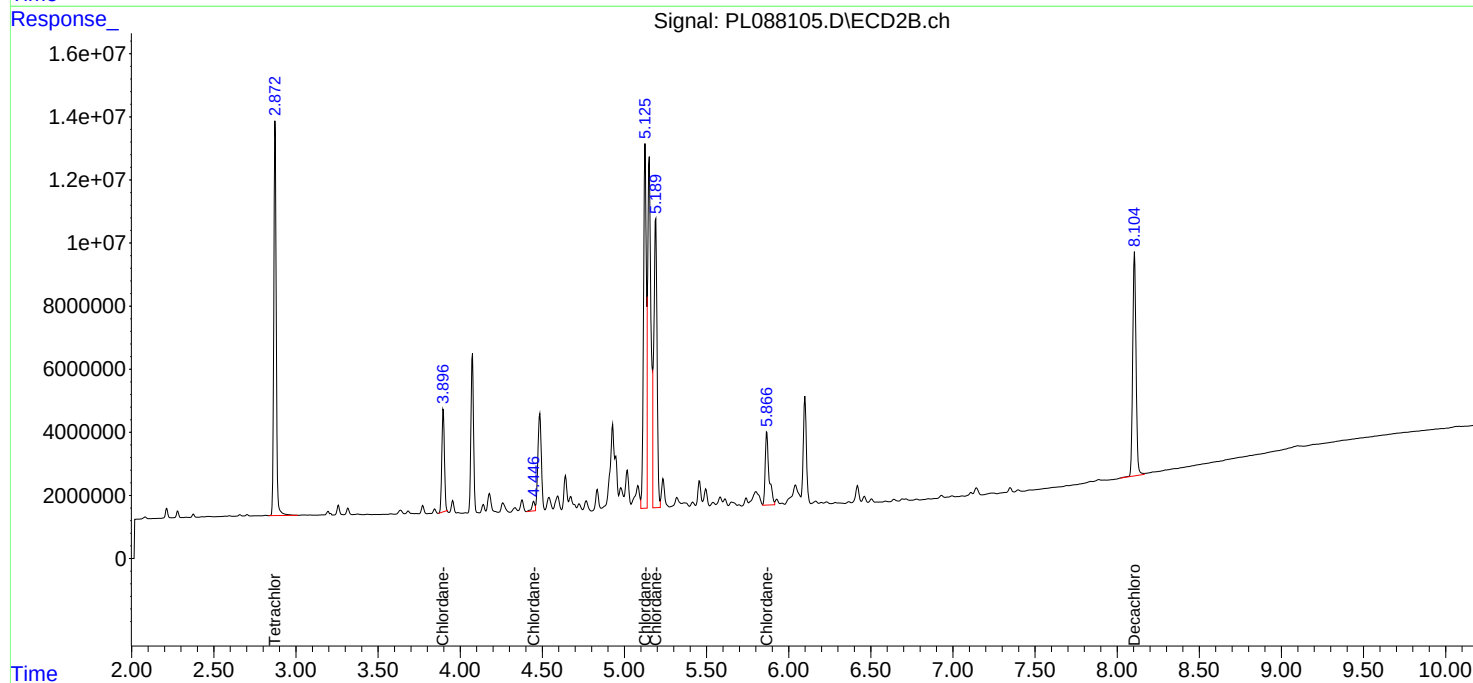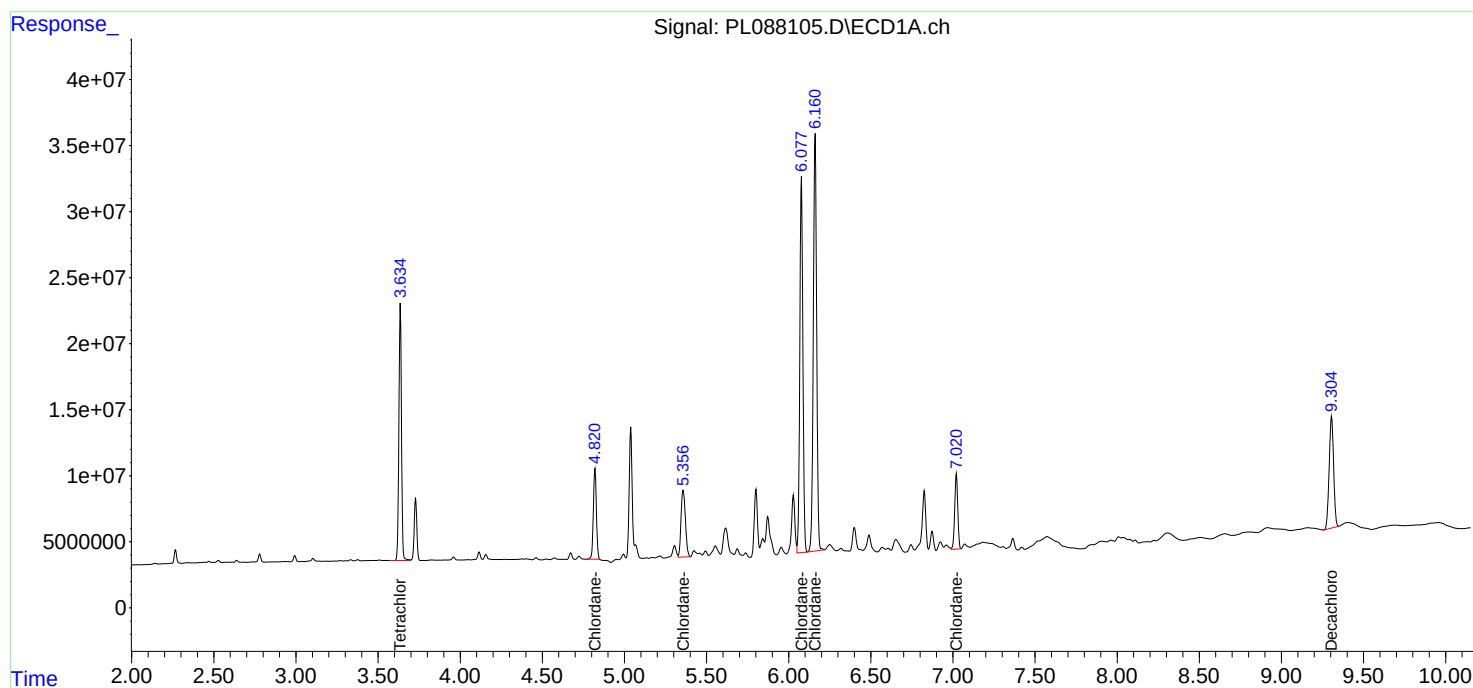


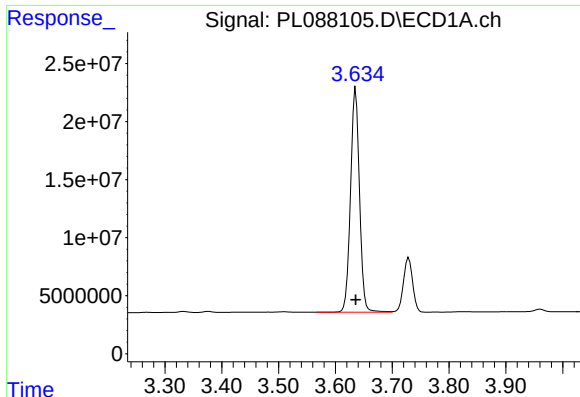

#1 Tetrachloro-m-xylene


R.T.: 3.636 min
Delta R.T.: 0.000 min
Response: 211964342
Conc: 73.66 ng/ml

Instrument :
ECD_S
ClientSampleId :

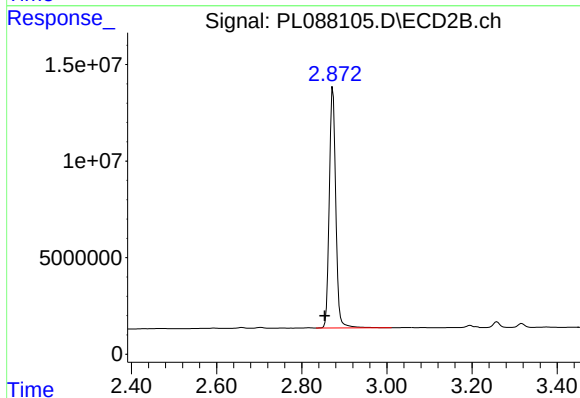


#1 Tetrachloro-m-xylene

R.T.: 2.873 min
Delta R.T.: 0.020 min
Response: 130930118
Conc: 74.70 ng/ml

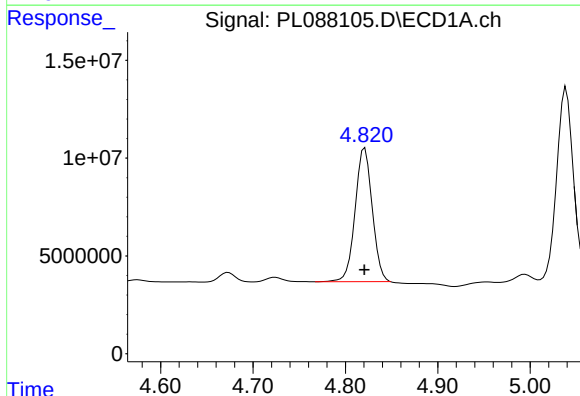


#23 Chlordane-1

R.T.: 4.821 min
Delta R.T.: 0.000 min
Response: 88041187
Conc: 722.59 ng/ml

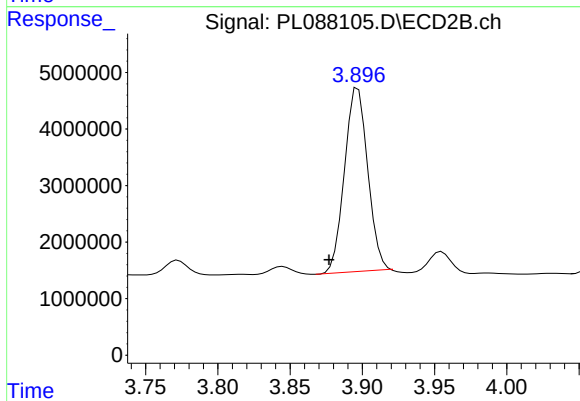

#23 Chlordane-1


R.T.: 3.897 min
Delta R.T.: 0.020 min
Response: 36160644
Conc: 715.67 ng/ml

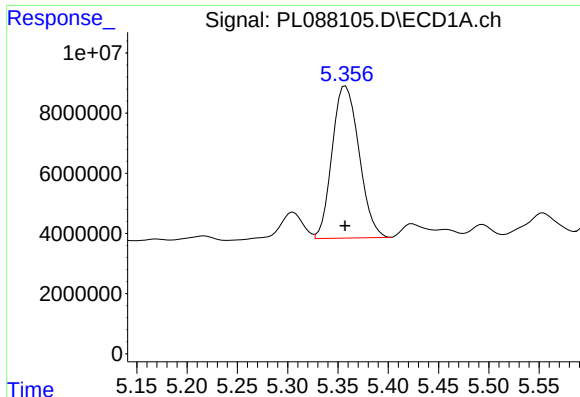

#24 Chlordane-2


R.T.: 5.358 min
Delta R.T.: 0.000 min
Response: 93984606
Conc: 717.34 ng/ml

Instrument :
ECD_S
ClientSampleId :

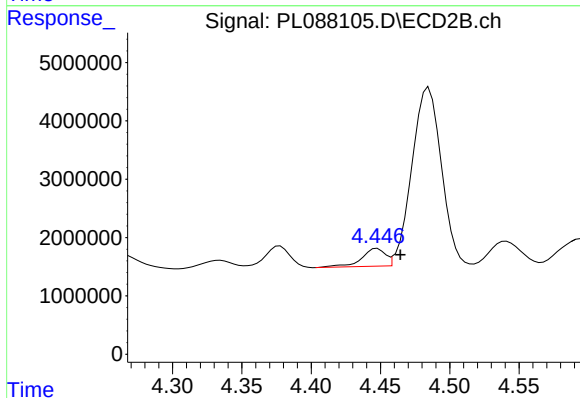


#24 Chlordane-2

R.T.: 4.448 min
Delta R.T.: -0.017 min
Response: 3646780
Conc: 58.97 ng/ml

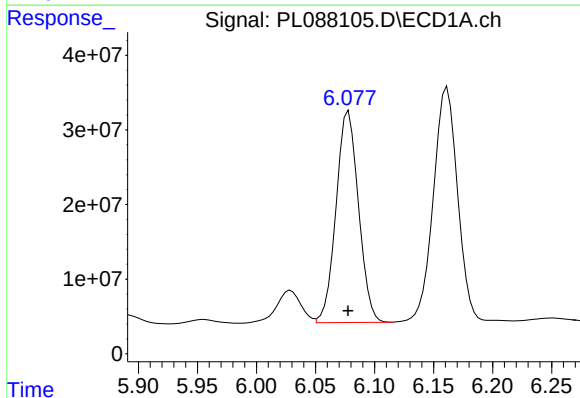


#25 Chlordane-3

R.T.: 6.078 min
Delta R.T.: 0.000 min
Response: 375061756
Conc: 744.13 ng/ml

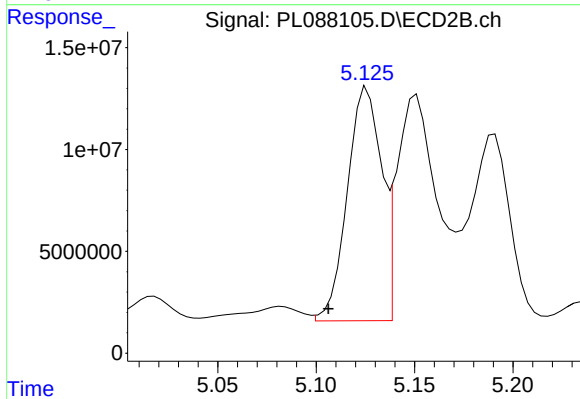

#25 Chlordane-3


R.T.: 5.126 min
Delta R.T.: 0.020 min
Response: 138374052
Conc: 744.06 ng/ml

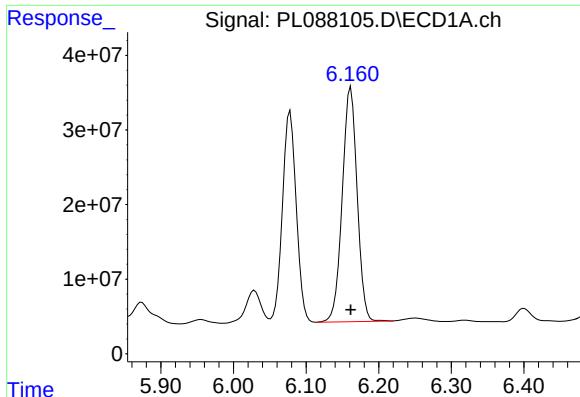

#26 Chlordane-4


R.T.: 6.162 min
Delta R.T.: 0.000 min
Response: 448526371
Conc: 739.75 ng/ml

Instrument :
ECD_S
ClientSampleId :

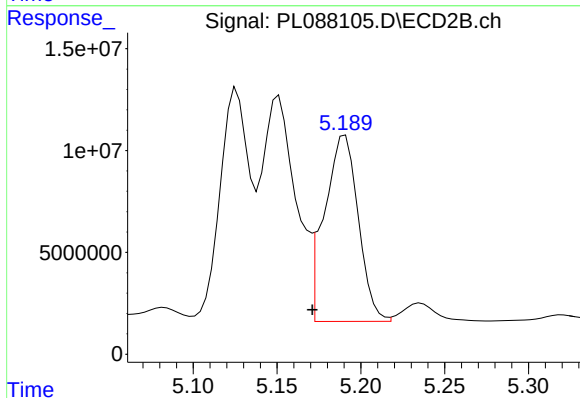


#26 Chlordane-4

R.T.: 5.191 min
Delta R.T.: 0.020 min
Response: 128453470
Conc: 747.89 ng/ml

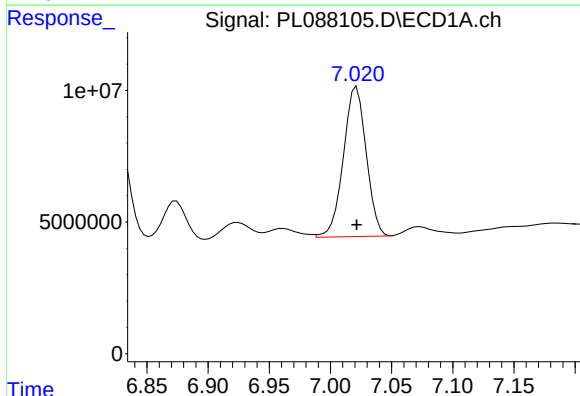


#27 Chlordane-5

R.T.: 7.021 min
Delta R.T.: 0.000 min
Response: 73834071
Conc: 732.78 ng/ml

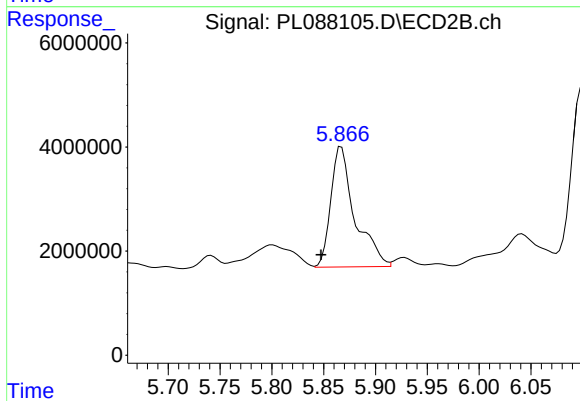

#27 Chlordane-5


R.T.: 5.867 min
Delta R.T.: 0.020 min
Response: 37333297
Conc: 731.59 ng/ml

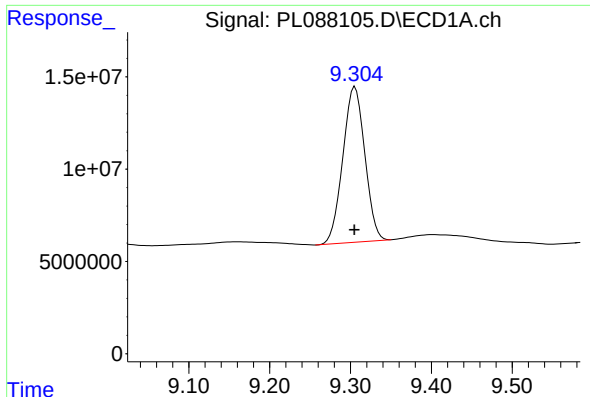

#28 Decachlorobiphenyl

R.T.: 9.306 min
Delta R.T.: 0.000 min
Response: 159058884
Conc: 73.37 ng/ml

Instrument :
ECD_S
ClientSampleId :

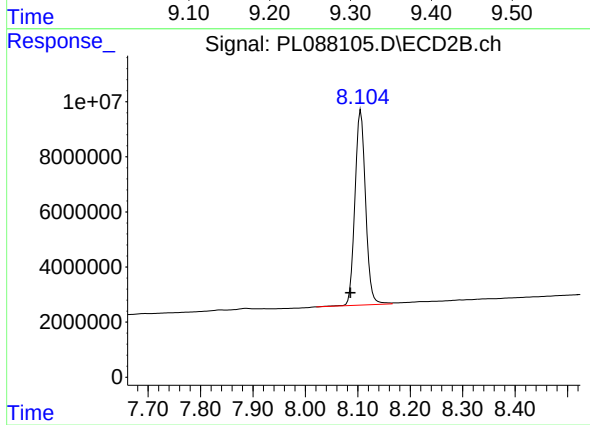

#28 Decachlorobiphenyl

R.T.: 8.106 min
Delta R.T.: 0.020 min
Response: 99611871
Conc: 72.56 ng/ml