

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021623\
 Data File : PS022158.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Feb 2023 10:52
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 15 20:26:10 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020223.M
 Quant Title : 8080.M
 QLast Update : Fri Feb 03 10:03:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.306	6.730	1143.0E6	1133.0E6	501.448	559.695
Target Compounds							
1) T	Dalapon	2.412	0.000	1125795	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.701	0.000	489286	0	<MDL	N.D. #
3) T	4-Nitroph...	6.173	6.369	5566301	1094870	4.136	<MDL #
6) T	MCP	0.000	7.033f	0	3751895	N.D.	<MDL
7) T	MCPA	6.711	7.138f	626967	25063956	<MDL	2.495 #
10) T	Pentachlo...	7.468	8.226	6567295	6326941	<MDL	<MDL #
11) T	2,4,5-TP ...	7.962	8.607	298942	2732729	<MDL	<MDL #
12) T	2,4,5-T	8.207	9.027f	133961	2372298	<MDL	<MDL #
13) T	2,4-DB	8.760	0.000	340858	0	<MDL	N.D. #
14) T	DINOSEB	9.802	9.794	2211307	3084488	<MDL	<MDL #
15) T	Picloram	9.625	10.713f	576665	6350779	<MDL	<MDL #
16) T	DCPA	10.059	10.713	3517425	6350779	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021623\
Data File : PS022158.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Feb 2023 10:52
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 15 20:26:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020223.M
Quant Title : 8080.M
QLast Update : Fri Feb 03 10:03:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

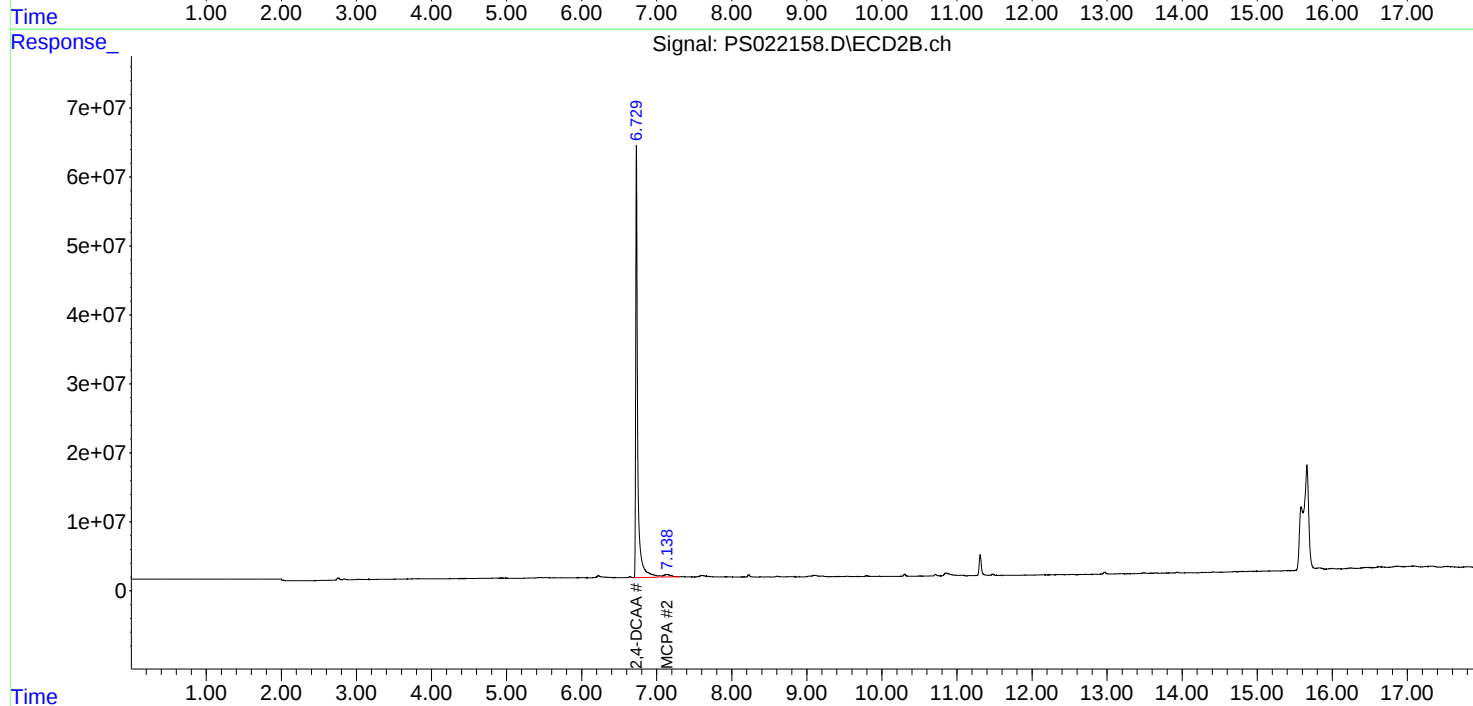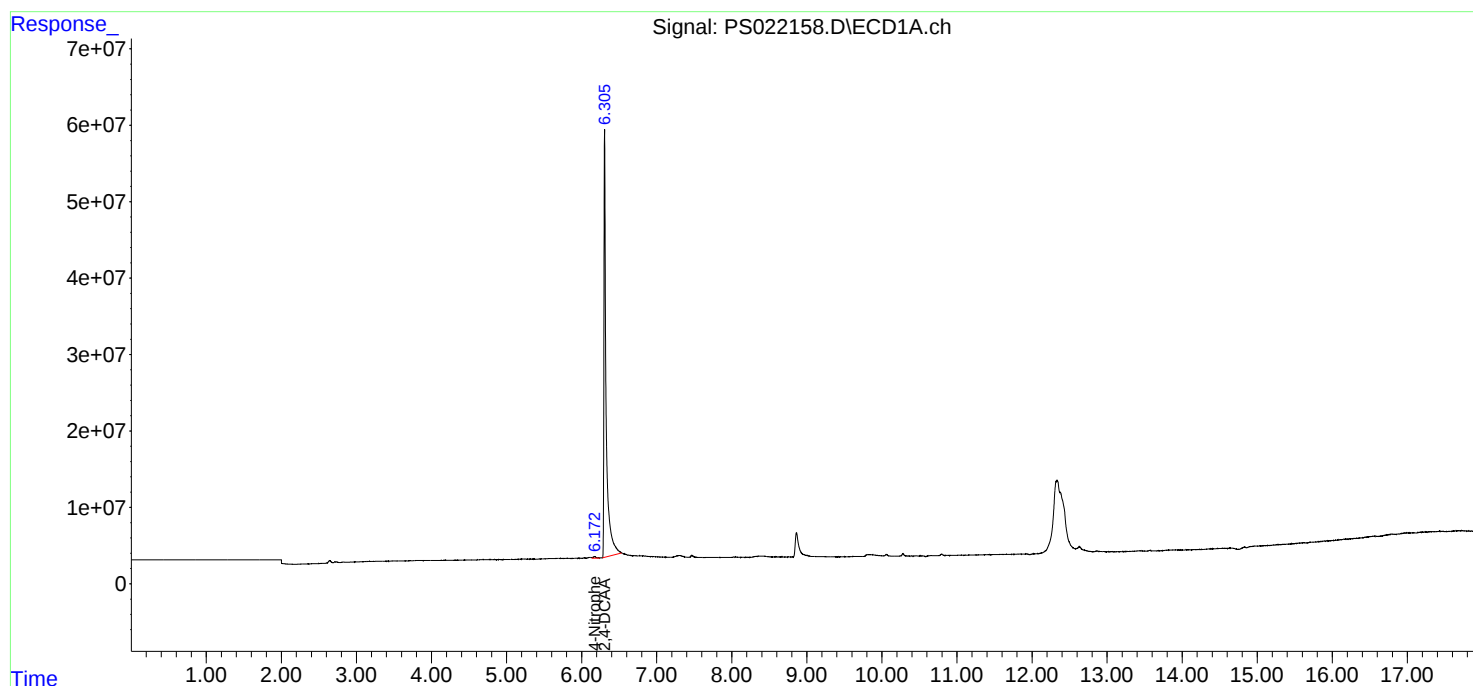


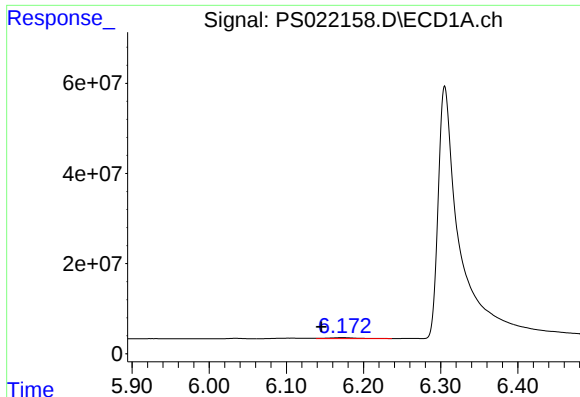

#3 4-Nitrophenol


R.T.: 6.173 min
Delta R.T.: 0.027 min
Response: 5566301
Conc: 4.14 ng/ml

Instrument :
ECD_S
ClientSampleId :

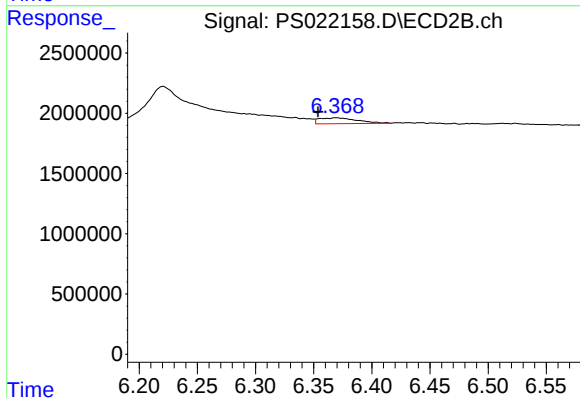


#3 4-Nitrophenol

R.T.: 6.369 min
Delta R.T.: 0.015 min
Response: 1094870
Conc: N.D.

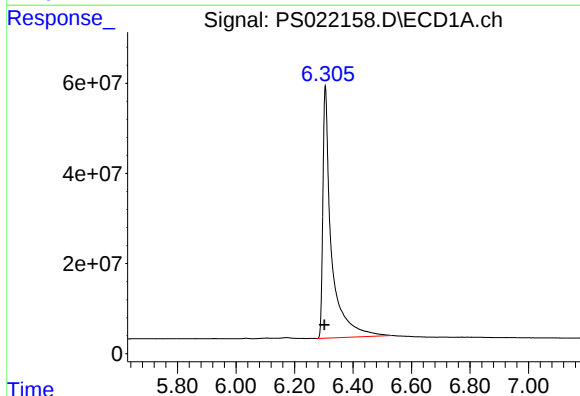


#4 2,4-DCAA

R.T.: 6.306 min
Delta R.T.: 0.004 min
Response: 1142982837
Conc: 501.45 ng/ml

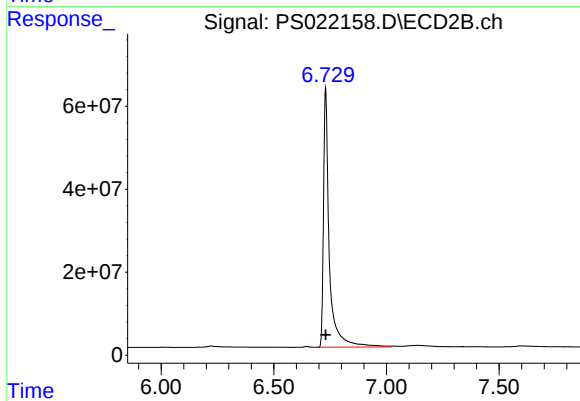

#4 2,4-DCAA


R.T.: 6.730 min
Delta R.T.: 0.000 min
Response: 1132957047
Conc: 559.70 ng/ml

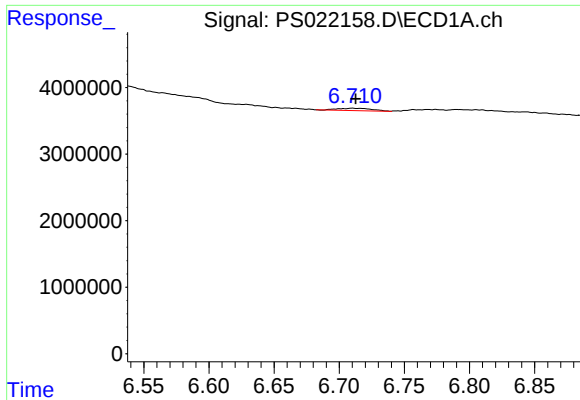

#7 MCPA

R.T.: 6.711 min
Delta R.T.: -0.002 min
Response: 626967
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

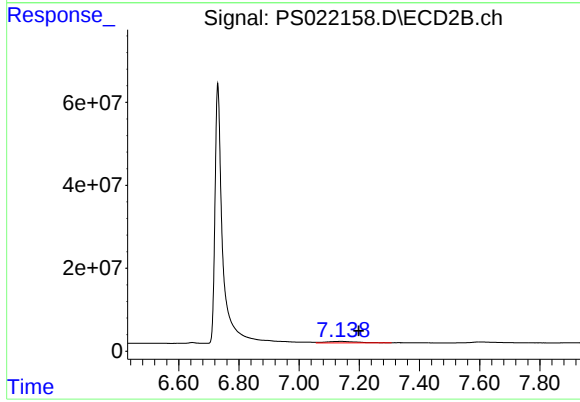

#7 MCPA

R.T.: 7.138 min
Delta R.T.: -0.060 min
Response: 25063956
Conc: 2.50 ug/ml