

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021623\
 Data File : PS022177.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Feb 2023 01:27
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 16 04:25:18 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020223.M
 Quant Title : 8080.M
 QLast Update : Fri Feb 03 10:03:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.302	6.728	1204.8E6	1126.6E6	528.566	556.549
Target Compounds							
1) T	Dalapon	2.428	0.000	1182155	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.675	0.000	2676243	0	<MDL	N.D. #
3) T	4-Nitroph...	6.164	0.000	4686166	0	3.482	N.D. #
5) T	DICAMBA	0.000	6.889	0	8819321	N.D.	<MDL
6) T	MCPD	0.000	6.941f	0	6789595	N.D.	<MDL
7) T	MCPA	0.000	7.131f	0	21187306	N.D.	2.109
8) T	DICHLORPROP	7.062	7.574f	325175	7702892	<MDL	3.220 #
9) T	2,4-D	7.224	7.865f	10824737	1588760	3.600	<MDL #
10) T	Pentachlo...	7.460	8.222	8871716	8847522	<MDL	<MDL #
11) T	2,4,5-TP ...	8.003	8.592	5209911	5350306	<MDL	<MDL #
12) T	2,4,5-T	8.253	9.002f	3218276	4973478	<MDL	<MDL #
13) T	2,4-DB	8.731	9.403f	205635	1717340	<MDL	1.017 #
14) T	DINOSEB	9.786	9.791	12955357	3544101	1.260	<MDL #
15) T	Picloram	9.647	10.710f	6241377	18551756	<MDL	1.022 #
16) T	DCPA	10.054	10.710	5121575	18551756	<MDL	1.205 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021623\
Data File : PS022177.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Feb 2023 01:27
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 16 04:25:18 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020223.M
Quant Title : 8080.M
QLast Update : Fri Feb 03 10:03:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

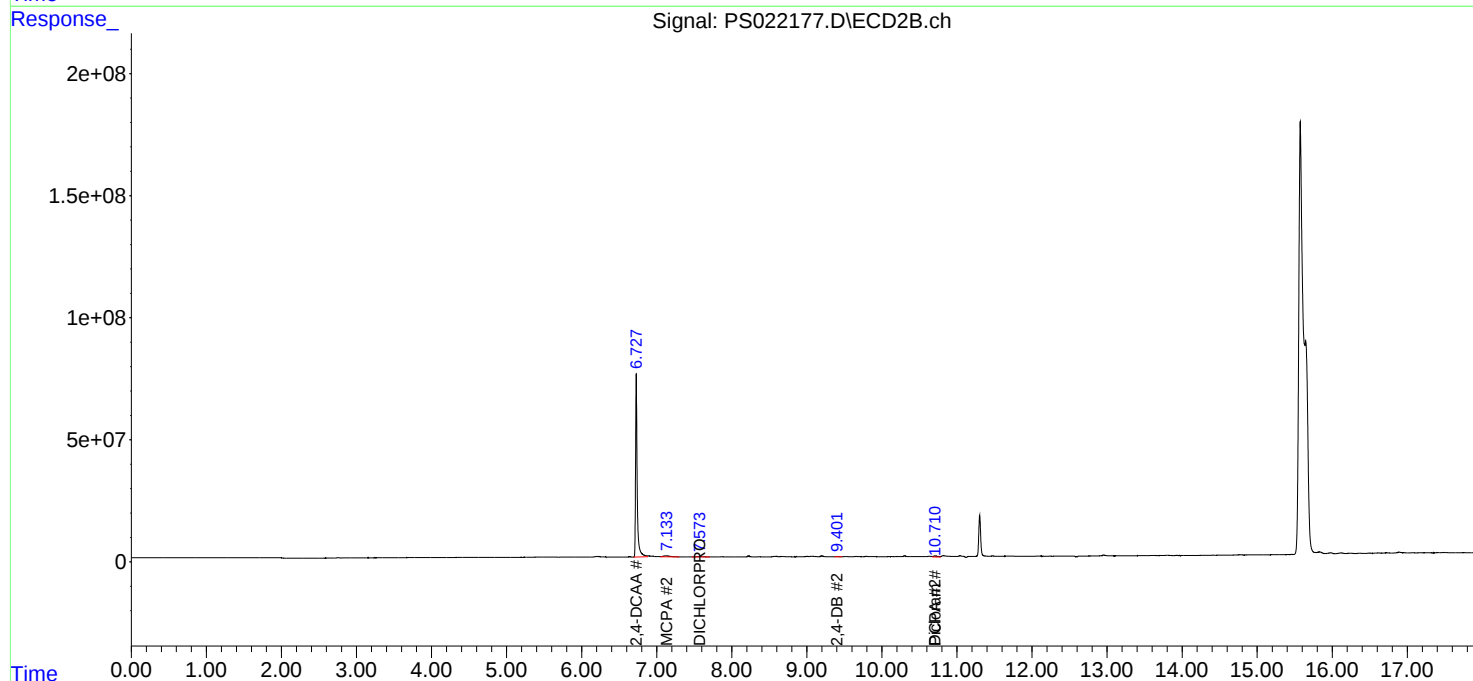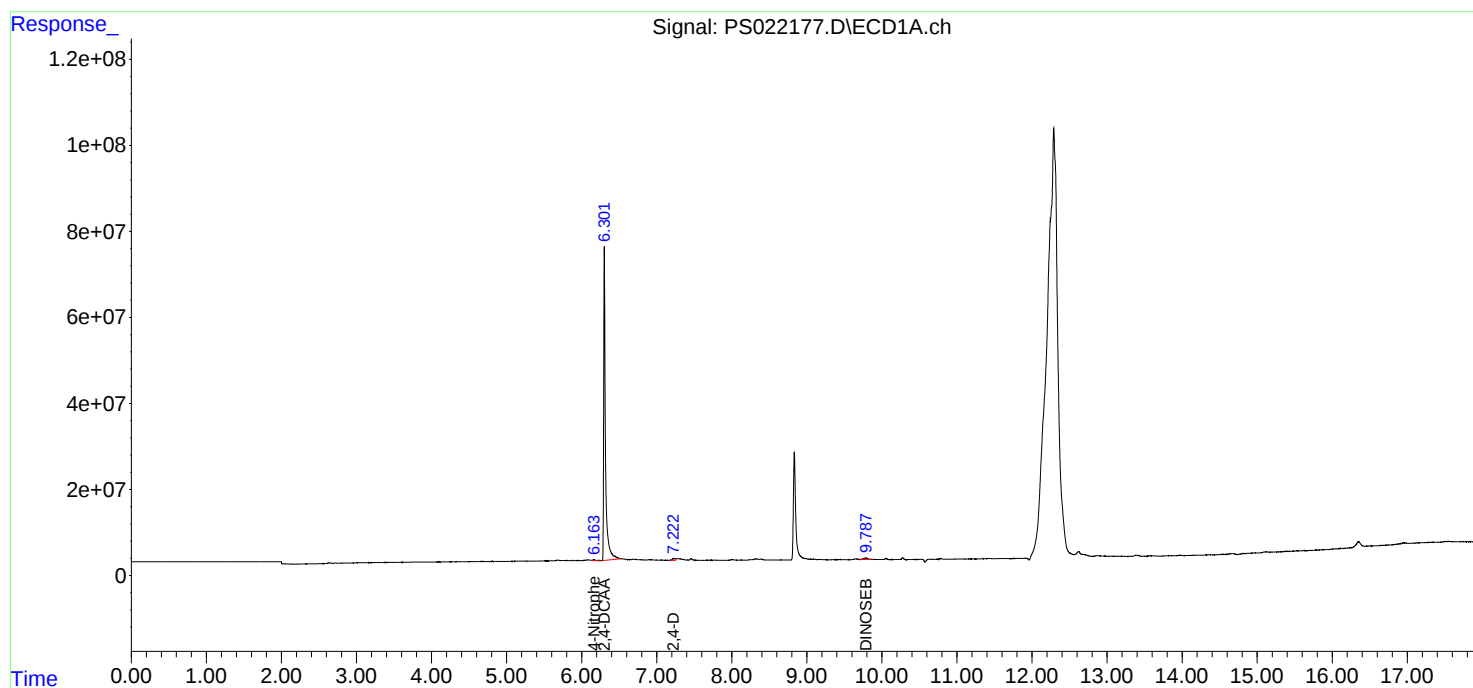


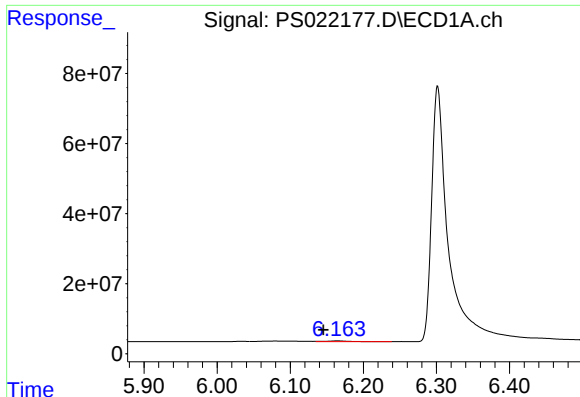

#3 4-Nitrophenol


R.T.: 6.164 min
Delta R.T.: 0.019 min
Response: 4686166
Conc: 3.48 ng/ml

Instrument :
ECD_S
ClientSampleId :

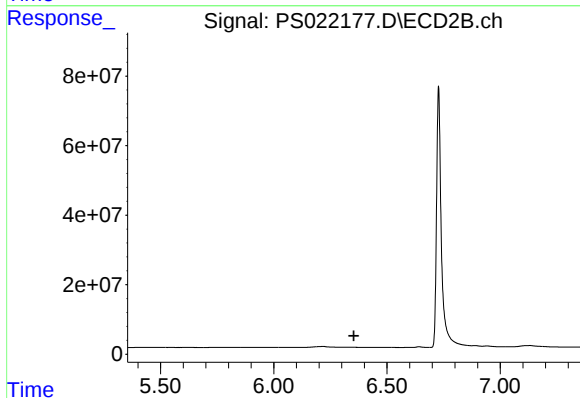


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.354 min
Response: 0
Conc: N.D.

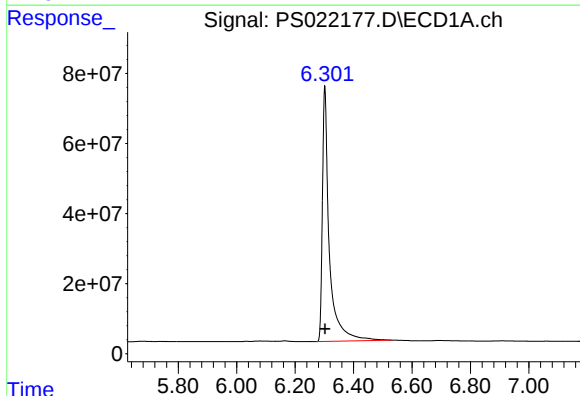


#4 2,4-DCAA

R.T.: 6.302 min
Delta R.T.: 0.000 min
Response: 1204795319
Conc: 528.57 ng/ml

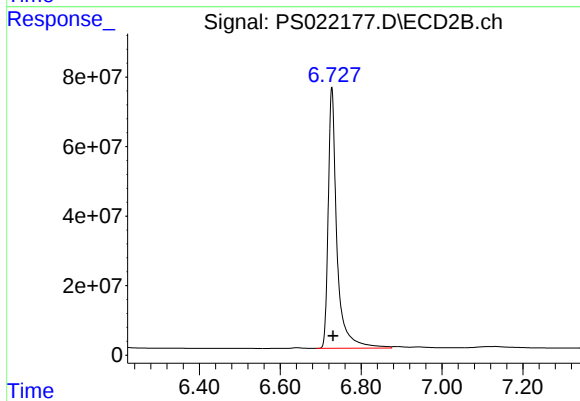

#4 2,4-DCAA


R.T.: 6.728 min
Delta R.T.: -0.003 min
Response: 1126588863
Conc: 556.55 ng/ml

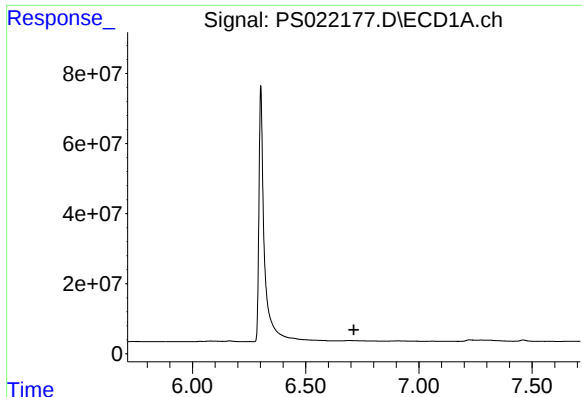

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.713 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

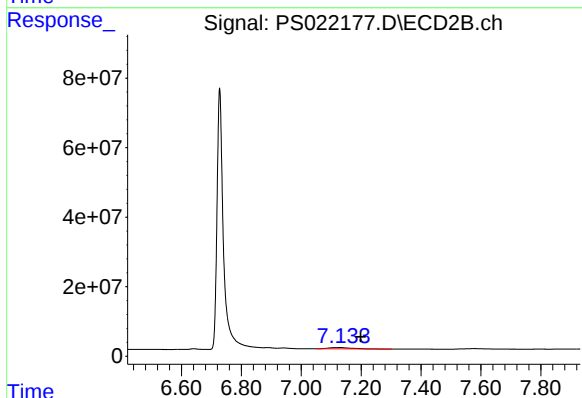


#7 MCPA

R.T.: 7.131 min
Delta R.T.: -0.067 min
Response: 21187306
Conc: 2.11 ug/ml

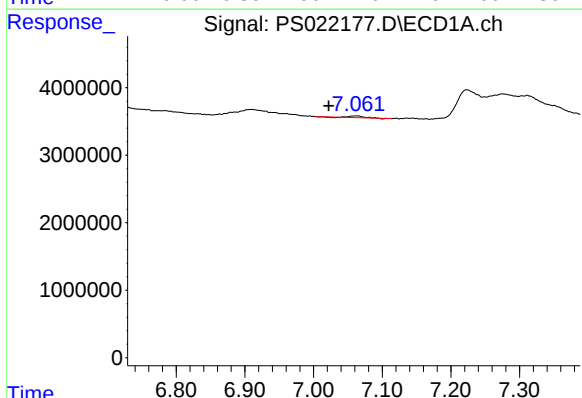


#8 DICHLORPROP

R.T.: 7.062 min
Delta R.T.: 0.040 min
Response: 325175
Conc: N.D.

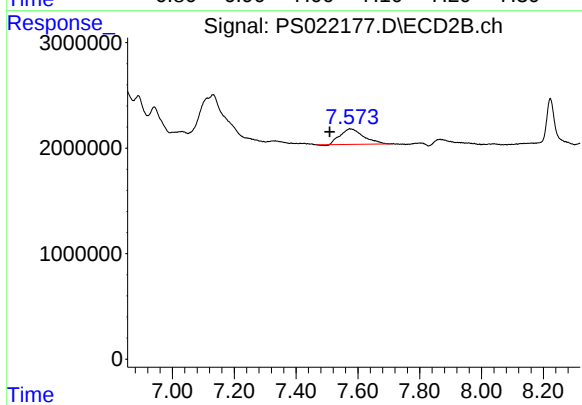

#8 DICHLORPROP


R.T.: 7.574 min
Delta R.T.: 0.065 min
Response: 7702892
Conc: 3.22 ng/ml

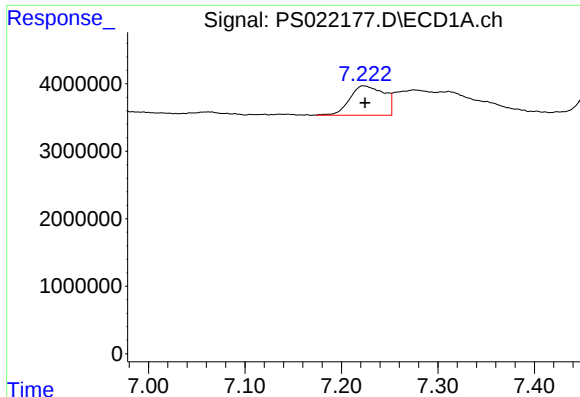

#9 2,4-D


R.T.: 7.224 min
Delta R.T.: -0.001 min
Response: 10824737
Conc: 3.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

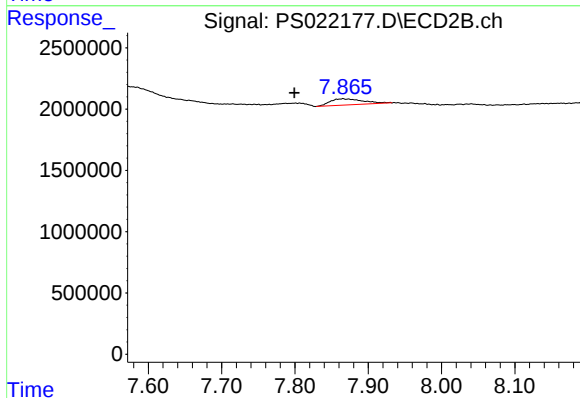


#9 2,4-D

R.T.: 7.865 min
Delta R.T.: 0.066 min
Response: 1588760
Conc: N.D.

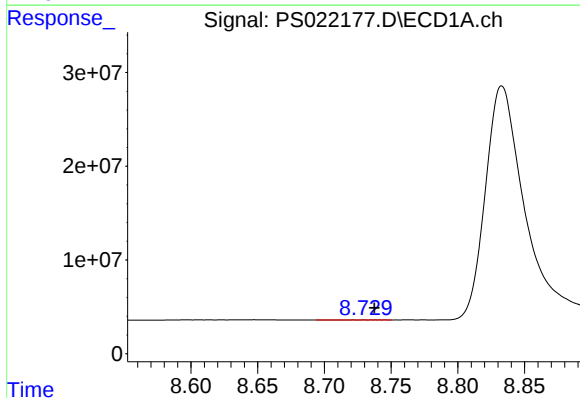


#13 2,4-DB

R.T.: 8.731 min
Delta R.T.: -0.006 min
Response: 205635
Conc: N.D.

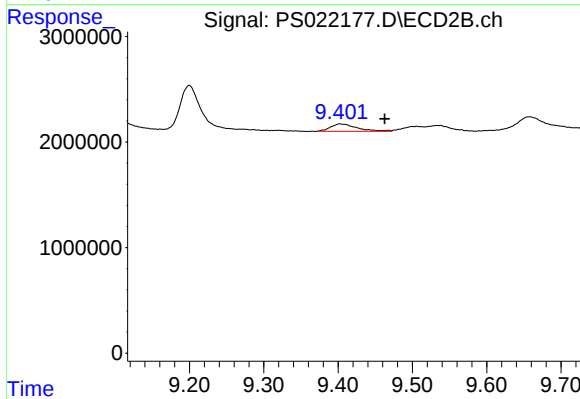

#13 2,4-DB


R.T.: 9.403 min
Delta R.T.: -0.059 min
Response: 1717340
Conc: 1.02 ng/ml

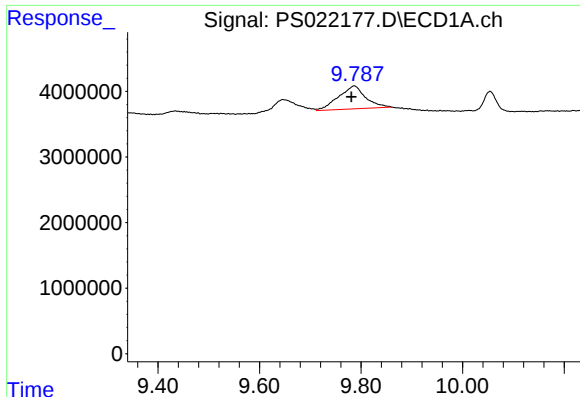

#14 DINOSEB


R.T.: 9.786 min
Delta R.T.: 0.006 min
Response: 12955357
Conc: 1.26 ng/ml

Instrument :
ECD_S
ClientSampleId :

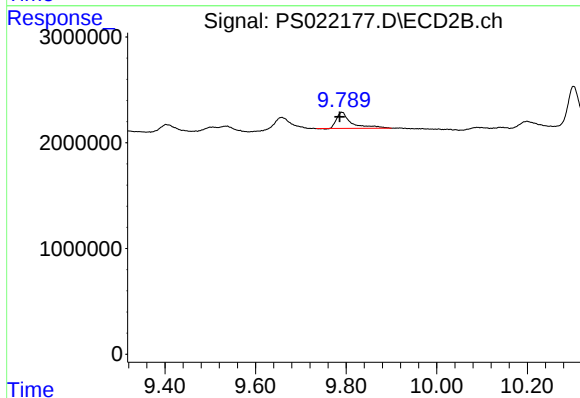


#14 DINOSEB

R.T.: 9.791 min
Delta R.T.: 0.005 min
Response: 3544101
Conc: N.D.

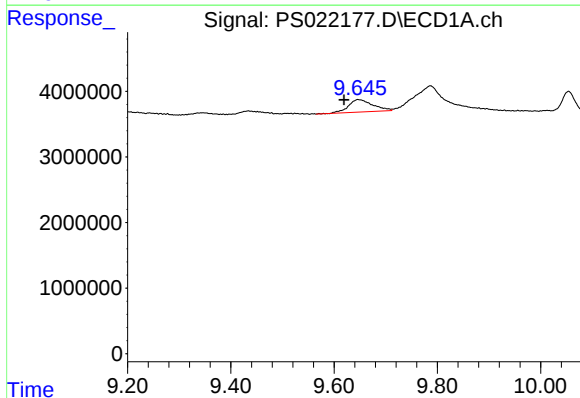


#15 Picloram

R.T.: 9.647 min
Delta R.T.: 0.028 min
Response: 6241377
Conc: N.D.

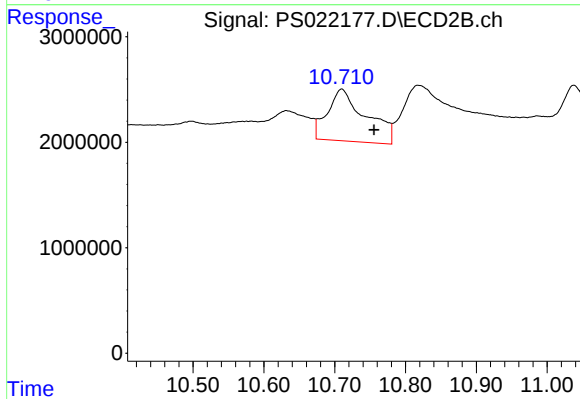

#15 Picloram


R.T.: 10.710 min
Delta R.T.: -0.046 min
Response: 18551756
Conc: 1.02 ng/ml

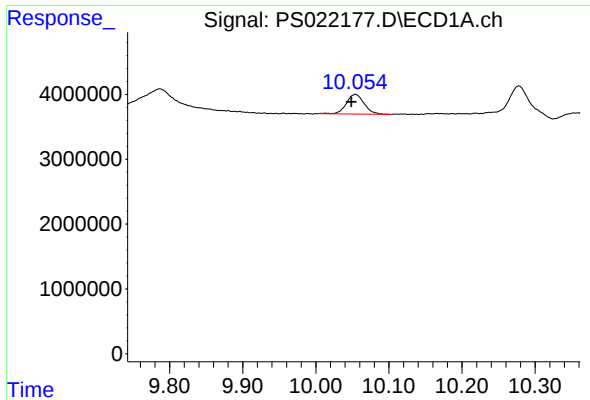

#16 DCPA

R.T.: 10.054 min
Delta R.T.: 0.005 min
Response: 5121575
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

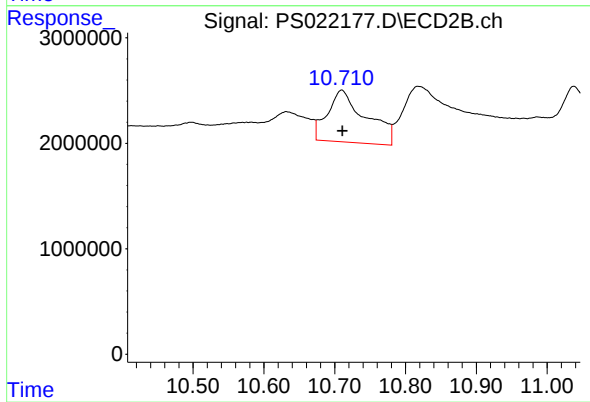

#16 DCPA

R.T.: 10.710 min
Delta R.T.: -0.001 min
Response: 18551756
Conc: 1.21 ng/ml