

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021720\
 Data File : PS008854.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Feb 2020 09:53
 Operator : DD\AJ
 Sample : PB126813BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB126813BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 17 14:17:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 05 02:36:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.249	6.941	1127.4E6	539.9E6	525.262	582.581
Target Compounds							
1) T	Dalapon	0.000	2.590	0	279.3E6	N.D.	232.903
2) T	3,5-DICHL...	0.000	6.115	0	89671630	N.D.	65.174
7) T	MCPA	7.802	0.000	62775335	0	7.308	N.D. #
11) T	2,4,5-TP ...	0.000	8.799	0	64102543	N.D.	12.507
12) T	2,4,5-T	0.000	9.262	0	118.5E6	N.D.	22.924
15) T	Picloram	11.048	11.034	738.5E6	413.4E6	48.768	54.763
16) T	DCPA	0.000	11.034	0	413.4E6	N.D.	63.552



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021720\
Data File : PS008854.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Feb 2020 09:53
Operator : DD\AJ
Sample : PB126813BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
PB126813BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 17 14:17:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
Quant Title : 8080.M
QLast Update : Wed Feb 05 02:36:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

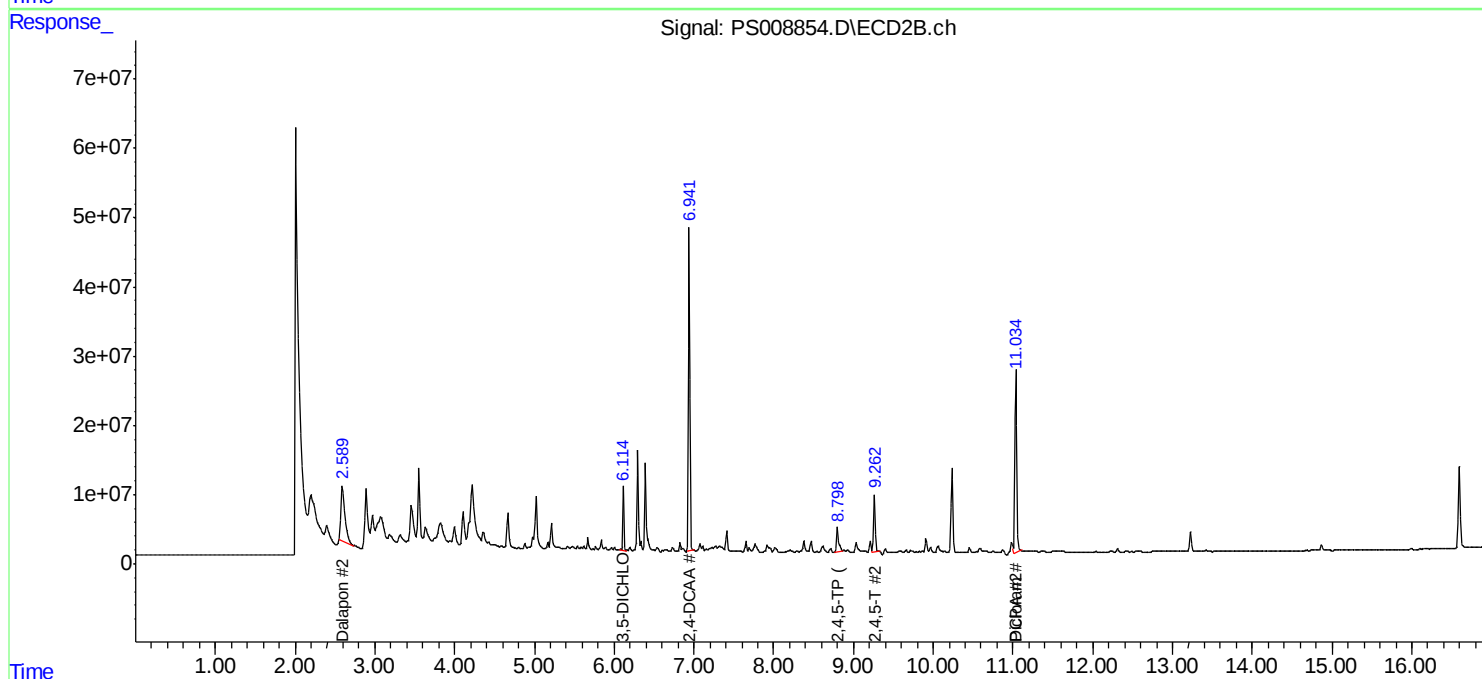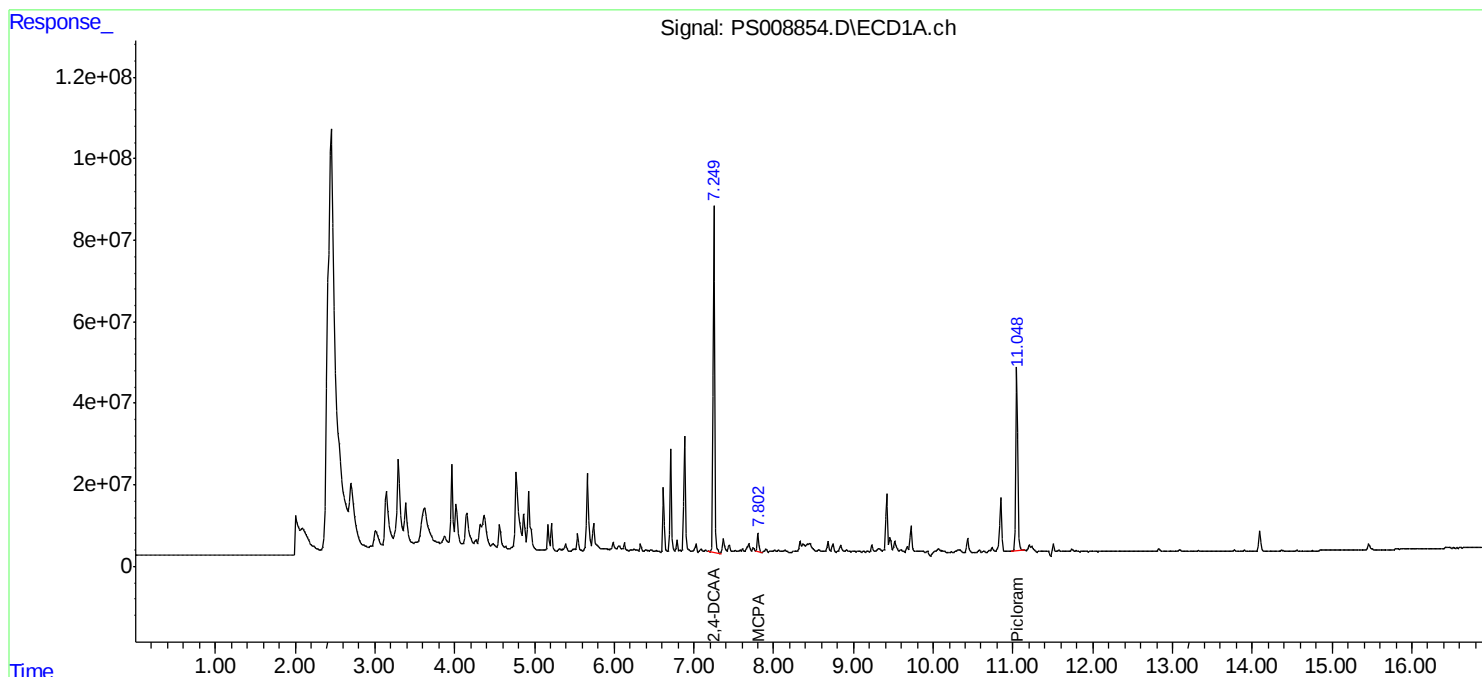


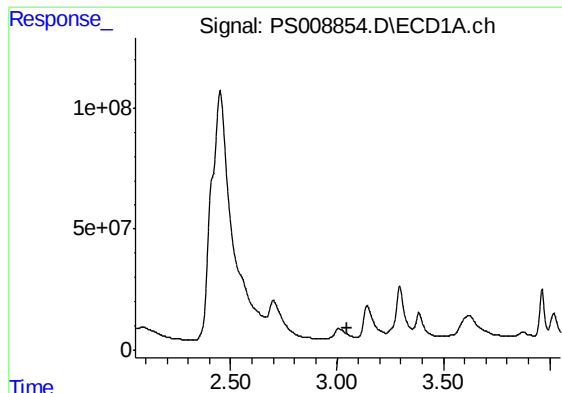

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.051 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB126813BL

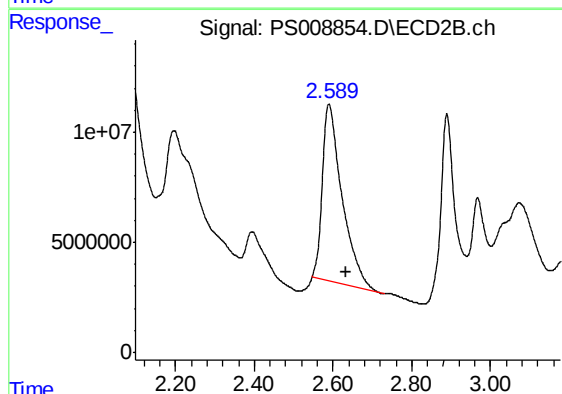


#1 Dalapon

R.T.: 2.590 min
Delta R.T.: -0.042 min
Response: 279325099
Conc: 232.90 ng/ml

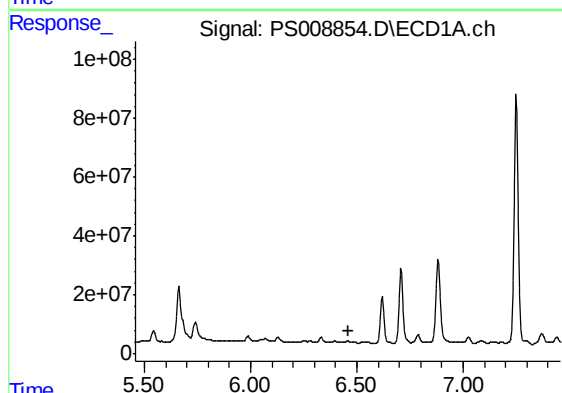


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.458 min
Response: 0
Conc: N.D.

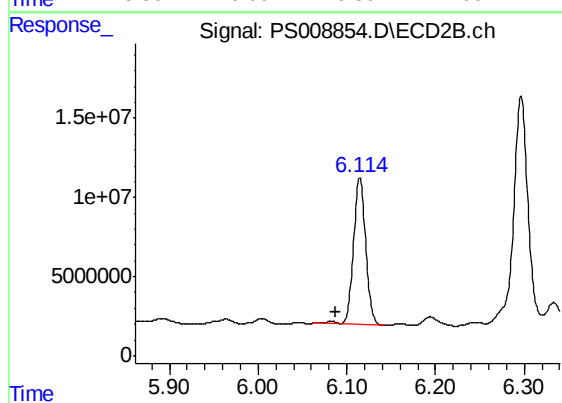

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.115 min
Delta R.T.: 0.027 min
Response: 89671630
Conc: 65.17 ng/ml

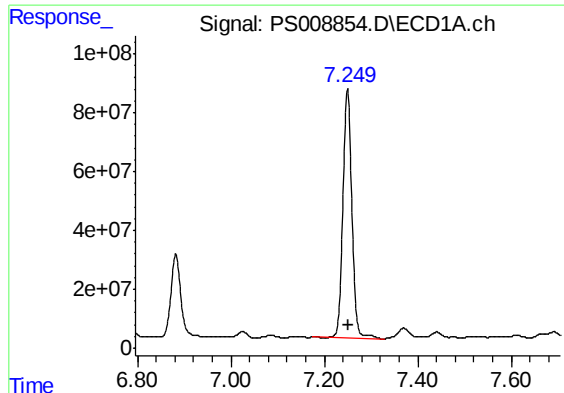

#4 2,4-DCAA


R.T.: 7.249 min
Delta R.T.: -0.002 min
Response: 1127373967
Conc: 525.26 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB126813BL

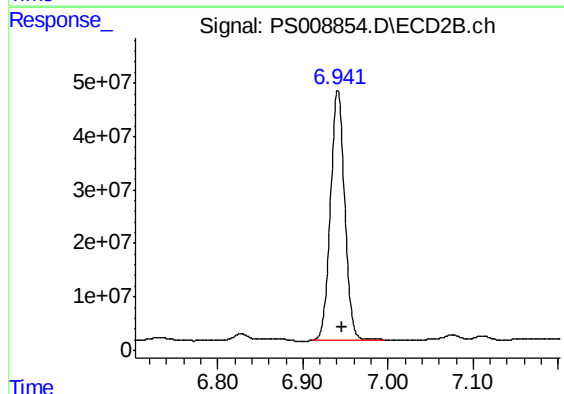


#4 2,4-DCAA

R.T.: 6.941 min
Delta R.T.: -0.006 min
Response: 539949935
Conc: 582.58 ng/ml

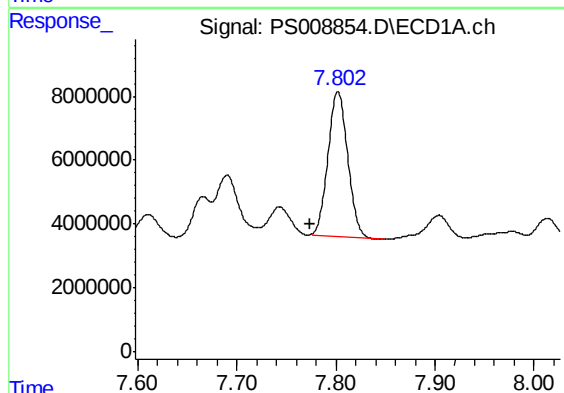


#7 MCPA

R.T.: 7.802 min
Delta R.T.: 0.029 min
Response: 62775335
Conc: 7.31 ug/ml

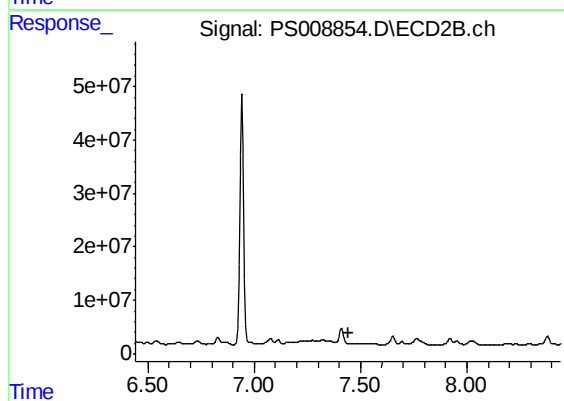

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 7.441 min
Response: 0
Conc: N.D.

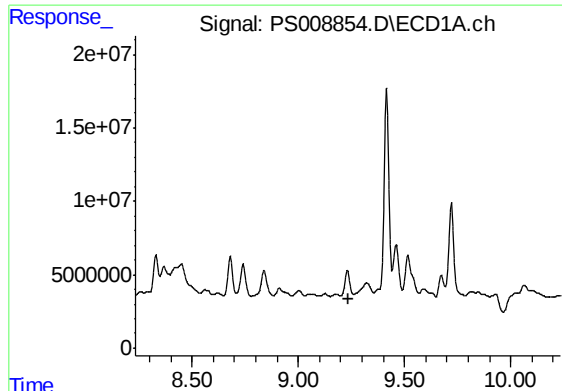

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 9.234 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB126813BL

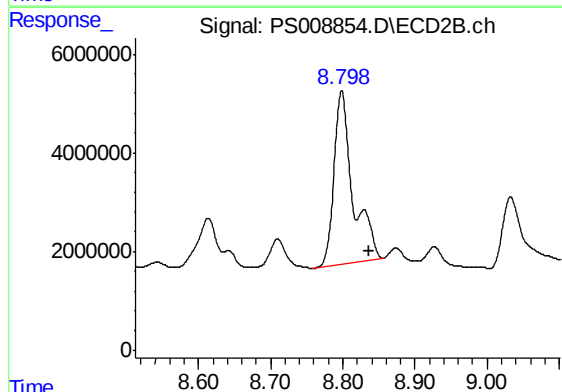


#11 2,4,5-TP (SILVEX)

R.T.: 8.799 min
Delta R.T.: -0.038 min
Response: 64102543
Conc: 12.51 ng/ml

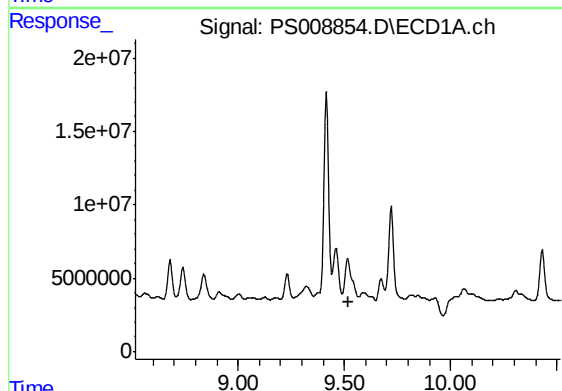


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.517 min
Response: 0
Conc: N.D.

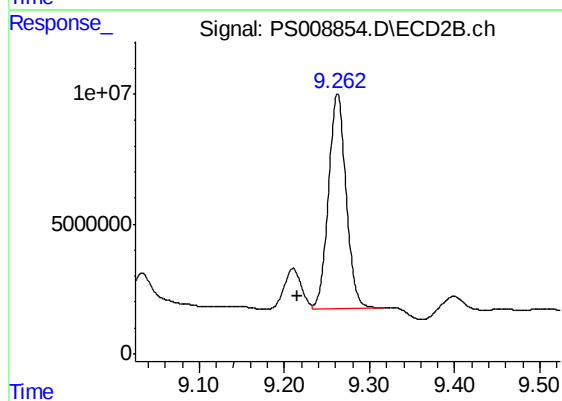

#12 2,4,5-T


R.T.: 9.262 min
Delta R.T.: 0.047 min
Response: 118463185
Conc: 22.92 ng/ml

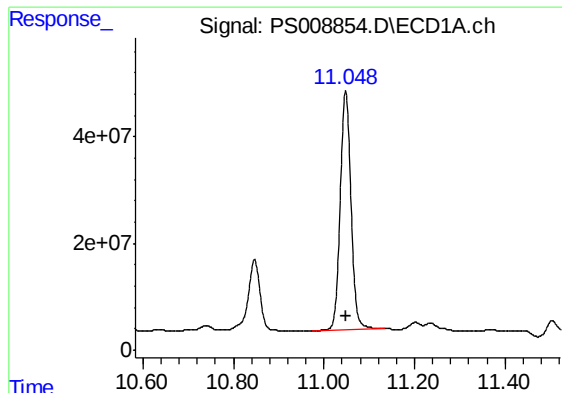

#15 Picloram


R.T.: 11.048 min
Delta R.T.: -0.002 min
Response: 738538500
Conc: 48.77 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB126813BL

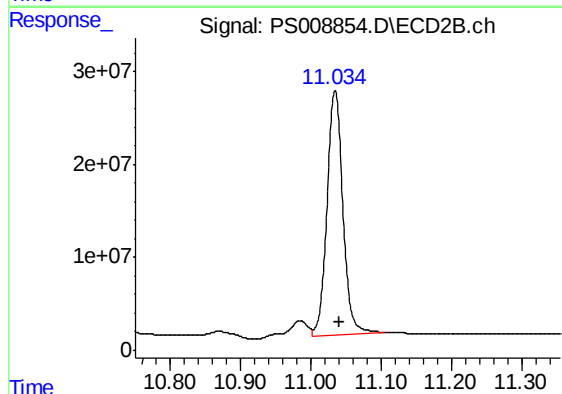


#15 Picloram

R.T.: 11.034 min
Delta R.T.: -0.007 min
Response: 413354043
Conc: 54.76 ng/ml

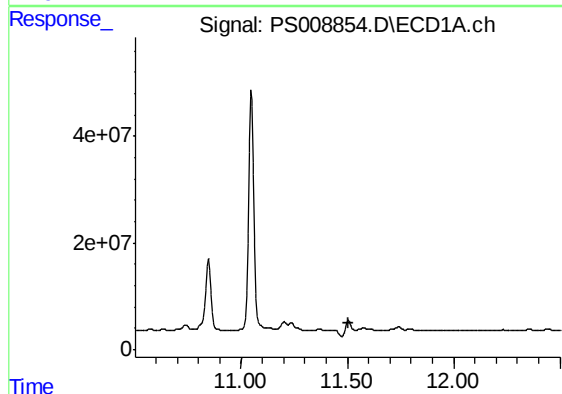

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.503 min
Response: 0
Conc: N.D.

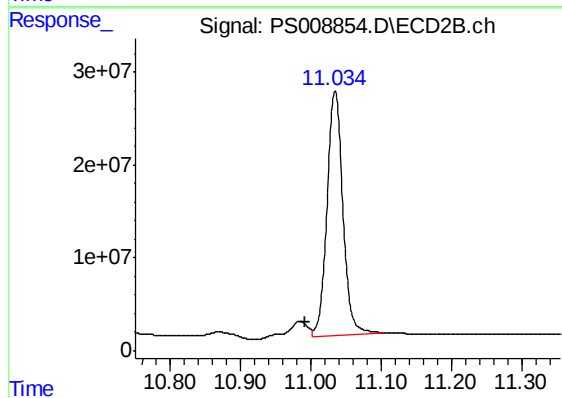

#16 DCPA

R.T.: 11.034 min
Delta R.T.: 0.042 min
Response: 413354043
Conc: 63.55 ng/ml