

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021720\
 Data File : PS008857.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Feb 2020 11:01
 Operator : DD\AJ
 Sample : L1523-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 COMP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 17 14:18:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 05 02:36:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.248	6.942	855.1E6	403.5E6	398.392	435.304
Target Compounds							
1) T	Dalapon	0.000	2.593	0	245.5E6	N.D.	204.693
2) T	3,5-DICHL...	0.000	6.117	0	61230582	N.D.	44.503
7) T	MCPA	7.800	7.410	59169408	77425635	6.888	18.551 #
11) T	2,4,5-TP ...	0.000	8.800	0	48194728	N.D.	9.403
12) T	2,4,5-T	9.458	0.000	121.9E6	0	11.073	N.D. #
15) T	Picloram	0.000	11.041	0	46320160	N.D.	6.137
16) T	DCPA	0.000	11.041	0	46320160	N.D.	7.122



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021720\
Data File : PS008857.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Feb 2020 11:01
Operator : DD\AJ
Sample : L1523-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
COMP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 17 14:18:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
Quant Title : 8080.M
QLast Update : Wed Feb 05 02:36:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

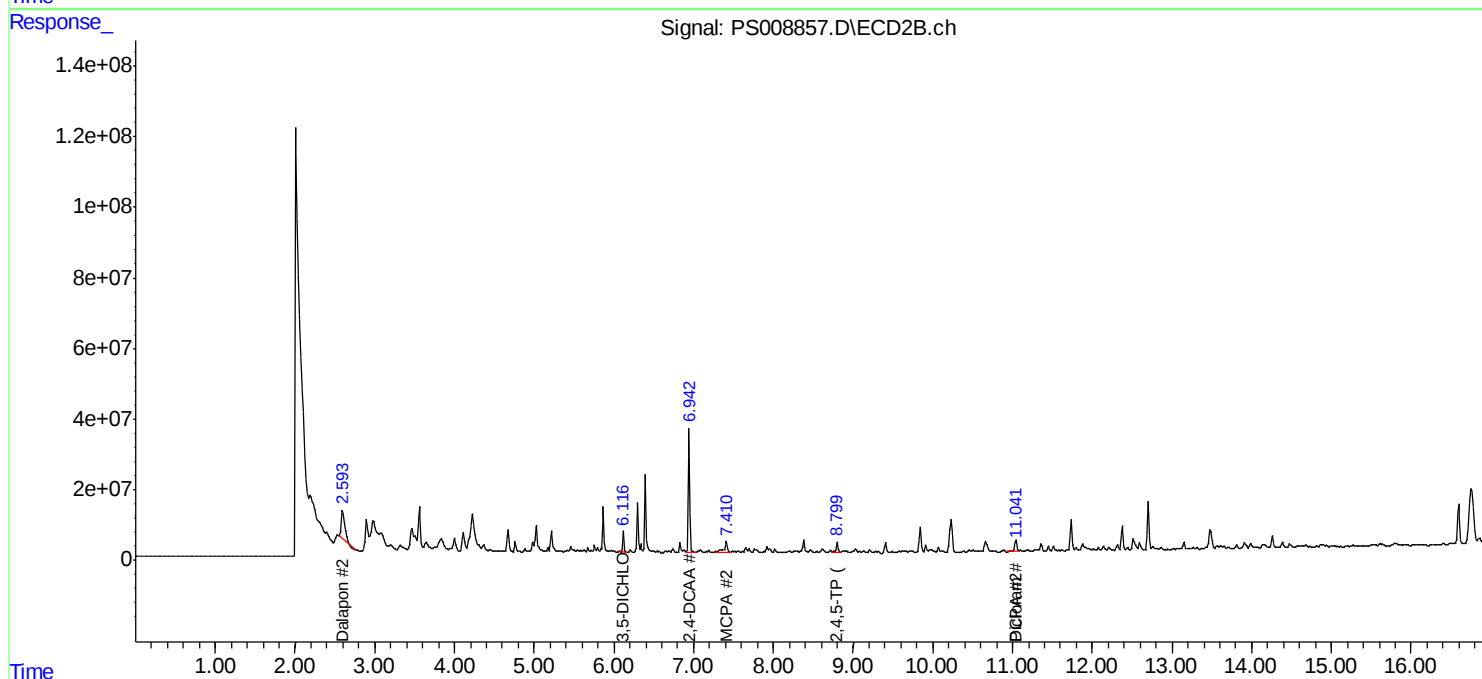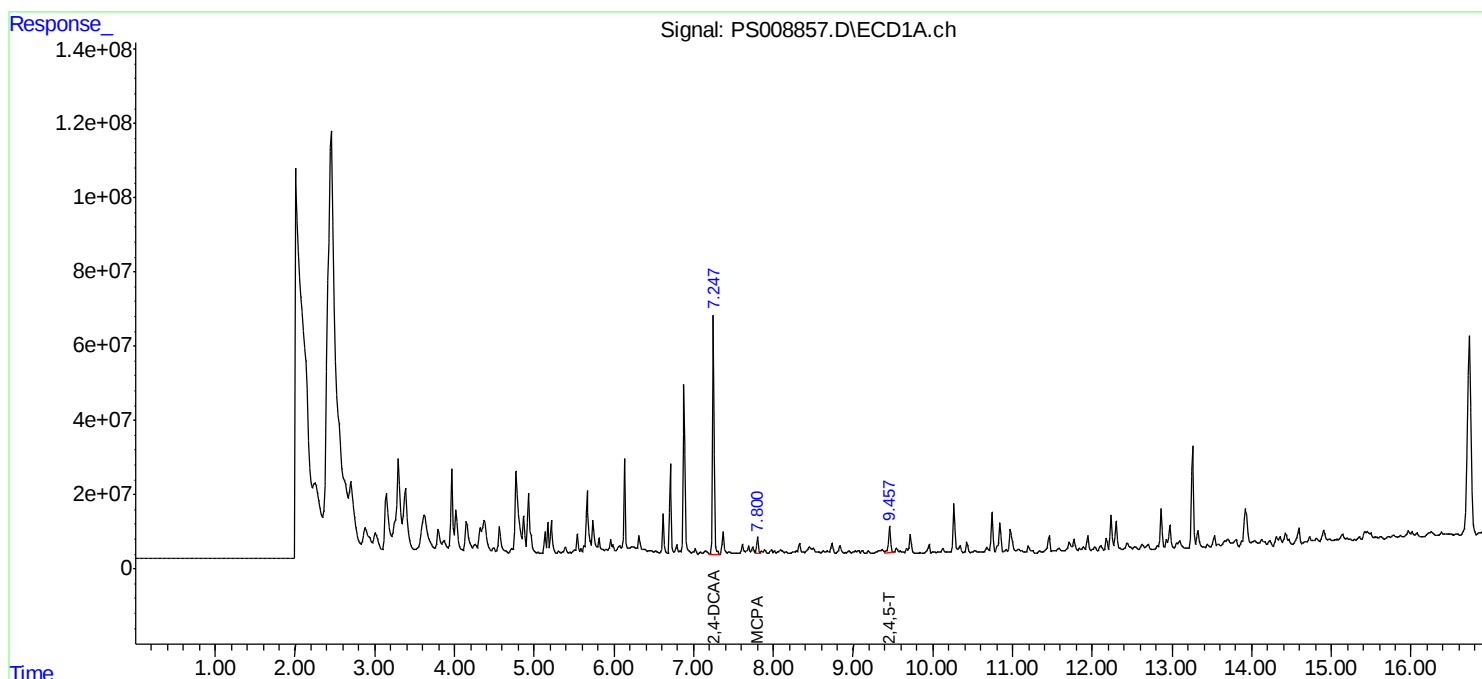


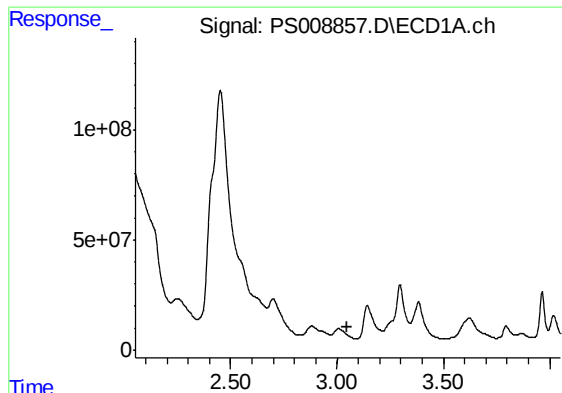

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 3.051 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-1

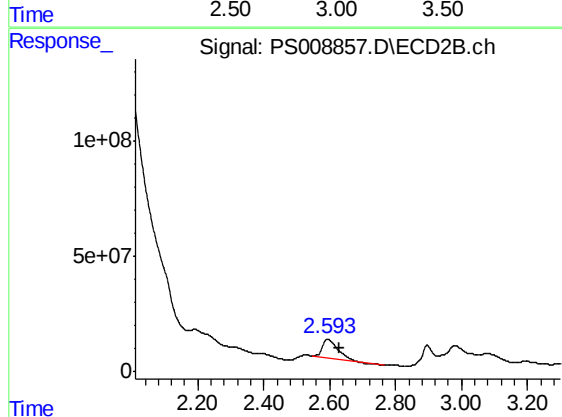


#1 Dalapon

R.T.: 2.593 min
Delta R.T.: -0.038 min
Response: 245492500
Conc: 204.69 ng/ml

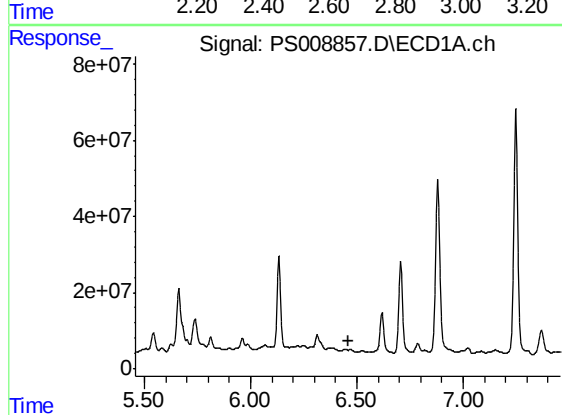


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.458 min
Response: 0
Conc: N.D.

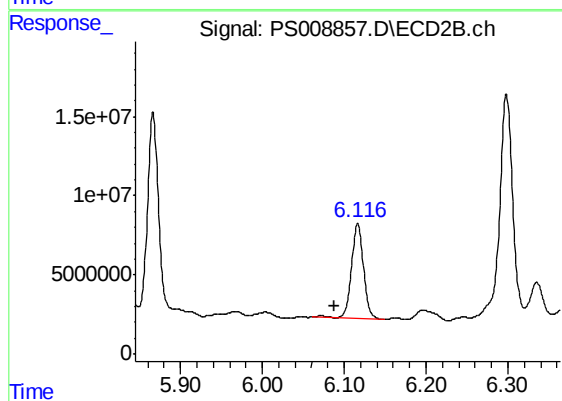

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.117 min
Delta R.T.: 0.028 min
Response: 61230582
Conc: 44.50 ng/ml

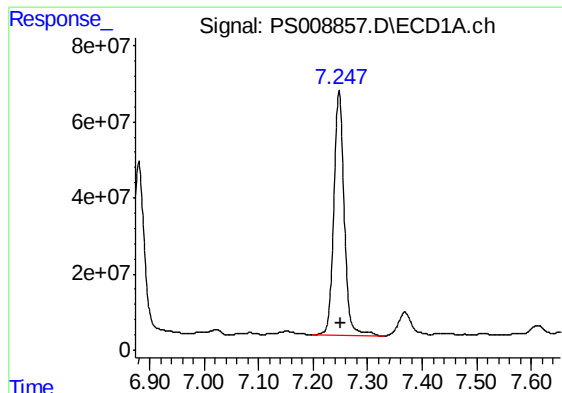

#4 2,4-DCAA


R.T.: 7.248 min
Delta R.T.: -0.004 min
Response: 855072377
Conc: 398.39 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-1

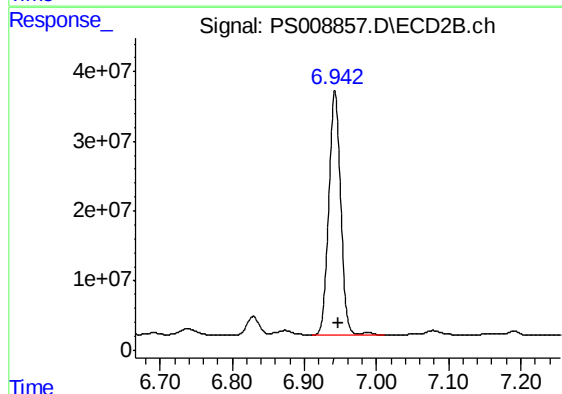


#4 2,4-DCAA

R.T.: 6.942 min
Delta R.T.: -0.004 min
Response: 403450697
Conc: 435.30 ng/ml

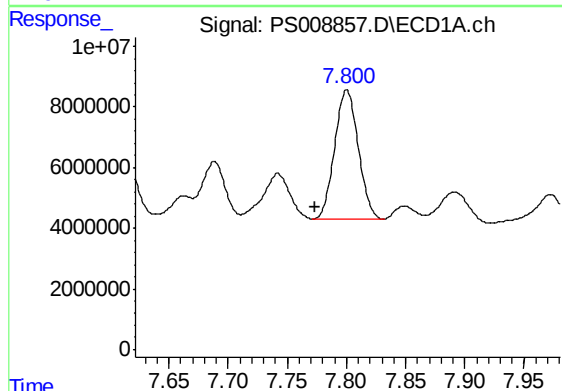


#7 MCPA

R.T.: 7.800 min
Delta R.T.: 0.027 min
Response: 59169408
Conc: 6.89 ug/ml

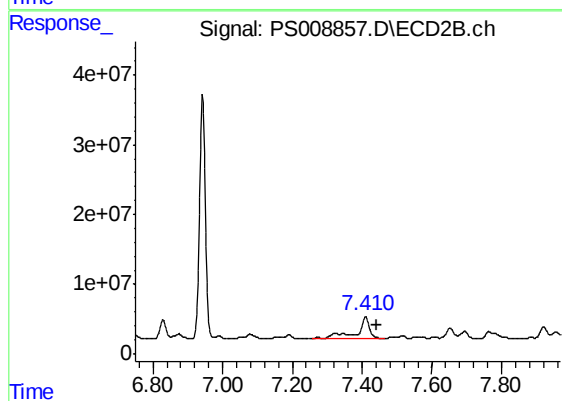

#7 MCPA


R.T.: 7.410 min
Delta R.T.: -0.030 min
Response: 77425635
Conc: 18.55 ug/ml

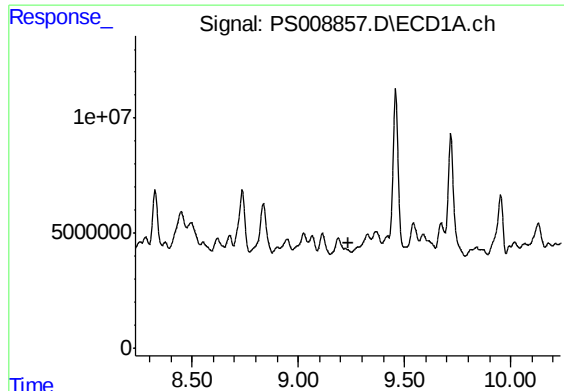

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 9.234 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-1

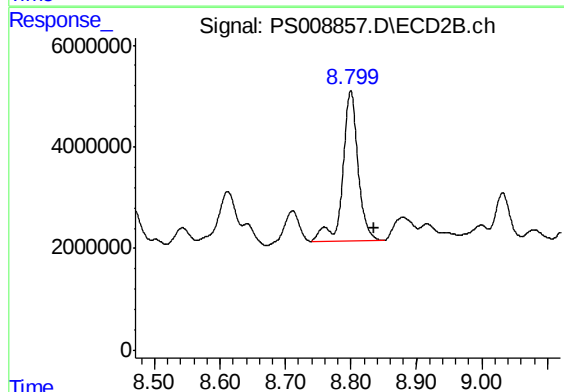


#11 2,4,5-TP (SILVEX)

R.T.: 8.800 min
Delta R.T.: -0.037 min
Response: 48194728
Conc: 9.40 ng/ml

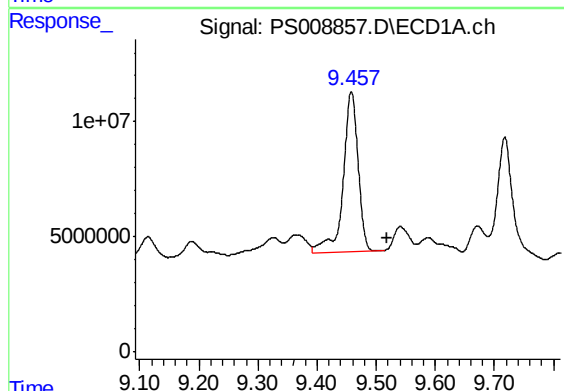


#12 2,4,5-T

R.T.: 9.458 min
Delta R.T.: -0.059 min
Response: 121867577
Conc: 11.07 ng/ml

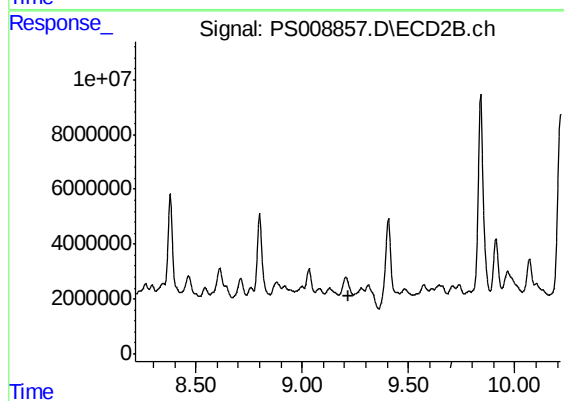

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 9.216 min
Response: 0
Conc: N.D.

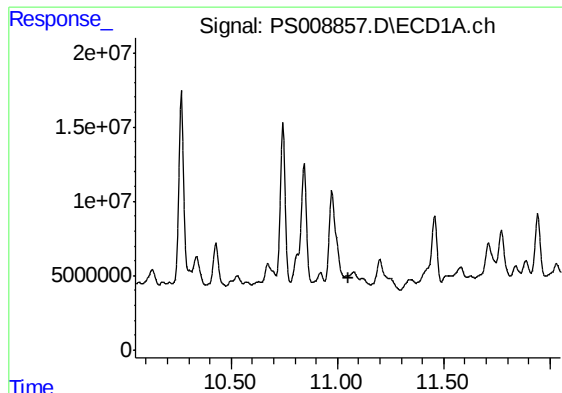

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 11.050 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-1

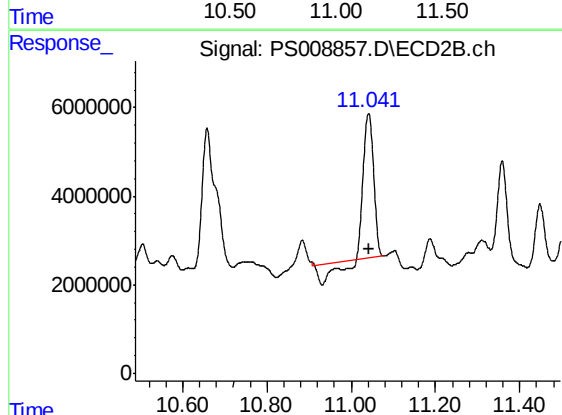


#15 Picloram

R.T.: 11.041 min
Delta R.T.: 0.000 min
Response: 46320160
Conc: 6.14 ng/ml

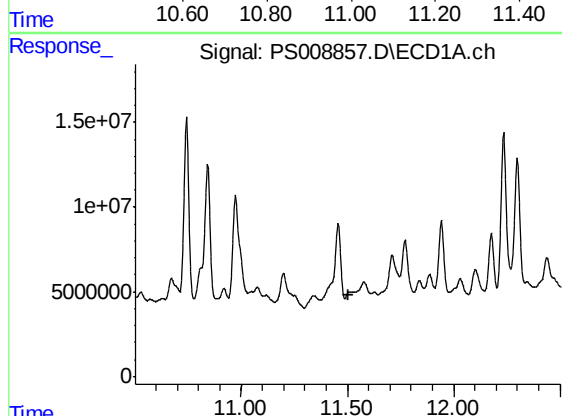

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.503 min
Response: 0
Conc: N.D.

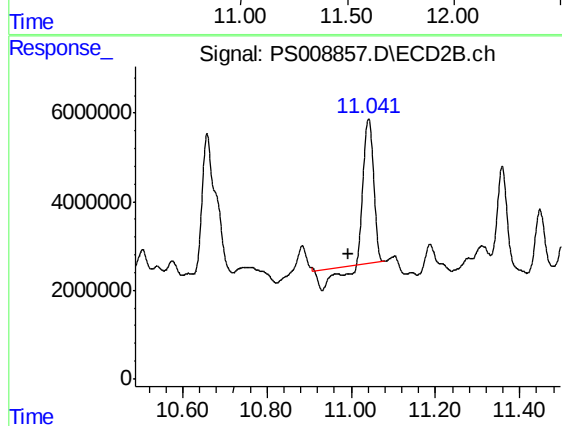

#16 DCPA

R.T.: 11.041 min
Delta R.T.: 0.049 min
Response: 46320160
Conc: 7.12 ng/ml