

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021720\
 Data File : PS008861.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Feb 2020 12:32
 Operator : DD\AJ
 Sample : L1523-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 COMP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 17 14:19:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 05 02:36:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.247	6.942	834.3E6	366.7E6	388.707	395.622
Target Compounds							
2) T	3,5-DICHL...	0.000	6.116	0	127.2E6	N.D.	92.470
7) T	MCPA	7.799	7.410	59749600	2073418	6.955	<MDL #
12) T	2,4,5-T	9.456	0.000	87612977	0	7.960	N.D. #
16) T	DCPA	11.552	0.000	90221520	0	6.436	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021720\
Data File : PS008861.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Feb 2020 12:32
Operator : DD\AJ
Sample : L1523-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
COMP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 17 14:19:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
Quant Title : 8080.M
QLast Update : Wed Feb 05 02:36:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

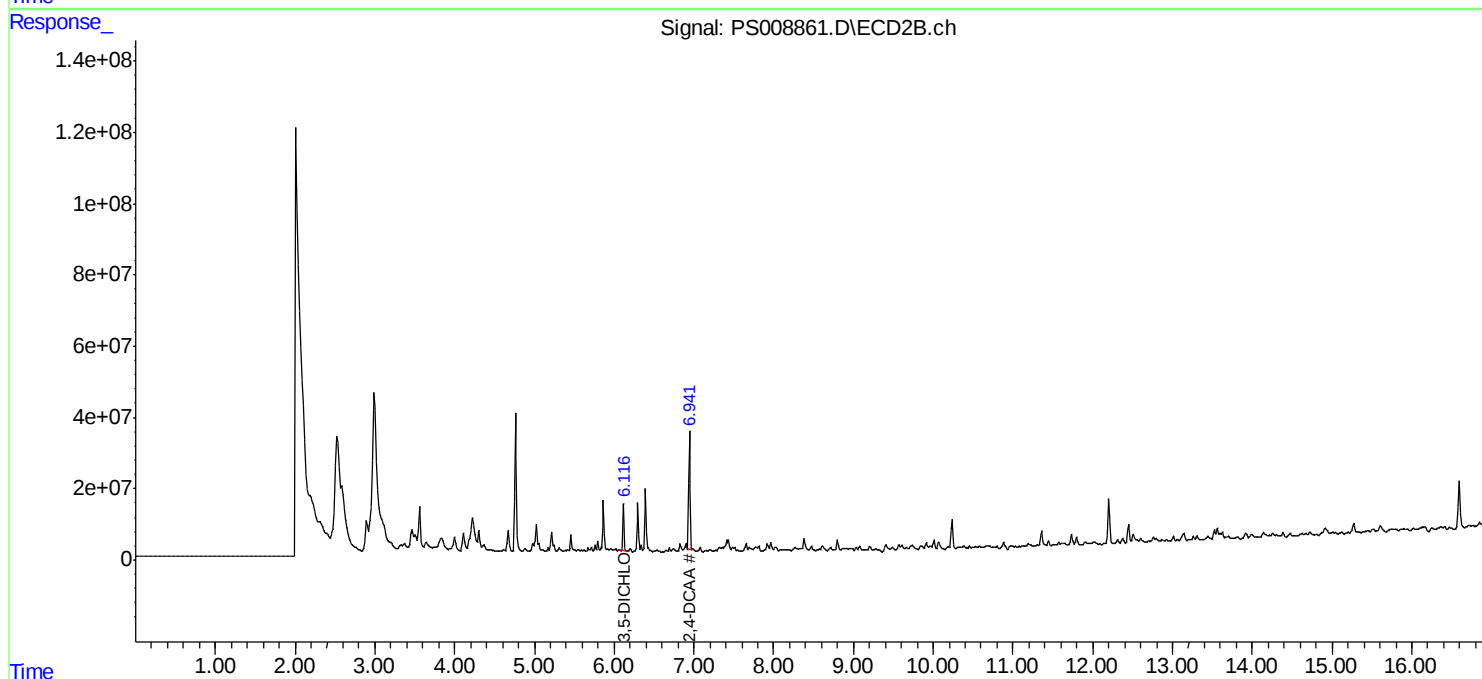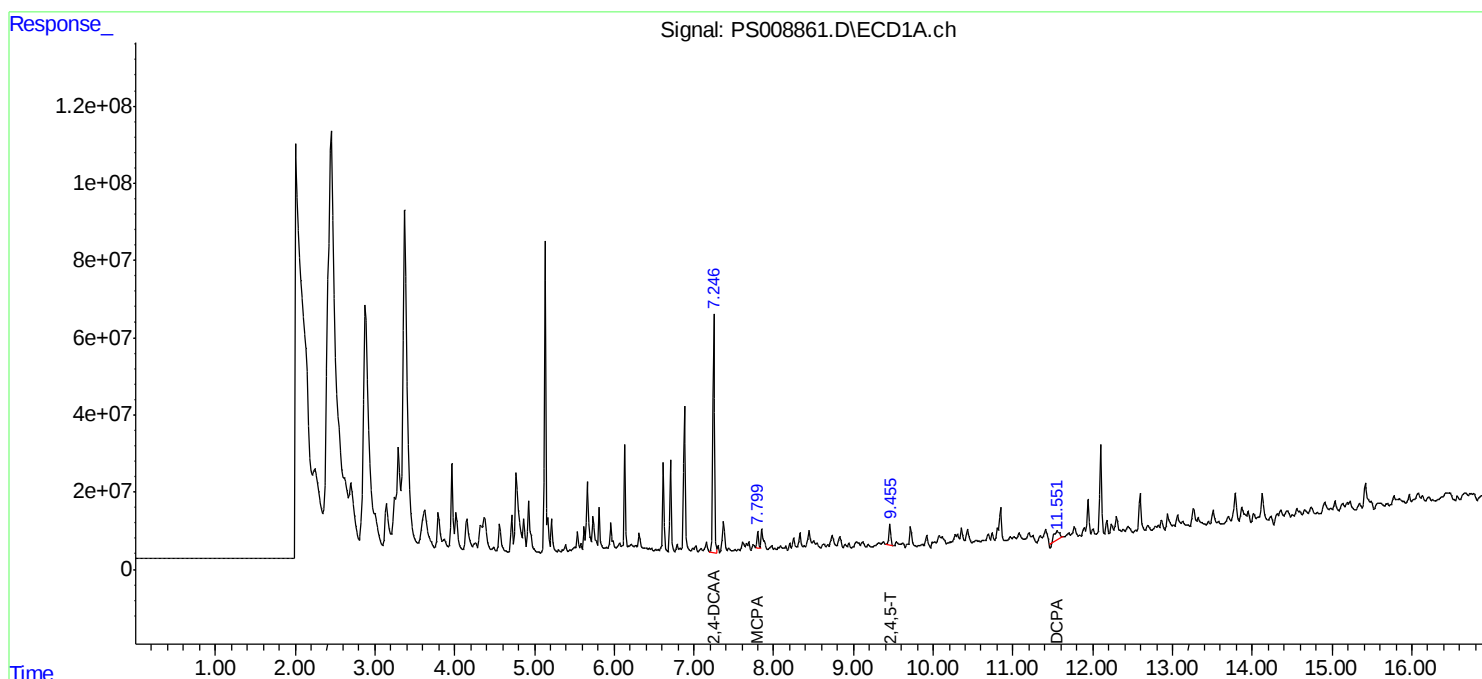


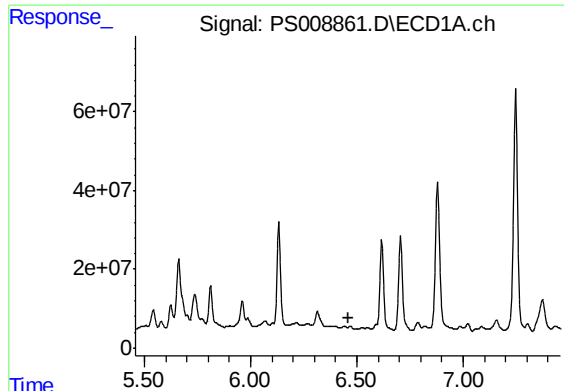

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.458 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-3

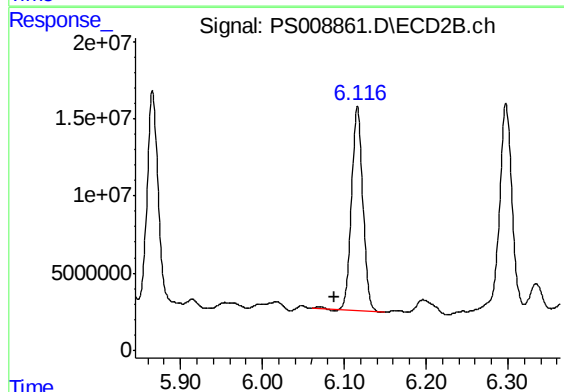


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.116 min
Delta R.T.: 0.028 min
Response: 127228415
Conc: 92.47 ng/ml

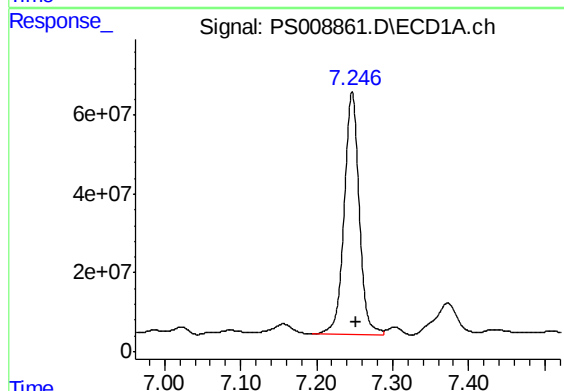


#4 2,4-DCAA

R.T.: 7.247 min
Delta R.T.: -0.005 min
Response: 834284868
Conc: 388.71 ng/ml

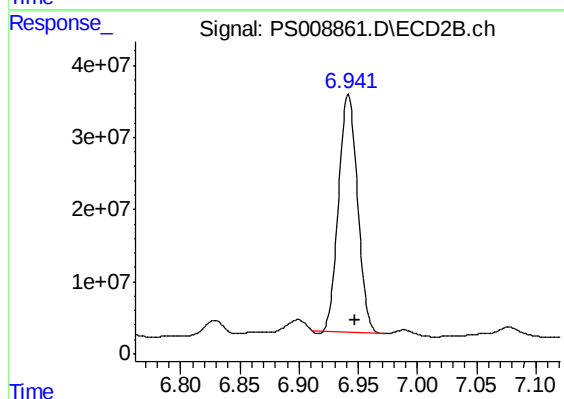

#4 2,4-DCAA


R.T.: 6.942 min
Delta R.T.: -0.005 min
Response: 366672401
Conc: 395.62 ng/ml

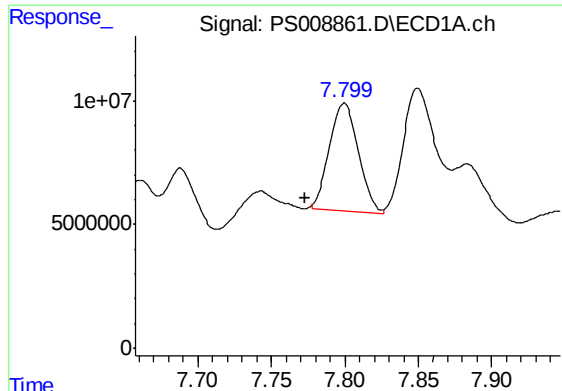

#7 MCPA


R.T.: 7.799 min
Delta R.T.: 0.026 min
Response: 59749600
Conc: 6.96 ug/ml

Instrument :
ECD_S
ClientSampleId :
COMP-3

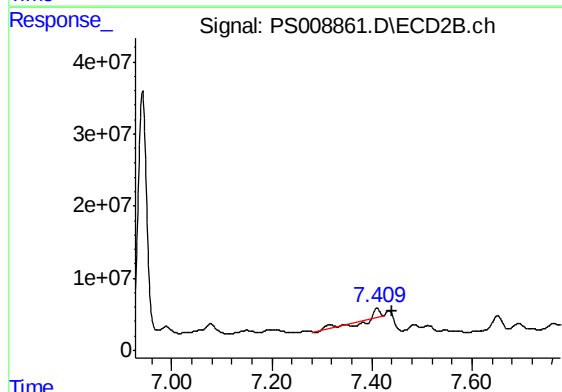


#7 MCPA

R.T.: 7.410 min
Delta R.T.: -0.031 min
Response: 2073418
Conc: N.D.

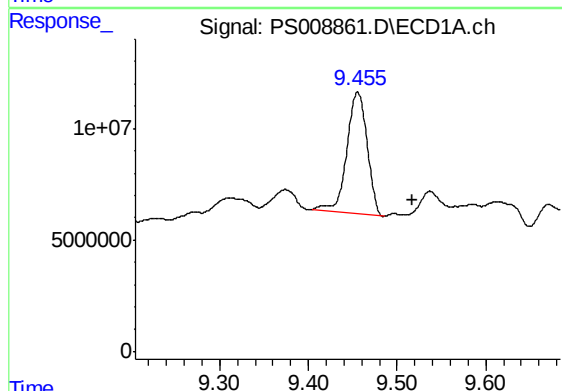


#12 2,4,5-T

R.T.: 9.456 min
Delta R.T.: -0.062 min
Response: 87612977
Conc: 7.96 ng/ml

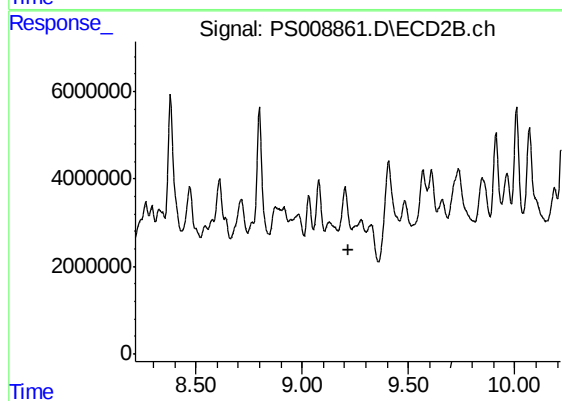

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 9.216 min
Response: 0
Conc: N.D.

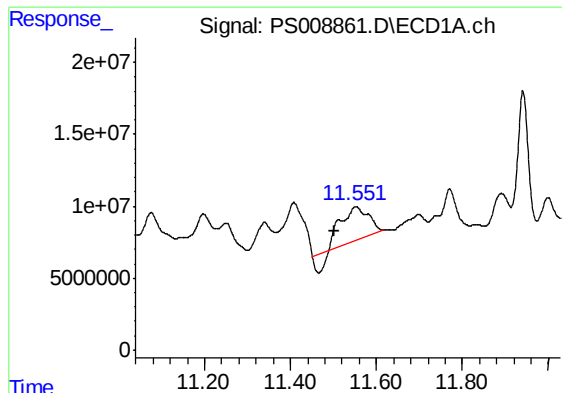

#16 DCPA

R.T.: 11.552 min
Delta R.T.: 0.049 min
Response: 90221520
Conc: 6.44 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-3

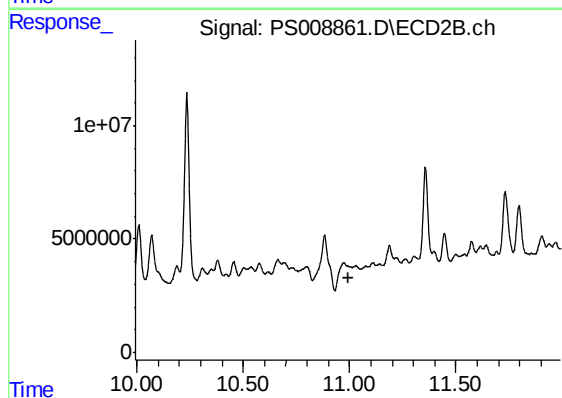

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.992 min
Response: 0
Conc: N.D.