

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021720\
 Data File : PS008862.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Feb 2020 12:55
 Operator : DD\AJ
 Sample : L1528-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 FK-GF-02-048-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 17 14:19:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 05 02:36:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.247	6.942	572.2E6	222.3E6	266.587	239.855
Target Compounds							
2) T	3,5-DICHL...	0.000	6.117	0	127.7E6	N.D.	92.804
7) T	MCPA	7.800	0.000	84320507	0	9.816	N.D. #
9) T	2,4-D	8.373	0.000	161.2E6	0	75.340	N.D. #
11) T	2,4,5-TP ...	0.000	8.798	0	51937493	N.D.	10.134
12) T	2,4,5-T	9.456	0.000	128.8E6	0	11.707	N.D. #
14) T	DINOSEB	0.000	10.068	0	63952155	N.D.	17.411
16) T	DCPA	11.560	0.000	103.7E6	0	7.394	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021720\
Data File : PS008862.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Feb 2020 12:55
Operator : DD\AJ
Sample : L1528-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
FK-GF-02-048-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 17 14:19:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
Quant Title : 8080.M
QLast Update : Wed Feb 05 02:36:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

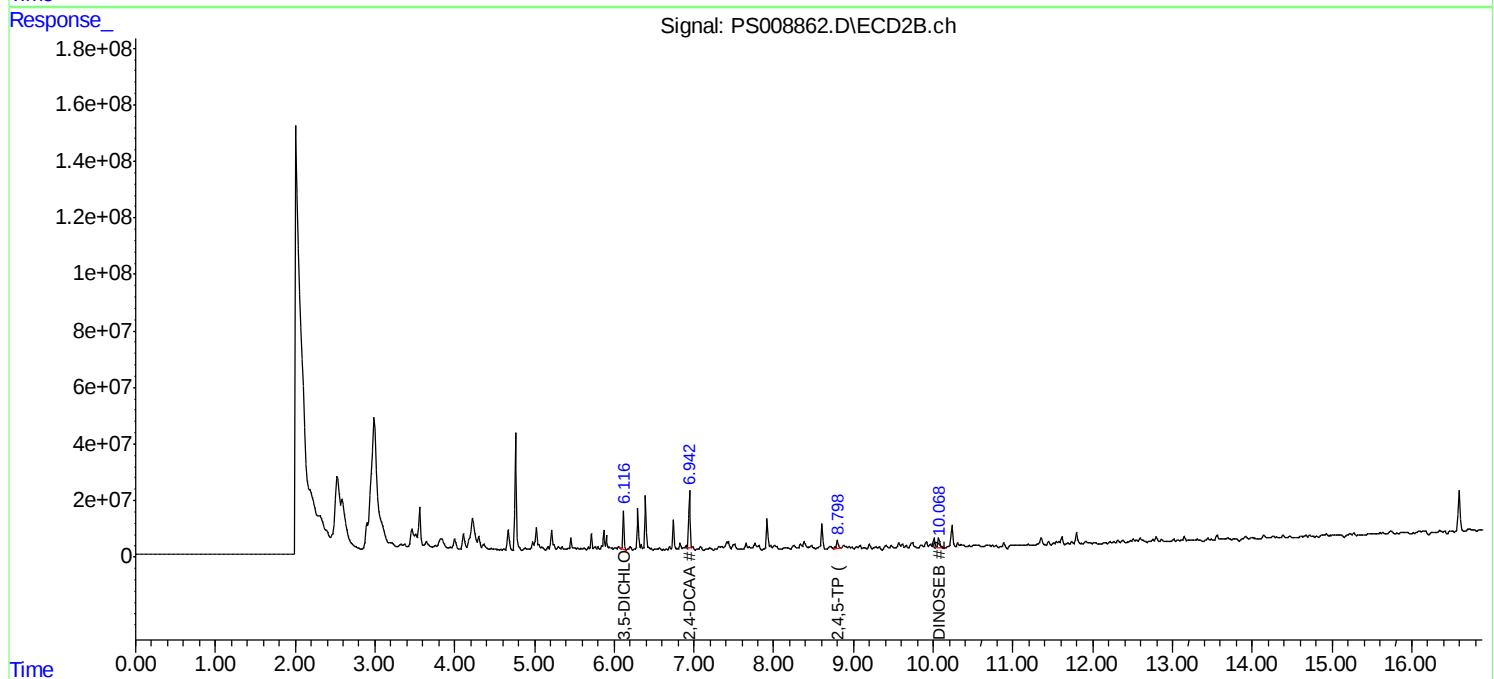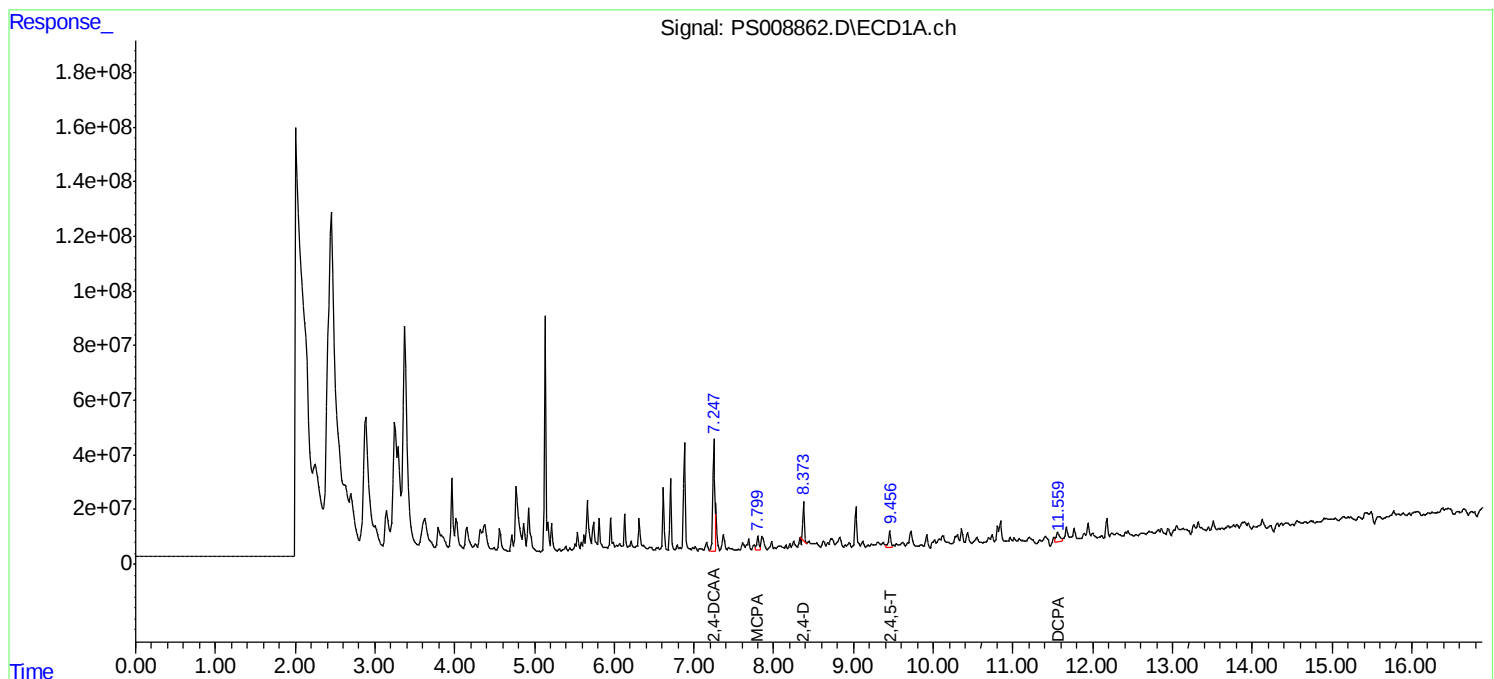


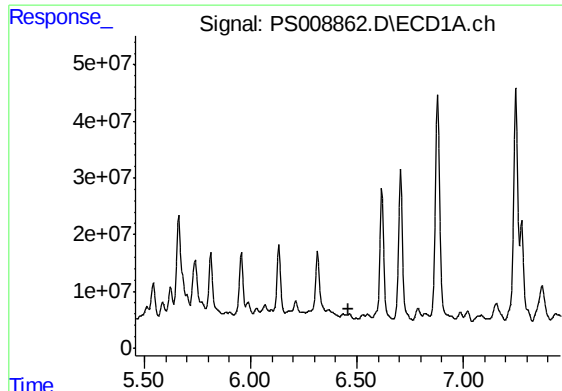

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.458 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FK-GF-02-048-A

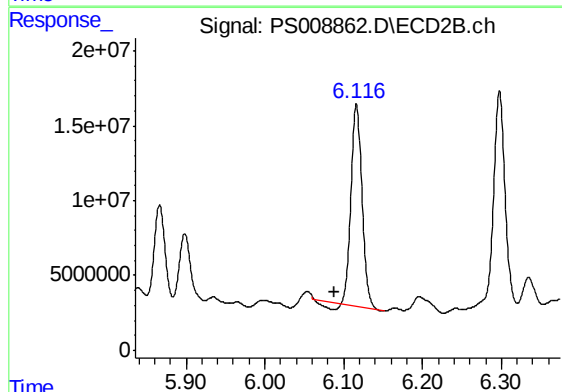


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.117 min
Delta R.T.: 0.028 min
Response: 127687310
Conc: 92.80 ng/ml

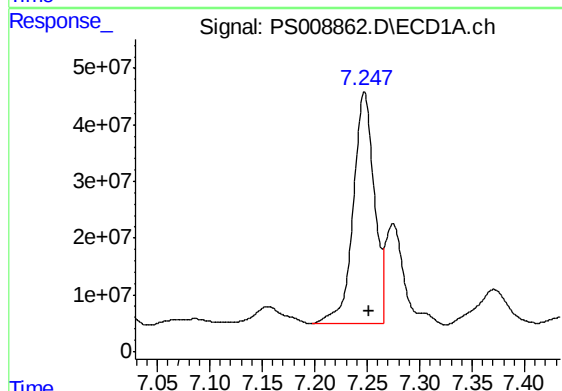


#4 2,4-DCAA

R.T.: 7.247 min
Delta R.T.: -0.004 min
Response: 572177403
Conc: 266.59 ng/ml

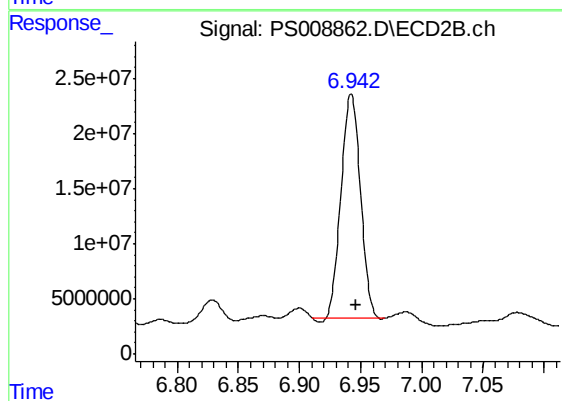

#4 2,4-DCAA


R.T.: 6.942 min
Delta R.T.: -0.004 min
Response: 222303246
Conc: 239.85 ng/ml

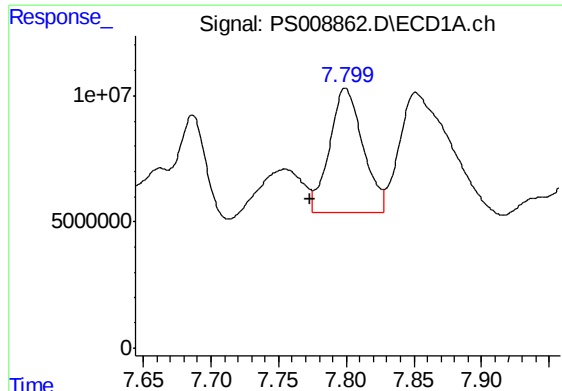

#7 MCPA


R.T.: 7.800 min
Delta R.T.: 0.026 min
Response: 84320507
Conc: 9.82 ug/ml

Instrument :
ECD_S
ClientSampleId :
FK-GF-02-048-A

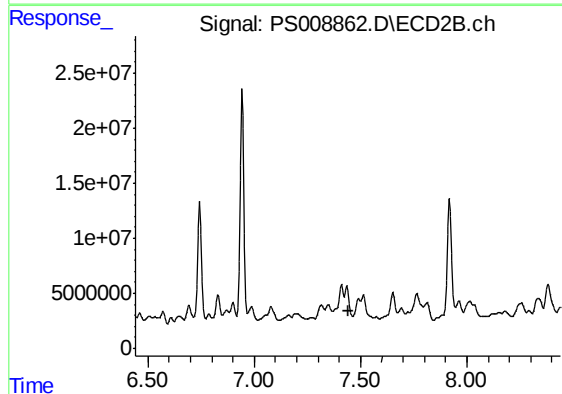


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.441 min
Response: 0
Conc: N.D.

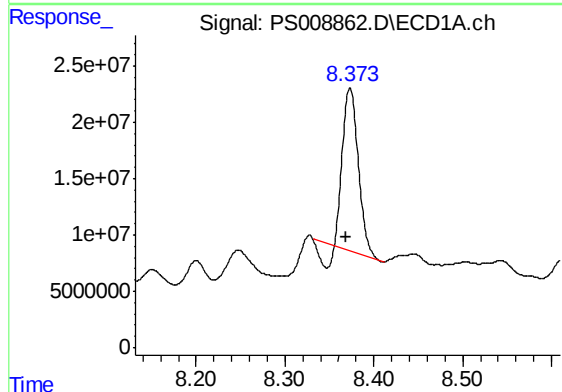


#9 2,4-D

R.T.: 8.373 min
Delta R.T.: 0.005 min
Response: 161231964
Conc: 75.34 ng/ml

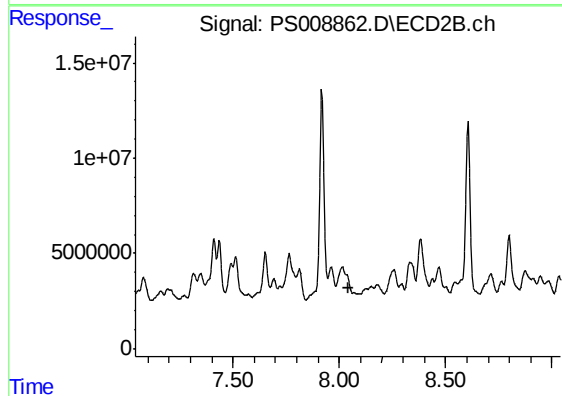

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 8.041 min
Response: 0
Conc: N.D.

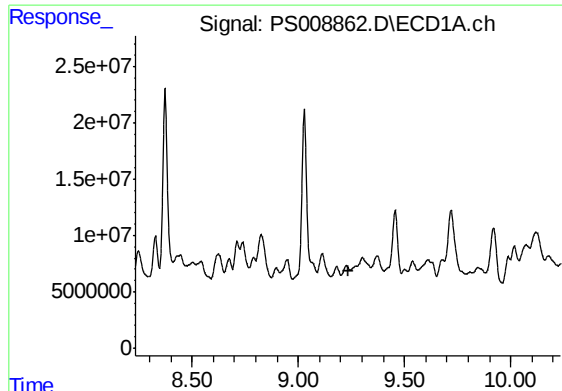

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 9.234 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FK-GF-02-048-A

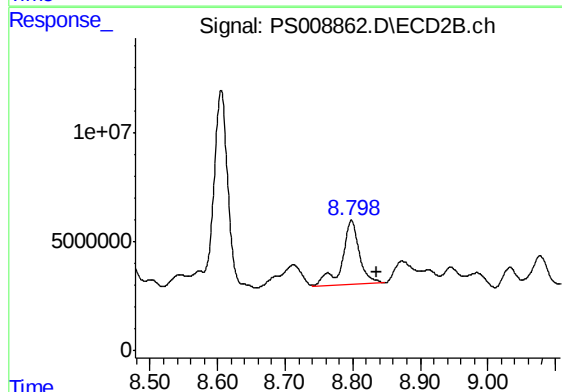


#11 2,4,5-TP (SILVEX)

R.T.: 8.798 min
Delta R.T.: -0.038 min
Response: 51937493
Conc: 10.13 ng/ml

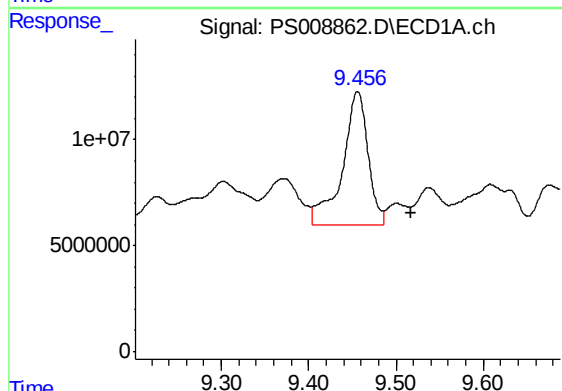


#12 2,4,5-T

R.T.: 9.456 min
Delta R.T.: -0.061 min
Response: 128848315
Conc: 11.71 ng/ml

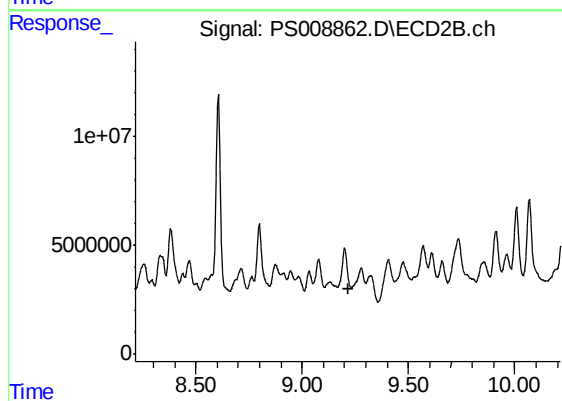

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 9.216 min
Response: 0
Conc: N.D.

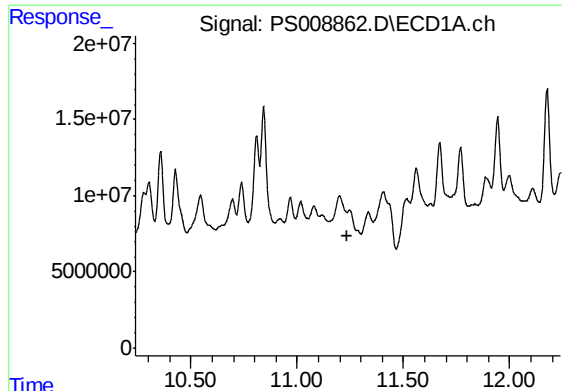

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 11.239 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FK-GF-02-048-A

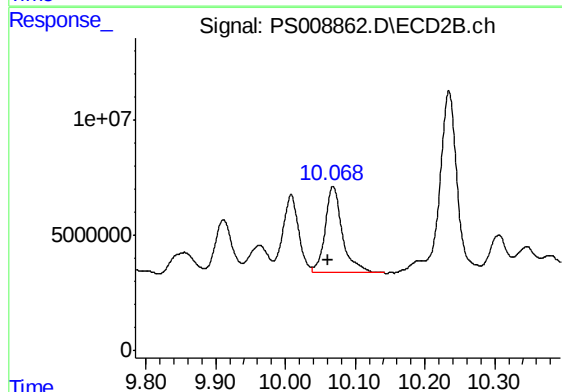


#14 DINOSEB

R.T.: 10.068 min
Delta R.T.: 0.008 min
Response: 63952155
Conc: 17.41 ng/ml

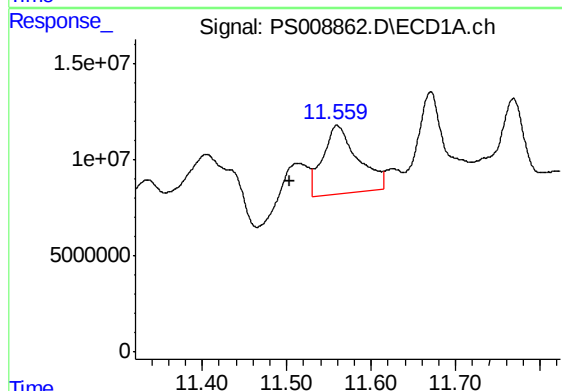

#16 DCPA

R.T.: 11.560 min
Delta R.T.: 0.057 min
Response: 103659889
Conc: 7.39 ng/ml

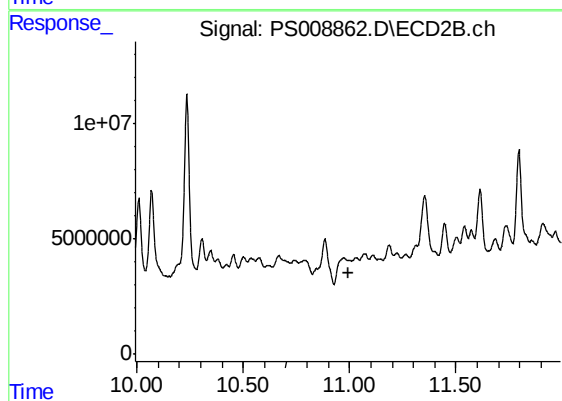

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.992 min
Response: 0
Conc: N.D.