

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021720\
 Data File : PS008863.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Feb 2020 13:18
 Operator : DD\AJ
 Sample : L1528-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 FK-GF-02-048-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 17 14:19:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 05 02:36:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.247	6.942	548.4E6	198.6E6	255.516	214.298
Target Compounds							
2) T	3,5-DICHL...	0.000	6.117	0	148.6E6	N.D.	108.034
7) T	MCPA	7.800	7.433	66318515	103.0E6	7.720	24.679 #
12) T	2,4,5-T	9.456	0.000	112.5E6	0	10.218	N.D. #
13) T	2,4-DB	10.074	0.000	170.8E6	0	104.984	N.D. #
14) T	DINOSEB	0.000	10.009	0	46305911	N.D.	12.607
16) T	DCPA	11.514	0.000	26435130	0	1.886	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021720\
Data File : PS008863.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Feb 2020 13:18
Operator : DD\AJ
Sample : L1528-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
FK-GF-02-048-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 17 14:19:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
Quant Title : 8080.M
QLast Update : Wed Feb 05 02:36:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

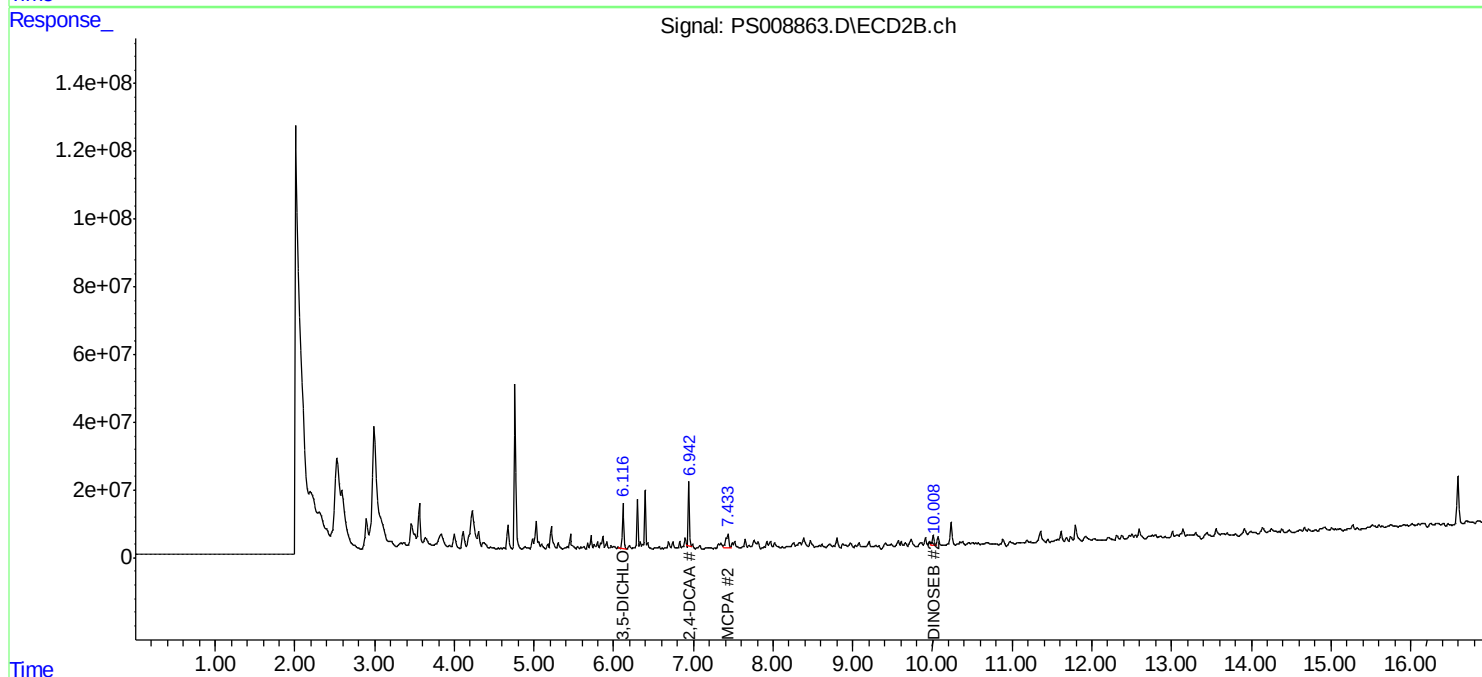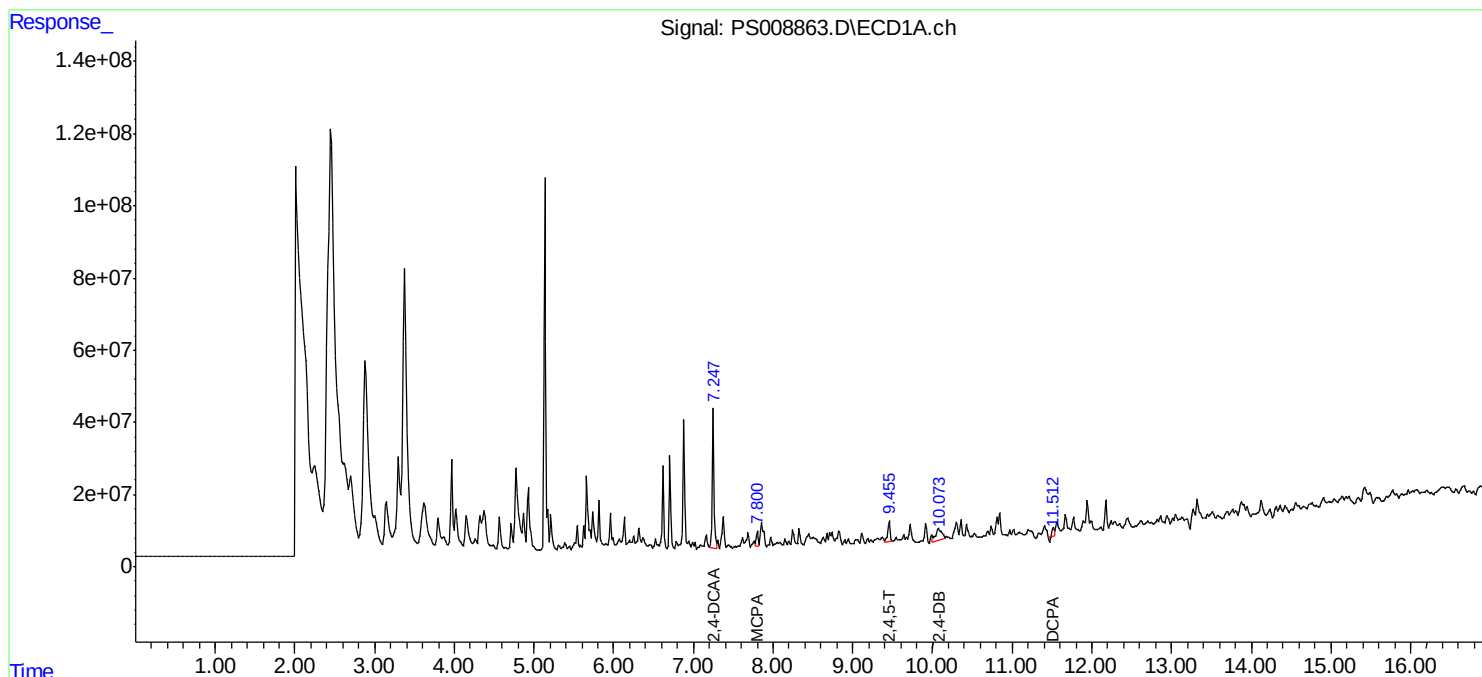


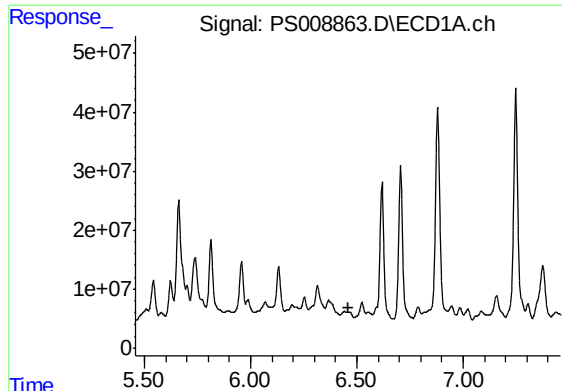

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.458 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FK-GF-02-048-B

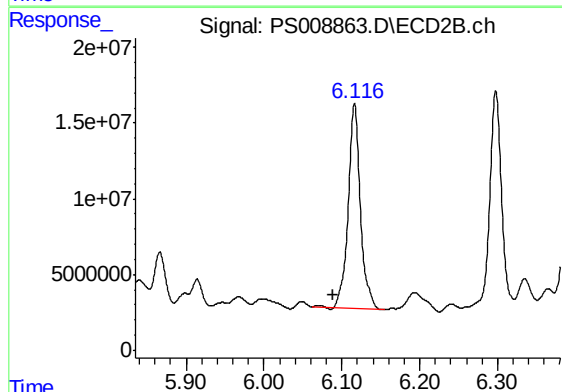


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.117 min
Delta R.T.: 0.028 min
Response: 148642695
Conc: 108.03 ng/ml

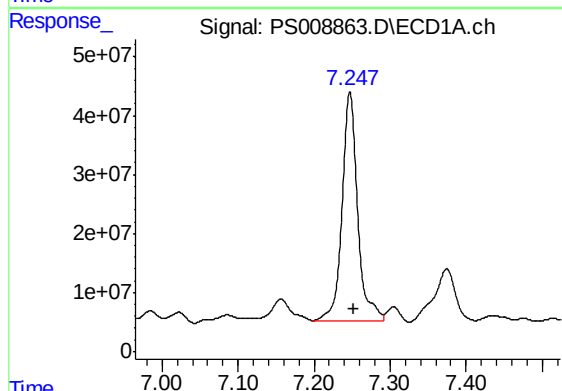


#4 2,4-DCAA

R.T.: 7.247 min
Delta R.T.: -0.005 min
Response: 548416790
Conc: 255.52 ng/ml

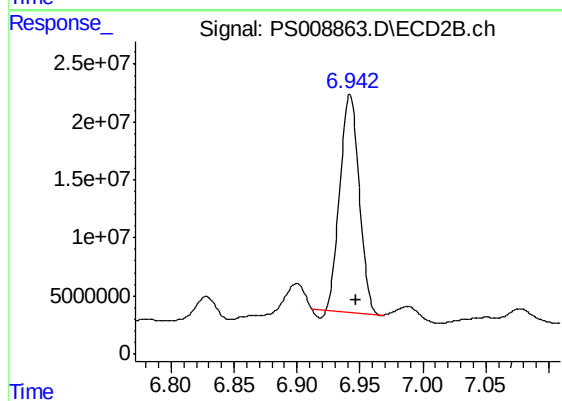

#4 2,4-DCAA


R.T.: 6.942 min
Delta R.T.: -0.005 min
Response: 198616203
Conc: 214.30 ng/ml

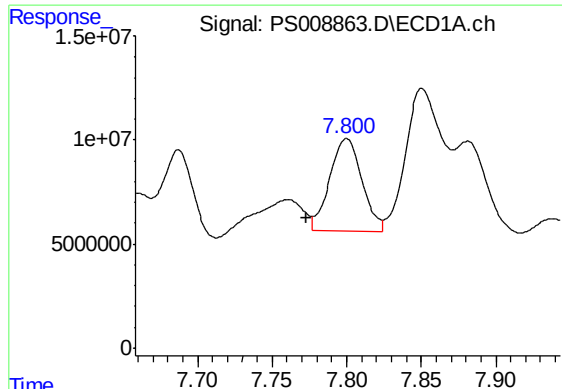

#7 MCPA


R.T.: 7.800 min
Delta R.T.: 0.027 min
Response: 66318515
Conc: 7.72 ug/ml

Instrument :
ECD_S
ClientSampleId :
FK-GF-02-048-B

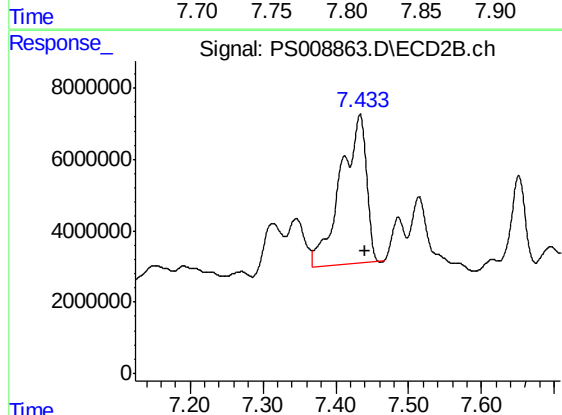


#7 MCPA

R.T.: 7.433 min
Delta R.T.: -0.008 min
Response: 102999863
Conc: 24.68 ug/ml

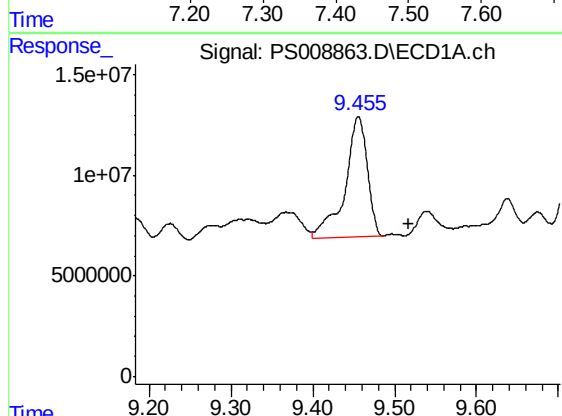


#12 2,4,5-T

R.T.: 9.456 min
Delta R.T.: -0.062 min
Response: 112465172
Conc: 10.22 ng/ml

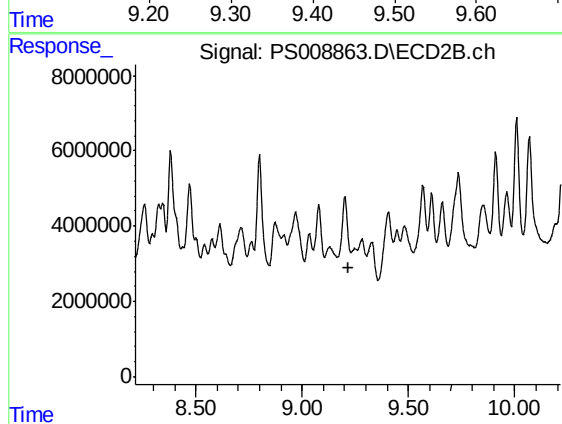

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 9.216 min
Response: 0
Conc: N.D.

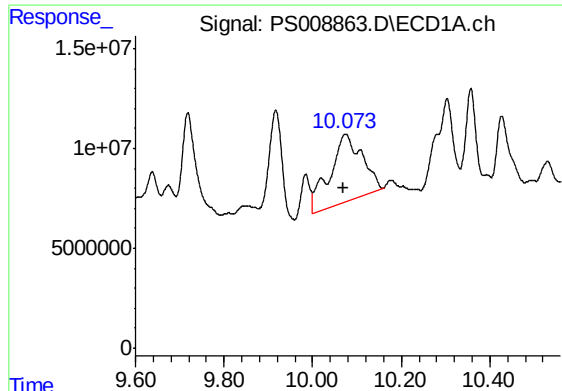

#13 2,4-DB


R.T.: 10.074 min
Delta R.T.: 0.003 min
Response: 170766128
Conc: 104.98 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-GF-02-048-B

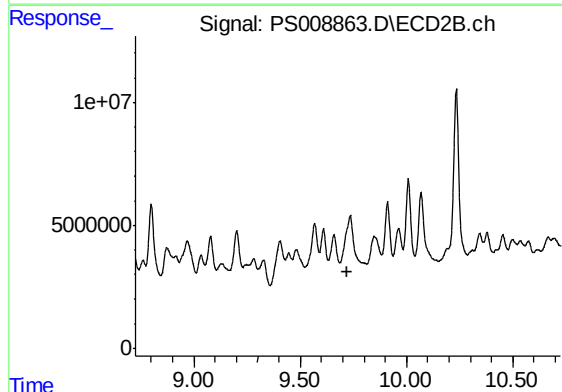


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.724 min
Response: 0
Conc: N.D.

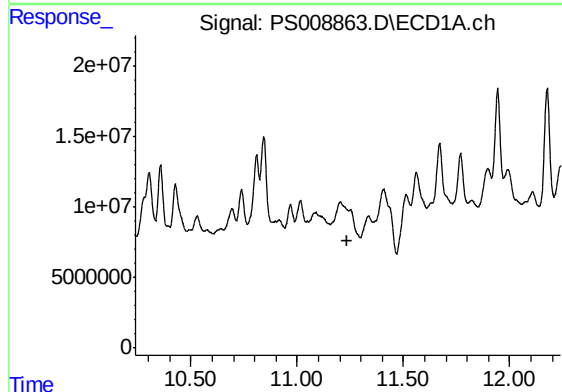


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.239 min
Response: 0
Conc: N.D.

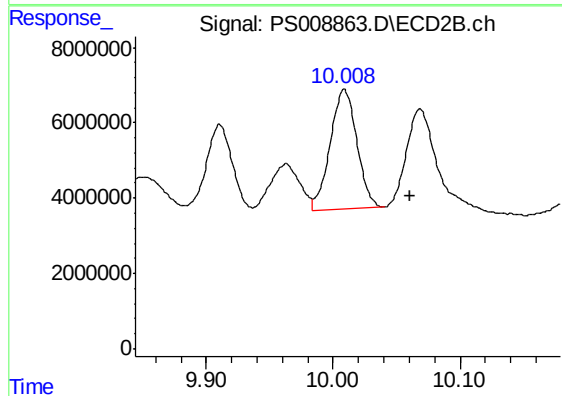

#14 DINOSEB


R.T.: 10.009 min
Delta R.T.: -0.052 min
Response: 46305911
Conc: 12.61 ng/ml

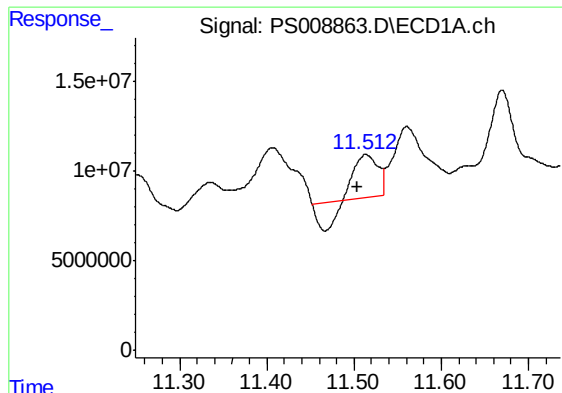

#16 DCPA

R.T.: 11.514 min
Delta R.T.: 0.010 min
Response: 26435130
Conc: 1.89 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-GF-02-048-B

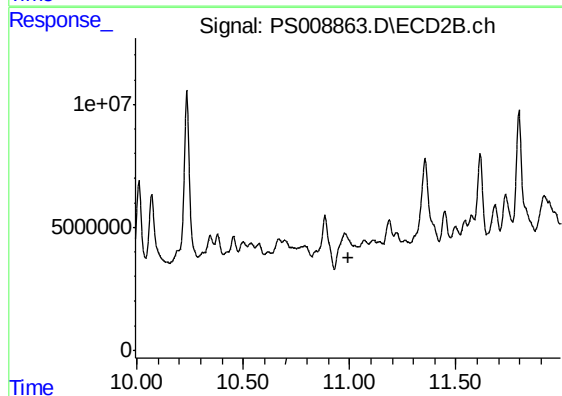

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.992 min
Response: 0
Conc: N.D.