

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021722\
 Data File : PS018356.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Feb 2022 10:24
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 18 00:41:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020822.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 09 15:57:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
5)	T	DICAMBA	7.217	0.000	8178166	0	1.295 N.D. #
8)	T	DICHLORPROP	7.909	0.000	3456447	0	2.191 N.D. #
9)	T	2,4-D	8.159	0.000	17570979	0	9.543 N.D. #
10)	T	Pentachlo...	8.425	0.000	13554860	0	<MDL N.D. #
11)	T	2,4,5-TP ...	8.978	0.000	13762403	0	1.611 N.D. #
12)	T	2,4,5-T	9.273	8.855	60495372	12231147	6.836 3.454 #
13)	T	2,4-DB	9.837	0.000	13048741	0	7.414 N.D. #
14)	T	DINOSEB	10.944	0.000	21425988	0	3.209 N.D. #
15)	T	Picloram	10.800	10.658	394.1E6	202.5E6	34.496 40.404
16)	T	DCPA	11.213	10.584	17821870	12723048	1.617 2.796 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021722\
Data File : PS018356.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Feb 2022 10:24
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 18 00:41:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020822.M
Quant Title : 8080.M
QLast Update : Wed Feb 09 15:57:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

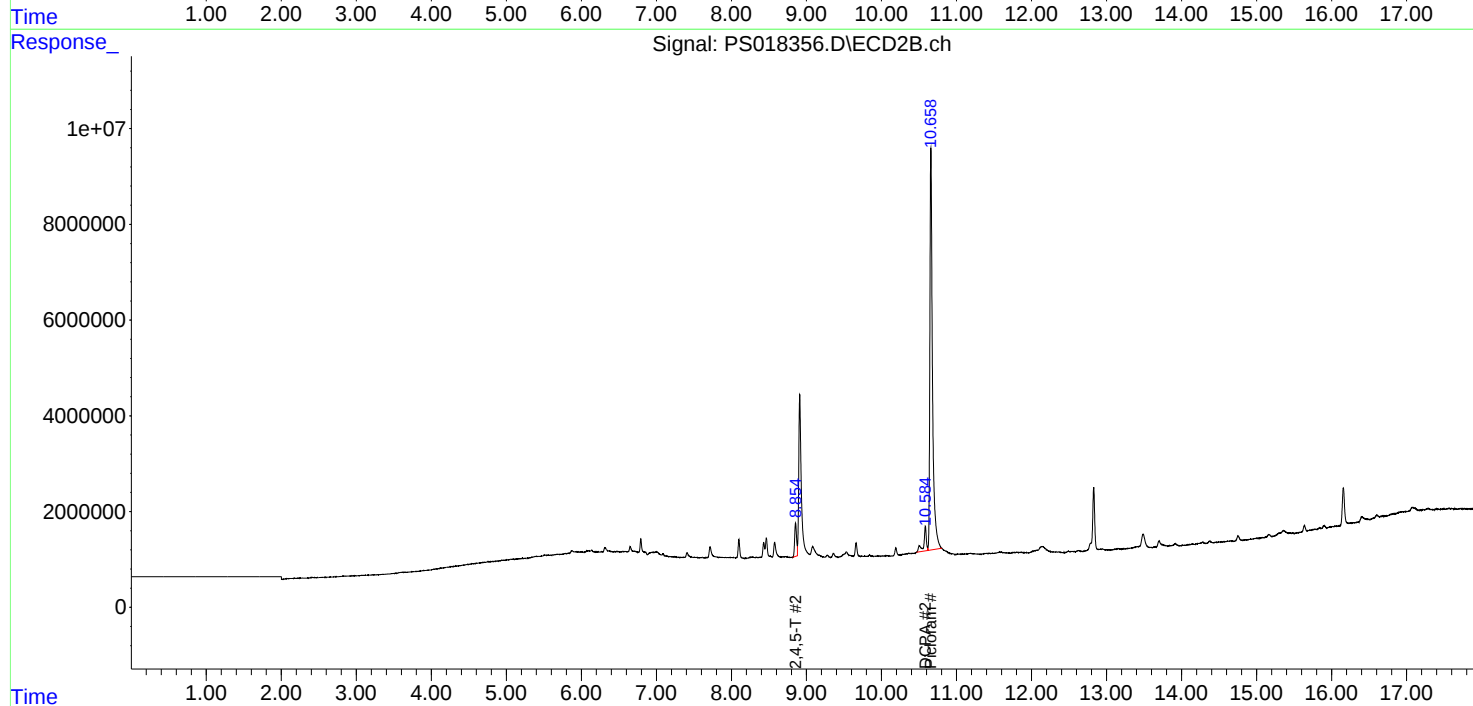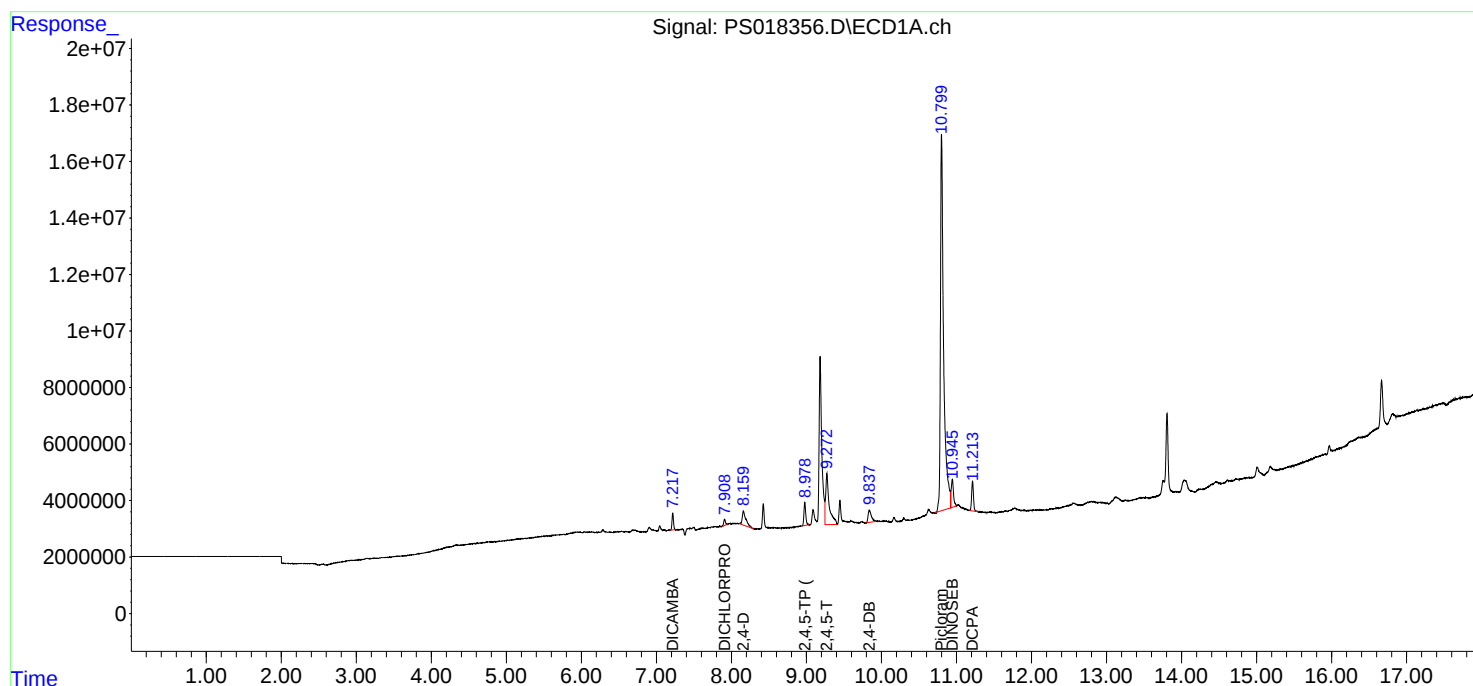


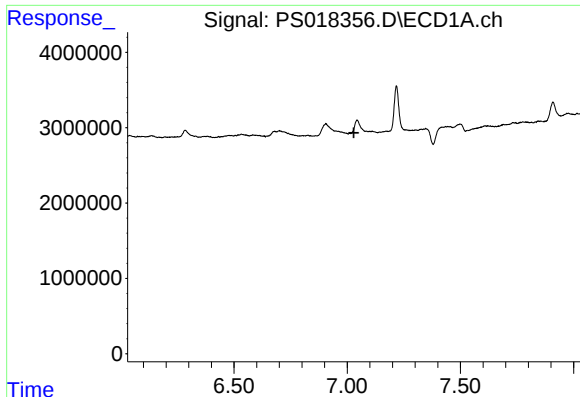

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.029 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

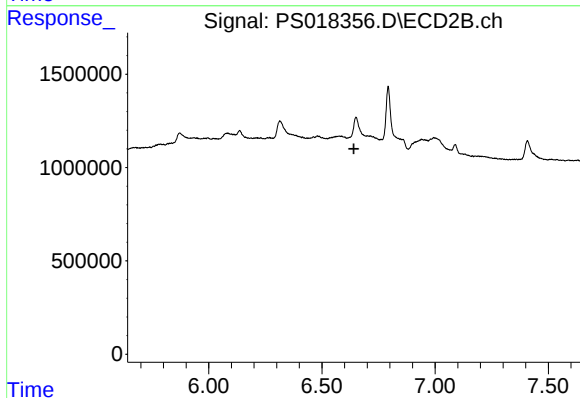


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.641 min
Response: 0
Conc: N.D.

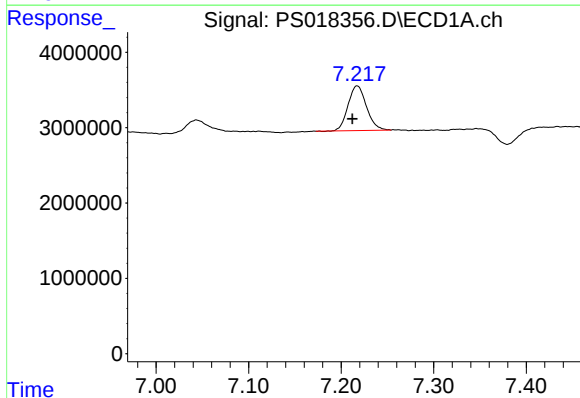


#5 DICAMBA

R.T.: 7.217 min
Delta R.T.: 0.005 min
Response: 8178166
Conc: 1.29 ng/ml

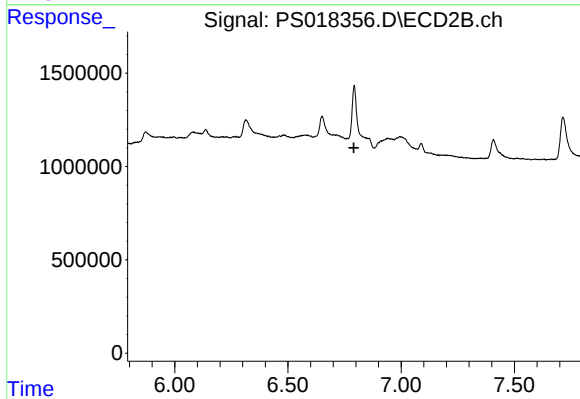

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.791 min
Response: 0
Conc: N.D.

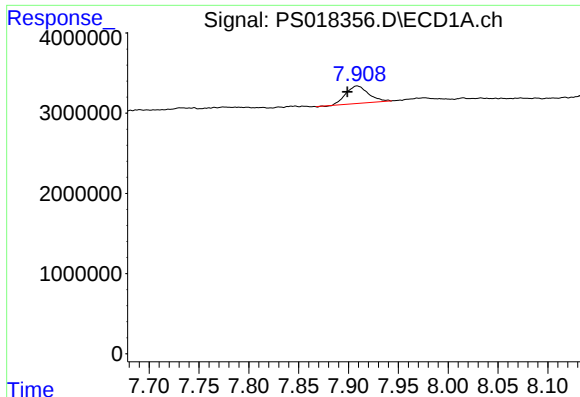

#8 DICHLORPROP


R.T.: 7.909 min
Delta R.T.: 0.010 min
Response: 3456447
Conc: 2.19 ng/ml

Instrument :
ECD_S
ClientSampleId :

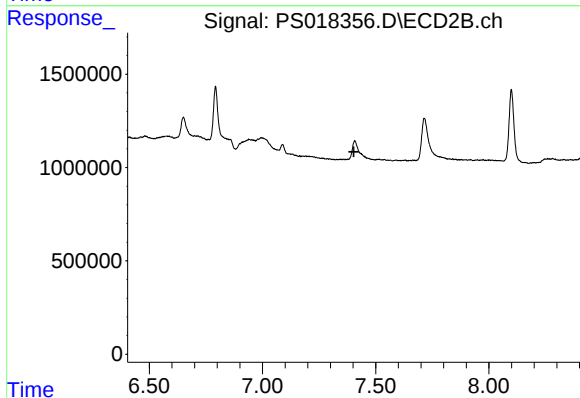


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.404 min
Response: 0
Conc: N.D.

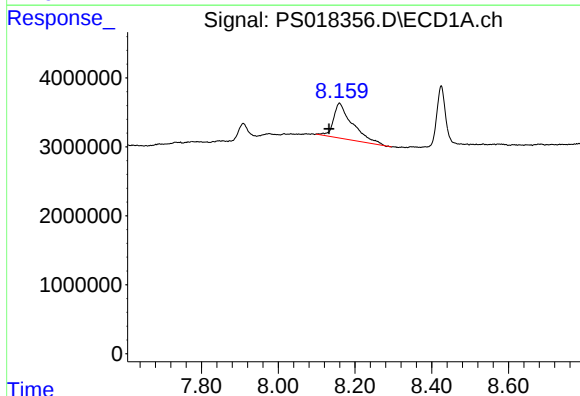


#9 2,4-D

R.T.: 8.159 min
Delta R.T.: 0.027 min
Response: 17570979
Conc: 9.54 ng/ml

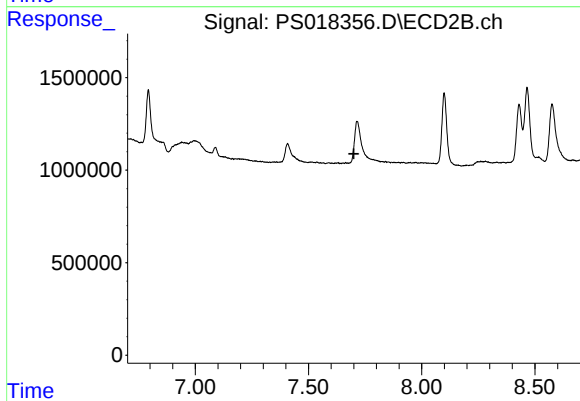

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.701 min
Response: 0
Conc: N.D.

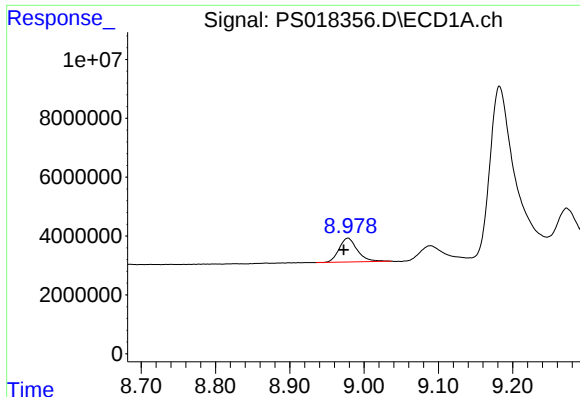

#11 2,4,5-TP (SILVEX)


R.T.: 8.978 min
Delta R.T.: 0.006 min
Response: 13762403
Conc: 1.61 ng/ml

Instrument :
ECD_S
ClientSampleId :

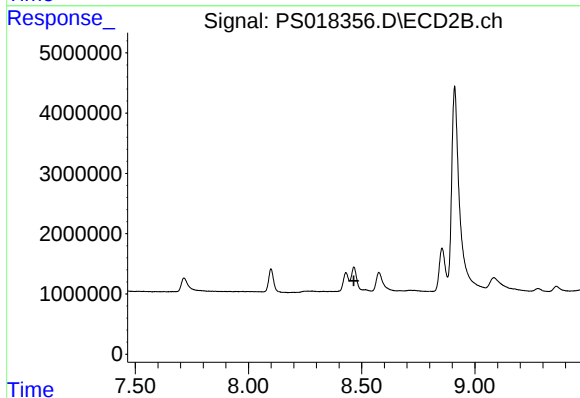


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 8.465 min
Response: 0
Conc: N.D.

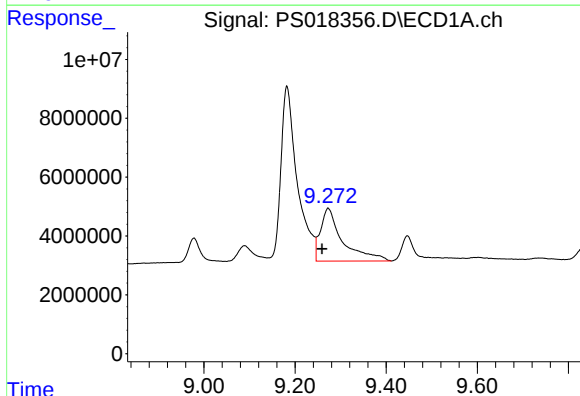


#12 2,4,5-T

R.T.: 9.273 min
Delta R.T.: 0.013 min
Response: 60495372
Conc: 6.84 ng/ml

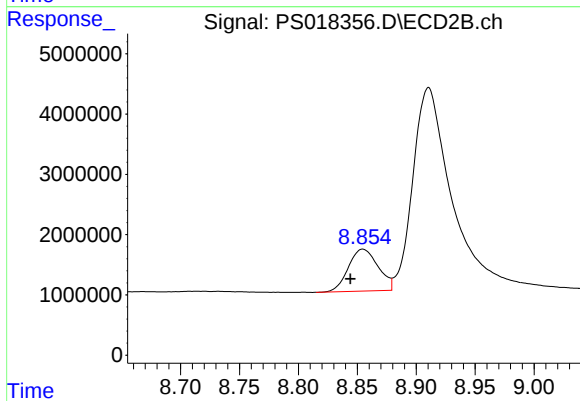

#12 2,4,5-T


R.T.: 8.855 min
Delta R.T.: 0.011 min
Response: 12231147
Conc: 3.45 ng/ml

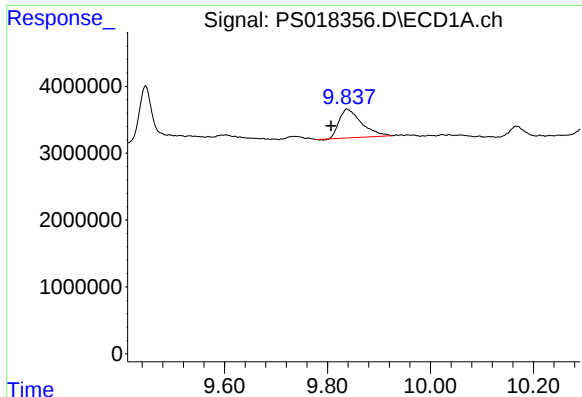

#13 2,4-DB


R.T.: 9.837 min
Delta R.T.: 0.030 min
Response: 13048741
Conc: 7.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

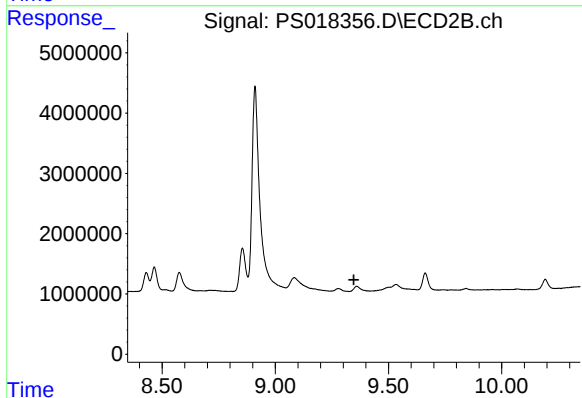


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.347 min
Response: 0
Conc: N.D.

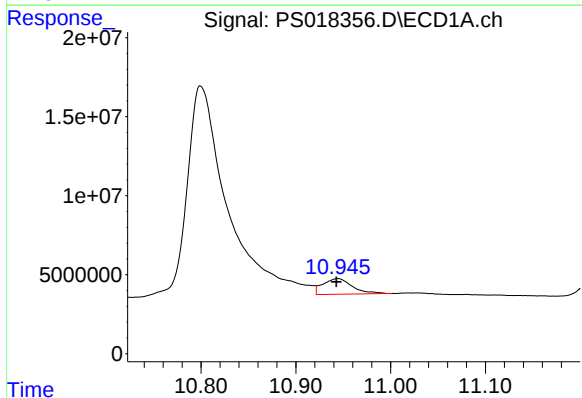


#14 DINOSEB

R.T.: 10.944 min
Delta R.T.: 0.002 min
Response: 21425988
Conc: 3.21 ng/ml

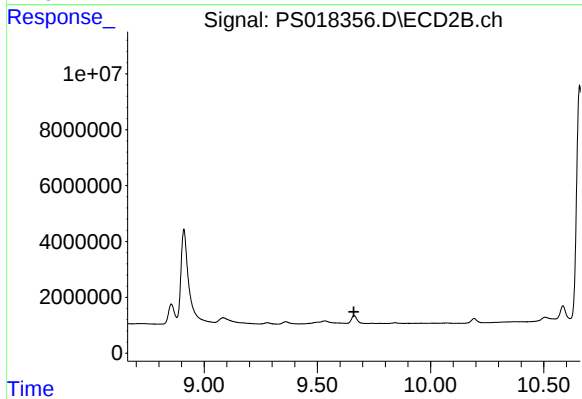

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.661 min
Response: 0
Conc: N.D.

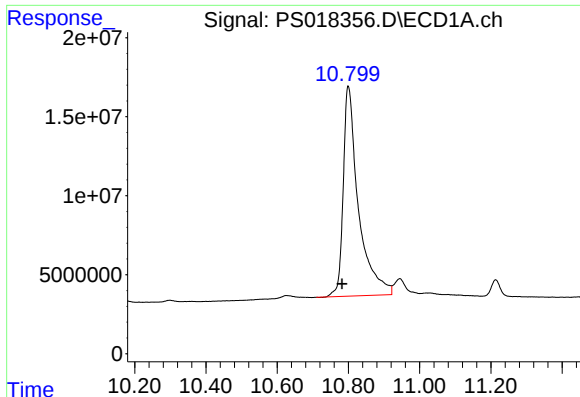

#15 Picloram


R.T.: 10.800 min
Delta R.T.: 0.017 min
Response: 394112317
Conc: 34.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

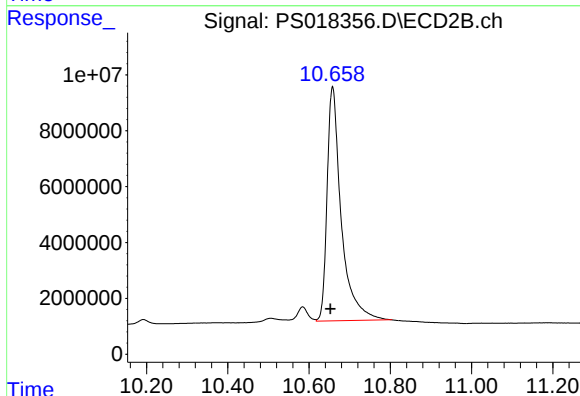


#15 Picloram

R.T.: 10.658 min
Delta R.T.: 0.005 min
Response: 202501322
Conc: 40.40 ng/ml

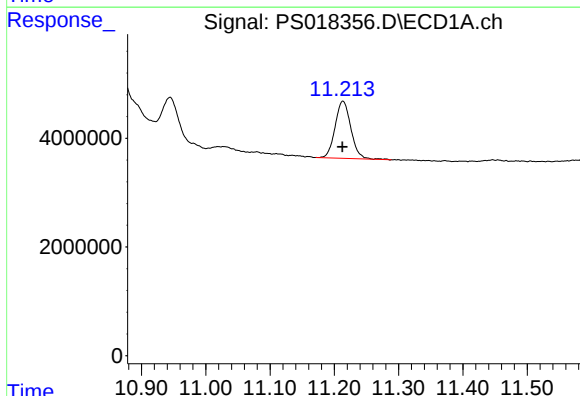

#16 DCPA

R.T.: 11.213 min
Delta R.T.: 0.000 min
Response: 17821870
Conc: 1.62 ng/ml

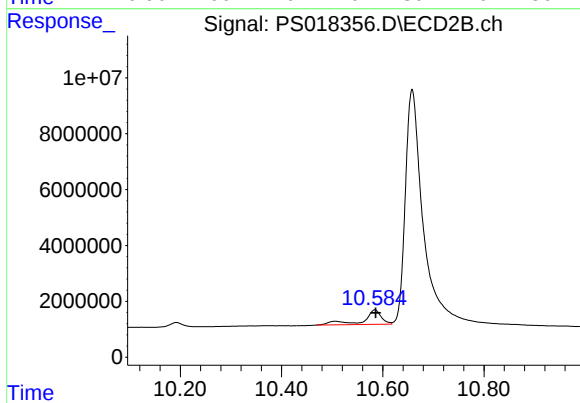

#16 DCPA

R.T.: 10.584 min
Delta R.T.: -0.002 min
Response: 12723048
Conc: 2.80 ng/ml