

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021722\
 Data File : PS018357.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Feb 2022 11:57
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 18 00:41:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020822.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 09 15:57:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.034	6.640	545.5E6	307.8E6	346.796	490.801 #
Target Compounds							
12) T	2,4,5-T	9.227	0.000	76696678	0	8.667	N.D. #
15) T	Picloram	10.846f	10.690	276.9E6	137.5E6	24.241	27.425



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021722\
Data File : PS018357.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Feb 2022 11:57
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 18 00:41:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020822.M
Quant Title : 8080.M
QLast Update : Wed Feb 09 15:57:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

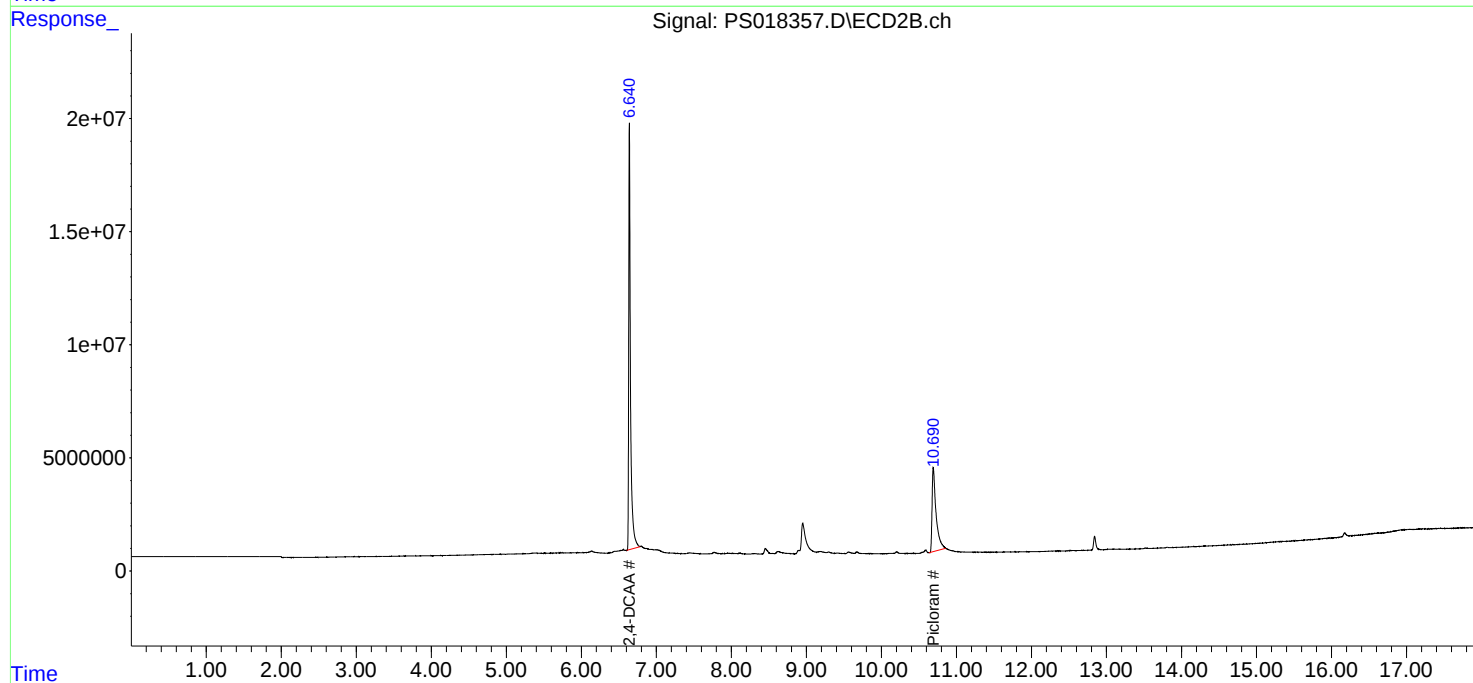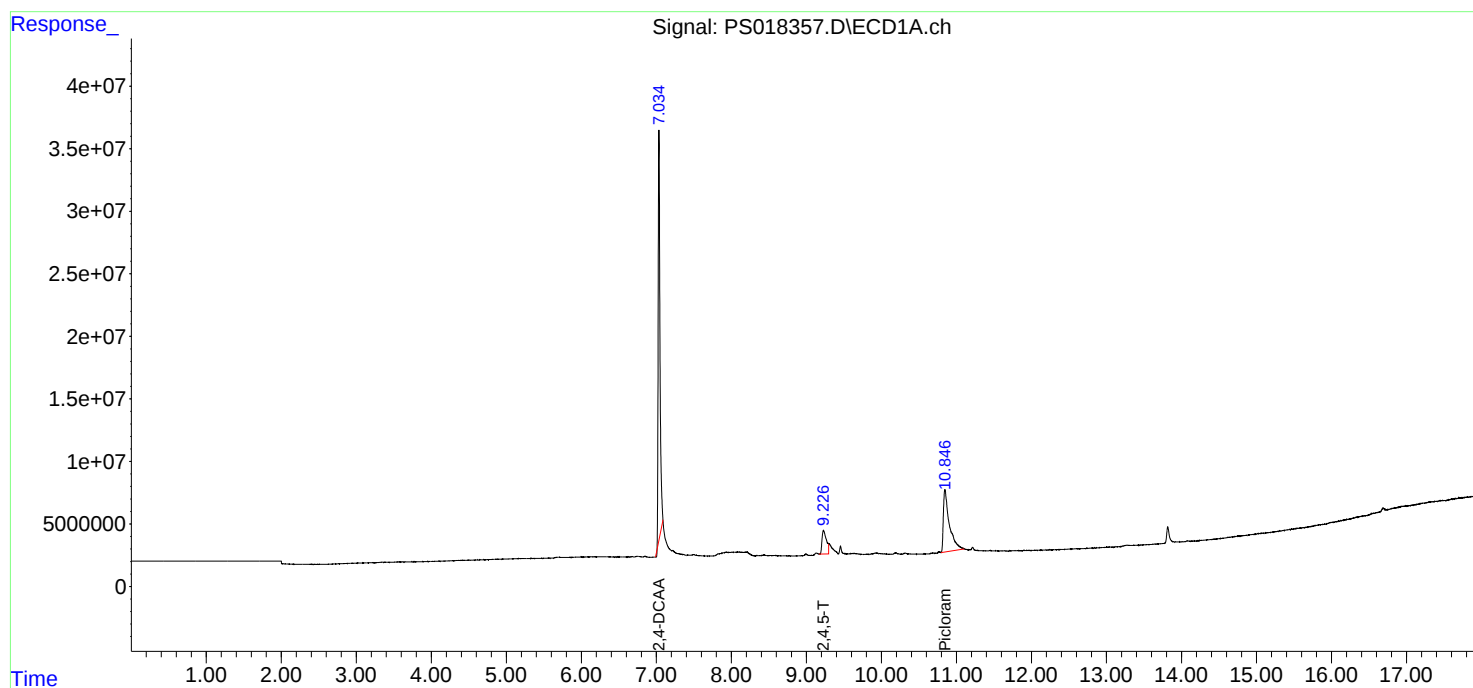


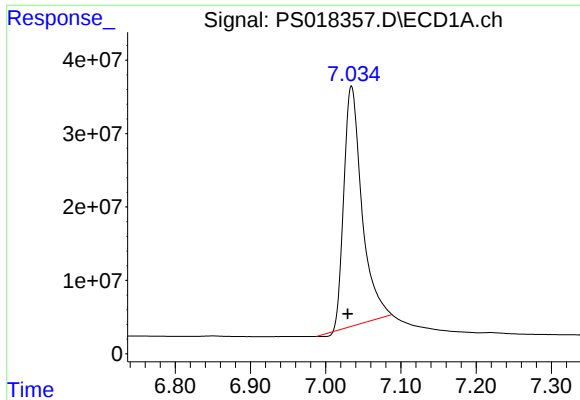

#4 2,4-DCAA


R.T.: 7.034 min
Delta R.T.: 0.005 min
Response: 545535289
Conc: 346.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

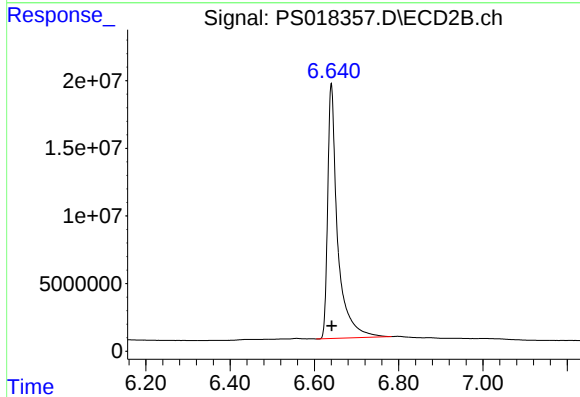


#4 2,4-DCAA

R.T.: 6.640 min
Delta R.T.: 0.000 min
Response: 307845317
Conc: 490.80 ng/ml

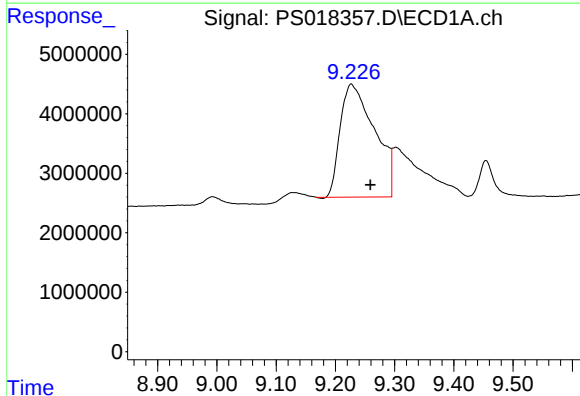


#12 2,4,5-T

R.T.: 9.227 min
Delta R.T.: -0.032 min
Response: 76696678
Conc: 8.67 ng/ml

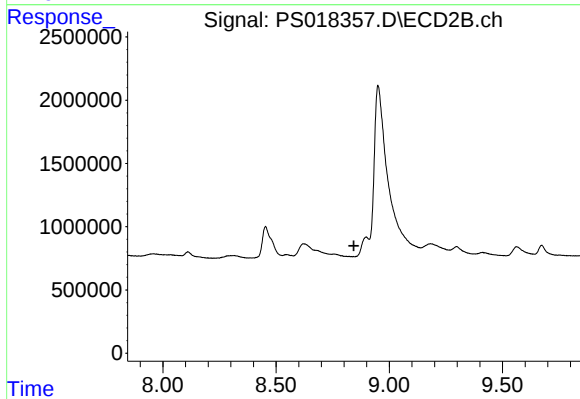

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 8.844 min
Response: 0
Conc: N.D.

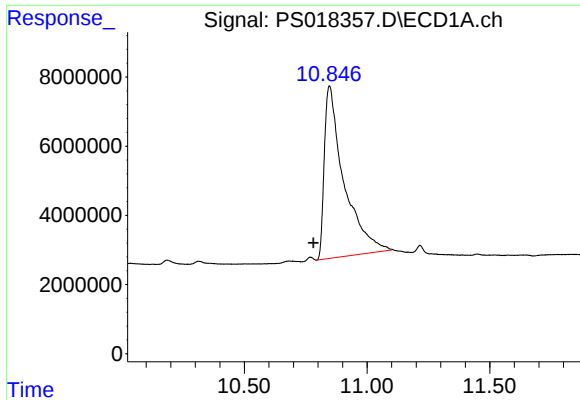

#15 Picloram

R.T.: 10.846 min
Delta R.T.: 0.064 min
Response: 276947133
Conc: 24.24 ng/ml

Instrument :
ECD_S
ClientSampleId :

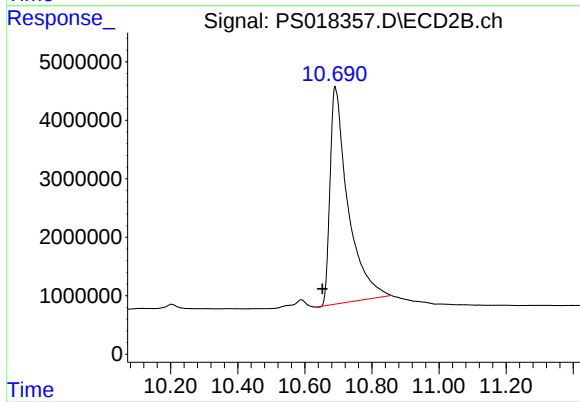

#15 Picloram

R.T.: 10.690 min
Delta R.T.: 0.037 min
Response: 137453605
Conc: 27.43 ng/ml