

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021722\
 Data File : PS018367.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Feb 2022 20:32
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 18 00:45:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020822.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 09 15:57:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.026	6.639	645.3E6	323.2E6	410.186	515.331 #
Target Compounds							
5) T	DICAMBA	7.211	0.000	7025727	0	1.112	N.D. #
9) T	2,4-D	8.185f	0.000	20818078	0	11.306	N.D. #
10) T	Pentachlo...	8.420	0.000	11091134	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.972	8.433	9161280	8140536	1.072	2.198 #
12) T	2,4,5-T	9.270	8.863	61746074	9069972	6.977	2.562 #
13) T	2,4-DB	9.845	0.000	9535257	0	5.418	N.D. #
14) T	DINOSEB	10.935	0.000	46946842	0	7.031	N.D. #
15) T	Picloram	10.803	10.665	324.6E6	159.7E6	28.409	31.865
16) T	DCPA	11.206	0.000	15103680	0	1.370	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021722\
Data File : PS018367.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Feb 2022 20:32
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 18 00:45:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020822.M
Quant Title : 8080.M
QLast Update : Wed Feb 09 15:57:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

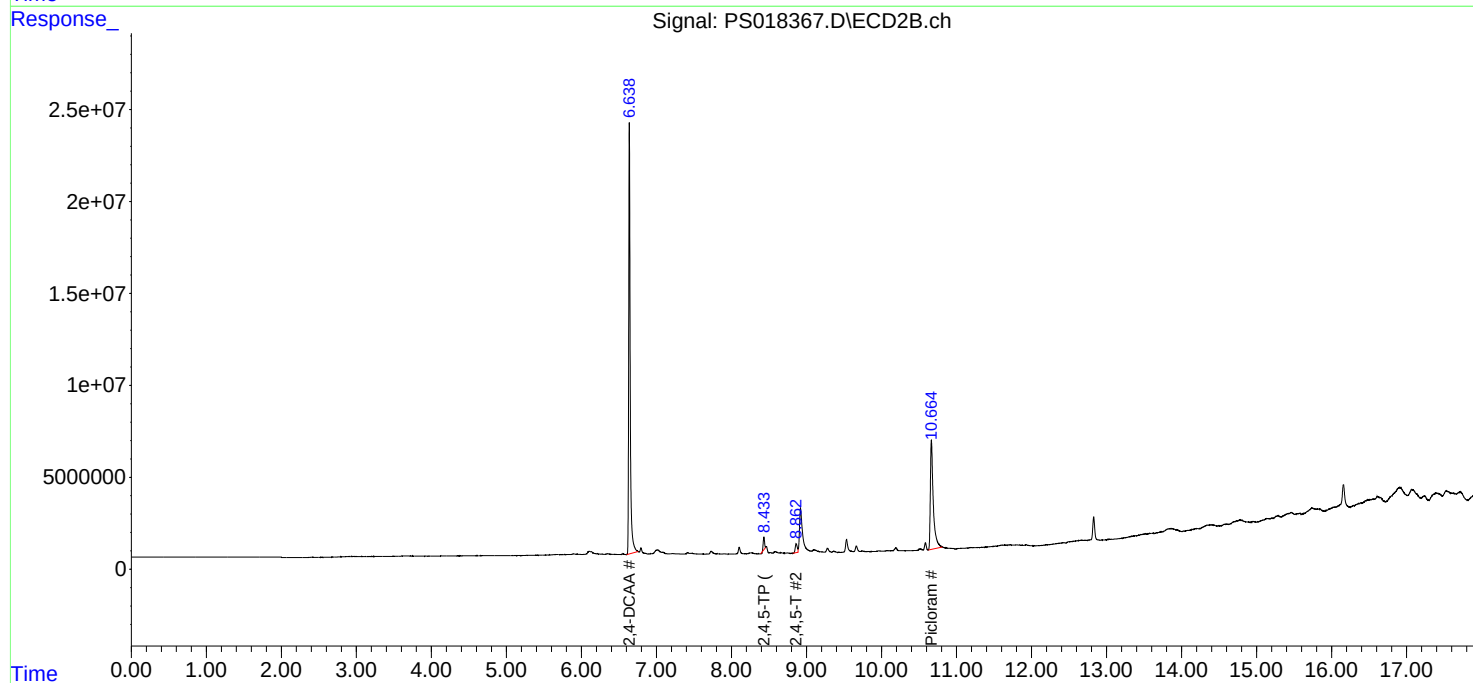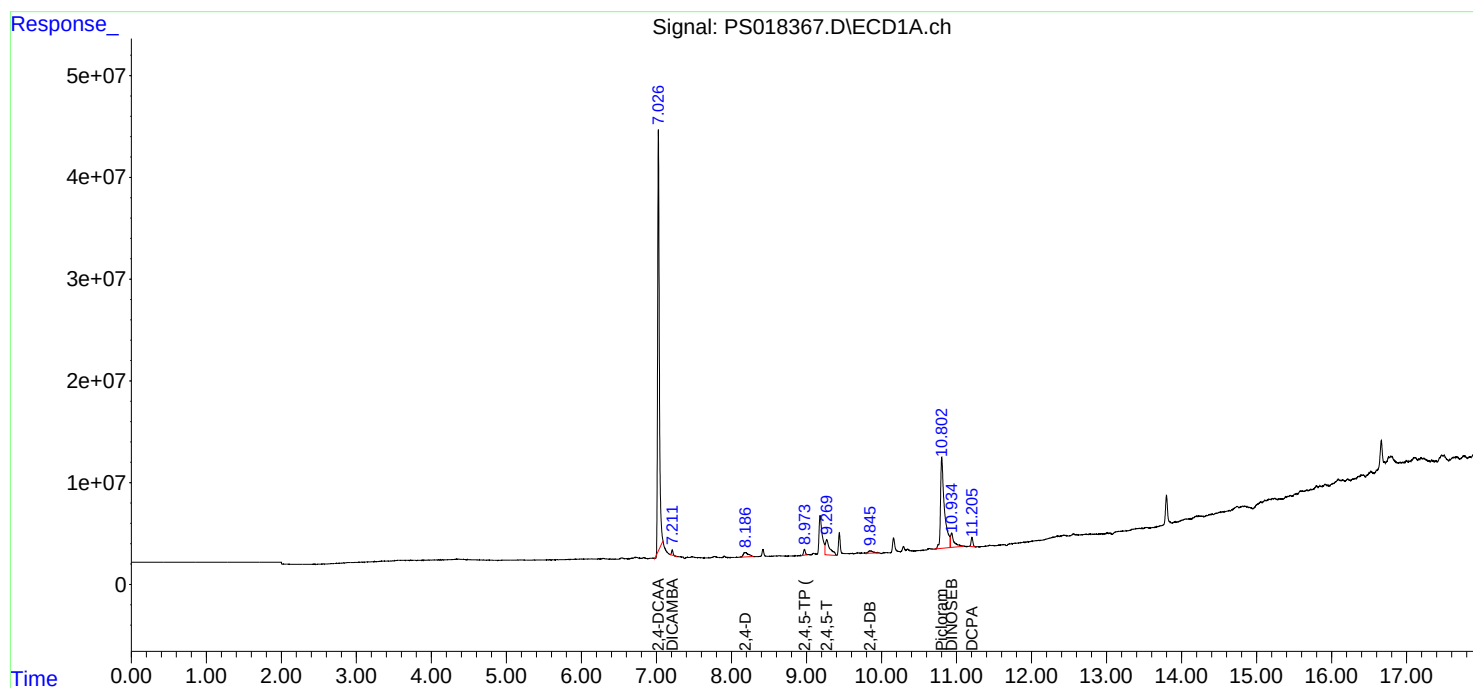


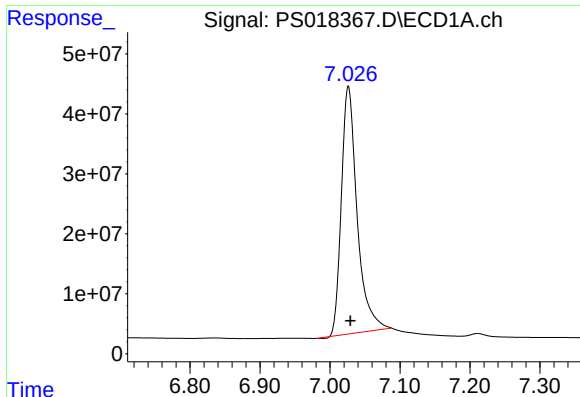

#4 2,4-DCAA


R.T.: 7.026 min
Delta R.T.: -0.003 min
Response: 645252852
Conc: 410.19 ng/ml

Instrument :
ECD_S
ClientSampleId :

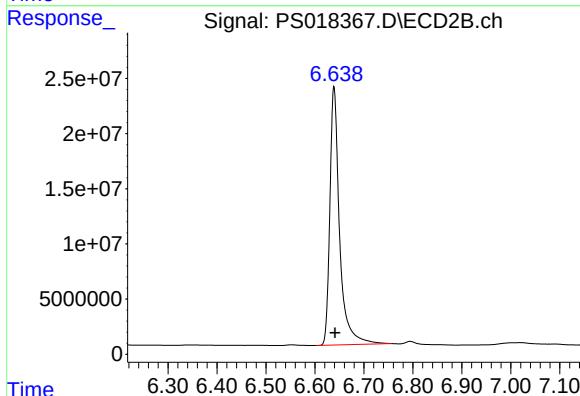


#4 2,4-DCAA

R.T.: 6.639 min
Delta R.T.: -0.002 min
Response: 323231183
Conc: 515.33 ng/ml

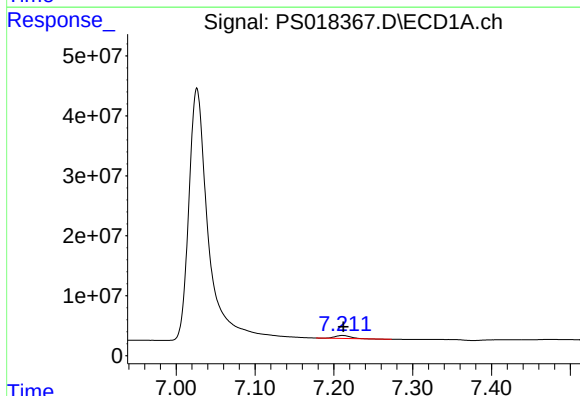


#5 DICAMBA

R.T.: 7.211 min
Delta R.T.: -0.001 min
Response: 7025727
Conc: 1.11 ng/ml

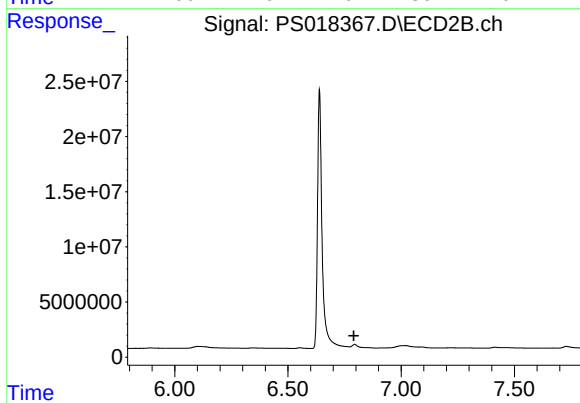

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 6.791 min
Response: 0
Conc: N.D.

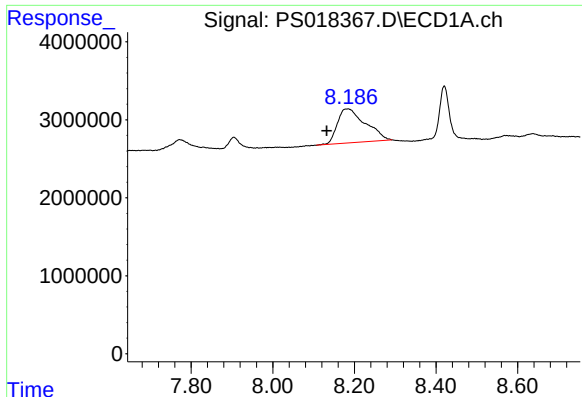

#9 2,4-D


R.T.: 8.185 min
Delta R.T.: 0.053 min
Response: 20818078
Conc: 11.31 ng/ml

Instrument :
ECD_S
ClientSampleId :

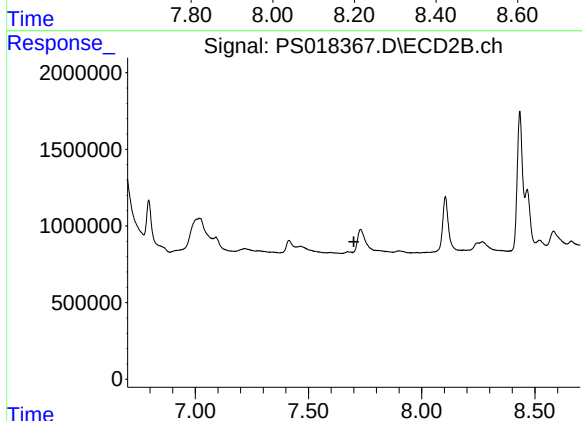


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.701 min
Response: 0
Conc: N.D.

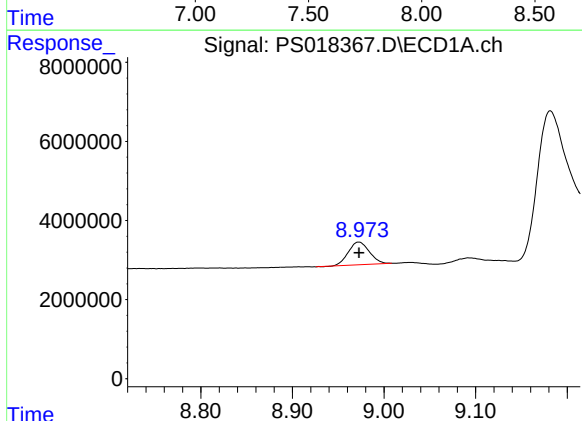


#11 2,4,5-TP (SILVEX)

R.T.: 8.972 min
Delta R.T.: 0.000 min
Response: 9161280
Conc: 1.07 ng/ml

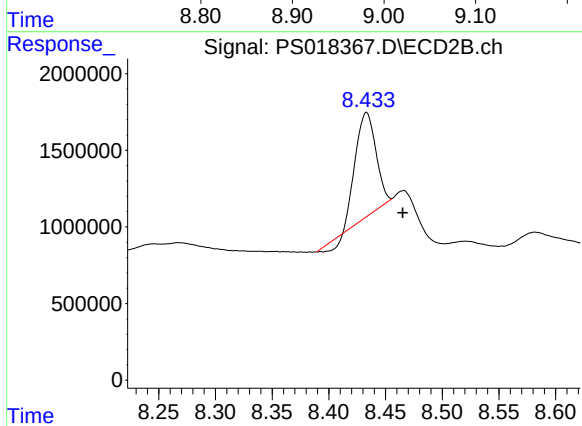

#11 2,4,5-TP (SILVEX)


R.T.: 8.433 min
Delta R.T.: -0.032 min
Response: 8140536
Conc: 2.20 ng/ml

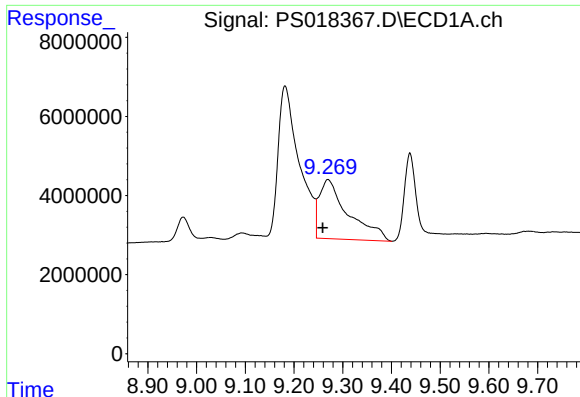

#12 2,4,5-T


R.T.: 9.270 min
Delta R.T.: 0.010 min
Response: 61746074
Conc: 6.98 ng/ml

Instrument :
ECD_S
ClientSampleId :

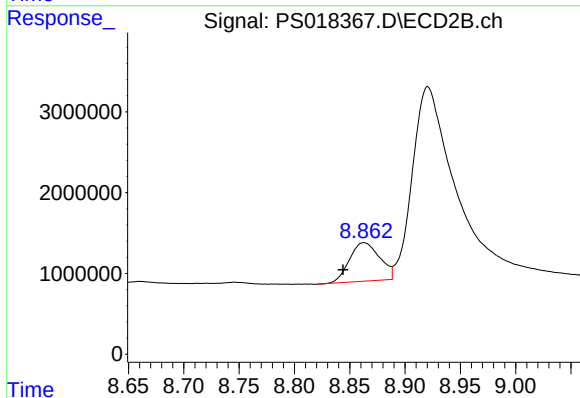


#12 2,4,5-T

R.T.: 8.863 min
Delta R.T.: 0.019 min
Response: 9069972
Conc: 2.56 ng/ml

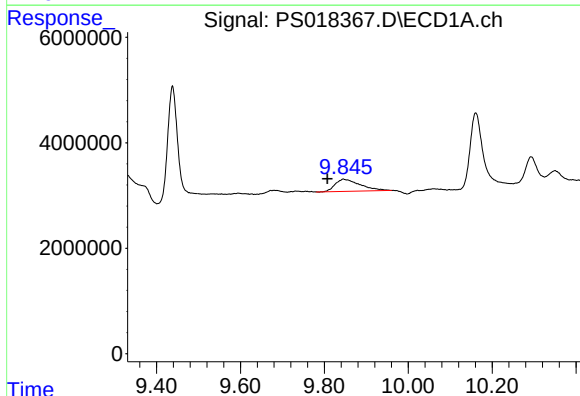


#13 2,4-DB

R.T.: 9.845 min
Delta R.T.: 0.038 min
Response: 9535257
Conc: 5.42 ng/ml

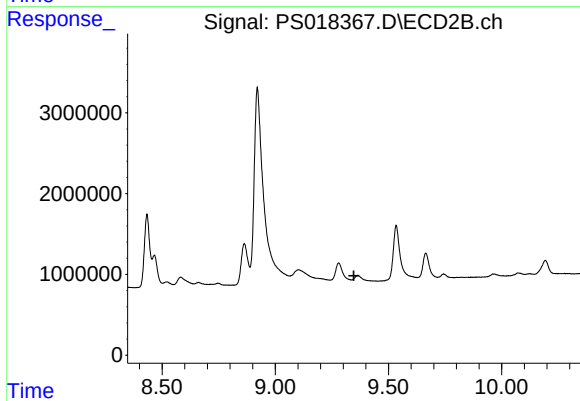

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.347 min
Response: 0
Conc: N.D.

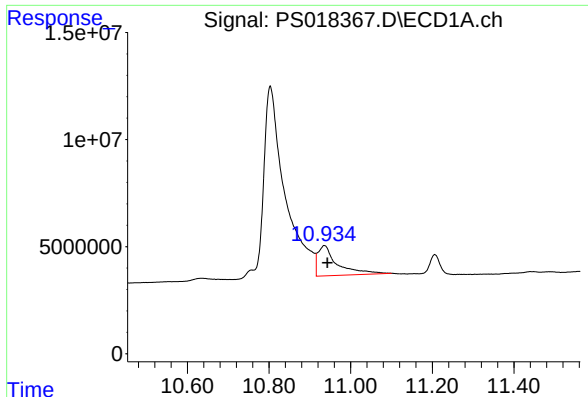

#14 DINOSEB


R.T.: 10.935 min
Delta R.T.: -0.007 min
Response: 46946842
Conc: 7.03 ng/ml

Instrument :
ECD_S
ClientSampleId :

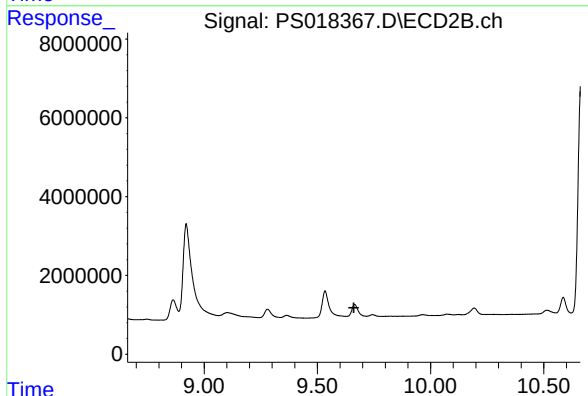


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.661 min
Response: 0
Conc: N.D.

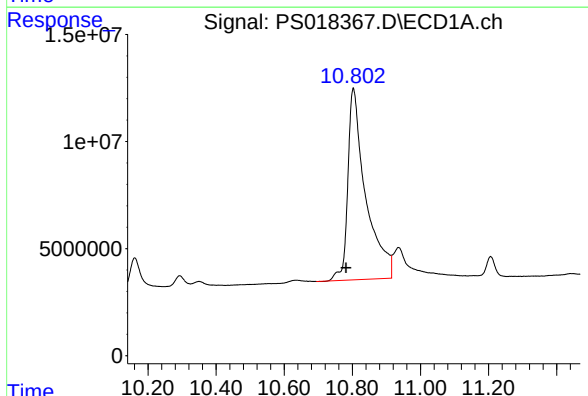


#15 Picloram

R.T.: 10.803 min
Delta R.T.: 0.021 min
Response: 324570116
Conc: 28.41 ng/ml

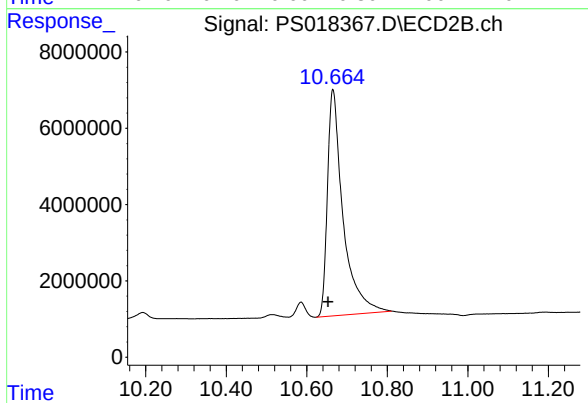

#15 Picloram


R.T.: 10.665 min
Delta R.T.: 0.012 min
Response: 159706546
Conc: 31.87 ng/ml

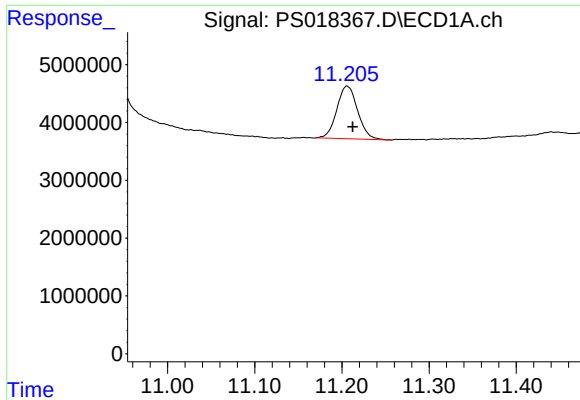

#16 DCPA

R.T.: 11.206 min
Delta R.T.: -0.007 min
Response: 15103680
Conc: 1.37 ng/ml

Instrument :
ECD_S
ClientSampleId :

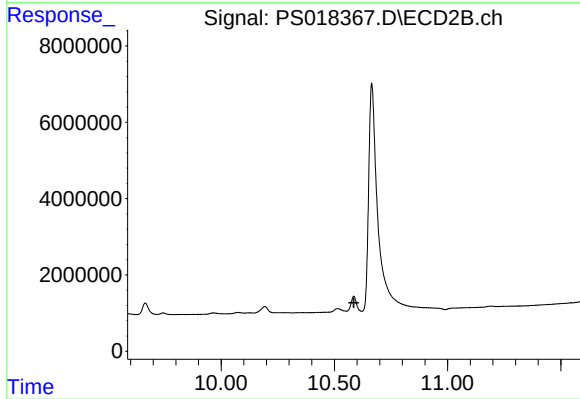

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.586 min
Response: 0
Conc: N.D.