

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021819\
 Data File : PS003235.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Feb 2019 19:36
 Operator : EI\SJ
 Sample : PB117192TB
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB117192TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 19 05:10:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.297	10.796	114.3E6	117.2E6	301.046	274.155
Target Compounds							
6) T	MCP	11.978	0.000	17509709	0	14.614	N.D. #
9) T	2,4-D	0.000	12.761	0	2472608	N.D.	4.932 #
11) T	2,4,5-TP ...	14.421	0.000	3156509	0	1.253	N.D. #
12) T	2,4,5-T	0.000	14.419	0	4981526	N.D.	2.603 #
15) T	Picloram	0.000	16.730	0	19564238	N.D.	6.508 #
16) T	DCPA	0.000	16.730	0	19564238	N.D.	6.316 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021819\
Data File : PS003235.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Feb 2019 19:36
Operator : EI\SJ
Sample : PB117192TB
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB117192TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 19 05:10:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

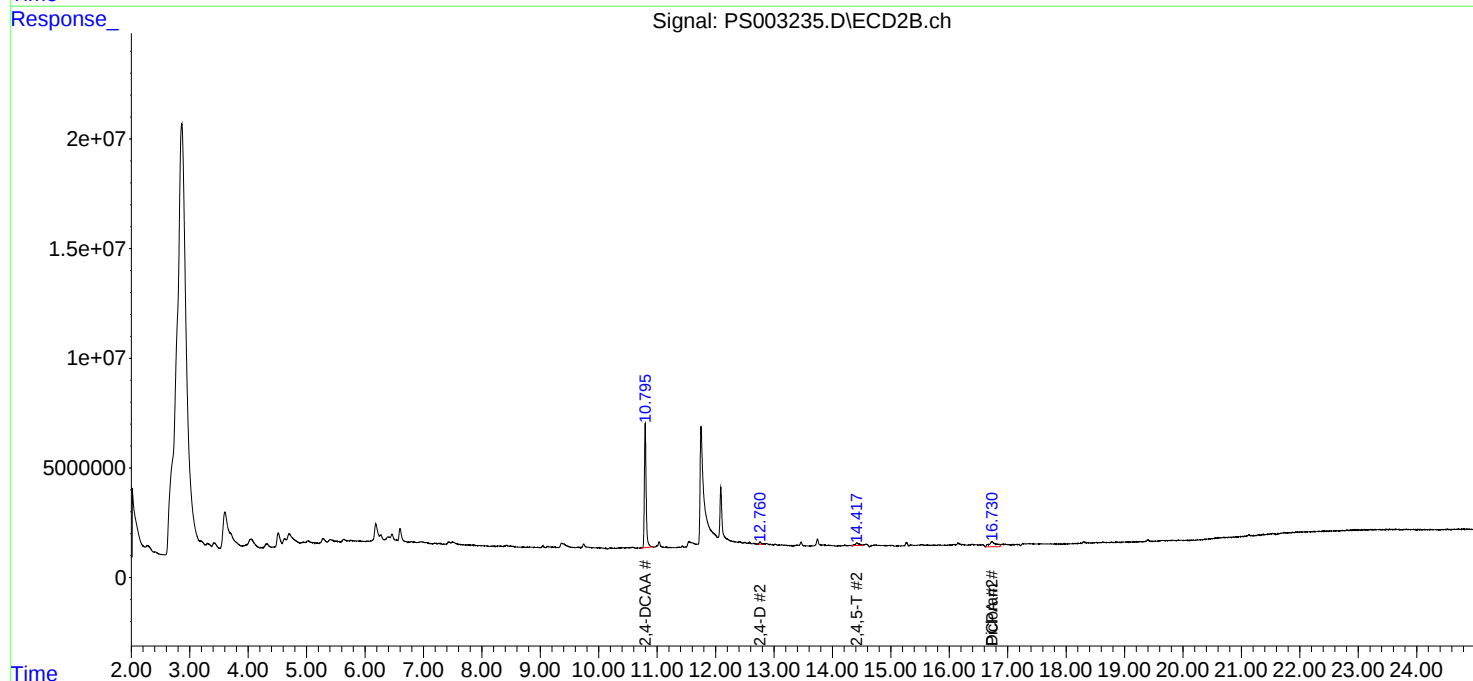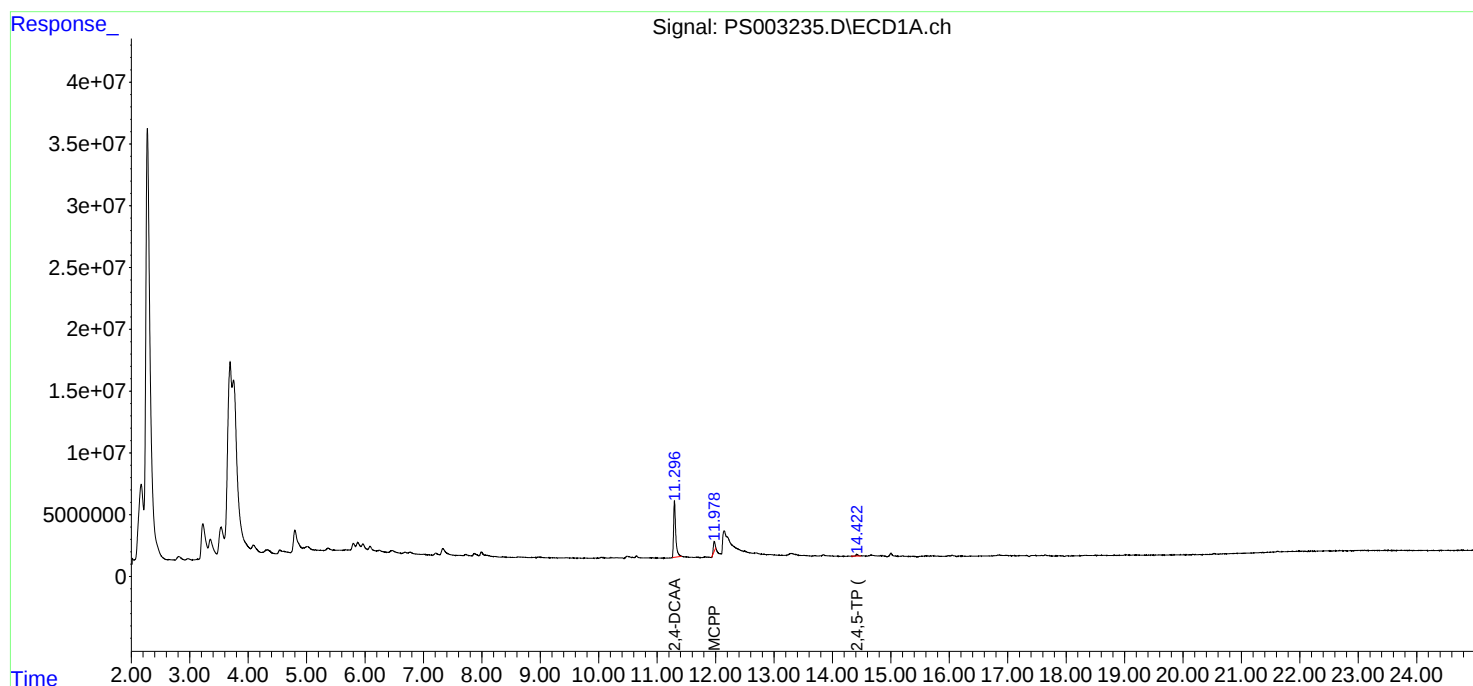


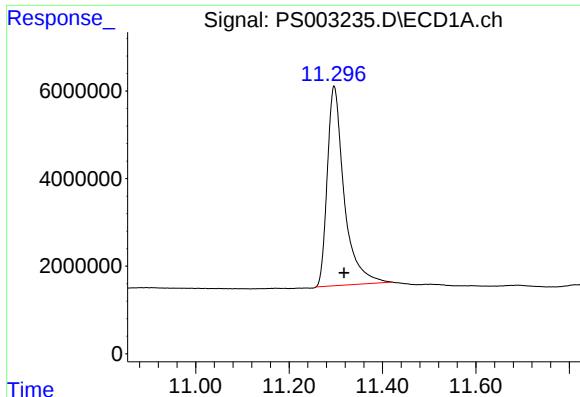

#4 2,4-DCAA


R.T.: 11.297 min
Delta R.T.: -0.021 min
Response: 114289385
Conc: 301.05 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB117192TB

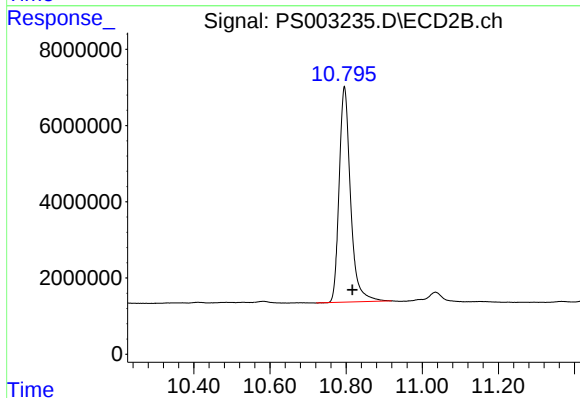


#4 2,4-DCAA

R.T.: 10.796 min
Delta R.T.: -0.021 min
Response: 117213812
Conc: 274.16 ng/ml

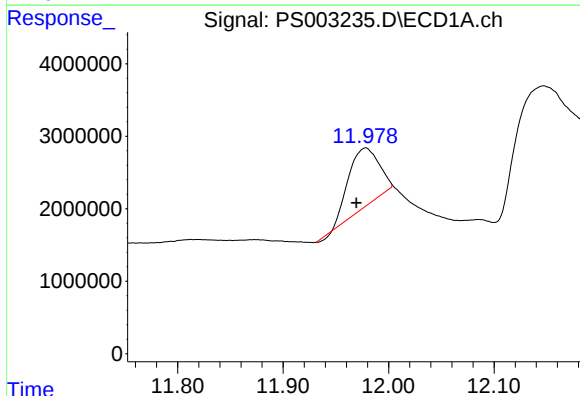


#6 MCP

R.T.: 11.978 min
Delta R.T.: 0.009 min
Response: 17509709
Conc: 14.61 ug/ml

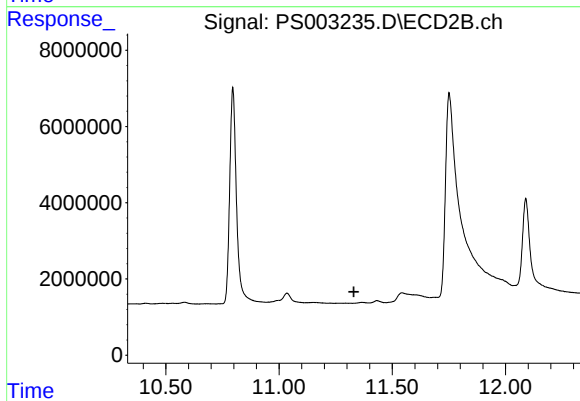

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.330 min
Response: 0
Conc: N.D.

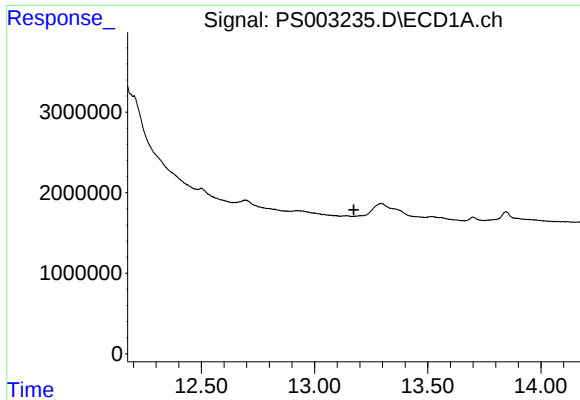

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.173 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB117192TB

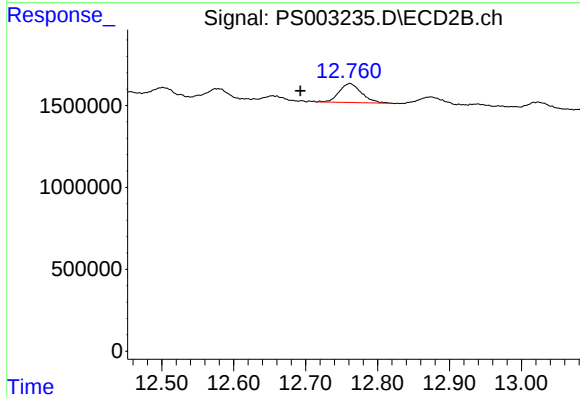


#9 2,4-D

R.T.: 12.761 min
Delta R.T.: 0.069 min
Response: 2472608
Conc: 4.93 ng/ml

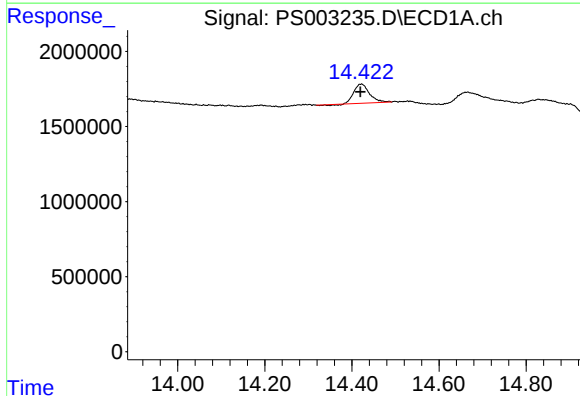


#11 2,4,5-TP (SILVEX)

R.T.: 14.421 min
Delta R.T.: 0.002 min
Response: 3156509
Conc: 1.25 ng/ml

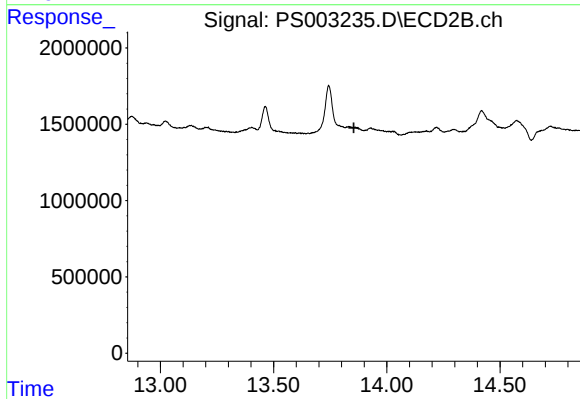

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 13.854 min
Response: 0
Conc: N.D.

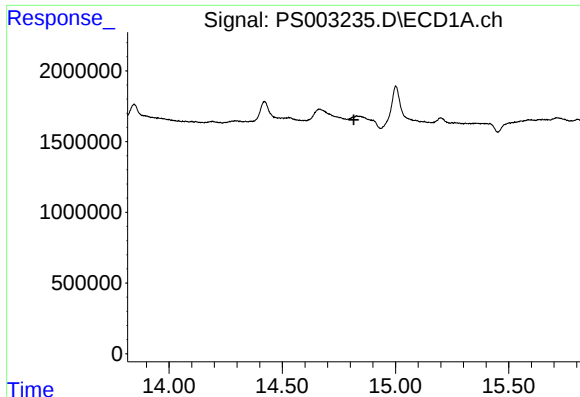

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 14.817 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB117192TB

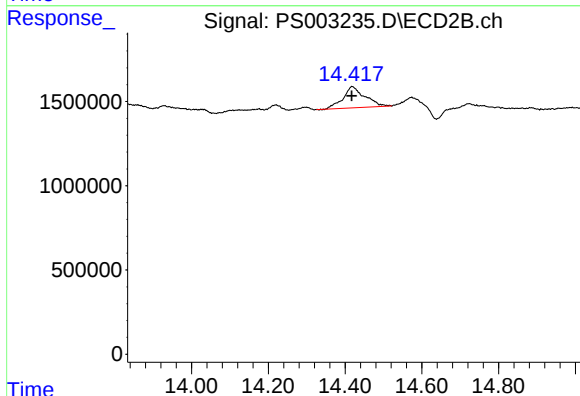


#12 2,4,5-T

R.T.: 14.419 min
Delta R.T.: 0.002 min
Response: 4981526
Conc: 2.60 ng/ml

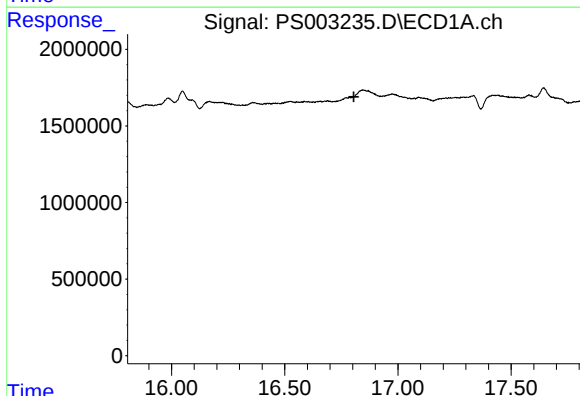


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.806 min
Response: 0
Conc: N.D.

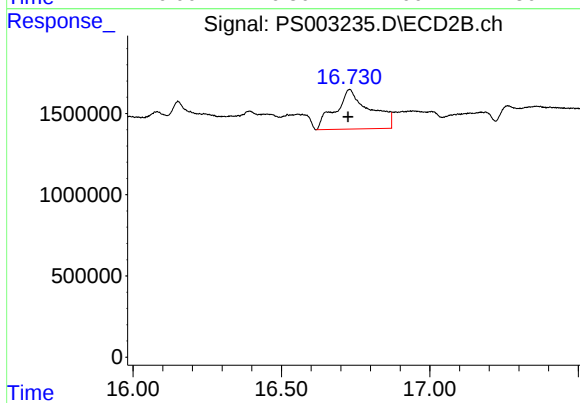

#15 Picloram


R.T.: 16.730 min
Delta R.T.: 0.005 min
Response: 19564238
Conc: 6.51 ng/ml

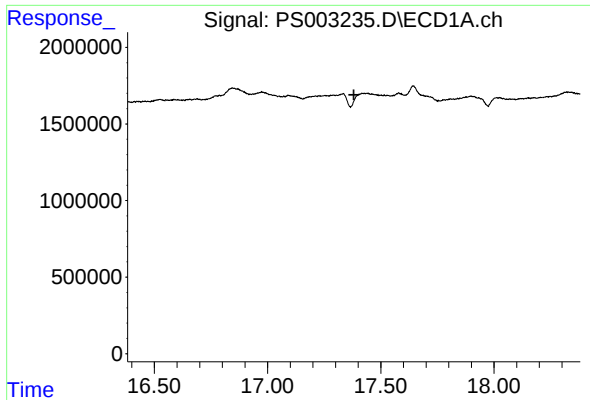

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB117192TB

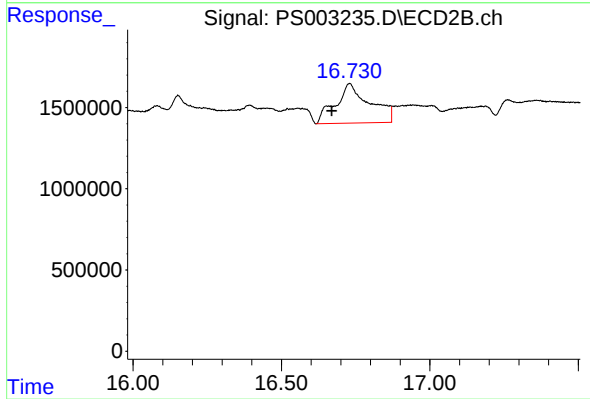

#16 DCPA

R.T.: 16.730 min
Delta R.T.: 0.060 min
Response: 19564238
Conc: 6.32 ng/ml