

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021819\
 Data File : PS003241.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Feb 2019 22:42
 Operator : EI\SJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 19 05:12:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.275	10.776	43350236	312.3E6	114.188	730.514 #
Target Compounds							
1) T	Dalapon	2.840	2.311	42992428	375.4E6	77.935	700.498 #
3) T	4-Nitroph...	0.000	9.927	0	150.3E6	N.D.	719.021 #
8) T	DICHLORPROP	0.000	12.181	0	276.1E6	N.D.	722.077 #
9) T	2,4-D	0.000	12.653	0	164.5E6	N.D.	328.166 #
11) T	2,4,5-TP ...	14.374	13.813	1881.0E6	1740.7E6	746.900	701.805
12) T	2,4,5-T	14.774	14.377	1809.7E6	-17651600	741.876	N.D. #
14) T	DINOSEB	16.985	0.000	1425.5E6	0	757.694	N.D. #
15) T	Picloram	16.763	16.684	2048.6E6	1912.1E6	647.544	636.008
16) T	DCPA	0.000	16.684	0	1912.1E6	N.D.	617.285 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021819\
Data File : PS003241.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Feb 2019 22:42
Operator : EI\SJ
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 19 05:12:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

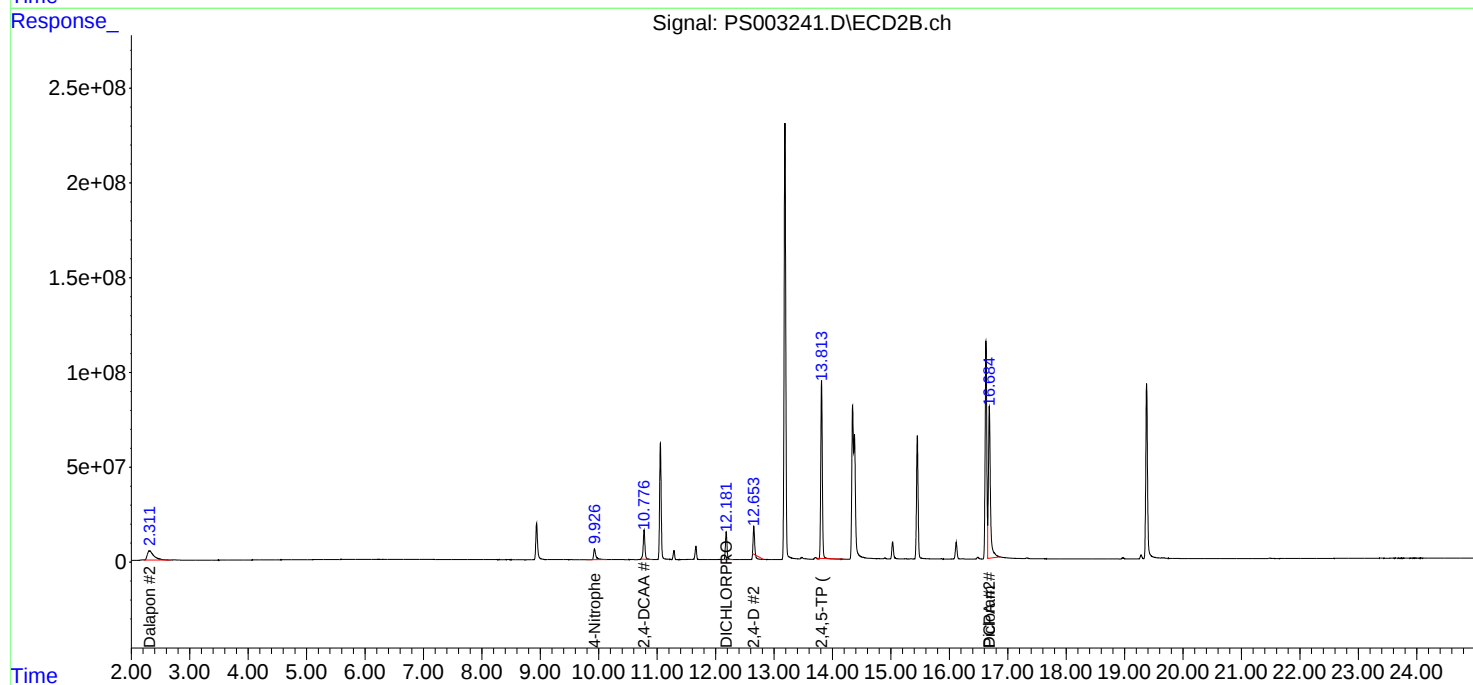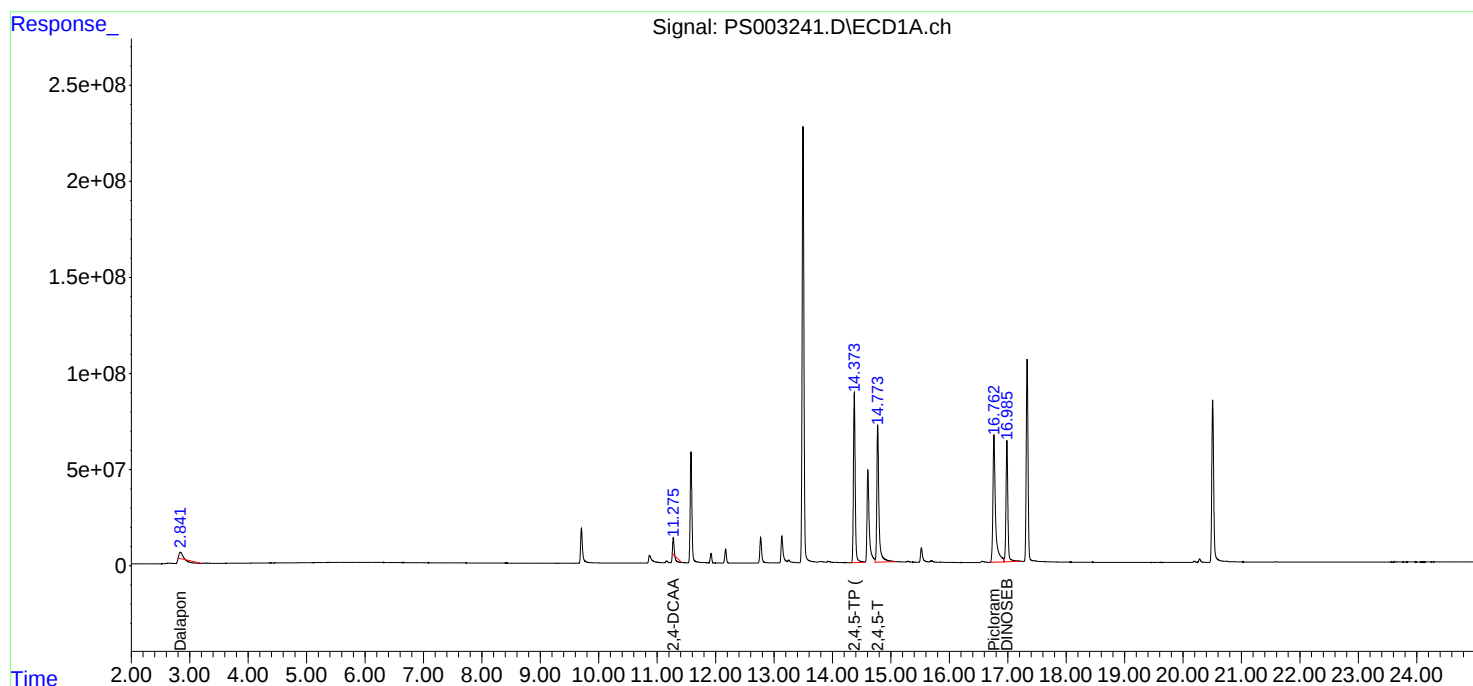


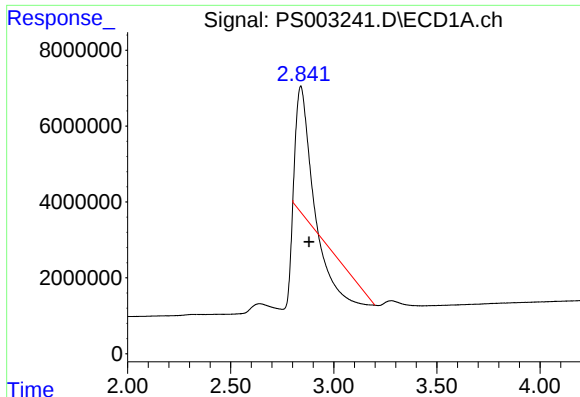

#1 Dalapon


R.T.: 2.840 min
Delta R.T.: -0.040 min
Response: 42992428
Conc: 77.93 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

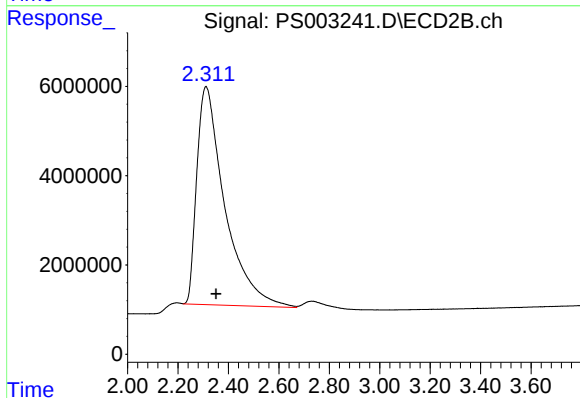


#1 Dalapon

R.T.: 2.311 min
Delta R.T.: -0.040 min
Response: 375411580
Conc: 700.50 ng/ml

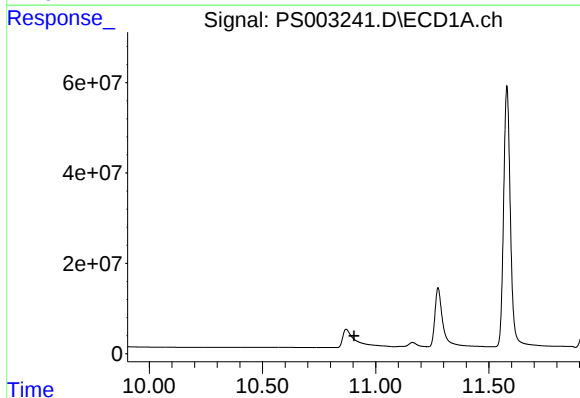


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 10.904 min
Response: 0
Conc: N.D.

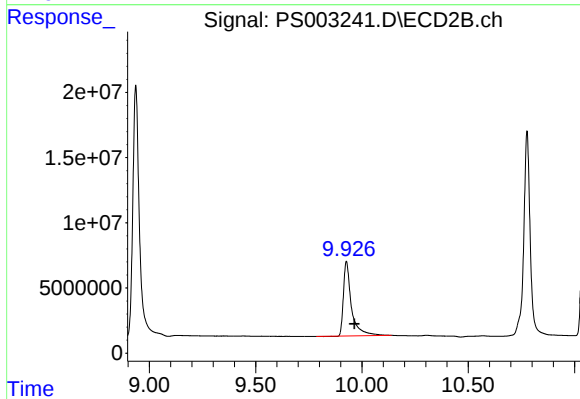

#3 4-Nitrophenol


R.T.: 9.927 min
Delta R.T.: -0.039 min
Response: 150291626
Conc: 719.02 ng/ml

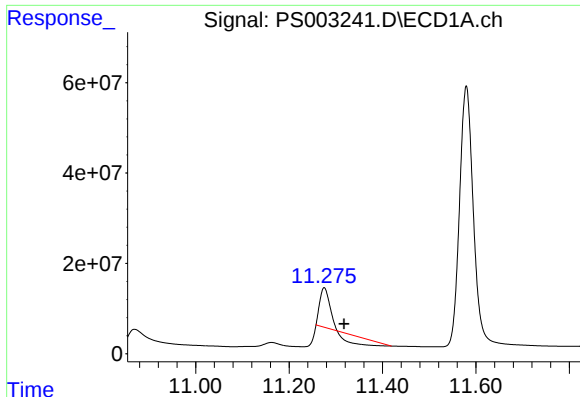

#4 2,4-DCAA


R.T.: 11.275 min
Delta R.T.: -0.042 min
Response: 43350236
Conc: 114.19 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

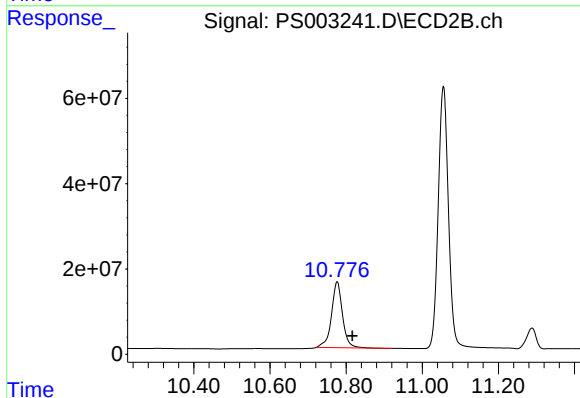


#4 2,4-DCAA

R.T.: 10.776 min
Delta R.T.: -0.040 min
Response: 312328000
Conc: 730.51 ng/ml

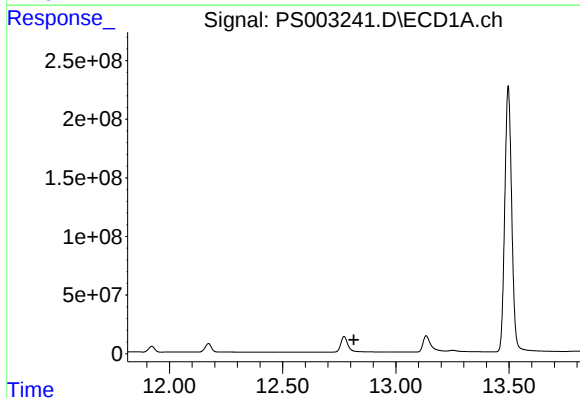


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.815 min
Response: 0
Conc: N.D.

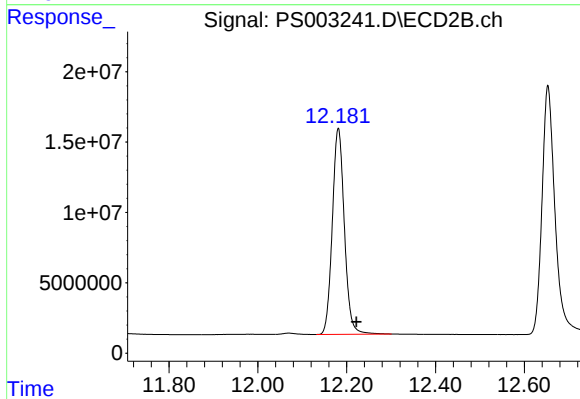

#8 DICHLORPROP


R.T.: 12.181 min
Delta R.T.: -0.041 min
Response: 276079637
Conc: 722.08 ng/ml

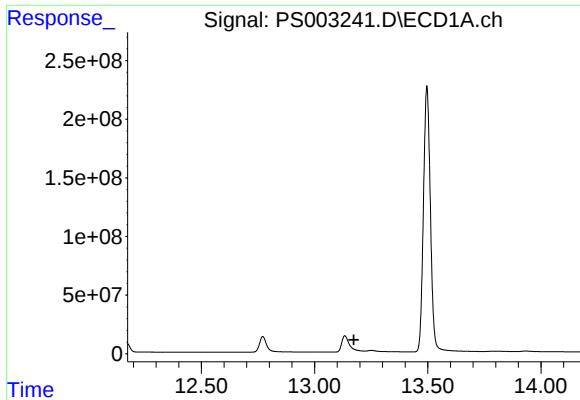

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.173 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

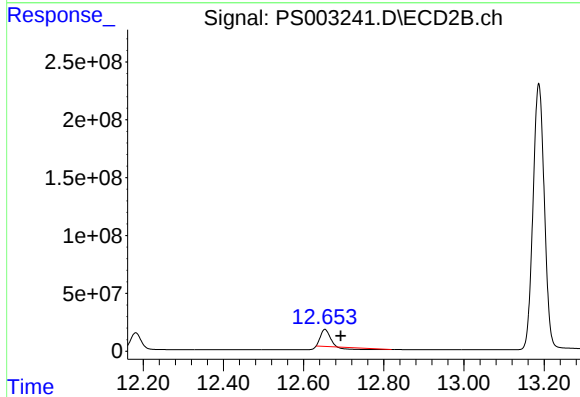


#9 2,4-D

R.T.: 12.653 min
Delta R.T.: -0.040 min
Response: 164537691
Conc: 328.17 ng/ml

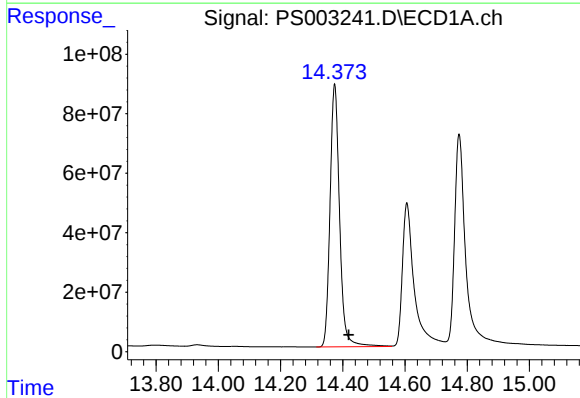


#11 2,4,5-TP (SILVEX)

R.T.: 14.374 min
Delta R.T.: -0.045 min
Response: 1880972566
Conc: 746.90 ng/ml

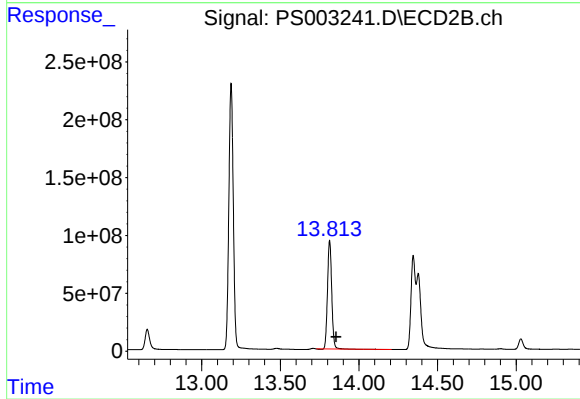

#11 2,4,5-TP (SILVEX)


R.T.: 13.813 min
Delta R.T.: -0.041 min
Response: 1740725374
Conc: 701.80 ng/ml

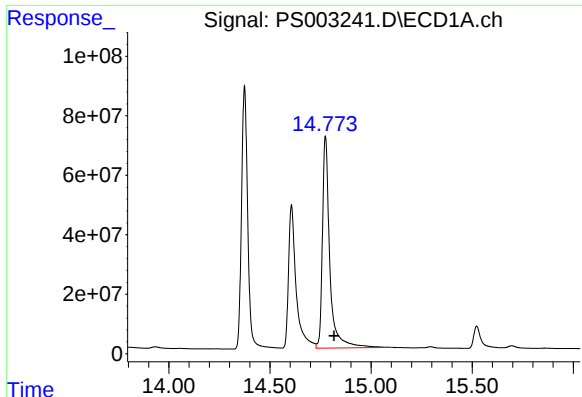

#12 2,4,5-T


R.T.: 14.774 min
Delta R.T.: -0.042 min
Response: 1809734841
Conc: 741.88 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

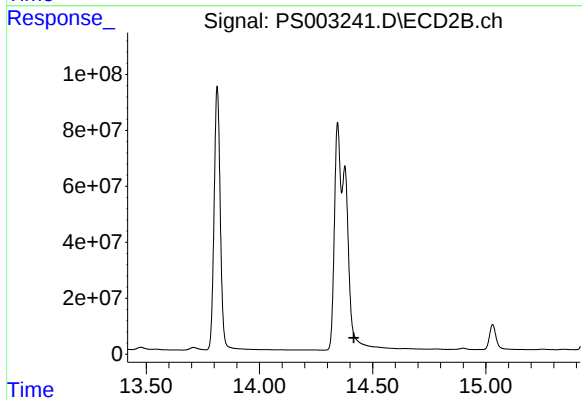


#12 2,4,5-T

R.T.: 14.377 min
Delta R.T.: -0.040 min
Response: -17651600
Conc: N.D.

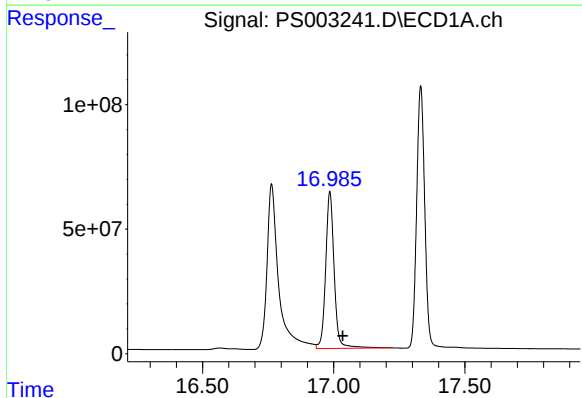


#14 DINOSEB

R.T.: 16.985 min
Delta R.T.: -0.050 min
Response: 1425470562
Conc: 757.69 ng/ml

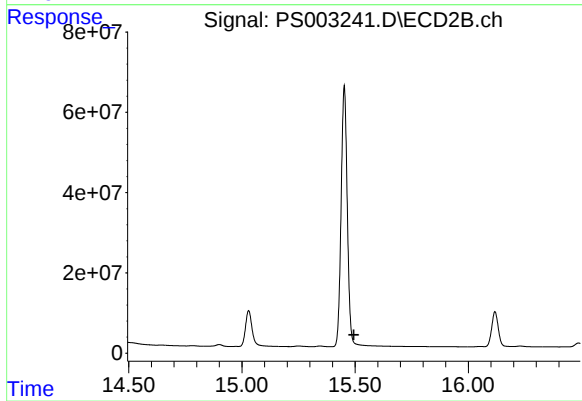

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 15.495 min
Response: 0
Conc: N.D.

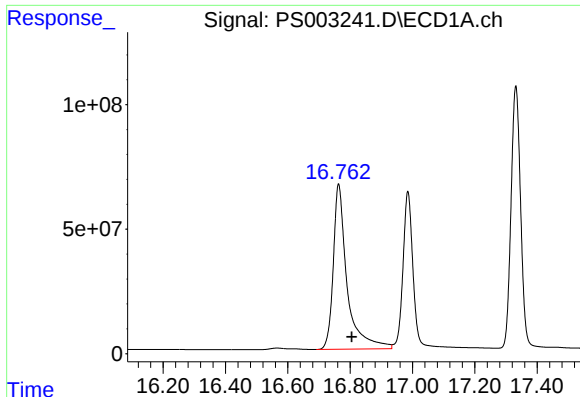

#15 Picloram


R.T.: 16.763 min
Delta R.T.: -0.043 min
Response: 2048592002
Conc: 647.54 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

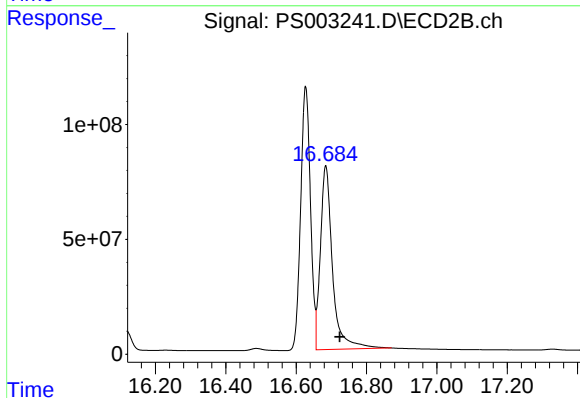


#15 Picloram

R.T.: 16.684 min
Delta R.T.: -0.040 min
Response: 1912095929
Conc: 636.01 ng/ml

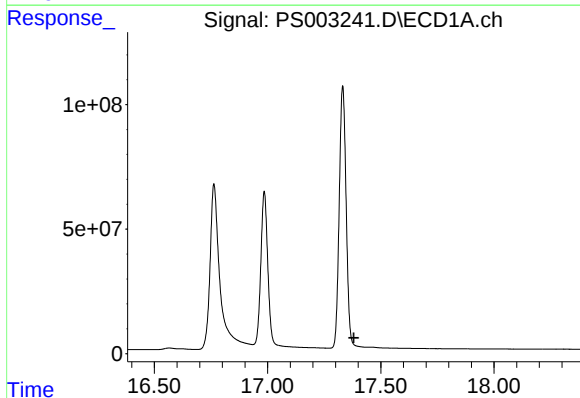

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

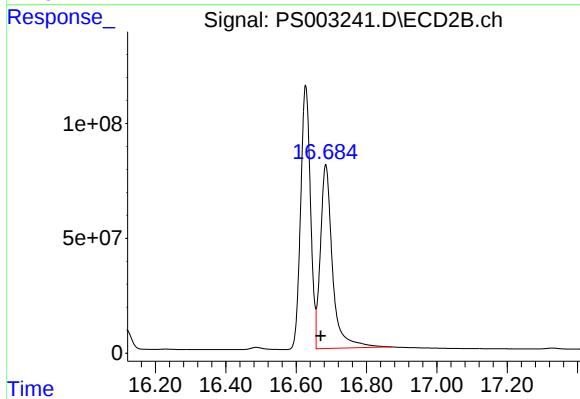

#16 DCPA

R.T.: 16.684 min
Delta R.T.: 0.014 min
Response: 1912095929
Conc: 617.29 ng/ml