

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021819\
 Data File : PS003242.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Feb 2019 23:13
 Operator : EI\SJ
 Sample : K1508-12
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 M-13-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 19 05:12:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.294	10.795	186.1E6	187.8E6	490.300	439.311
Target Compounds							
6) T	MCP	11.982	0.000	6628419	0	5.532	N.D. #
7) T	MCPA	12.163	0.000	27169195	0	15.350	N.D. #
12) T	2,4,5-T	0.000	14.415	0	6579282	N.D.	3.438 #
15) T	Picloram	16.843	16.722	3904635	15670743	1.234	5.212 #
16) T	DCPA	0.000	16.722	0	15670743	N.D.	5.059 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021819\
Data File : PS003242.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Feb 2019 23:13
Operator : EI\SJ
Sample : K1508-12
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
M-13-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 19 05:12:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

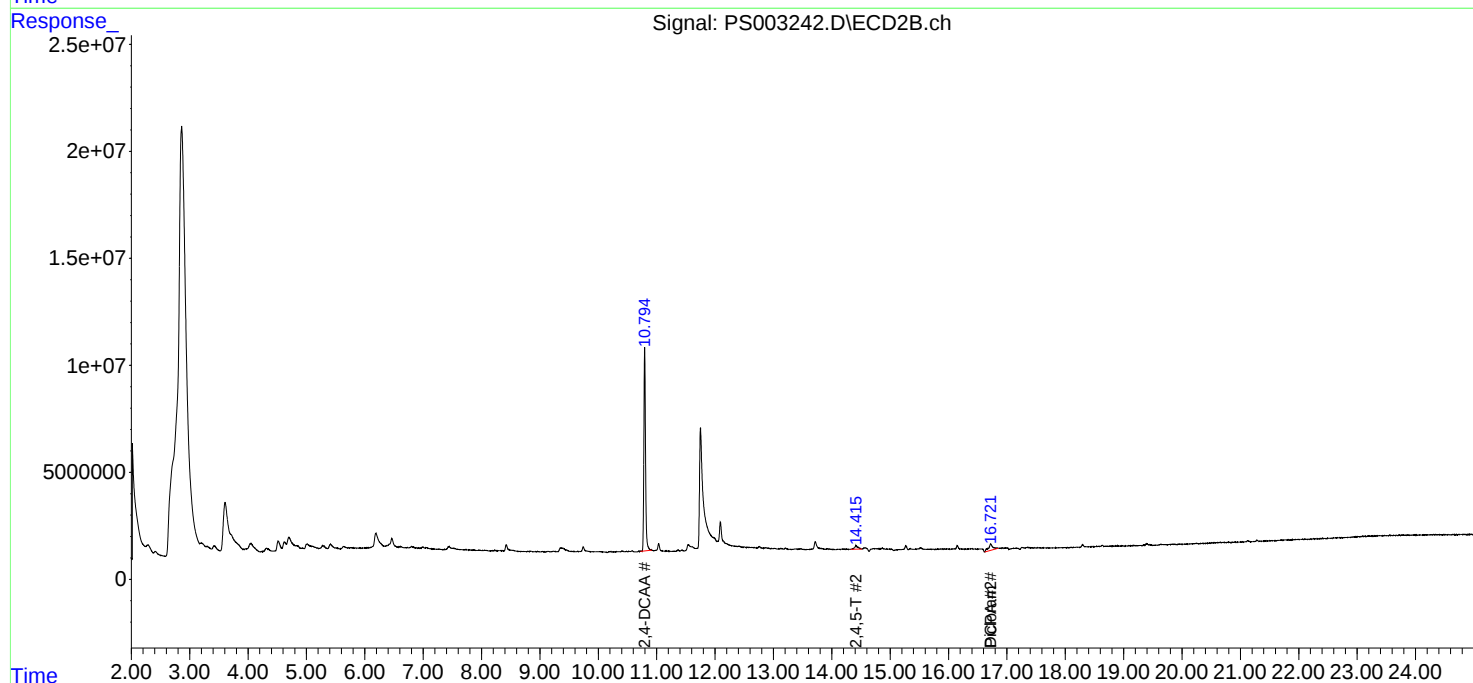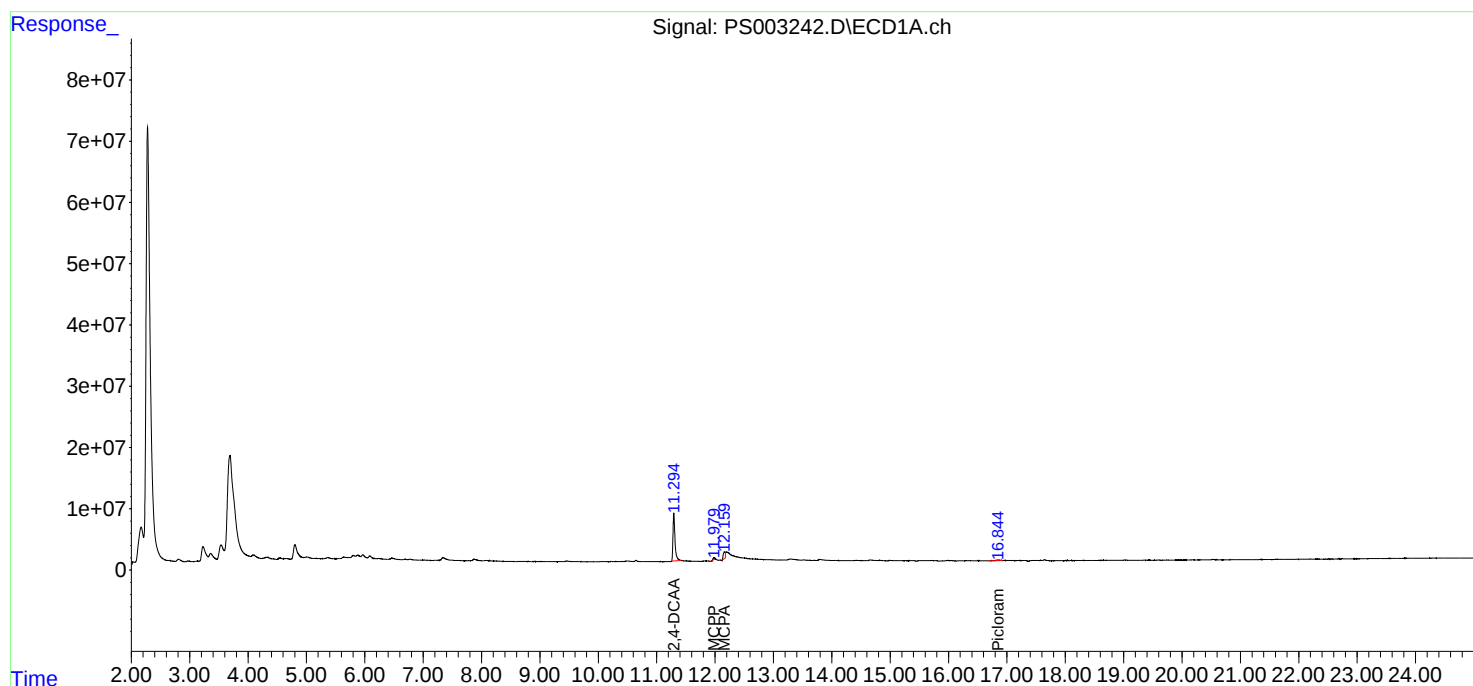


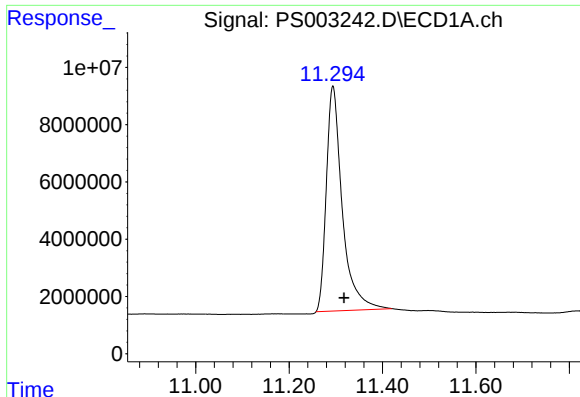

#4 2,4-DCAA


R.T.: 11.294 min
Delta R.T.: -0.023 min
Response: 186138052
Conc: 490.30 ng/ml

Instrument :
ECD_S
ClientSampleId :
M-13-S

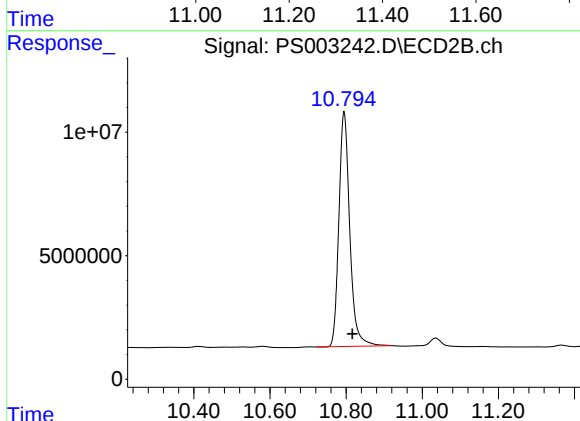


#4 2,4-DCAA

R.T.: 10.795 min
Delta R.T.: -0.022 min
Response: 187825358
Conc: 439.31 ng/ml

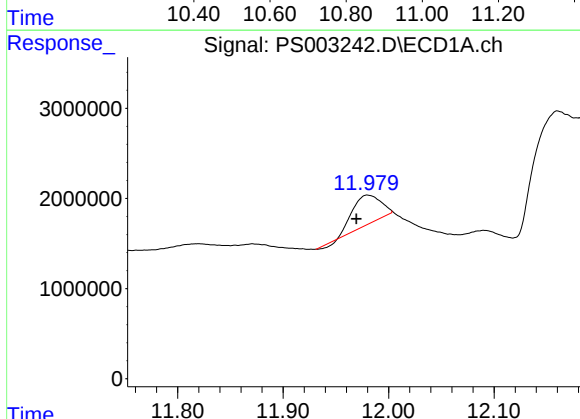


#6 MCP

R.T.: 11.982 min
Delta R.T.: 0.012 min
Response: 6628419
Conc: 5.53 ug/ml

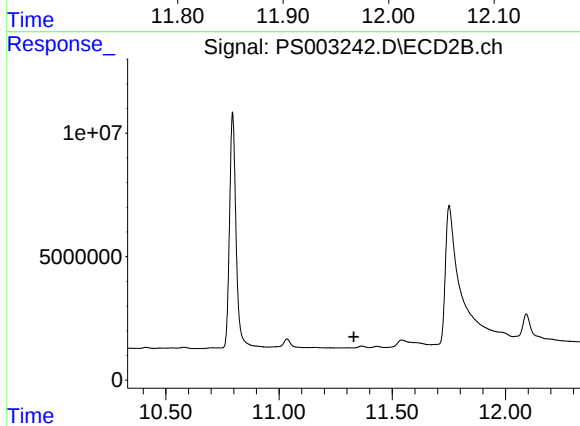

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.330 min
Response: 0
Conc: N.D.

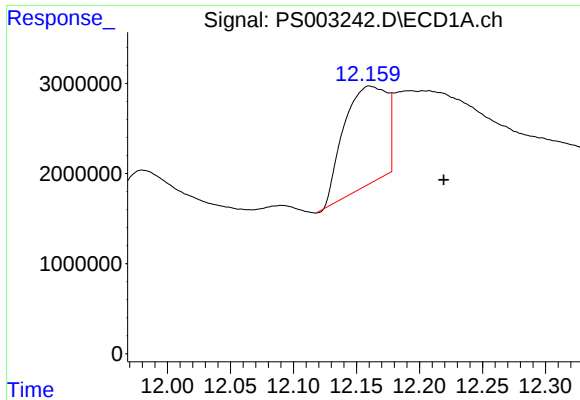

#7 MCPA


R.T.: 12.163 min
Delta R.T.: -0.056 min
Response: 27169195
Conc: 15.35 ug/ml

Instrument :
ECD_S
ClientSampleId :
M-13-S

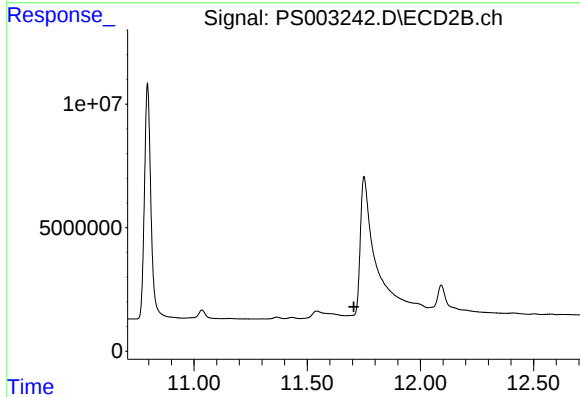


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 11.706 min
Response: 0
Conc: N.D.

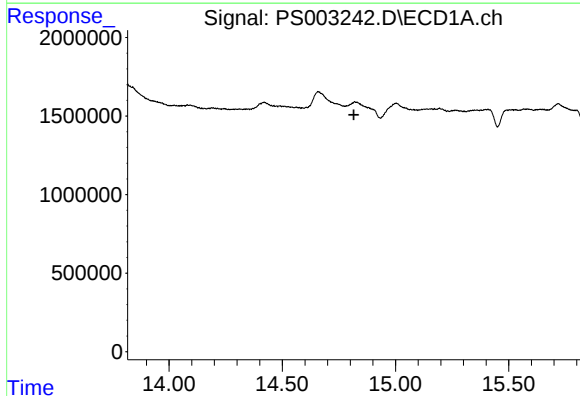


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.817 min
Response: 0
Conc: N.D.

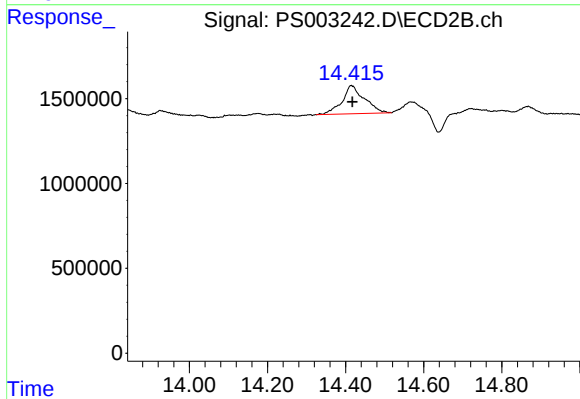

#12 2,4,5-T


R.T.: 14.415 min
Delta R.T.: -0.002 min
Response: 6579282
Conc: 3.44 ng/ml

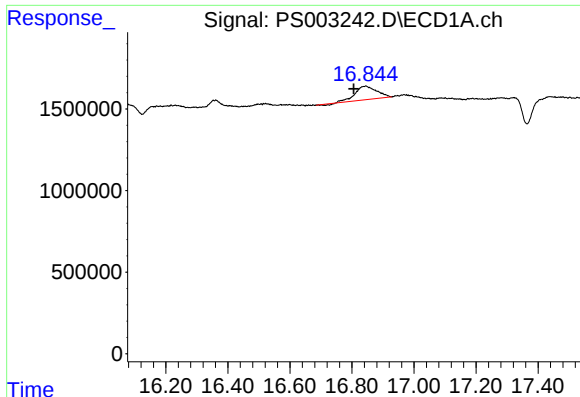

#15 Picloram


R.T.: 16.843 min
Delta R.T.: 0.037 min
Response: 3904635
Conc: 1.23 ng/ml

Instrument :
ECD_S
ClientSampleId :
M-13-S

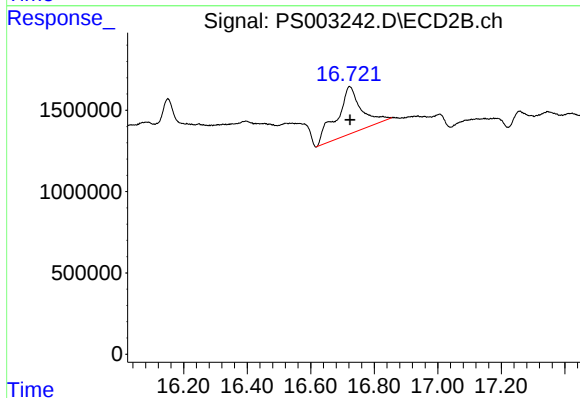


#15 Picloram

R.T.: 16.722 min
Delta R.T.: -0.002 min
Response: 15670743
Conc: 5.21 ng/ml

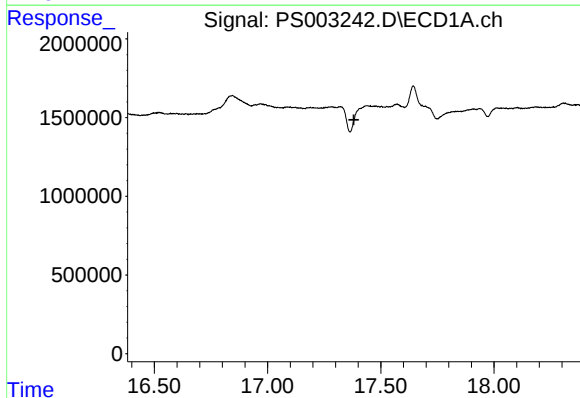

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

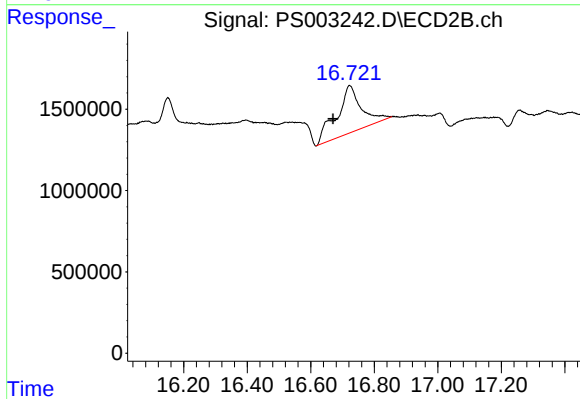

#16 DCPA

R.T.: 16.722 min
Delta R.T.: 0.053 min
Response: 15670743
Conc: 5.06 ng/ml