

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021819\
 Data File : PS003245.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Feb 2019 00:47
 Operator : EI\SJ
 Sample : K1513-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 FLOORS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 19 05:13:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.291	10.792	174.3E6	171.6E6	459.230	401.456
Target Compounds							
1) T	Dalapon	0.000	2.282	0	12960995	N.D.	24.185 #
5) T	DICAMBA	11.598	11.071	12734922	7353640	7.945	4.635 #
6) T	MCPD	11.964	0.000	14126962	0	11.791	N.D. #
8) T	DICHLORPROP	0.000	12.199	0	2953355	N.D.	7.724 #
9) T	2,4-D	13.156	12.672	44659222	53580784	96.862	106.865
10) T	Pentachlo...	13.517	13.205	23738052	14560671	3.702	2.356 #
14) T	DINOSEB	17.070	15.508	9260209	6130372	4.922	3.497 #
15) T	Picloram	16.805	16.712	28672744	36081764	9.063	12.002 #
16) T	DCPA	0.000	16.712	0	36081764	N.D.	11.648 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021819\
Data File : PS003245.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Feb 2019 00:47
Operator : EI\SJ
Sample : K1513-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
FLOORS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 19 05:13:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS021819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

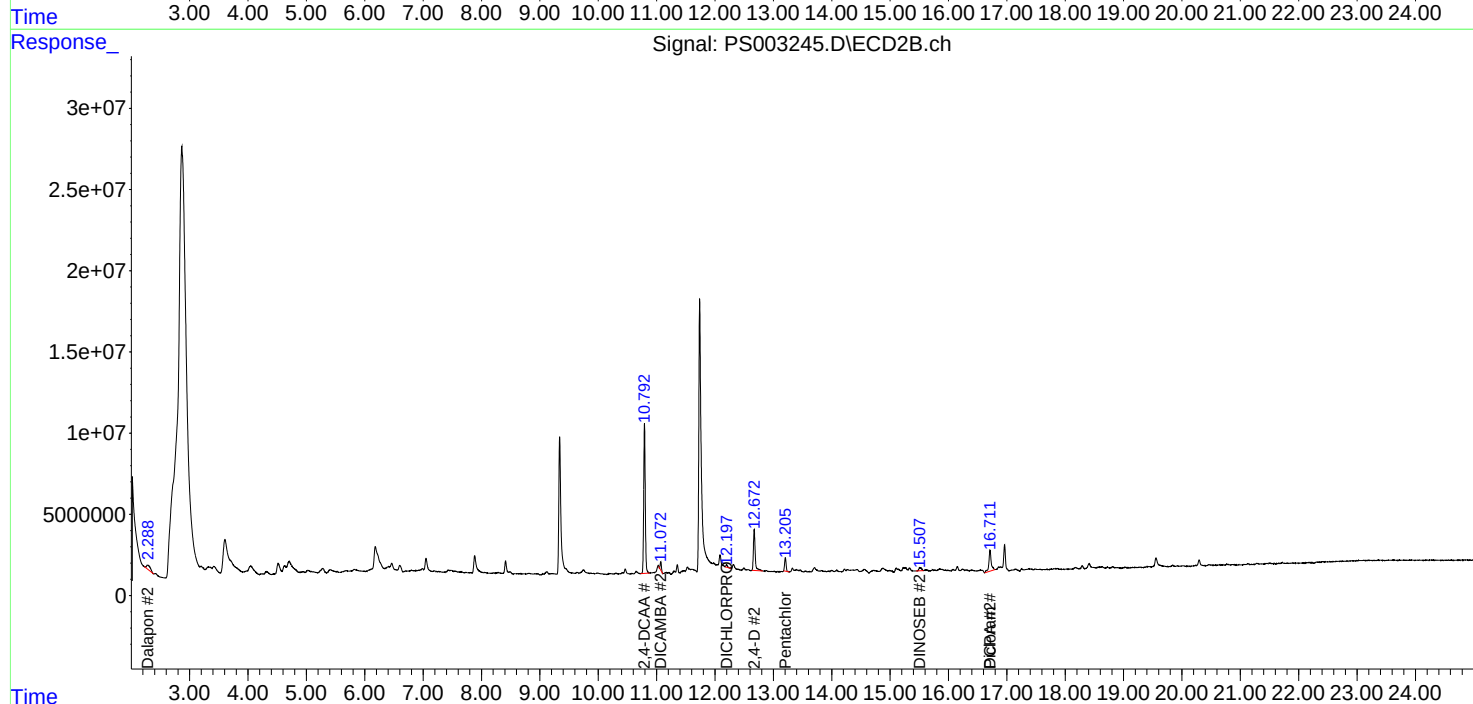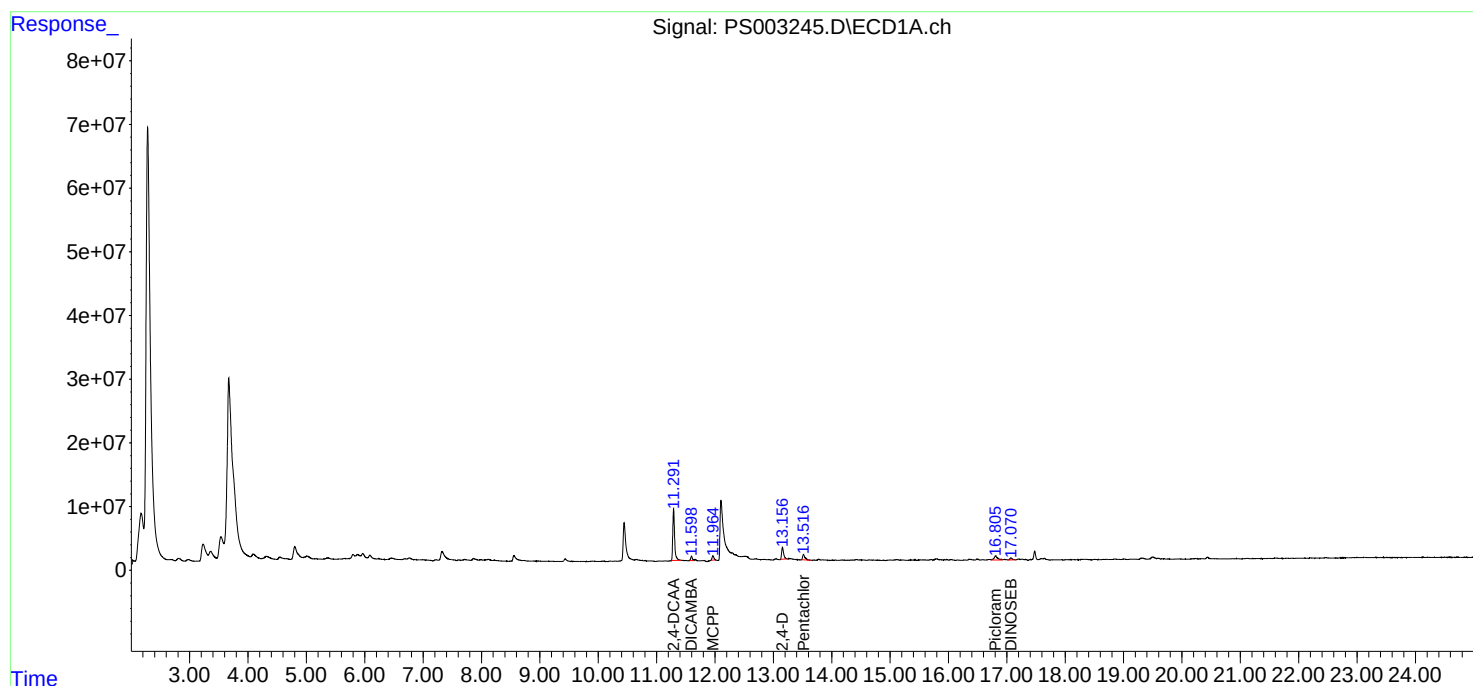


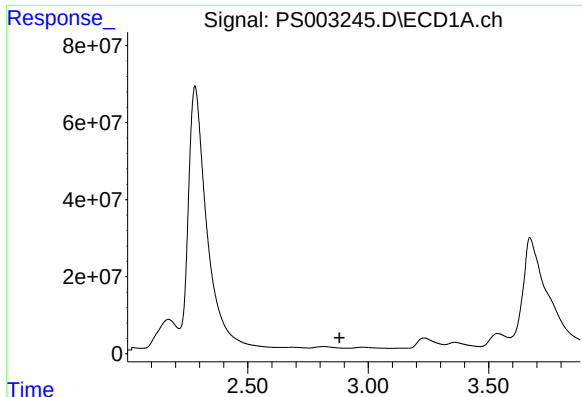

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FLOORS

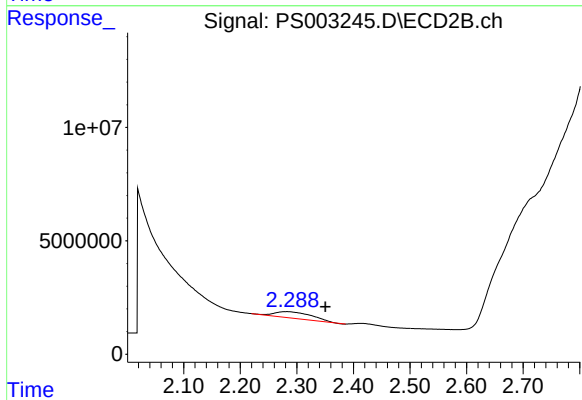


#1 Dalapon

R.T.: 2.282 min
Delta R.T.: -0.069 min
Response: 12960995
Conc: 24.18 ng/ml

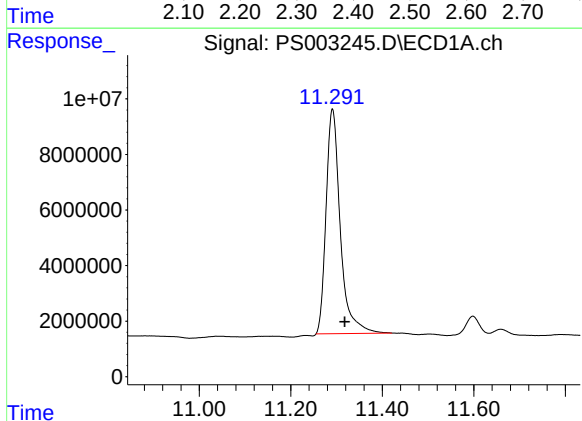


#4 2,4-DCAA

R.T.: 11.291 min
Delta R.T.: -0.027 min
Response: 174342375
Conc: 459.23 ng/ml

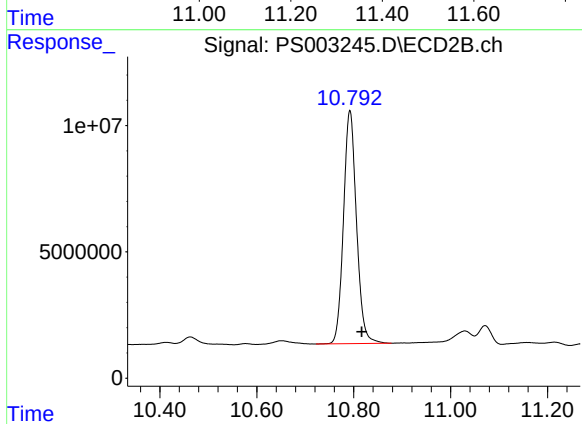

#4 2,4-DCAA


R.T.: 10.792 min
Delta R.T.: -0.024 min
Response: 171640749
Conc: 401.46 ng/ml

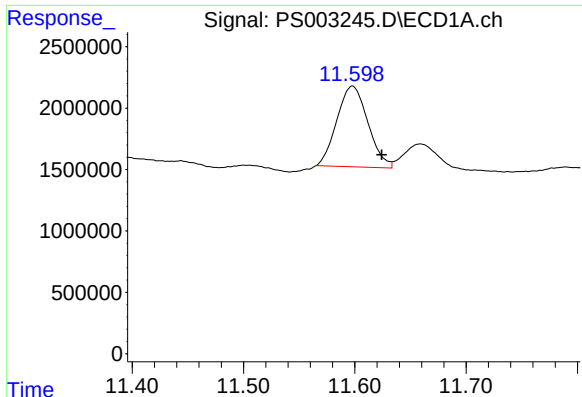

#5 DICAMBA


R.T.: 11.598 min
Delta R.T.: -0.026 min
Response: 12734922
Conc: 7.94 ng/ml

Instrument :
ECD_S
ClientSampleId :
FLOORS

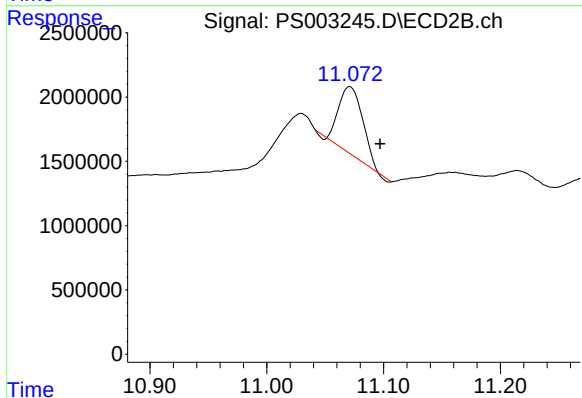


#5 DICAMBA

R.T.: 11.071 min
Delta R.T.: -0.026 min
Response: 7353640
Conc: 4.63 ng/ml

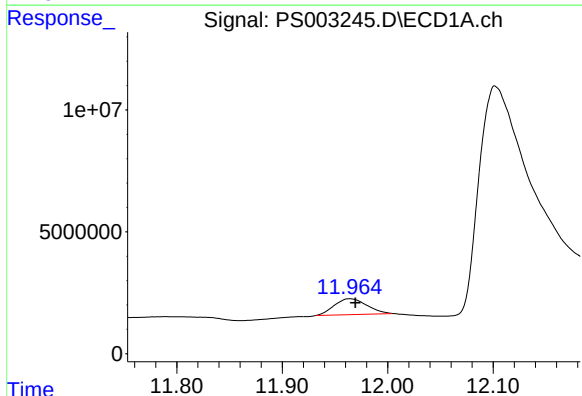


#6 MCP

R.T.: 11.964 min
Delta R.T.: -0.005 min
Response: 14126962
Conc: 11.79 ug/ml

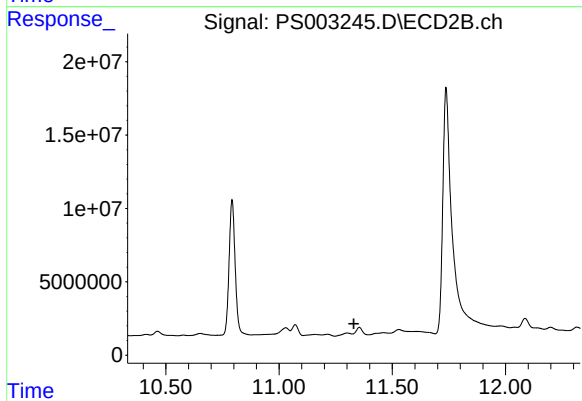

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.330 min
Response: 0
Conc: N.D.

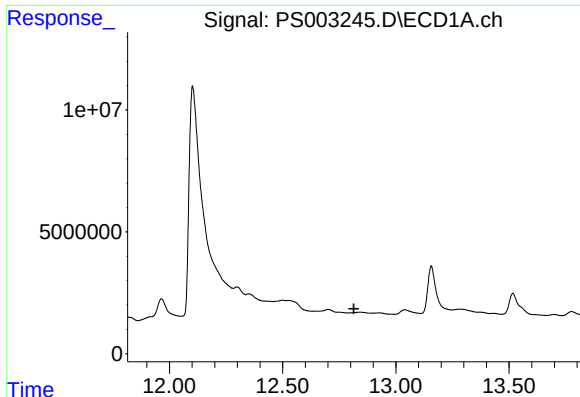

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.815 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FLOORS

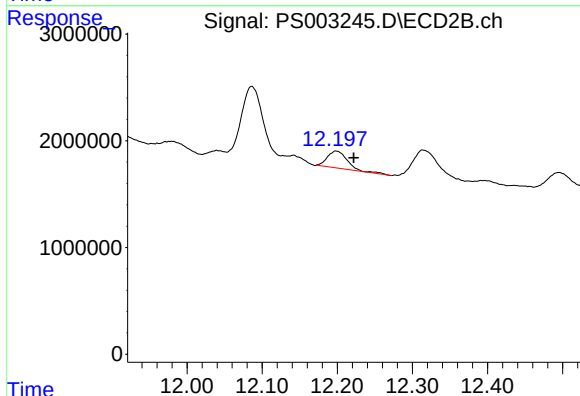


#8 DICHLORPROP

R.T.: 12.199 min
Delta R.T.: -0.023 min
Response: 2953355
Conc: 7.72 ng/ml

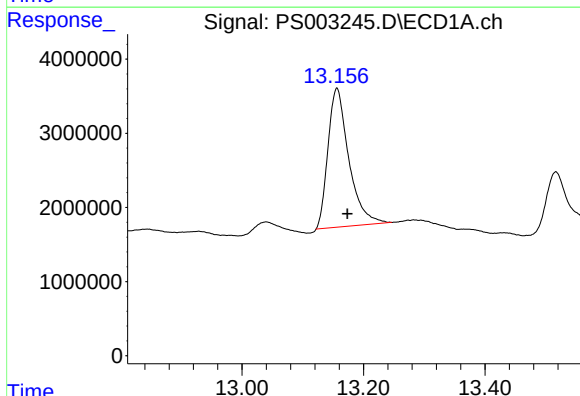


#9 2,4-D

R.T.: 13.156 min
Delta R.T.: -0.017 min
Response: 44659222
Conc: 96.86 ng/ml

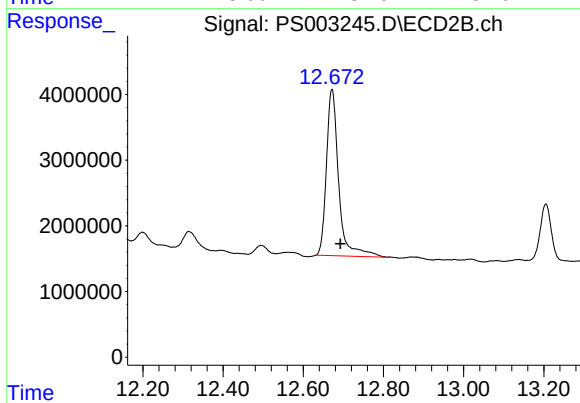

#9 2,4-D


R.T.: 12.672 min
Delta R.T.: -0.021 min
Response: 53580784
Conc: 106.87 ng/ml

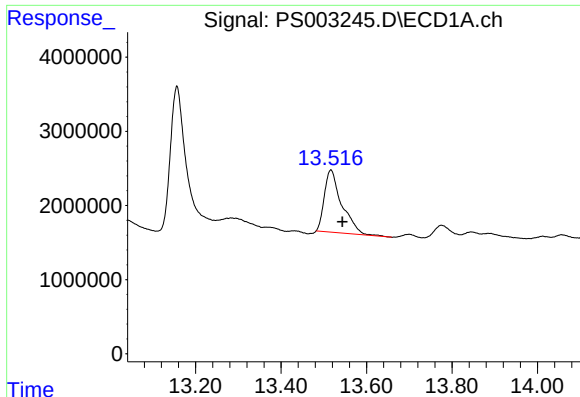

#10 Pentachlorophenol


R.T.: 13.517 min
Delta R.T.: -0.027 min
Response: 23738052
Conc: 3.70 ng/ml

Instrument :
ECD_S
ClientSampleId :
FLOORS

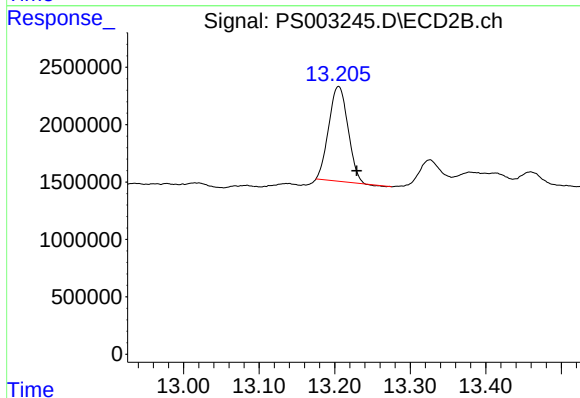


#10 Pentachlorophenol

R.T.: 13.205 min
Delta R.T.: -0.024 min
Response: 14560671
Conc: 2.36 ng/ml

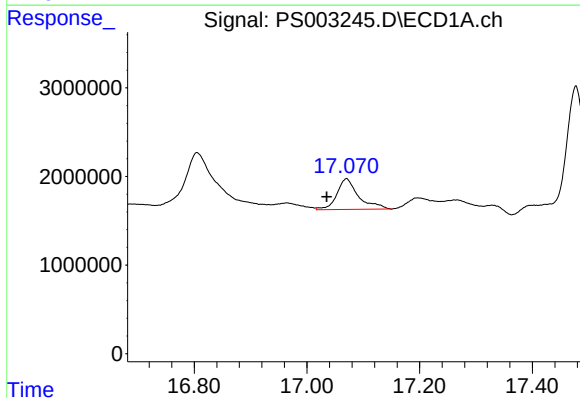


#14 DINOSEB

R.T.: 17.070 min
Delta R.T.: 0.035 min
Response: 9260209
Conc: 4.92 ng/ml

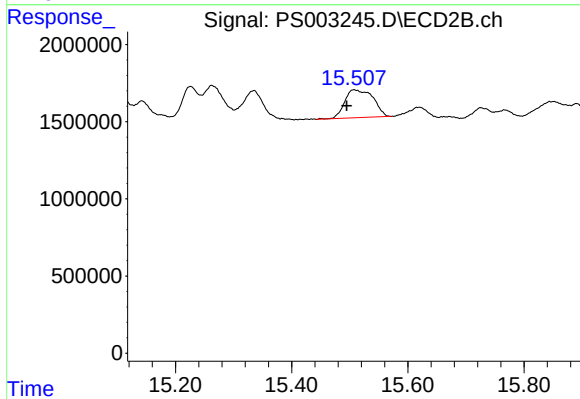

#14 DINOSEB


R.T.: 15.508 min
Delta R.T.: 0.013 min
Response: 6130372
Conc: 3.50 ng/ml

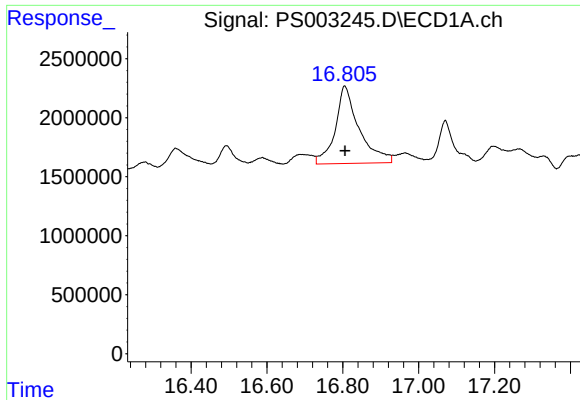

#15 Picloram


R.T.: 16.805 min
Delta R.T.: 0.000 min
Response: 28672744
Conc: 9.06 ng/ml

Instrument :
ECD_S
ClientSampleId :
FLOORS

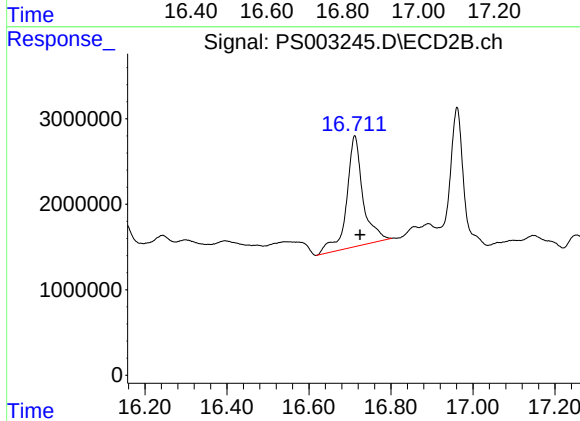


#15 Picloram

R.T.: 16.712 min
Delta R.T.: -0.013 min
Response: 36081764
Conc: 12.00 ng/ml

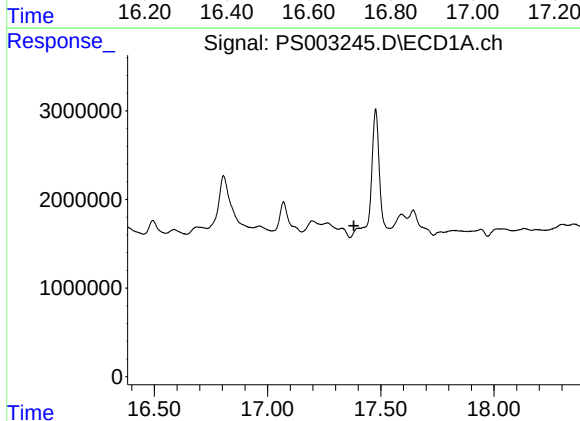

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

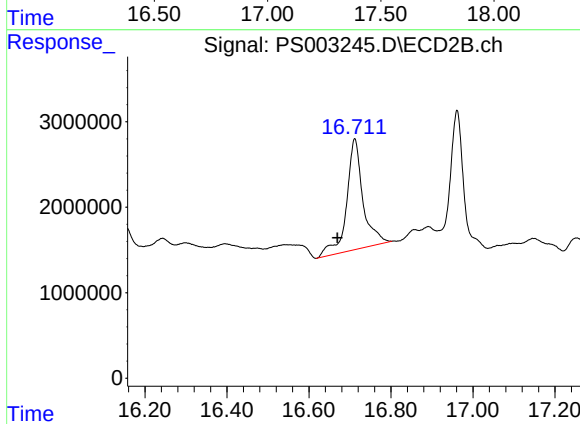

#16 DCPA

R.T.: 16.712 min
Delta R.T.: 0.042 min
Response: 36081764
Conc: 11.65 ng/ml