

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021819\
 Data File : PS003247.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Feb 2019 01:49
 Operator : EI\SJ
 Sample : K1513-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 INNER-WALL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 19 05:14:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.314	10.815	148.4E6	147.0E6	391.001	343.751
Target Compounds							
1) T	Dalapon	2.839	0.000	6500591	0	11.784	N.D. #
5) T	DICAMBA	11.687	0.000	1941444	0	1.211	N.D. #
6) T	MCPD	11.989	11.327	6617613	1704099	5.523	1.545 #
7) T	MCPA	0.000	11.764	0	282.5E6	N.D.	179.577 #
10) T	Pentachlo...	13.538	13.227	14451506	10185749	2.253	1.648 #
11) T	2,4,5-TP ...	14.439	0.000	3440038	0	1.366	N.D. #
14) T	DINOSEB	0.000	15.529	0	5259148	N.D.	3.000 #
15) T	Picloram	16.790	16.779	7073844	8255432	2.236	2.746



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021819\
Data File : PS003247.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Feb 2019 01:49
Operator : EI\SJ
Sample : K1513-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleID :
INNER-WALL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 19 05:14:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

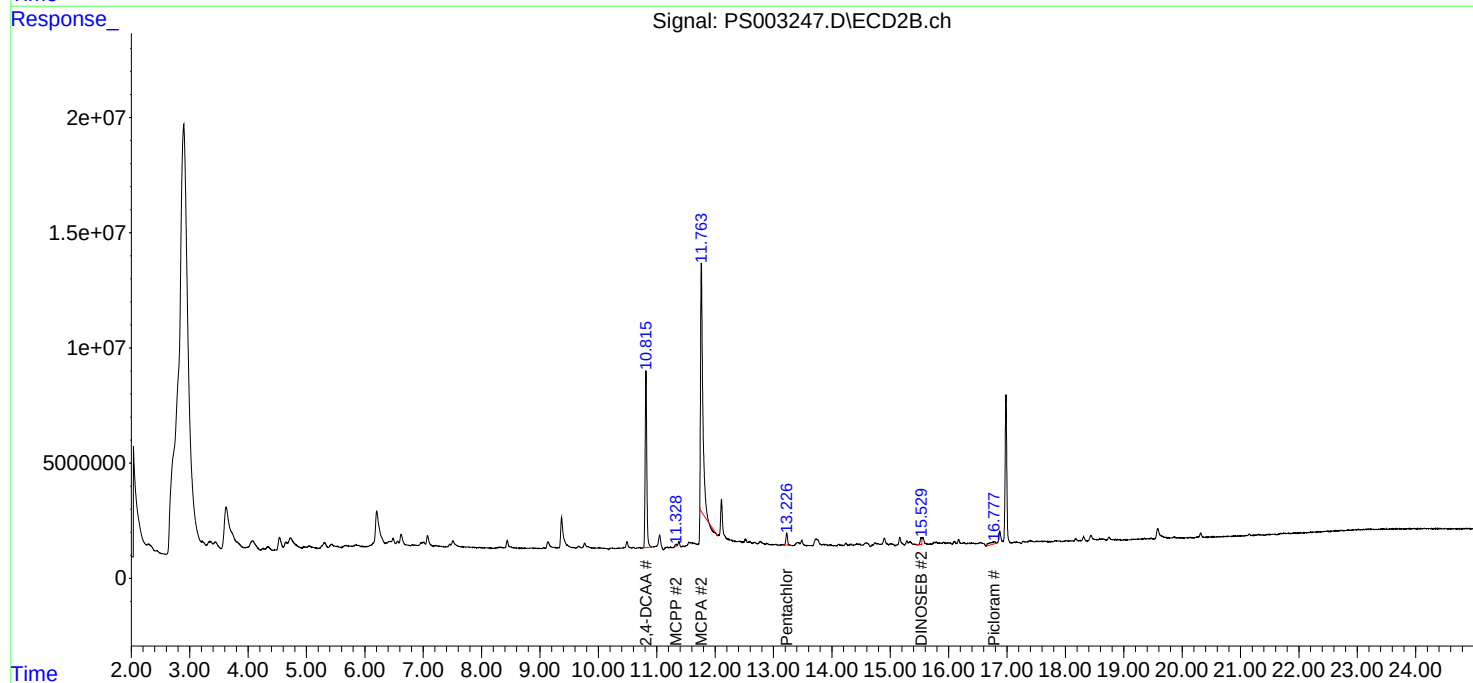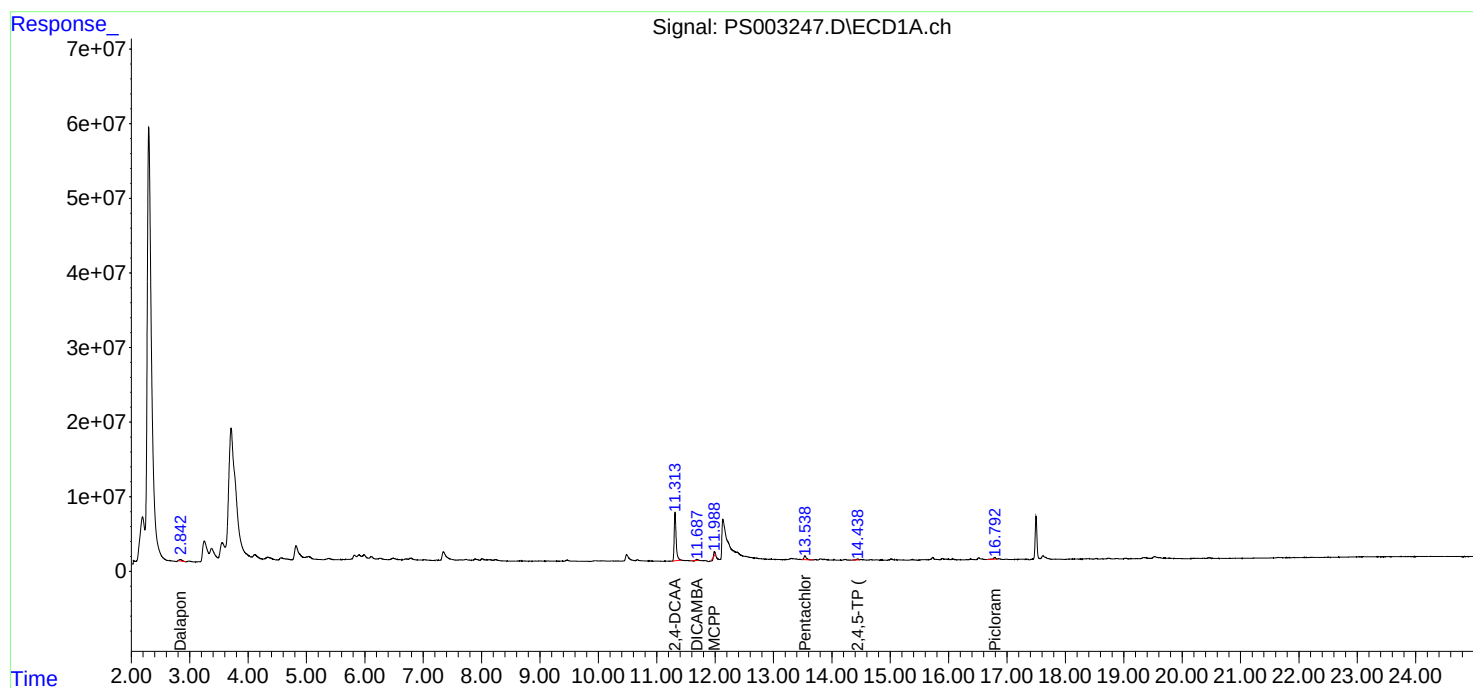


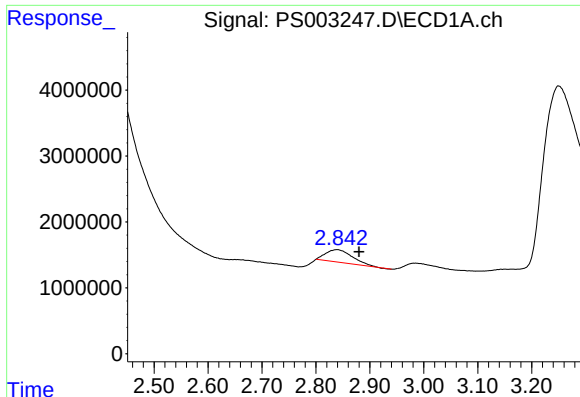

#1 Dalapon


R.T.: 2.839 min
Delta R.T.: -0.041 min
Response: 6500591
Conc: 11.78 ng/ml

Instrument :
ECD_S
ClientSampleId :
INNER-WALL

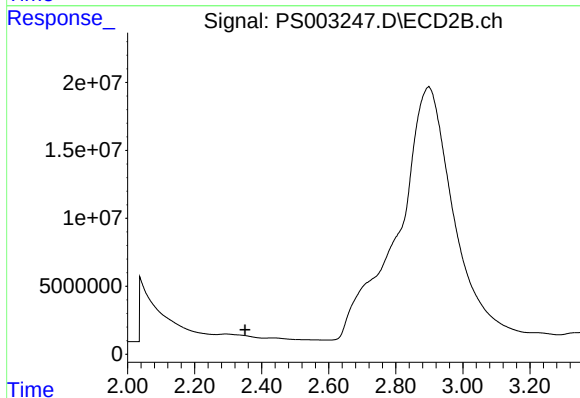


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.351 min
Response: 0
Conc: N.D.

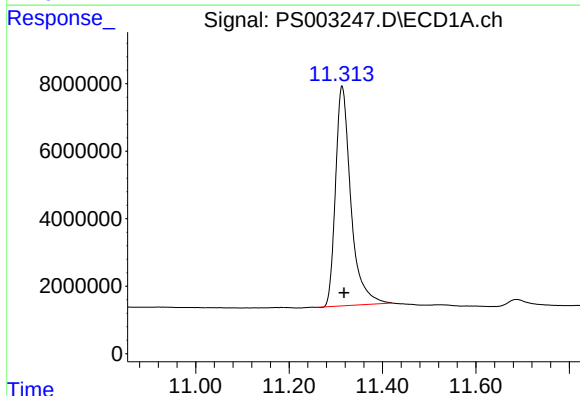


#4 2,4-DCAA

R.T.: 11.314 min
Delta R.T.: -0.004 min
Response: 148439864
Conc: 391.00 ng/ml

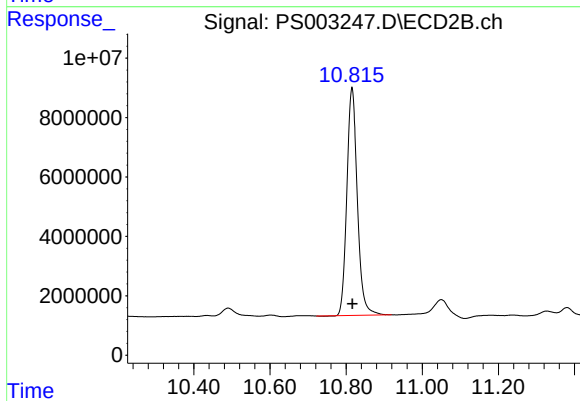

#4 2,4-DCAA


R.T.: 10.815 min
Delta R.T.: -0.001 min
Response: 146969314
Conc: 343.75 ng/ml

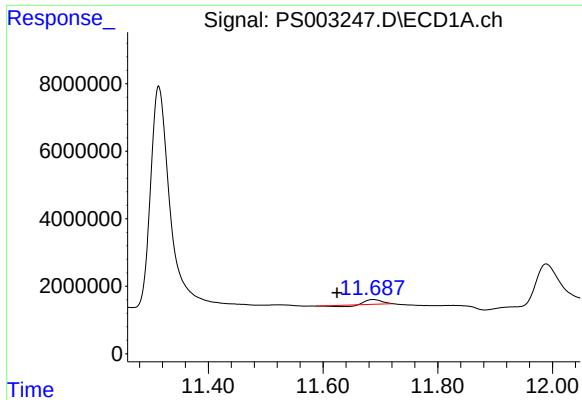

#5 DICAMBA


R.T.: 11.687 min
Delta R.T.: 0.063 min
Response: 1941444
Conc: 1.21 ng/ml

Instrument :
ECD_S
ClientSampleId :
INNER-WALL

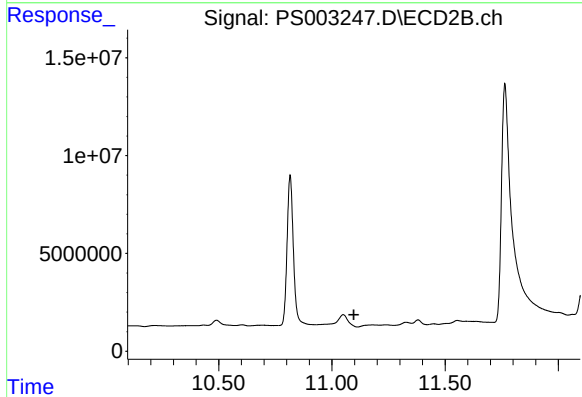


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 11.097 min
Response: 0
Conc: N.D.

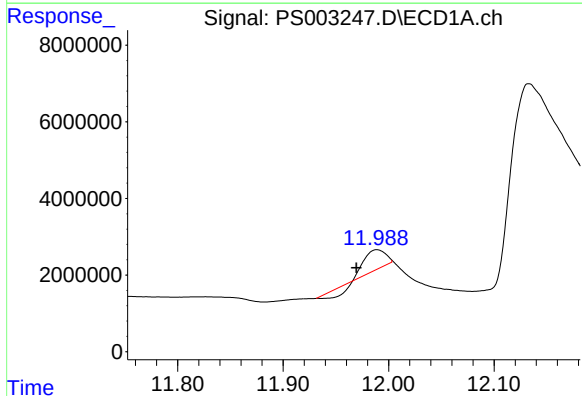


#6 MCP

R.T.: 11.989 min
Delta R.T.: 0.020 min
Response: 6617613
Conc: 5.52 ug/ml

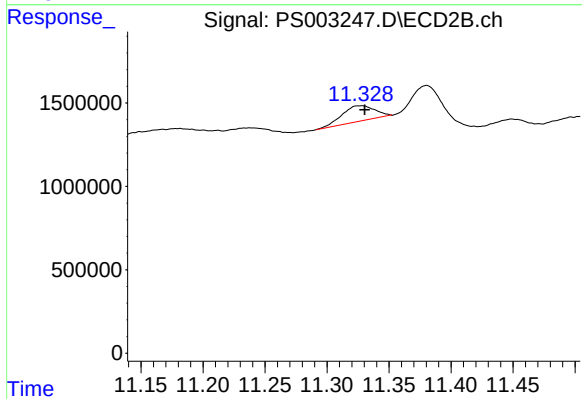

#6 MCP


R.T.: 11.327 min
Delta R.T.: -0.003 min
Response: 1704099
Conc: 1.55 ug/ml

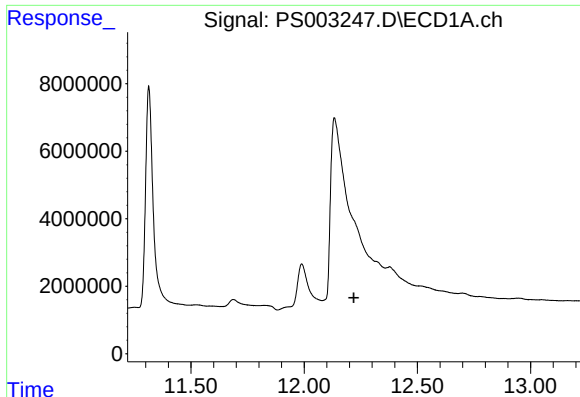

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.219 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
INNER-WALL

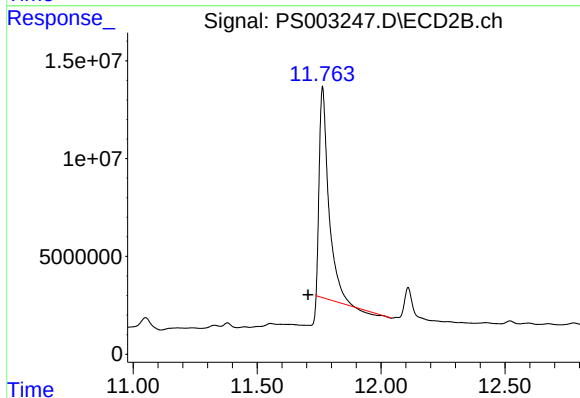


#7 MCPA

R.T.: 11.764 min
Delta R.T.: 0.058 min
Response: 282486214
Conc: 179.58 ug/ml

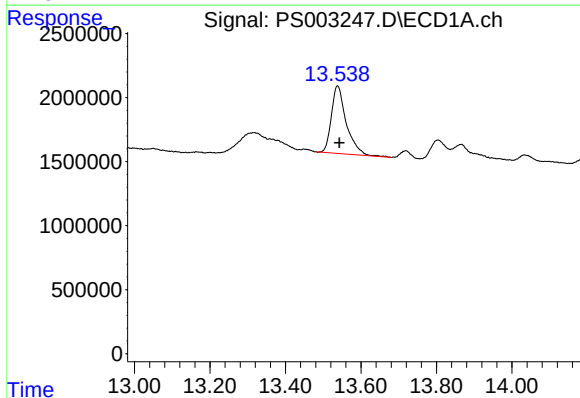


#10 Pentachlorophenol

R.T.: 13.538 min
Delta R.T.: -0.005 min
Response: 14451506
Conc: 2.25 ng/ml

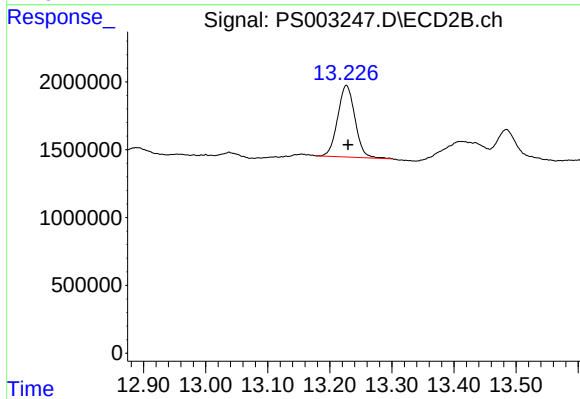

#10 Pentachlorophenol


R.T.: 13.227 min
Delta R.T.: -0.003 min
Response: 10185749
Conc: 1.65 ng/ml

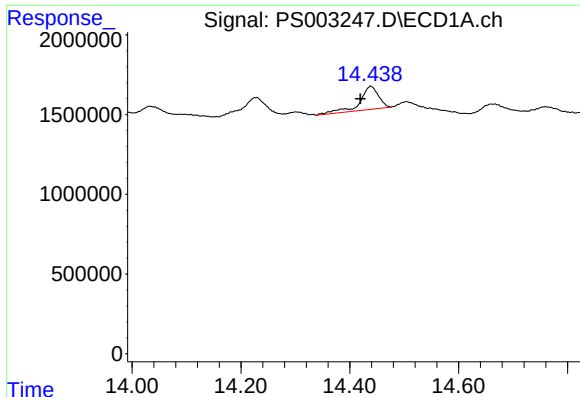

#11 2,4,5-TP (SILVEX)


R.T.: 14.439 min
Delta R.T.: 0.019 min
Response: 3440038
Conc: 1.37 ng/ml

Instrument :
ECD_S
ClientSampleId :
INNER-WALL

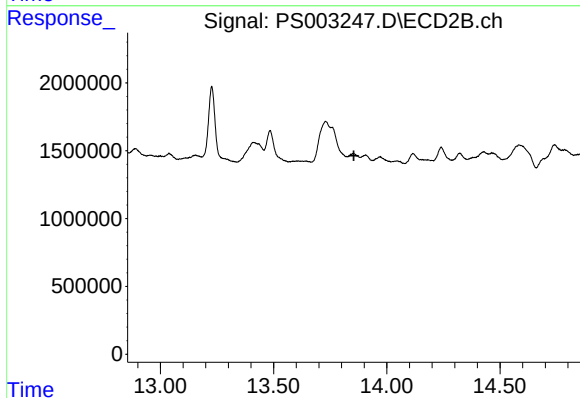


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 13.854 min
Response: 0
Conc: N.D.

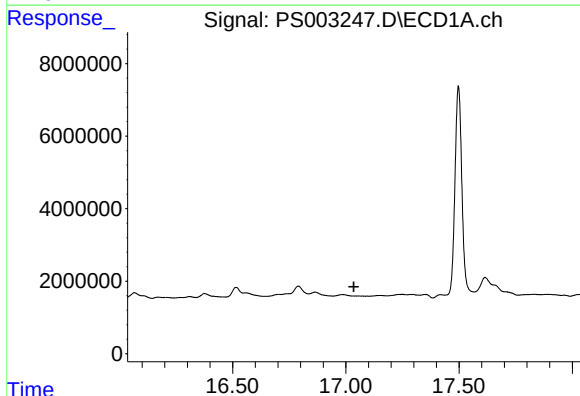


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.035 min
Response: 0
Conc: N.D.

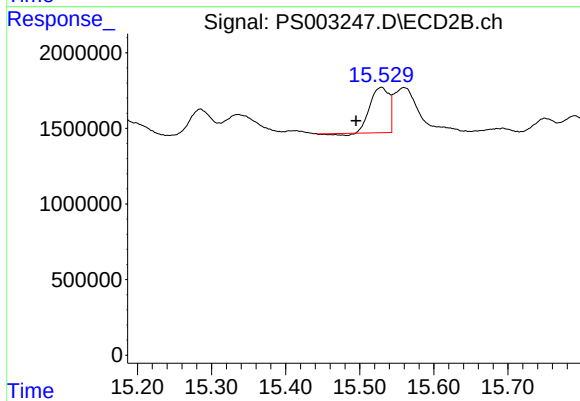

#14 DINOSEB


R.T.: 15.529 min
Delta R.T.: 0.034 min
Response: 5259148
Conc: 3.00 ng/ml

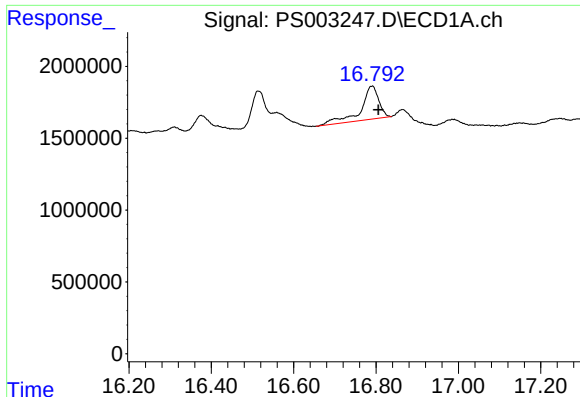

#15 Picloram

R.T.: 16.790 min
Delta R.T.: -0.015 min
Response: 7073844
Conc: 2.24 ng/ml

Instrument :
ECD_S
ClientSampleId :
INNER-WALL

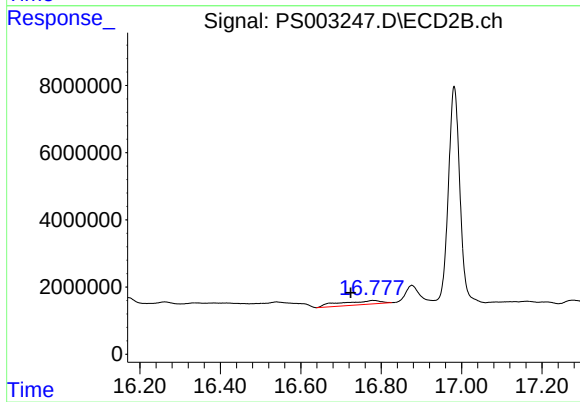

#15 Picloram

R.T.: 16.779 min
Delta R.T.: 0.055 min
Response: 8255432
Conc: 2.75 ng/ml