

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021820\
 Data File : PS008871.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Feb 2020 09:46
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 19 00:44:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 05 02:36:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.250	6.941	937.1E6	461.4E6	436.588	497.824
Target Compounds							
12) T	2,4,5-T	9.516	9.262	73793609	150.8E6	6.705	29.183 #
15) T	Picloram	11.049	11.033	645.8E6	343.8E6	42.644	45.545
16) T	DCPA	11.500	11.033	65640539	343.8E6	4.682	52.855 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021820\
Data File : PS008871.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Feb 2020 09:46
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 19 00:44:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
Quant Title : 8080.M
QLast Update : Wed Feb 05 02:36:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

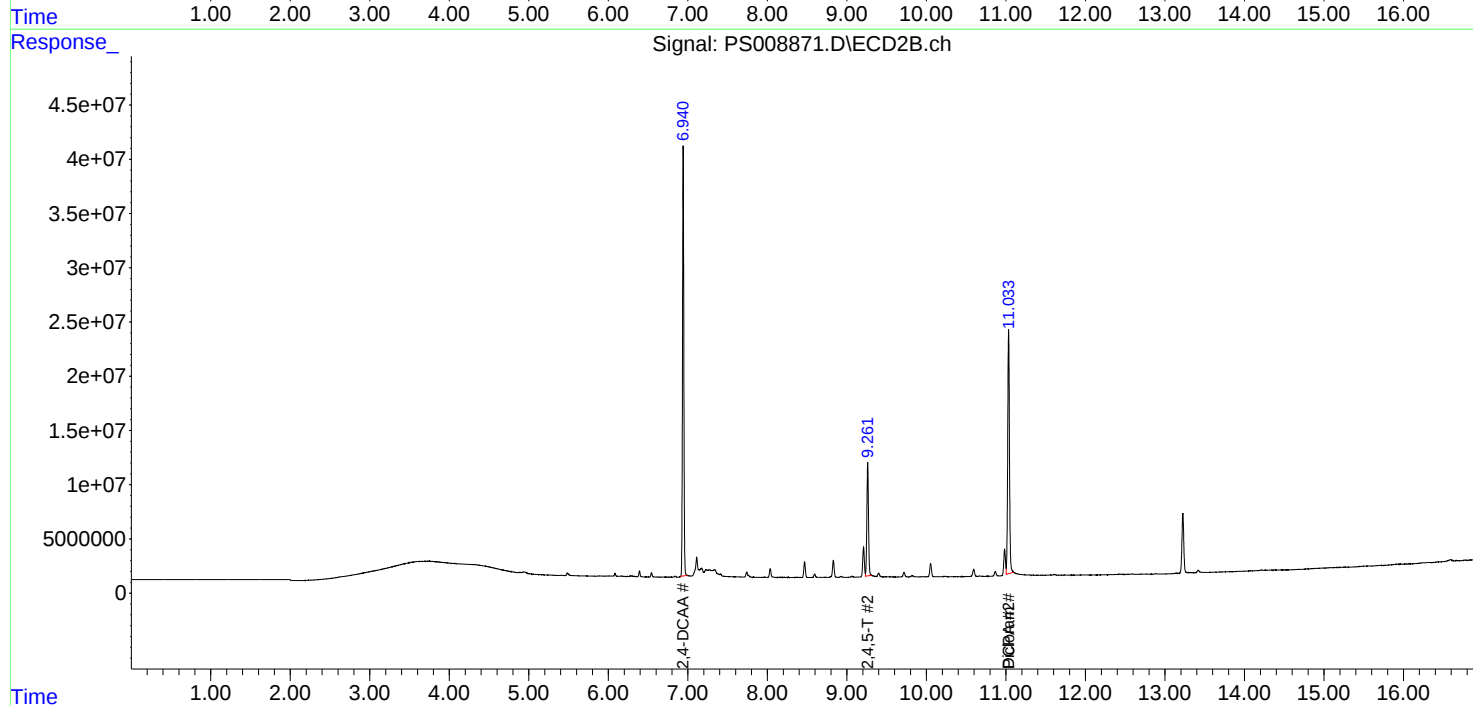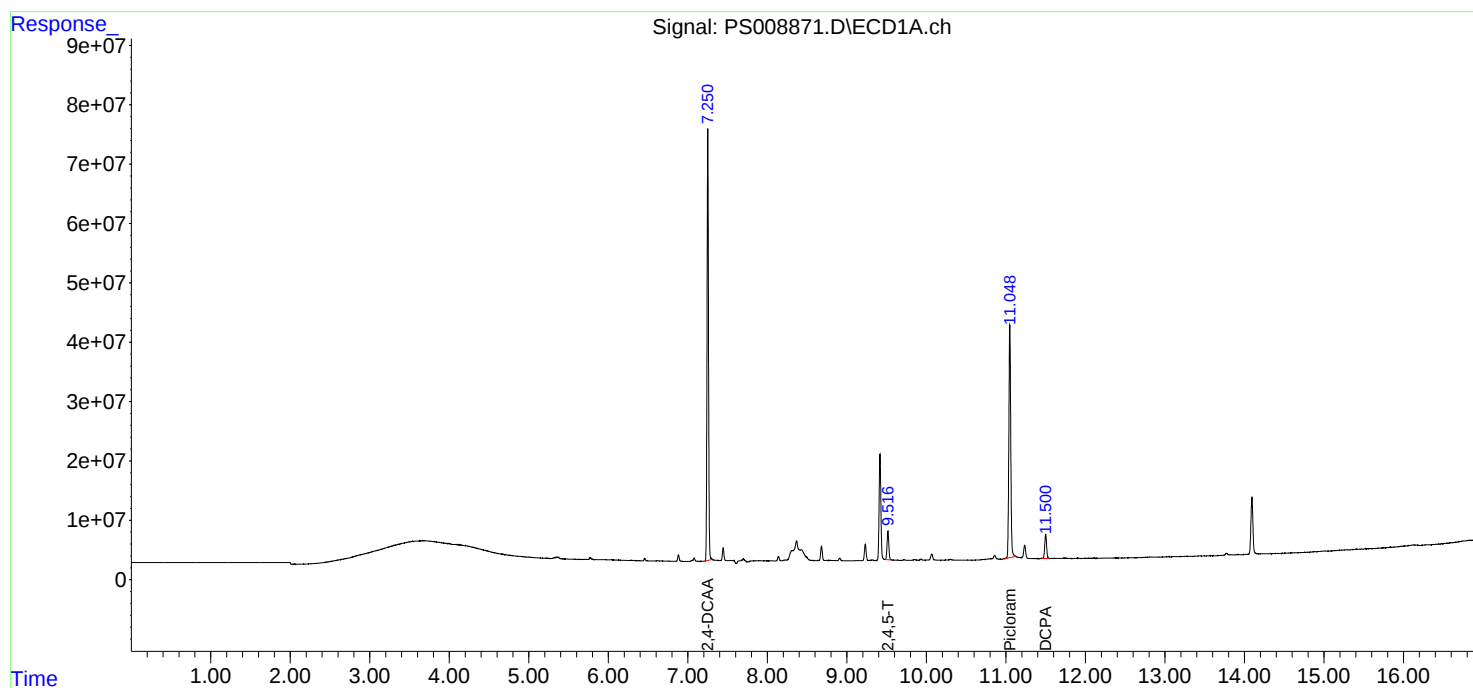


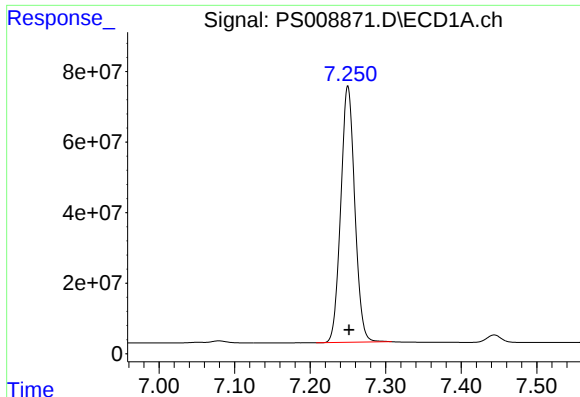

#4 2,4-DCAA


R.T.: 7.250 min
Delta R.T.: -0.002 min
Response: 937053128
Conc: 436.59 ng/ml

Instrument :
ECD_S
ClientSampleId :

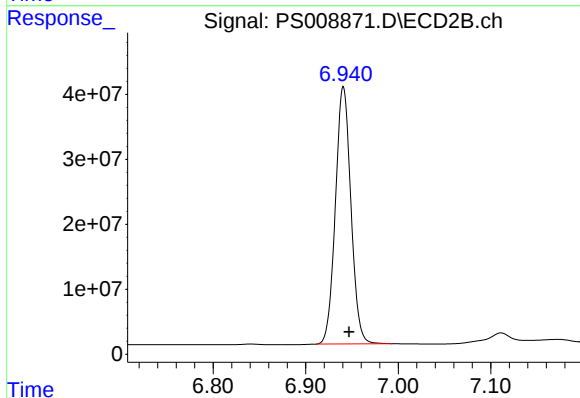


#4 2,4-DCAA

R.T.: 6.941 min
Delta R.T.: -0.006 min
Response: 461395271
Conc: 497.82 ng/ml

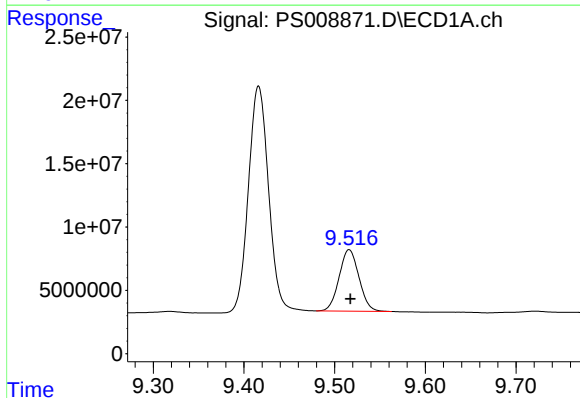


#12 2,4,5-T

R.T.: 9.516 min
Delta R.T.: -0.001 min
Response: 73793609
Conc: 6.70 ng/ml

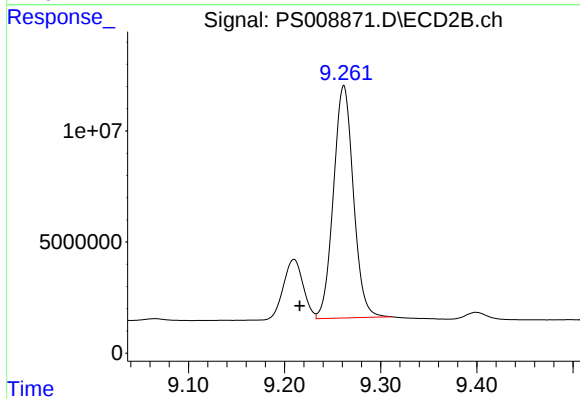

#12 2,4,5-T


R.T.: 9.262 min
Delta R.T.: 0.046 min
Response: 150804005
Conc: 29.18 ng/ml

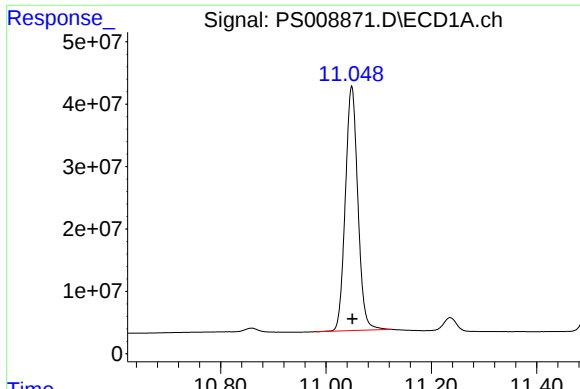

#15 Picloram


R.T.: 11.049 min
Delta R.T.: 0.000 min
Response: 645788260
Conc: 42.64 ng/ml

Instrument :
ECD_S
ClientSampleId :

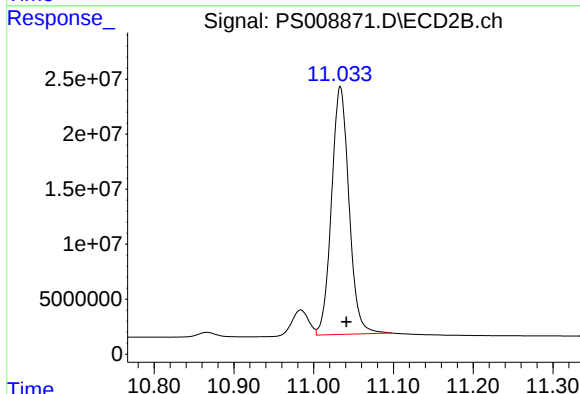


#15 Picloram

R.T.: 11.033 min
Delta R.T.: -0.008 min
Response: 343778382
Conc: 45.55 ng/ml

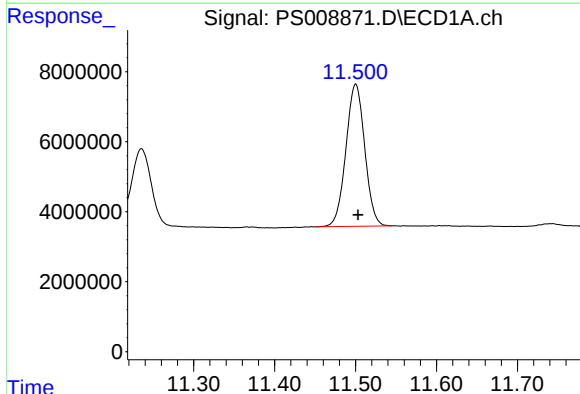

#16 DCPA

R.T.: 11.500 min
Delta R.T.: -0.003 min
Response: 65640539
Conc: 4.68 ng/ml

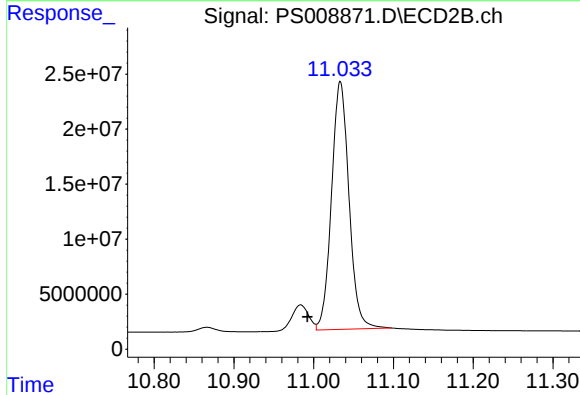

#16 DCPA

R.T.: 11.033 min
Delta R.T.: 0.041 min
Response: 343778382
Conc: 52.85 ng/ml