

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021820\
 Data File : PS008873.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Feb 2020 11:04
 Operator : DD\AJ
 Sample : PB126847BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 19 00:45:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 05 02:36:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.250	6.941	1064.4E6	505.0E6	495.912	544.874
Target Compounds							
1) T	Dalapon	0.000	2.588	0	286.4E6	N.D.	238.778
2) T	3,5-DICHL...	0.000	6.114	0	107.4E6	N.D.	78.056
6) T	MCP	7.690	0.000	99857070	0	16.245	N.D. #
12) T	2,4,5-T	0.000	9.261	0	161.1E6	N.D.	31.184
15) T	Picloram	11.047	11.033	1047.4E6	561.6E6	69.161	74.397
16) T	DCPA	0.000	11.033	0	561.6E6	N.D.	86.338



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021820\
Data File : PS008873.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Feb 2020 11:04
Operator : DD\AJ
Sample : PB126847BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 19 00:45:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
Quant Title : 8080.M
QLast Update : Wed Feb 05 02:36:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

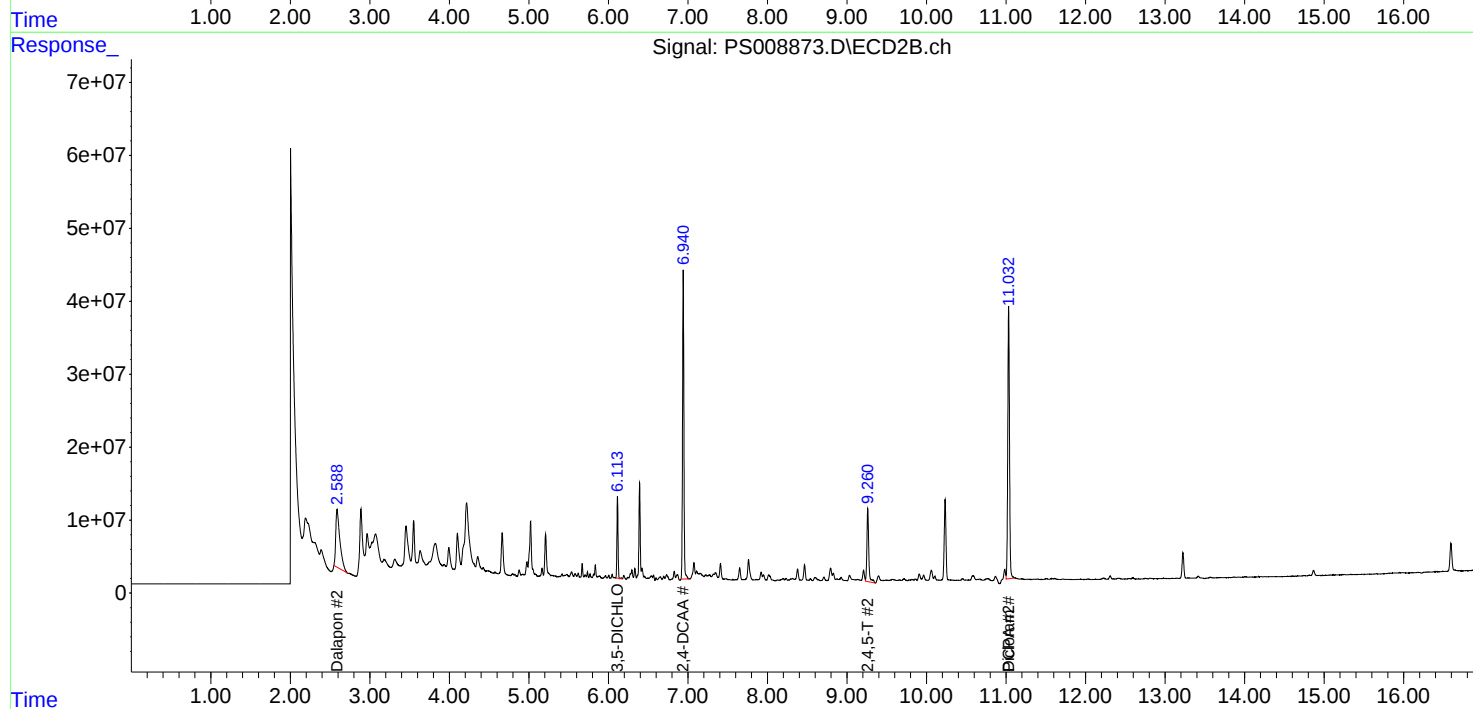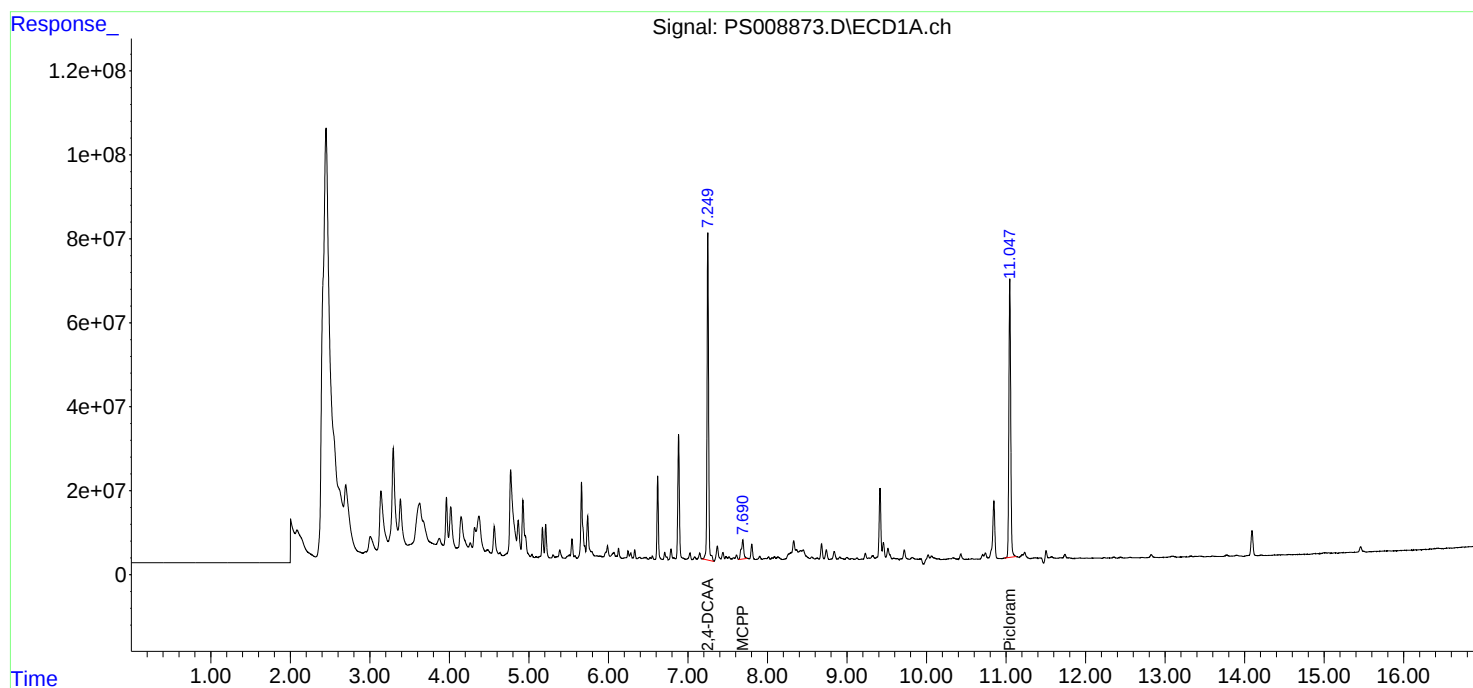


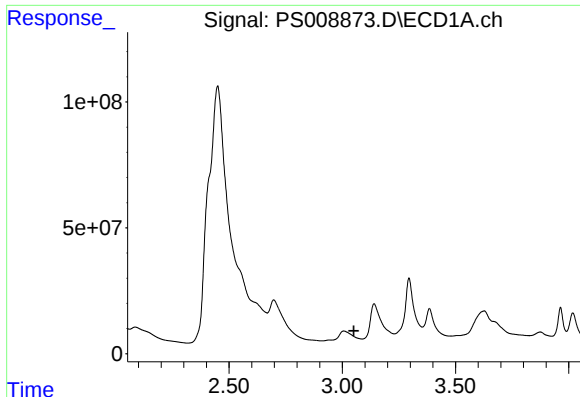

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.051 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

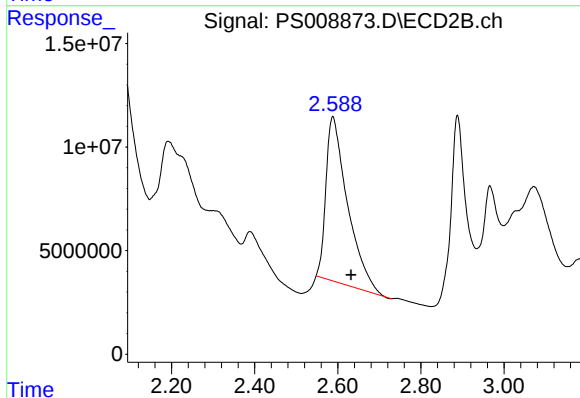


#1 Dalapon

R.T.: 2.588 min
Delta R.T.: -0.044 min
Response: 286371022
Conc: 238.78 ng/ml

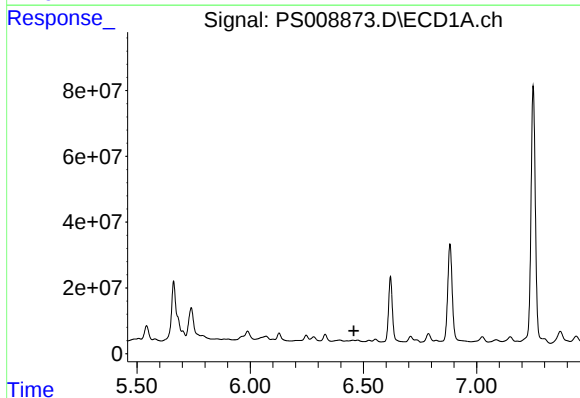


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.458 min
Response: 0
Conc: N.D.

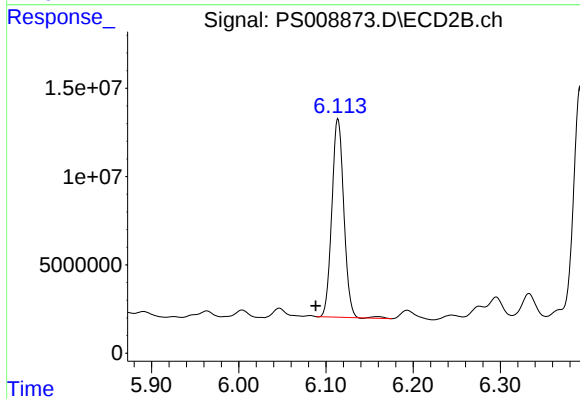

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.114 min
Delta R.T.: 0.026 min
Response: 107396552
Conc: 78.06 ng/ml

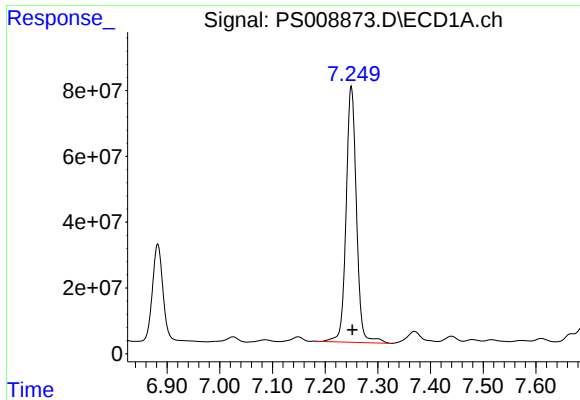

#4 2,4-DCAA


R.T.: 7.250 min
Delta R.T.: -0.002 min
Response: 1064381312
Conc: 495.91 ng/ml

Instrument :
ECD_S
ClientSampleId :

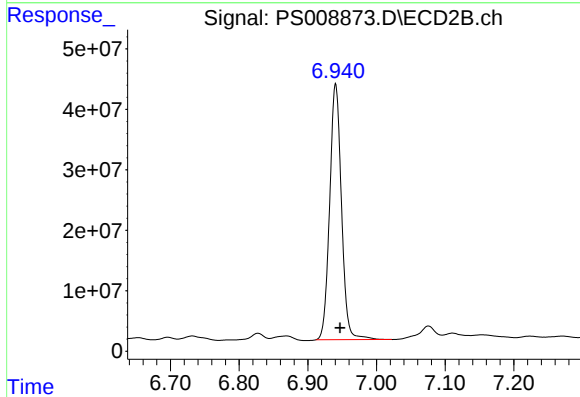


#4 2,4-DCAA

R.T.: 6.941 min
Delta R.T.: -0.006 min
Response: 505002326
Conc: 544.87 ng/ml

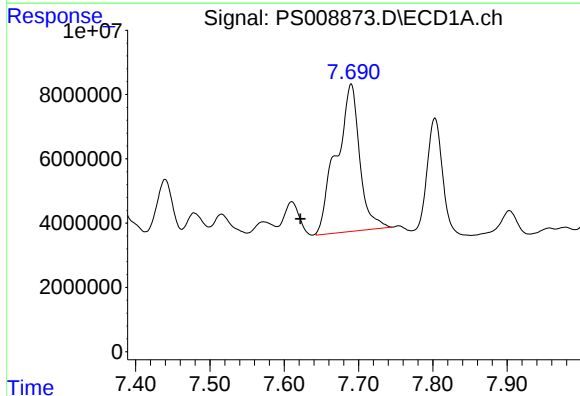


#6 MCP

R.T.: 7.690 min
Delta R.T.: 0.068 min
Response: 99857070
Conc: 16.25 ug/ml

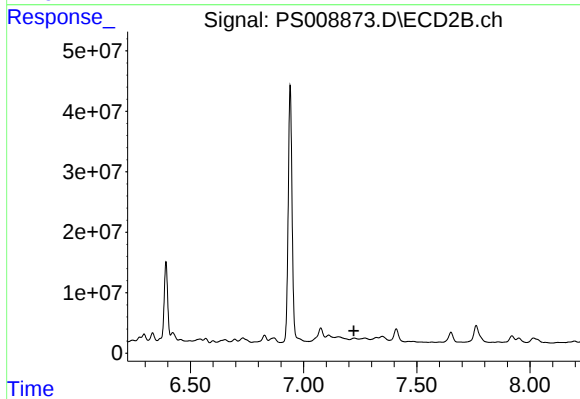

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.222 min
Response: 0
Conc: N.D.

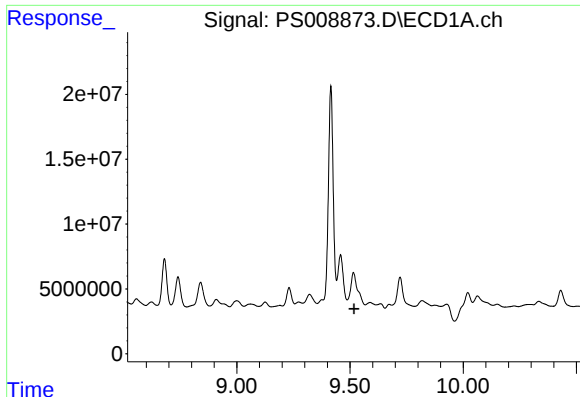

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.517 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

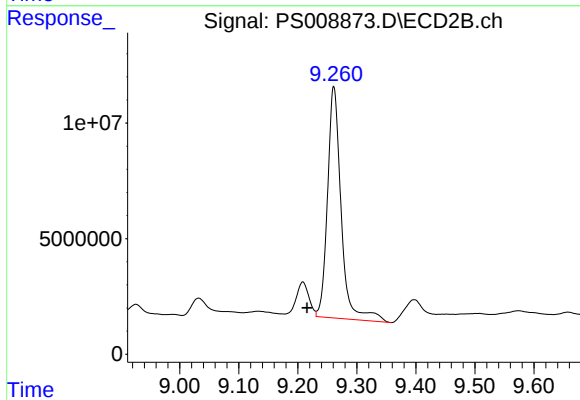


#12 2,4,5-T

R.T.: 9.261 min
Delta R.T.: 0.045 min
Response: 161144319
Conc: 31.18 ng/ml

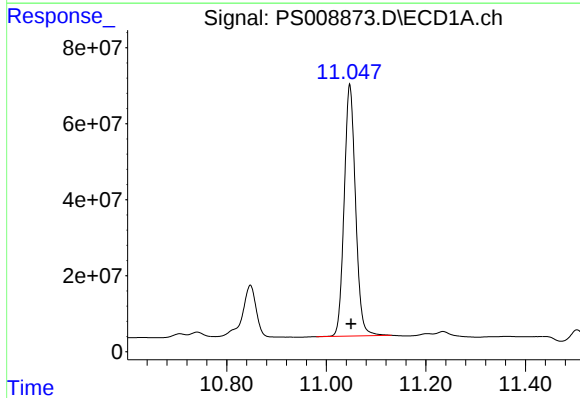


#15 Picloram

R.T.: 11.047 min
Delta R.T.: -0.003 min
Response: 1047361454
Conc: 69.16 ng/ml

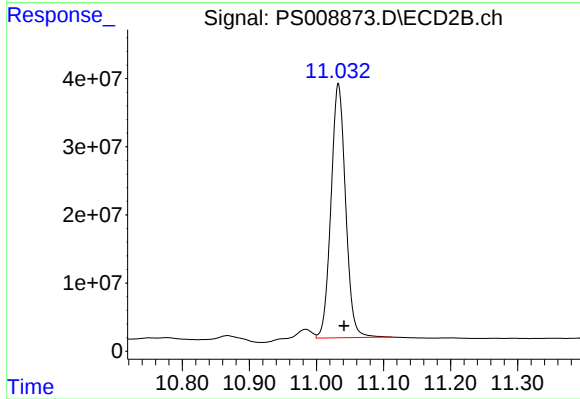

#15 Picloram


R.T.: 11.033 min
Delta R.T.: -0.008 min
Response: 561557629
Conc: 74.40 ng/ml

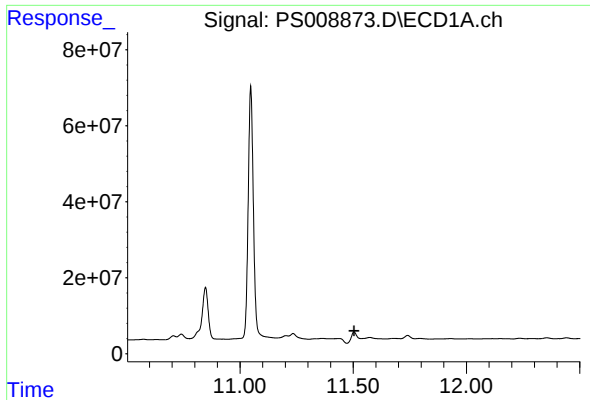

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.503 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

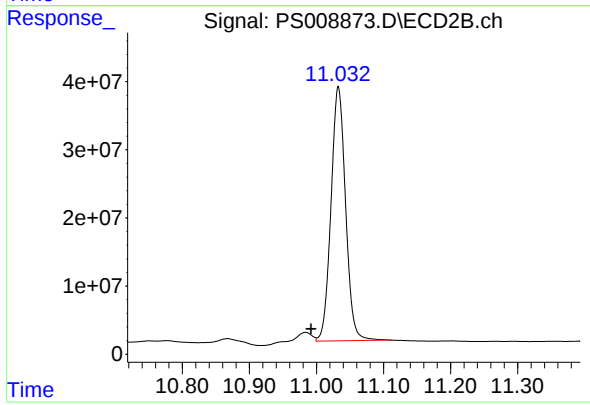

#16 DCPA

R.T.: 11.033 min
Delta R.T.: 0.041 min
Response: 561557629
Conc: 86.34 ng/ml