

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021820\
 Data File : PS008879.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Feb 2020 13:20
 Operator : DD\AJ
 Sample : L1547-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 19 00:46:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 05 02:36:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.247	6.941	378.4E6	78237657	176.284	84.415 #
Target Compounds							
2) T	3,5-DICHL...	0.000	6.116	0	89865586	N.D.	65.315
5) T	DICAMBA	7.376	0.000	251.1E6	0	31.135	N.D. #
7) T	MCPA	7.799	7.433	112.0E6	114.0E6	13.036	27.312 #
9) T	2,4-D	8.393	0.000	22219296	0	10.383	N.D. #
10) T	Pentachlo...	0.000	8.515	0	74298242	N.D.	5.633
12) T	2,4,5-T	9.455	0.000	71096327	0	6.460	N.D. #
14) T	DINOSEB	0.000	10.008	0	61139543	N.D.	16.645
16) T	DCPA	11.508	0.000	48236243	0	3.441	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021820\
Data File : PS008879.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Feb 2020 13:20
Operator : DD\AJ
Sample : L1547-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 19 00:46:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
Quant Title : 8080.M
QLast Update : Wed Feb 05 02:36:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

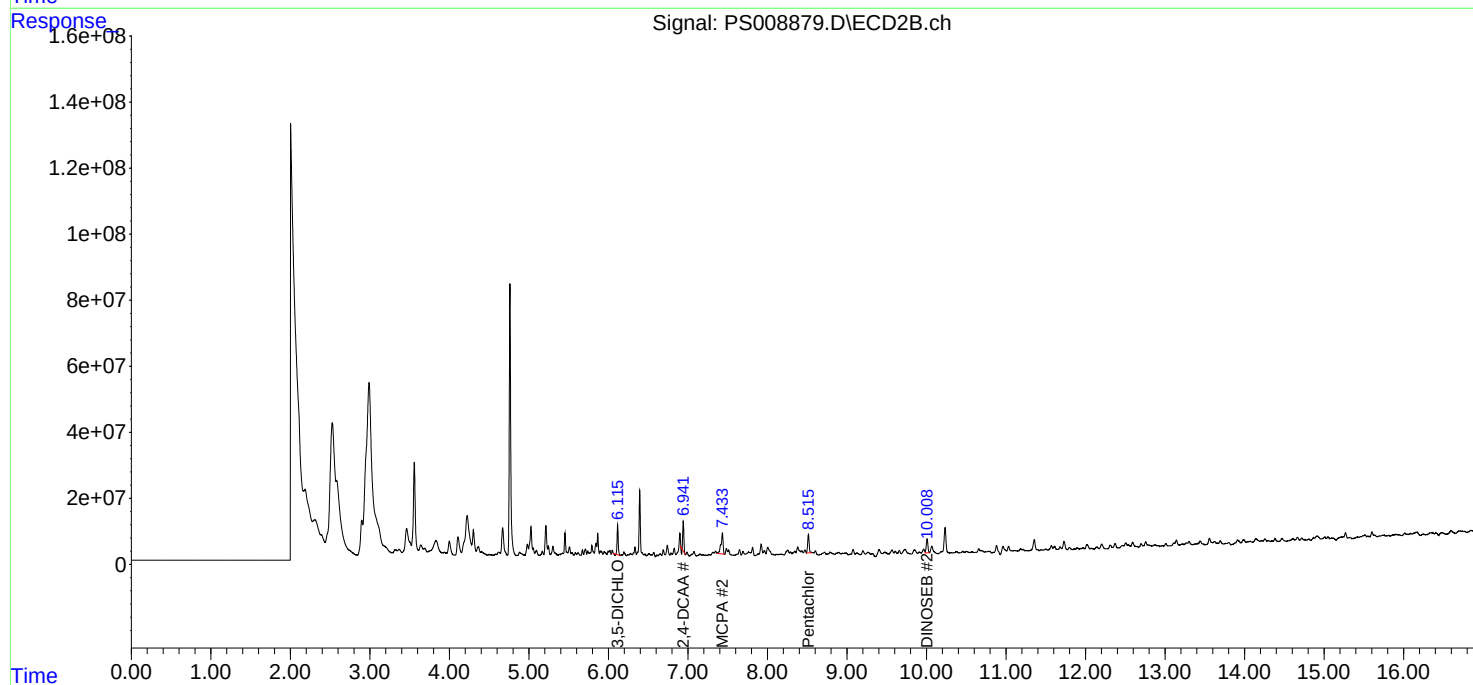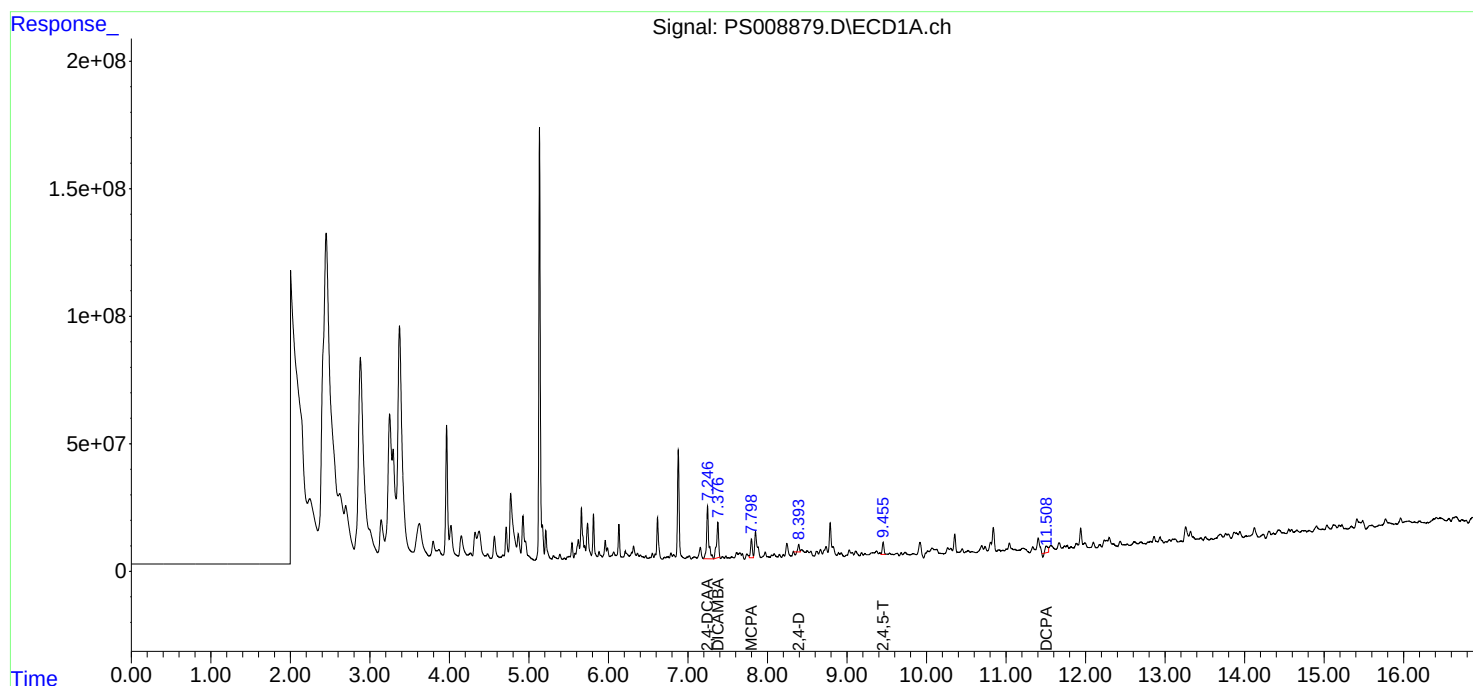


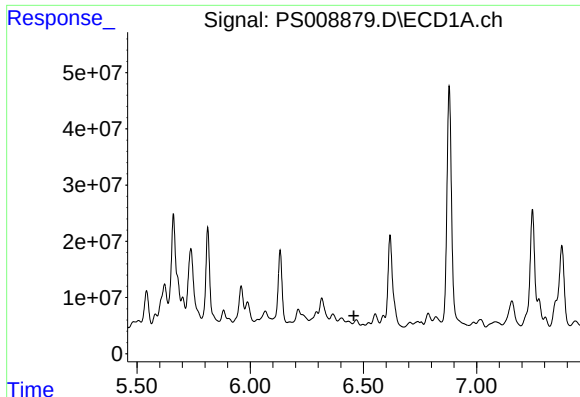

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.458 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

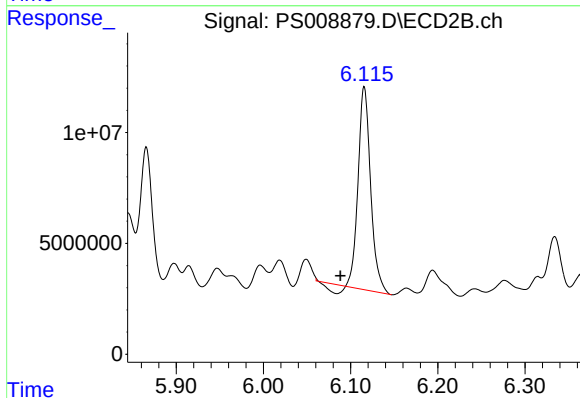


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.116 min
Delta R.T.: 0.028 min
Response: 89865586
Conc: 65.31 ng/ml

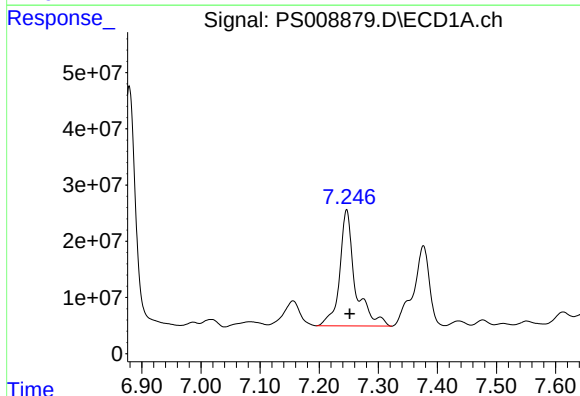


#4 2,4-DCAA

R.T.: 7.247 min
Delta R.T.: -0.005 min
Response: 378359208
Conc: 176.28 ng/ml

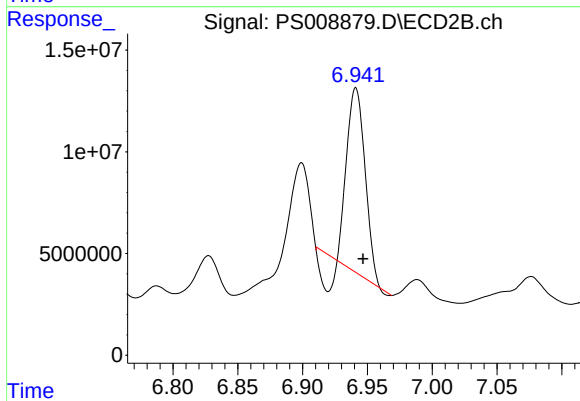

#4 2,4-DCAA


R.T.: 6.941 min
Delta R.T.: -0.006 min
Response: 78237657
Conc: 84.41 ng/ml

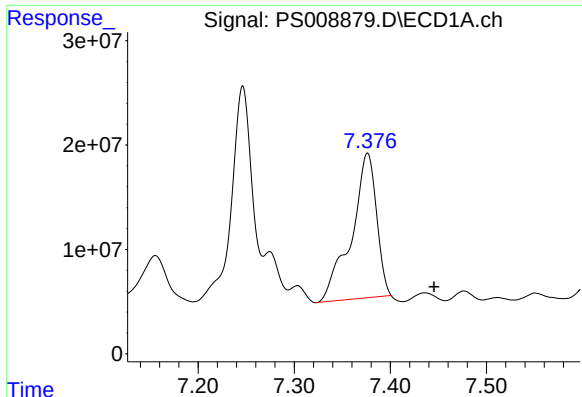

#5 DICAMBA


R.T.: 7.376 min
Delta R.T.: -0.069 min
Response: 251127770
Conc: 31.13 ng/ml

Instrument :
ECD_S
ClientSampleId :

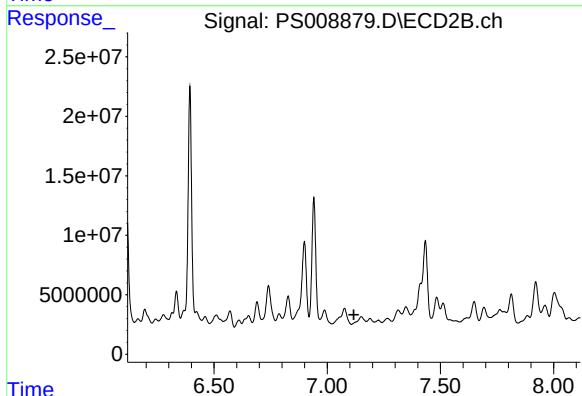


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.118 min
Response: 0
Conc: N.D.

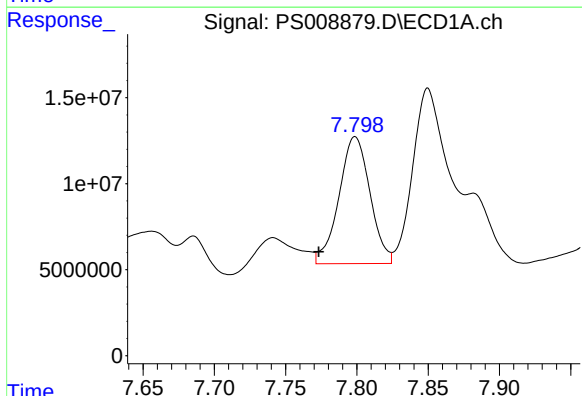


#7 MCPA

R.T.: 7.799 min
Delta R.T.: 0.025 min
Response: 111984374
Conc: 13.04 ug/ml

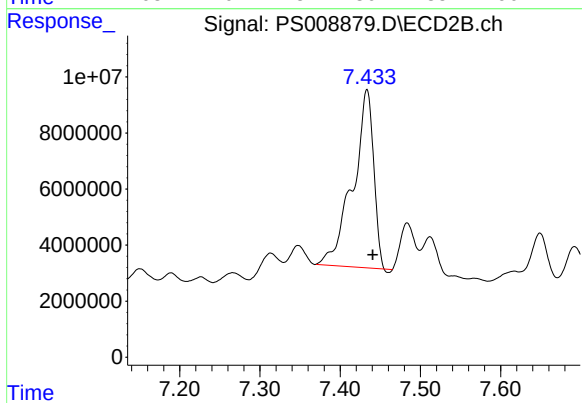

#7 MCPA


R.T.: 7.433 min
Delta R.T.: -0.007 min
Response: 113988394
Conc: 27.31 ug/ml

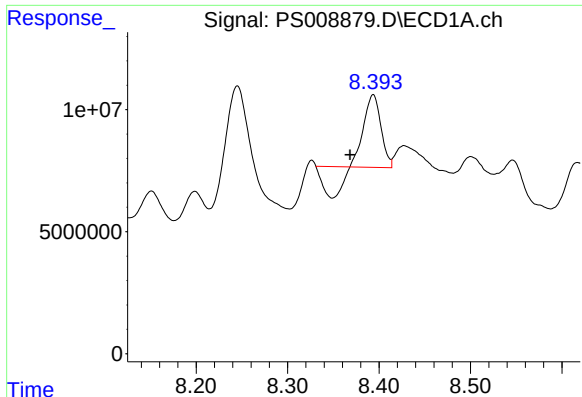

#9 2,4-D


R.T.: 8.393 min
Delta R.T.: 0.025 min
Response: 22219296
Conc: 10.38 ng/ml

Instrument :
ECD_S
ClientSampleId :

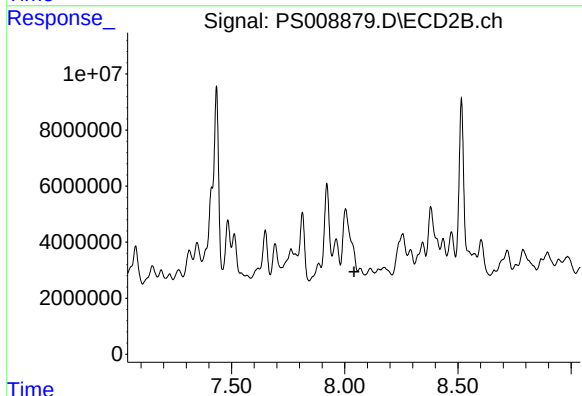


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.041 min
Response: 0
Conc: N.D.

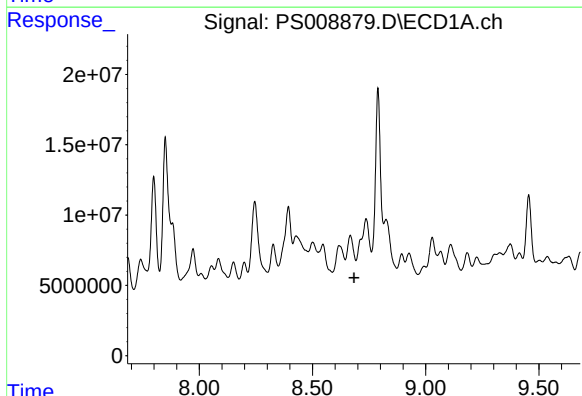


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 8.683 min
Response: 0
Conc: N.D.

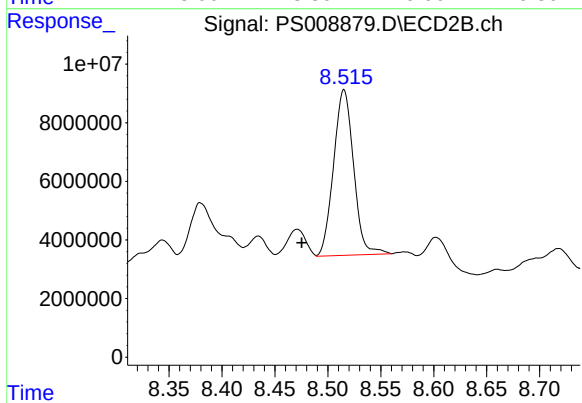

#10 Pentachlorophenol


R.T.: 8.515 min
Delta R.T.: 0.040 min
Response: 74298242
Conc: 5.63 ng/ml

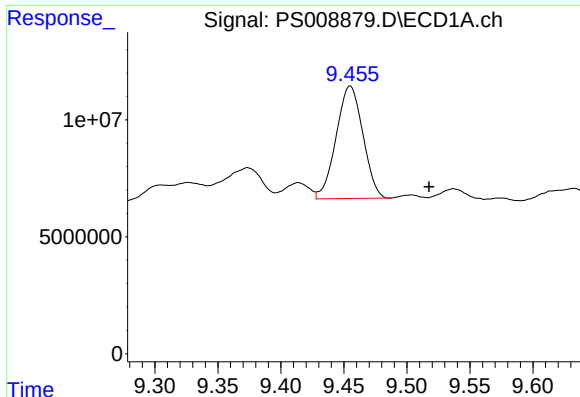

#12 2,4,5-T


R.T.: 9.455 min
Delta R.T.: -0.063 min
Response: 71096327
Conc: 6.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

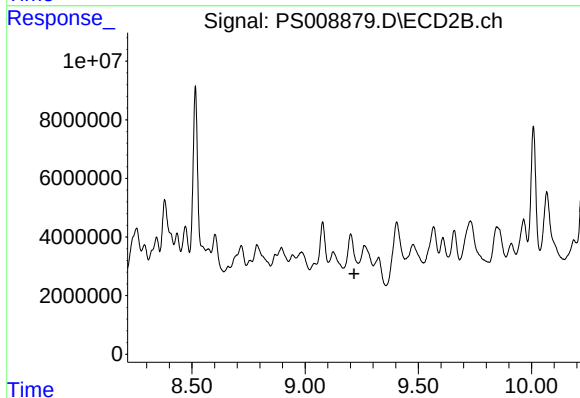


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.216 min
Response: 0
Conc: N.D.

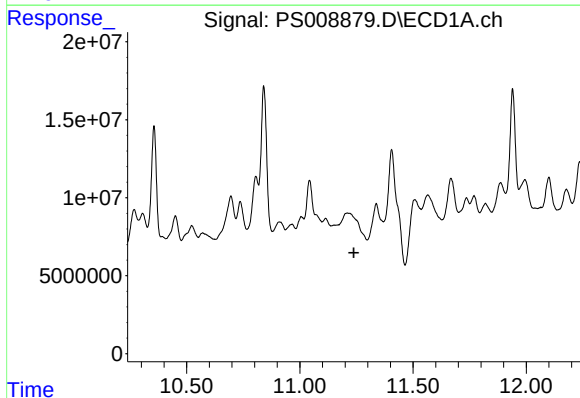


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.239 min
Response: 0
Conc: N.D.

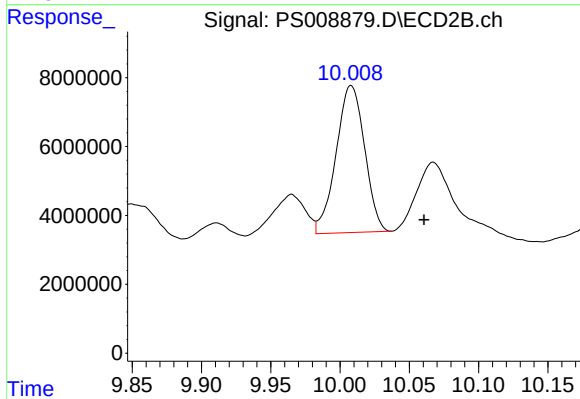

#14 DINOSEB


R.T.: 10.008 min
Delta R.T.: -0.053 min
Response: 61139543
Conc: 16.65 ng/ml

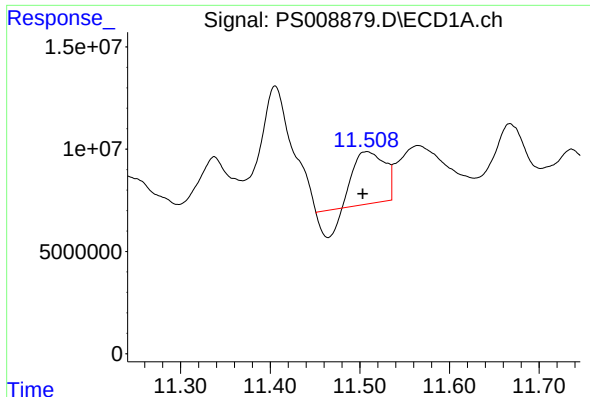

#16 DCPA

R.T.: 11.508 min
Delta R.T.: 0.004 min
Response: 48236243
Conc: 3.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

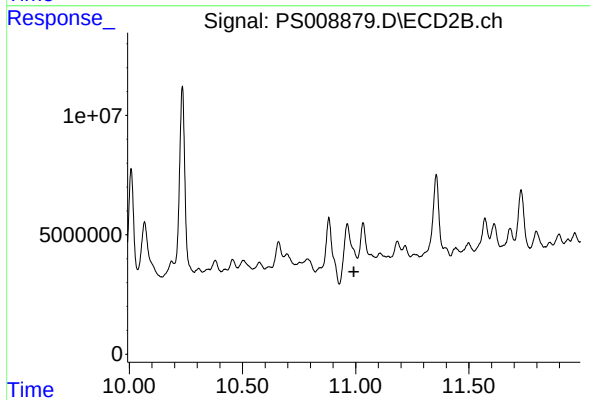

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.992 min
Response: 0
Conc: N.D.